

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028844.D
 Acq On : 22 Nov 2023 18:07
 Operator : MA/JU
 Sample : 05268-16
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKD9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 21:37:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.694	152	8620	0.400	ng/u1	-0.04
4) Naphthalene-d8	10.429	136	33227	0.400	ng/u1	#-0.03
9) Acenaphthene-d10	14.297	164	16009	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.056	188	30376	0.400	ng/u1	0.00
17) Chrysene-d12	21.275	240	21016	0.400	ng/u1	0.00
23) Perylene-d12	23.543	264	24080	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	51818m	5.439	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.051	152	11228m	0.224	ng/u1	-0.02
18) Fluoranthene-d10	19.094	212	26908	0.398	ng/u1	0.00
Target Compounds						Qvalue
16) Anthracene	17.182	178	23834	0.279	ng/u1	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028844.D
Acq On : 22 Nov 2023 18:07
Operator : MA/JU
Sample : 05268-16
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCKD9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023


Quant Time: Nov 22 21:37:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

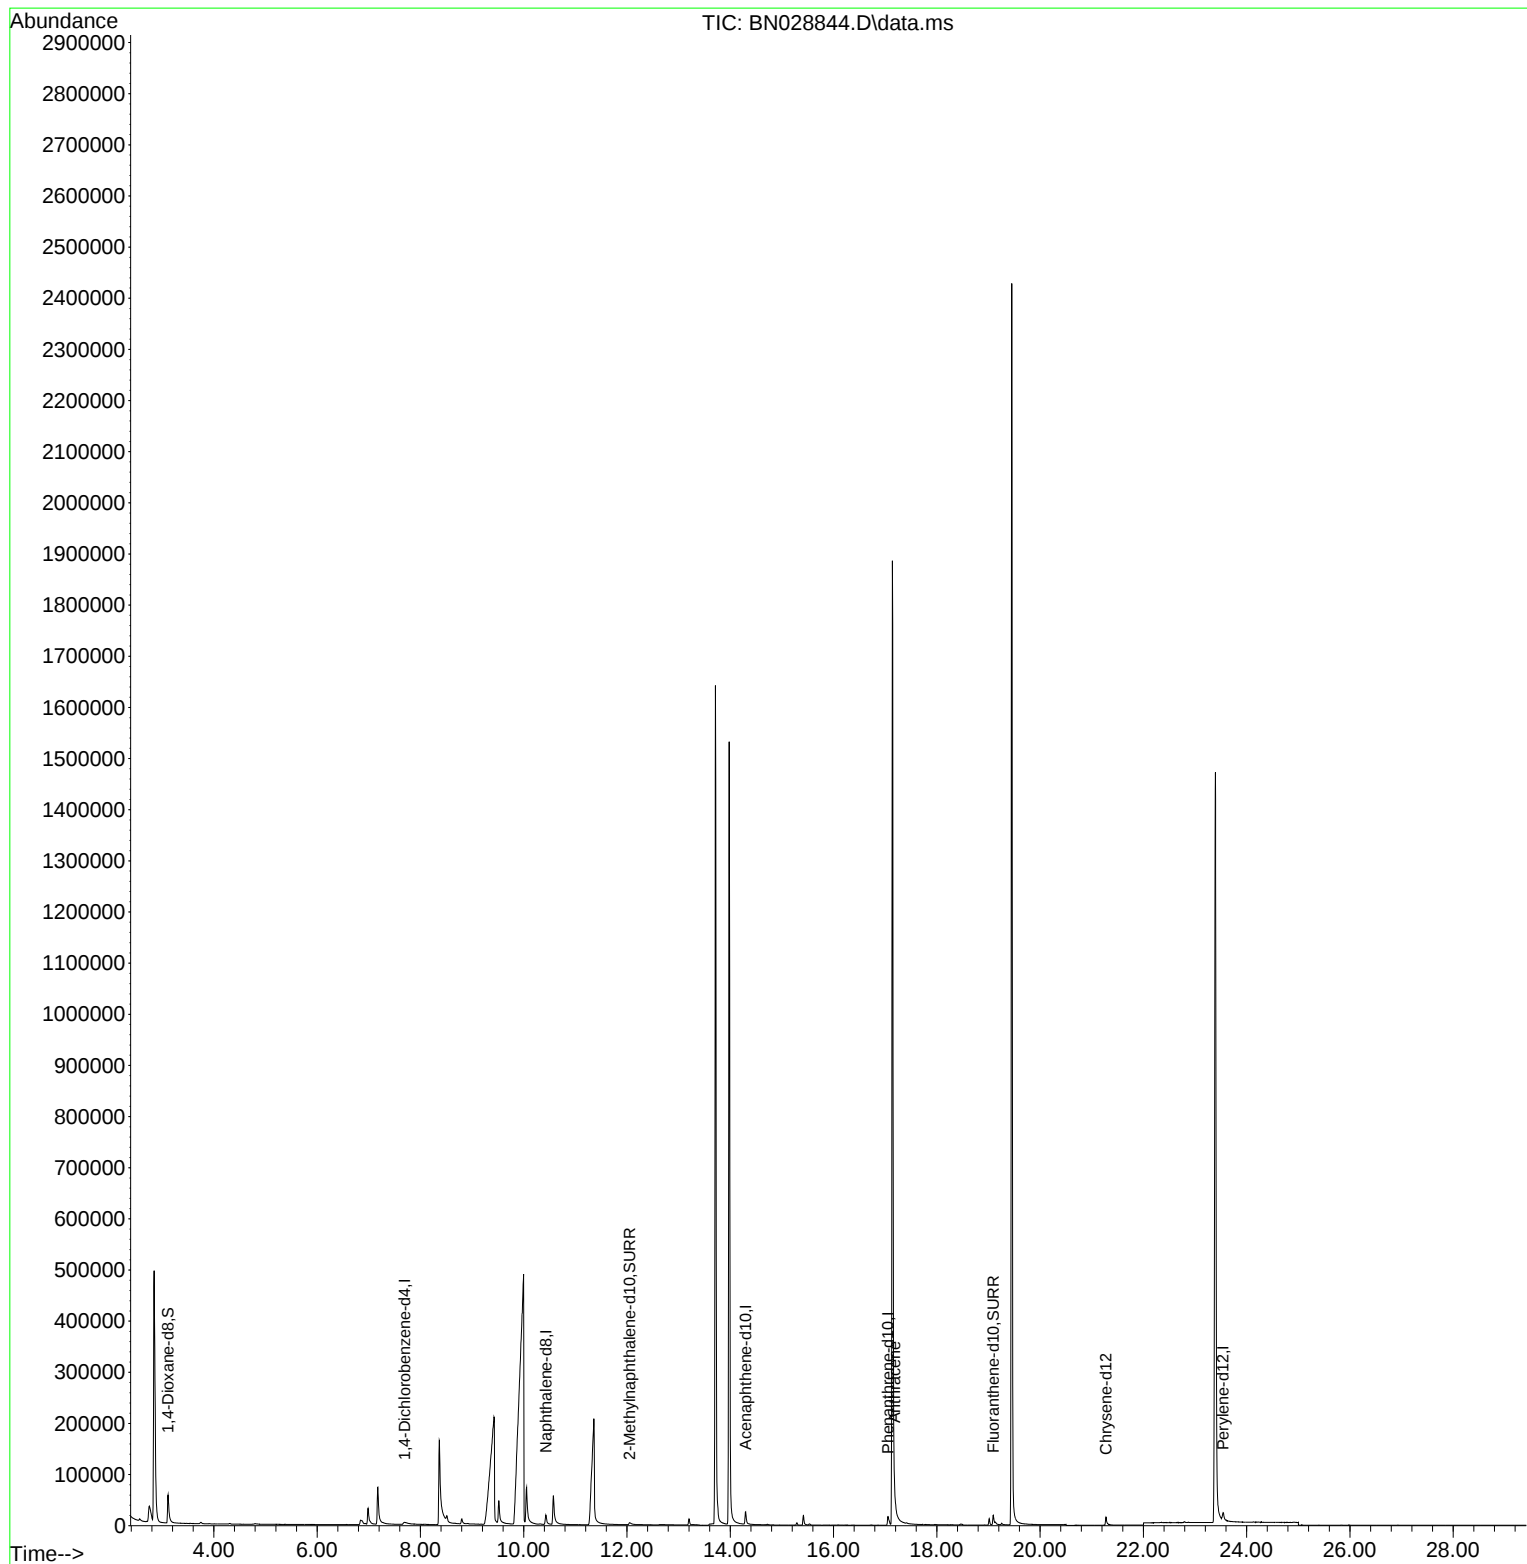

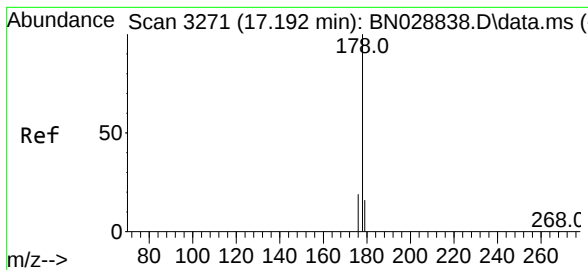

#16
 Anthracene
 Concen: 0.279 ng/ul
 RT: 17.182 min Scan# 31
 Delta R.T. -0.022 min
 Lab File: BN028844.D
 Acq: 22 Nov 2023 18:07

Instrument :
 BNA_N
 ClientSampleId :
 DCKD9

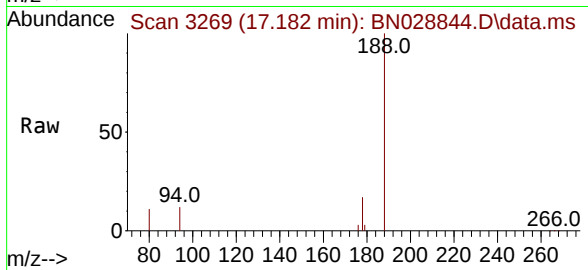

Tgt Ion:178 Resp: 23834
 Ion Ratio Lower Upper
 178 100
 179 17.8 12.6 18.8
 176 20.2 14.9 22.3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

