

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
 Data File : BN028845.D
 Acq On : 22 Nov 2023 18:43
 Operator : MA/JU
 Sample : 05268-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCKE6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/23/2023
 Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 21:37:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 21 23:49:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.702	152	6317	0.400	ng/u1	-0.03
4) Naphthalene-d8	10.445	136	23788	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.297	164	11840	0.400	ng/u1	# 0.00
13) Phenanthrene-d10	17.059	188	21141	0.400	ng/u1	0.00
17) Chrysene-d12	21.280	240	13830	0.400	ng/u1	# 0.00
23) Perylene-d12	23.545	264	17364	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.112	96	41046m	5.879	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.089	152	9136m	0.255	ng/u1	0.02
18) Fluoranthene-d10	19.093	212	22638	0.509	ng/u1	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.713	266	1517	0.299	ng/u1	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112223\
Data File : BN028845.D
Acq On : 22 Nov 2023 18:43
Operator : MA/JU
Sample : 05268-18
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DCKE6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/23/2023
Supervised By :mohammad ahmed 11/25/2023

Quant Time: Nov 22 21:37:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 21 23:49:43 2023
Response via : Initial Calibration

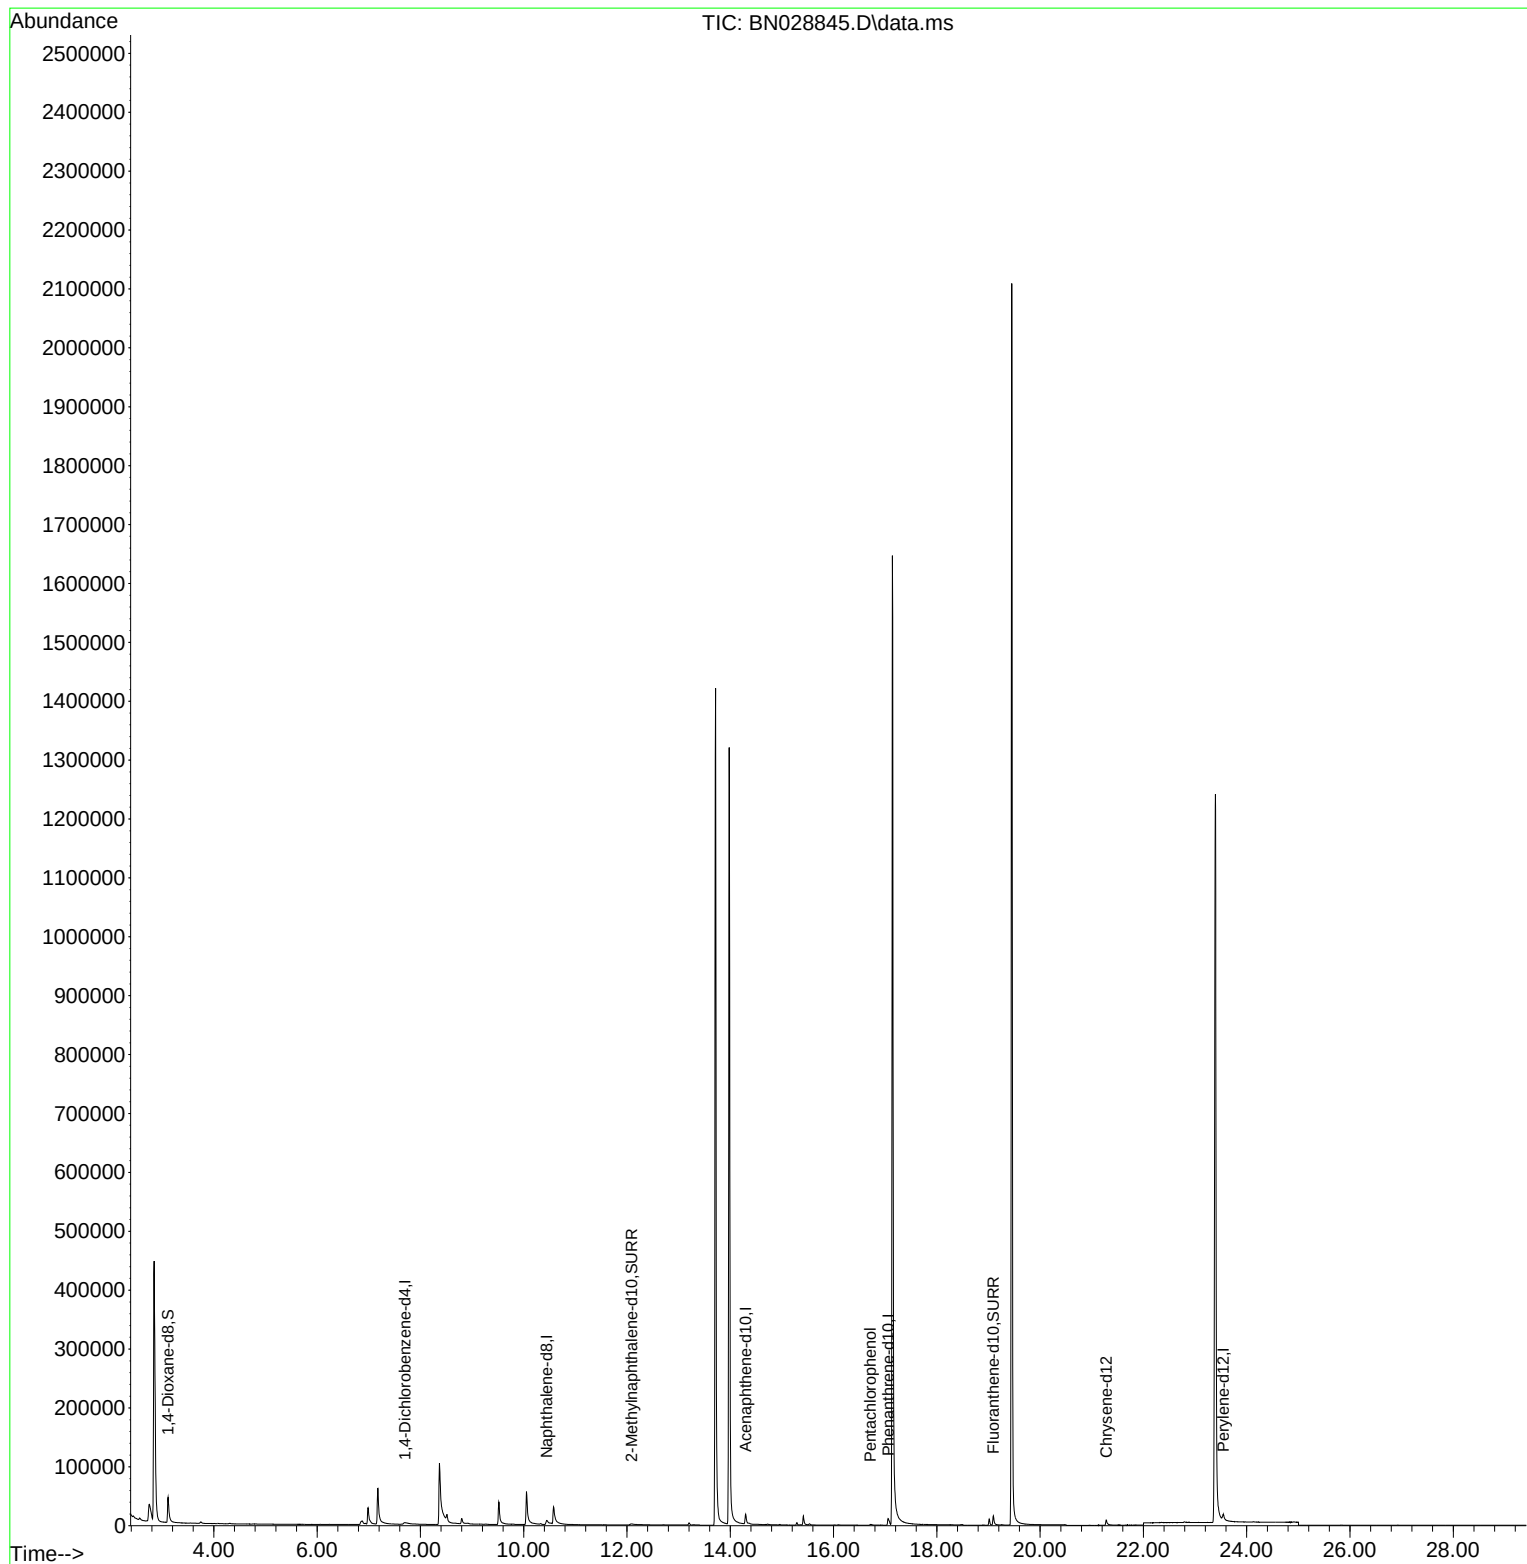

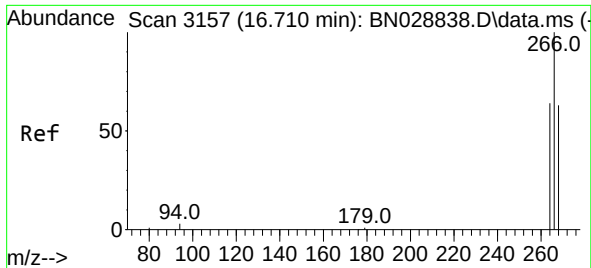

#14

Pentachlorophenol

Concen: 0.299 ng/ul

RT: 16.713 min Scan# 3157

Delta R.T. -0.010 min

Lab File: BN028845.D


Acq: 22 Nov 2023 18:43

Instrument :

BNA_N

ClientSampleId :

DCKE6

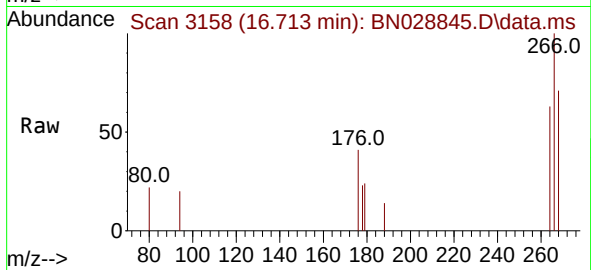

Tgt Ion:266 Resp: 151

Ion Ratio Lower Upper

266 100

264 62.2 50.1 75.1

268 62.7 50.6 75.8

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/23/2023

Supervised By :mohammad ahmed 11/25/2023

