




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035238.D
Acq On : 22 Nov 2024 12:35
Operator : RC/JU
Sample : PB164981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK981

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 13:00:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

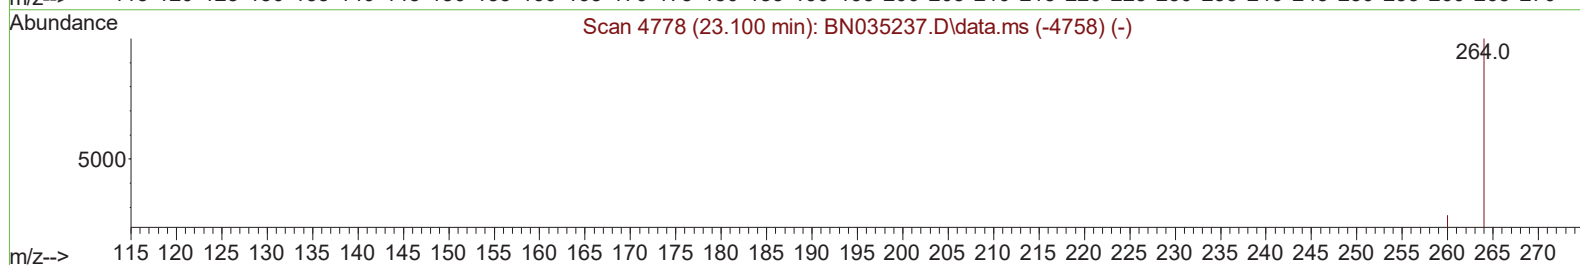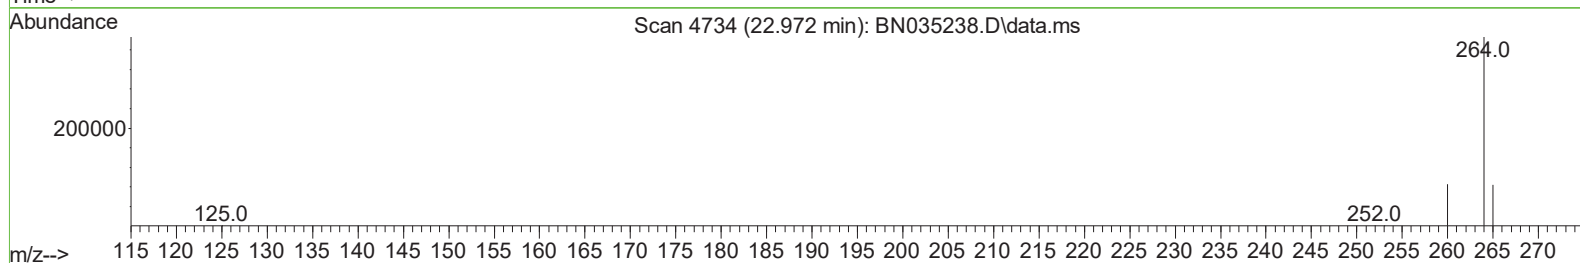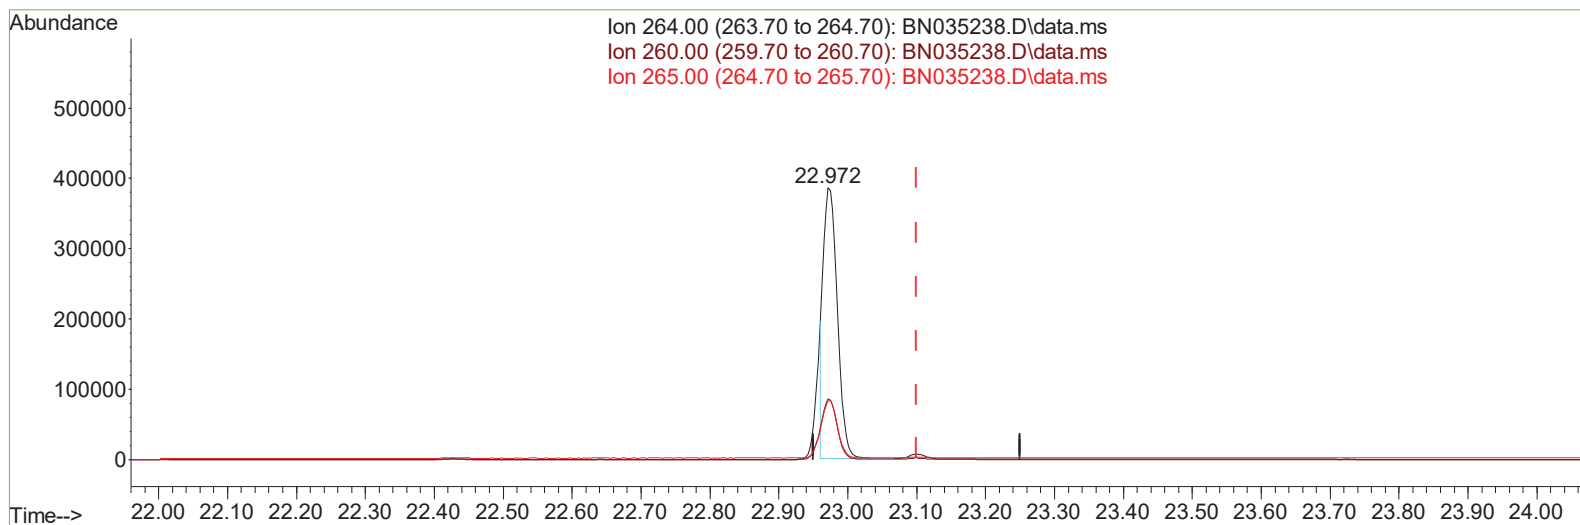

TIC: BN035238.D\data.ms

(23) Perylene-d12 (I)

22.972min (-0.129) 0.40 ng/u1

response 550875

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.26
265.00	75.50	21.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035238.D
Acq On : 22 Nov 2024 12:35
Operator : RC/JU
Sample : PB164981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK981

Manual IntegrationsAPPROVED

Quant Time: Nov 22 13:00:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

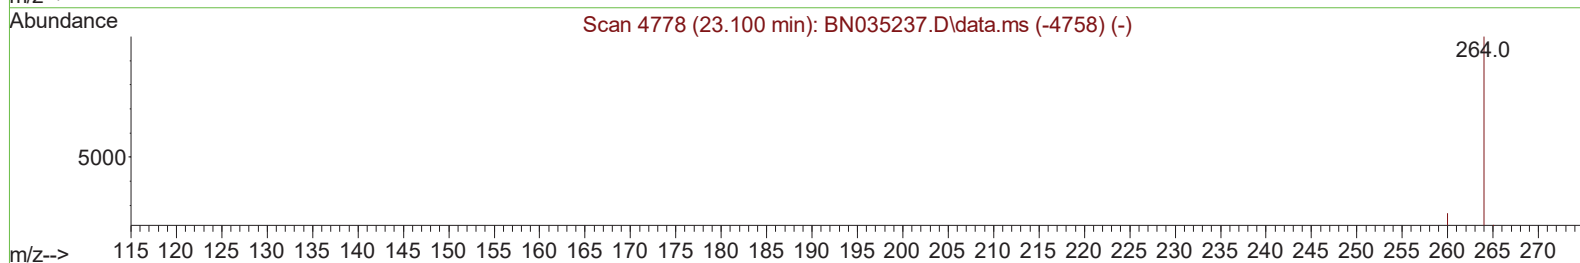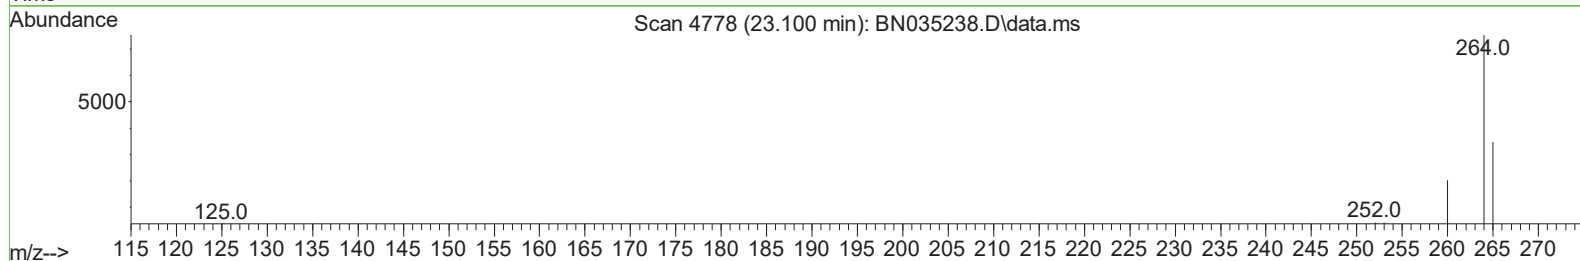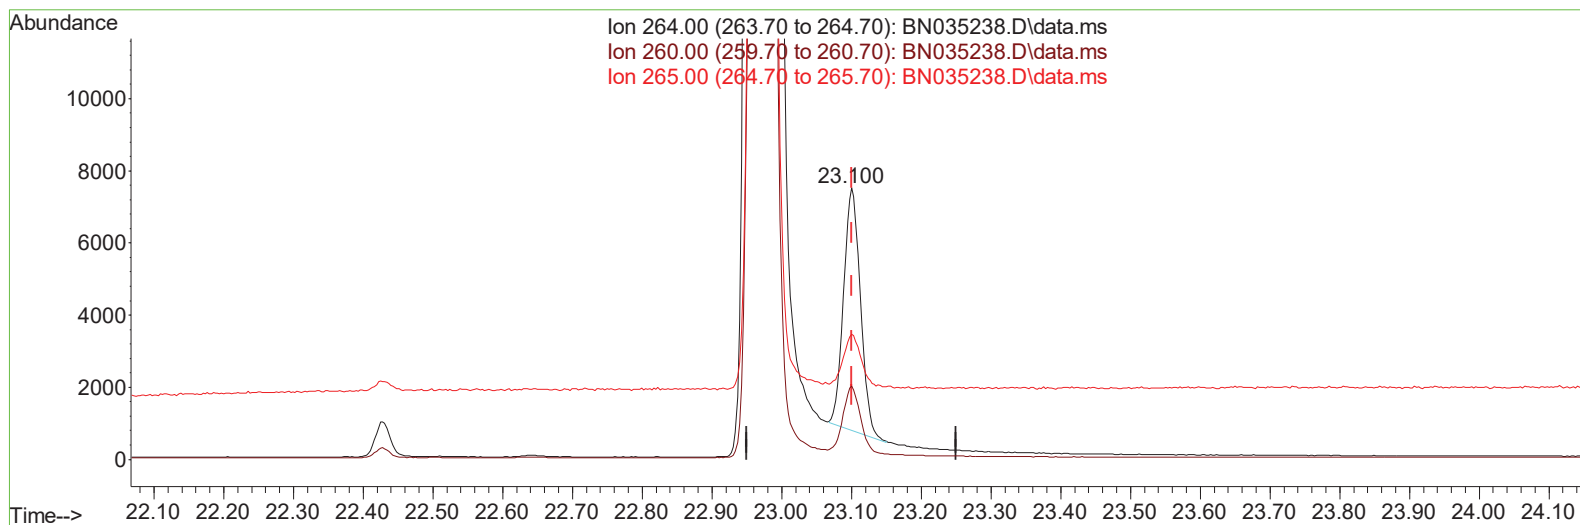

TIC: BN035238.D\data.ms

(23) Perylene-d12 (I)

23.100min (-0.000) 0.40 ng/ul m

response 11263

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.07
265.00	75.50	46.20#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035238.D
Acq On : 22 Nov 2024 12:35
Operator : RC/JU
Sample : PB164981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK981

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 13:00:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.318	152		4399	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136		11408	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164		7512	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.751	188		17322	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.996	240		13352	0.400	ng/ul	# 0.00
23) Perylene-d12	23.100	264		11263m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		17712	4.405	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.675	152		4042	0.242	ng/ul	0.00
18) Fluoranthene-d10	18.800	212		10844	0.294	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035238.D
Acq On : 22 Nov 2024 12:35
Operator : RC/JU
Sample : PB164981BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK981

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/27/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 13:00:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

