




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035241.D
Acq On : 22 Nov 2024 14:29
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 22 14:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

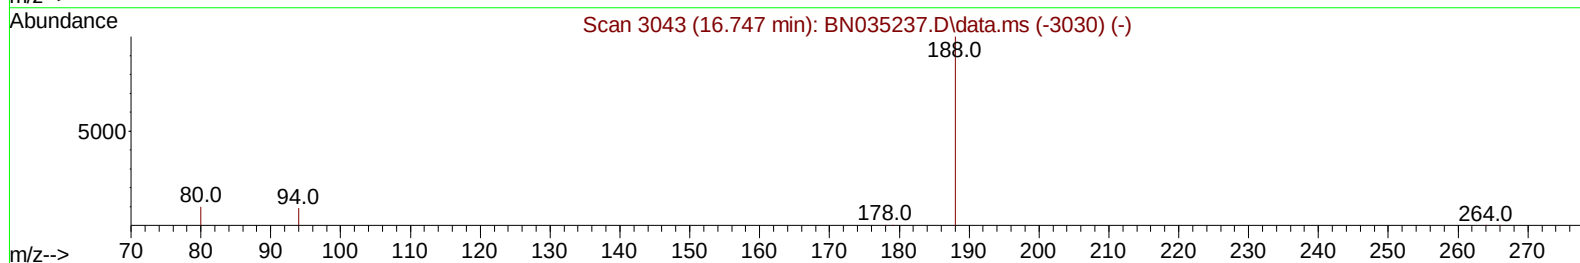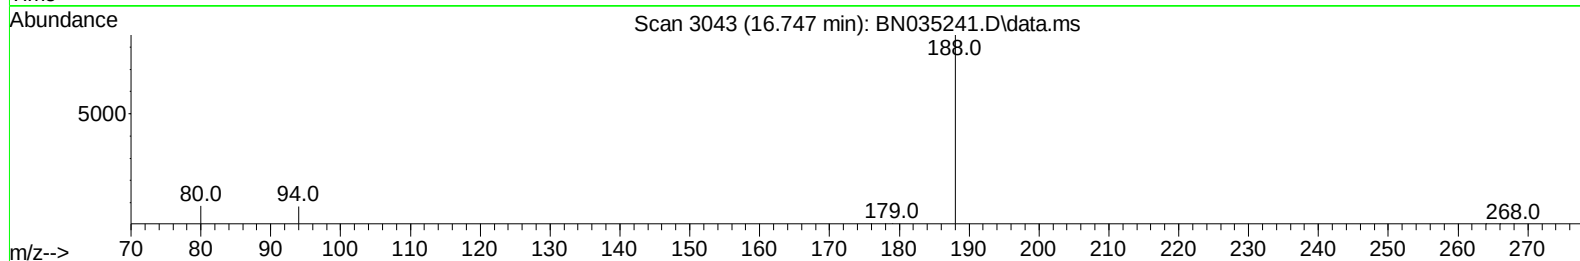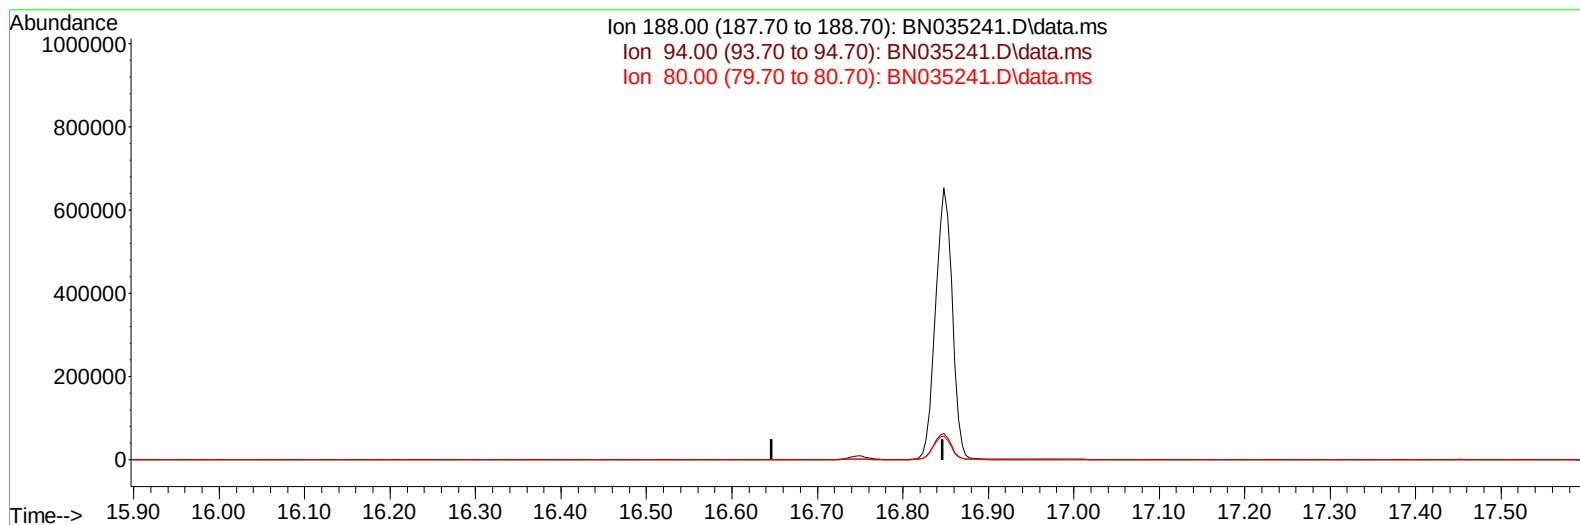

TIC: BN035241.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (-16.747) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035241.D
Acq On : 22 Nov 2024 14:29
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 22 14:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

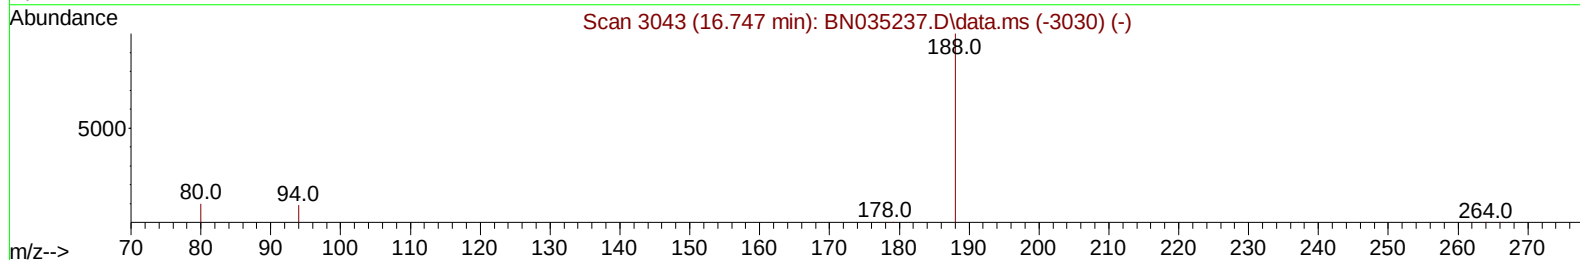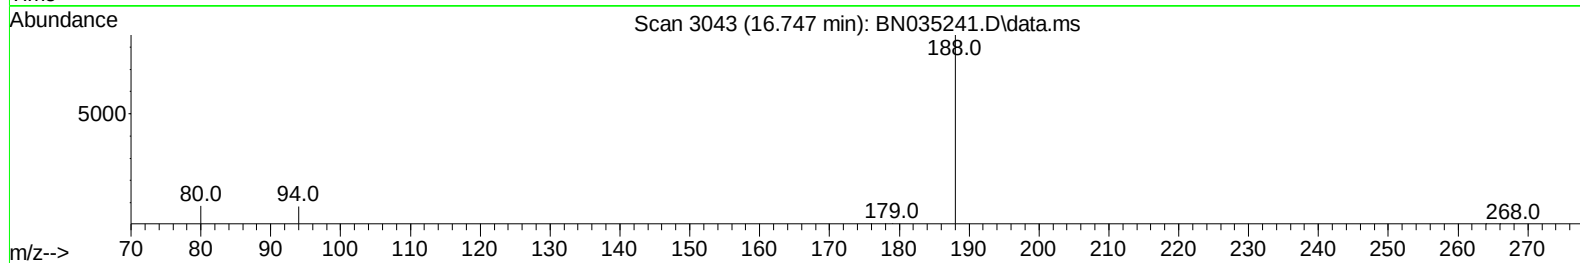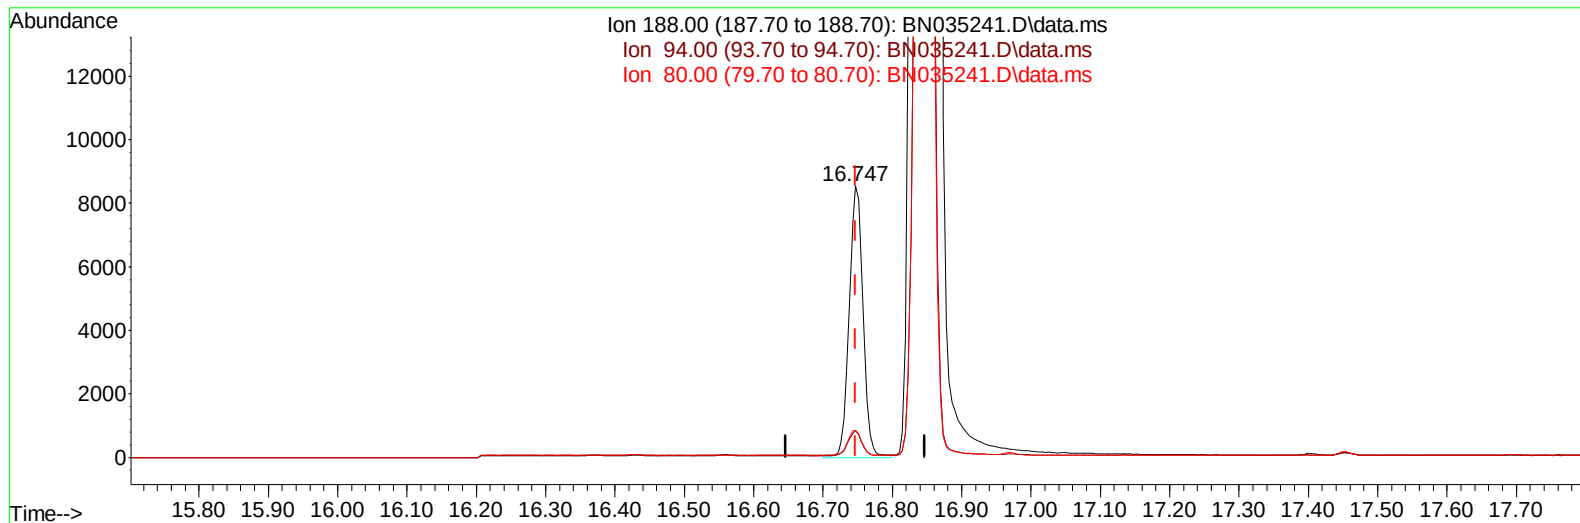

TIC: BN035241.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (+ 0.000) 0.40 ng/ul m

response 11892

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	9.78#
80.00	7.60	9.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035241.D
Acq On : 22 Nov 2024 14:29
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 14:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

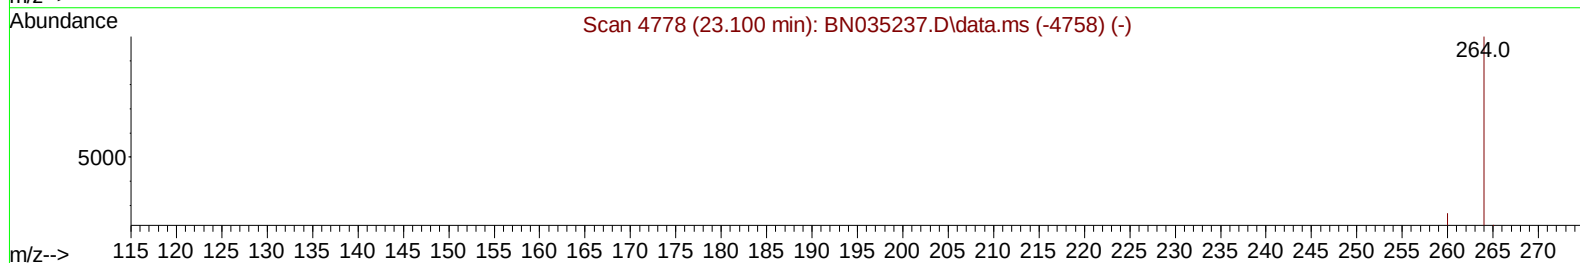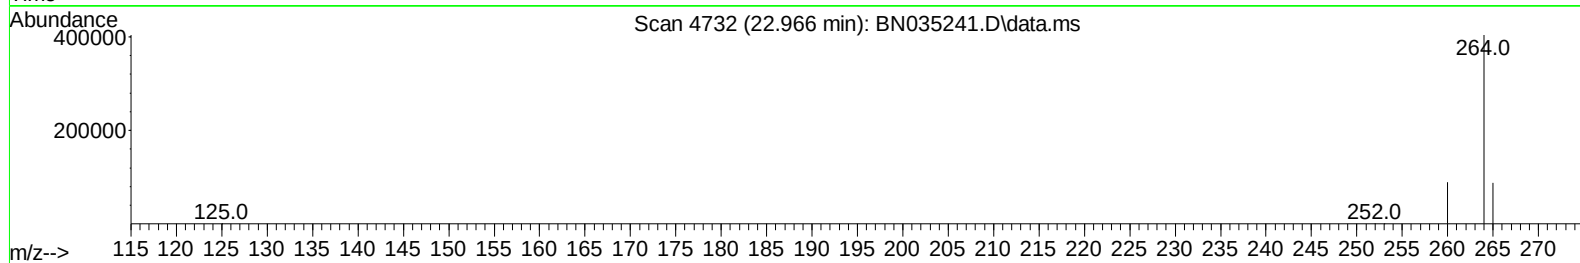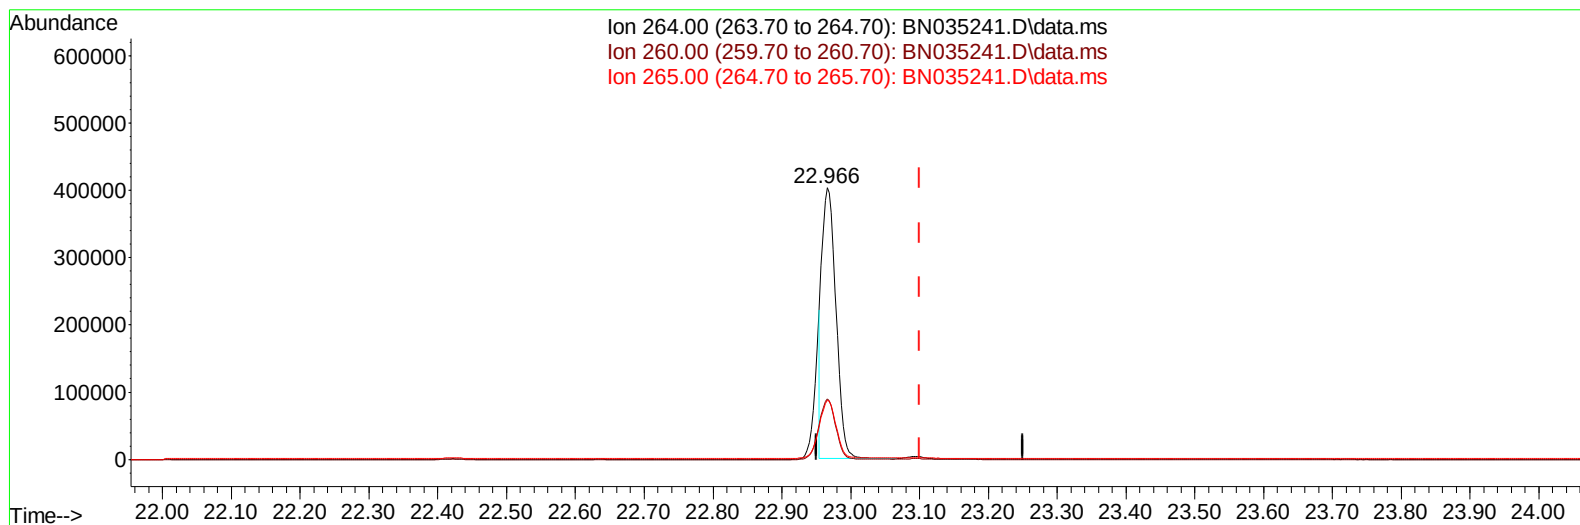

TIC: BN035241.D\data.ms

(23) Perylene-d12 (I)

22.966min (-0.134) 0.40 ng/u1

response 570786

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.21
265.00	75.50	21.76#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035241.D
Acq On : 22 Nov 2024 14:29
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 22 14:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

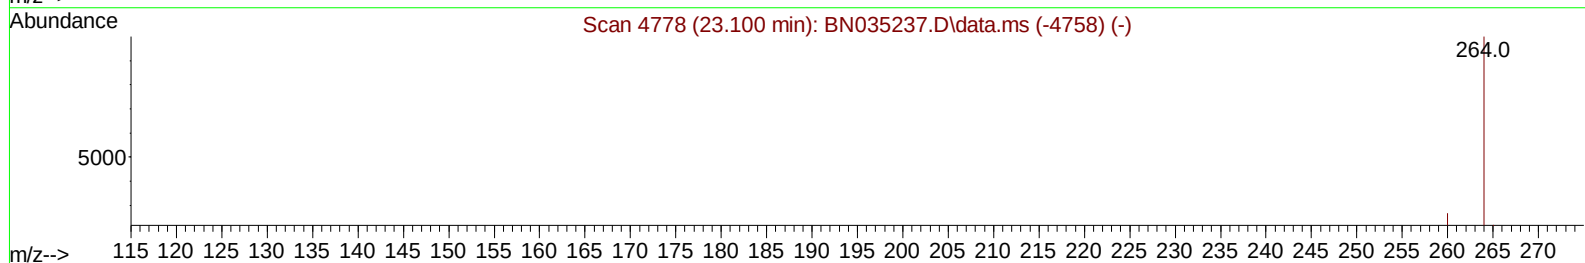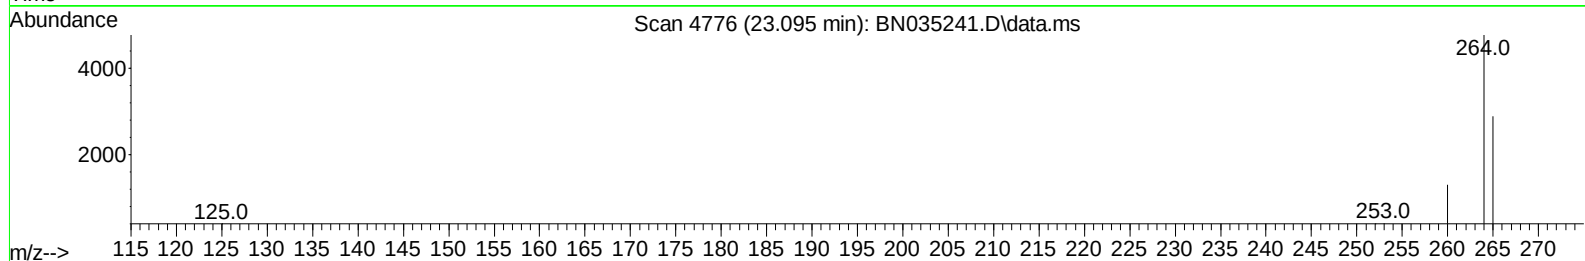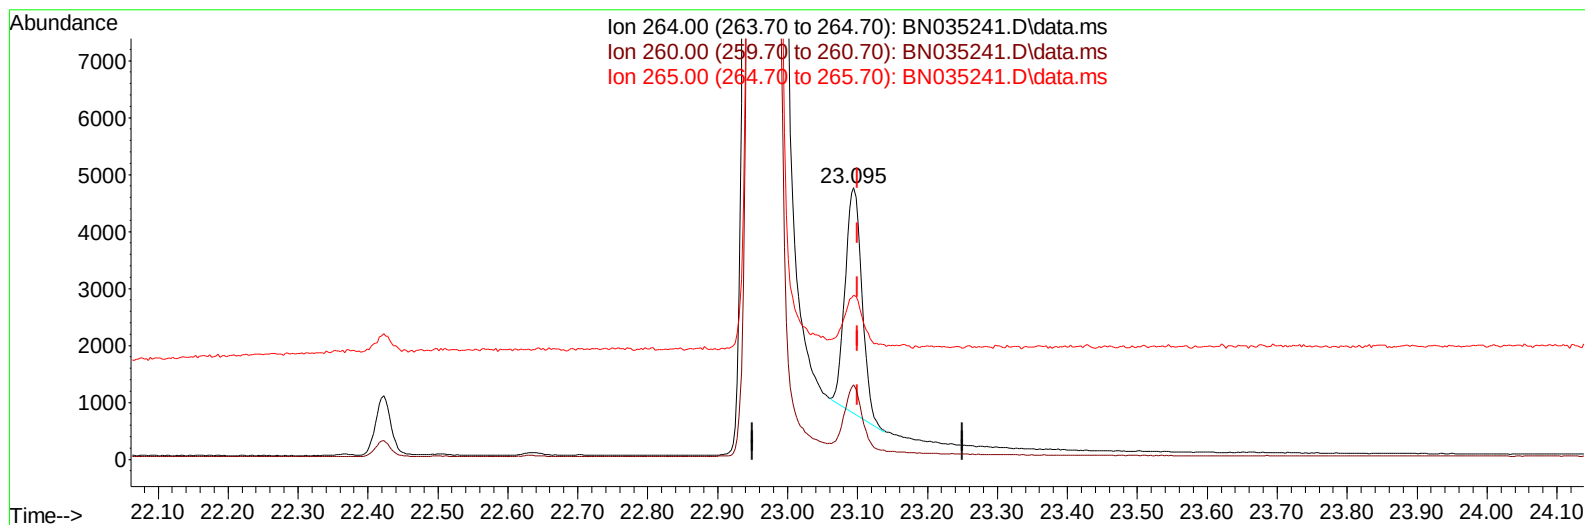

TIC: BN035241.D\data.ms

(23) Perylene-d12 (I)

23.095min (-0.006) 0.40 ng/ul m

response 6579

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.38
265.00	75.50	60.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035241.D
 Acq On : 22 Nov 2024 14:29
 Operator : RC/JU
 Sample : P4875-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A20

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 14:57:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.318	152	3089	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136	8139	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164	5307	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188	11892m	0.400	ng/ul	0.00
17) Chrysene-d12	20.991	240	8274	0.400	ng/ul	# 0.00
23) Perylene-d12	23.095	264	6579m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	12523	4.436	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152	3453	0.290	ng/ul	0.00
18) Fluoranthene-d10	18.800	212	11123	0.487	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035241.D
Acq On : 22 Nov 2024 14:29
Operator : RC/JU
Sample : P4875-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E2A20

Manual IntegrationsAPPROVED

Quant Time: Nov 22 14:57:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

