




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

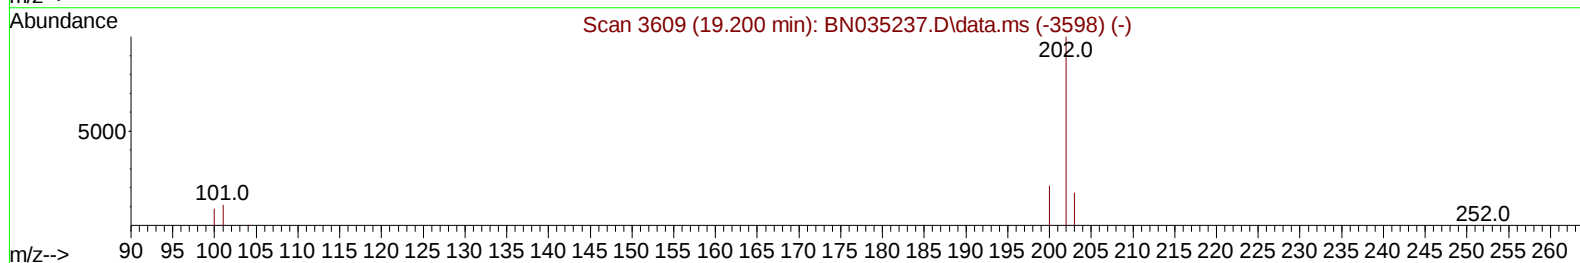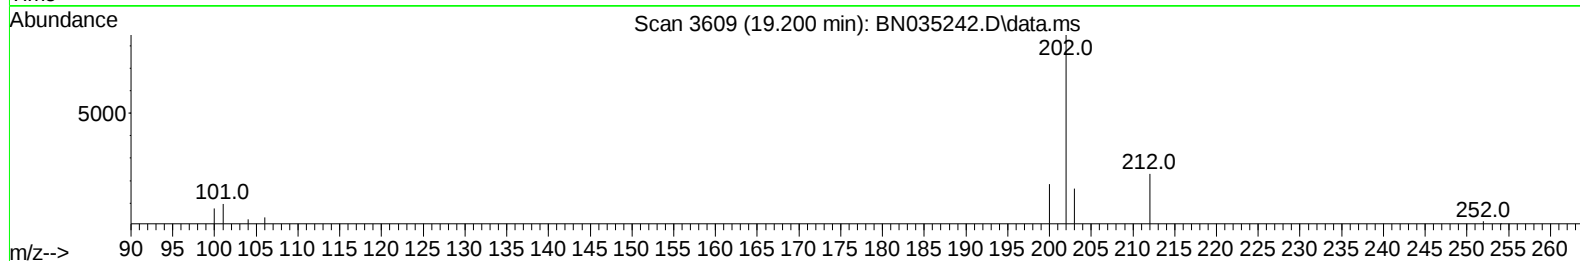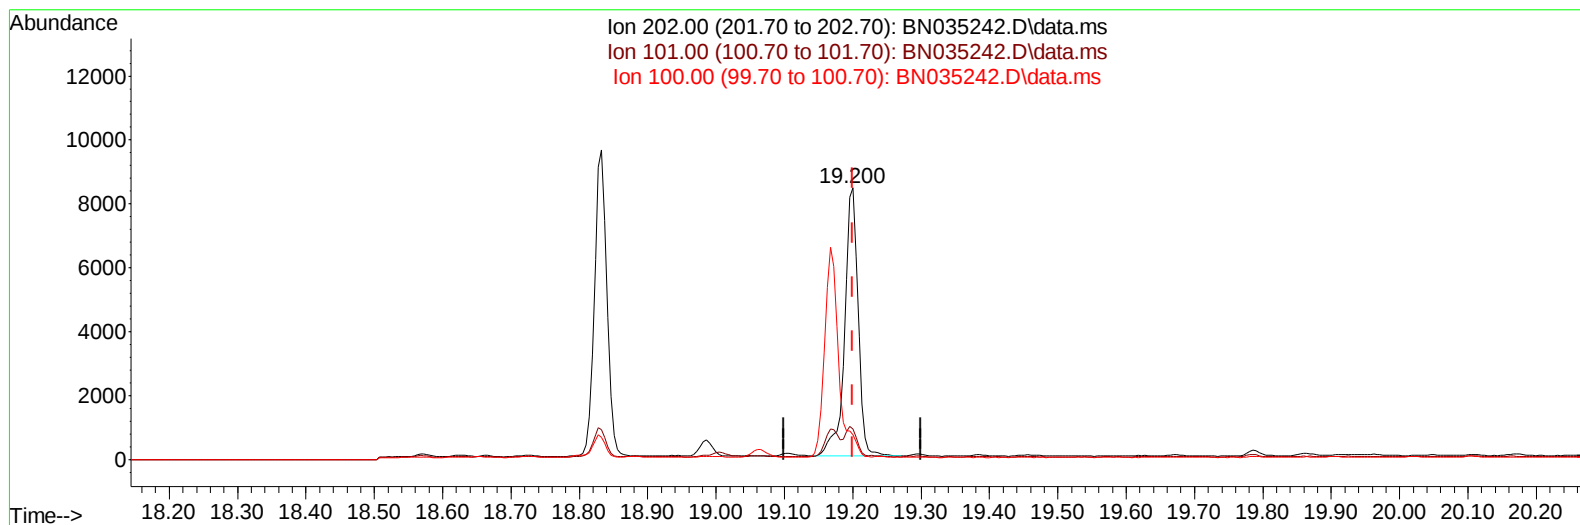

TIC: BN035242.D\data.ms

(20) Pyrene

19.200min (+ 0.000) 0.41 ng/u1

response 11599

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	11.12#
100.00	6.40	9.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

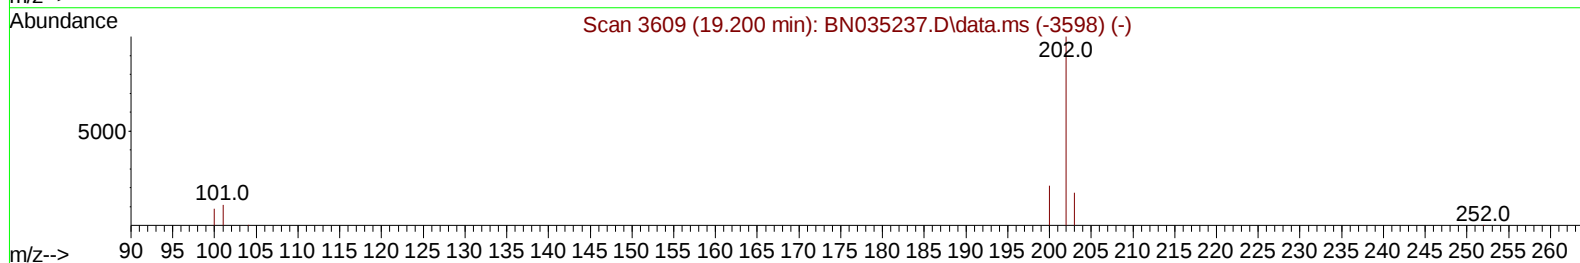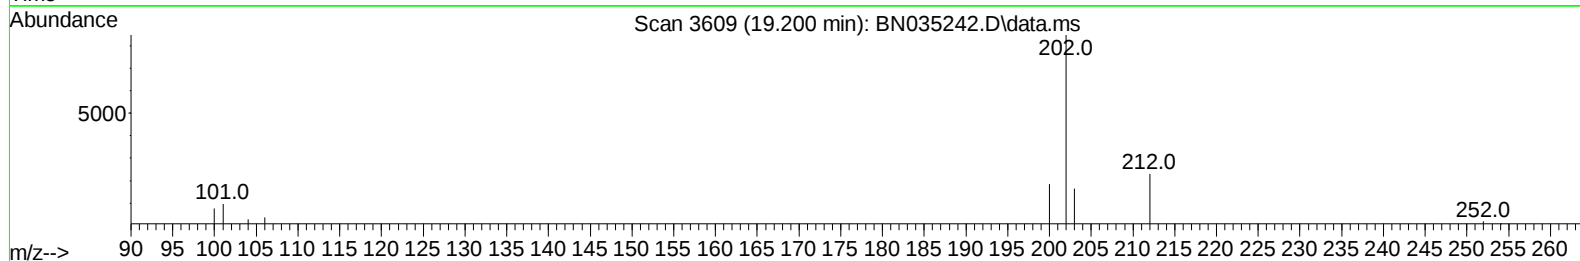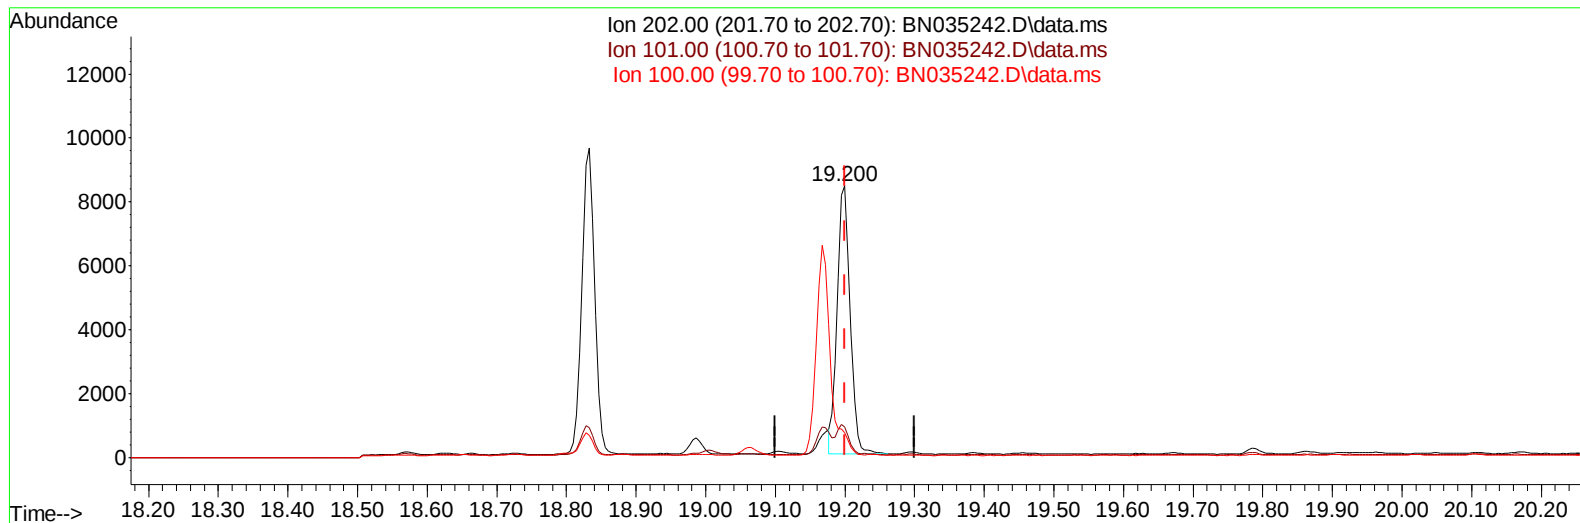

TIC: BN035242.D\data.ms

(20) Pyrene

19.200min (+ 0.000) 0.38 ng/ul m

response 10805

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	11.12#
100.00	6.40	9.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

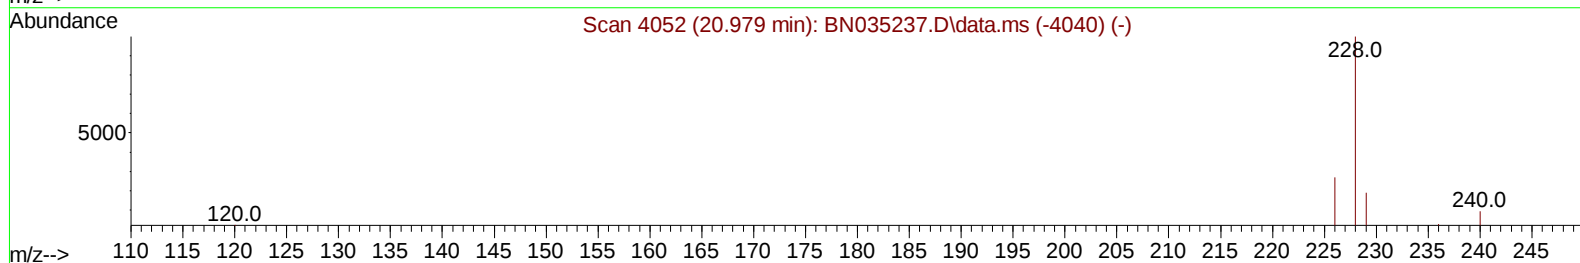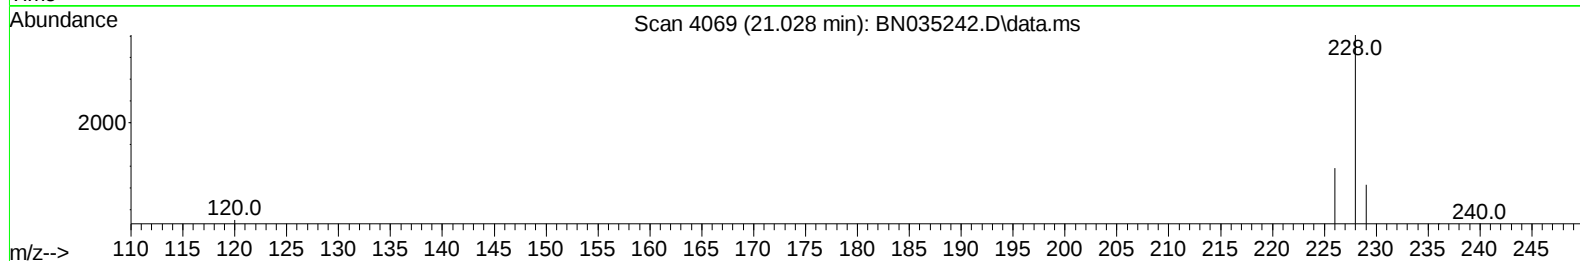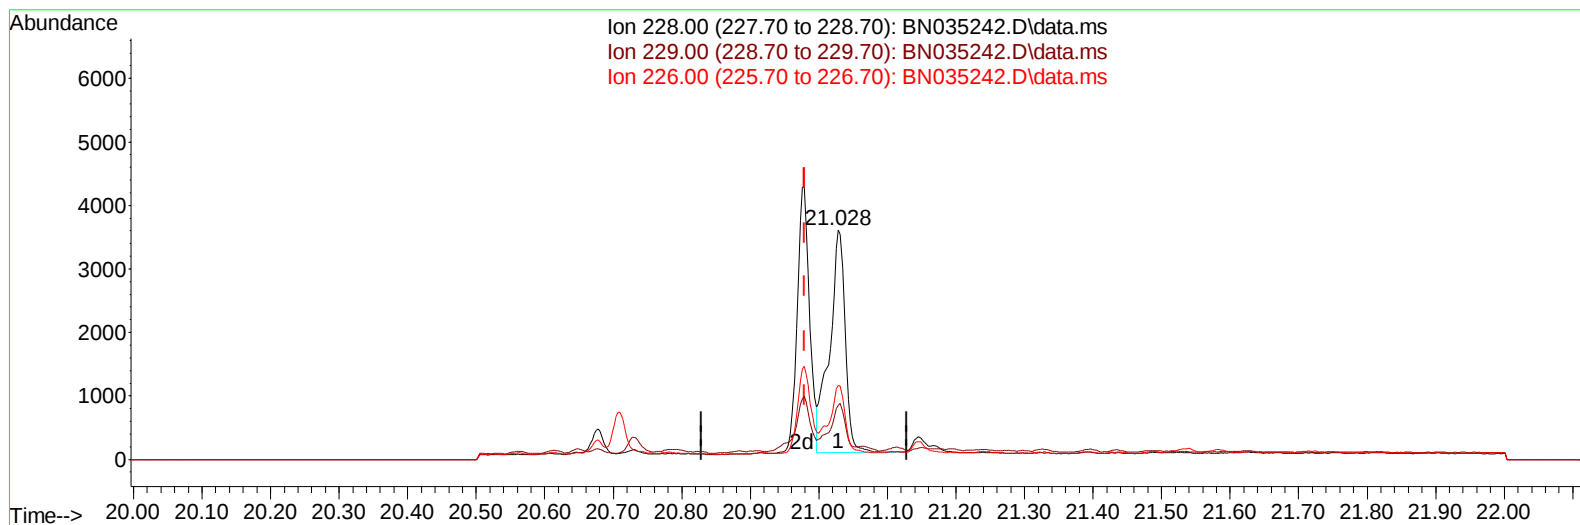

TIC: BN035242.D\data.ms

(21) Benzo(a)anthracene

21.028min (+ 0.050) 0.21 ng/u1

response 5594

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	23.49
226.00	27.30	32.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

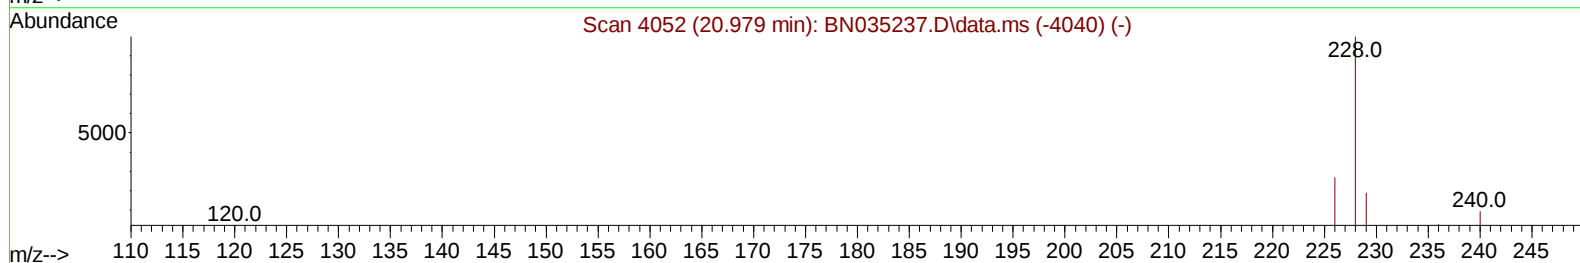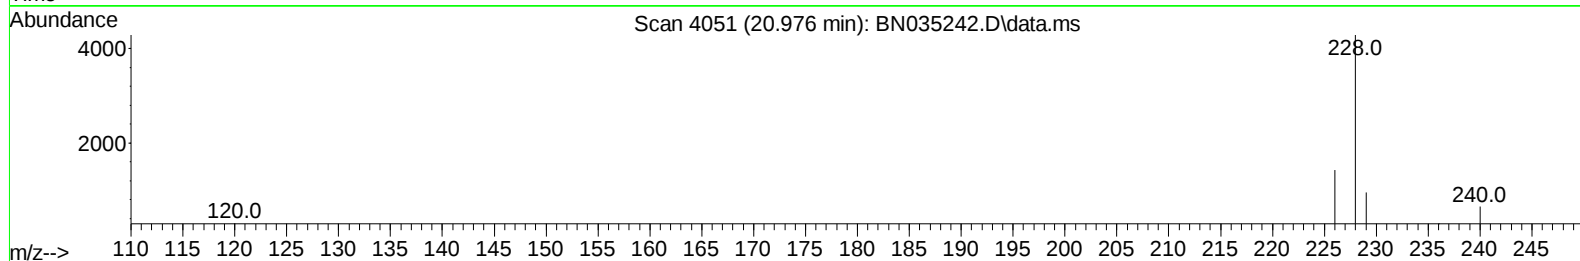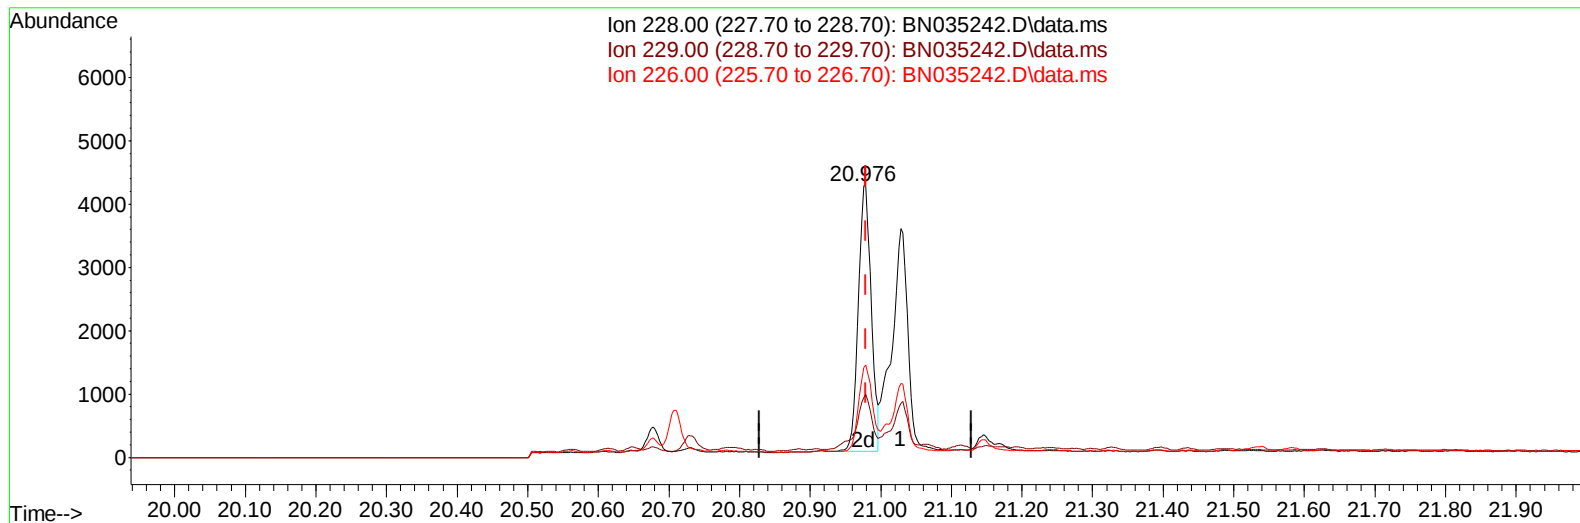

TIC: BN035242.D\data.ms

(21) Benzo(a)anthracene

20.976min (-0.003) 0.20 ng/u1 m

response 5333

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	22.14
226.00	27.30	33.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

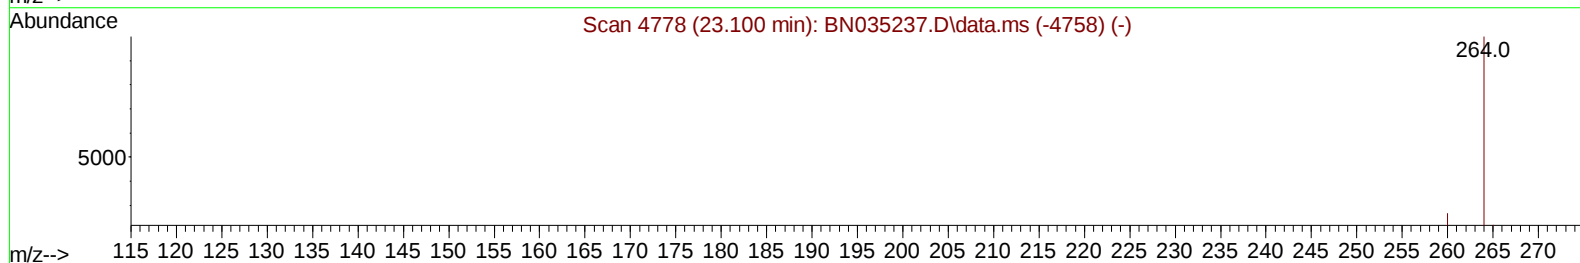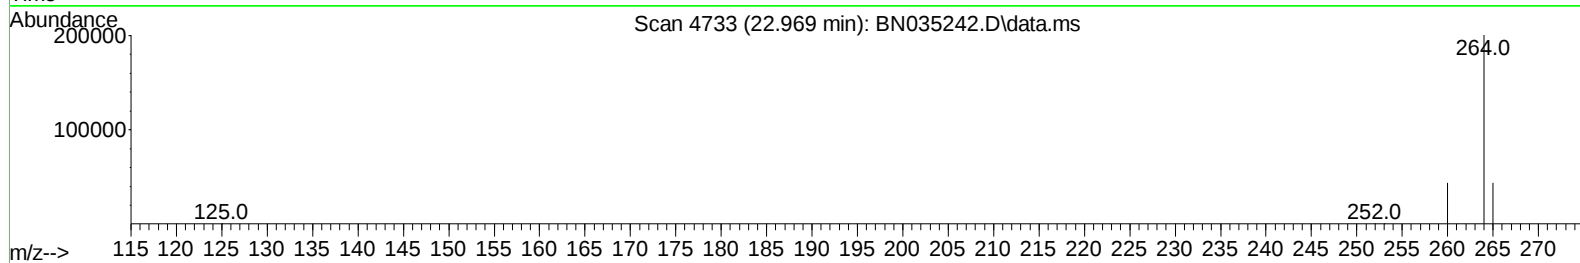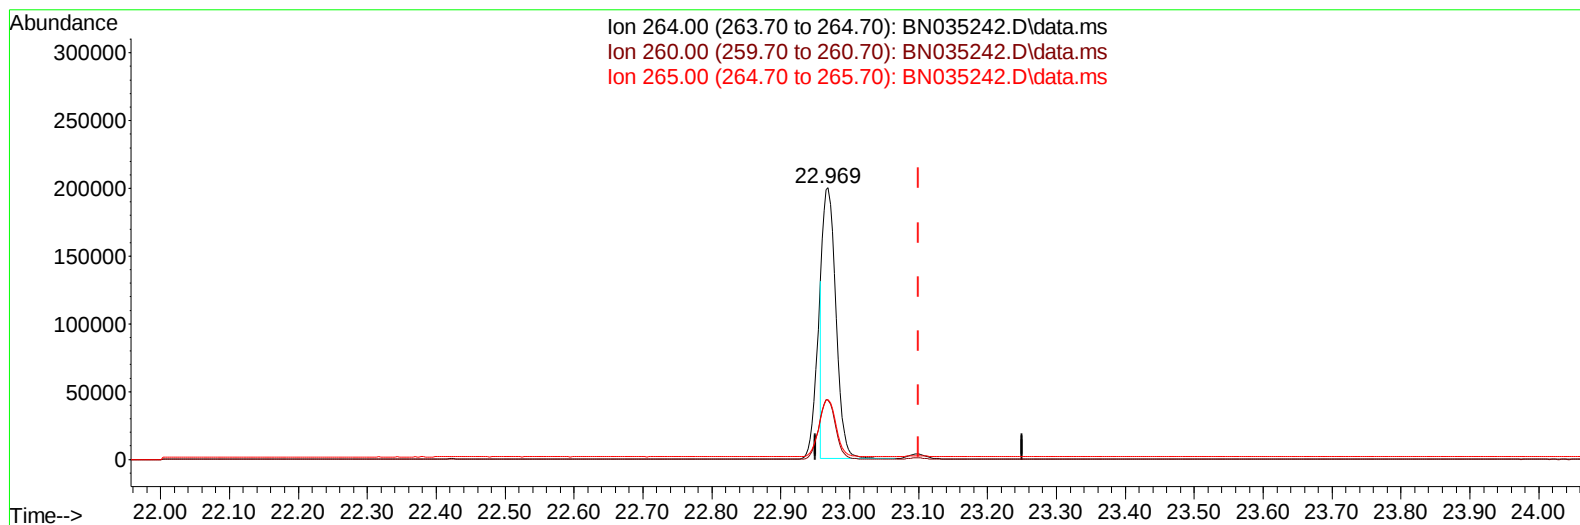

TIC: BN035242.D\data.ms

(23) Perylene-d12 (I)

22.969min (-0.132) 0.40 ng/u1

response 271307

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.78
265.00	75.50	22.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

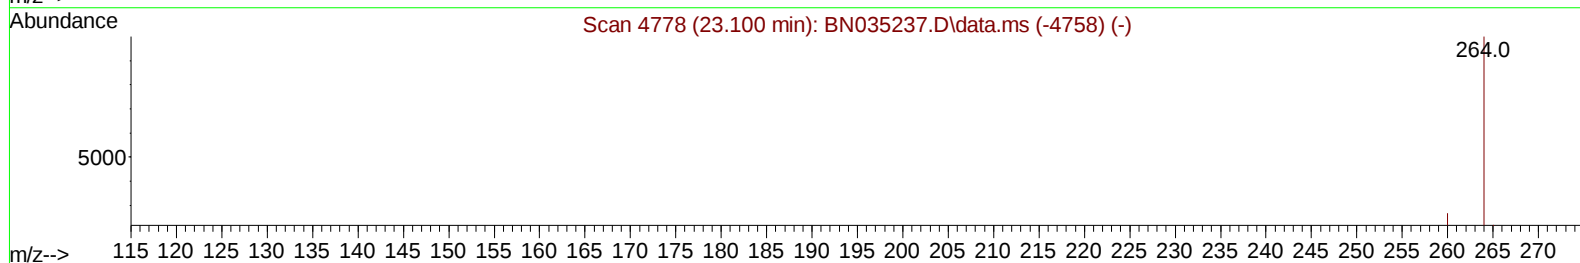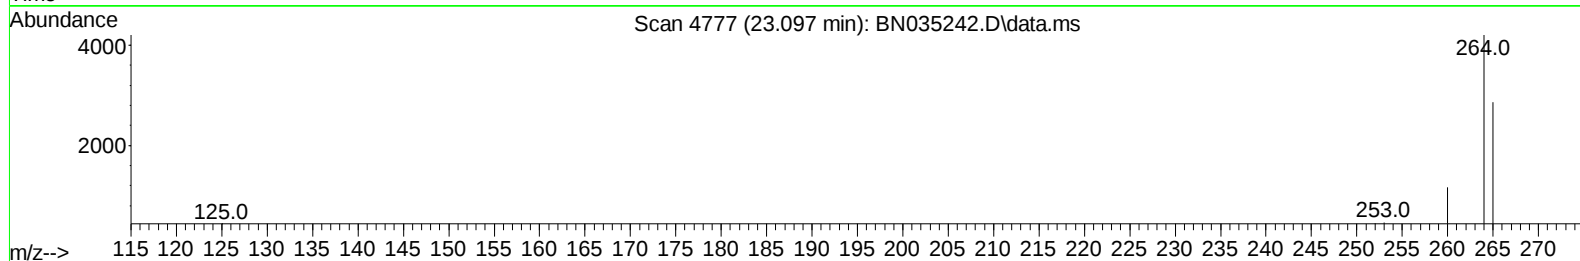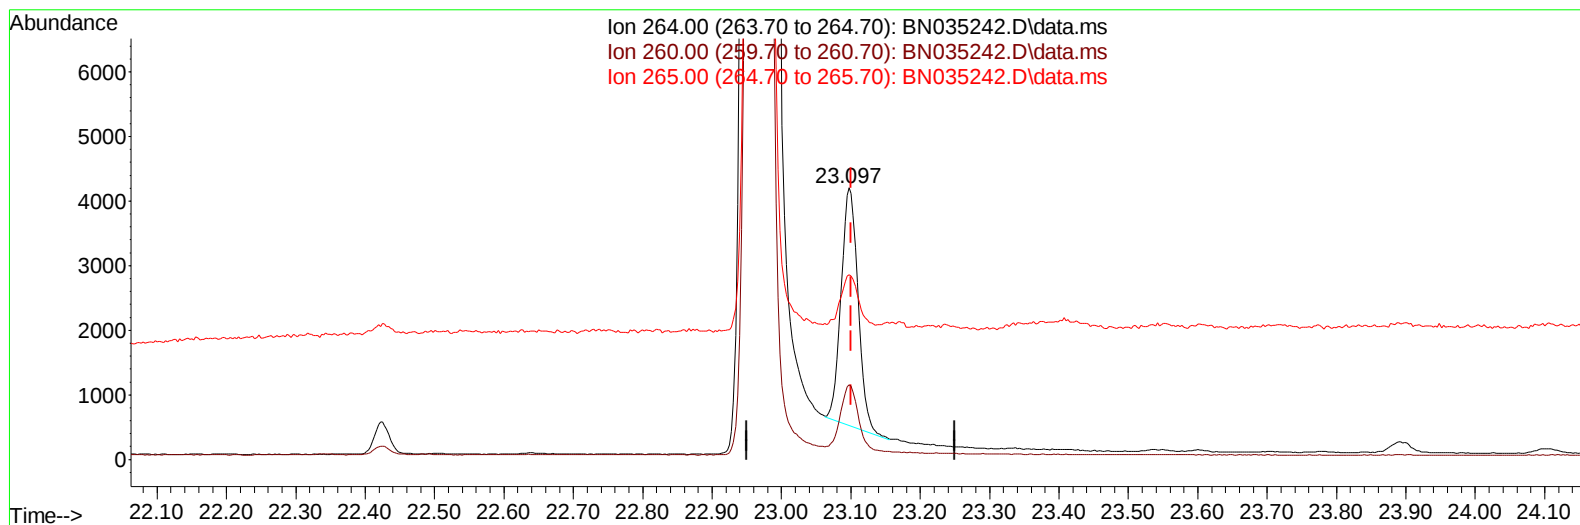

TIC: BN035242.D\data.ms

(23) Perylene-d12 (I)

23.097min (-0.003) 0.40 ng/ul m

response 6218

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.60
265.00	75.50	67.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

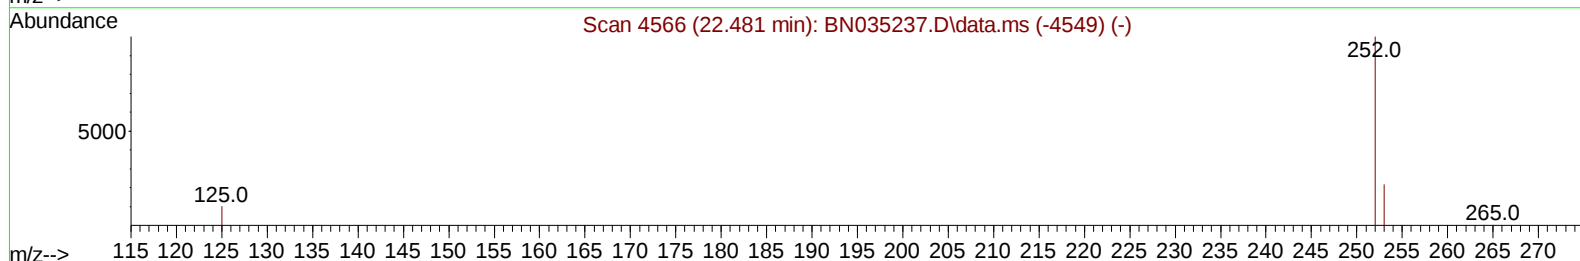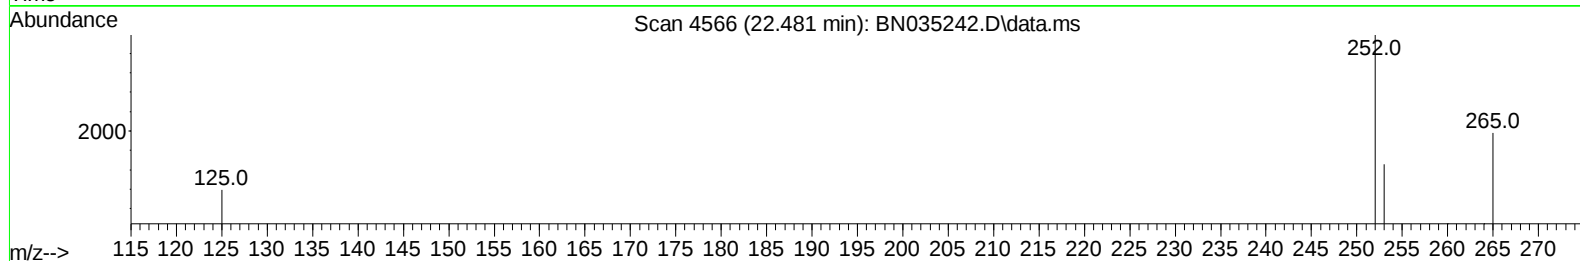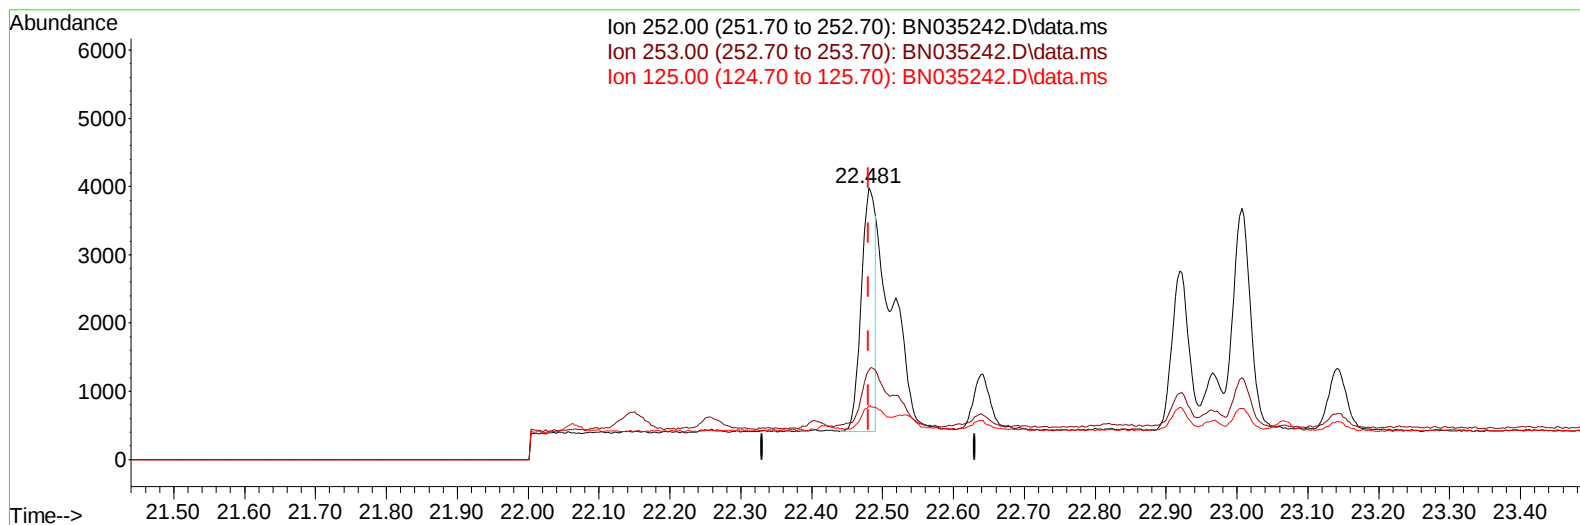

TIC: BN035242.D\data.ms

(24) Benzo(b)fluoranthene

22.481min (+ 0.000) 0.23 ng/u1

response 4733

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	33.02
125.00	9.70	19.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

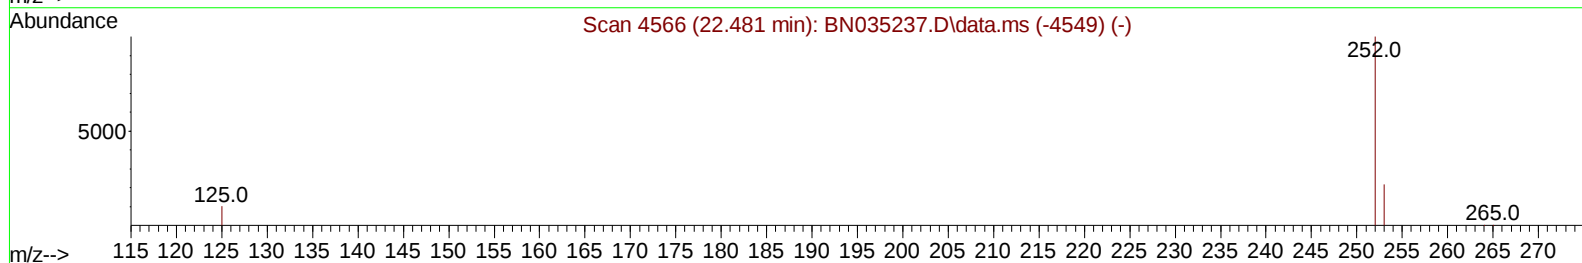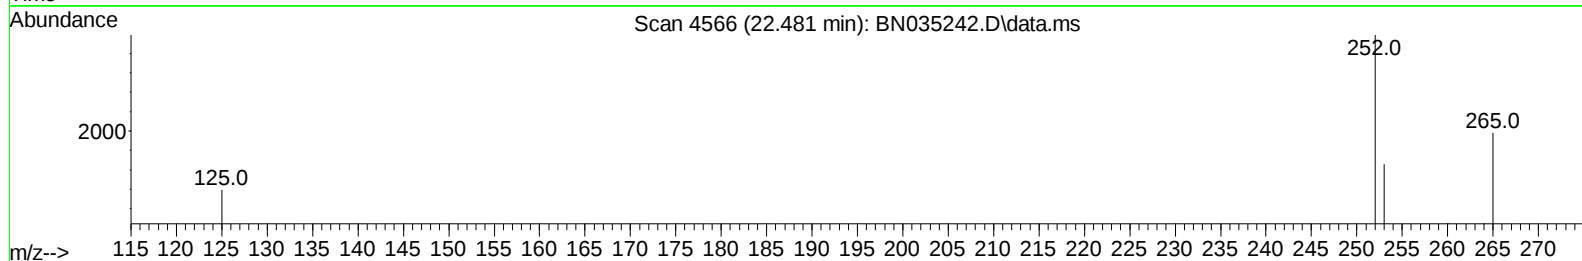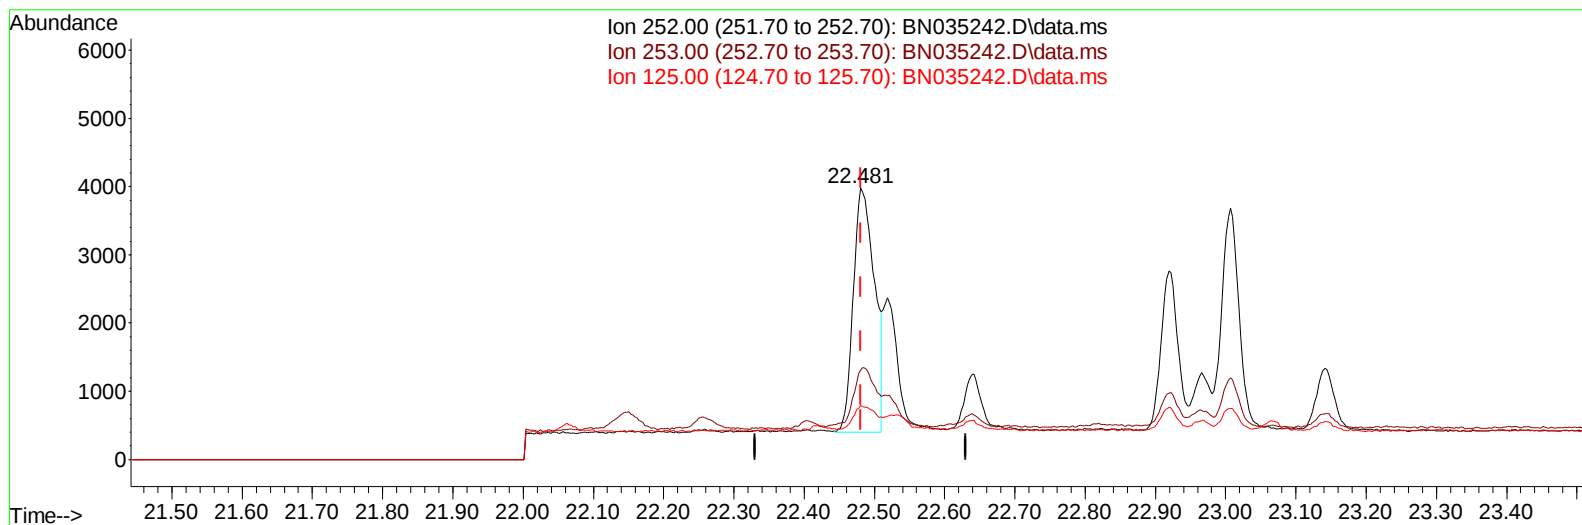

TIC: BN035242.D\data.ms

(24) Benzo(b)fluoranthene

22.481min (+ 0.000) 0.37 ng/u1 m

response 7529

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	33.02
125.00	9.70	19.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

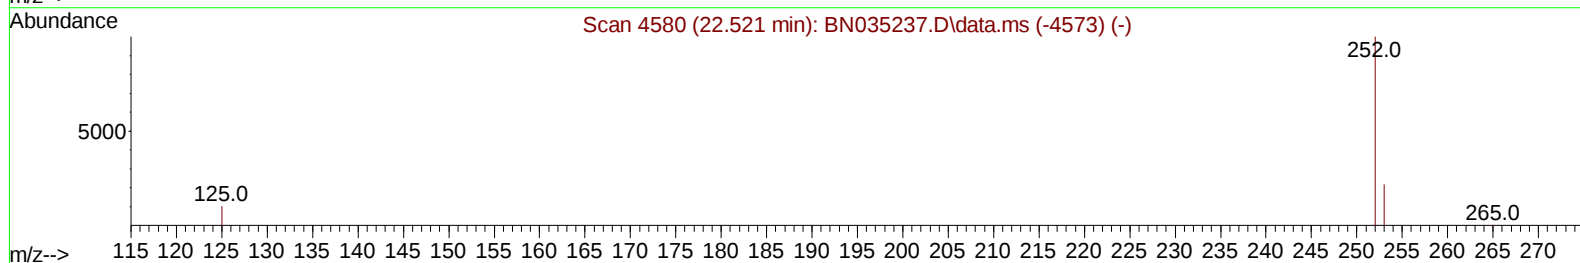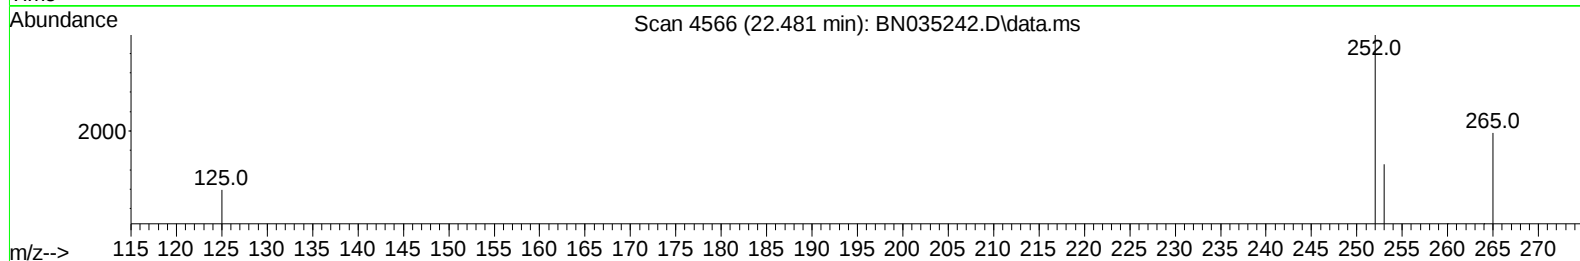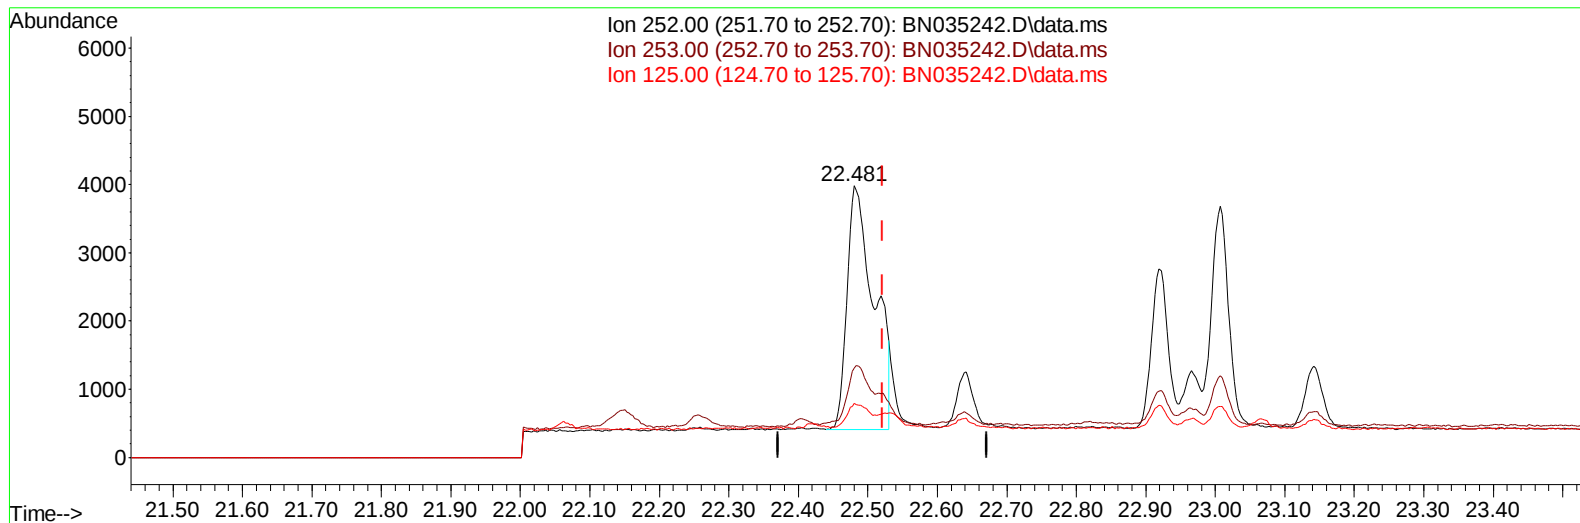

TIC: BN035242.D\data.ms

(25) Benzo(k)fluoranthene

22.481min (-0.041) 0.45 ng/u1

response 9597

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	33.02#
125.00	10.70	19.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

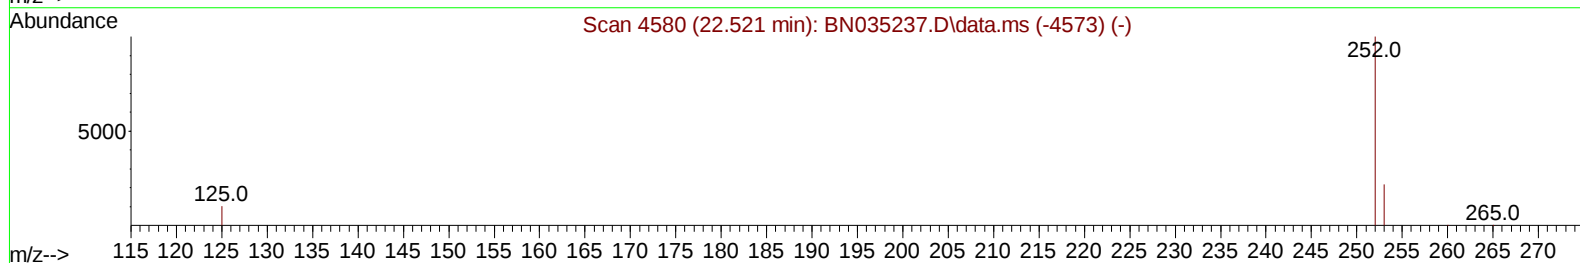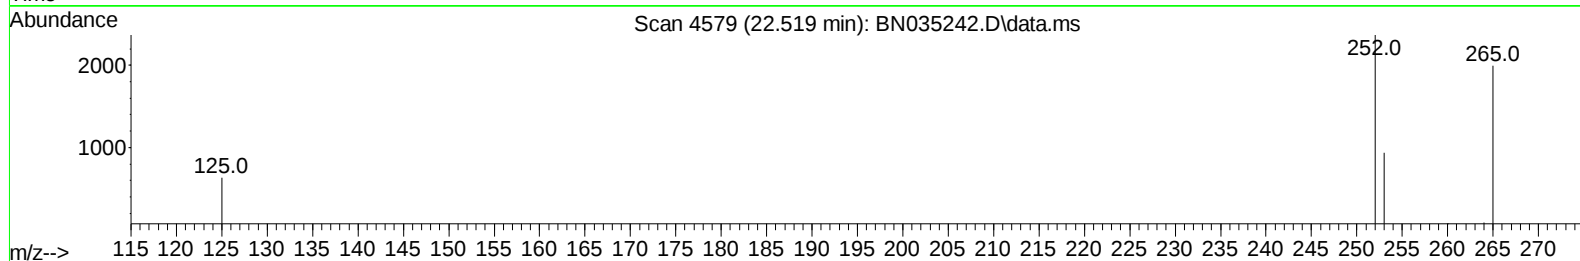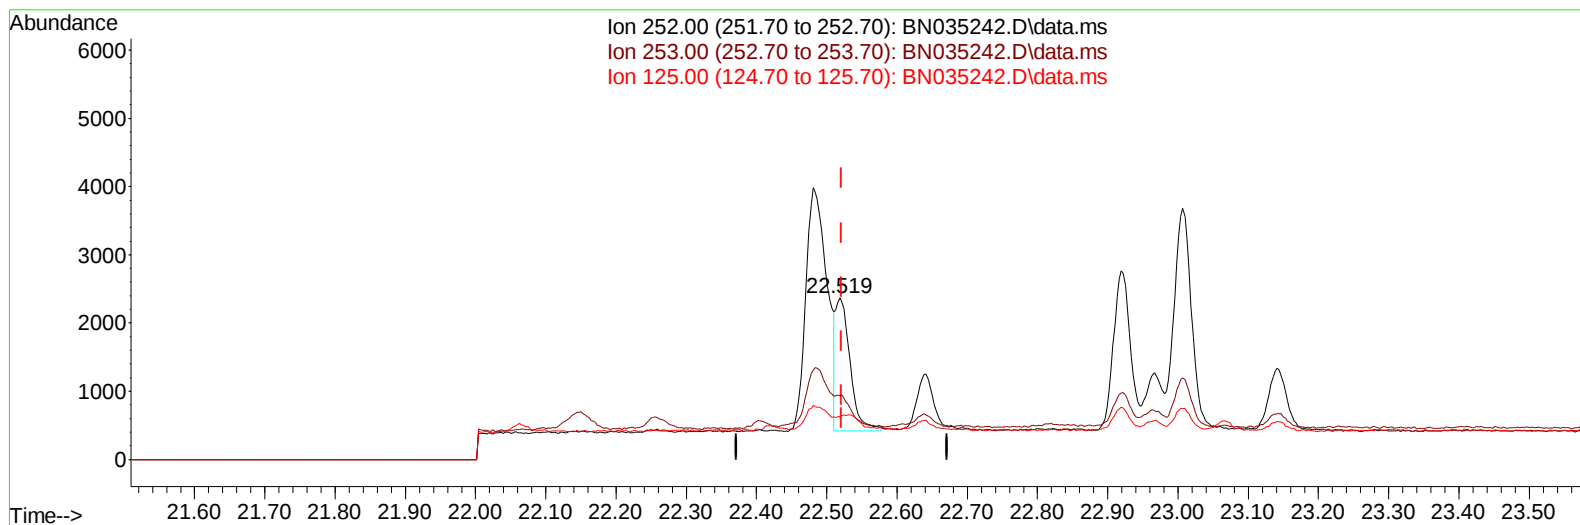

TIC: BN035242.D\data.ms

(25) Benzo(k)fluoranthene

22.519min (-0.003) 0.13 ng/u1 m

response 2795

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	39.59#
125.00	10.70	26.85#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

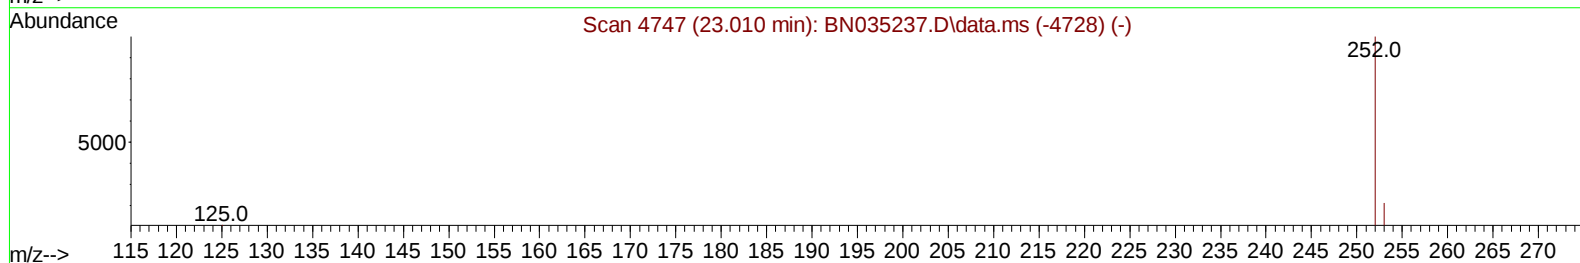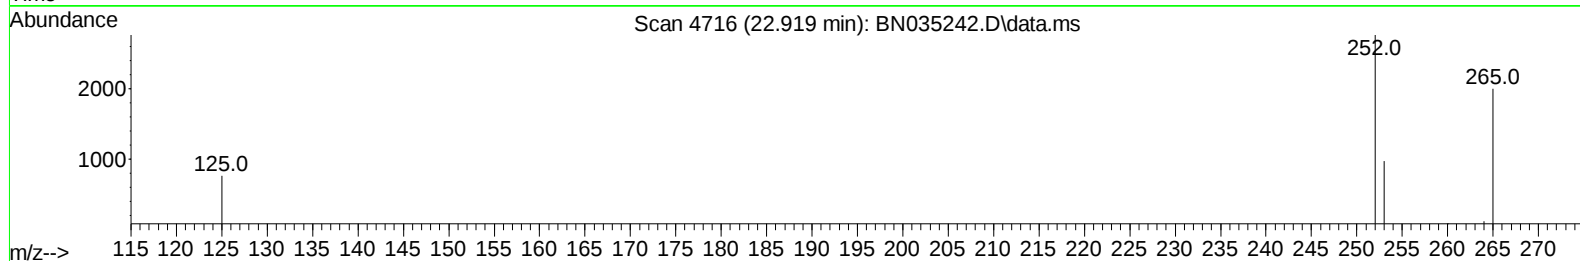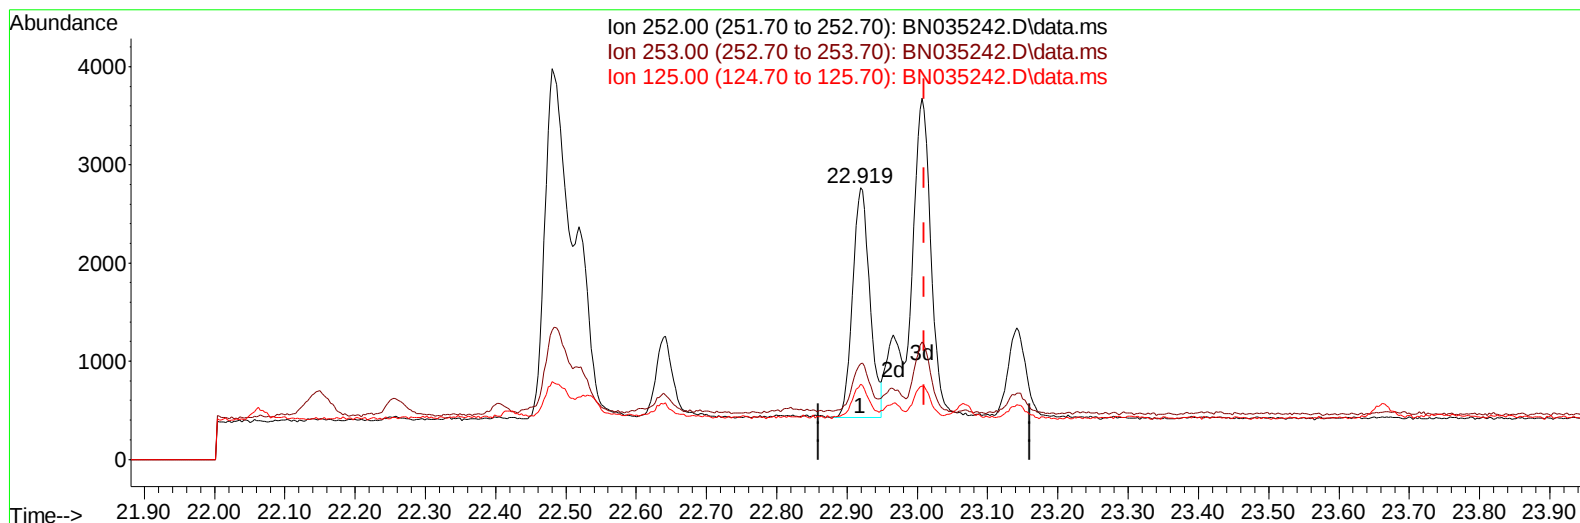

TIC: BN035242.D\data.ms

(26) Benzo(a)pyrene (C)

22.919min (-0.091) 0.21 ng/u1

response 3975

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	35.26#
125.00	11.80	27.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

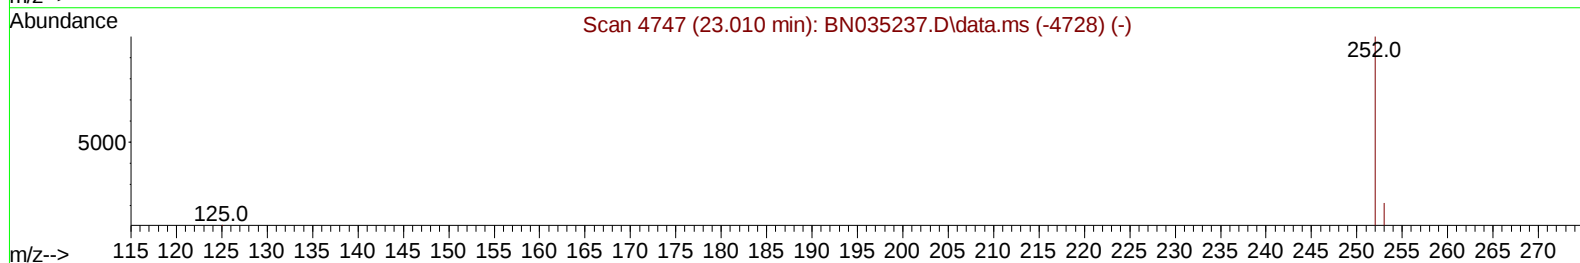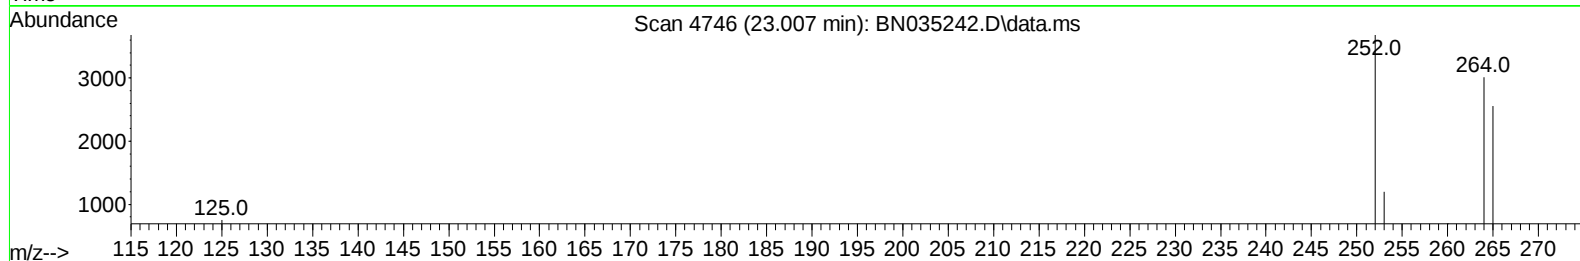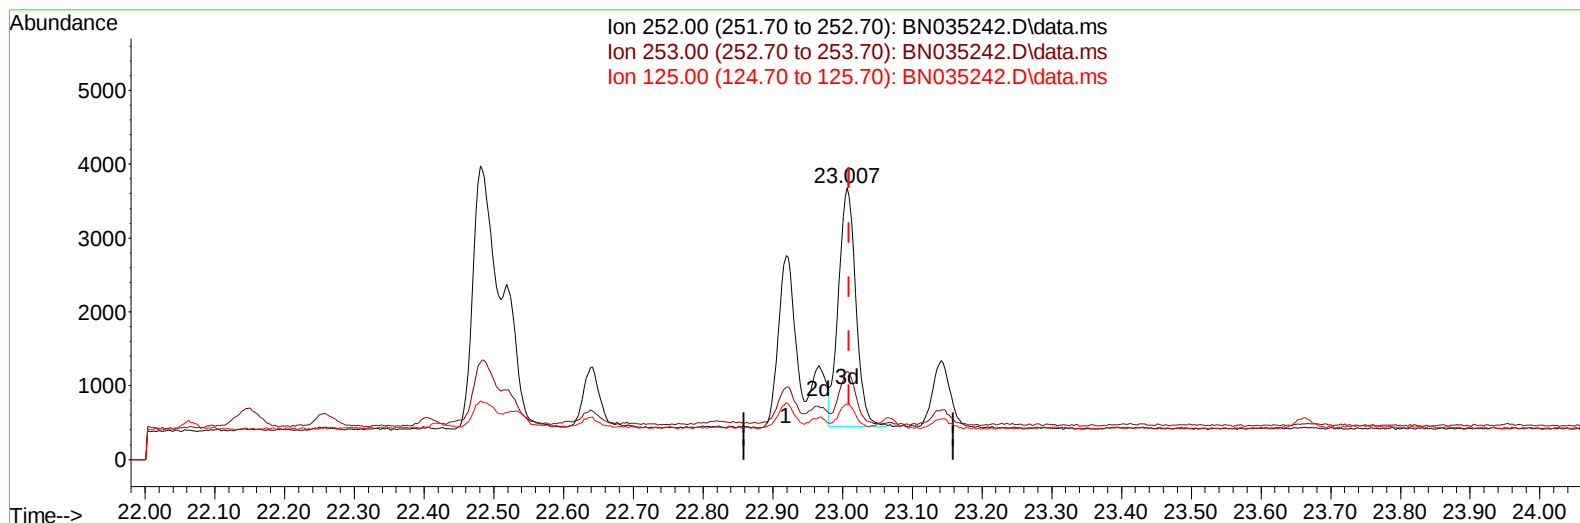

TIC: BN035242.D\data.ms

(26) Benzo(a)pyrene (C)

23.007min (-0.003) 0.30 ng/u1 m

response 5565

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	32.54
125.00	11.80	20.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

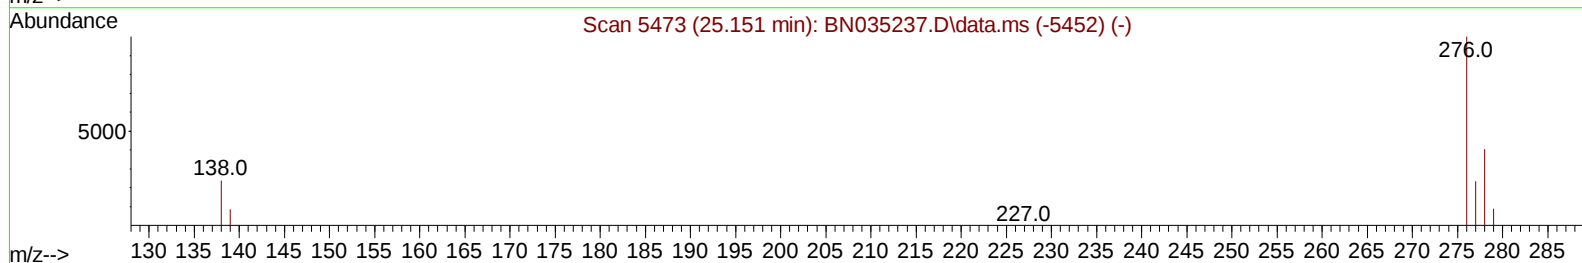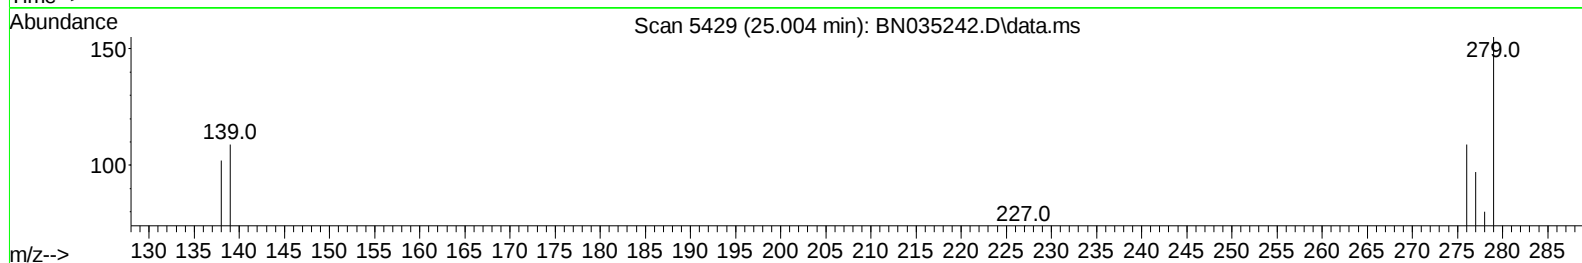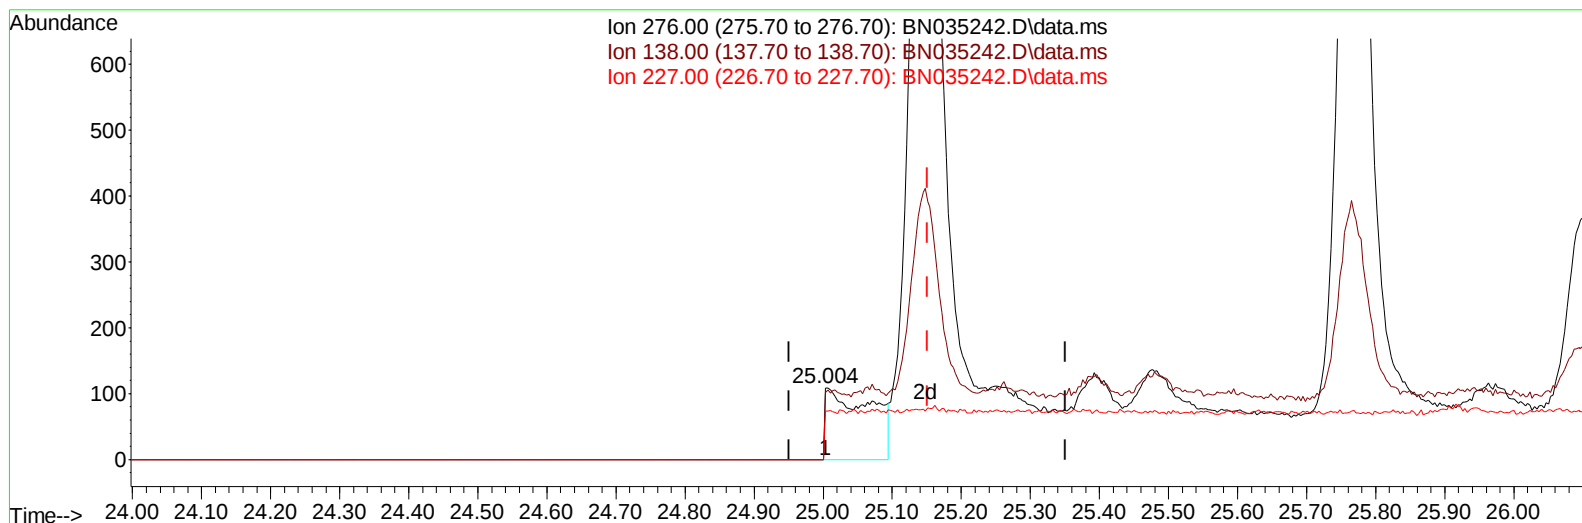

TIC: BN035242.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.004min (-0.148) 0.02 ng/u1

response 485

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	0.00#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

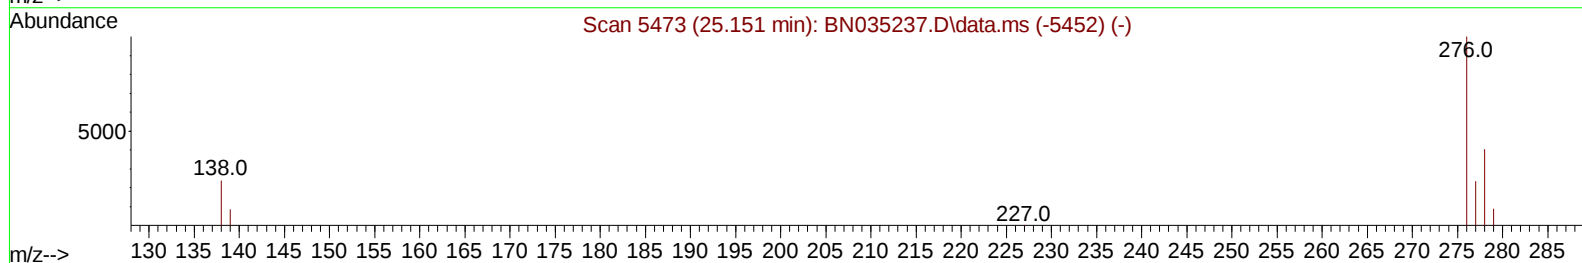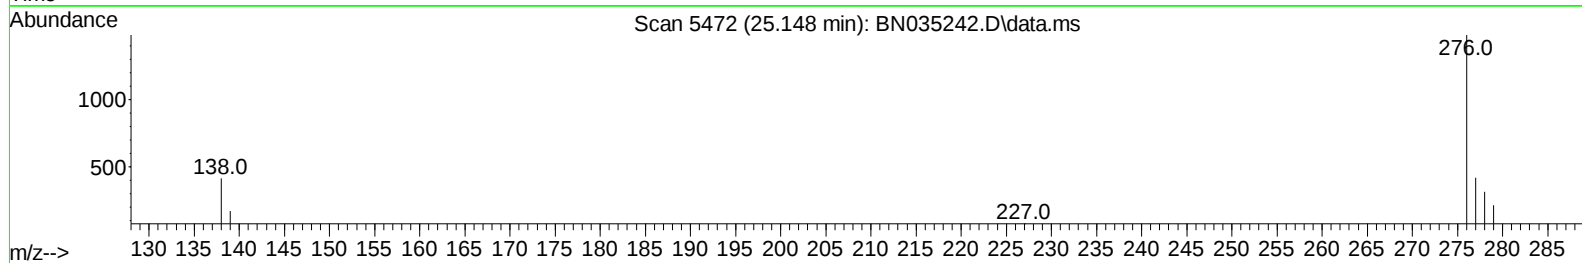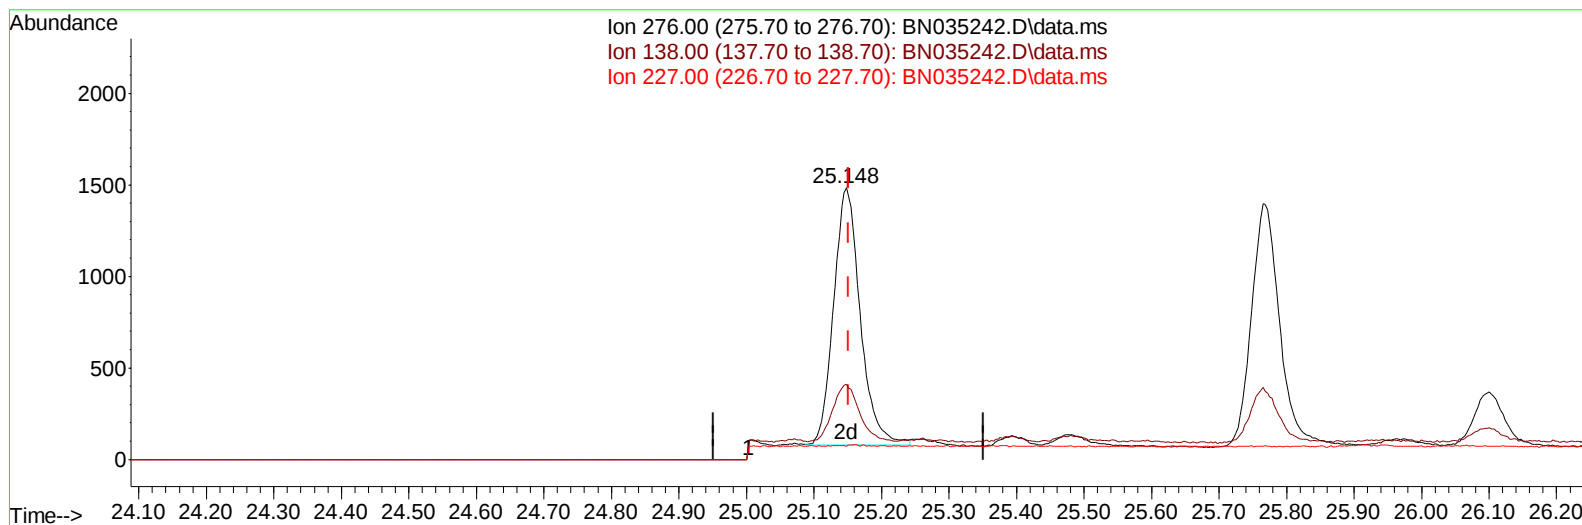

TIC: BN035242.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.148min (-0.003) 0.15 ng/u1 m

response 3853

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	0.00#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

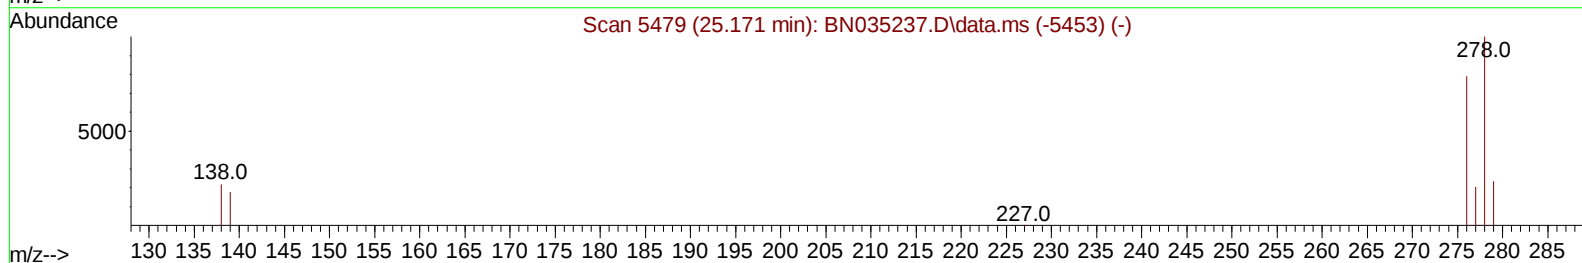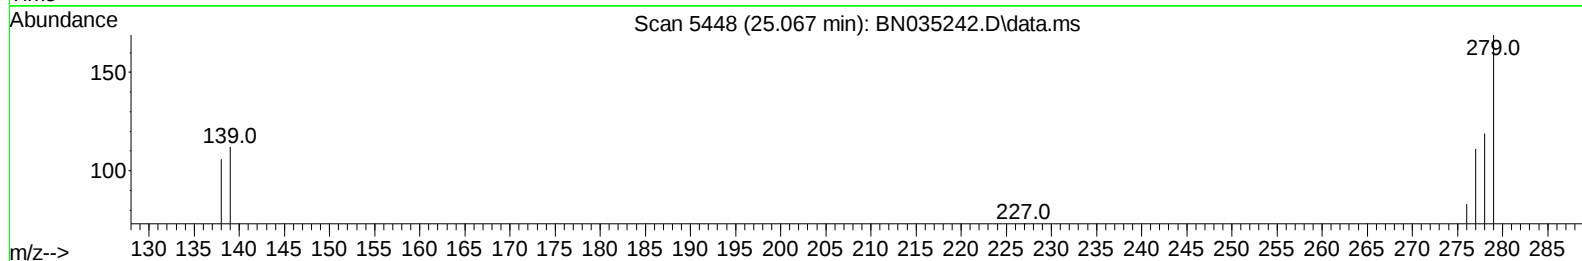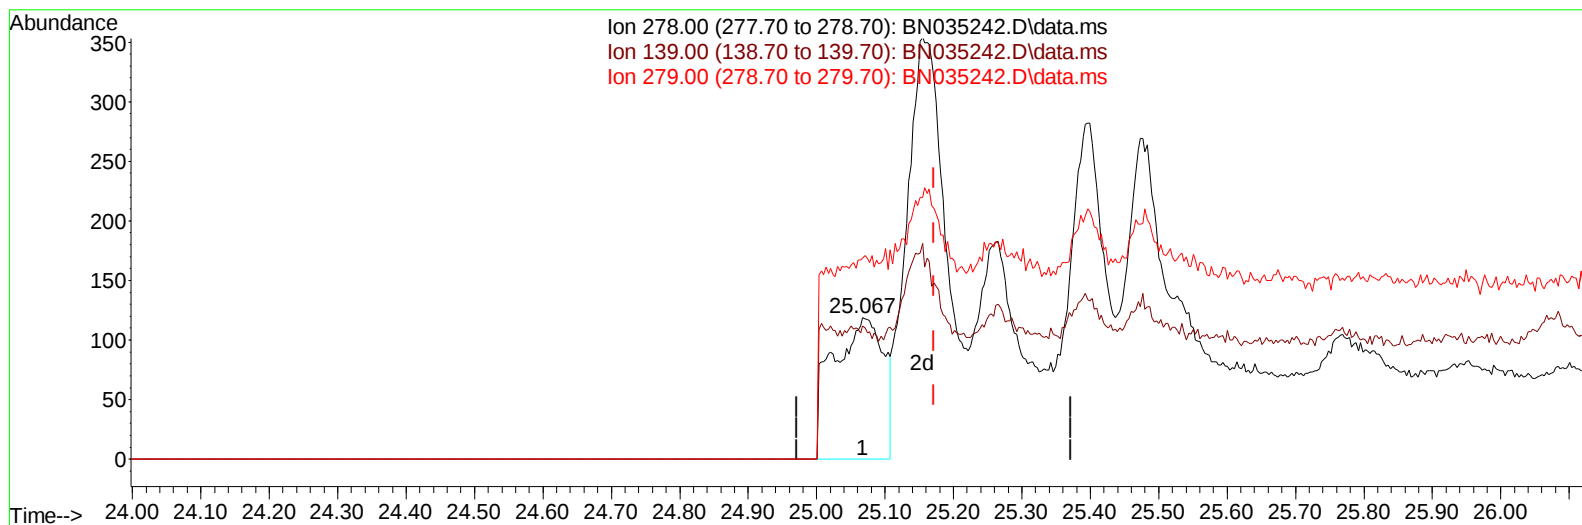

TIC: BN035242.D\data.ms

(28) Dibenzo(a,h)anthracene

25.067min (-0.104) 0.03 ng/u1

response 607

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	94.12#
279.00	28.50	142.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

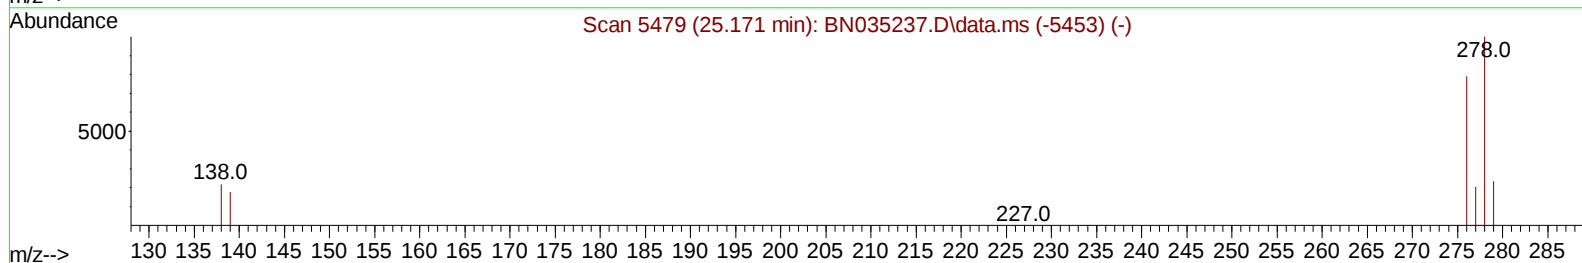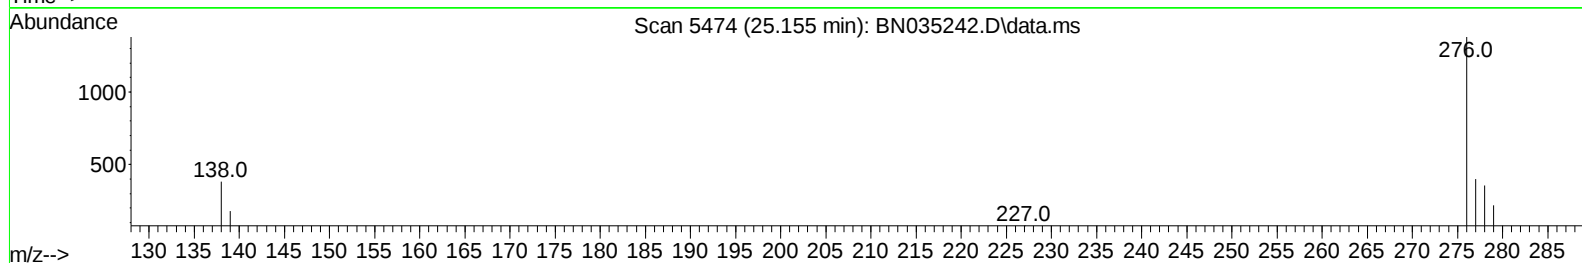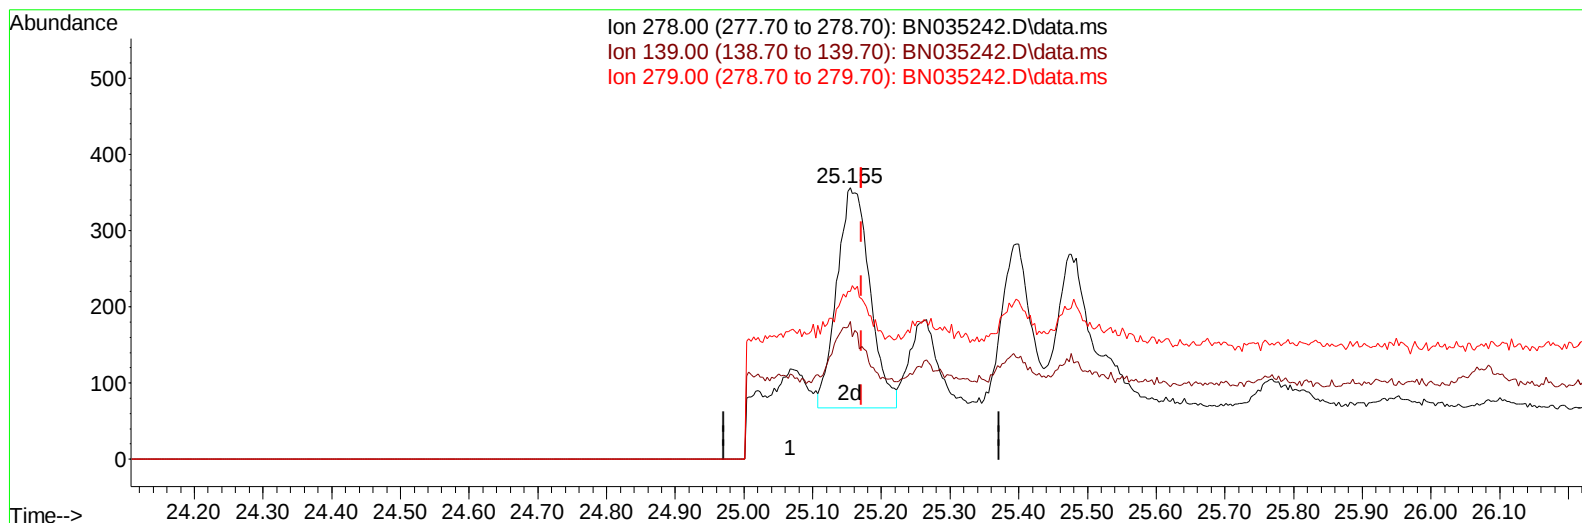

TIC: BN035242.D\data.ms

(28) Dibenzo(a,h)anthracene

25.155min (-0.017) 0.05 ng/ul m

response 968

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	50.84#
279.00	28.50	61.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

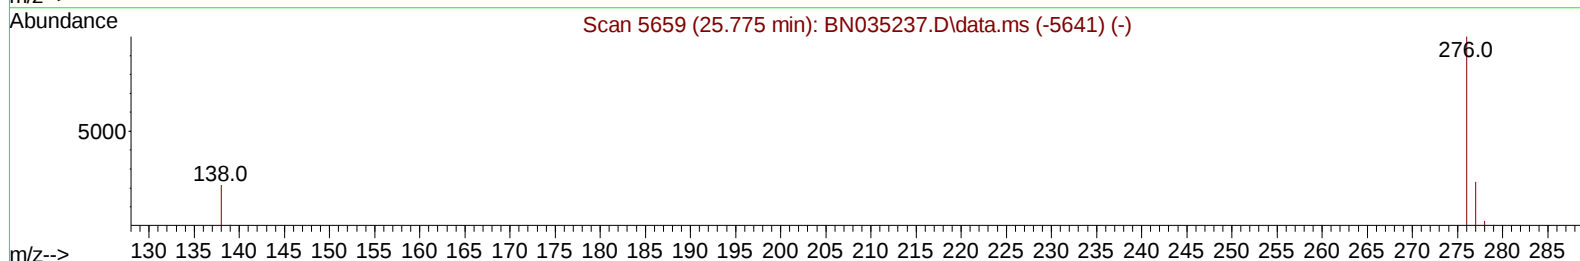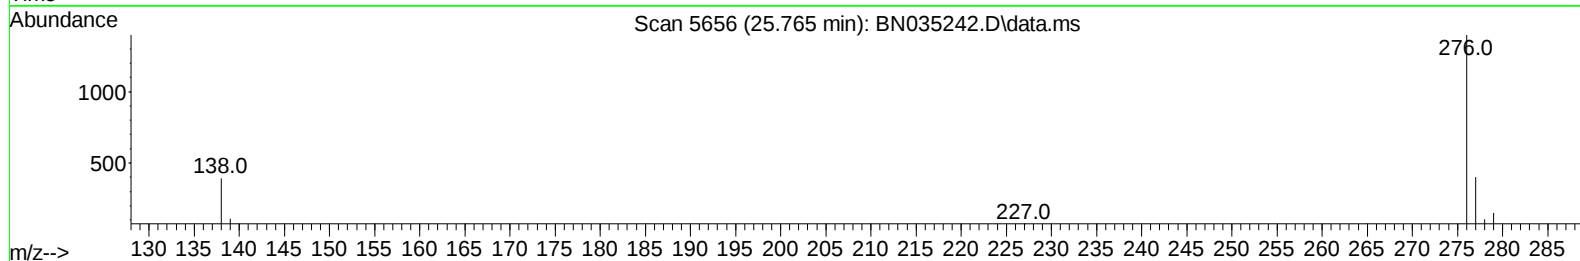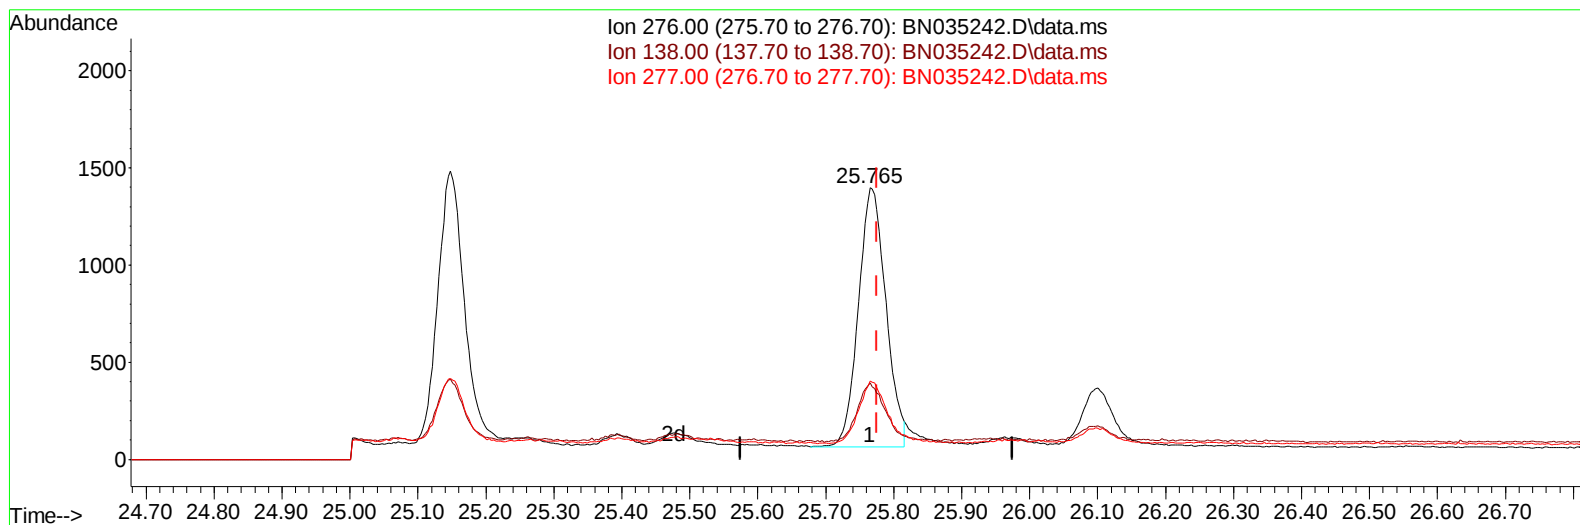

TIC: BN035242.D\data.ms

(29) Benzo(g,h,i)perylene

25.765min (-0.010) 0.19 ng/u1

response 3750

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	28.13#
277.00	25.60	28.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035242.D
 Acq On : 22 Nov 2024 15:22
 Operator : RC/JU
 Sample : P4872-22
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

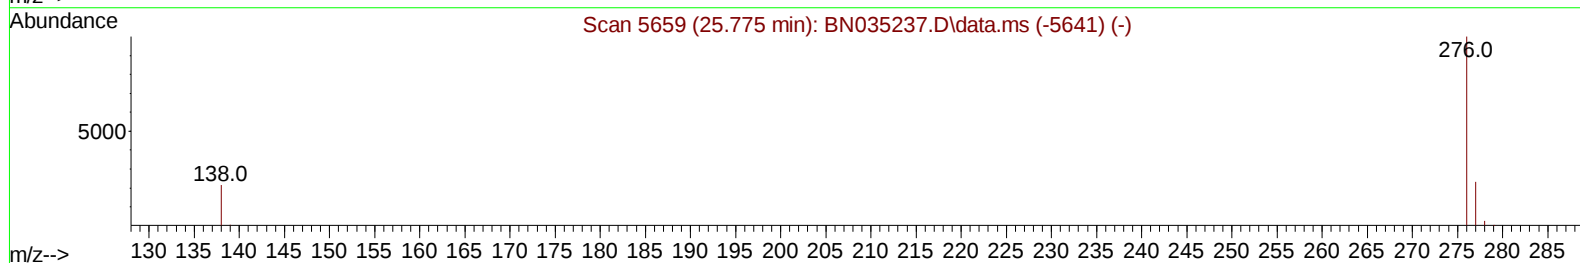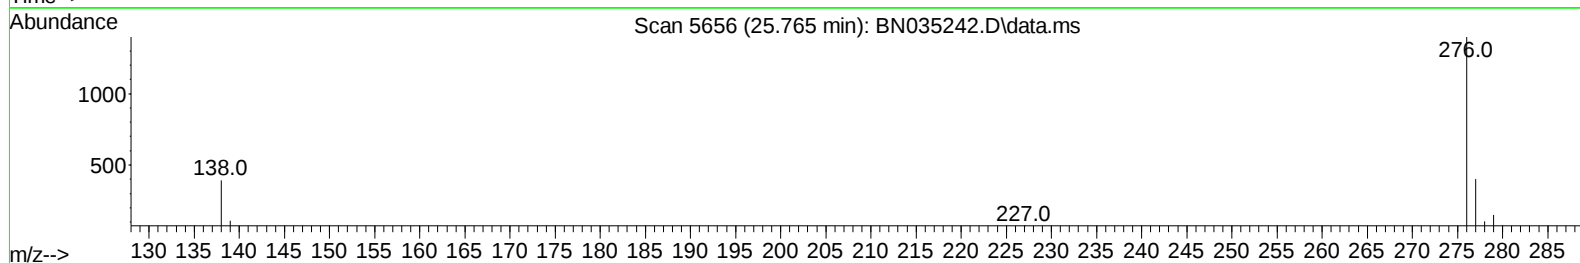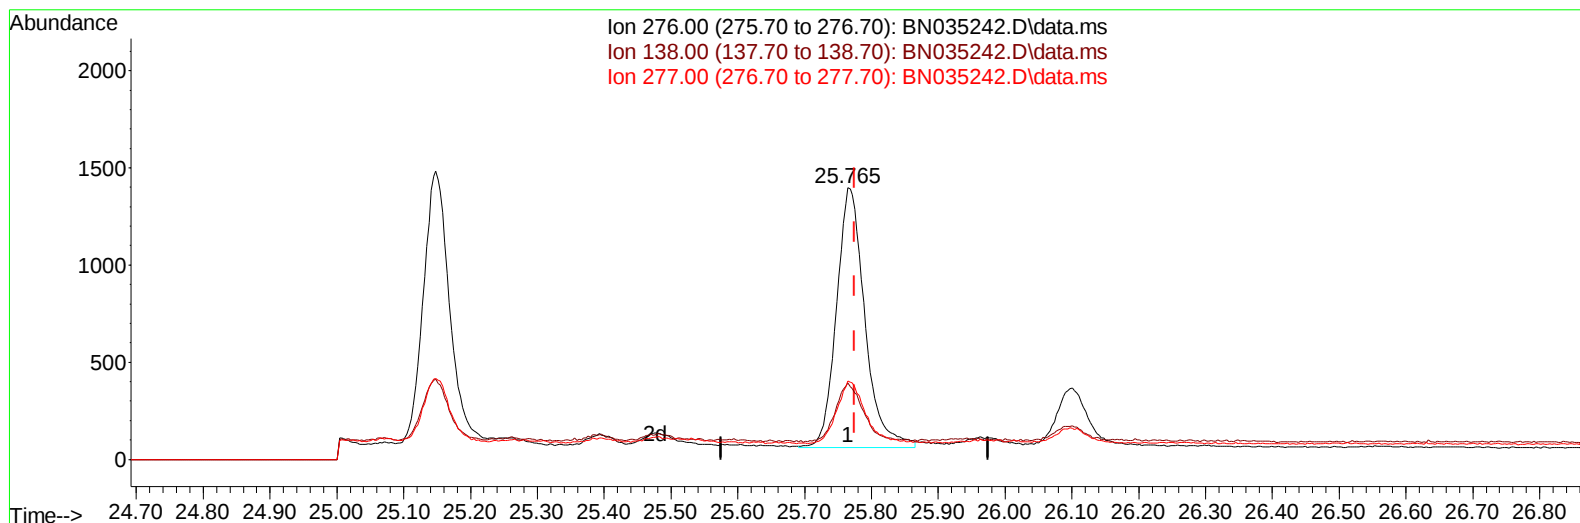

TIC: BN035242.D\data.ms

(29) Benzo(g,h,i)perylene

25.765min (-0.010) 0.20 ng/ul m

response 3940

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	28.13#
277.00	25.60	28.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035242.D
 Acq On : 22 Nov 2024 15:22
 Operator : RC/JU
 Sample : P4872-22
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.318	152		3122	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136		8322	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164		5275	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188		11579	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.993	240		7764	0.400	ng/ul	# 0.00
23) Perylene-d12	23.097	264		6218m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		7955	2.788	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152		2148	0.176	ng/ul	0.00
18) Fluoranthene-d10	18.800	212		5866	0.274	ng/ul	0.00
Target Compounds							
							Qvalue
10) Acenaphthylene	13.694	152		1604	0.077	ng/ul#	88
12) Fluorene	15.045	166		446	0.024	ng/ul#	91
15) Phenanthrene	16.789	178		5799	0.189	ng/ul	97
16) Anthracene	16.882	178		1558	0.055	ng/ul#	87
19) Fluoranthene	18.833	202		12492	0.462	ng/ul#	94
20) Pyrene	19.200	202		10805m	0.384	ng/ul	
21) Benzo(a)anthracene	20.976	228		5333m	0.198	ng/ul	
22) Chrysene	21.028	228		5573	0.206	ng/ul	96
24) Benzo(b)fluoranthene	22.481	252		7529m	0.366	ng/ul	
25) Benzo(k)fluoranthene	22.519	252		2795m	0.132	ng/ul	
26) Benzo(a)pyrene	23.007	252		5565m	0.296	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.148	276		3853m	0.152	ng/ul	
28) Dibenzo(a,h)anthracene	25.155	278		968m	0.049	ng/ul	
29) Benzo(g,h,i)perylene	25.765	276		3940m	0.197	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035242.D
Acq On : 22 Nov 2024 15:22
Operator : RC/JU
Sample : P4872-22
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 15:56:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

