




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035246.D
Acq On : 22 Nov 2024 17:46
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:31:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

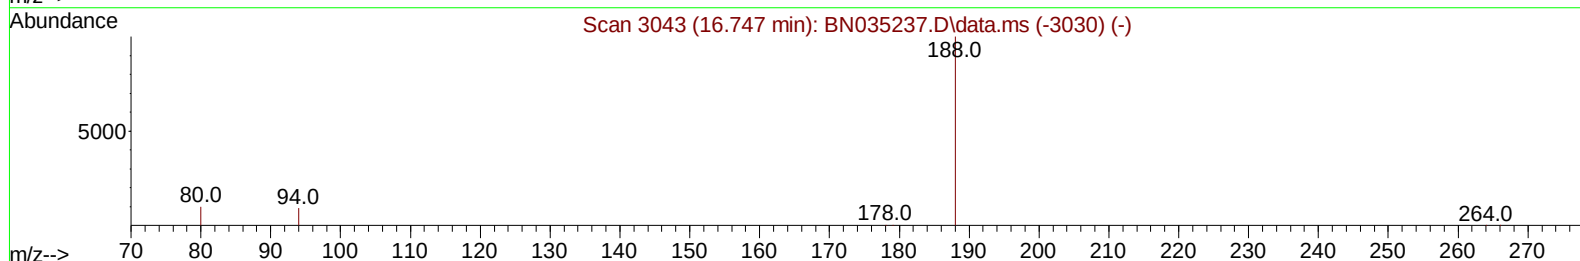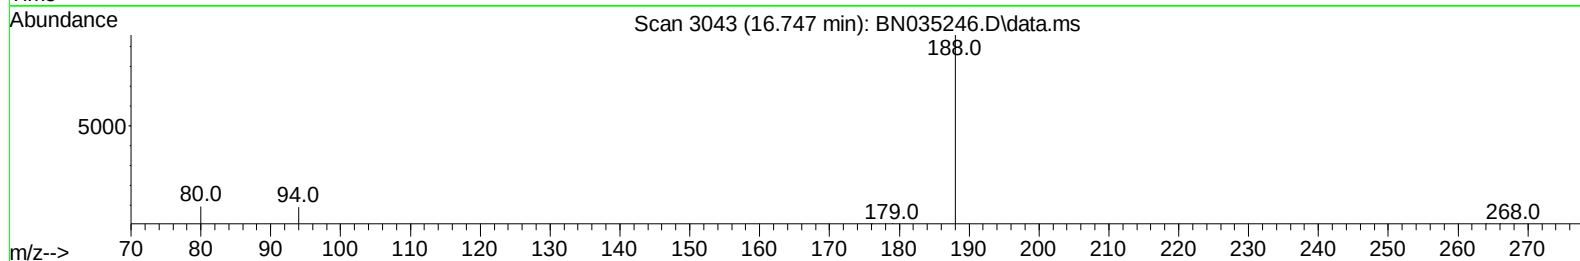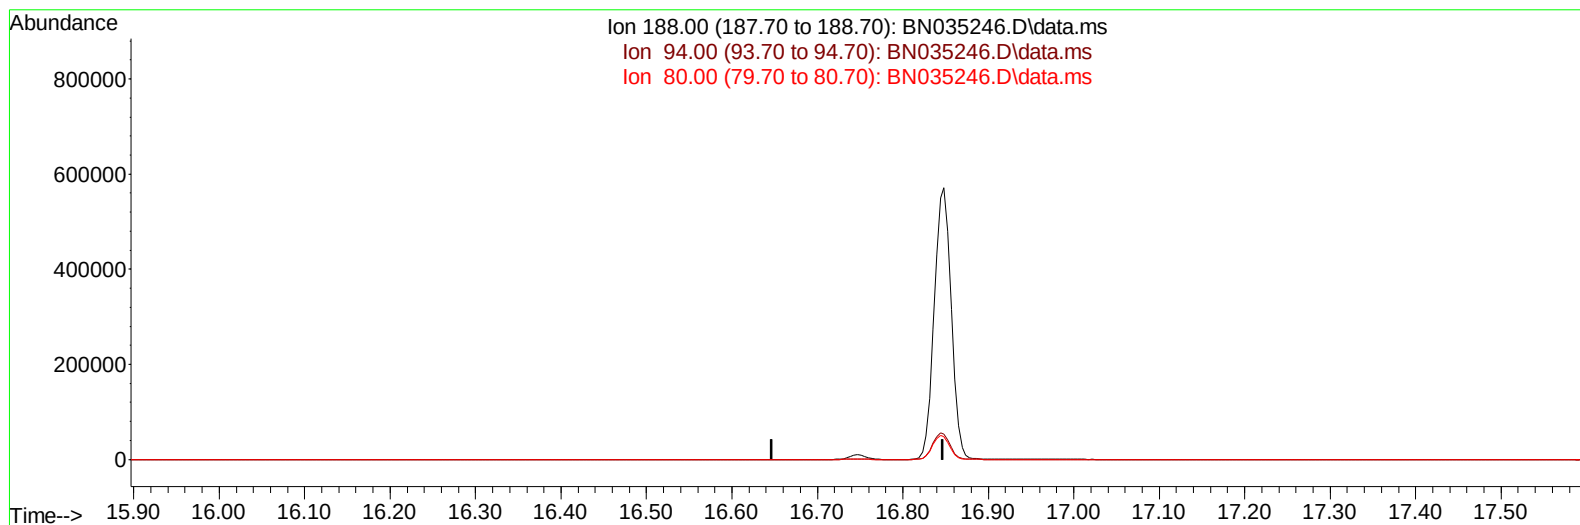

TIC: BN035246.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (-16.747) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035246.D
Acq On : 22 Nov 2024 17:46
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:31:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

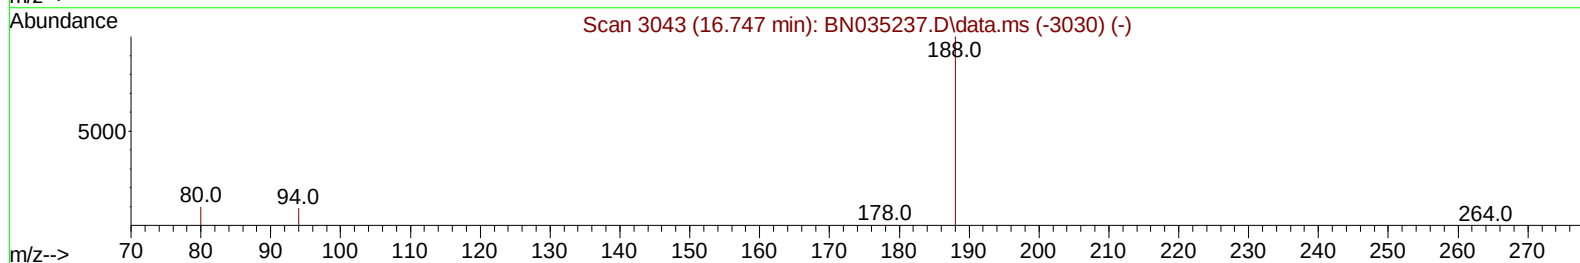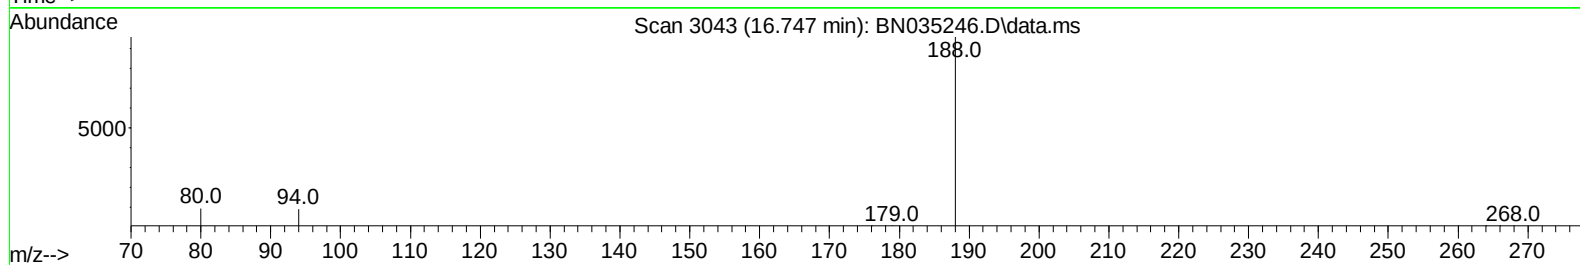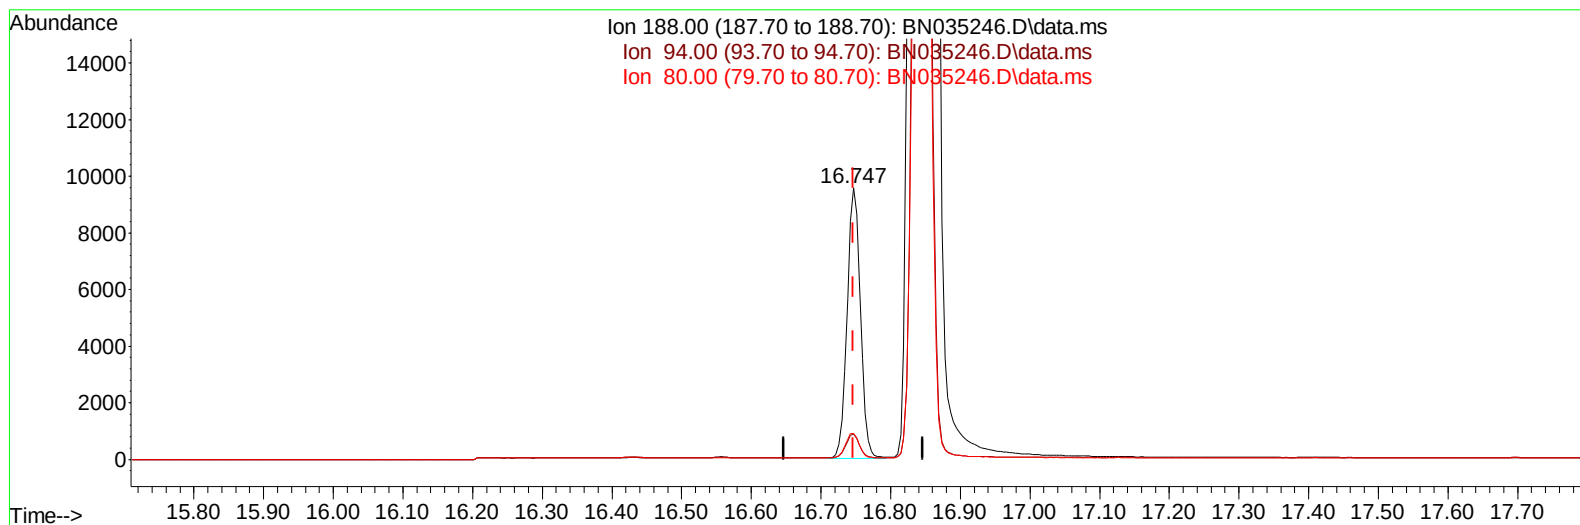

TIC: BN035246.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (+ 0.000) 0.40 ng/ul m

response 12670

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	9.35#
80.00	7.60	9.65#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035246.D
 Acq On : 22 Nov 2024 17:46
 Operator : RC/JU
 Sample : PB165200BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK200

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:31:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

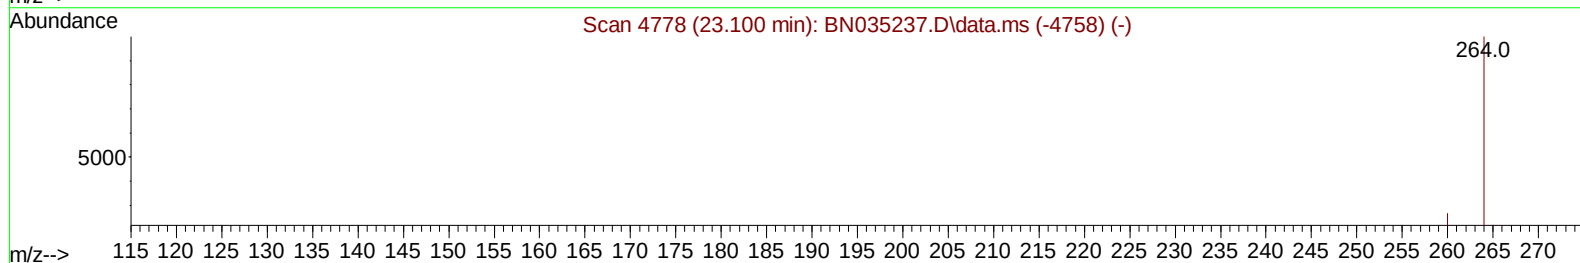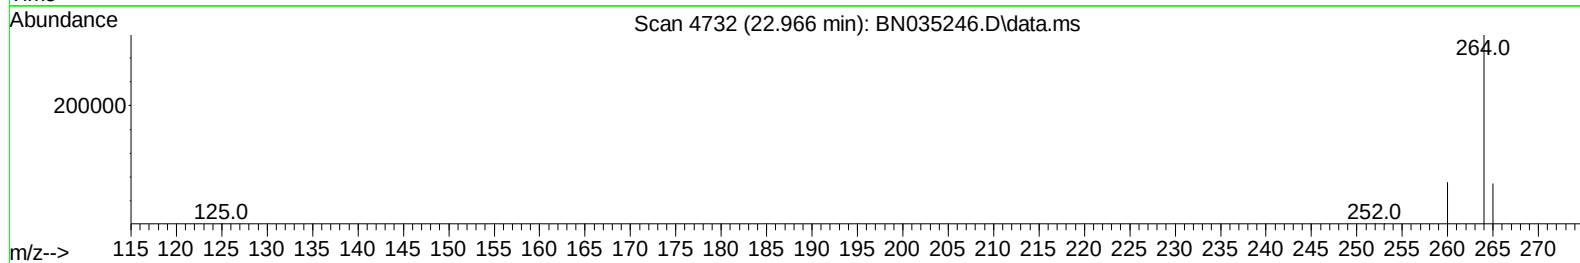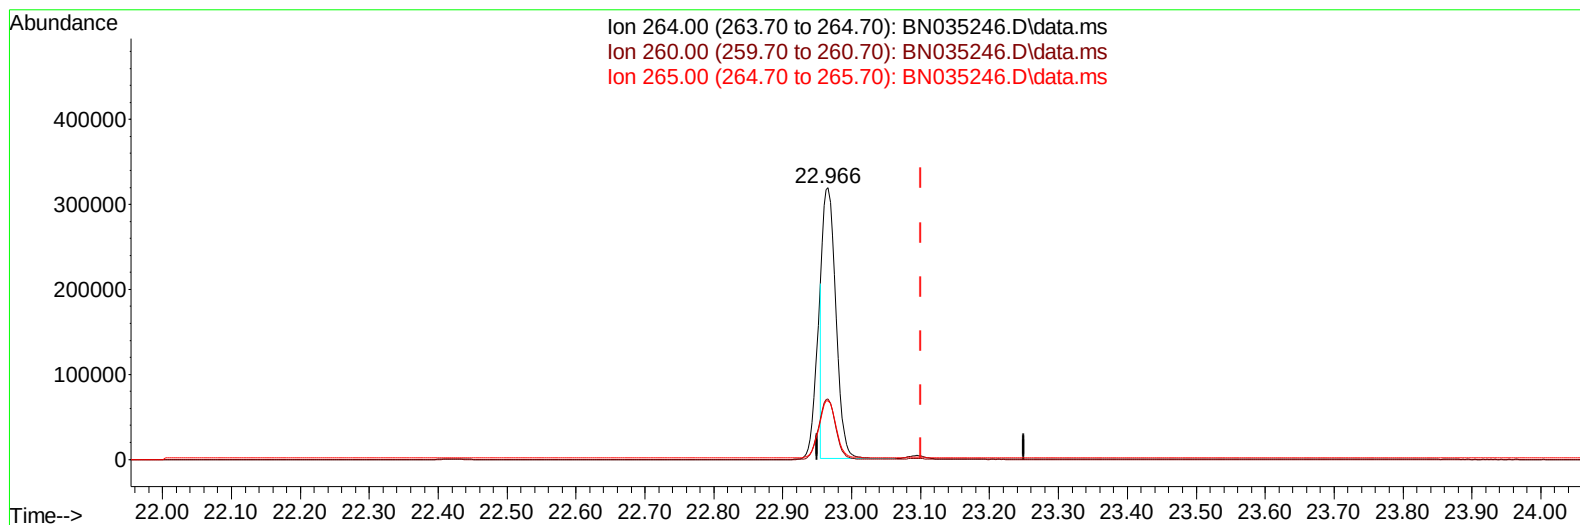

TIC: BN035246.D\data.ms

(23) Perylene-d12 (I)

22.966min (-0.134) 0.40 ng/u1

response 430982

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.23
265.00	75.50	21.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035246.D
Acq On : 22 Nov 2024 17:46
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:31:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

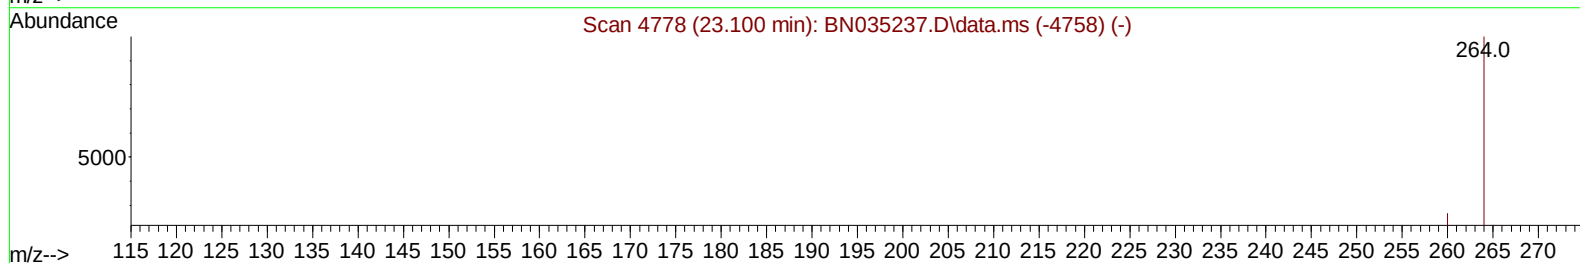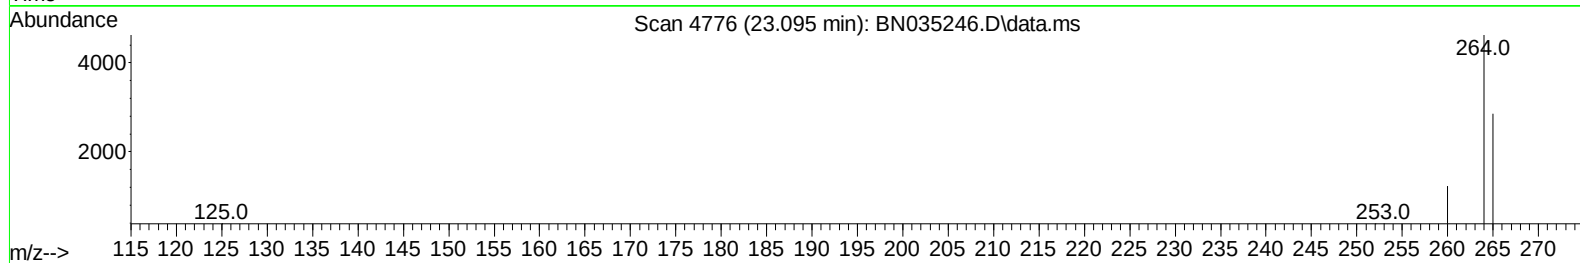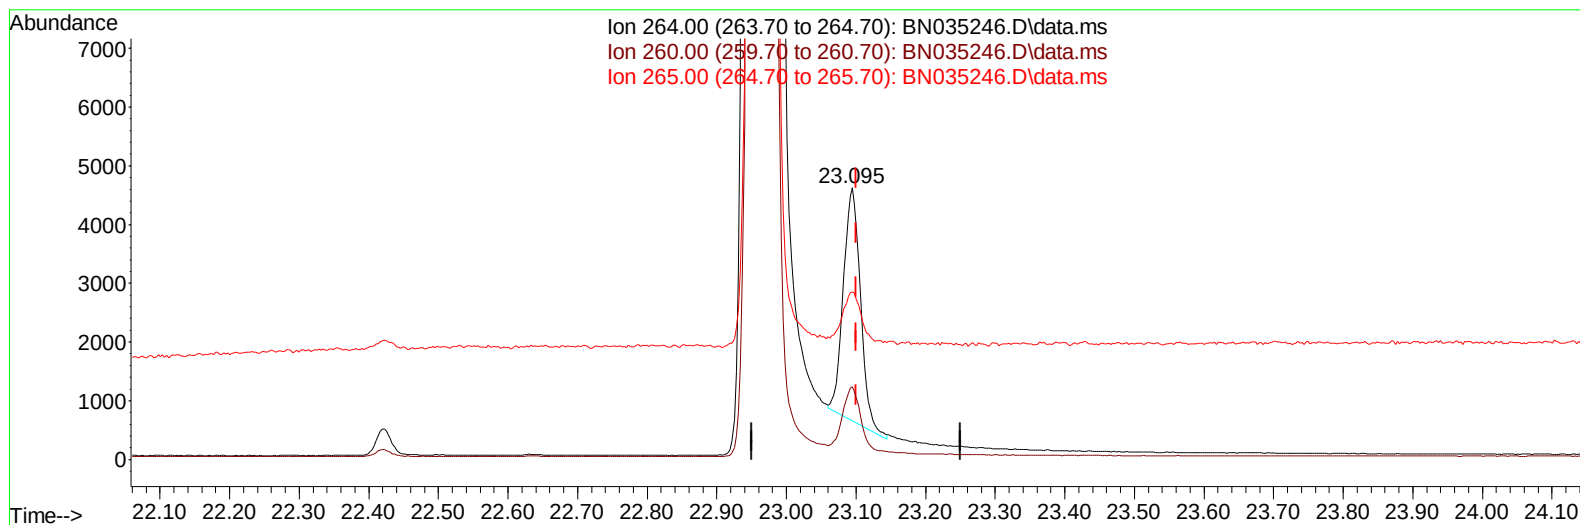

TIC: BN035246.D\data.ms

(23) Perylene-d12 (I)

23.095min (-0.006) 0.40 ng/ul m

response 6760

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.74
265.00	75.50	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035246.D
 Acq On : 22 Nov 2024 17:46
 Operator : RC/JU
 Sample : PB165200BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK200

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 22:31:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.322	152	3561	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136	9357	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164	5903	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188	12670m	0.400	ng/ul	0.00
17) Chrysene-d12	20.991	240	7822	0.400	ng/ul	# 0.00
23) Perylene-d12	23.095	264	6760m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	17775	5.461	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.675	152	4098	0.299	ng/ul	0.00
18) Fluoranthene-d10	18.800	212	9460	0.438	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035246.D
Acq On : 22 Nov 2024 17:46
Operator : RC/JU
Sample : PB165200BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK200

Manual IntegrationsAPPROVED

Quant Time: Nov 22 22:31:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

