




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035253.D
 Acq On : 22 Nov 2024 22:34
 Operator : RC/JU
 Sample : P4872-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29X9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:18:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

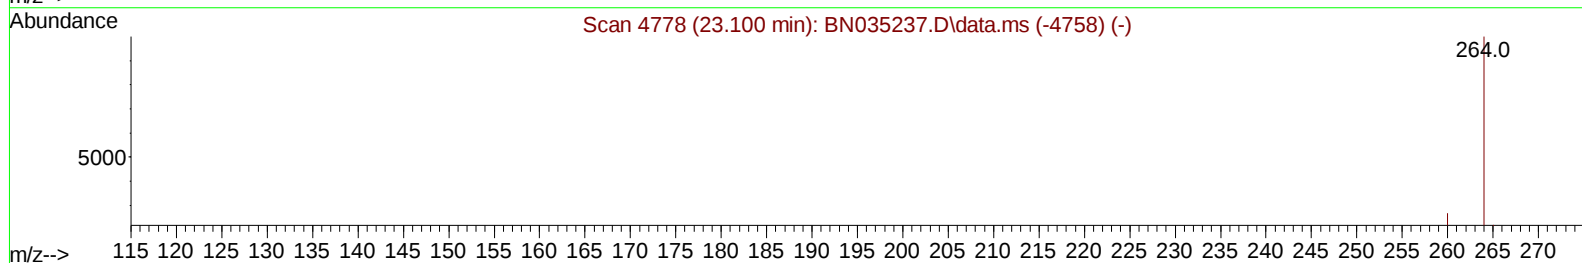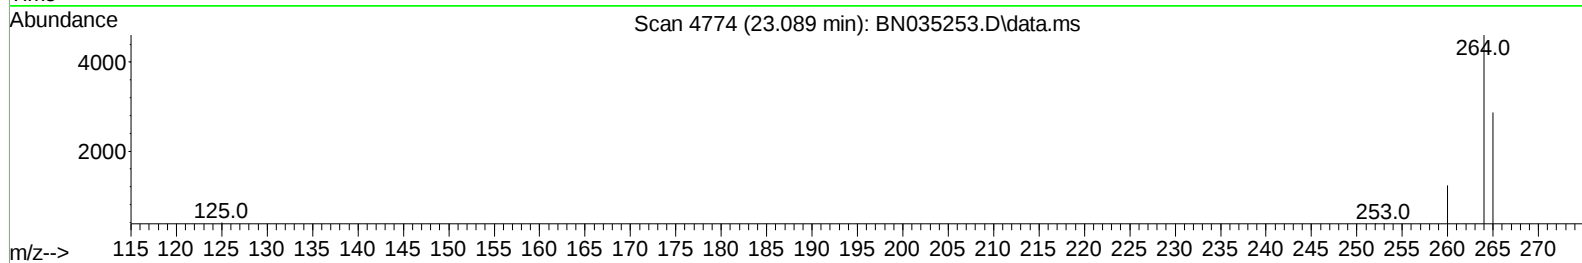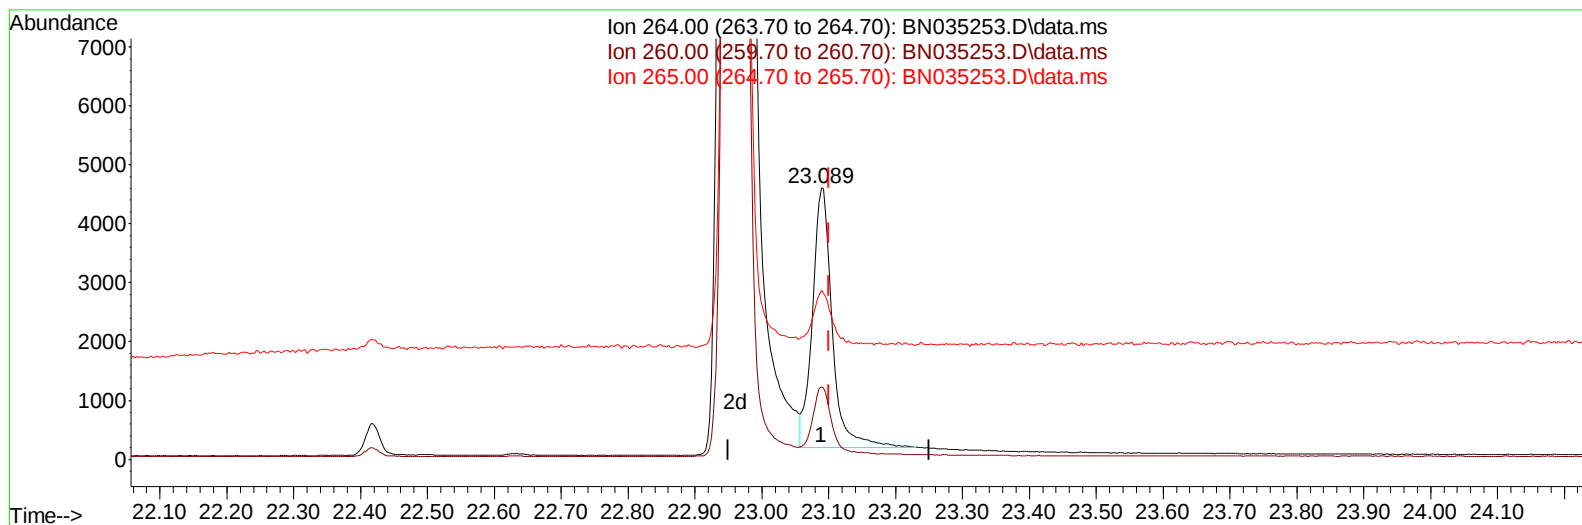

TIC: BN035253.D\data.ms

(23) Perylene-d12 (I)

23.089min (-0.012) 0.40 ng/u1

response 9008

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.84
265.00	75.50	62.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035253.D
Acq On : 22 Nov 2024 22:34
Operator : RC/JU
Sample : P4872-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29X9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:18:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

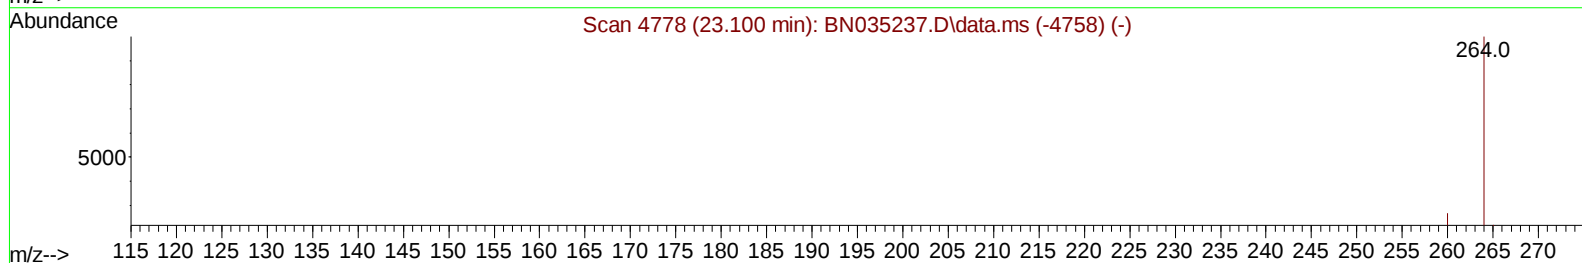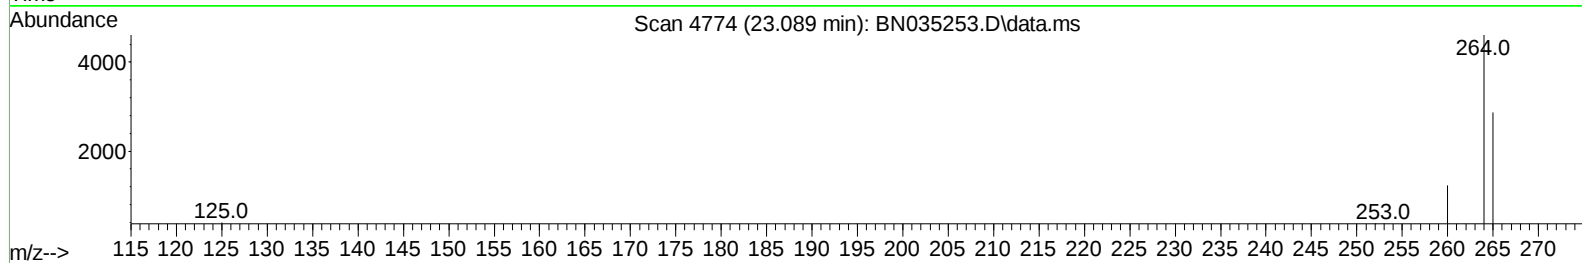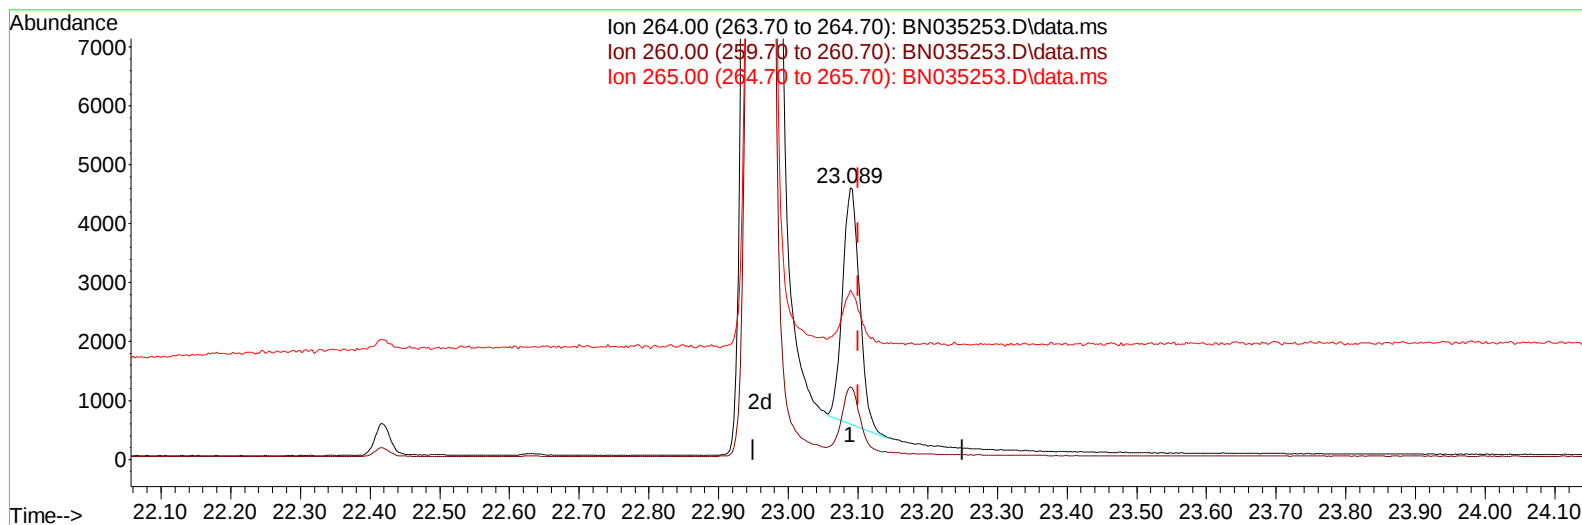

TIC: BN035253.D\data.ms

(23) Perylene-d12 (I)

23.089min (-0.012) 0.40 ng/ul m

response 6875

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.84
265.00	75.50	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035253.D
 Acq On : 22 Nov 2024 22:34
 Operator : RC/JU
 Sample : P4872-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29X9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 23:18:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.318	152	3345	0.400	ng/ul	0.00
4) Naphthalene-d8	10.070	136	8582	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164	5446	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188	12026	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.988	240	8558	0.400	ng/ul	# 0.00
23) Perylene-d12	23.089	264	6875m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.972	96	9074	2.968	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152	2363	0.188	ng/ul	0.00
18) Fluoranthene-d10	18.800	212	6223	0.264	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035253.D
Acq On : 22 Nov 2024 22:34
Operator : RC/JU
Sample : P4872-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29X9

Manual IntegrationsAPPROVED

Quant Time: Nov 22 23:18:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

