




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035254.D
Acq On : 22 Nov 2024 23:10
Operator : RC/JU
Sample : P4872-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 23 00:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

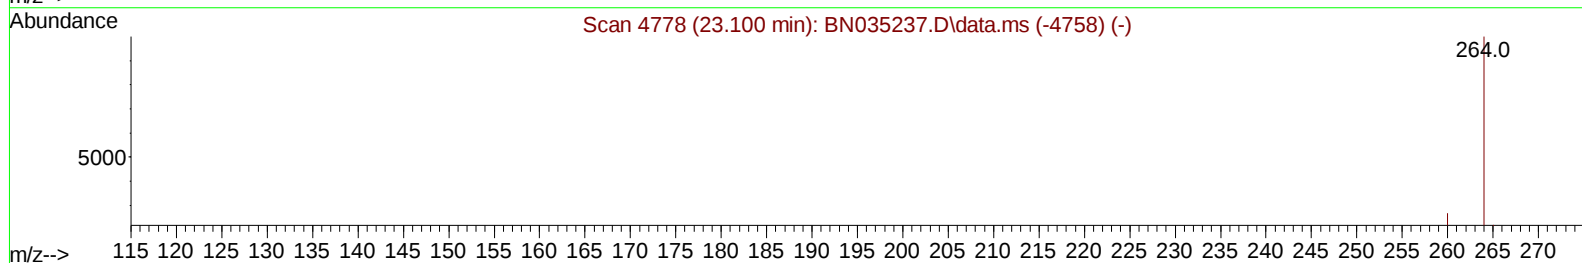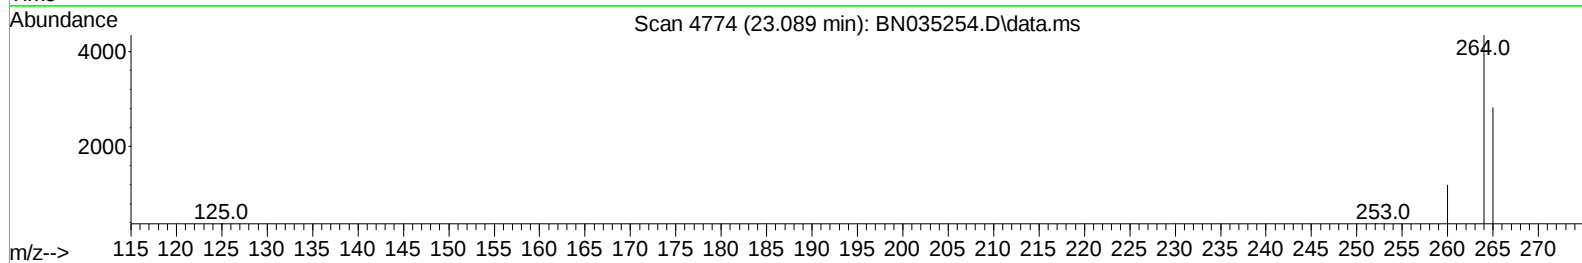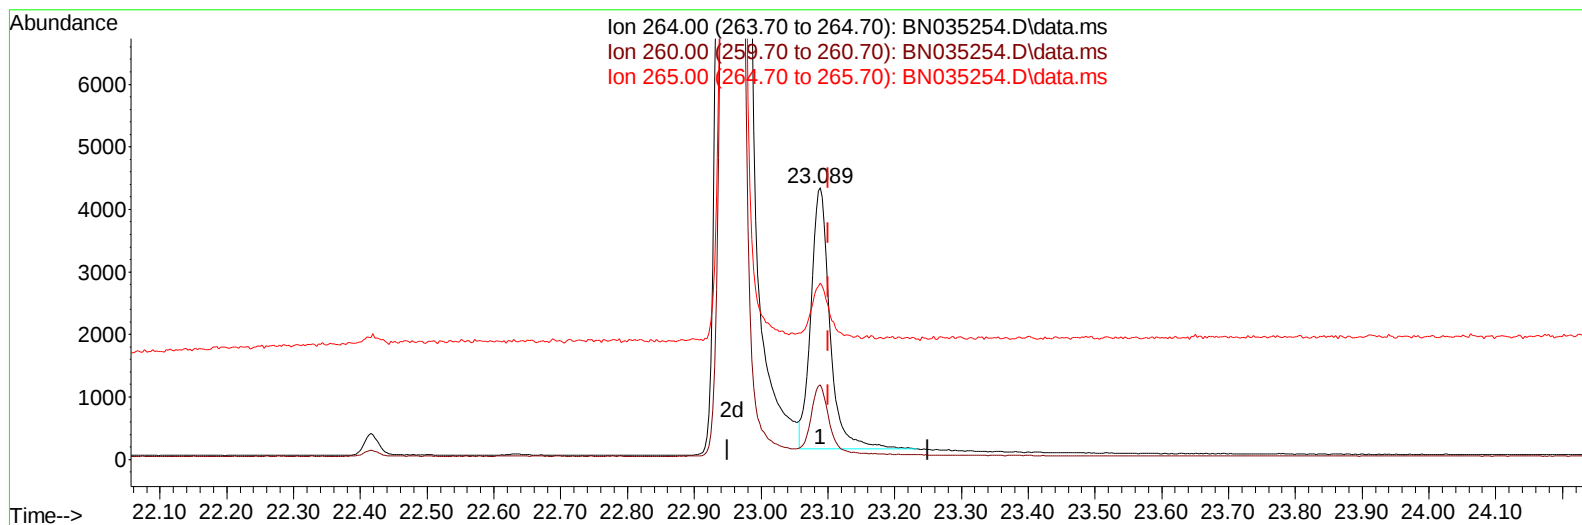

TIC: BN035254.D\data.ms

(23) Perylene-d12 (I)

23.089min (-0.012) 0.40 ng/u1

response 8414

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.56
265.00	75.50	64.96
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035254.D
Acq On : 22 Nov 2024 23:10
Operator : RC/JU
Sample : P4872-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y0

Manual IntegrationsAPPROVED

Quant Time: Nov 23 00:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

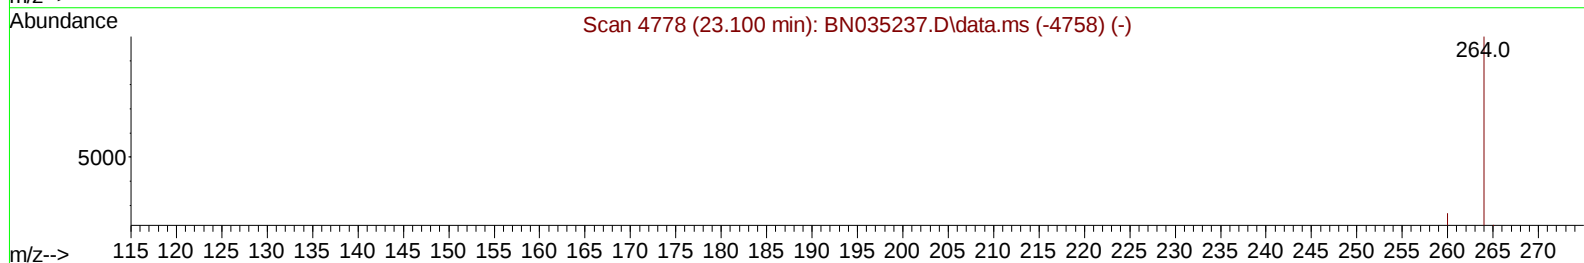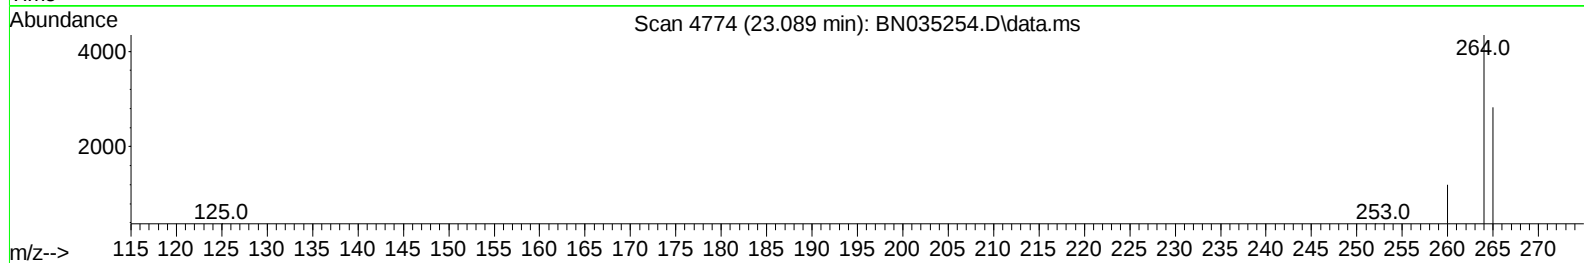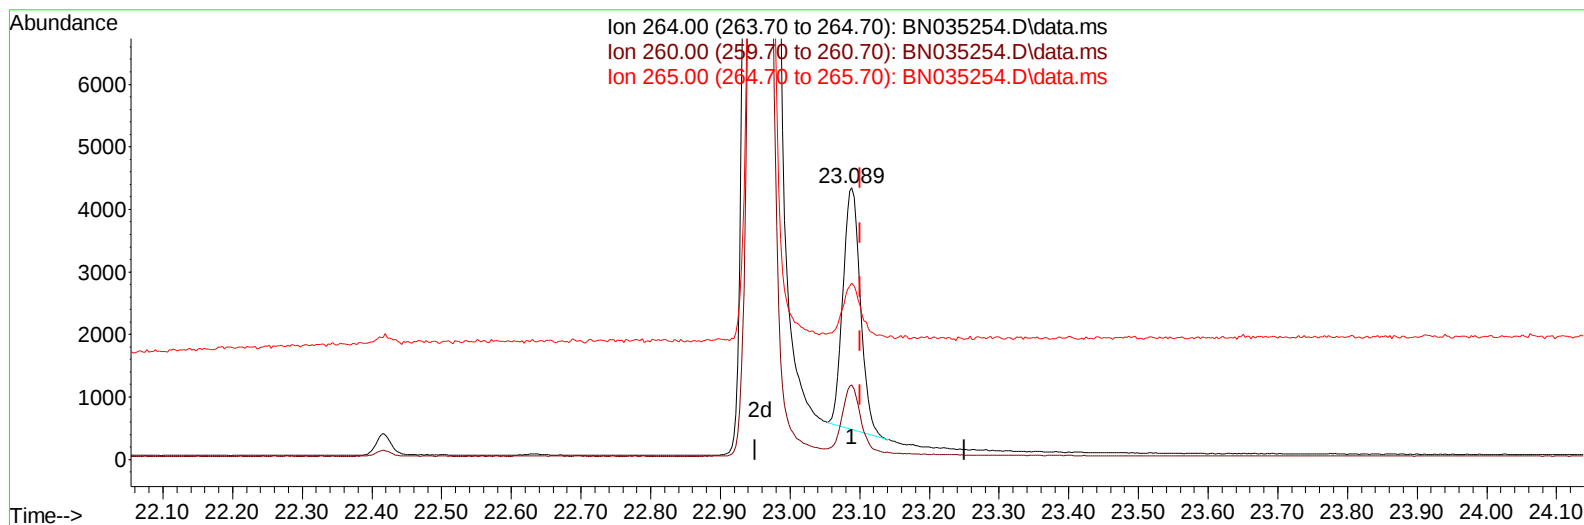

TIC: BN035254.D\data.ms

(23) Perylene-d12 (I)

23.089min (-0.012) 0.40 ng/ul m

response 6733

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.56
265.00	75.50	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035254.D
 Acq On : 22 Nov 2024 23:10
 Operator : RC/JU
 Sample : P4872-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 23 00:00:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.318	152	3279	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136	8435	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164	5315	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188	11759	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.988	240	8285	0.400	ng/ul	# 0.00
23) Perylene-d12	23.089	264	6733m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	5651	1.886	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152	1487	0.120	ng/ul	0.00
18) Fluoranthene-d10	18.800	212	3769	0.165	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035254.D
Acq On : 22 Nov 2024 23:10
Operator : RC/JU
Sample : P4872-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 23 00:00:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

