




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035268.D
Acq On : 23 Nov 2024 08:11
Operator : RC/JU
Sample : PB165115BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK115

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

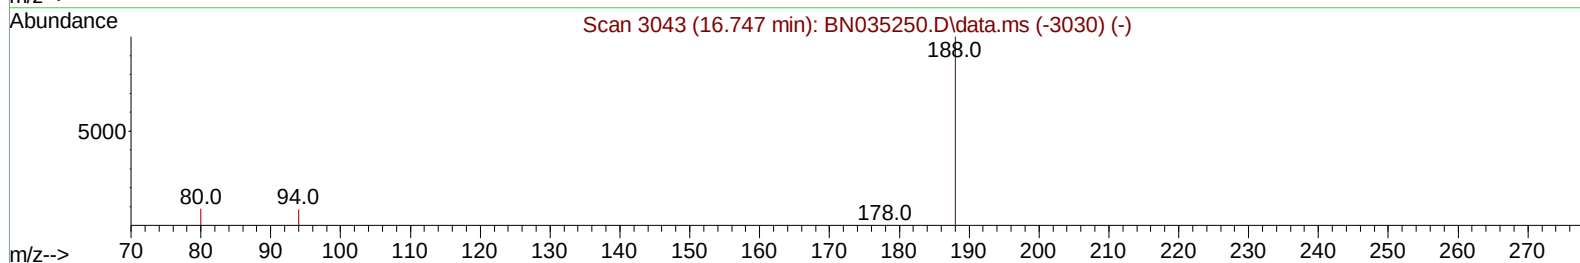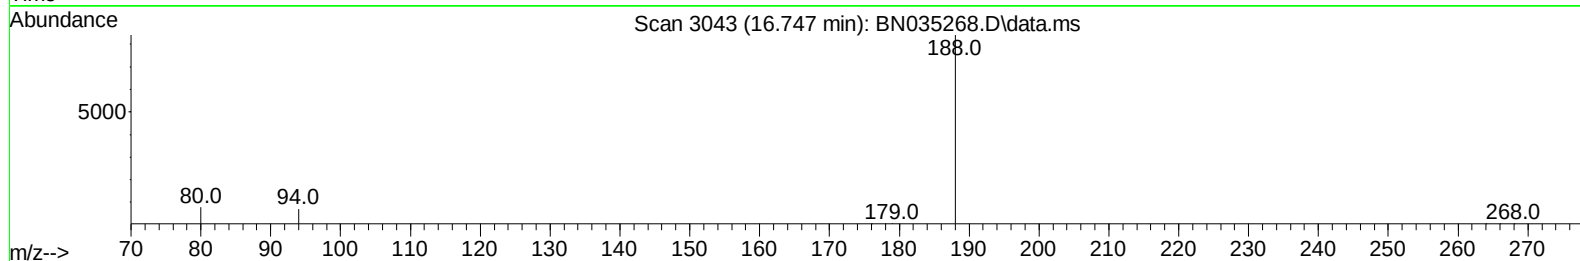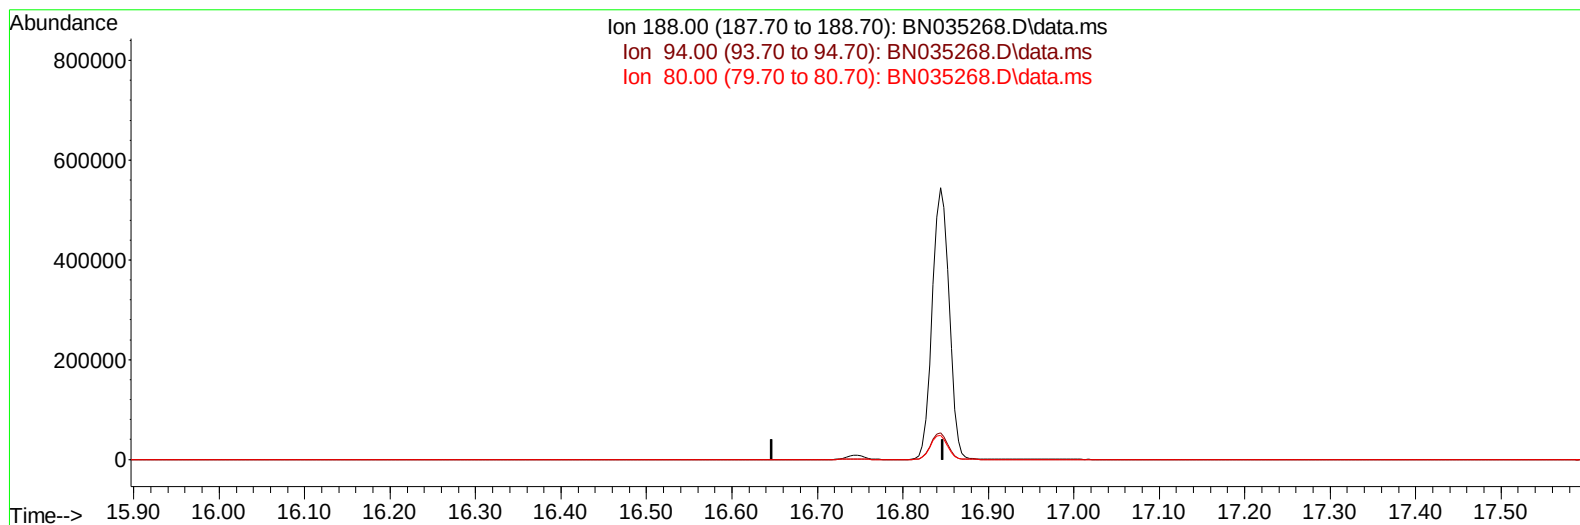

TIC: BN035268.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (-16.747) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035268.D
Acq On : 23 Nov 2024 08:11
Operator : RC/JU
Sample : PB165115BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK115

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

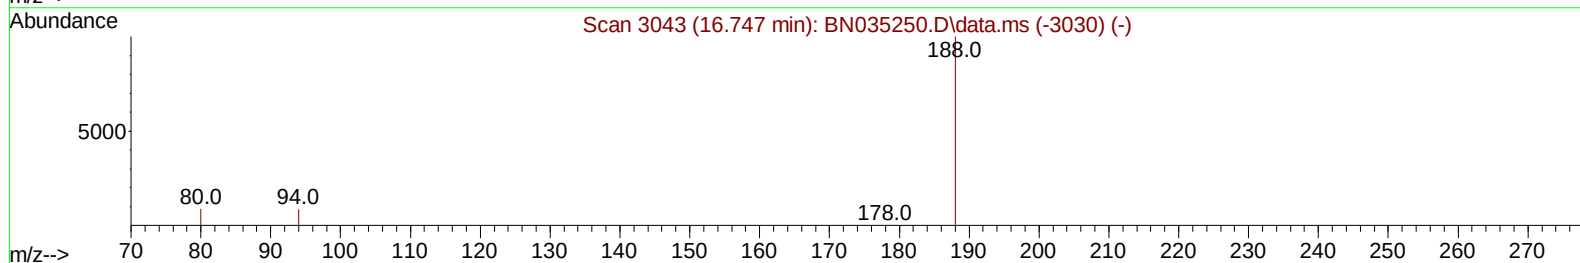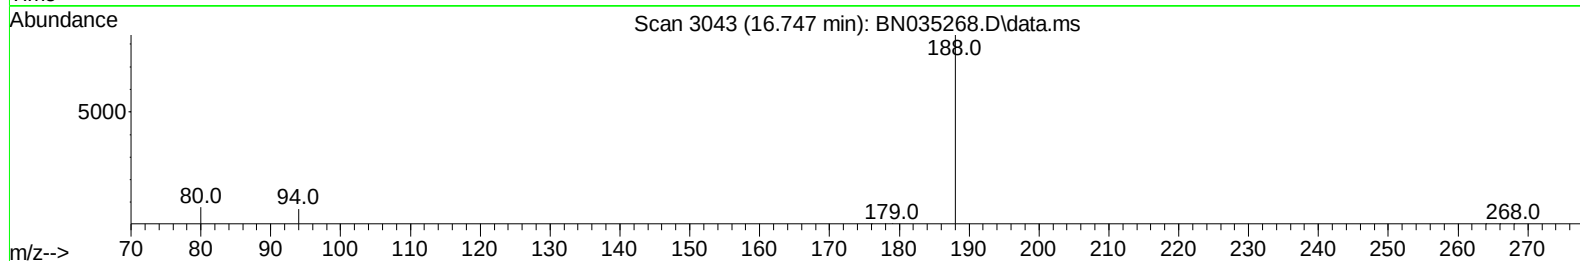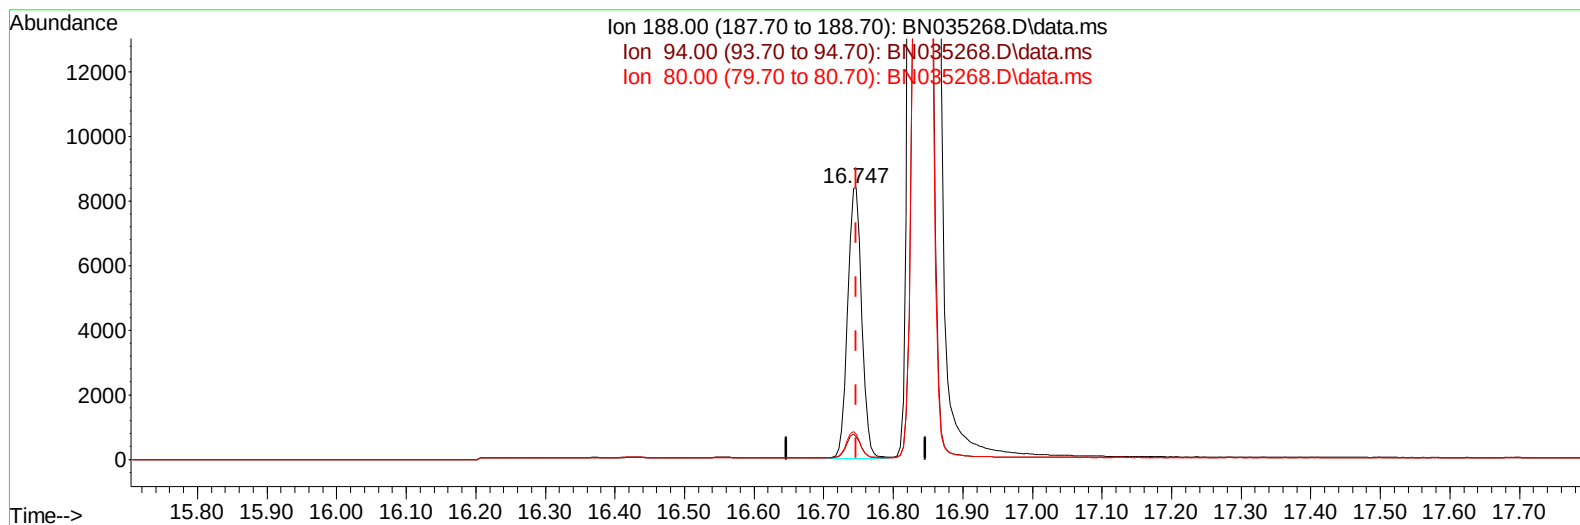

TIC: BN035268.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (-0.000) 0.40 ng/ul m

response 11709

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.38
80.00	7.60	9.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035268.D
Acq On : 23 Nov 2024 08:11
Operator : RC/JU
Sample : PB165115BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK115

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

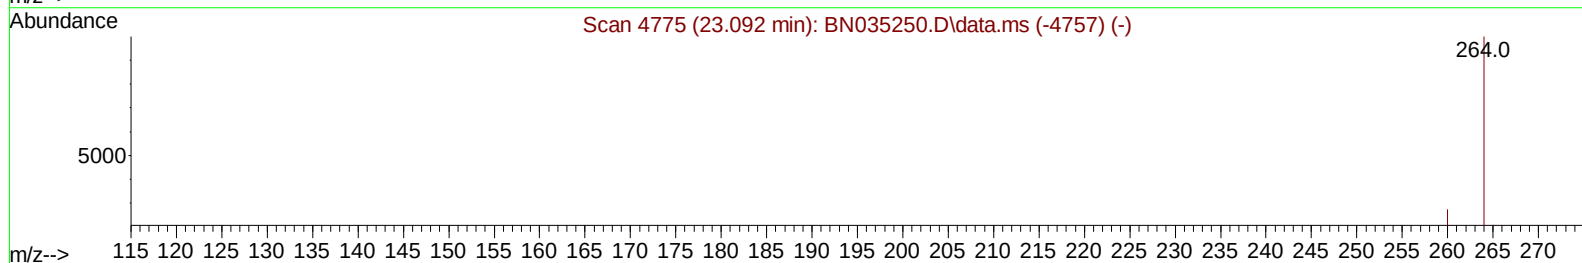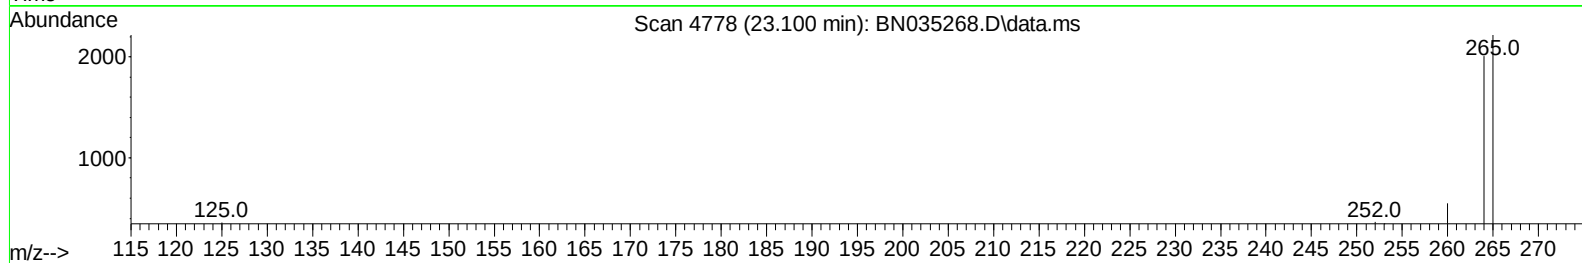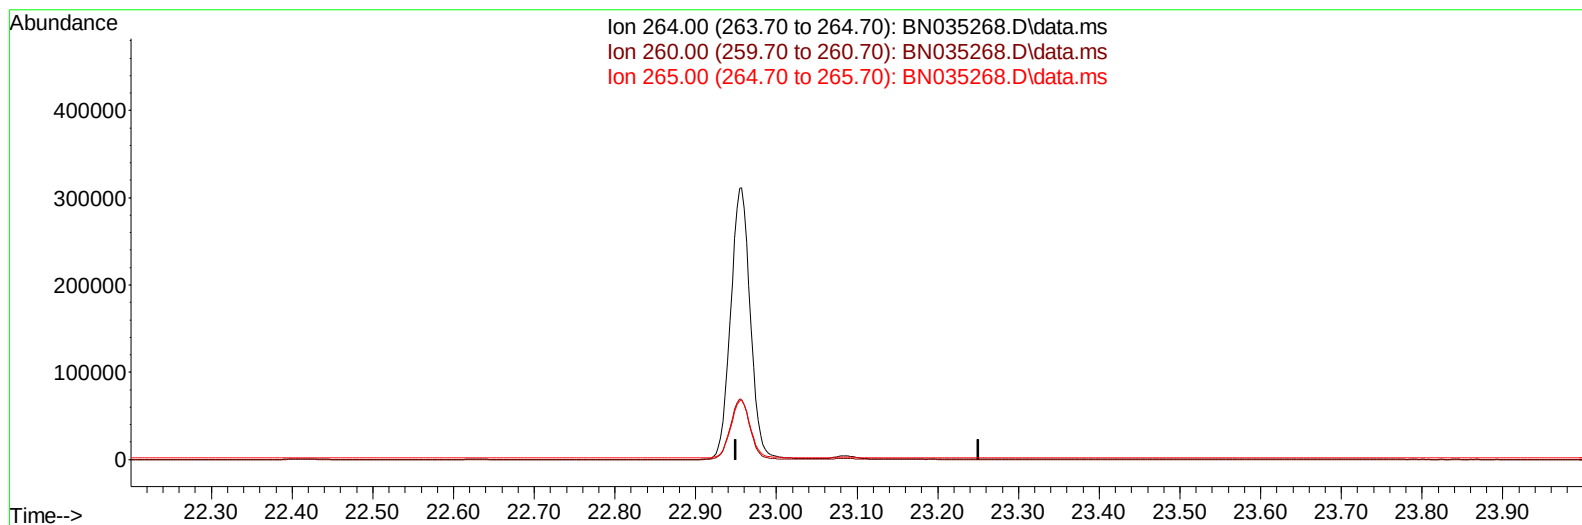

TIC: BN035268.D\data.ms

(23) Perylene-d12 (I)

23.100min (-23.100) 0.00 ng/u1

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	26.20	0.00#
265.00	75.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035268.D
 Acq On : 23 Nov 2024 08:11
 Operator : RC/JU
 Sample : PB165115BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK115

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

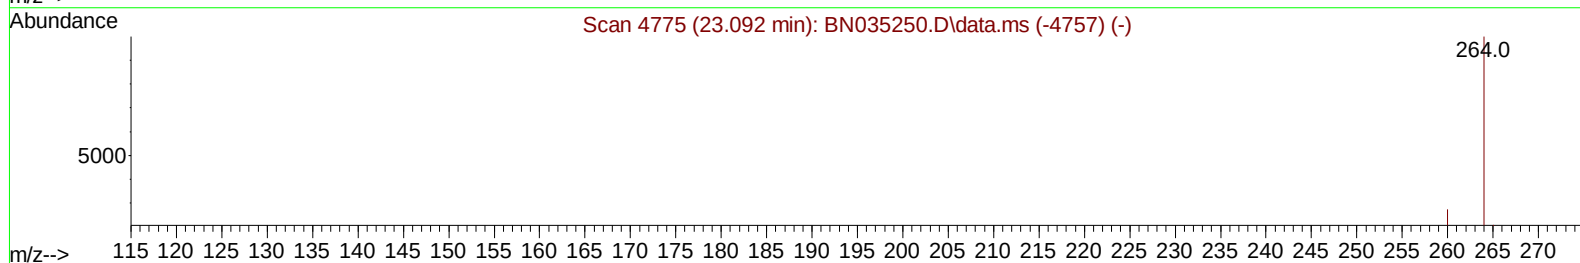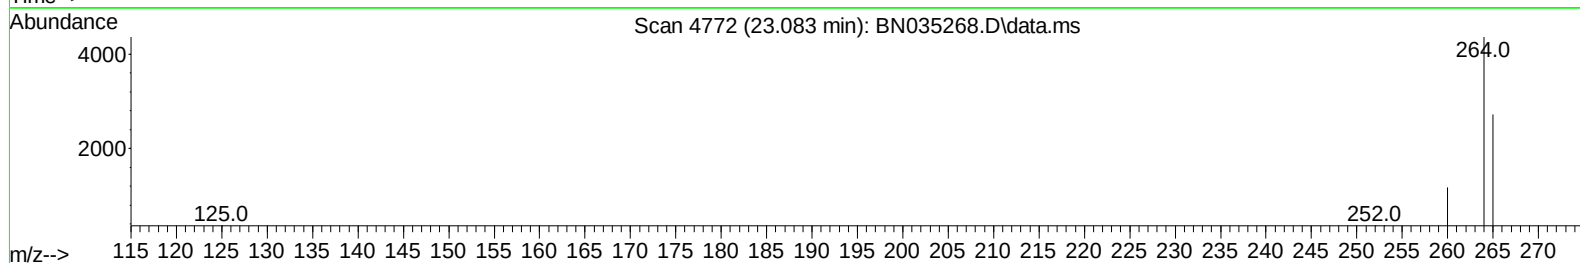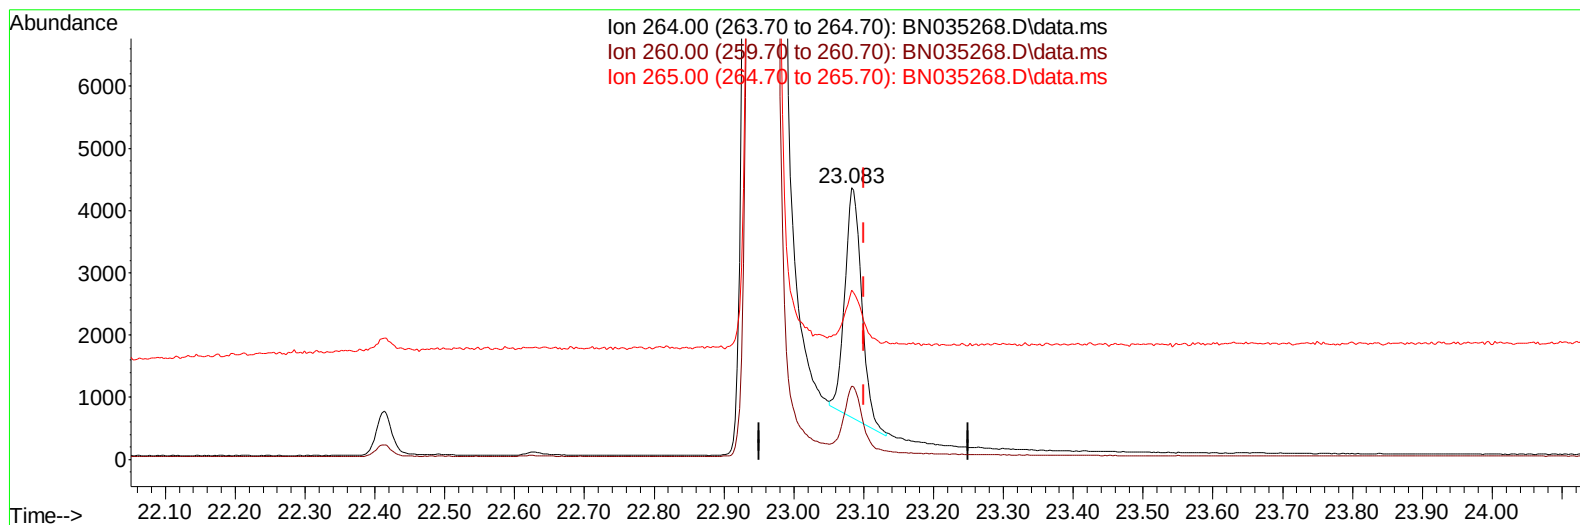

TIC: BN035268.D\data.ms

(23) Perylene-d12 (I)

23.083min (-0.018) 0.40 ng/ul m

response 6204

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.04
265.00	75.50	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035268.D
 Acq On : 23 Nov 2024 08:11
 Operator : RC/JU
 Sample : PB165115BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK115

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.318	152		3245	0.400	ng/ul	0.00
4) Naphthalene-d8	10.064	136		8641	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.976	164		5334	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188		11709m	0.400	ng/ul	0.00
17) Chrysene-d12	20.988	240		7520	0.400	ng/ul	# 0.00
23) Perylene-d12	23.083	264		6204m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		12586	4.244	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152		3860	0.305	ng/ul	0.00
18) Fluoranthene-d10	18.795	212		9295	0.448	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035268.D
Acq On : 23 Nov 2024 08:11
Operator : RC/JU
Sample : PB165115BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK115

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

