




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

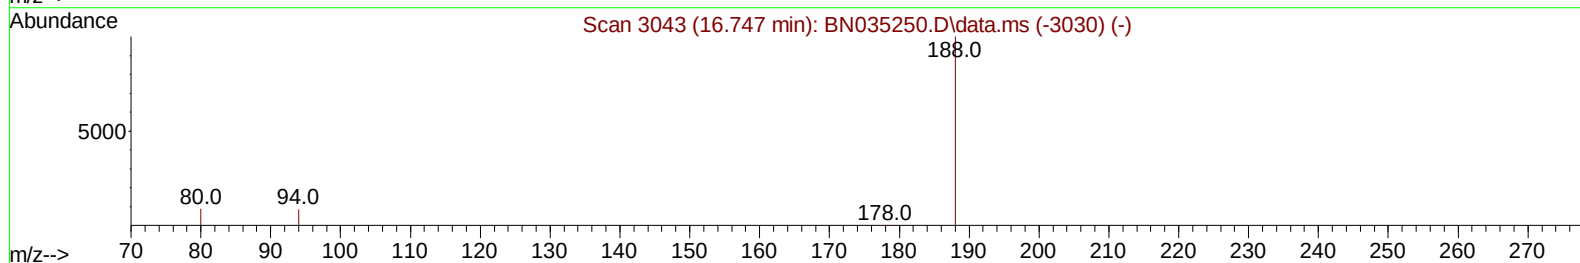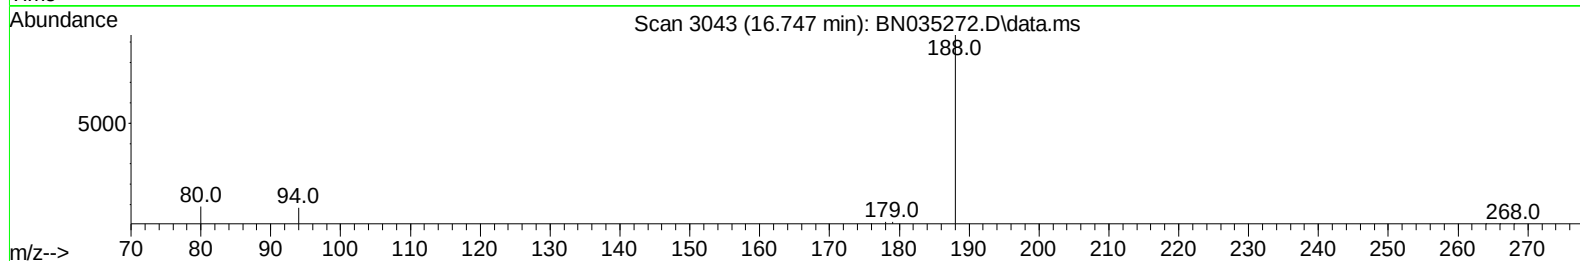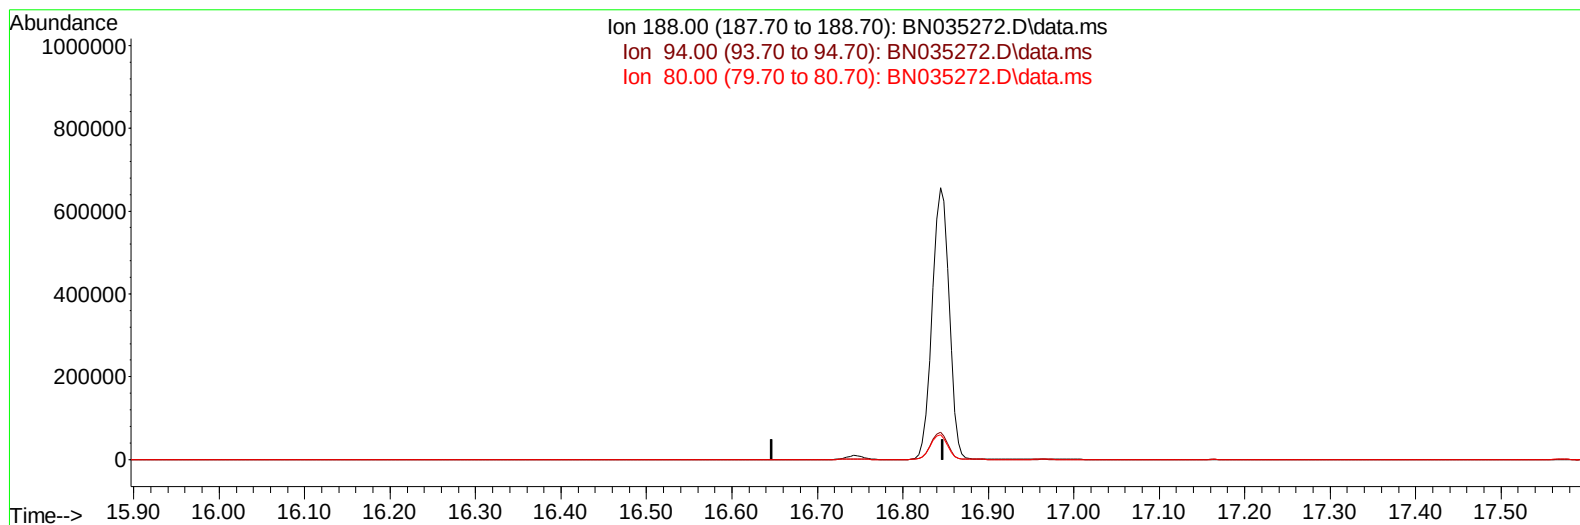

TIC: BN035272.D\data.ms

(13) Phenanthrene-d10 (I)

16.747min (-16.747) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

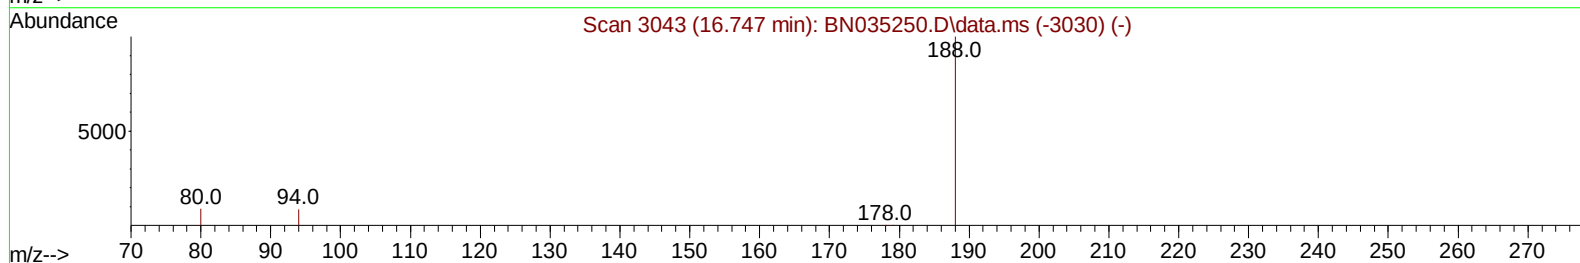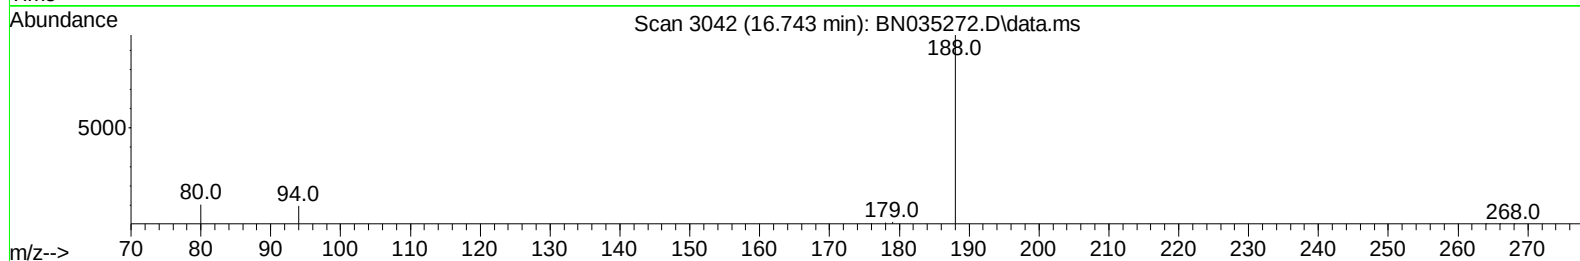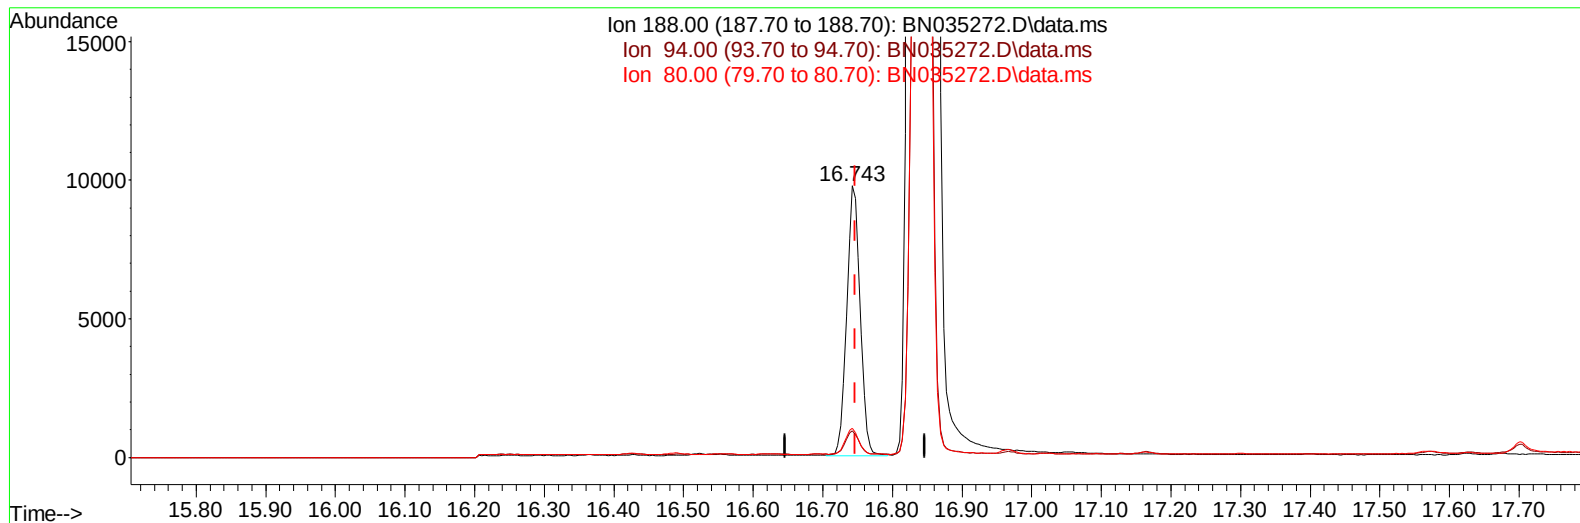

TIC: BN035272.D\data.ms

(13) Phenanthrene-d10 (I)

16.743min (-0.004) 0.40 ng/ul m

response 13003

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	9.79#
80.00	7.60	10.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

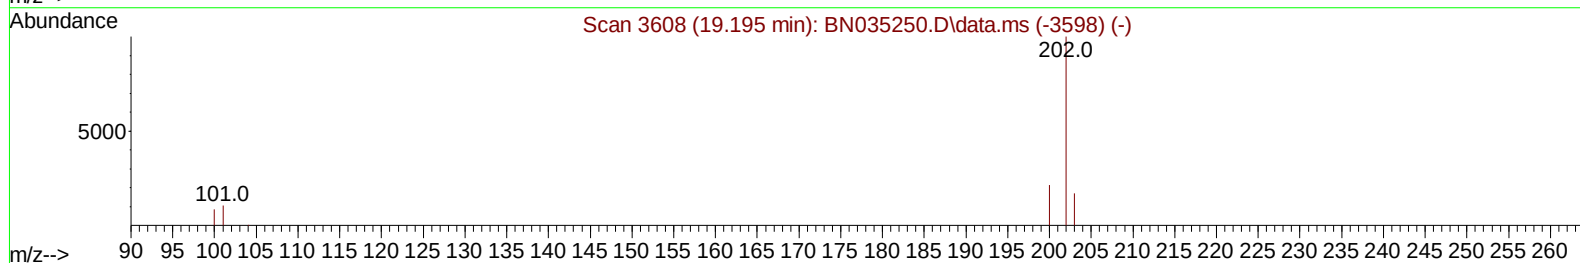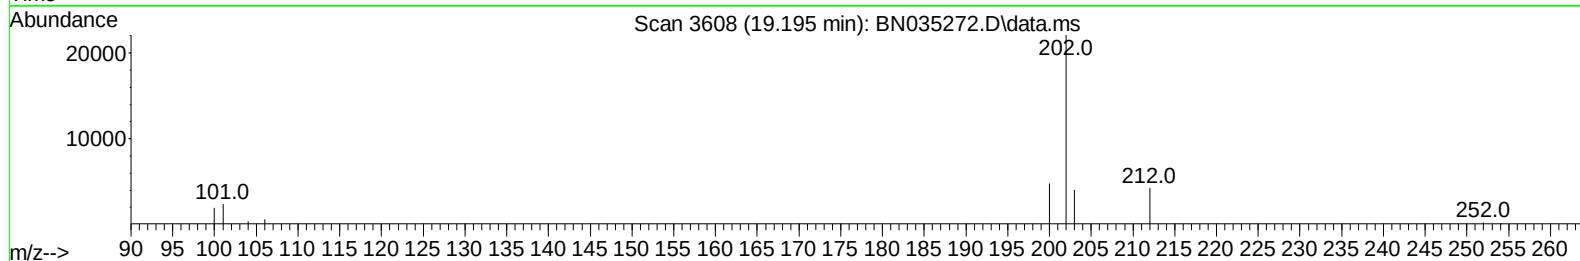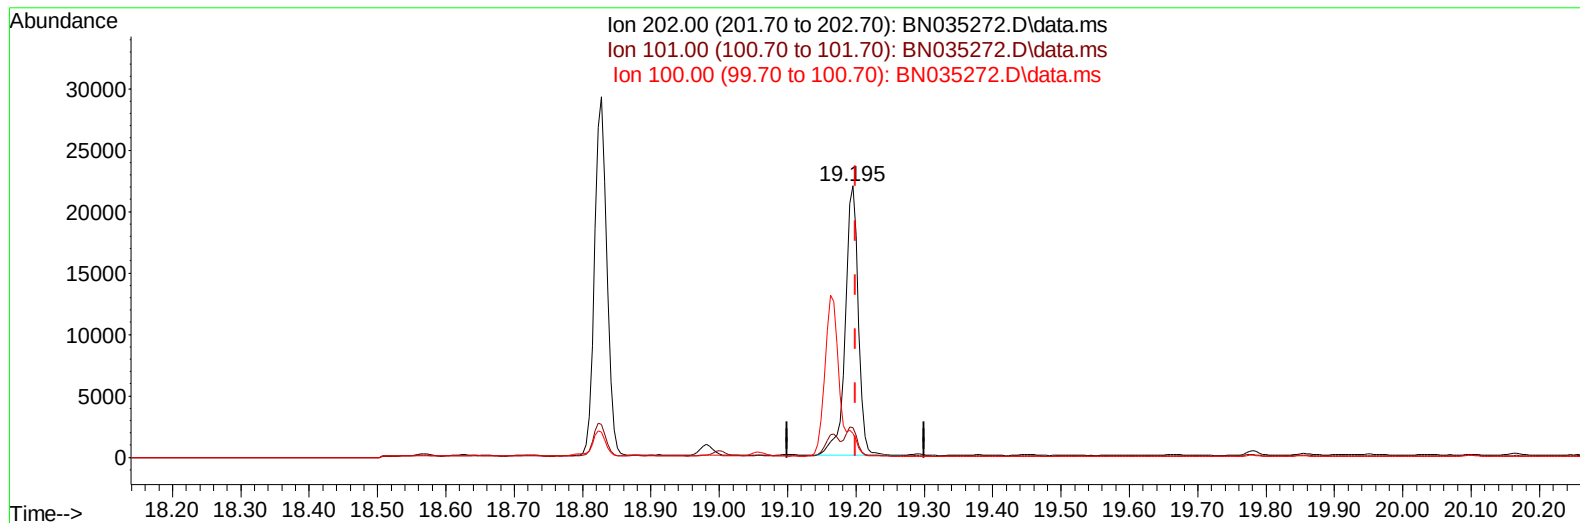

TIC: BN035272.D\data.ms

(20) Pyrene

19.195min (-0.005) 0.80 ng/u1

response 29591

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	10.98#
100.00	6.40	8.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

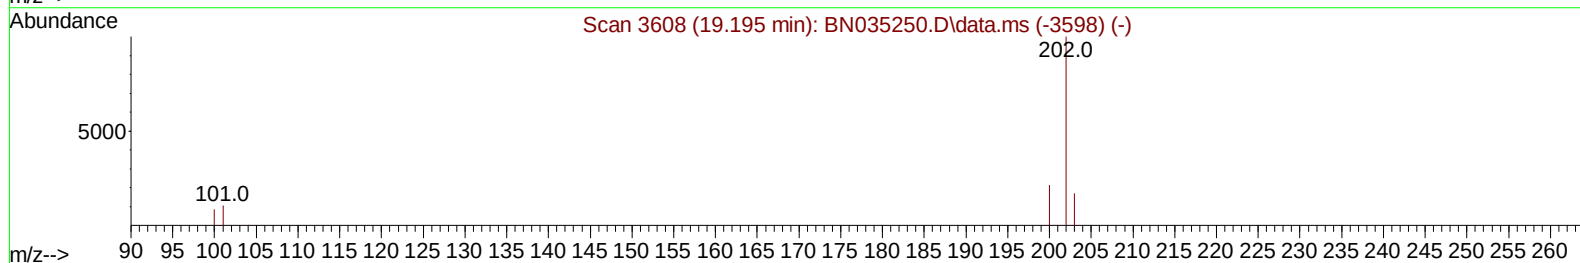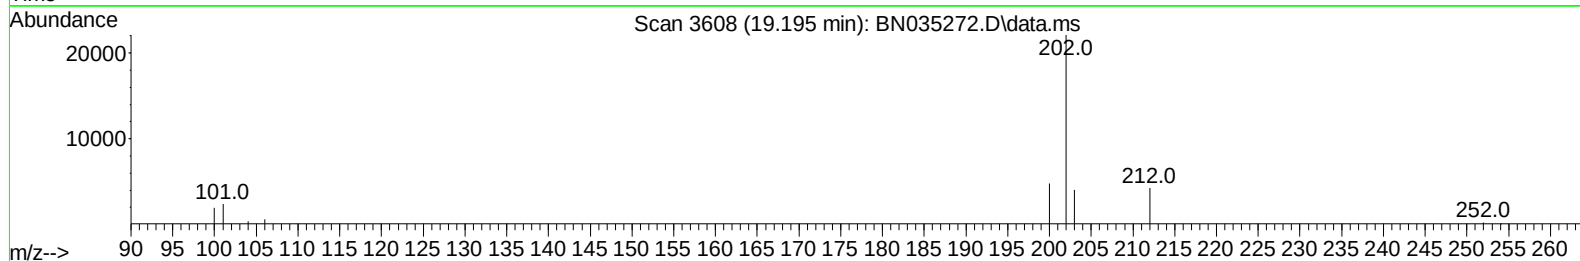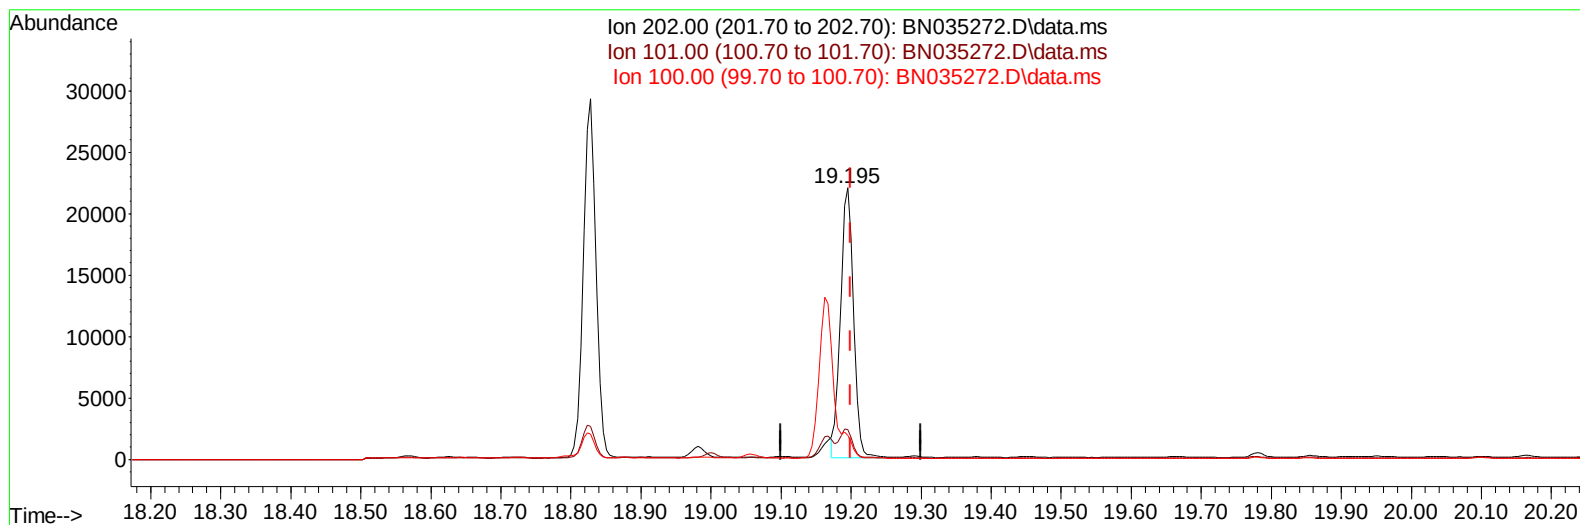

TIC: BN035272.D\data.ms

(20) Pyrene

19.195min (-0.005) 0.77 ng/ul m

response 28329

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	10.98#
100.00	6.40	8.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

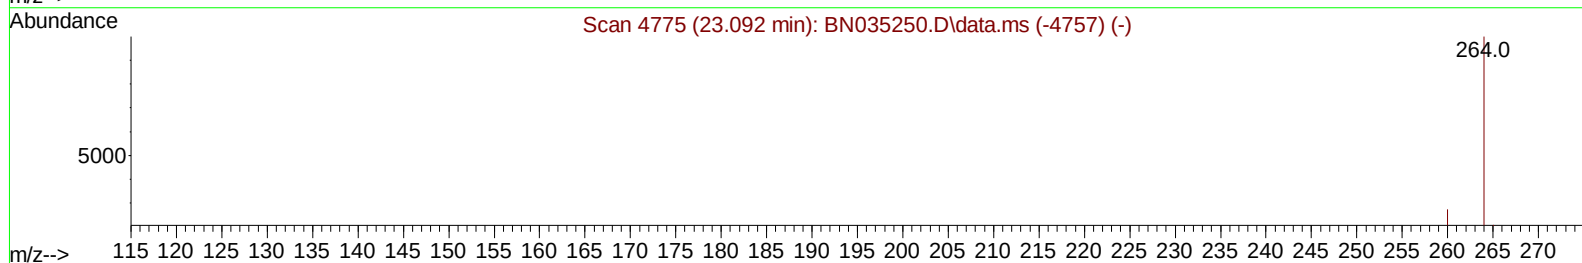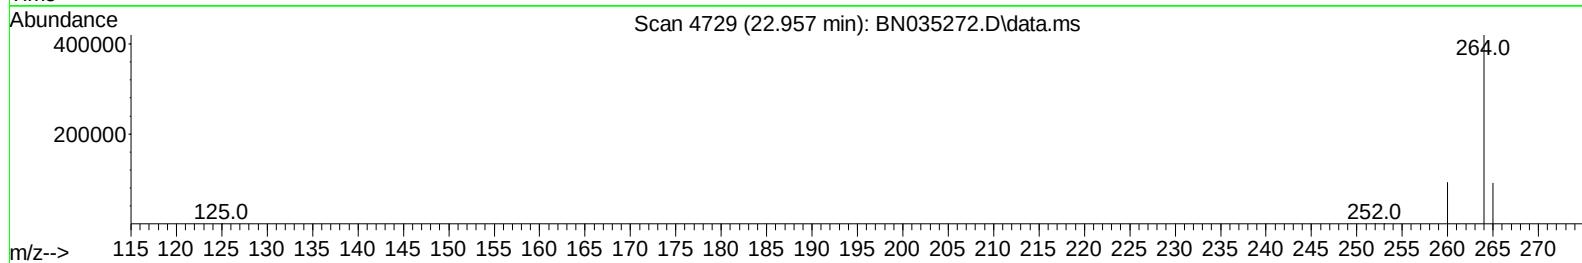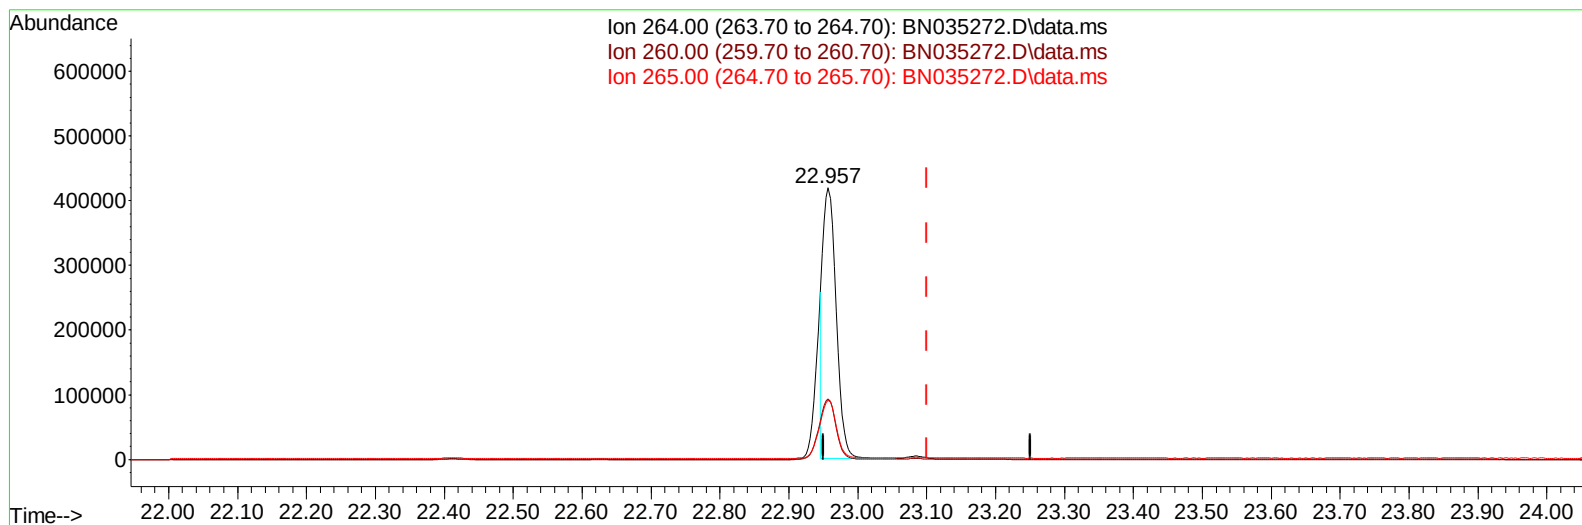

TIC: BN035272.D\data.ms

(23) Perylene-d12 (I)

22.957min (-0.143) 0.40 ng/u1

response 570589

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.32
265.00	75.50	21.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

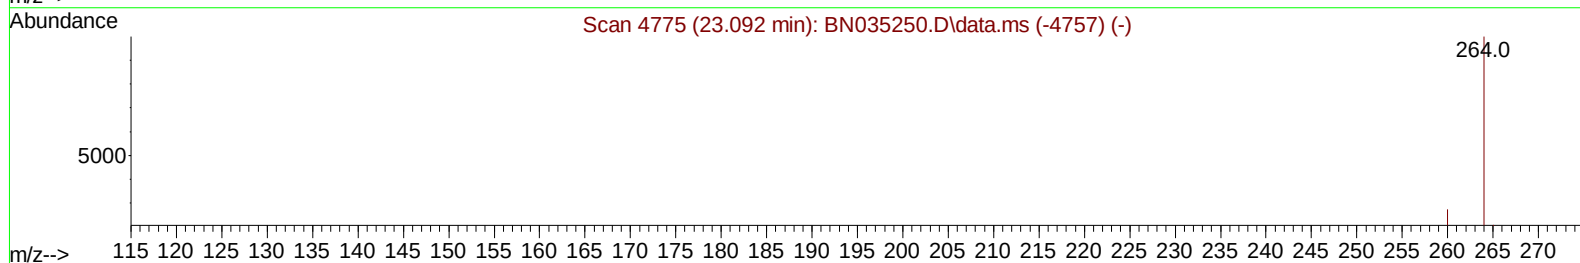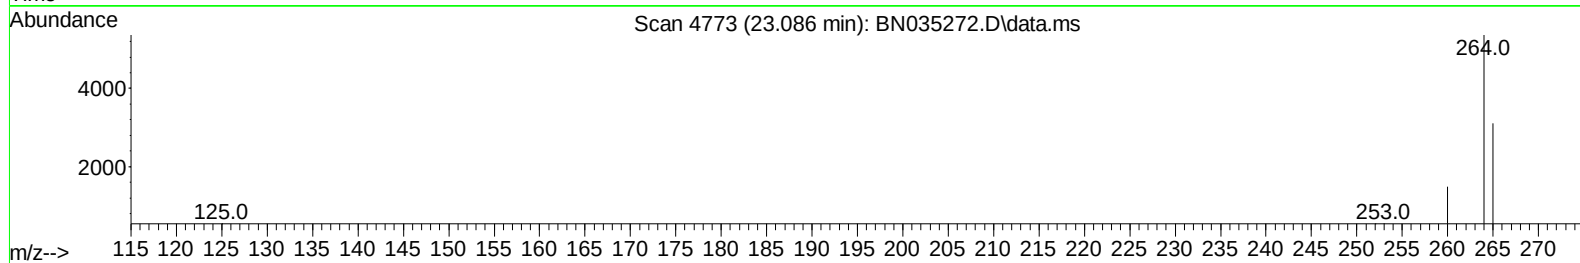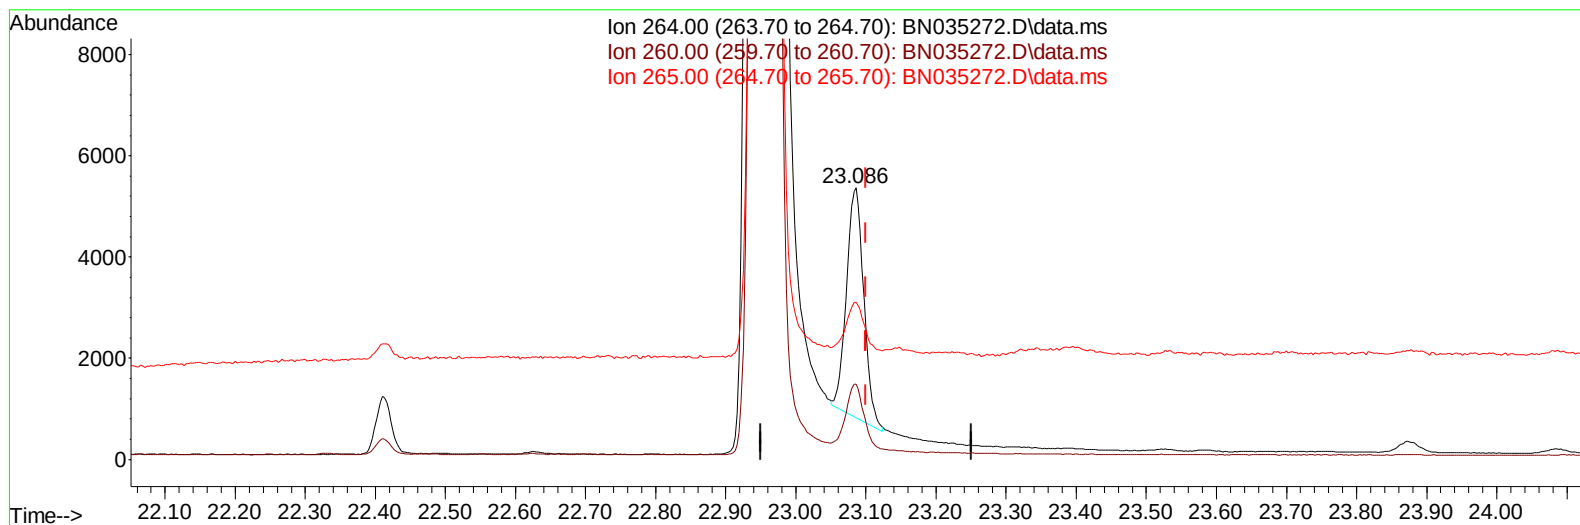

TIC: BN035272.D\data.ms

(23) Perylene-d12 (I)

23.086min (-0.015) 0.40 ng/ul m

response 7719

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.75
265.00	75.50	57.93#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

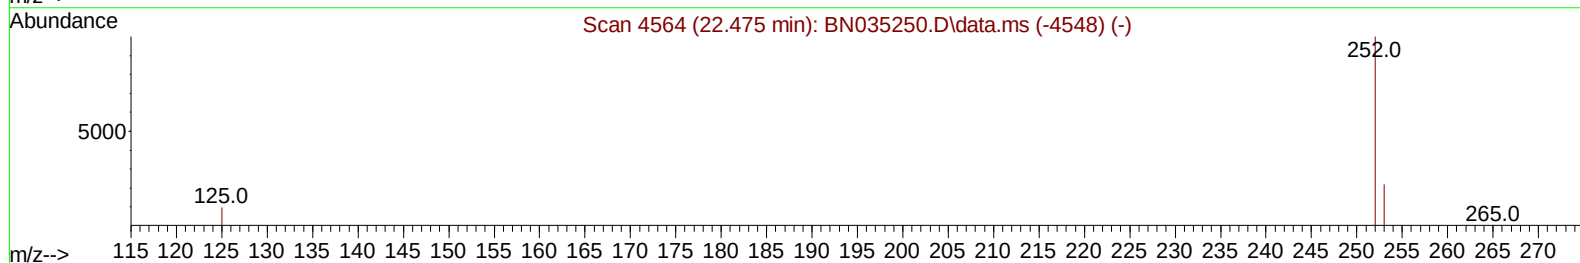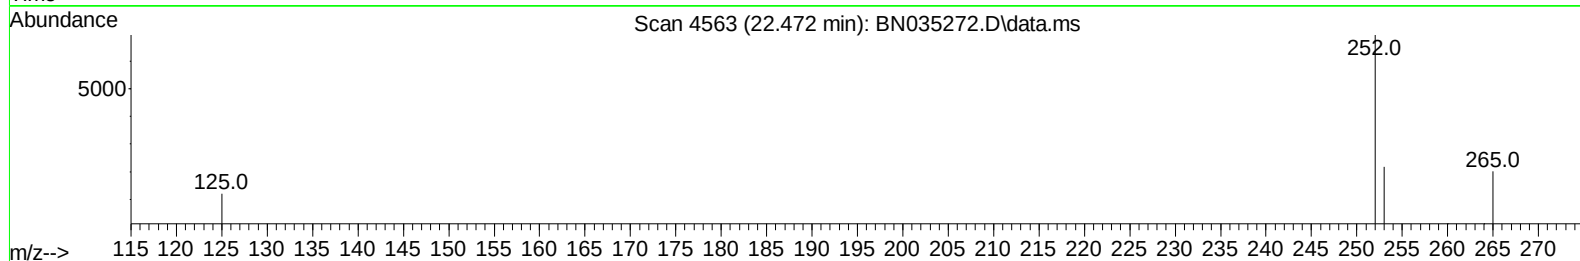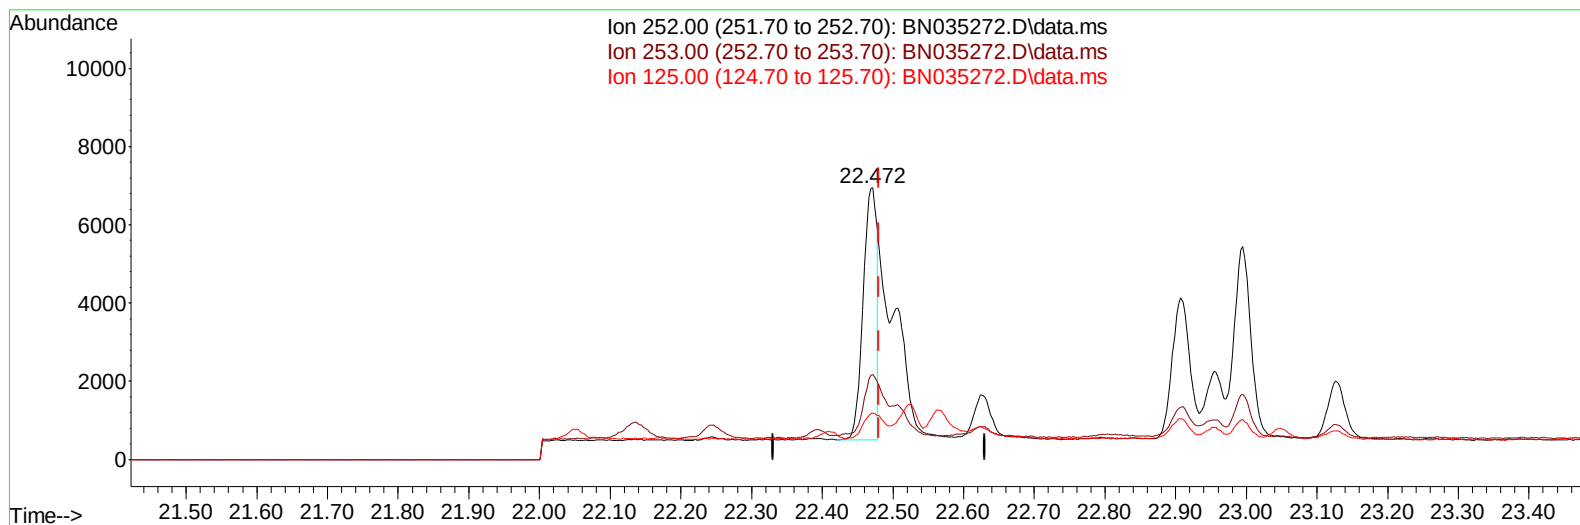

TIC: BN035272.D\data.ms

(24) Benzo(b)fluoranthene

22.472min (-0.009) 0.34 ng/u1

response 8602

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	31.17
125.00	9.70	17.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

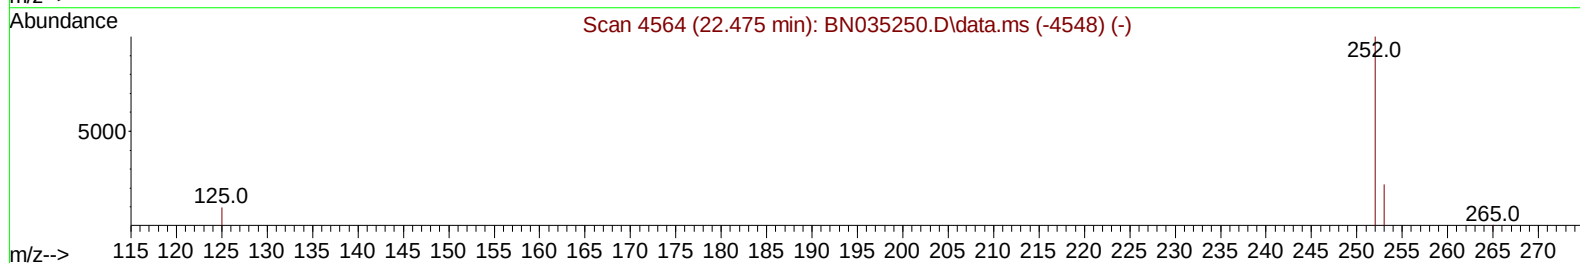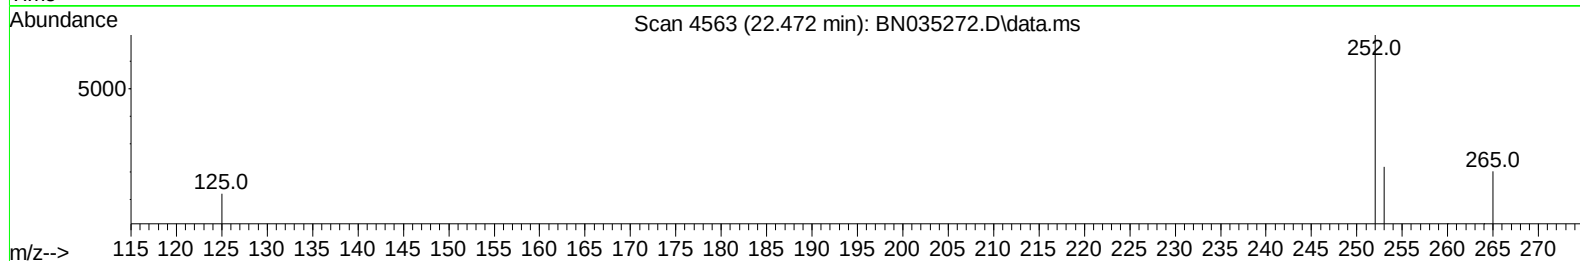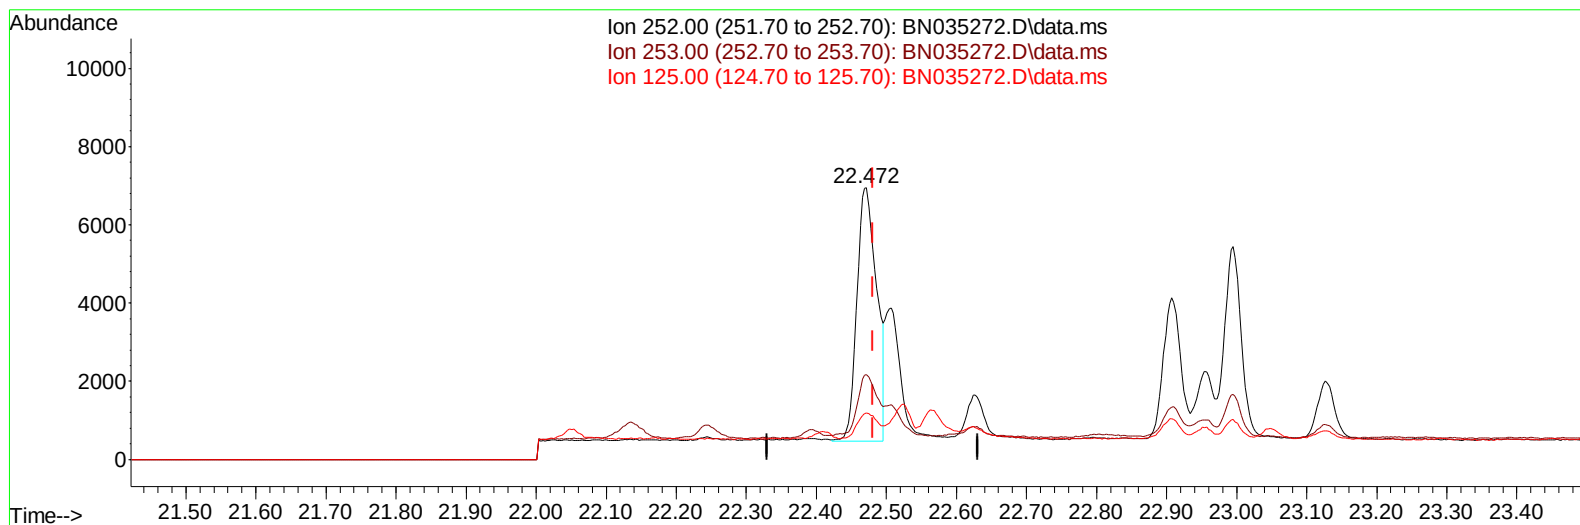

TIC: BN035272.D\data.ms

(24) Benzo(b)fluoranthene

22.472min (-0.009) 0.50 ng/ul m

response 12727

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	31.17
125.00	9.70	17.23
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

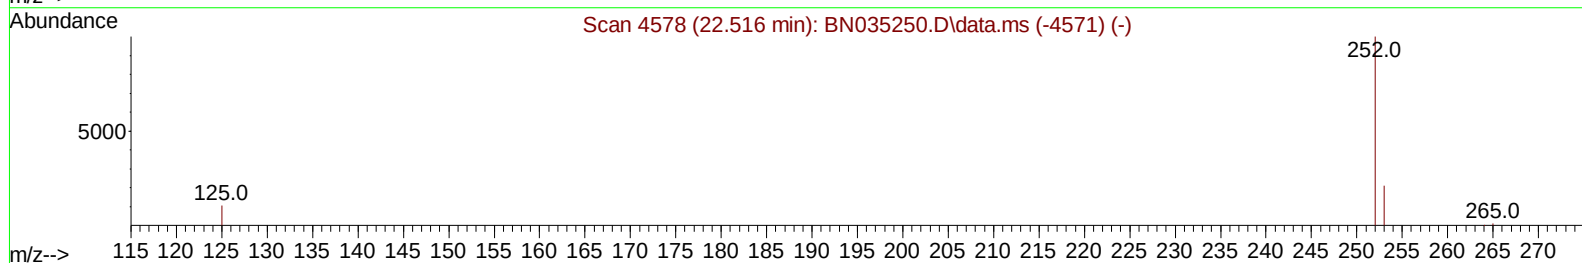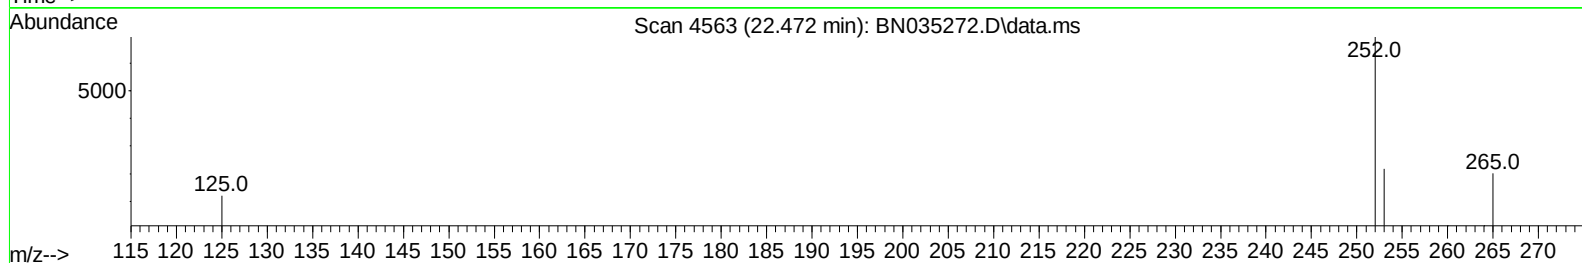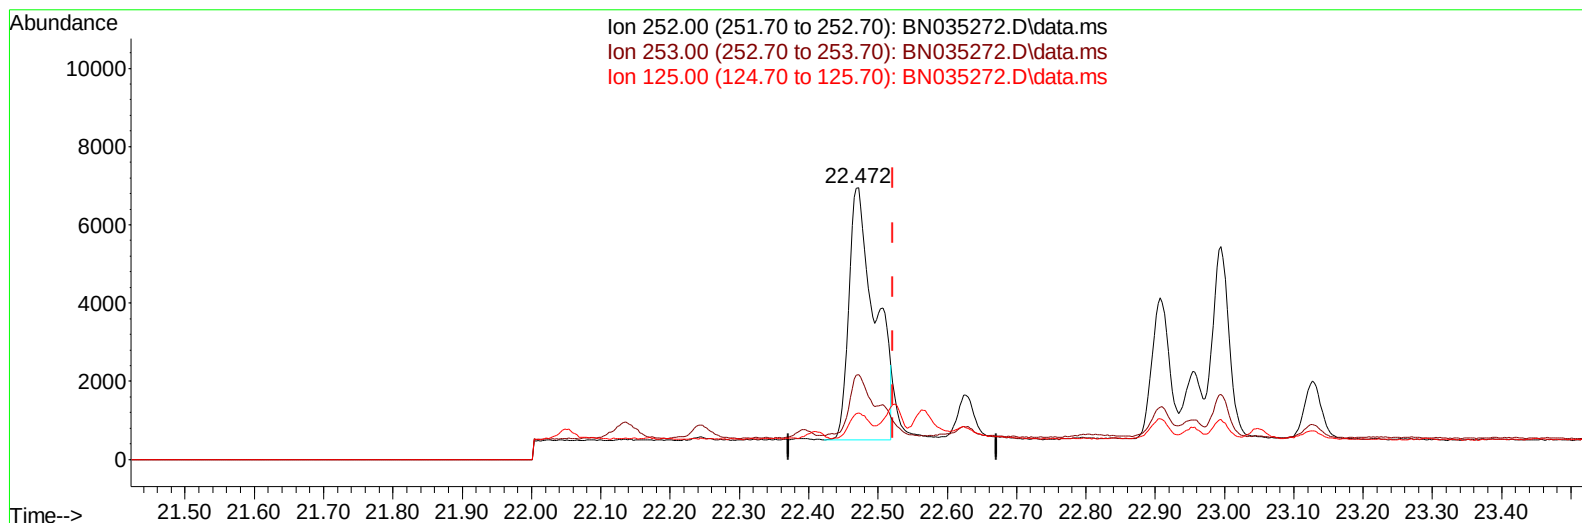

TIC: BN035272.D\data.ms

(25) Benzo(k)fluoranthene

22.472min (-0.050) 0.64 ng/u l

response 16723

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	31.17
125.00	10.70	17.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

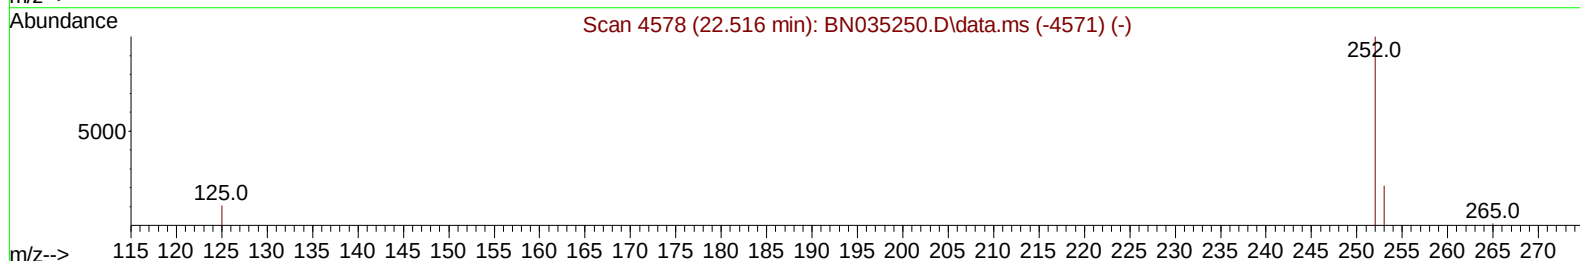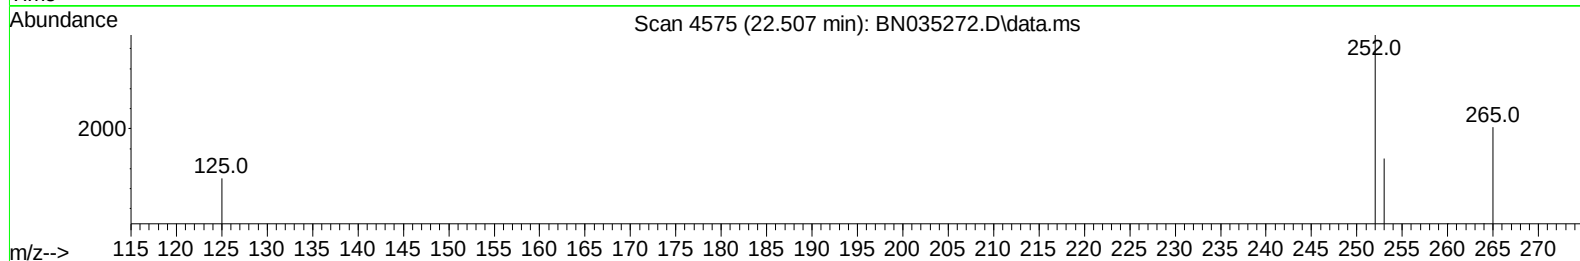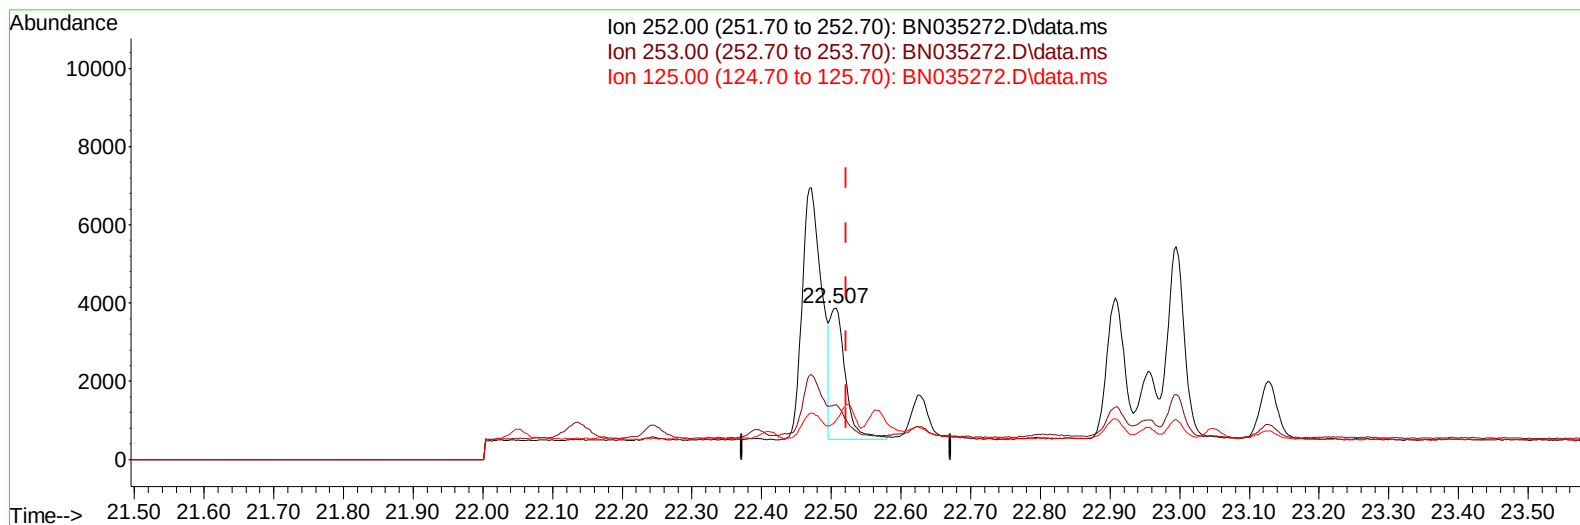

TIC: BN035272.D\data.ms

(25) Benzo(k)fluoranthene

22.507min (-0.015) 0.20 ng/ul m

response 5170

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	36.05#
125.00	10.70	25.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

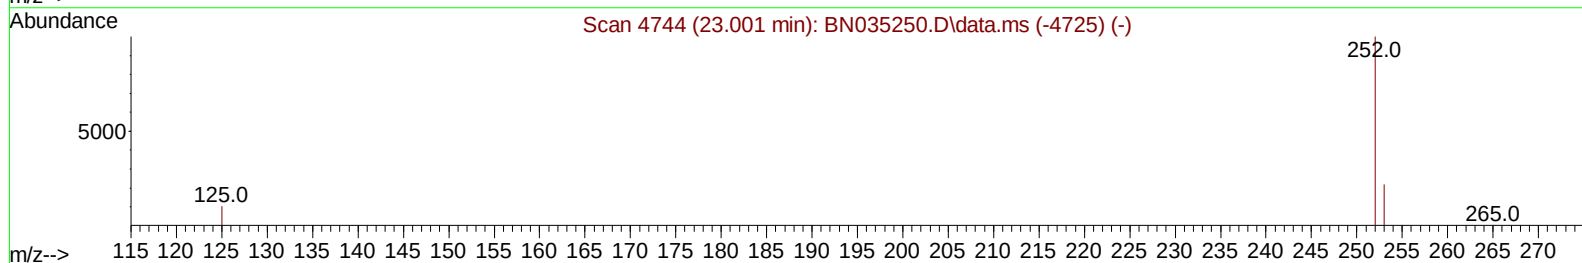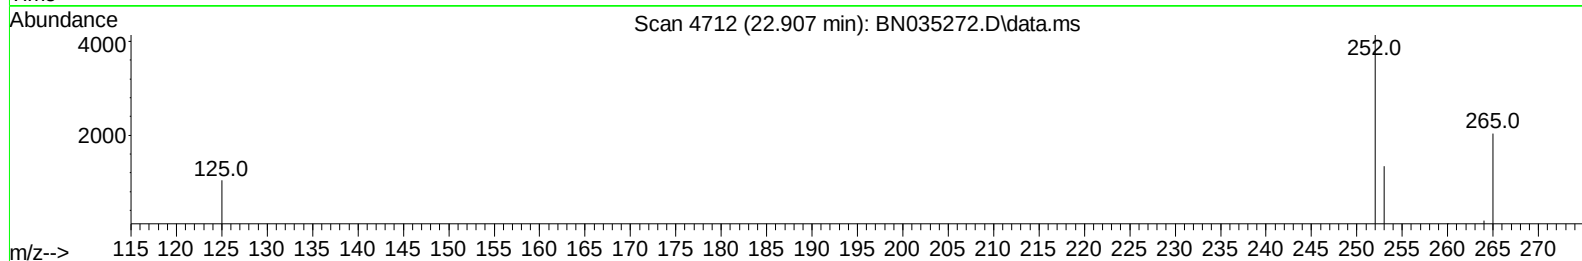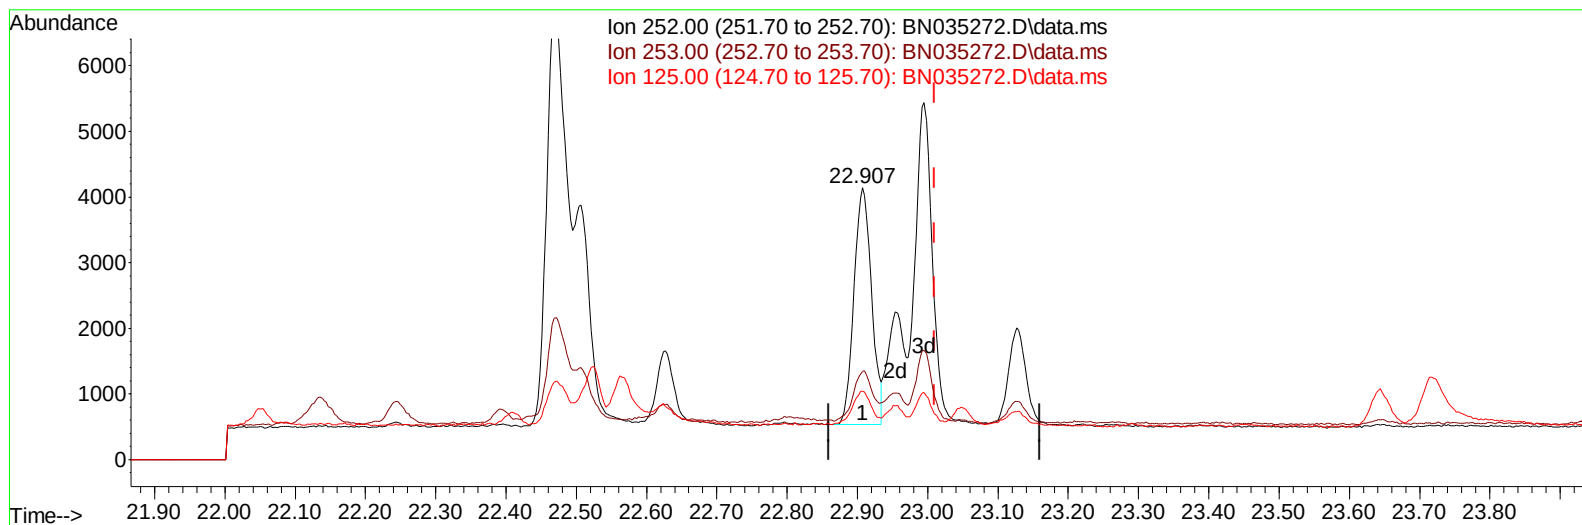

TIC: BN035272.D\data.ms

(26) Benzo(a)pyrene (C)

22.907min (-0.102) 0.27 ng/u1

response 6303

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	32.43
125.00	11.80	25.08#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

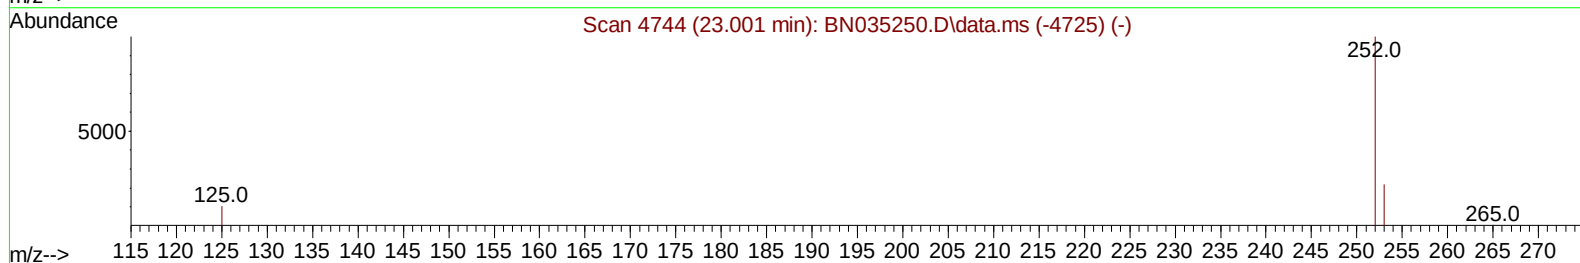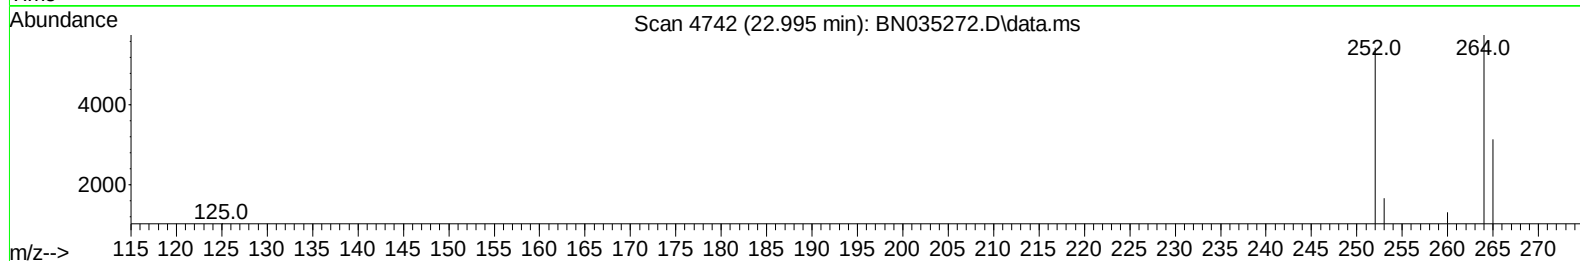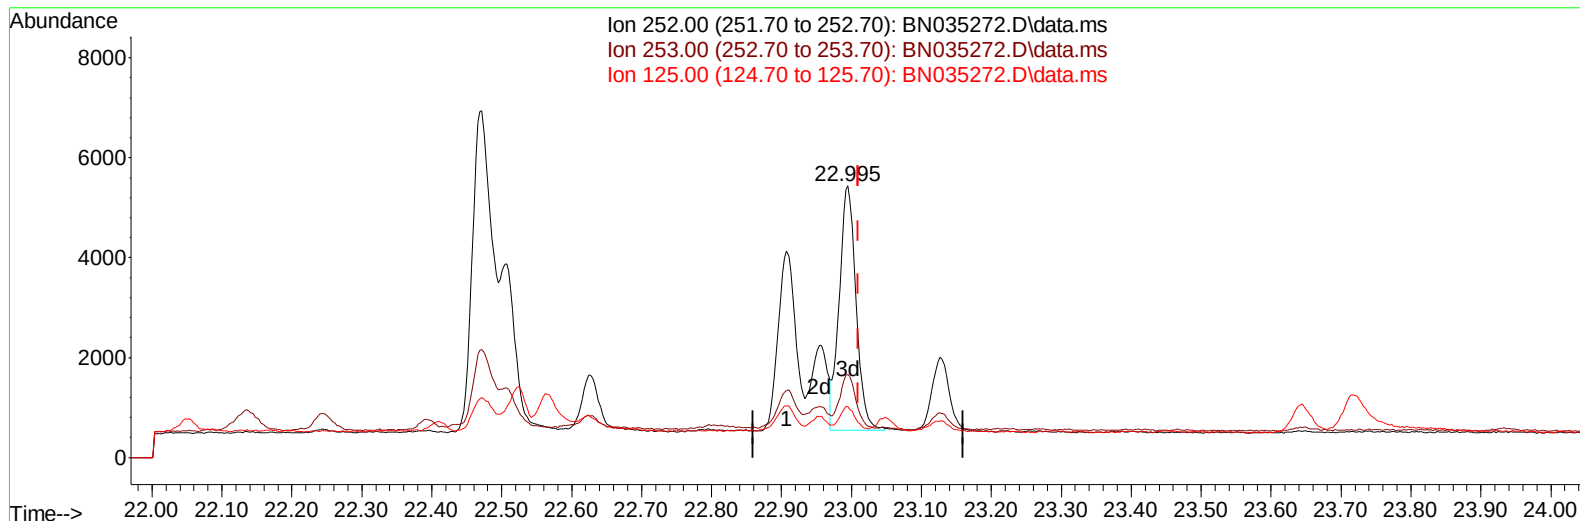

TIC: BN035272.D\data.ms

(26) Benzo(a)pyrene (C)

22.995min (-0.015) 0.35 ng/u1 m

response 8201

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	30.65
125.00	11.80	18.73#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

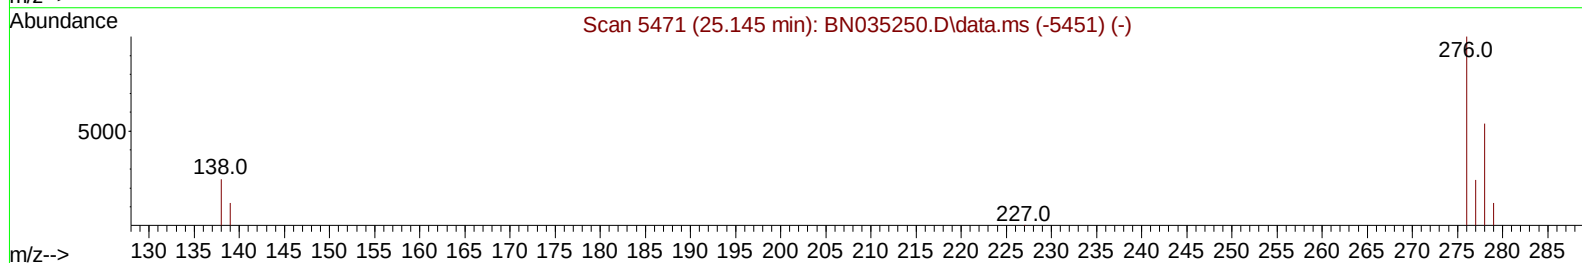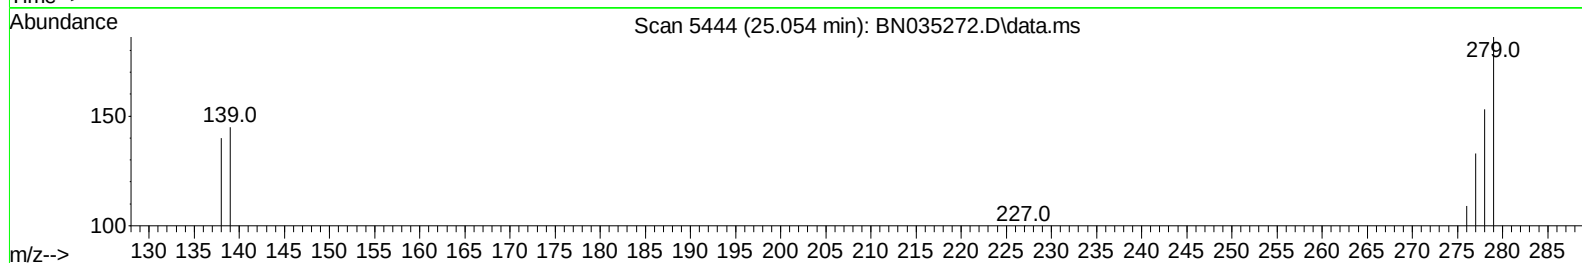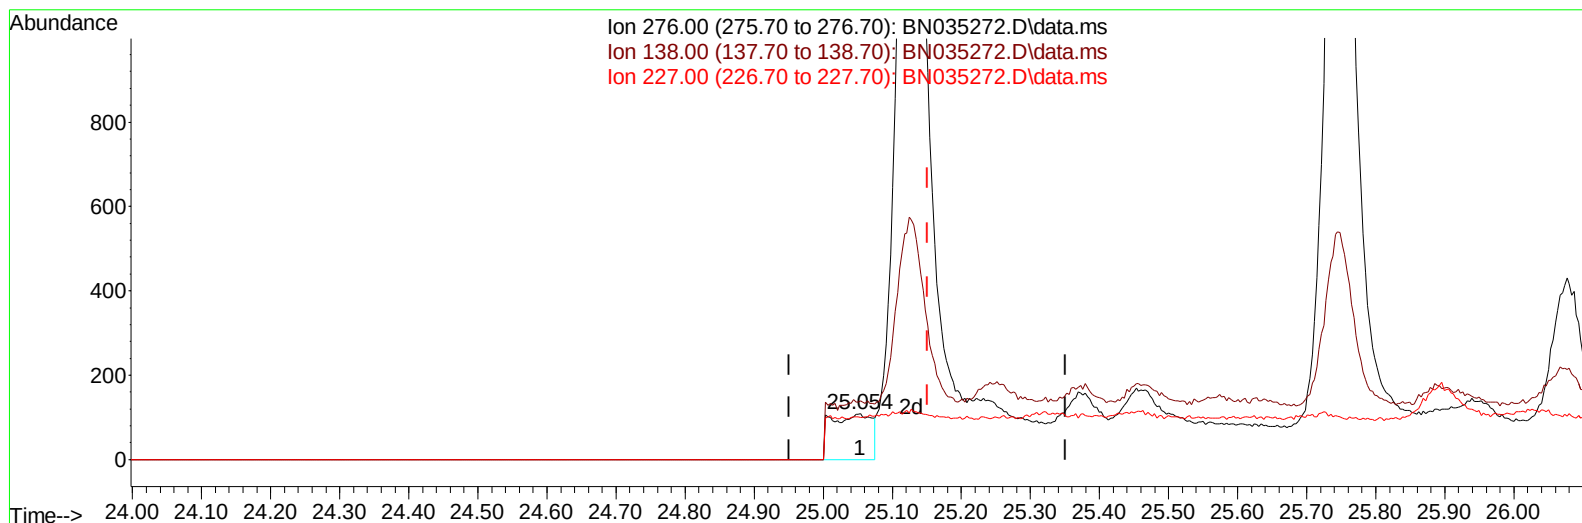

TIC: BN035272.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.054min (-0.097) 0.01 ng/u1

response 431

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	148.03#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

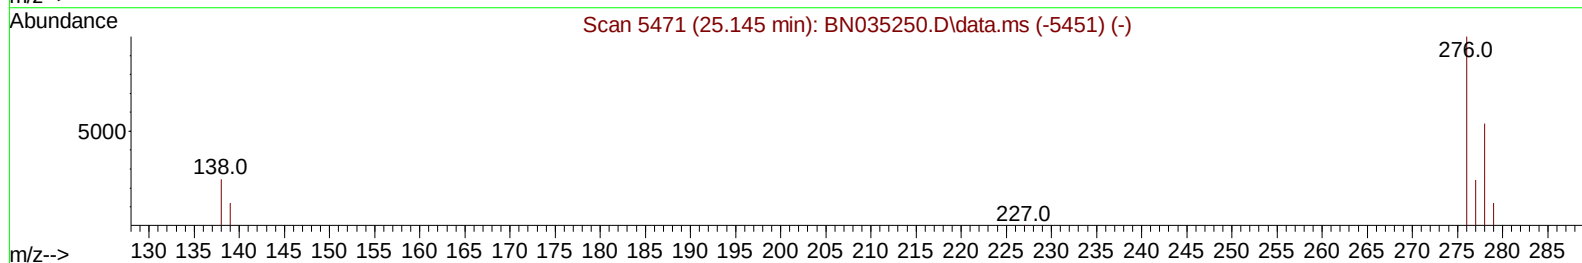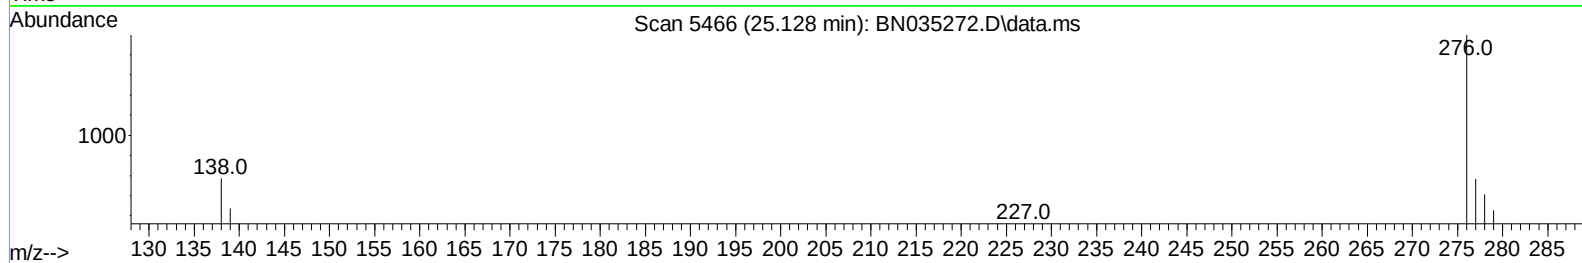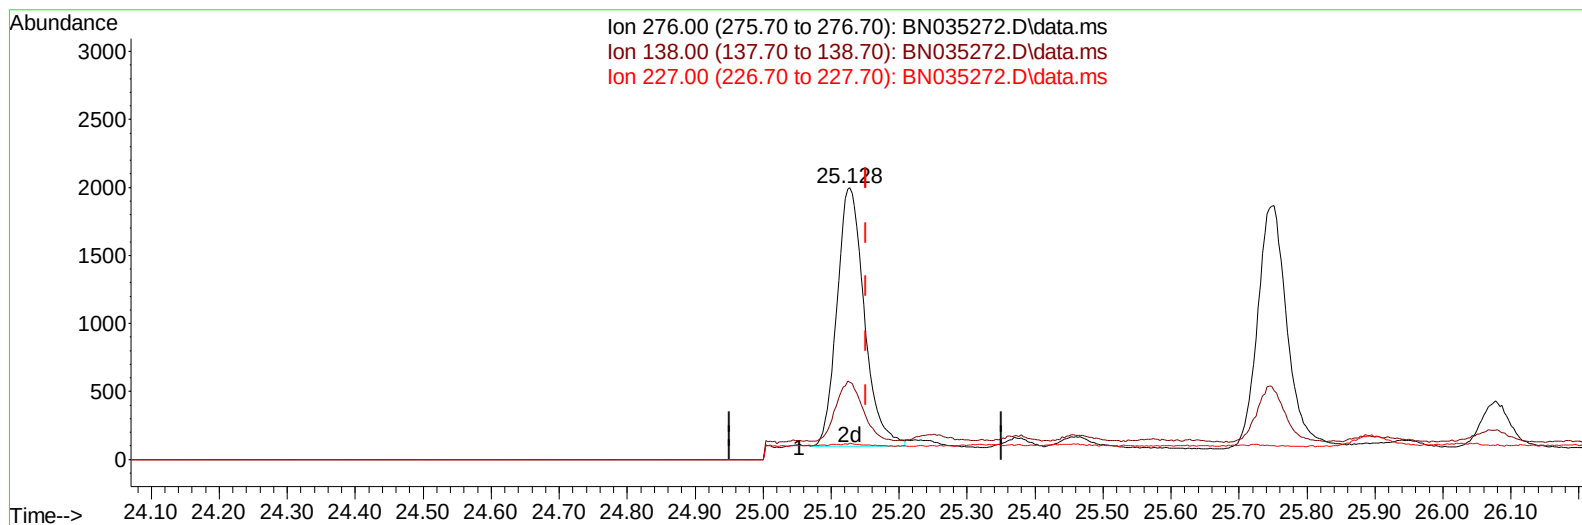

TIC: BN035272.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.128min (-0.024) 0.17 ng/ul m

response 5319

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	11.99#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

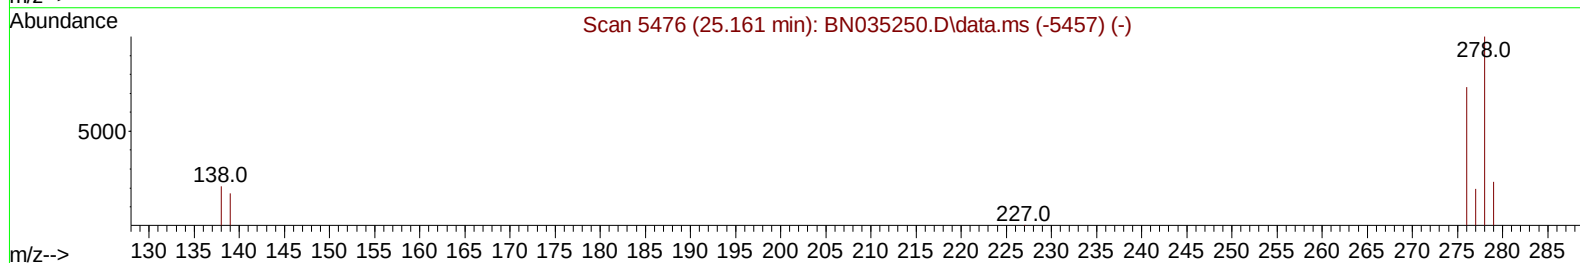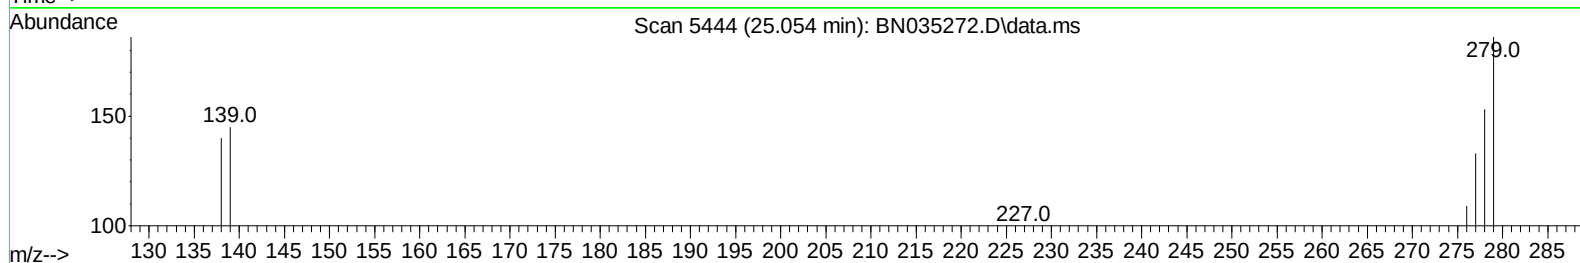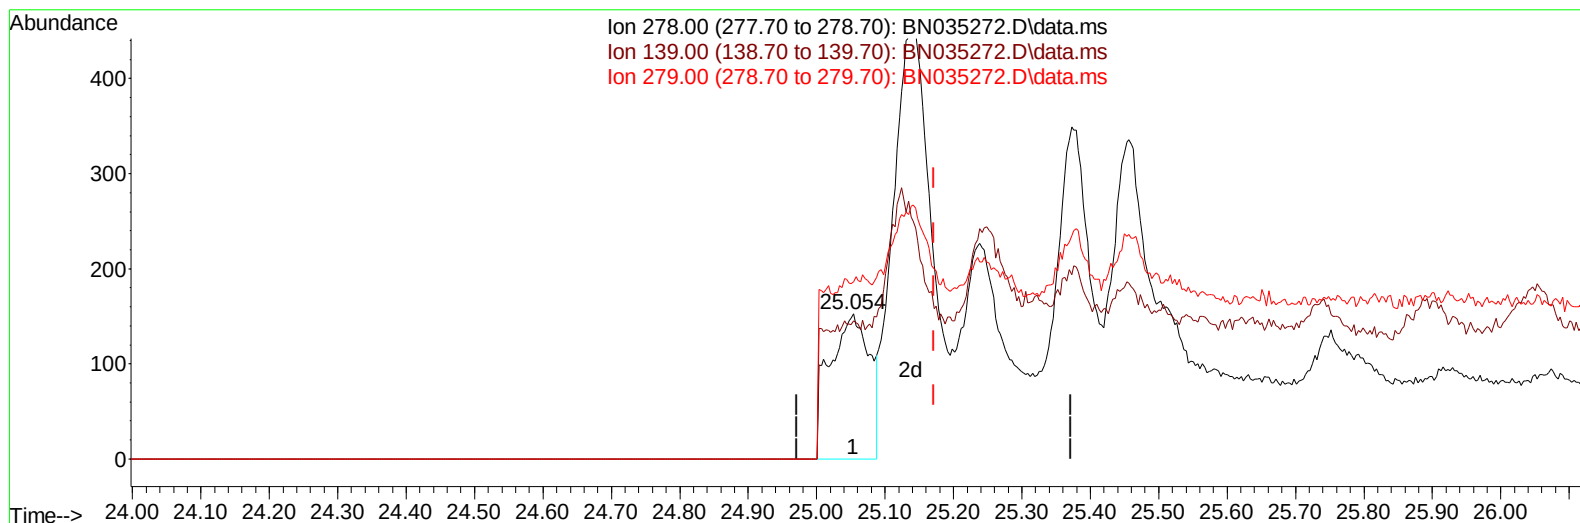

TIC: BN035272.D\data.ms

(28) Dibenzo(a,h)anthracene

25.054min (-0.117) 0.02 ng/u1

response 615

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	94.77#
279.00	28.50	121.57#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035272.D
 Acq On : 23 Nov 2024 10:35
 Operator : RC/JU
 Sample : P4872-21
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

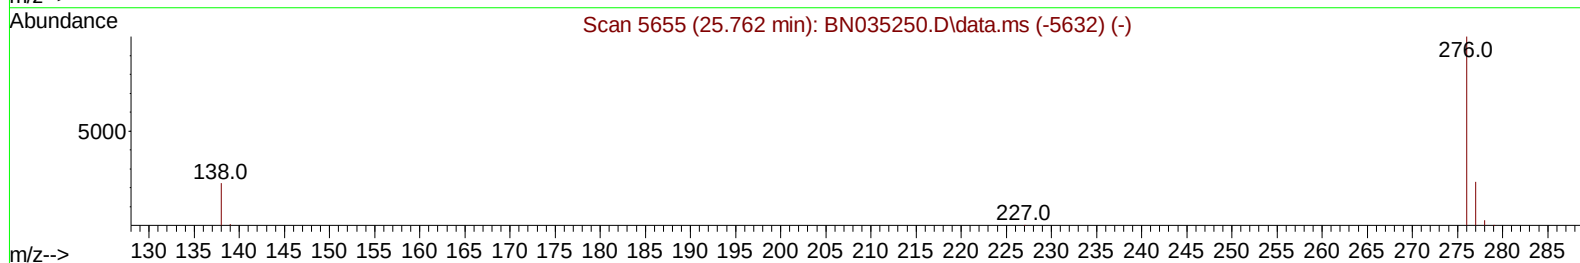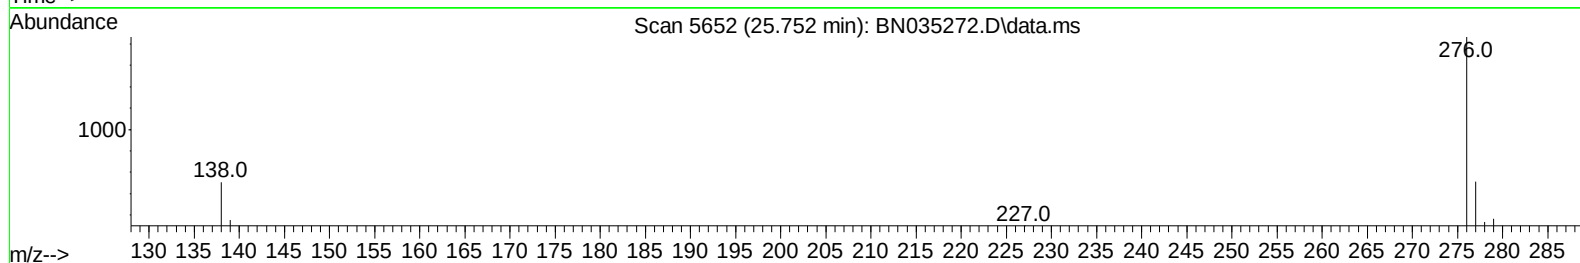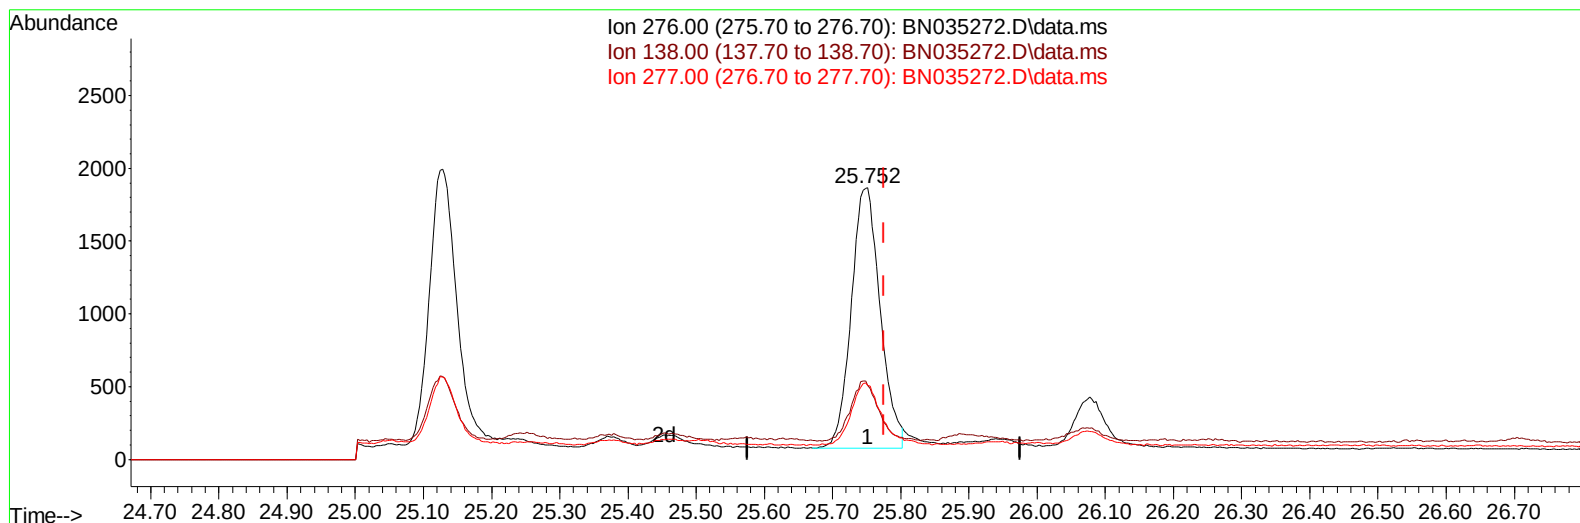

TIC: BN035272.D\data.ms

(29) Benzo(g,h,i)perylene

25.752min (-0.024) 0.21 ng/u1

response 5281

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	27.17#
277.00	25.60	27.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

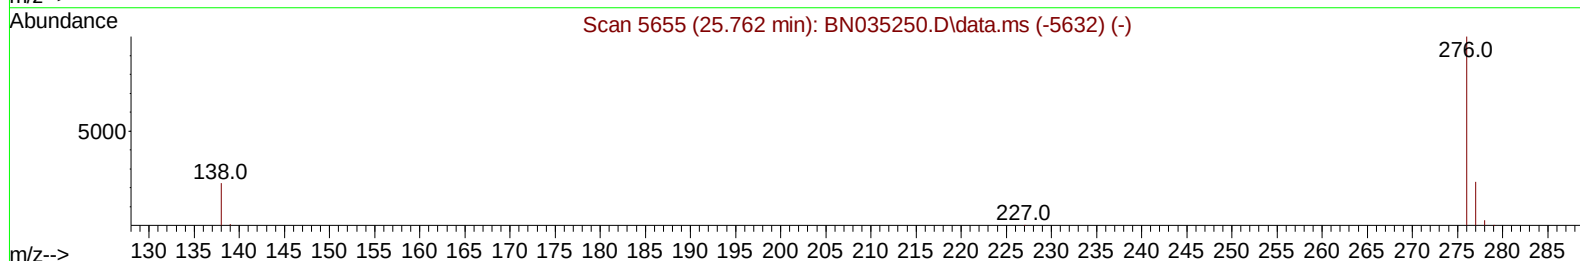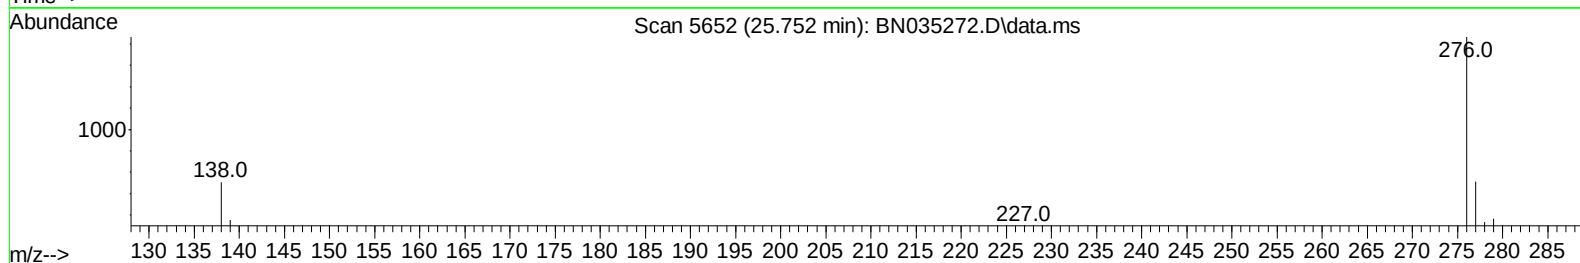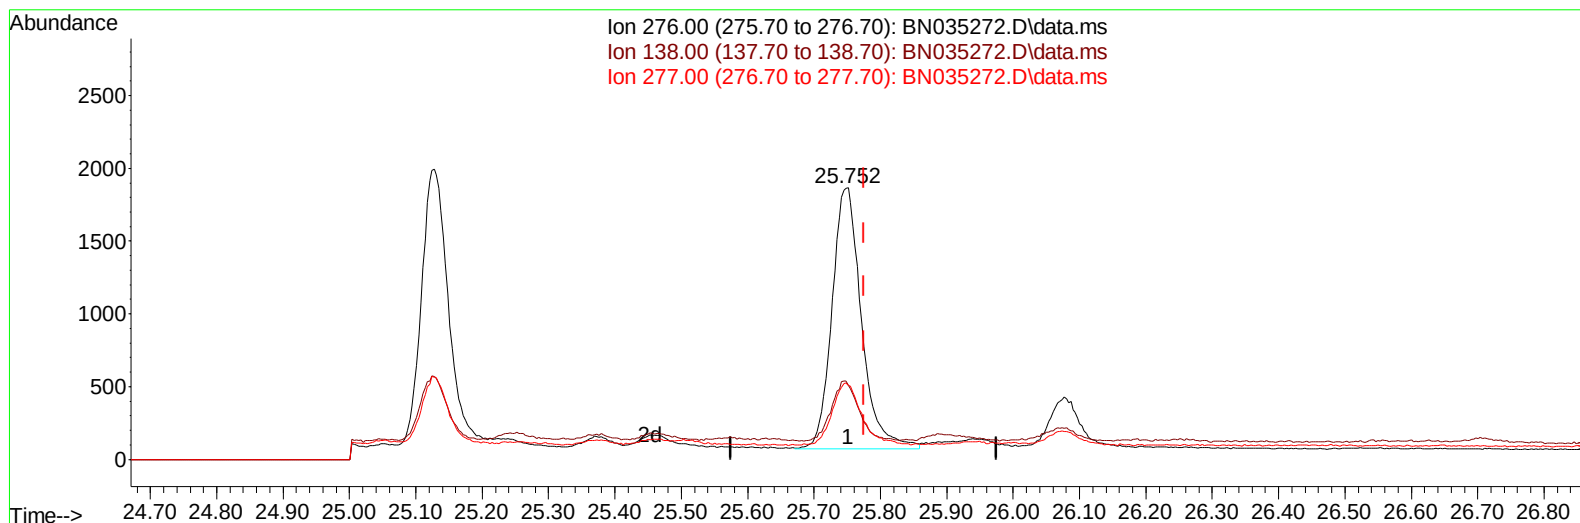

TIC: BN035272.D\data.ms

(29) Benzo(g,h,i)perylene

25.752min (-0.024) 0.22 ng/ul m

response 5510

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	27.17#
277.00	25.60	27.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035272.D
 Acq On : 23 Nov 2024 10:35
 Operator : RC/JU
 Sample : P4872-21
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.318	152		3186	0.400	ng/ul	0.00
4) Naphthalene-d8	10.064	136		8840	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	13.976	164		5706	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.743	188		13003m	0.400	ng/ul	0.00
17) Chrysene-d12	20.985	240		10167	0.400	ng/ul	# 0.00
23) Perylene-d12	23.086	264		7719m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		10811	3.713	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152		4261	0.329	ng/ul	0.00
18) Fluoranthene-d10	18.795	212		12785	0.456	ng/ul	0.00
Target Compounds					Qvalue		
10) Acenaphthylene	13.690	152		2187	0.097	ng/ul#	89
12) Fluorene	15.041	166		983	0.048	ng/ul#	92
15) Phenanthrene	16.785	178		16483	0.479	ng/ul	99
16) Anthracene	16.878	178		4460	0.140	ng/ul#	94
19) Fluoranthene	18.828	202		37118	1.049	ng/ul#	95
20) Pyrene	19.195	202		28329m	0.769	ng/ul	
21) Benzo(a)anthracene	20.970	228		11835	0.335	ng/ul	93
22) Chrysene	21.020	228		11651	0.328	ng/ul	96
24) Benzo(b)fluoranthene	22.472	252		12727m	0.499	ng/ul	
25) Benzo(k)fluoranthene	22.507	252		5170m	0.197	ng/ul	
26) Benzo(a)pyrene	22.995	252		8201m	0.352	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.128	276		5319m	0.169	ng/ul	
28) Dibenzo(a,h)anthracene	25.138	278		1120m	0.045	ng/ul	
29) Benzo(g,h,i)perylene	25.752	276		5510m	0.222	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035272.D
Acq On : 23 Nov 2024 10:35
Operator : RC/JU
Sample : P4872-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y8

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

