




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

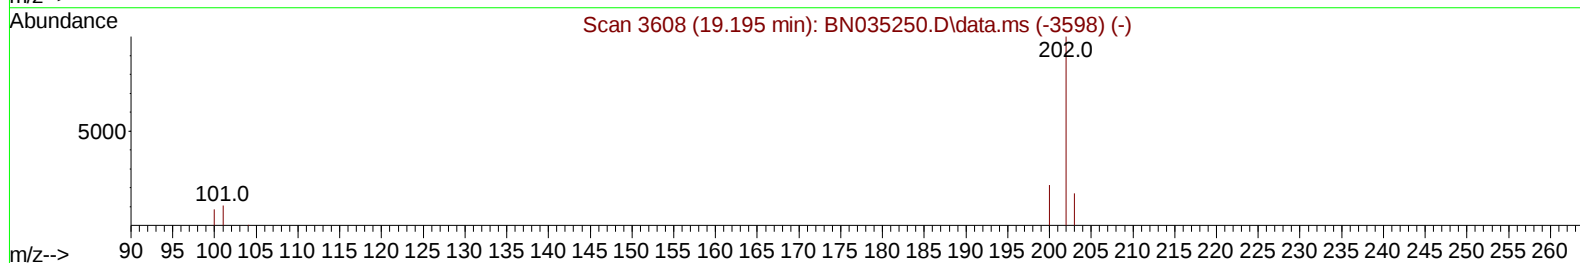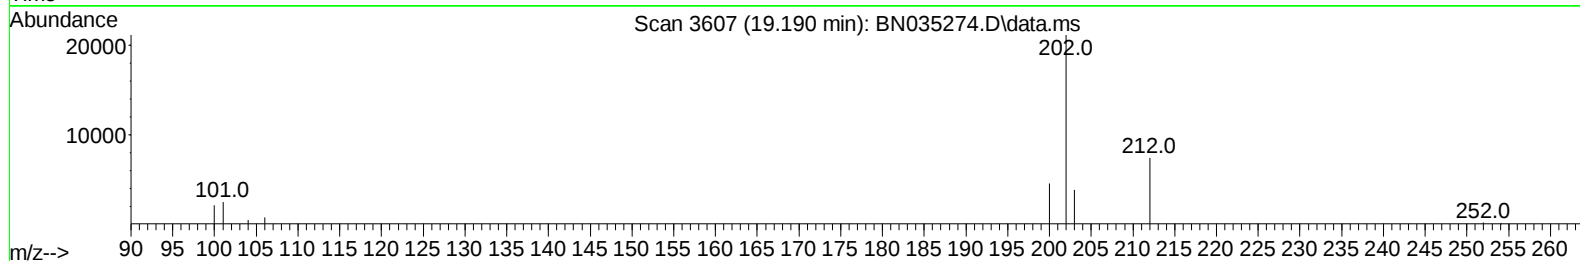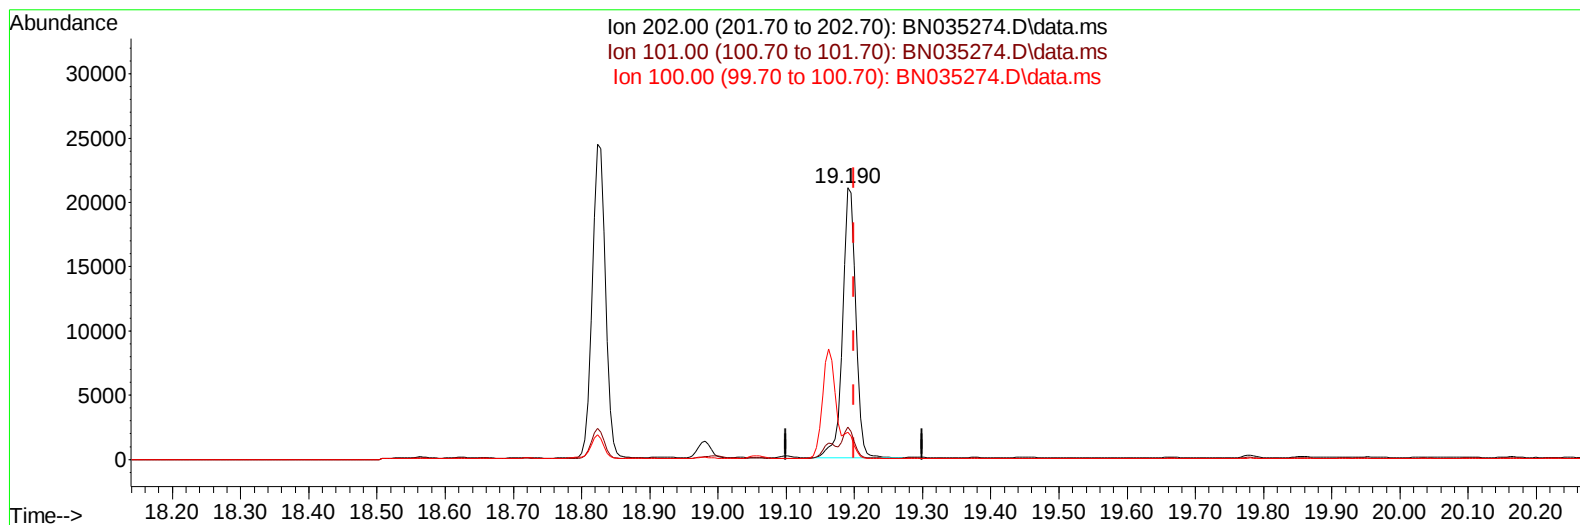

TIC: BN035274.D\data.ms

(20) Pyrene

19.190min (-0.009) 0.70 ng/u1

response 27810

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	11.87#
100.00	6.40	10.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

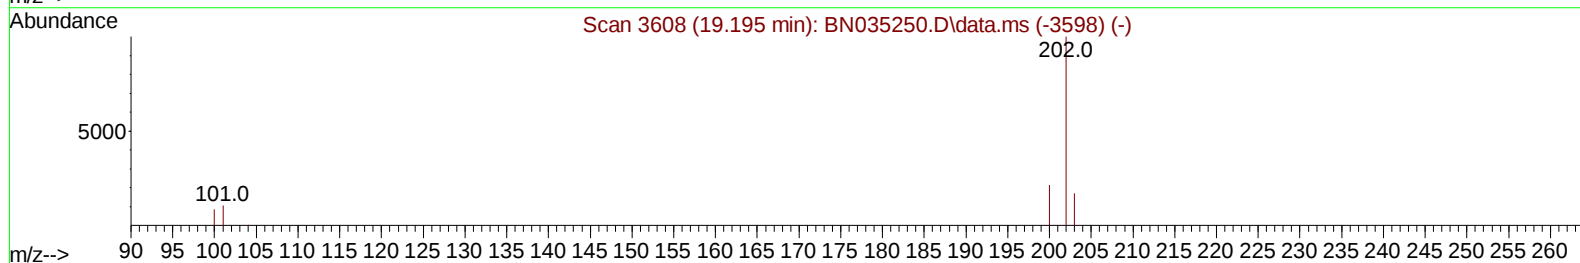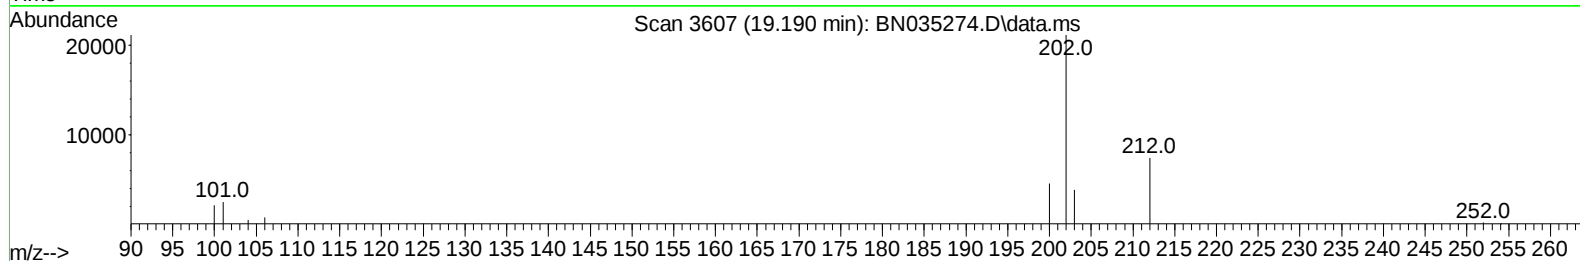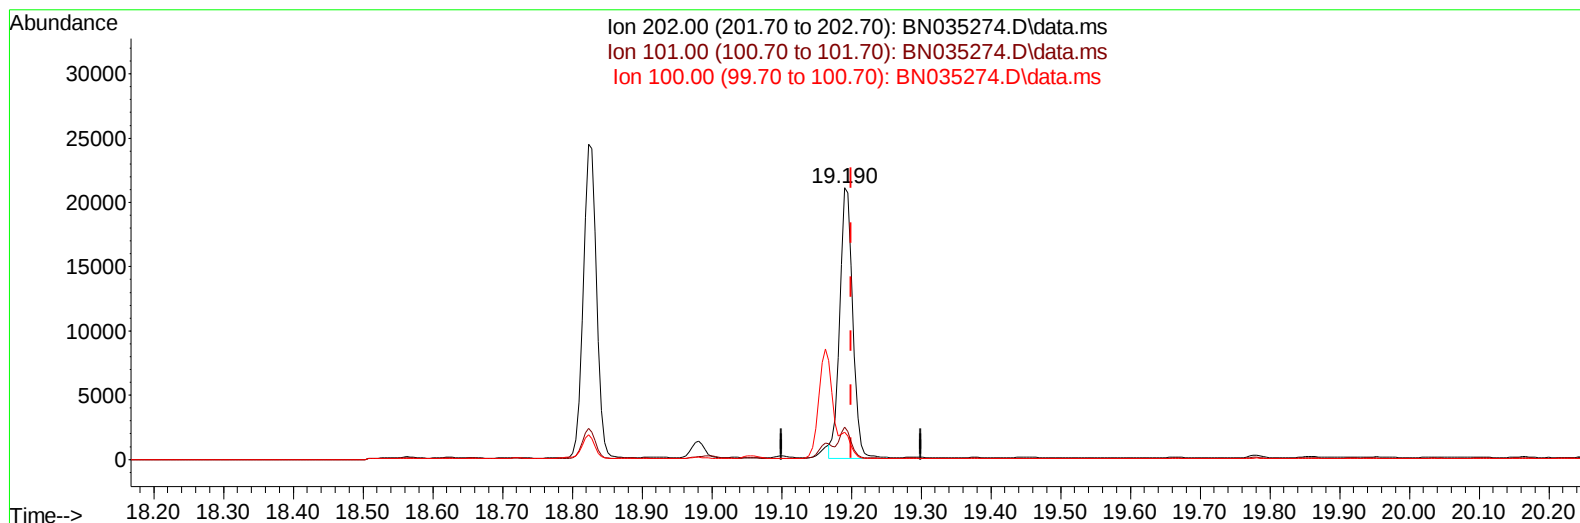

TIC: BN035274.D\data.ms

(20) Pyrene

19.190min (-0.009) 0.69 ng/ul m

response 27172

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	7.80	11.87#
100.00	6.40	10.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

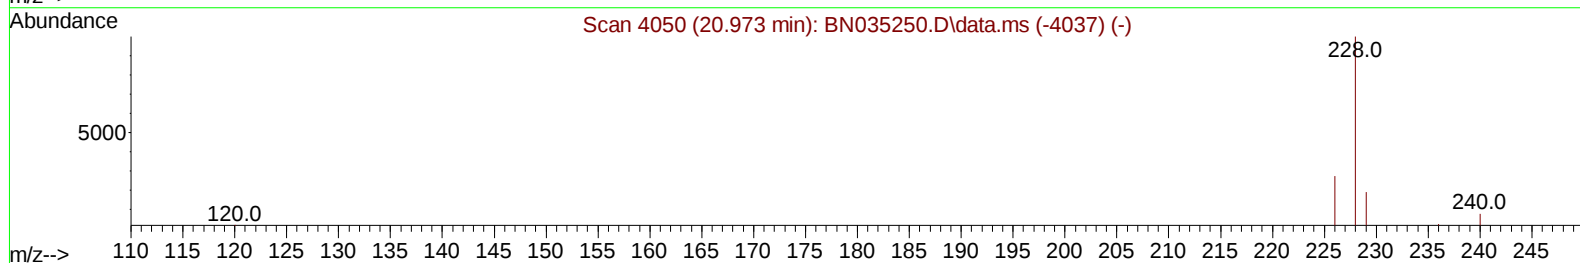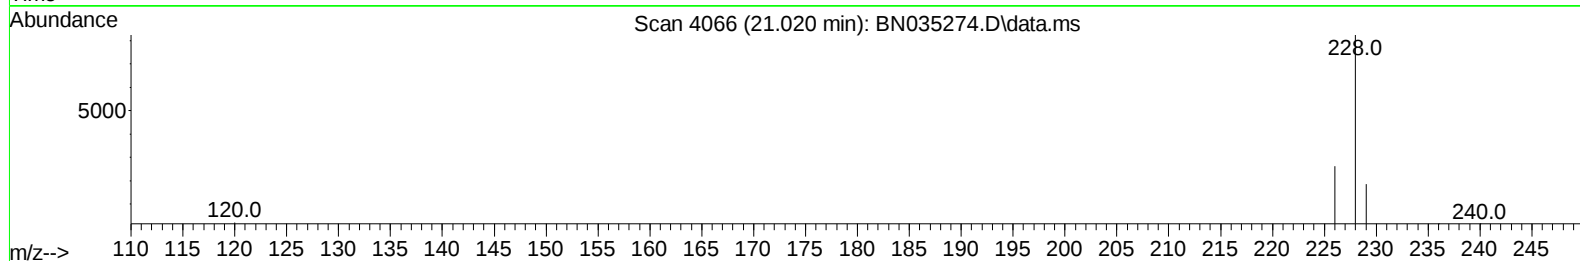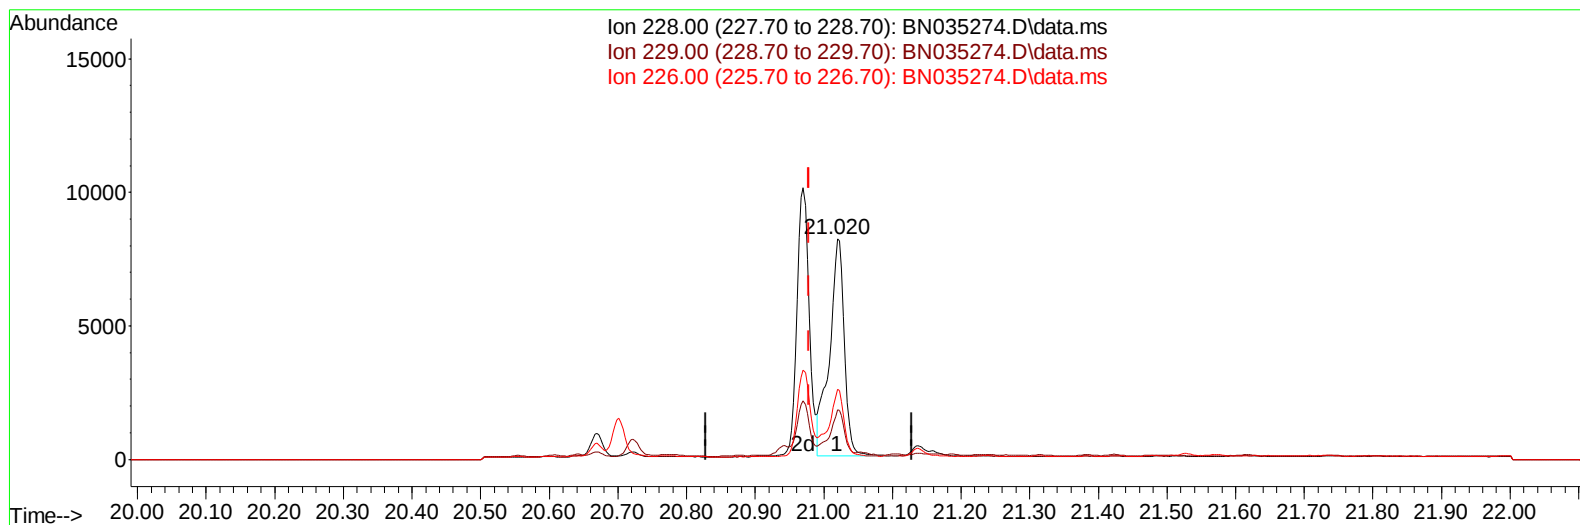

TIC: BN035274.D\data.ms

(21) Benzo(a)anthracene

21.020min (+ 0.041) 0.32 ng/u1

response 12212

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	22.42
226.00	27.30	31.94
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

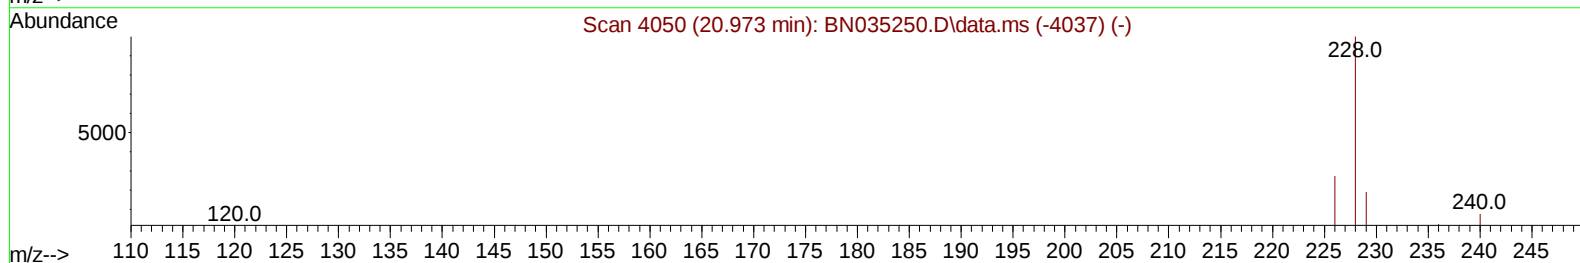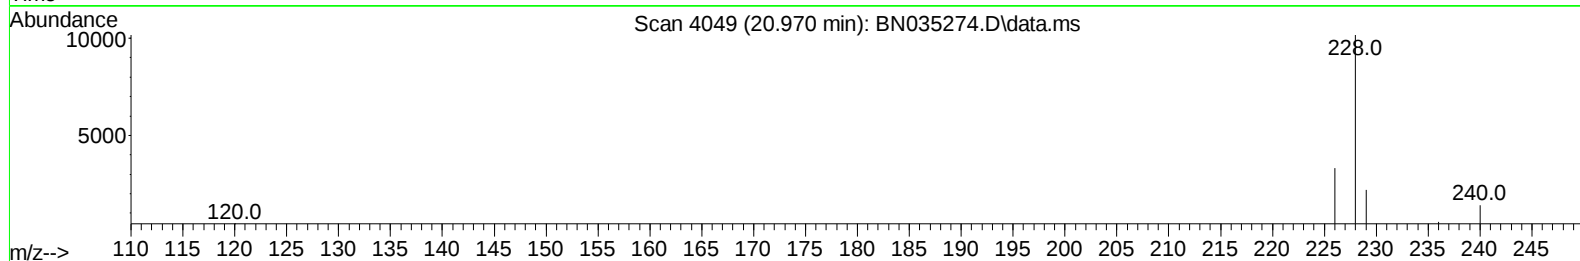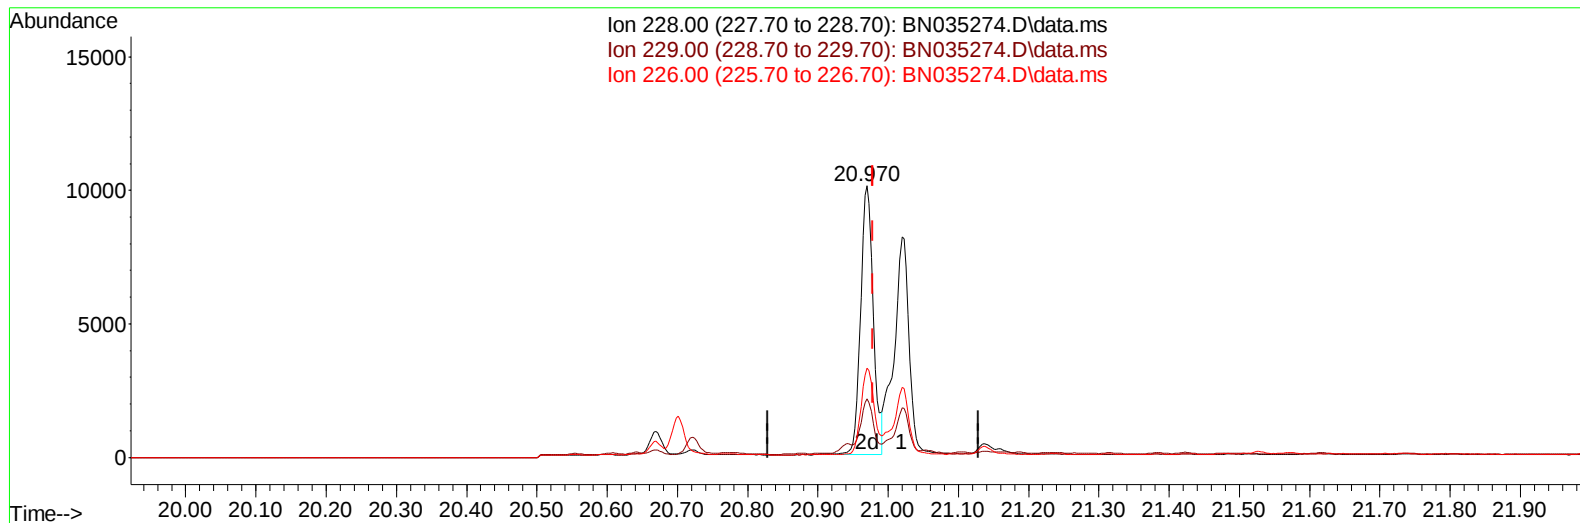

TIC: BN035274.D\data.ms

(21) Benzo(a)anthracene

20.970min (-0.009) 0.33 ng/u1 m

response 12589

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	21.58
226.00	27.30	32.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035274.D
 Acq On : 23 Nov 2024 11:47
 Operator : RC/JU
 Sample : P4872-18
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

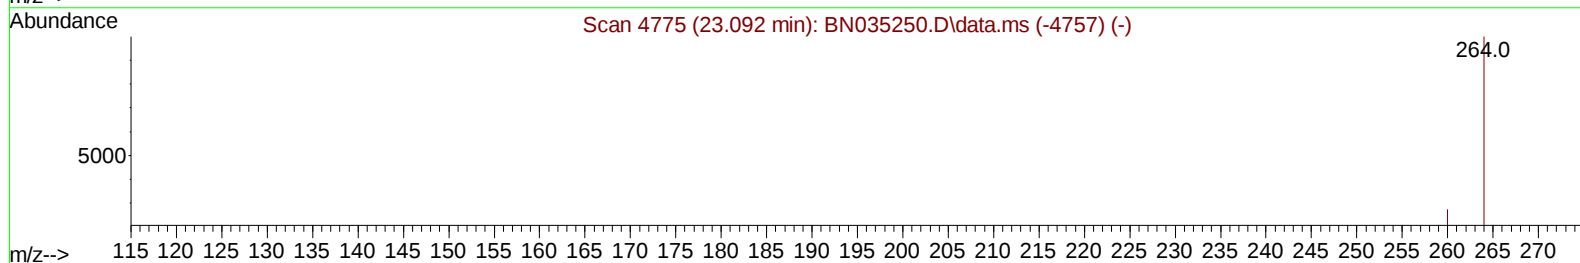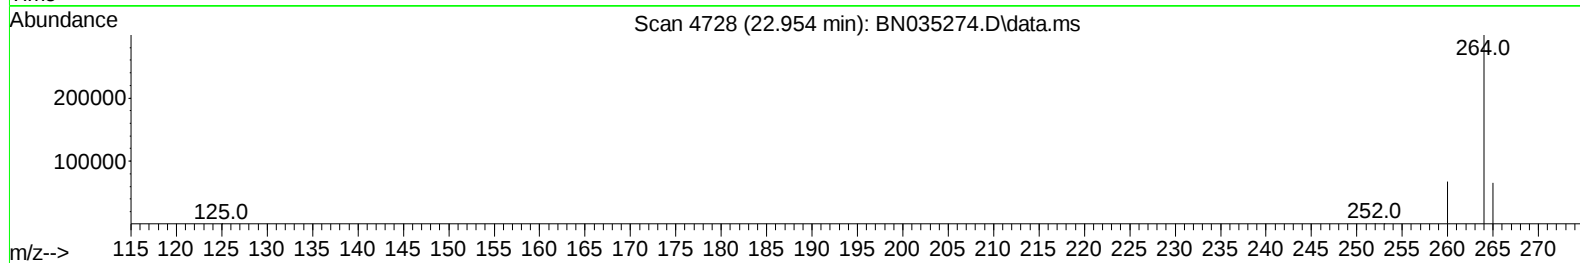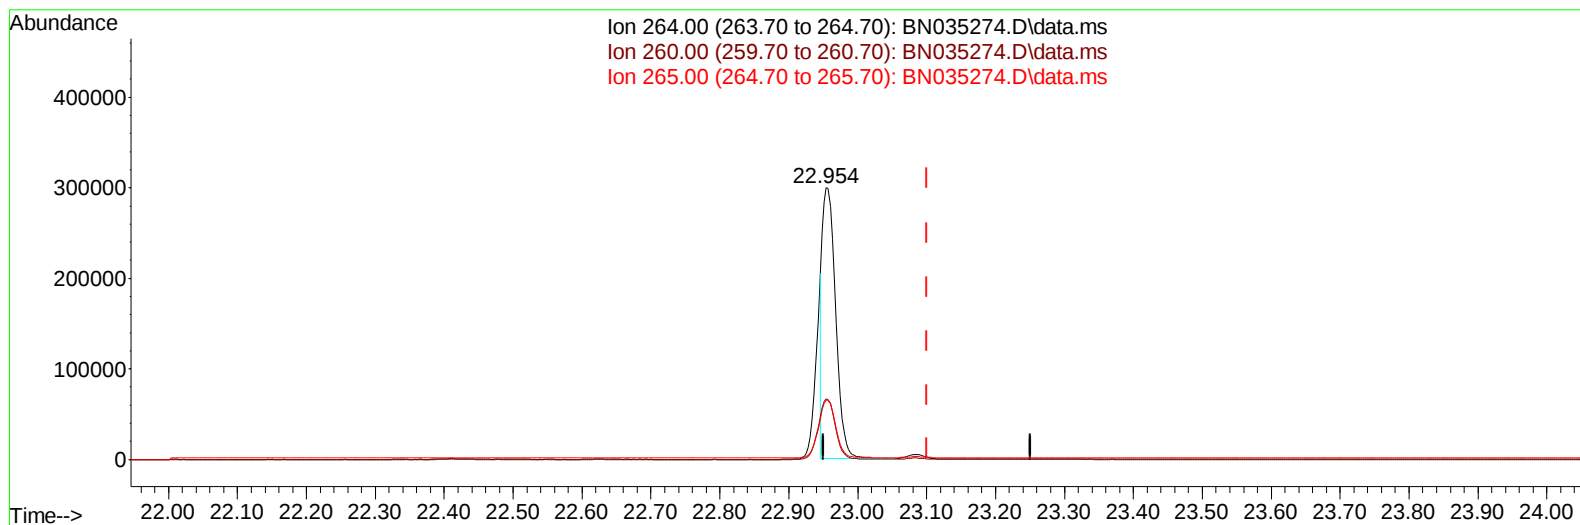

TIC: BN035274.D\data.ms

(23) Perylene-d12 (I)

22.954min (-0.146) 0.40 ng/u1

response 403757

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	22.38
265.00	75.50	21.79#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

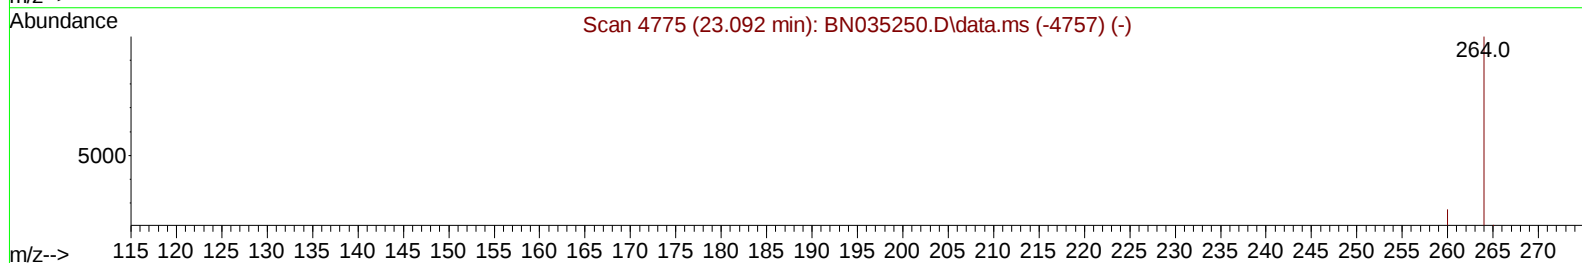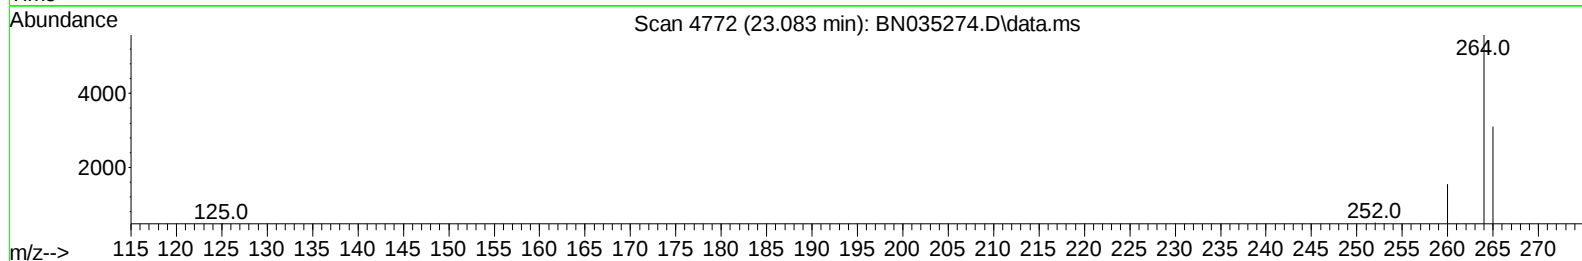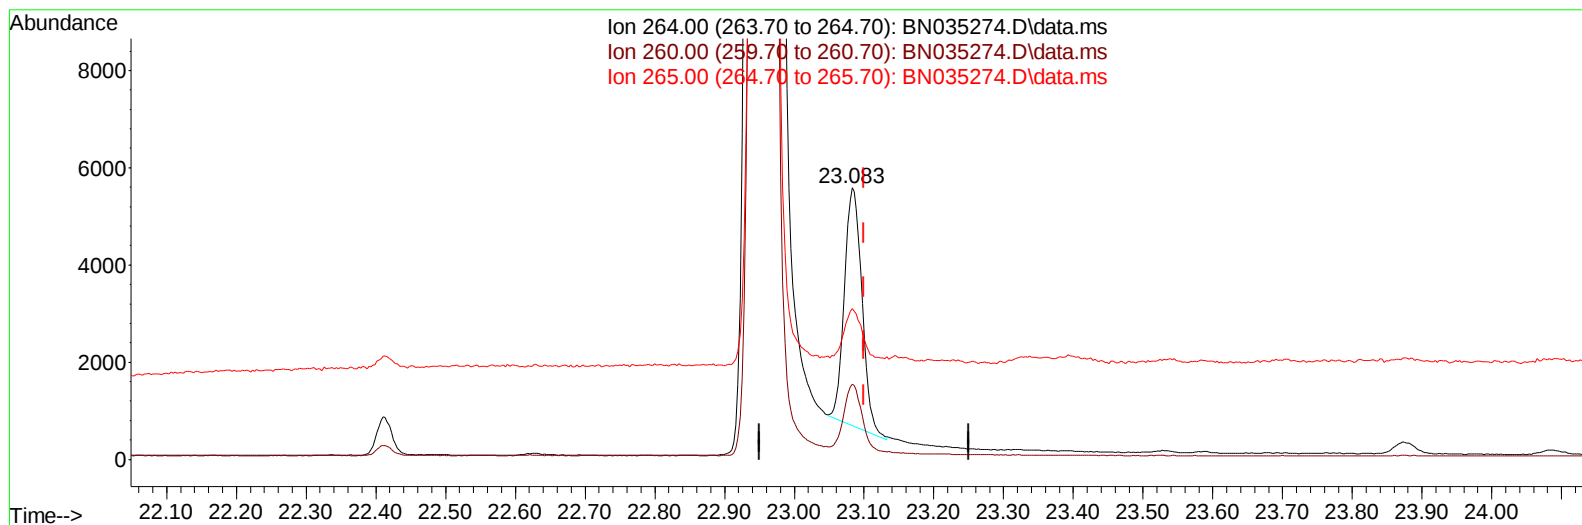

TIC: BN035274.D\data.ms

(23) Perylene-d12 (I)

23.083min (-0.017) 0.40 ng/ul m

response 8523

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	27.79
265.00	75.50	55.56#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

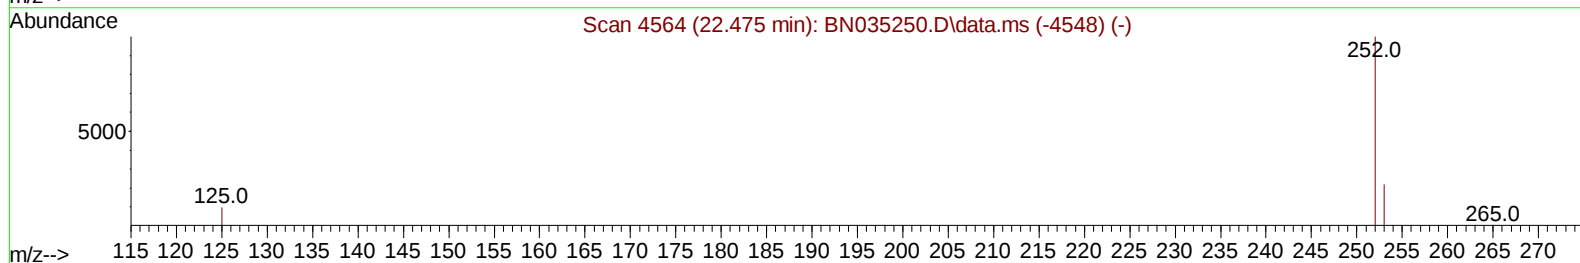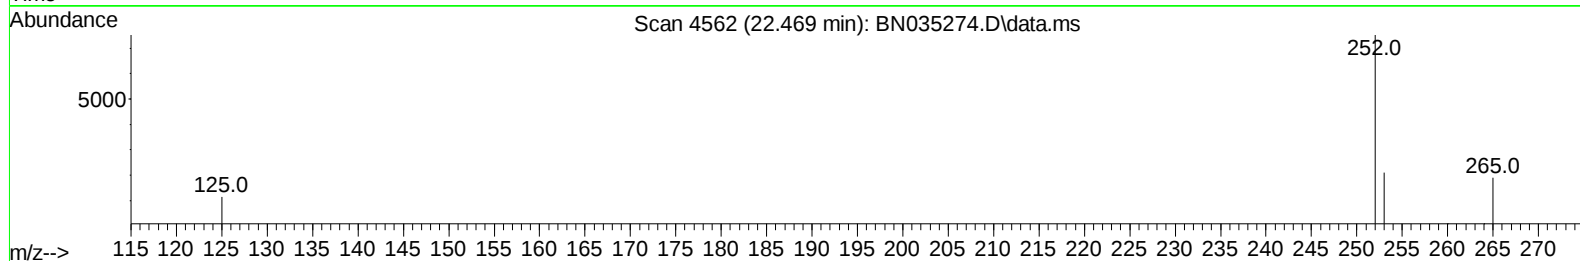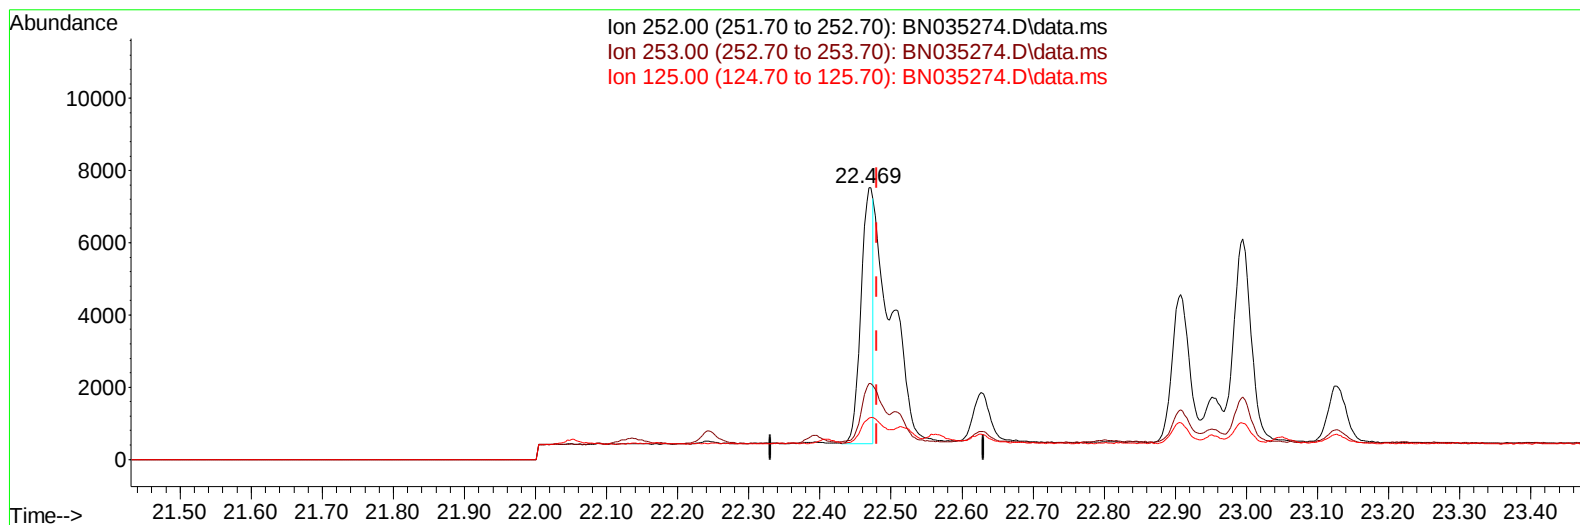

TIC: BN035274.D\data.ms

(24) Benzo(b)fluoranthene

22.469min (-0.012) 0.30 ng/u1

response 8447

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.96
125.00	9.70	15.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

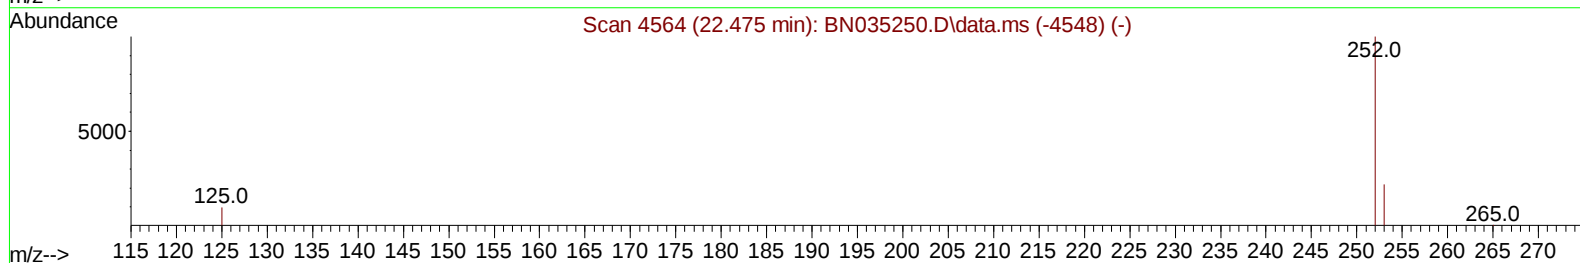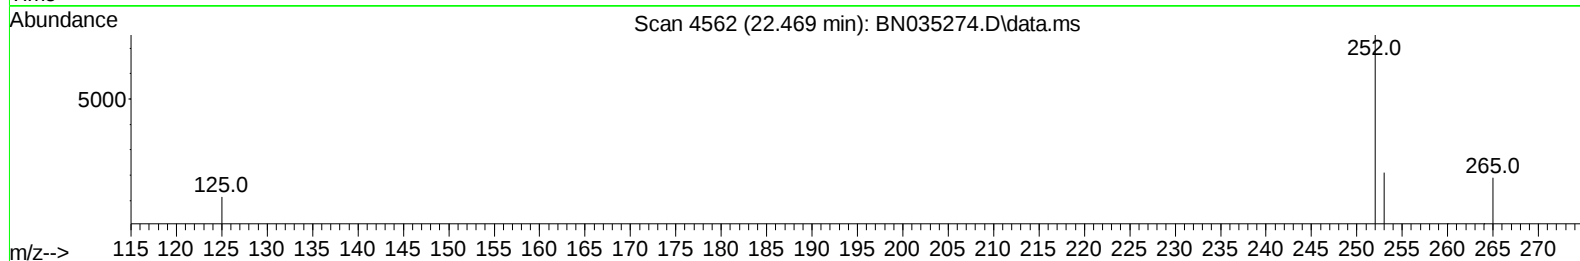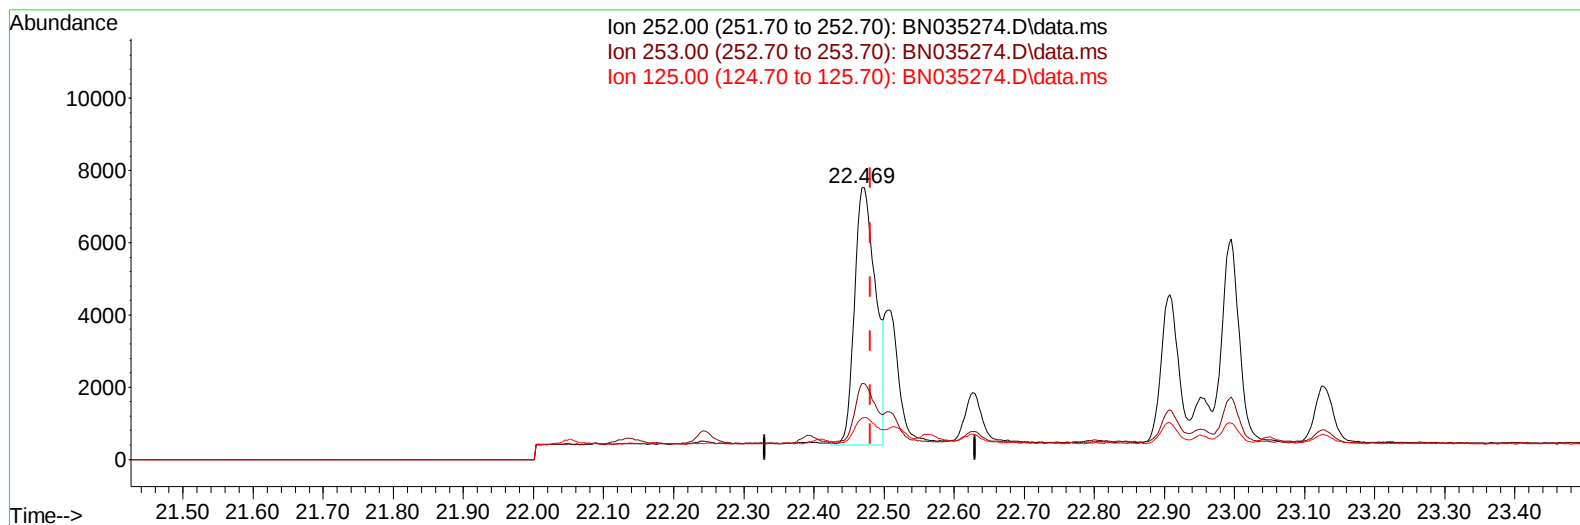

TIC: BN035274.D\data.ms

(24) Benzo(b)fluoranthene

22.469min (-0.012) 0.53 ng/u1 m

response 14966

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.00	27.96
125.00	9.70	15.28
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

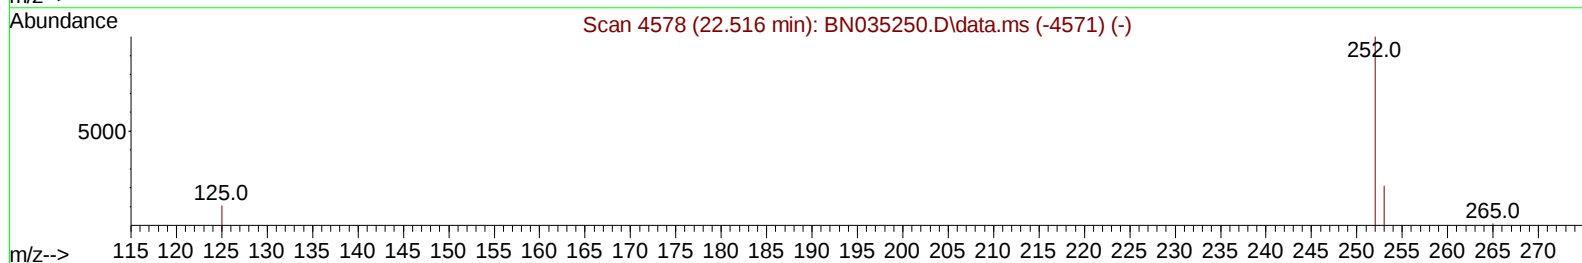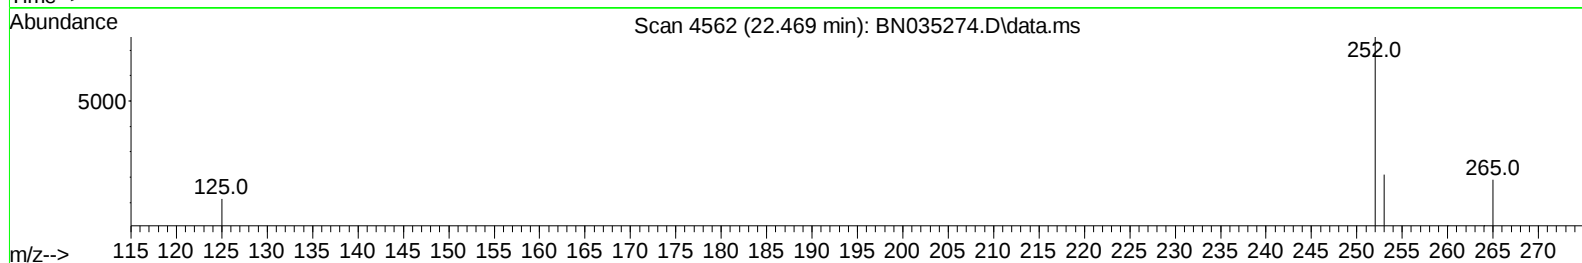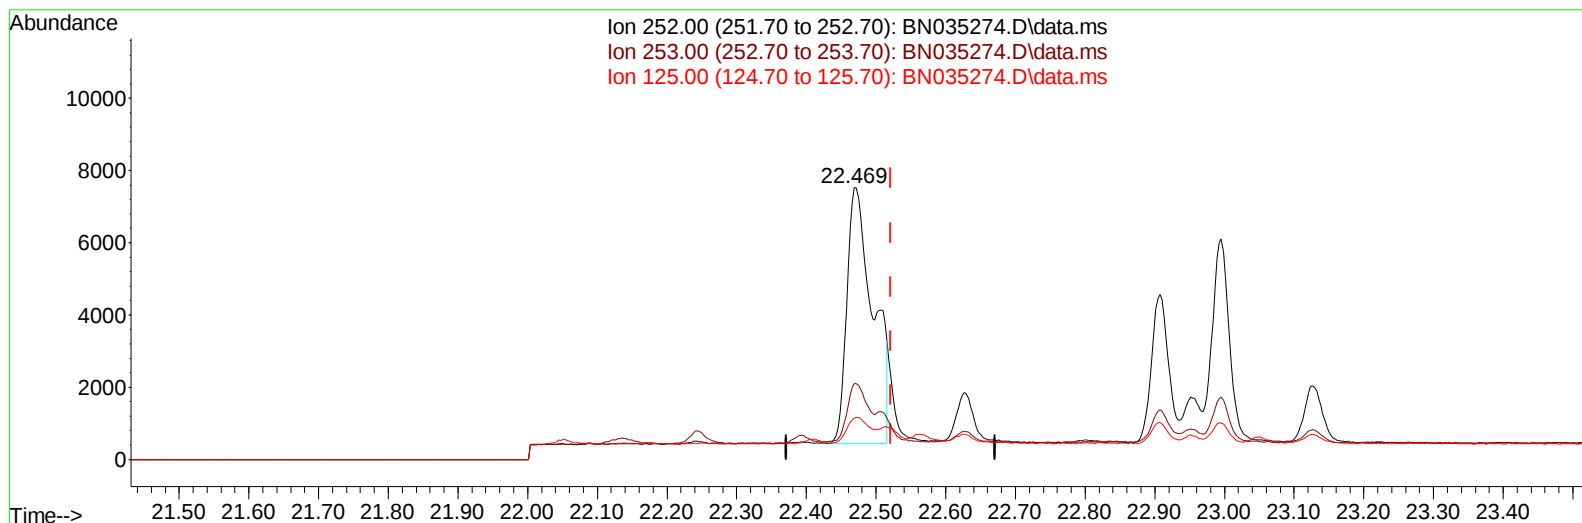

TIC: BN035274.D\data.ms

(25) Benzo(k)fluoranthene

22.469min (-0.053) 0.64 ng/u1

response 18482

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	27.96
125.00	10.70	15.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

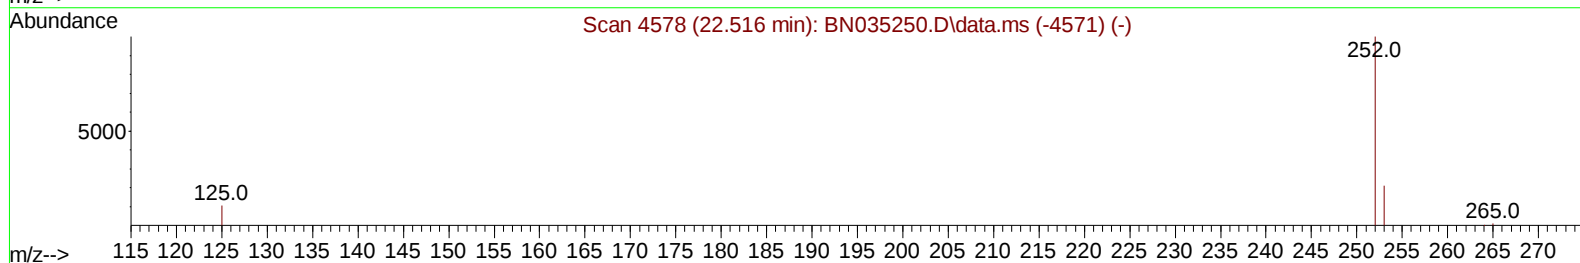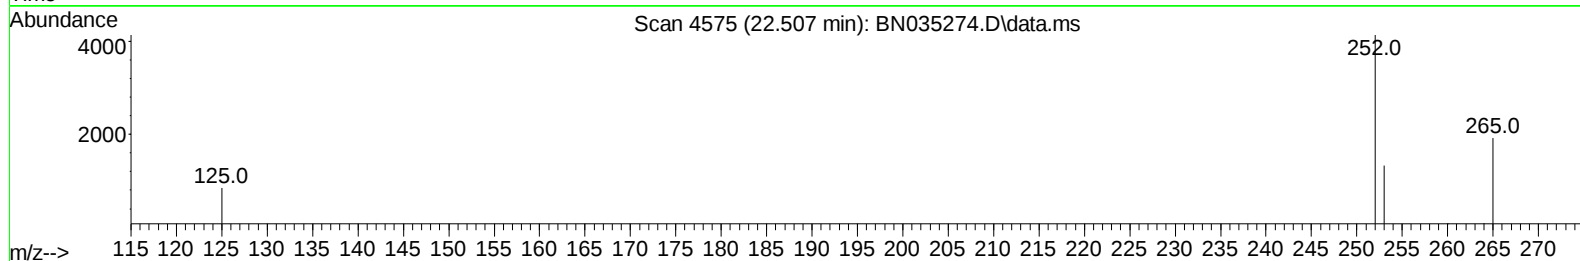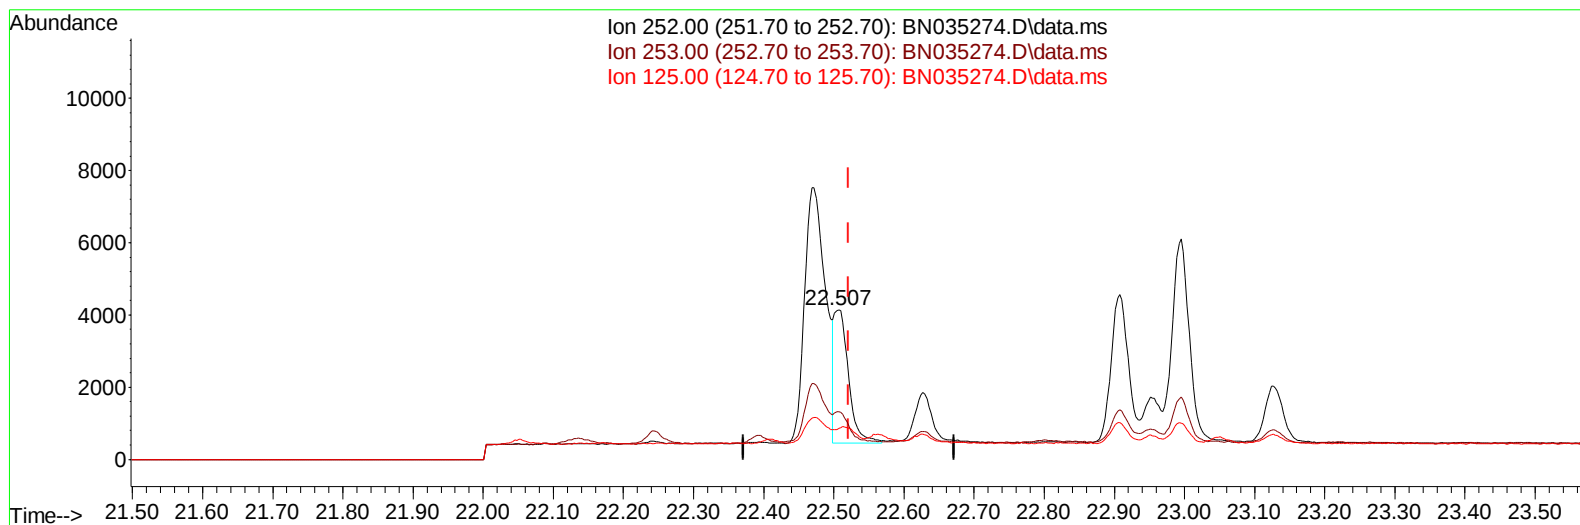

TIC: BN035274.D\data.ms

(25) Benzo(k)fluoranthene

22.507min (-0.015) 0.18 ng/u1 m

response 5191

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	32.12
125.00	10.70	20.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

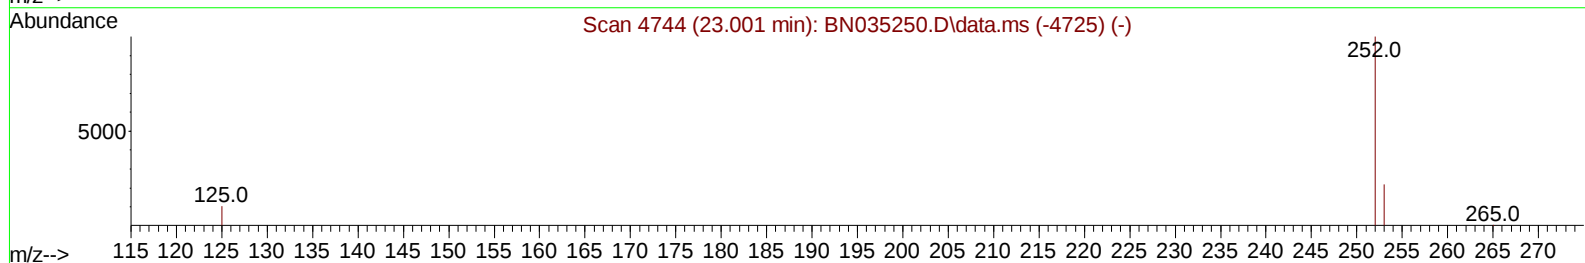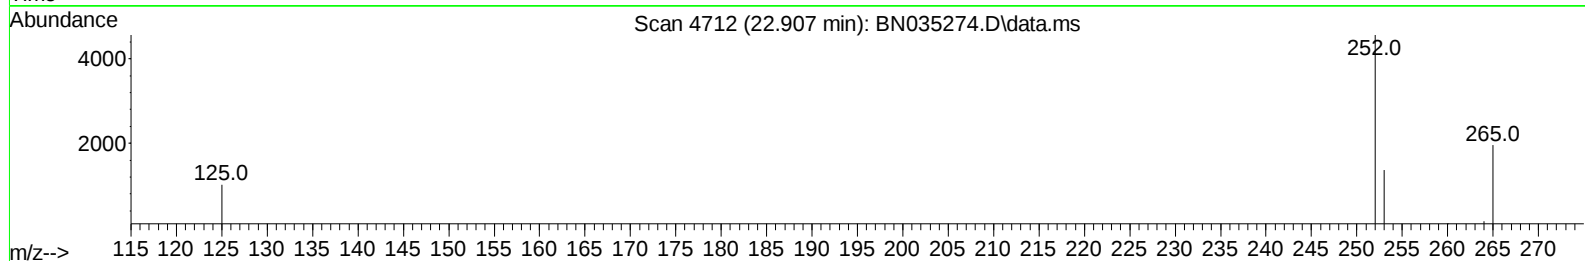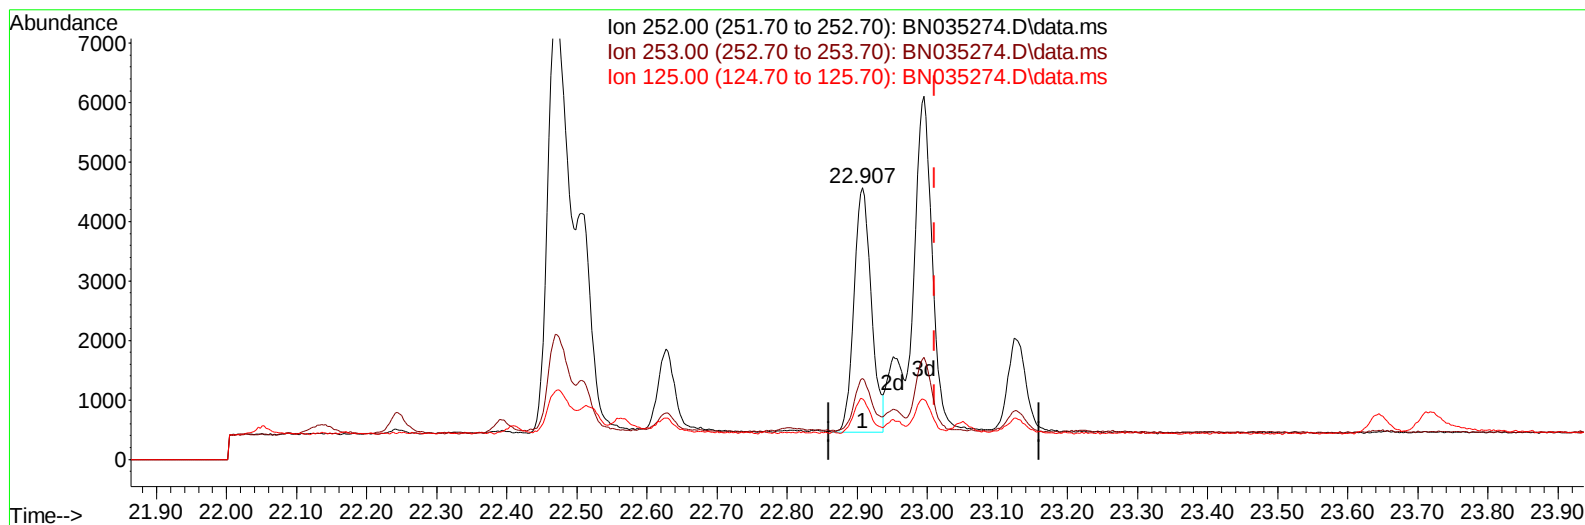

TIC: BN035274.D\data.ms

(26) Benzo(a)pyrene (C)

22.907min (-0.102) 0.28 ng/u1

response 7099

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	29.94
125.00	11.80	22.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

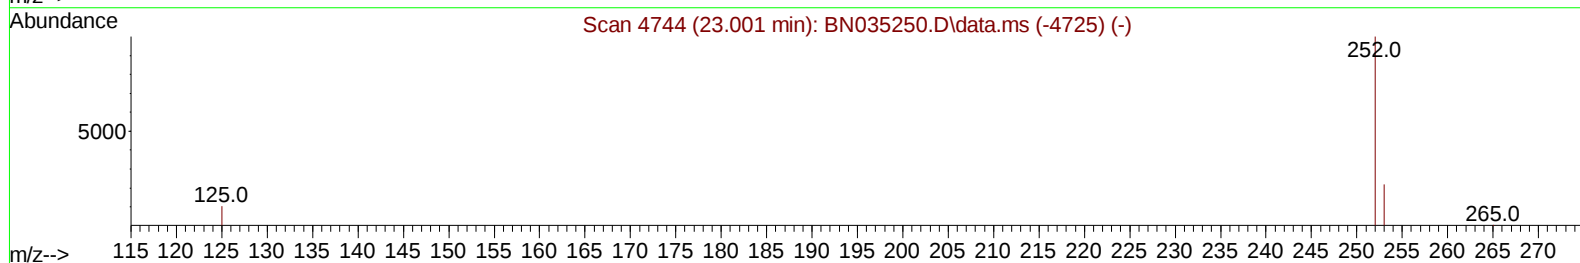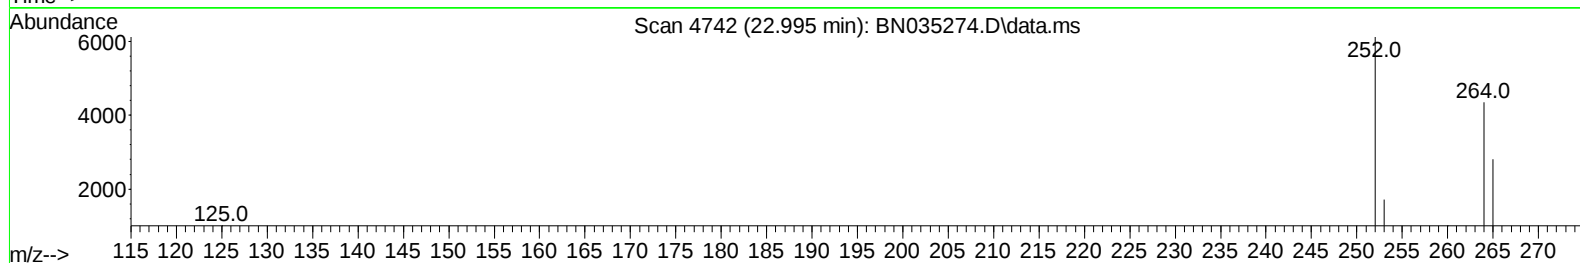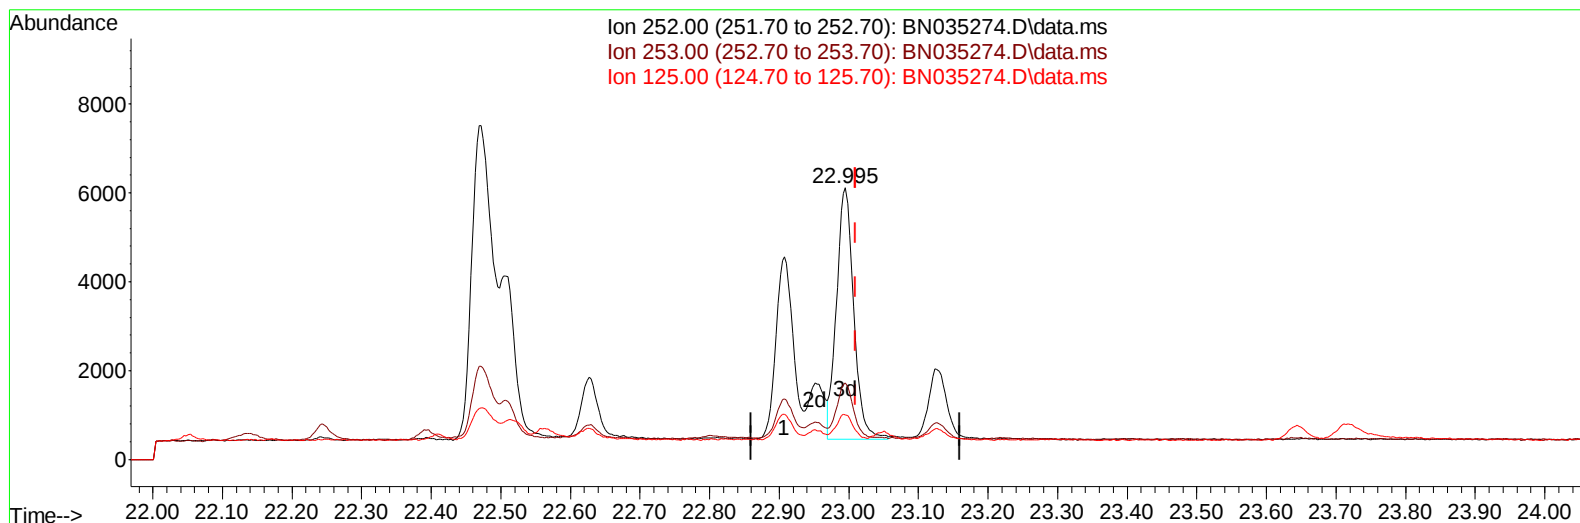

TIC: BN035274.D\data.ms

(26) Benzo(a)pyrene (C)

22.995min (-0.015) 0.38 ng/u1 m

response 9697

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.60	28.15
125.00	11.80	16.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

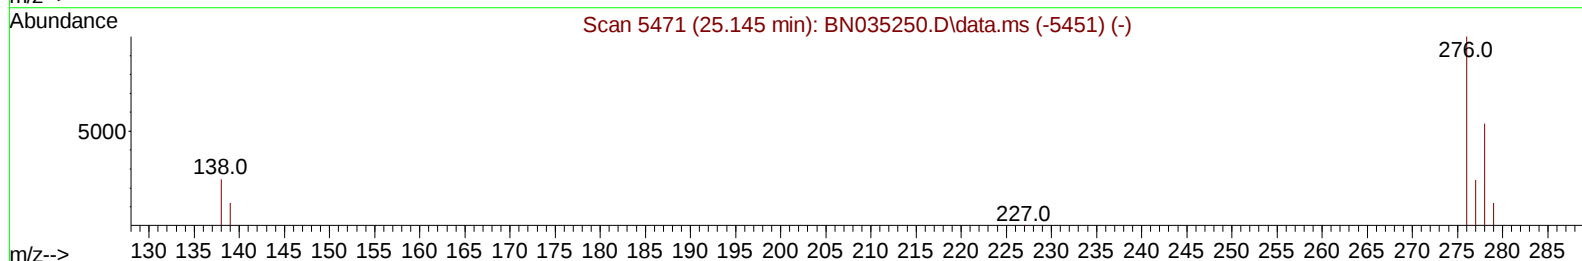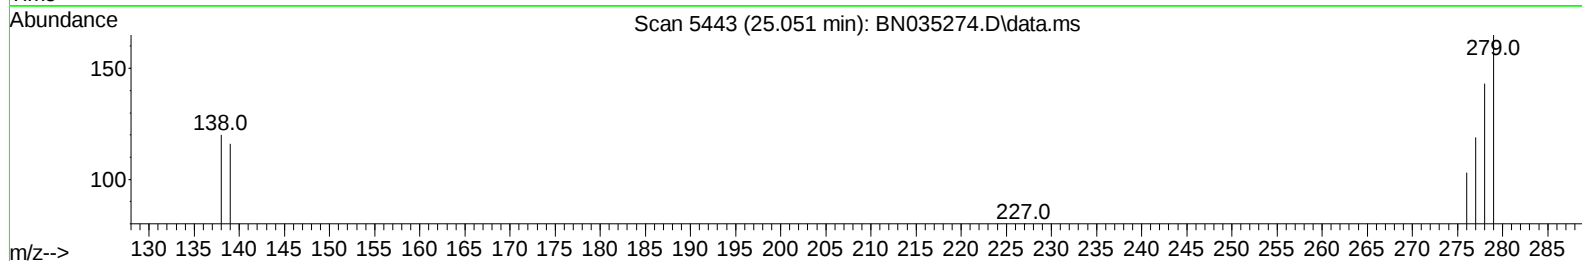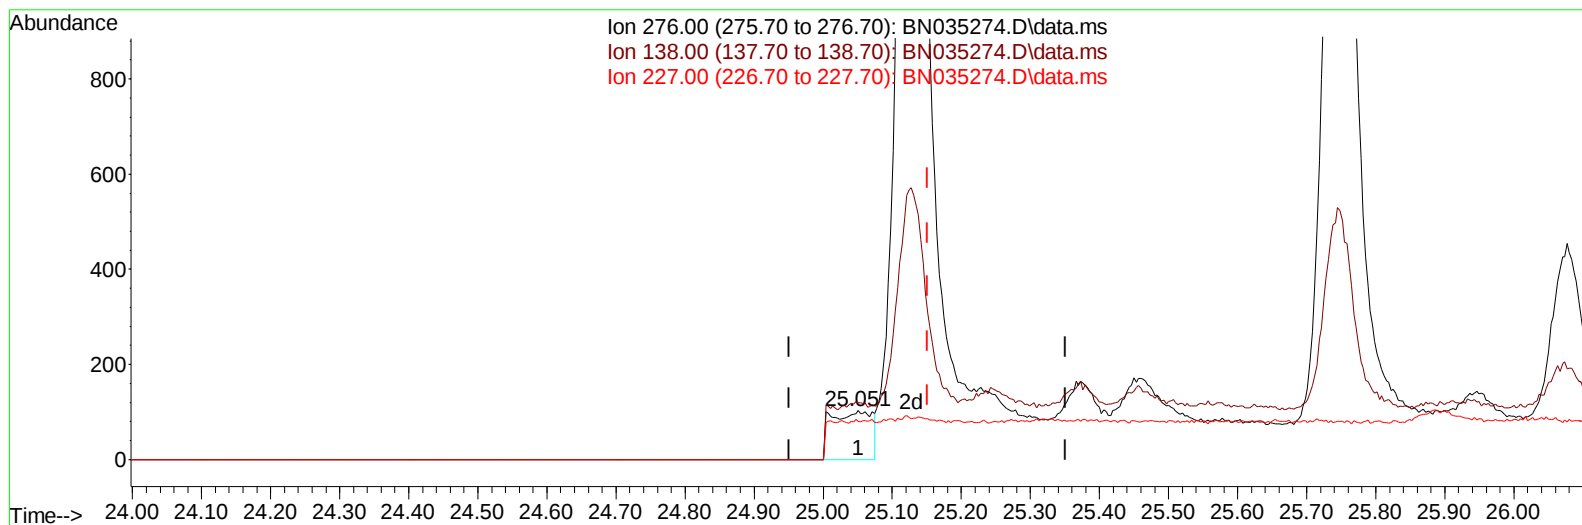

TIC: BN035274.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.051min (-0.101) 0.01 ng/u1

response 409

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	133.01#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

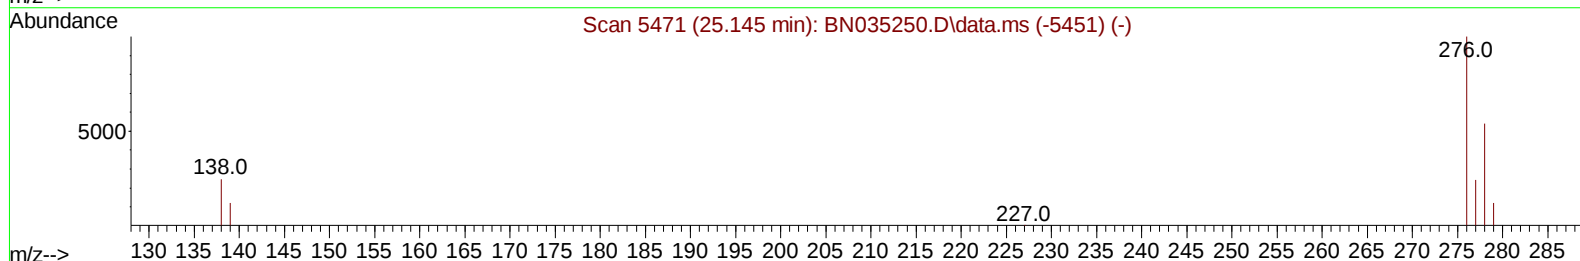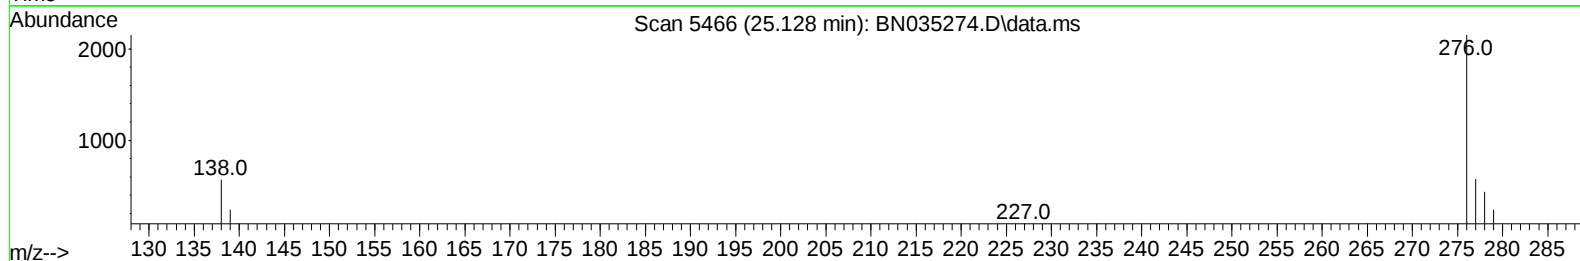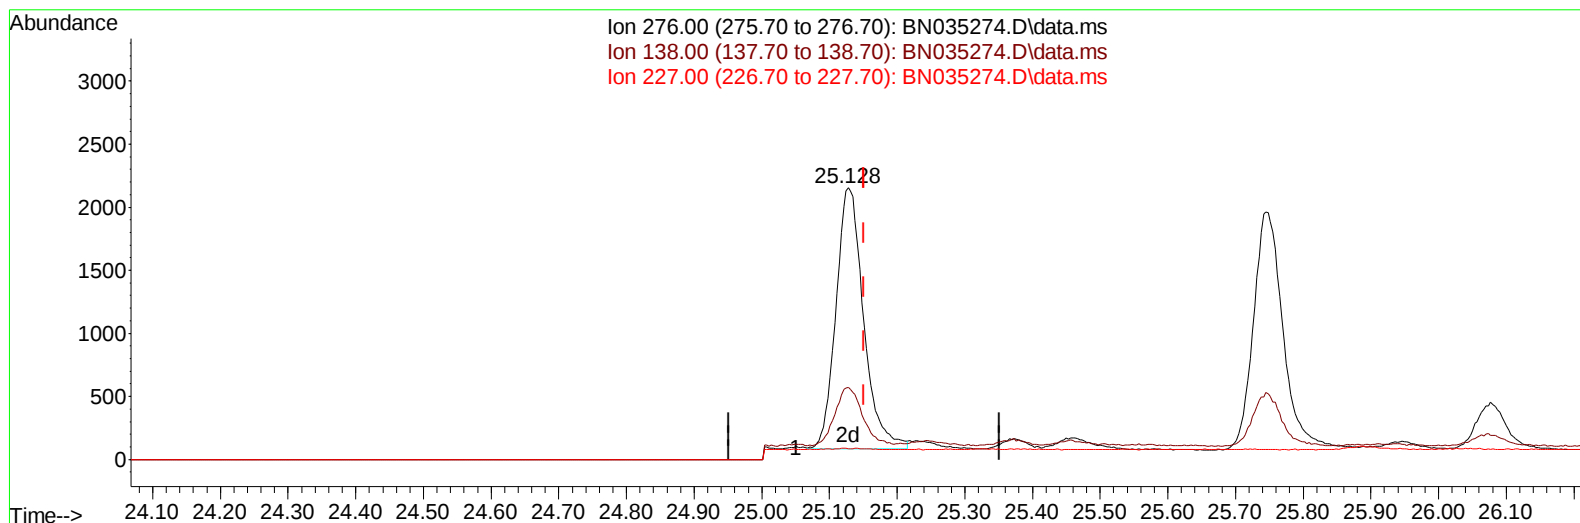

TIC: BN035274.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.128min (-0.023) 0.17 ng/u1 m

response 5894

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	17.30	9.23#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

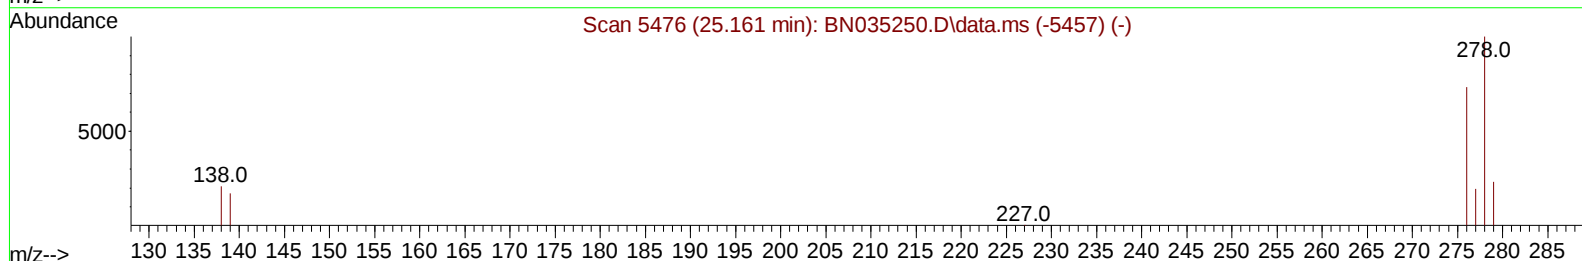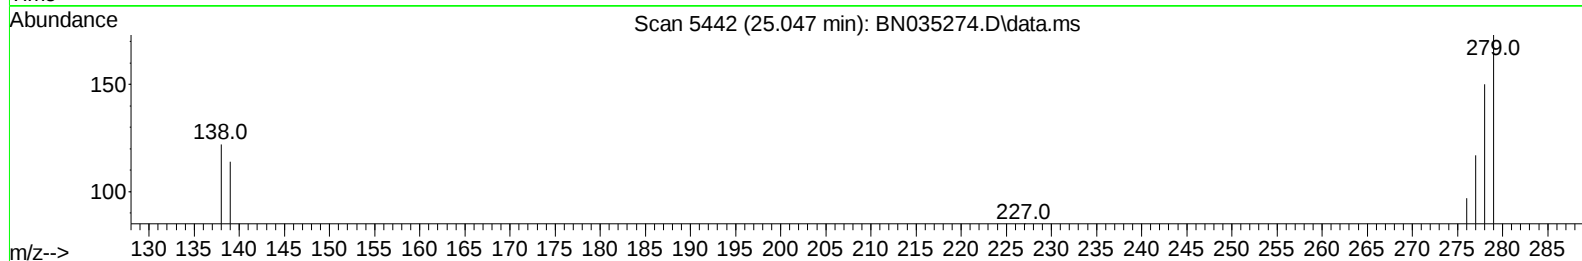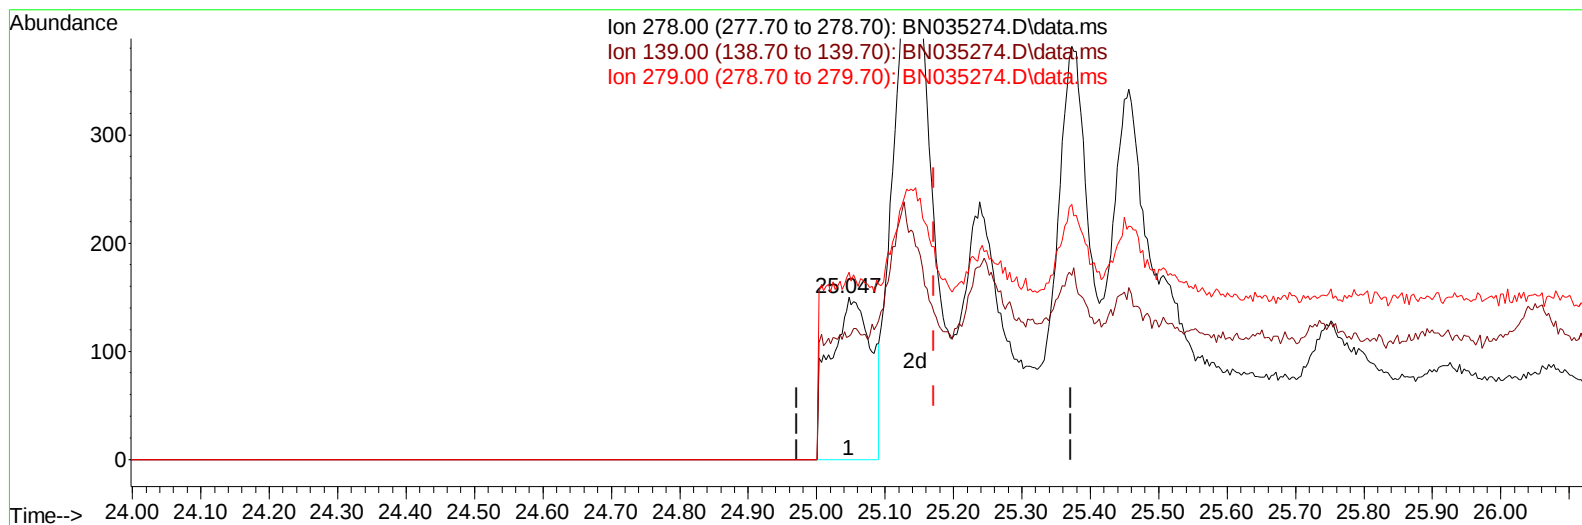

TIC: BN035274.D\data.ms

(28) Dibenzo(a,h)anthracene

25.047min (-0.124) 0.02 ng/u1

response 618

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	76.00#
279.00	28.50	115.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

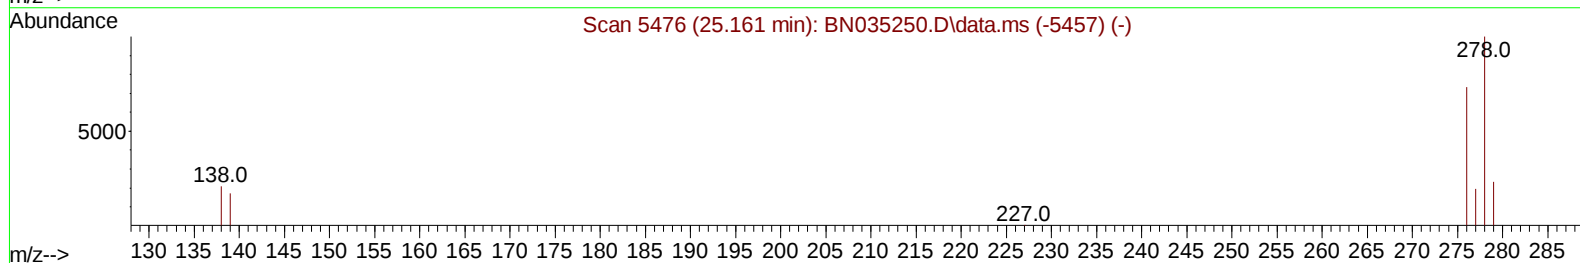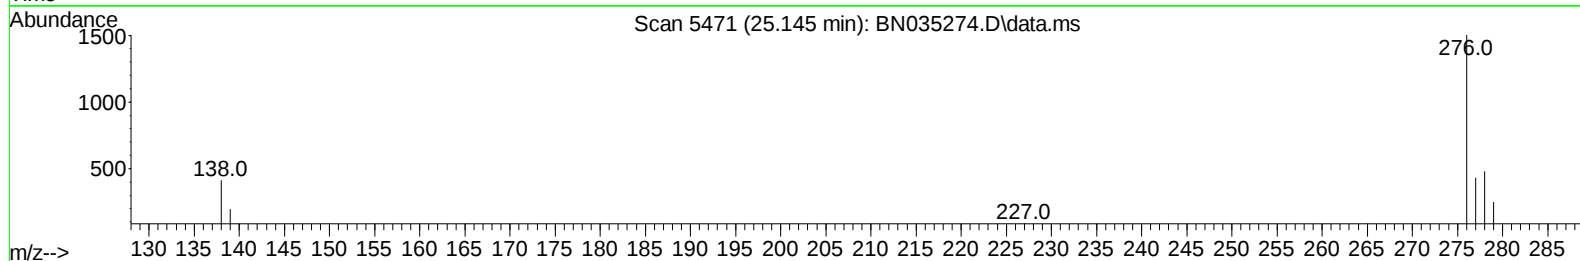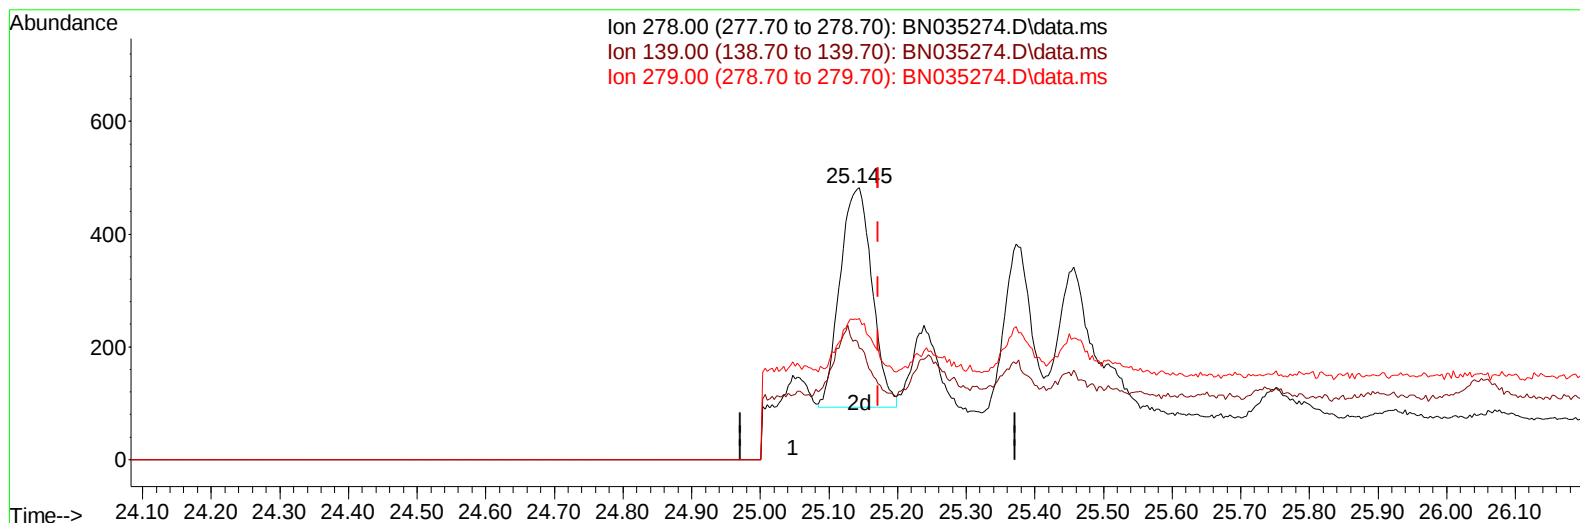

TIC: BN035274.D\data.ms

(28) Dibenzo(a,h)anthracene

25.145min (-0.027) 0.05 ng/u1 m

response 1262

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.40	40.87#
279.00	28.50	52.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

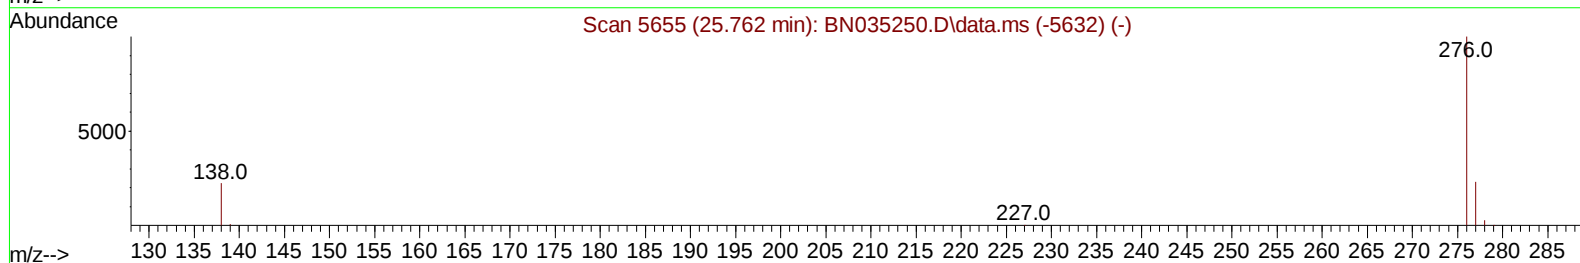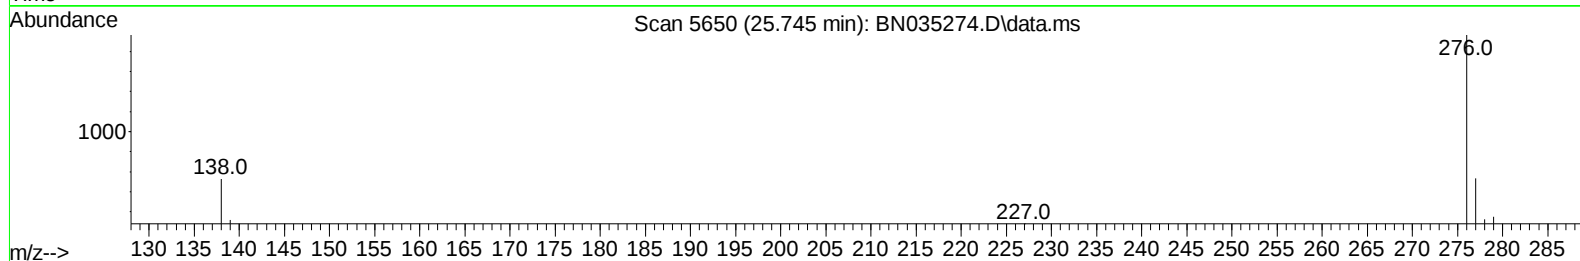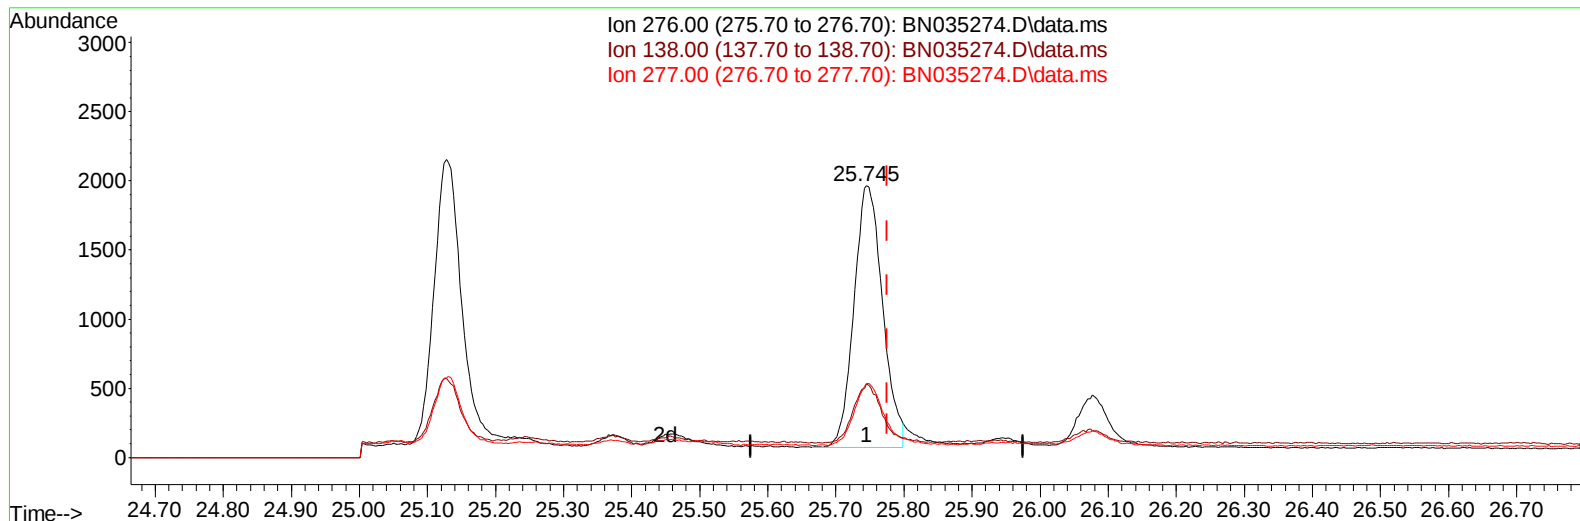

TIC: BN035274.D\data.ms

(29) Benzo(g,h,i)perylene

25.745min (-0.030) 0.20 ng/u1

response 5528

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	27.00#
277.00	25.60	27.31
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035274.D
 Acq On : 23 Nov 2024 11:47
 Operator : RC/JU
 Sample : P4872-18
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

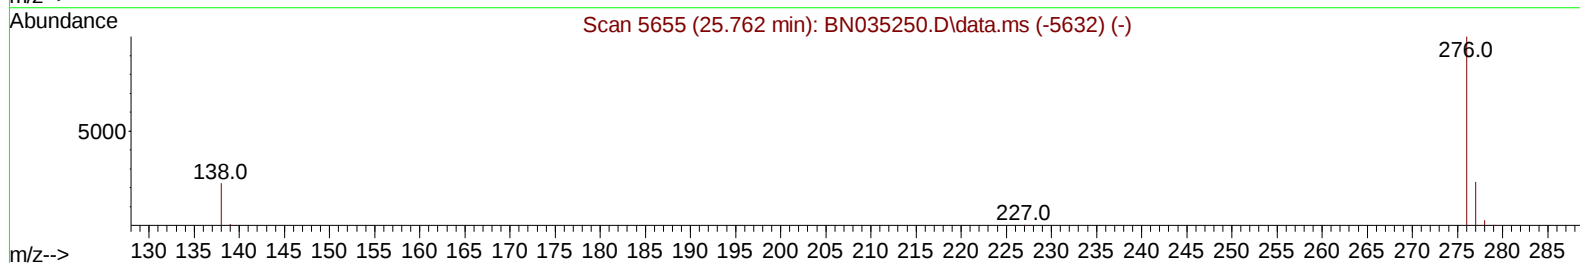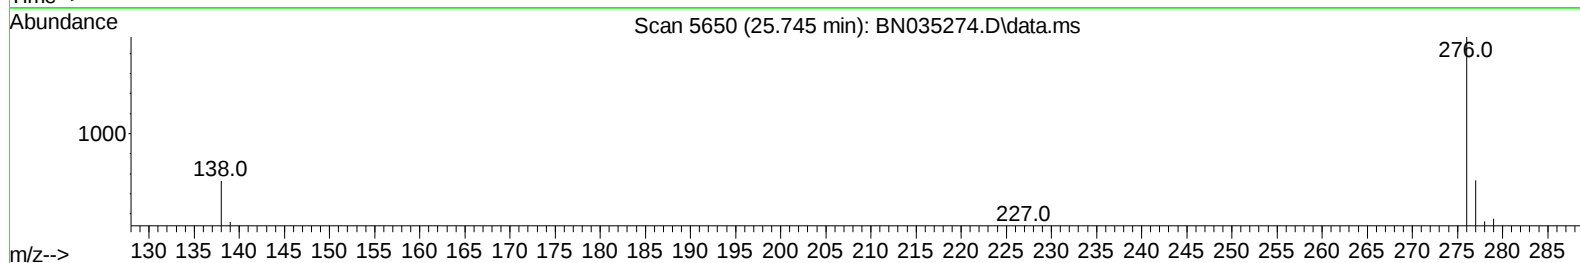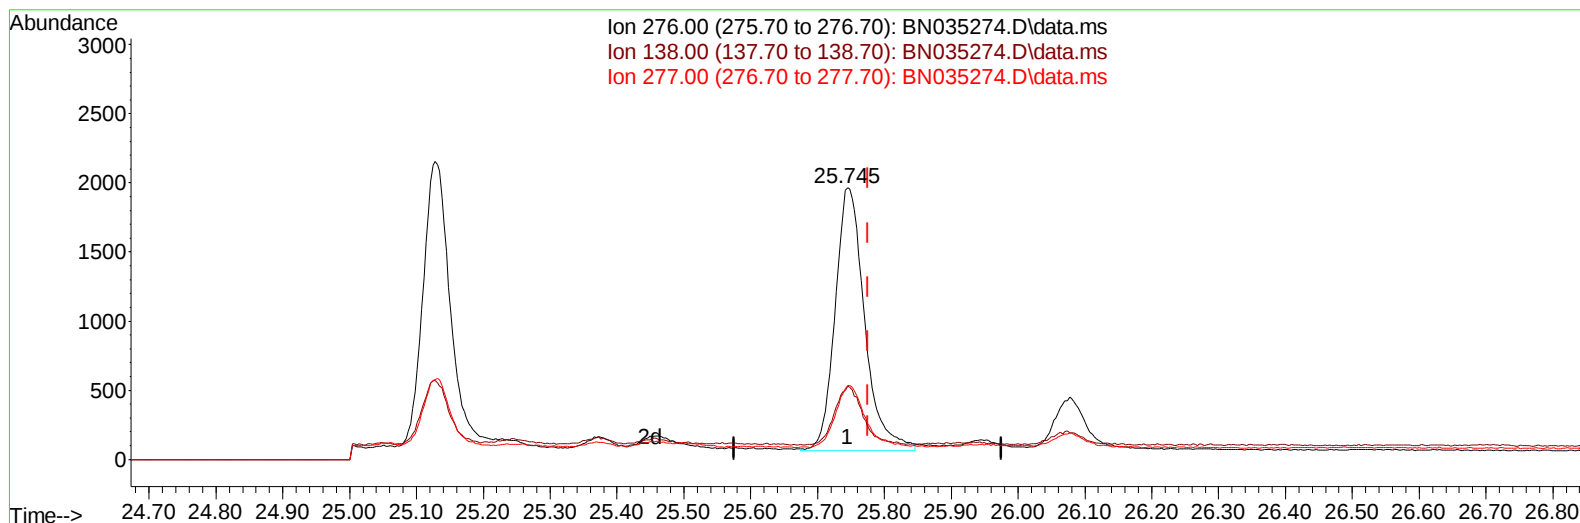

TIC: BN035274.D\data.ms

(29) Benzo(g,h,i)perylene

25.745min (-0.030) 0.21 ng/ul m

response 5843

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	16.30	27.00#
277.00	25.60	27.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035274.D
 Acq On : 23 Nov 2024 11:47
 Operator : RC/JU
 Sample : P4872-18
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E29Y5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 25 08:35:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.318	152		3024	0.400	ng/ul	0.00
4) Naphthalene-d8	10.064	136		8480	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	13.977	164		5426	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.743	188		12409	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.985	240		10907	0.400	ng/ul	# 0.00
23) Perylene-d12	23.083	264		8523m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.972	96		6859	2.482	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152		2477	0.199	ng/ul	0.00
18) Fluoranthene-d10	18.795	212		7645	0.254	ng/ul	0.00
Target Compounds							
							Qvalue
10) Acenaphthylene	13.690	152		3093	0.144	ng/ul	94
12) Fluorene	15.041	166		979	0.051	ng/ul#	95
15) Phenanthrene	16.785	178		15309	0.467	ng/ul	100
16) Anthracene	16.878	178		3379	0.111	ng/ul	94
19) Fluoranthene	18.823	202		32623	0.859	ng/ul#	93
20) Pyrene	19.190	202		27172m	0.688	ng/ul	
21) Benzo(a)anthracene	20.970	228		12589m	0.333	ng/ul	
22) Chrysene	21.020	228		12167	0.319	ng/ul	97
24) Benzo(b)fluoranthene	22.469	252		14966m	0.531	ng/ul	
25) Benzo(k)fluoranthene	22.507	252		5191m	0.179	ng/ul	
26) Benzo(a)pyrene	22.995	252		9697m	0.377	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.128	276		5894m	0.170	ng/ul	
28) Dibenzo(a,h)anthracene	25.145	278		1262m	0.046	ng/ul	
29) Benzo(g,h,i)perylene	25.745	276		5843m	0.213	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035274.D
Acq On : 23 Nov 2024 11:47
Operator : RC/JU
Sample : P4872-18
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E29Y5

Manual IntegrationsAPPROVED

Quant Time: Nov 25 08:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

