

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
 Data File : BN035245.D
 Acq On : 22 Nov 2024 17:10
 Operator : RC/JU
 Sample : P4875-22
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E2A24

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
 Supervised By :mohammad ahmed 11/27/2024

Quant Time: Nov 22 22:30:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 22 12:45:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.318	152	3192	0.400	ng/ul	0.00
4) Naphthalene-d8	10.069	136	8398	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.981	164	5462	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.747	188	11666m	0.400	ng/ul	0.00
17) Chrysene-d12	20.991	240	7362	0.400	ng/ul	# 0.00
23) Perylene-d12	23.092	264	6127m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.976	96	14599	5.004	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.670	152	3831	0.311	ng/ul	0.00
18) Fluoranthene-d10	18.800	212	10914	0.537	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.119	128	446	0.021	ng/ul#	68

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112224\
Data File : BN035245.D
Acq On : 22 Nov 2024 17:10
Operator : RC/JU
Sample : P4875-22
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E2A24

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024


Quant Time: Nov 22 22:30:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 22 12:45:23 2024
Response via : Initial Calibration

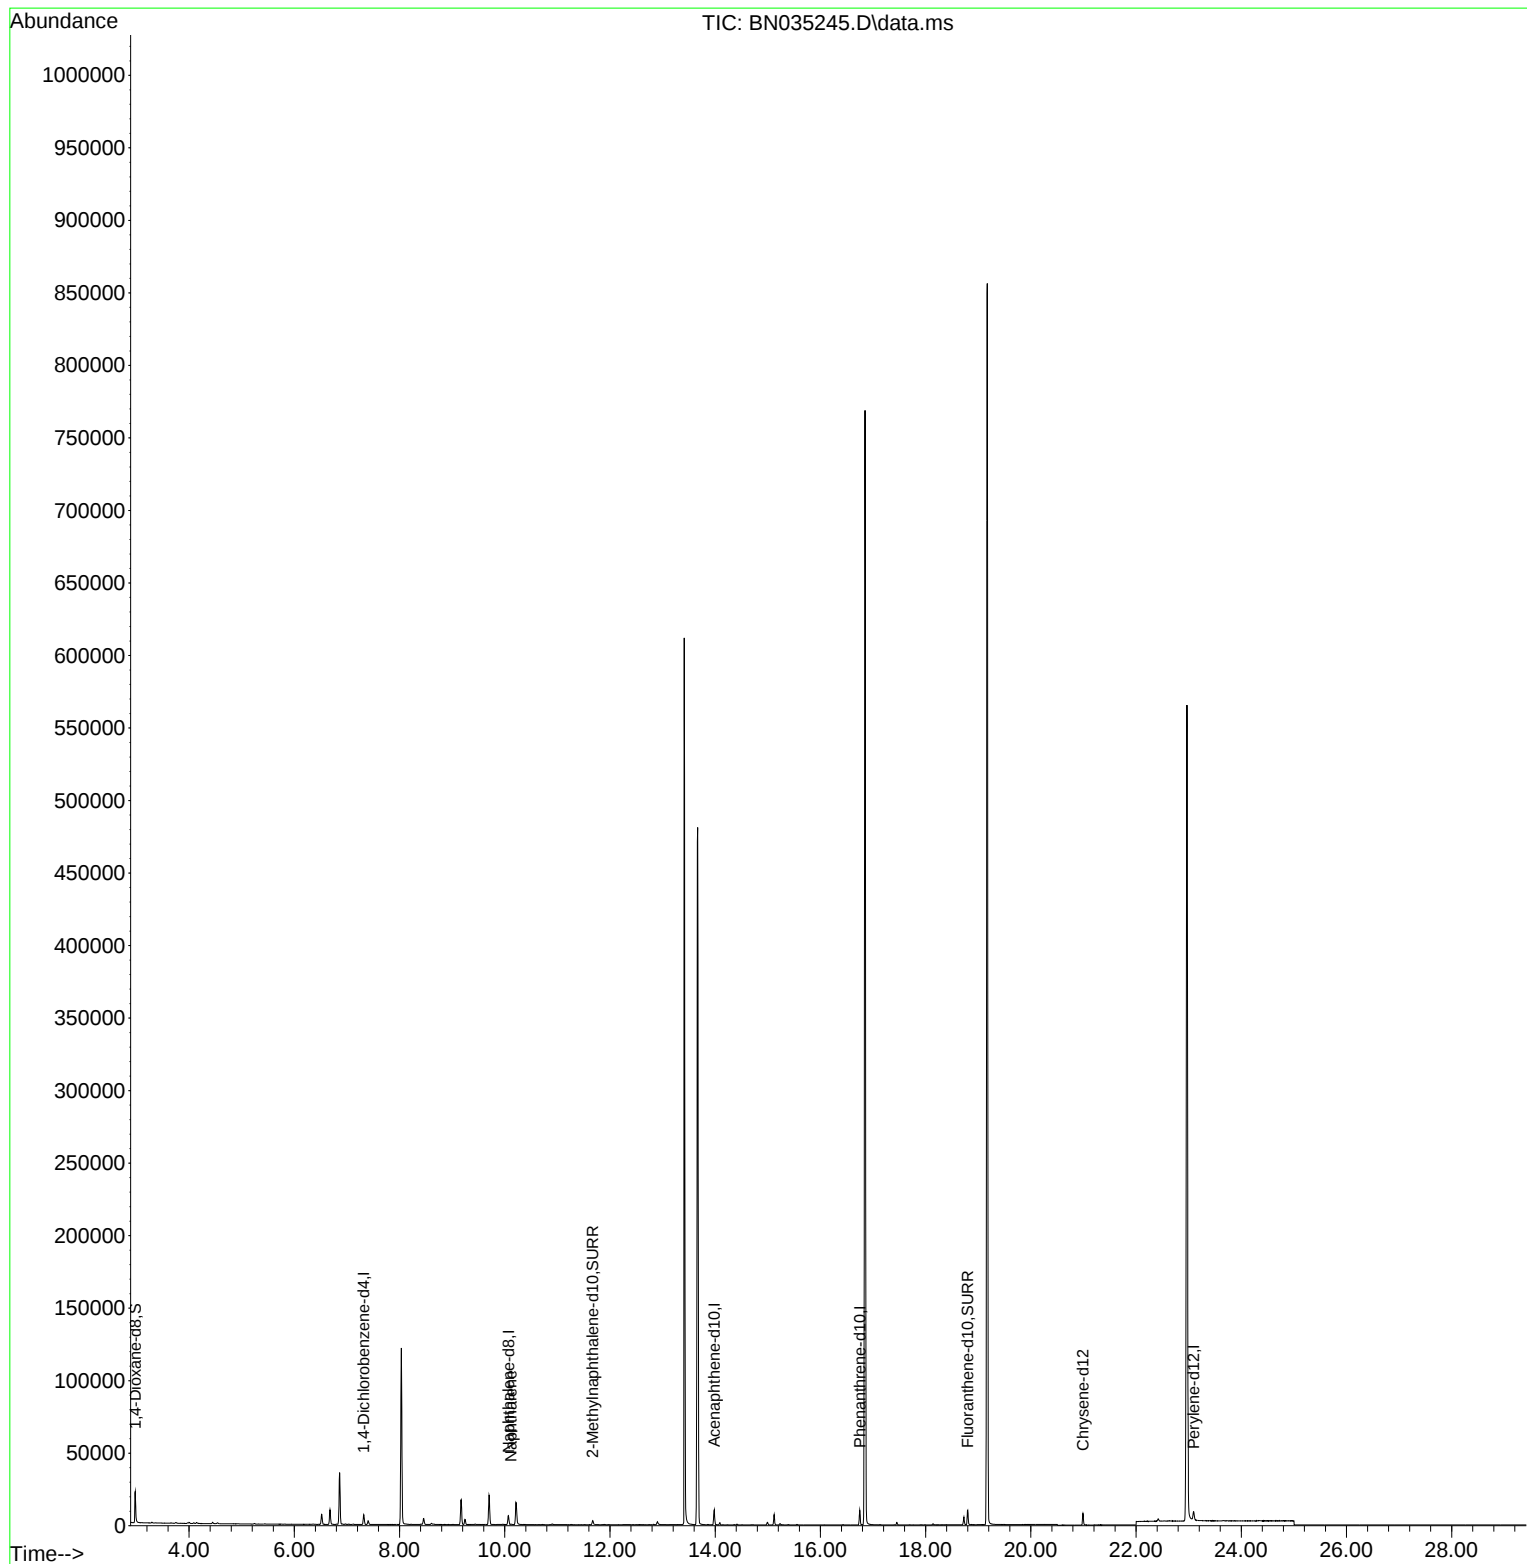

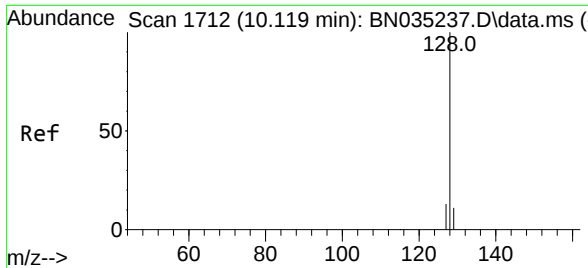

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.119 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN035245.D
Acq: 22 Nov 2024 17:10

Instrument :
BNA_N
ClientSampleId :
E2A24

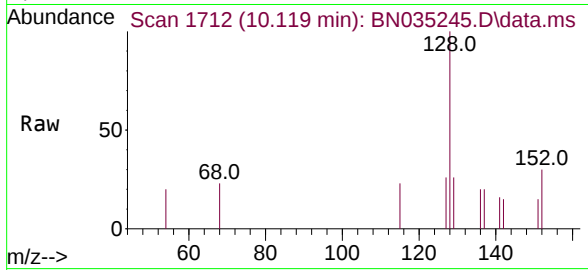

Tgt Ion:128 Resp: 440

Ion	Ratio	Lower	Upper
128	100		
129	26.3	9.9	14.9
127	26.0	11.4	17.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/26/2024
Supervised By :mohammad ahmed 11/27/2024

