
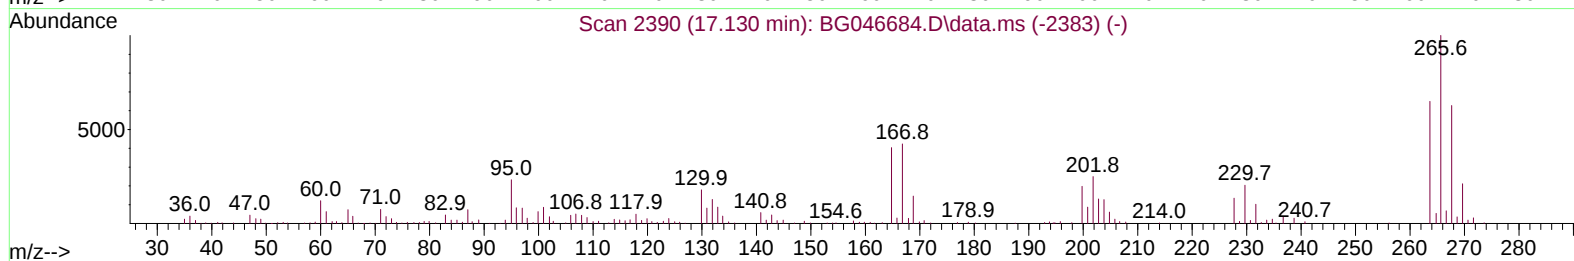
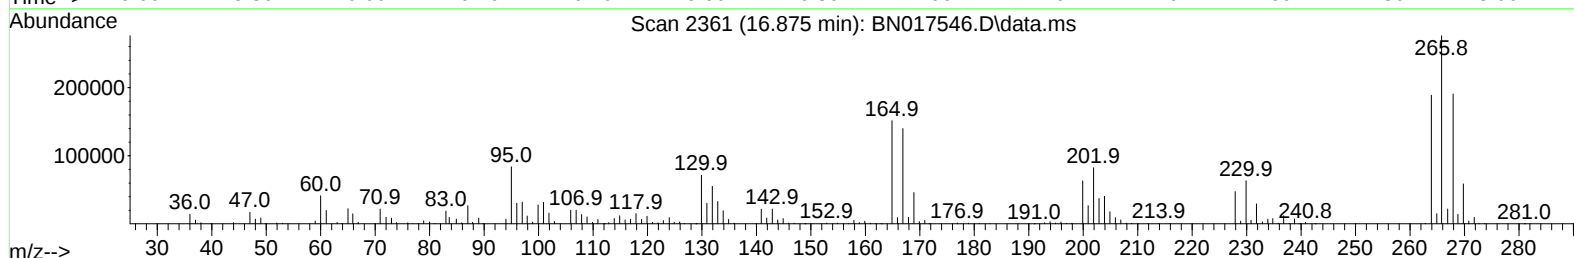


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112321\
Data File : BN017546.D
Acq On : 22 Nov 2021 15:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 03:11:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

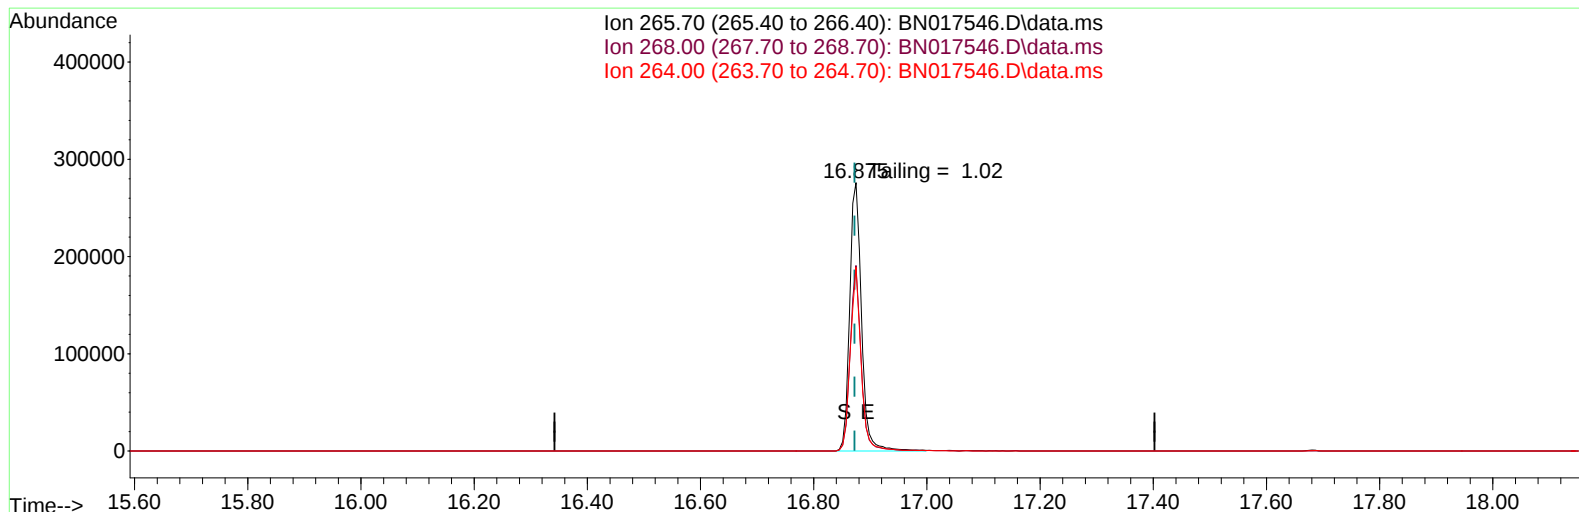

TIC: BN017546.D\data.ms

(70) Pentachlorophenol (C)




16.875min (+ 0.003) 16036.96 ng

response 400971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.09
264.00	61.60	68.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112321\
Data File : BN017546.D
Acq On : 22 Nov 2021 15:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 03:11:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

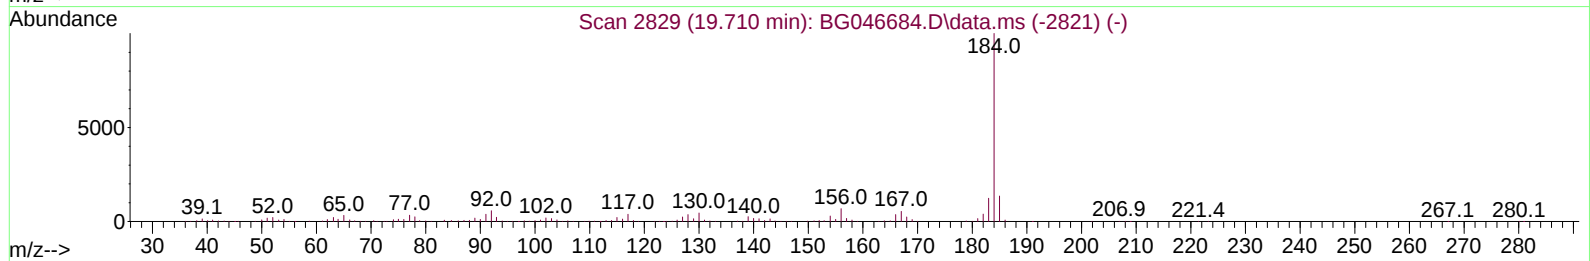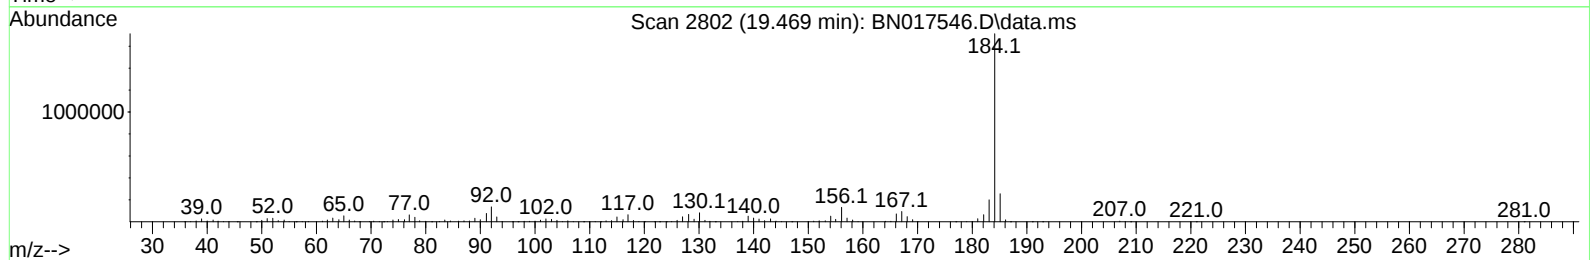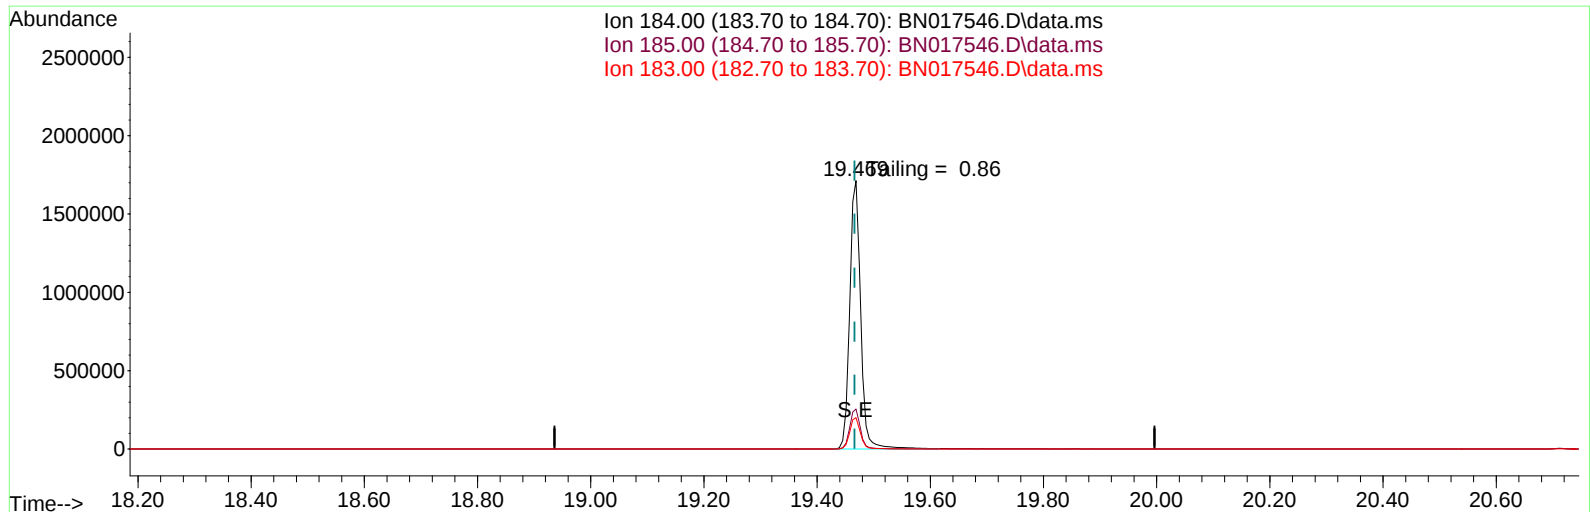

TIC: BN017546.D\data.ms

(77) Benzidine**19.469min (+ 0.003) 0.00 ng****response 2308249**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.94
183.00	13.20	11.69
0.00	0.00	0.00