
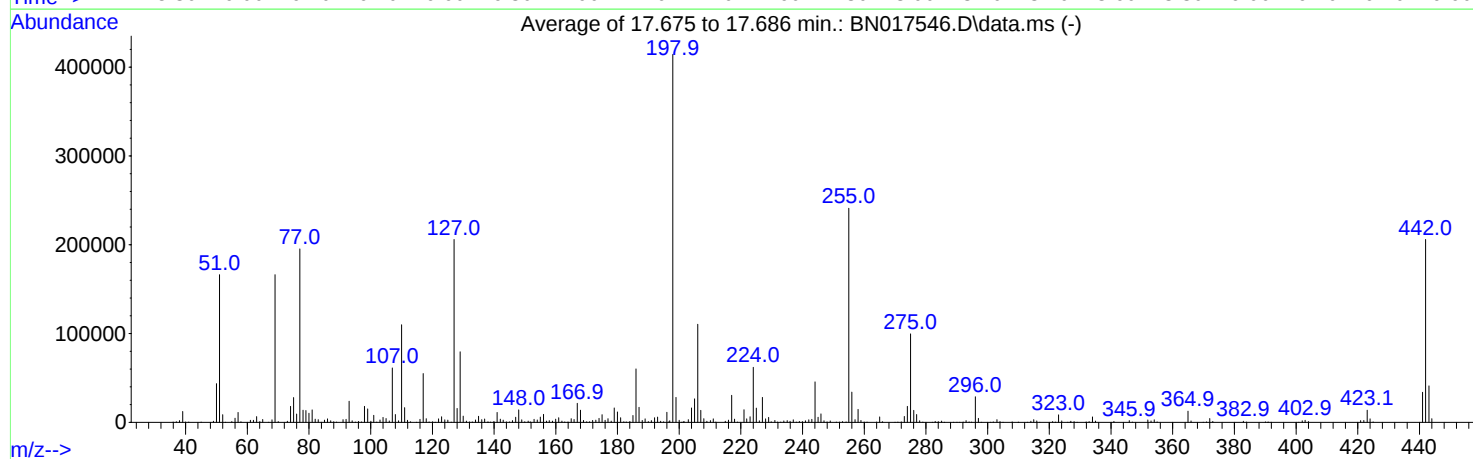


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112321\
 Data File : BN017546.D
 Acq On : 22 Nov 2021 15:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN111921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 19 14:57:14 2021

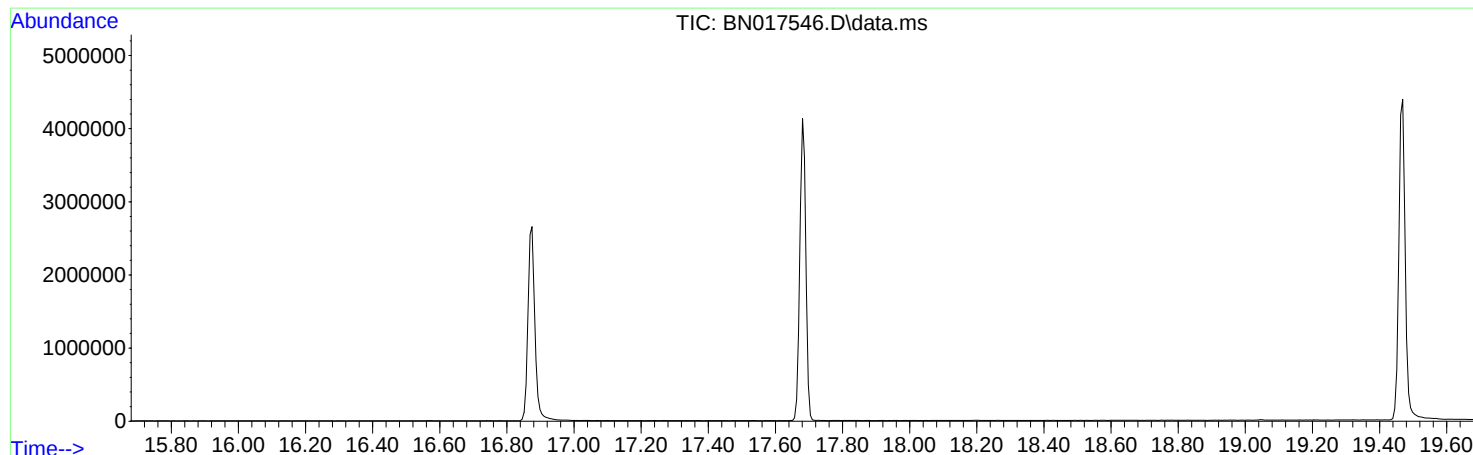




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	166379	PASS
68	69	0.00	2	1.7	2849	PASS
69	198	0.00	100	40.2	166315	PASS
70	69	0.00	2	0.5	887	PASS
127	198	10	80	49.7	206016	PASS
197	198	0.00	2	0.4	1785	PASS
198	198	100	100	100.0	414229	PASS
199	198	5	9	6.8	28120	PASS
275	198	10	60	24.1	99715	PASS
365	198	1	100	3.0	12584	PASS
441	198	0.01	100	8.2	33859	PASS
442	442	50	100	100.0	205963	PASS
443	442	15	24	20.0	41101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112321\
 Data File : BN017546.D
 Acq On : 22 Nov 2021 15:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 23 03:11:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 19 11:42:56 2021
 Response via : Initial Calibration

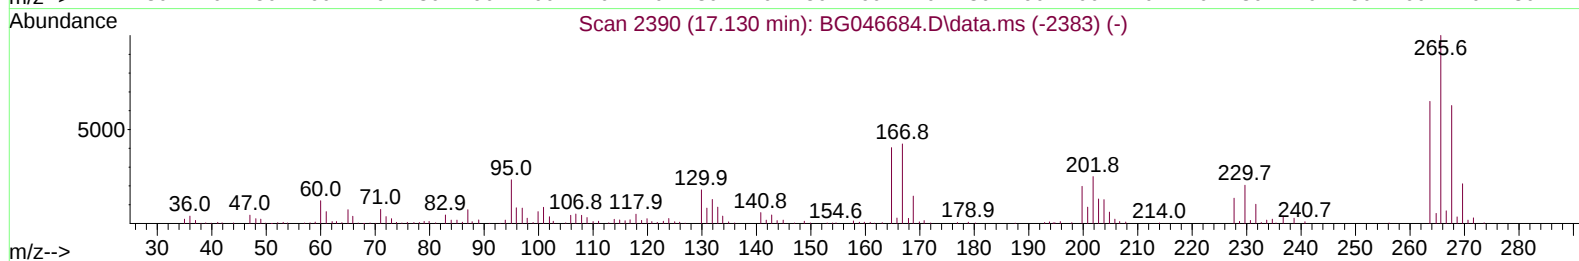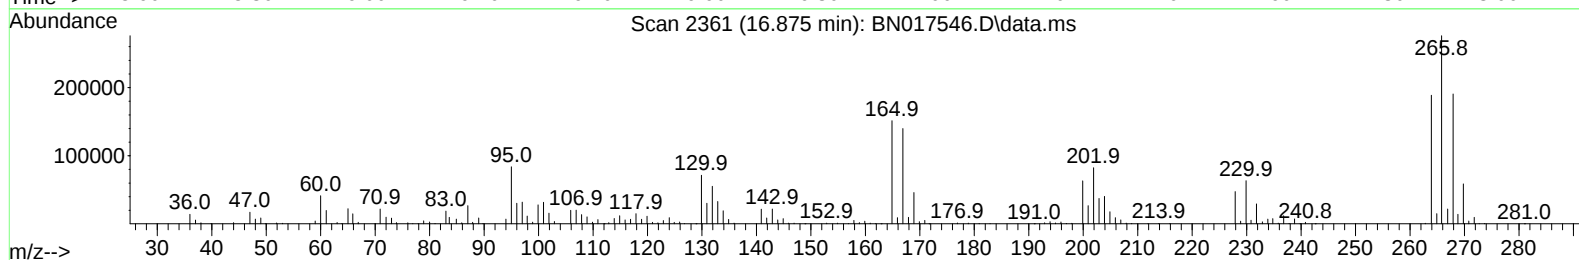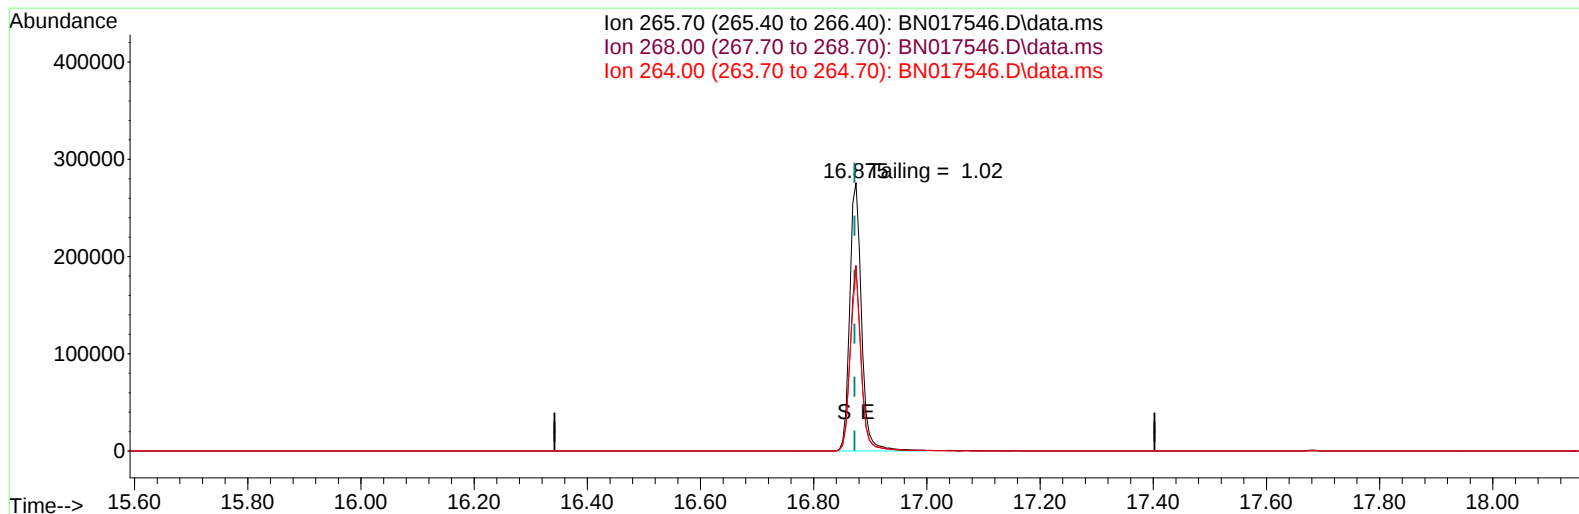

TIC: BN017546.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.003) 16036.96 ng




response 400971

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.09
264.00	61.60	68.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112321\
Data File : BN017546.D
Acq On : 22 Nov 2021 15:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 23 03:11:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 19 11:42:56 2021
Response via : Initial Calibration

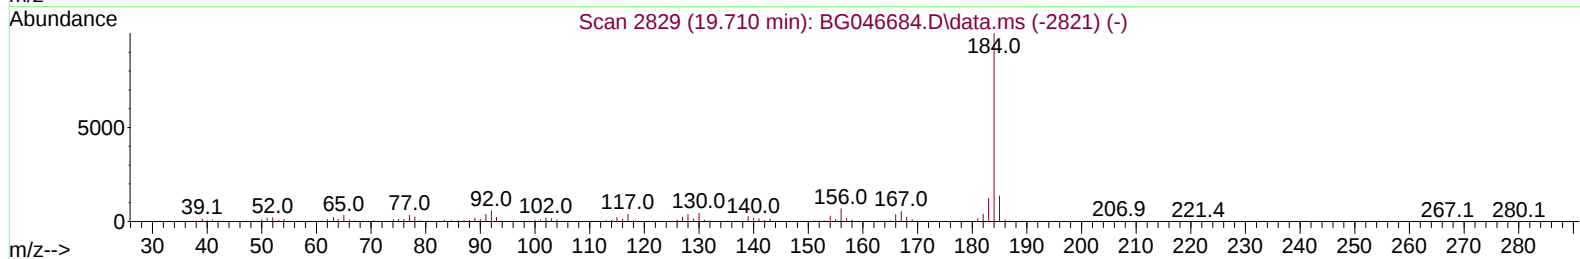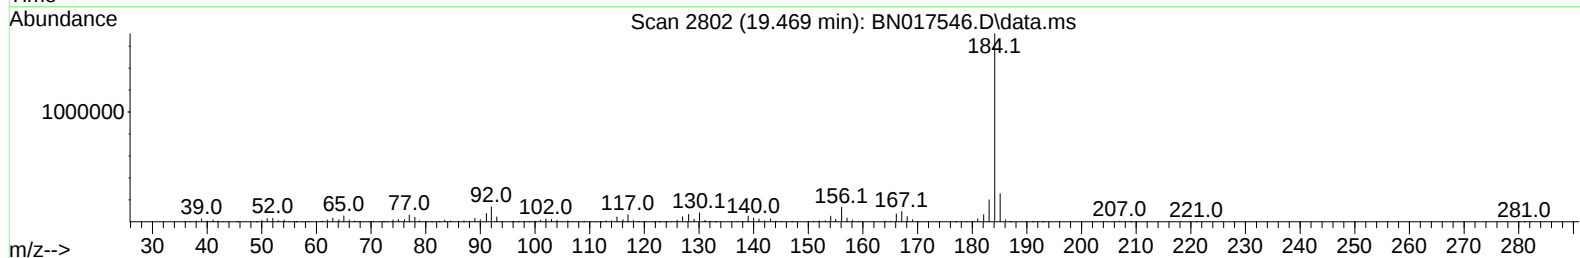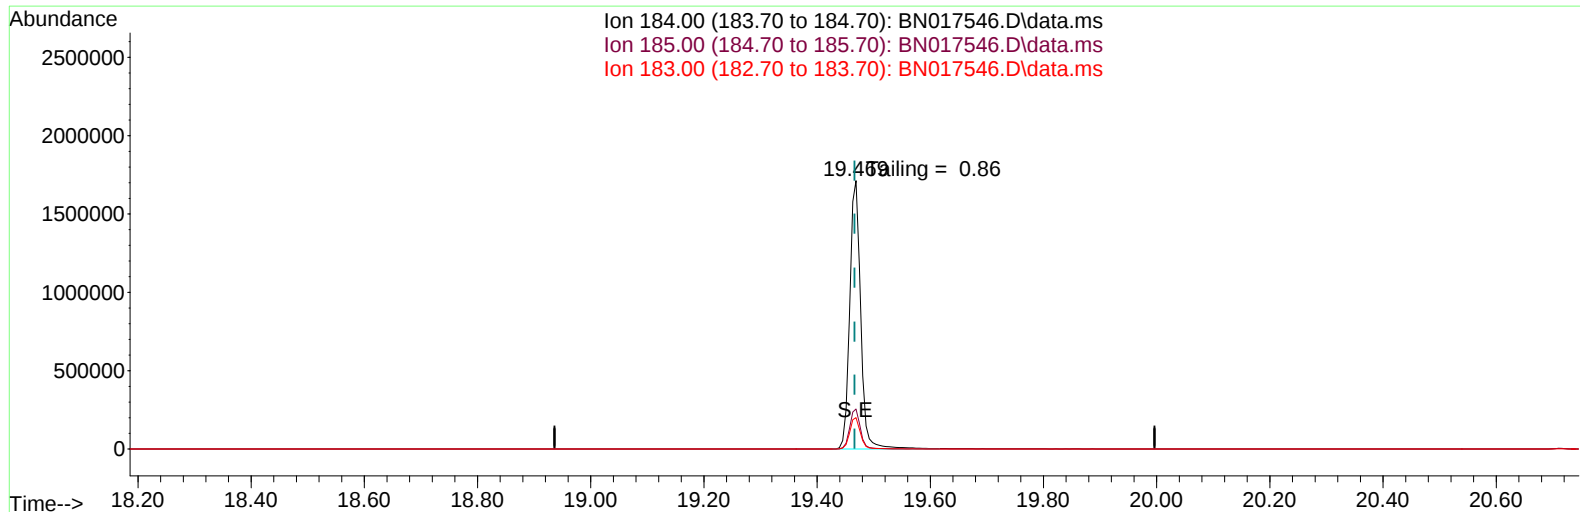

TIC: BN017546.D\data.ms

(77) Benzidine

19.469min (+ 0.003) 0.00 ng

response 2308249

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.94
183.00	13.20	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2021	BNA_N	<u>BN017546.D</u>
Compound Name	Response	Retention Time
DDT	1167527	20.716
DDD	12562	20.264
DDE	565	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13127	1180654	1.11

Instrument :
BNA_N
ClientSampleId :
DFTPP