
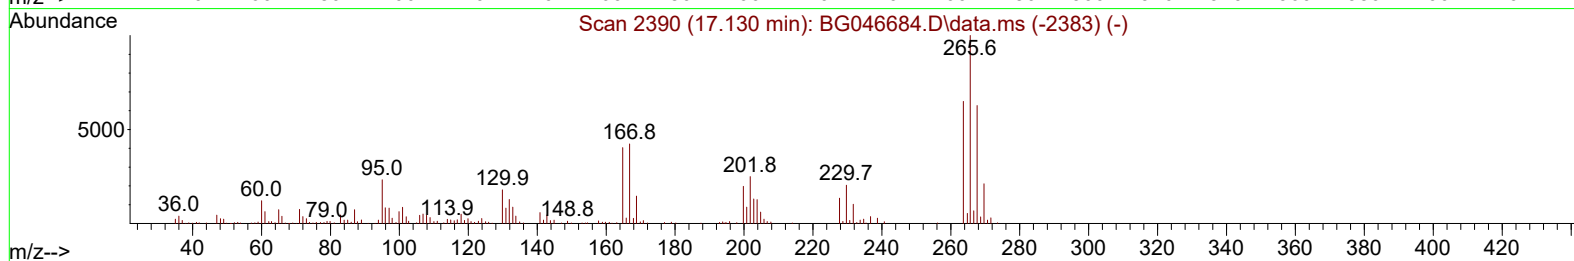
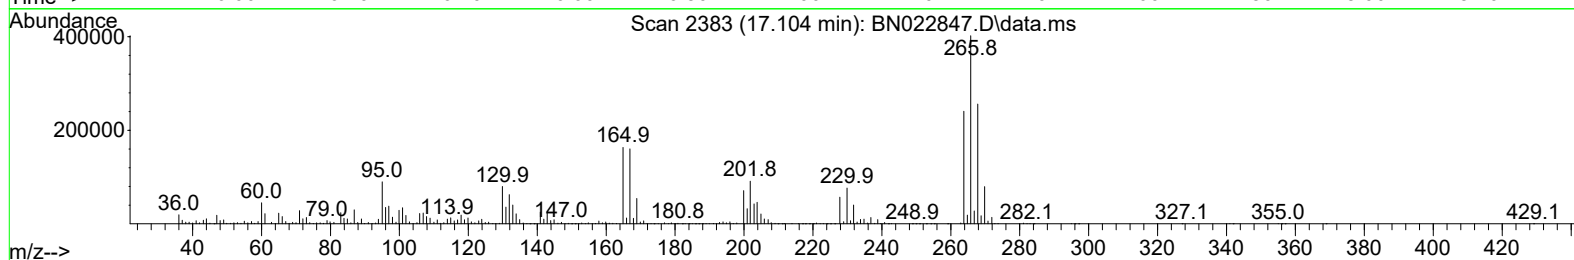


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112322\
Data File : BN022847.D
Acq On : 23 Nov 2022 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 05:39:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

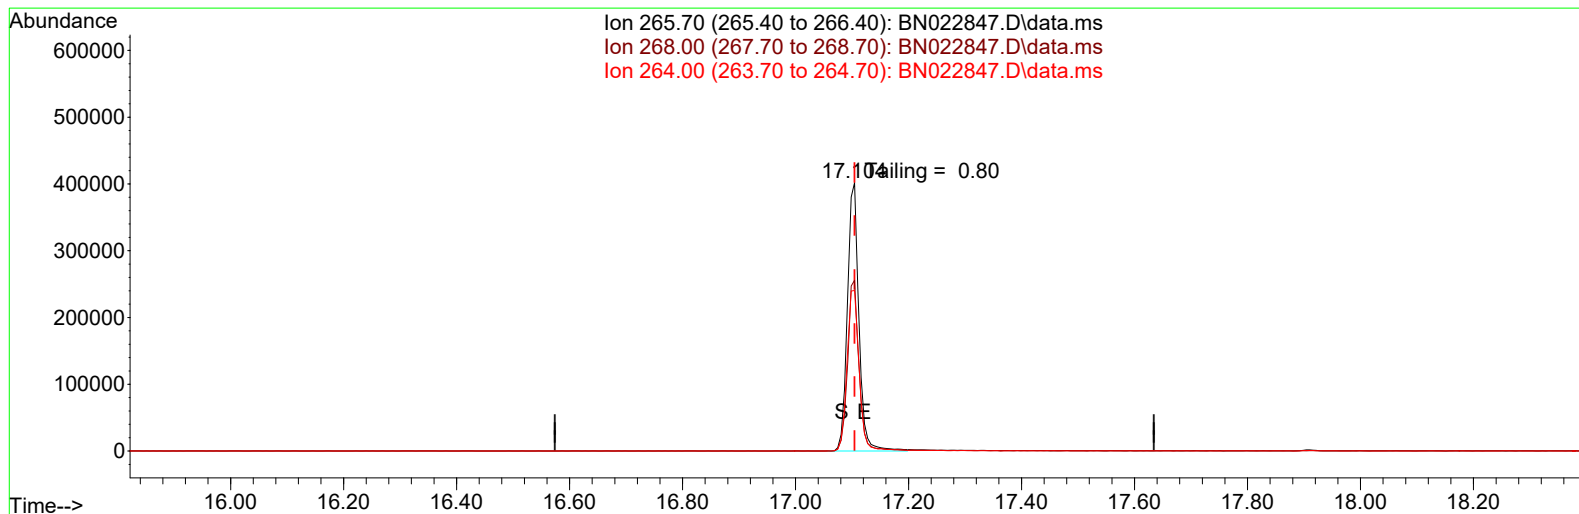

TIC: BN022847.D\data.ms

(70) Pentachlorophenol (C)




17.104min (0.000) 164760.92 ng

response 575386

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.64
264.00	61.60	59.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112322\
Data File : BN022847.D
Acq On : 23 Nov 2022 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 05:39:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

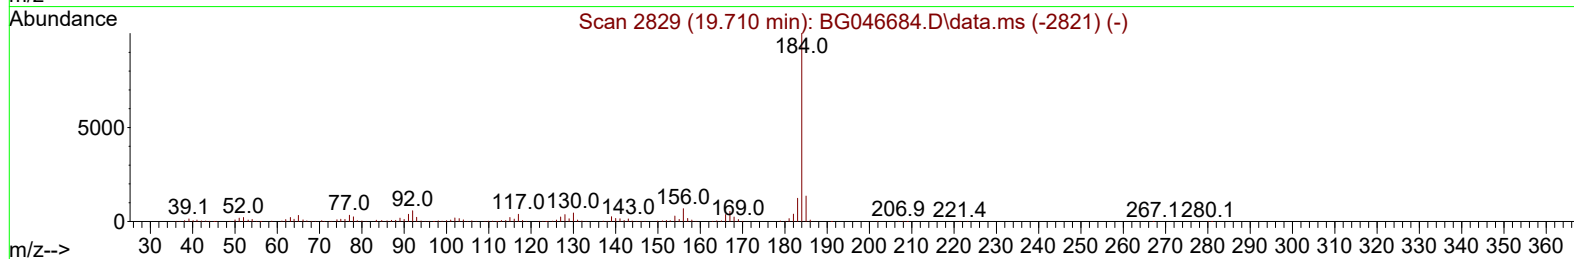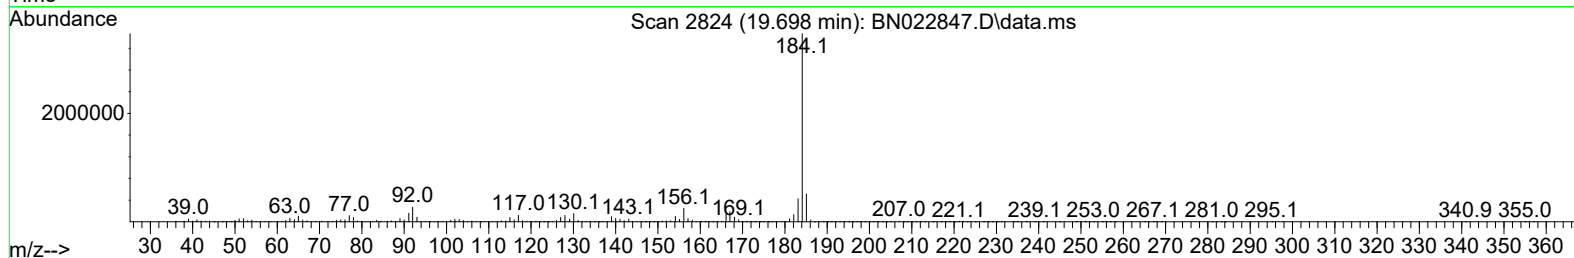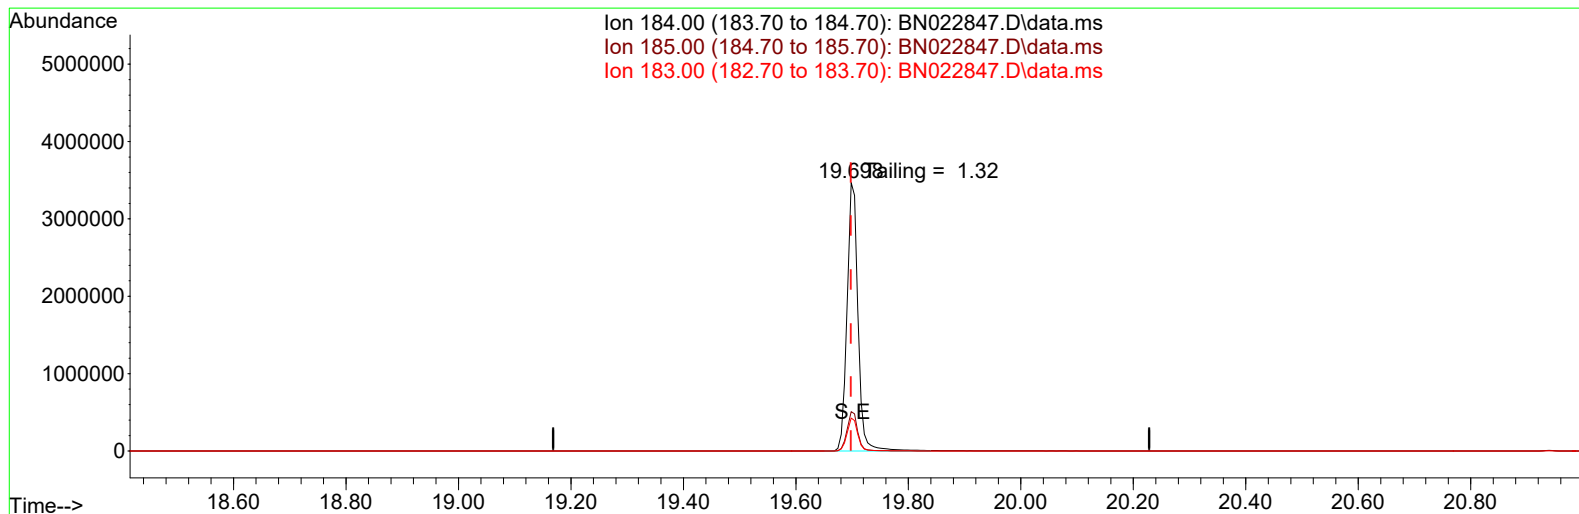

TIC: BN022847.D\data.ms

(77) Benzidine**19.698min (0.000) 666234.08 ng****response 4723490**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	13.20	12.27
0.00	0.00	0.00