


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112322\
 Data File : BN022847.D
 Acq On : 23 Nov 2022 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 24 03:45:05 2022

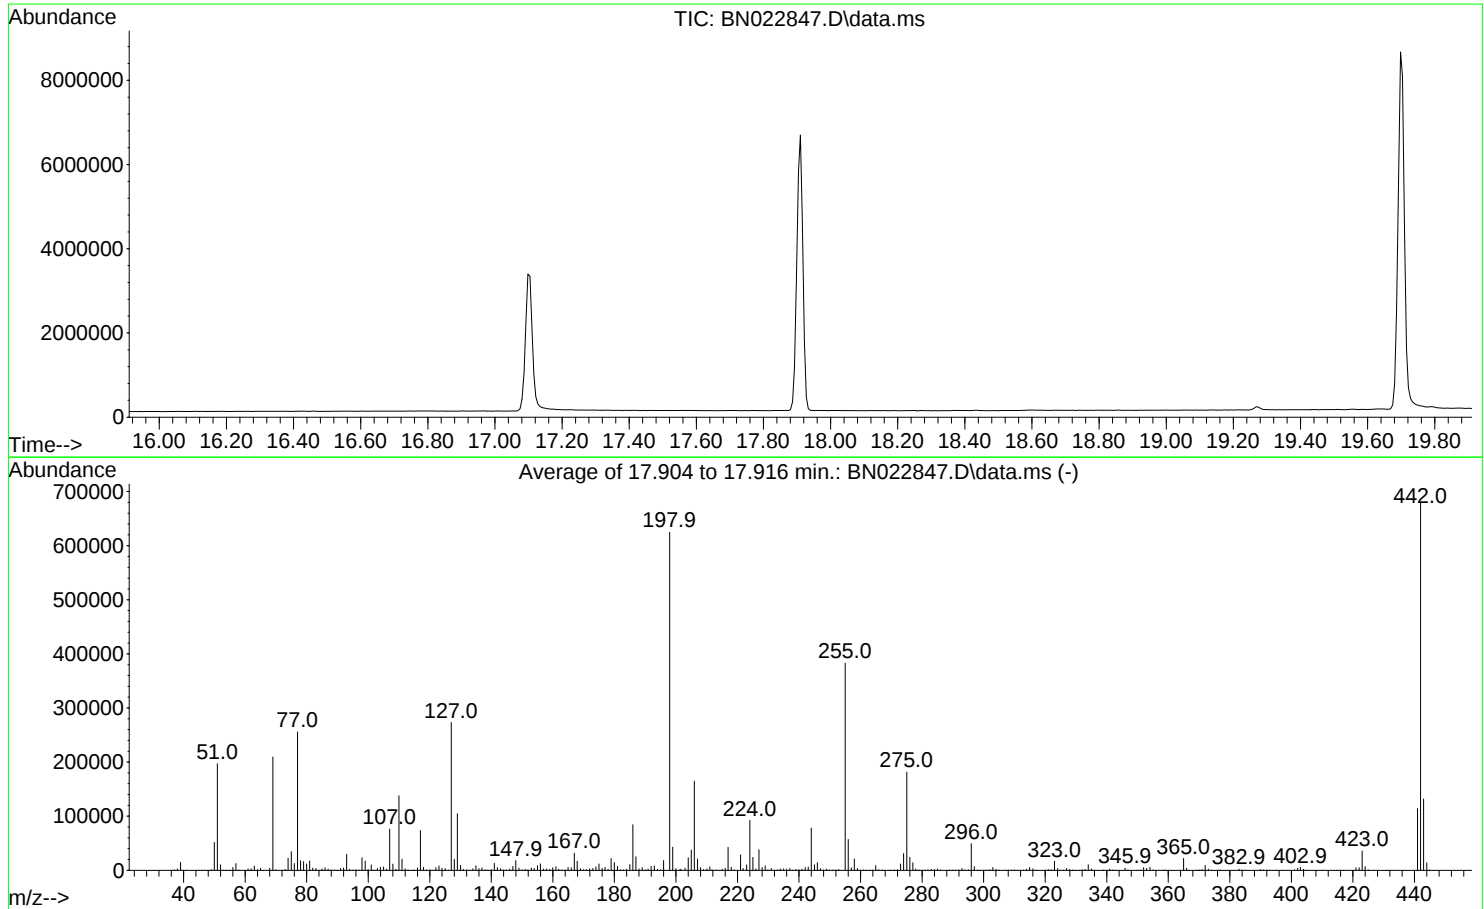




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	196883	PASS
68	69	0.00	2	1.7	3633	PASS
69	198	0.00	100	33.5	209589	PASS
70	69	0.00	2	0.5	1054	PASS
127	198	10	80	43.7	273213	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	624788	PASS
199	198	5	9	6.8	42654	PASS
275	198	10	60	29.0	181419	PASS
365	198	1	100	3.5	22101	PASS
441	198	0.01	100	18.3	114165	PASS
442	442	50	100	100.0	679893	PASS
443	442	15	24	19.4	131637	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112322\
 Data File : BN022847.D
 Acq On : 23 Nov 2022 15:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 24 05:39:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 05:39:37 2022
 Response via : Initial Calibration

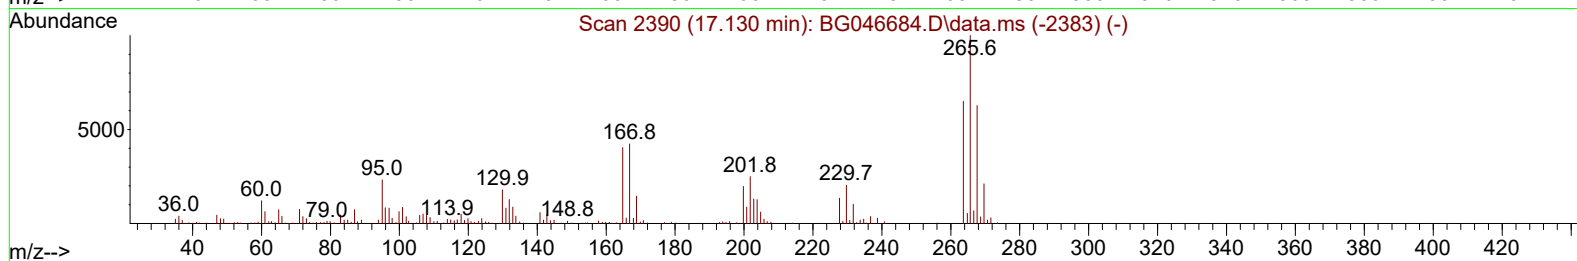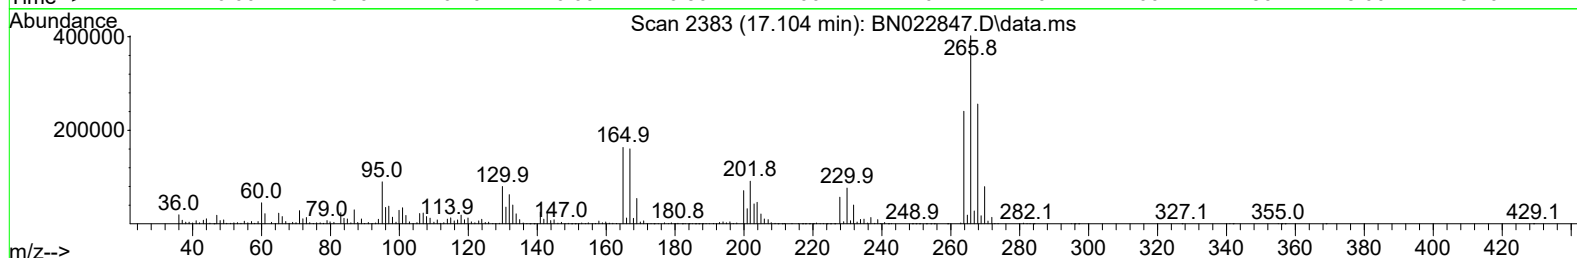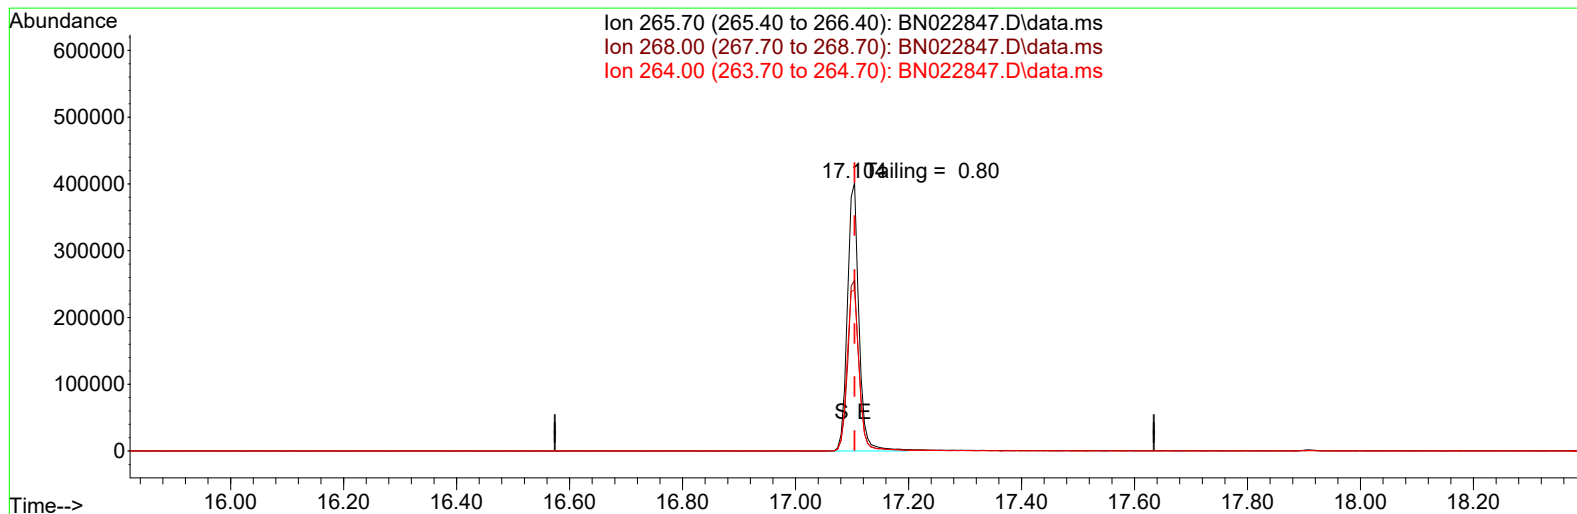

TIC: BN022847.D\data.ms

(70) Pentachlorophenol (C)

17.104min (0.000) 164760.92 ng




response 575386

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.64
264.00	61.60	59.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112322\
Data File : BN022847.D
Acq On : 23 Nov 2022 15:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 24 05:39:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

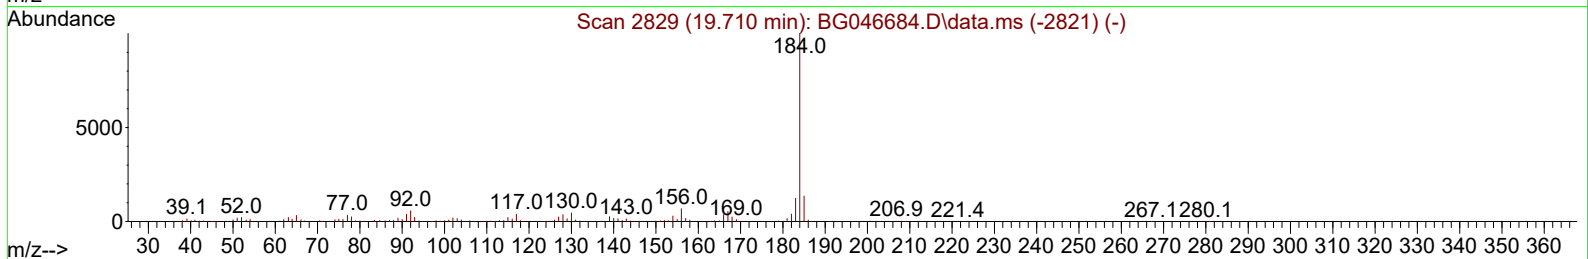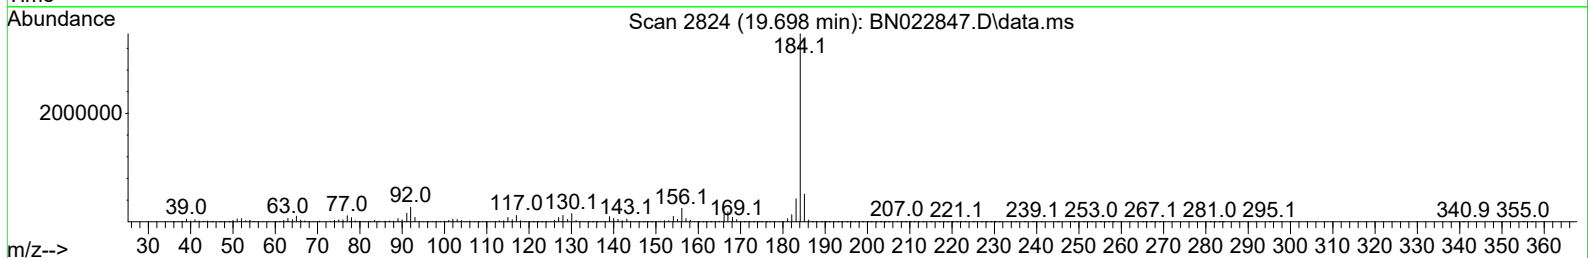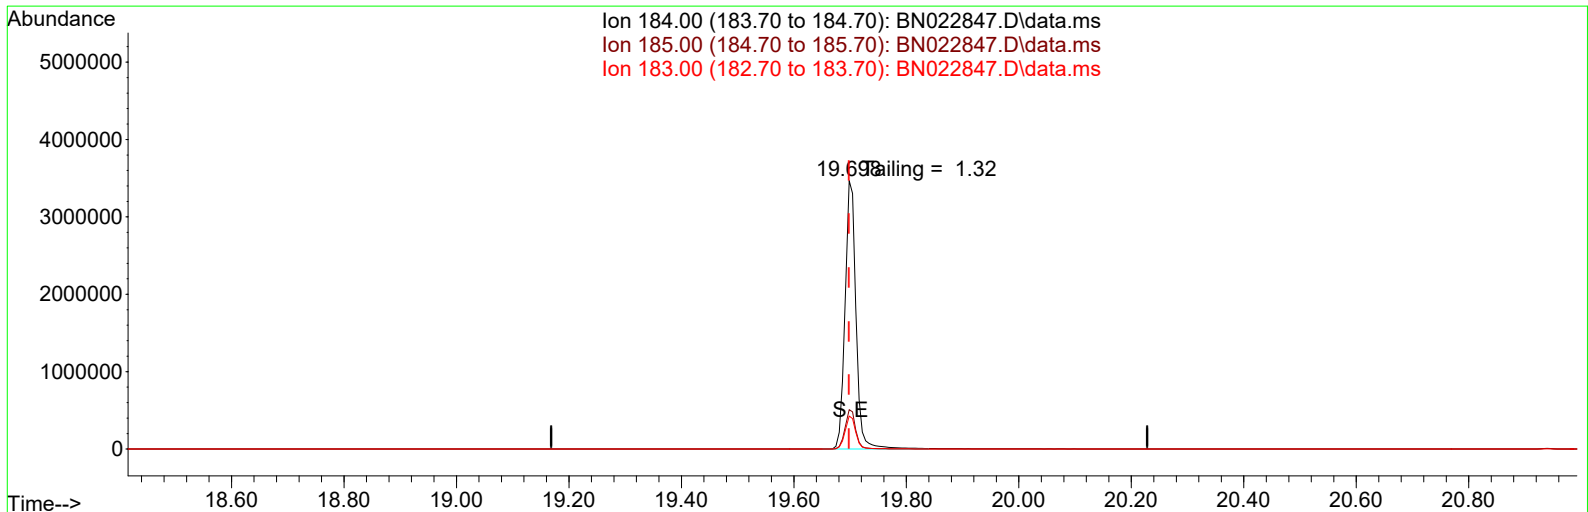

TIC: BN022847.D\data.ms

(77) Benzidine

19.698min (0.000) 666234.08 ng

response 4723490

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	13.20	12.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/23/2022	BNA_N	<u>BN022847.D</u>
Compound Name	Response	Retention Time
DDT	1858685	20.939
DDD	16679	20.551
DDE	121	19.992
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16800	1875485	0.90

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP