
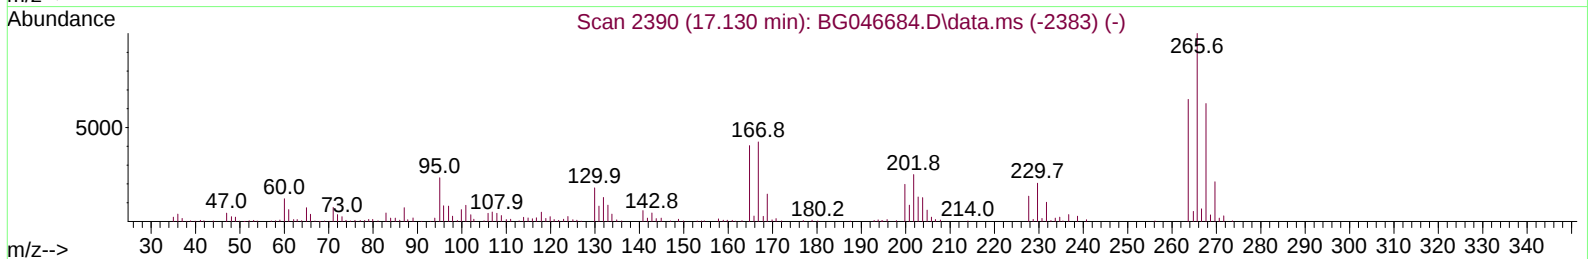
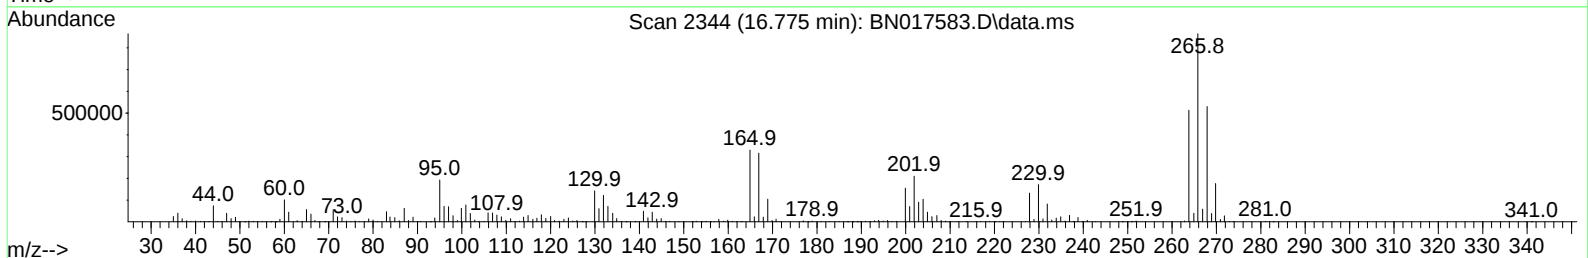


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112521\
Data File : BN017583.D
Acq On : 24 Nov 2021 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 08:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 08:22:06 2021
Response via : Initial Calibration

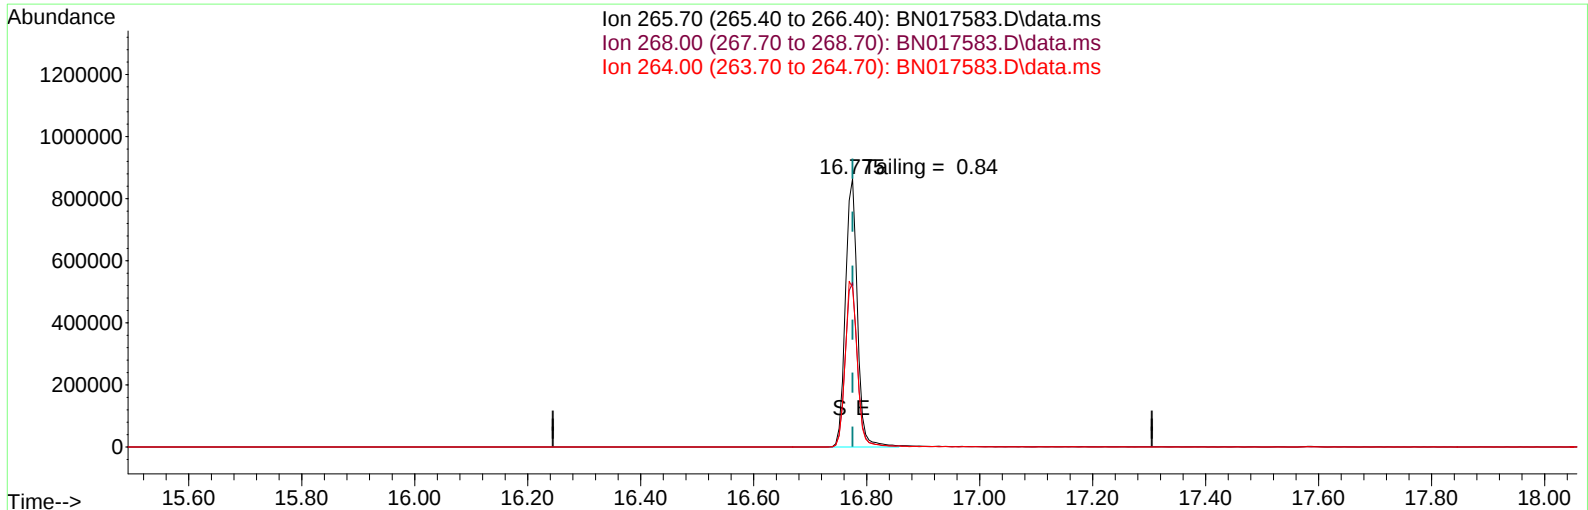

TIC: BN017583.D\data.ms

(70) Pentachlorophenol (C)




16.775min (0.000) 28331.64 ng

response 1283344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.26
264.00	61.60	59.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112521\
Data File : BN017583.D
Acq On : 24 Nov 2021 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 08:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 08:22:06 2021
Response via : Initial Calibration

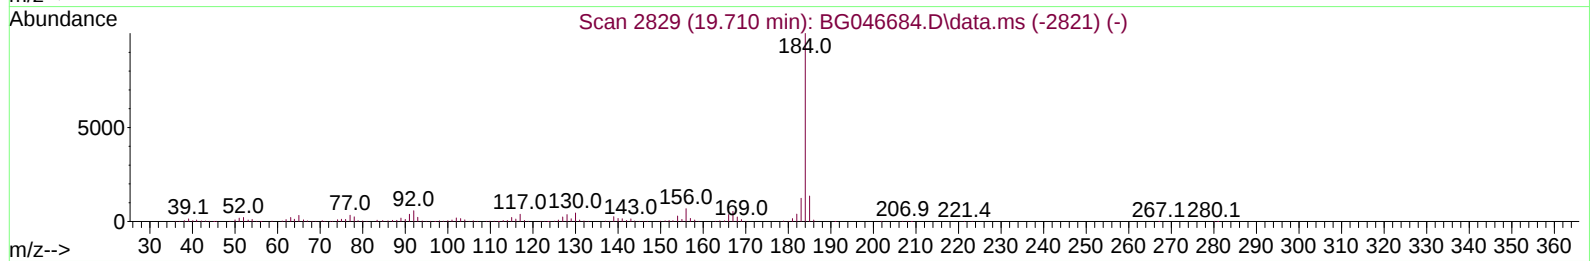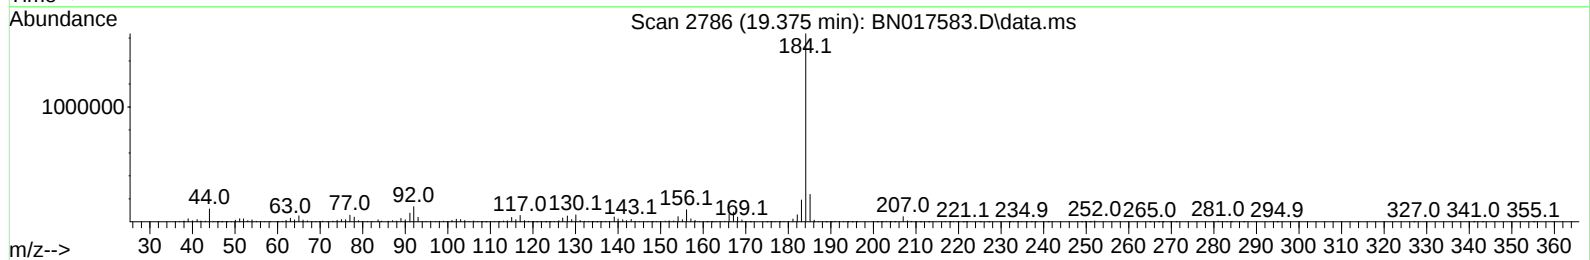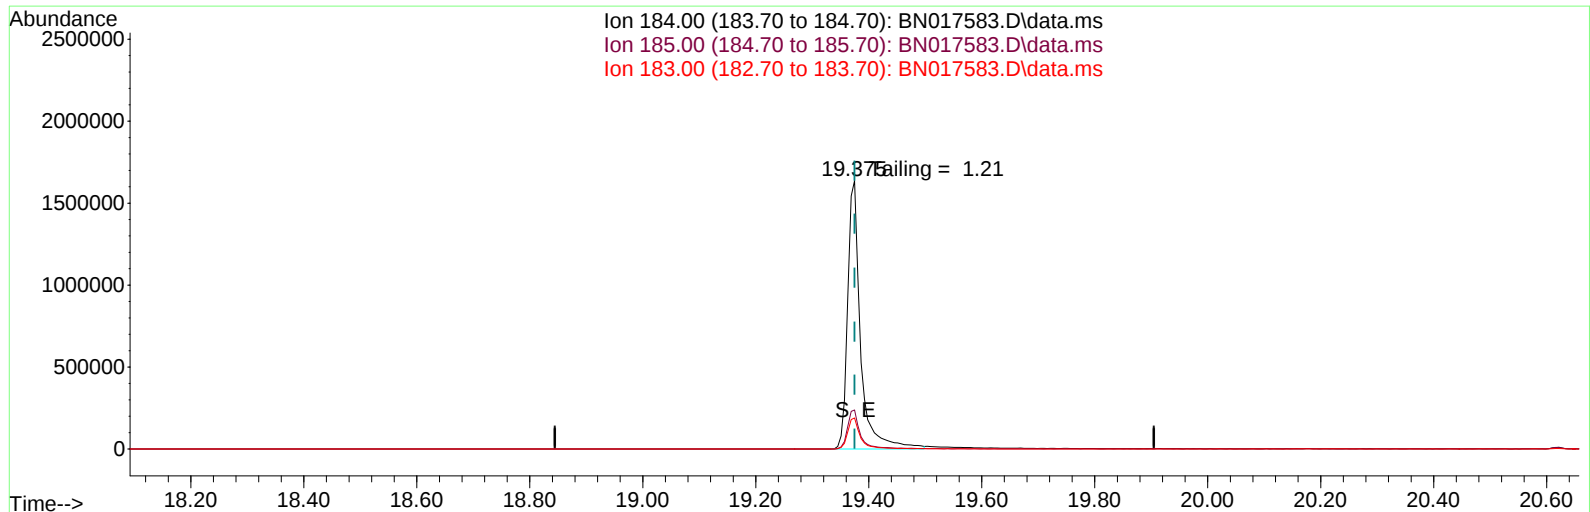

TIC: BN017583.D\data.ms

(77) Benzidine**19.375min (0.000) 57389.52 ng****response 2681885**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.60
0.00	0.00	0.00