
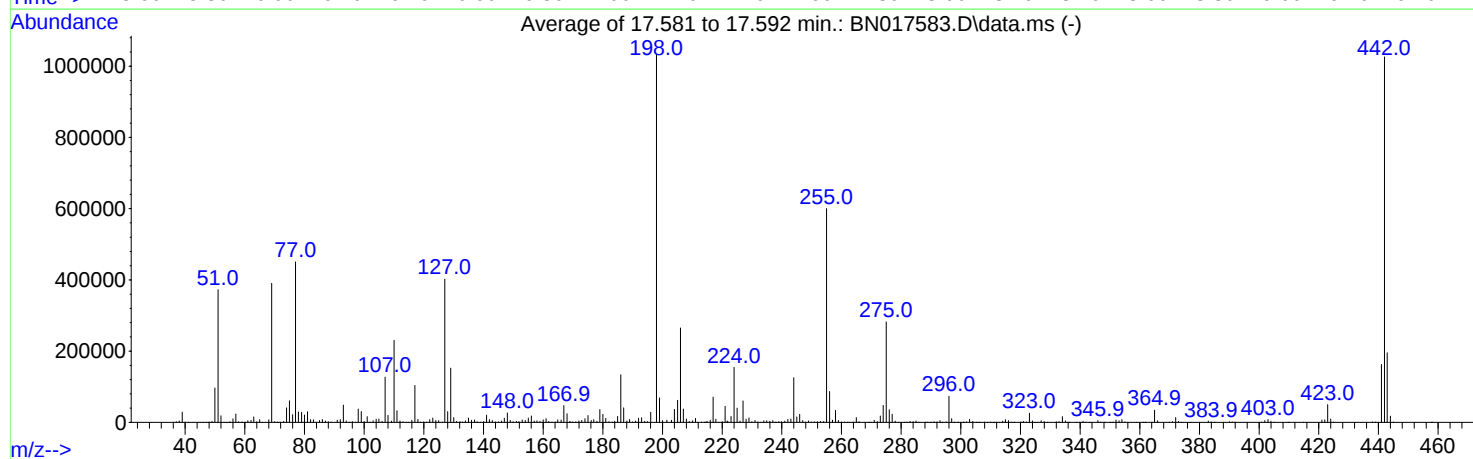


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112521\
 Data File : BN017583.D
 Acq On : 24 Nov 2021 16:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 25 03:24:52 2021

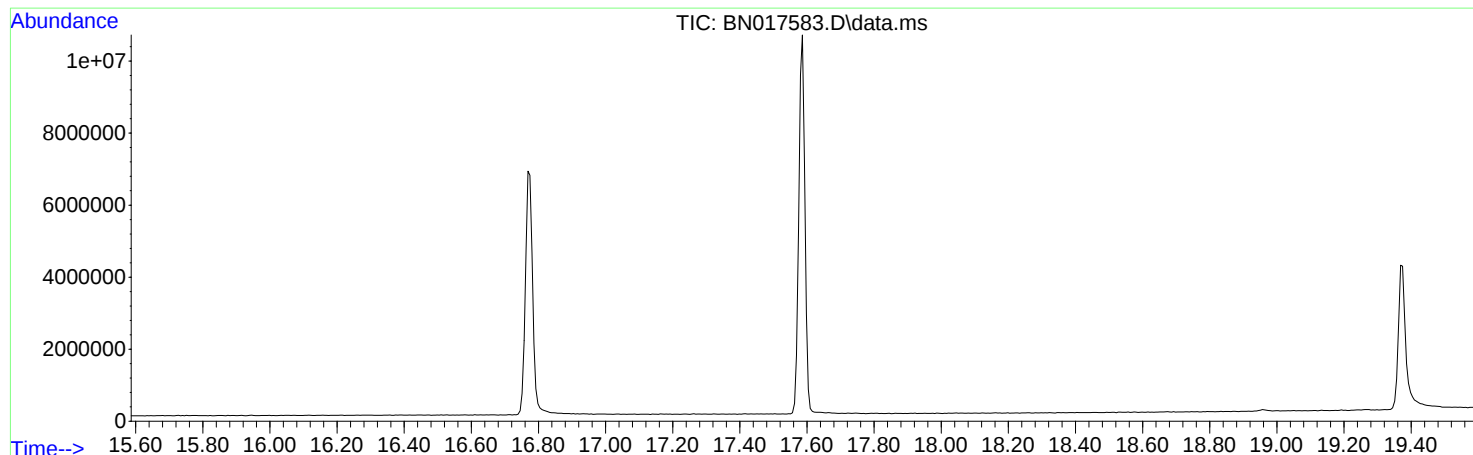




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	372614	PASS
68	69	0.00	2	1.8	7088	PASS
69	198	0.00	100	37.8	390222	PASS
70	69	0.00	2	0.6	2371	PASS
127	198	10	80	38.9	401920	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1032896	PASS
199	198	5	9	6.6	68587	PASS
275	198	10	60	27.3	281963	PASS
365	198	1	100	3.3	34219	PASS
441	198	0.01	100	15.7	162453	PASS
442	442	50	100	100.0	1025984	PASS
443	442	15	24	19.0	195413	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112521\
Data File : BN017583.D
Acq On : 24 Nov 2021 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 25 08:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 08:22:06 2021
Response via : Initial Calibration

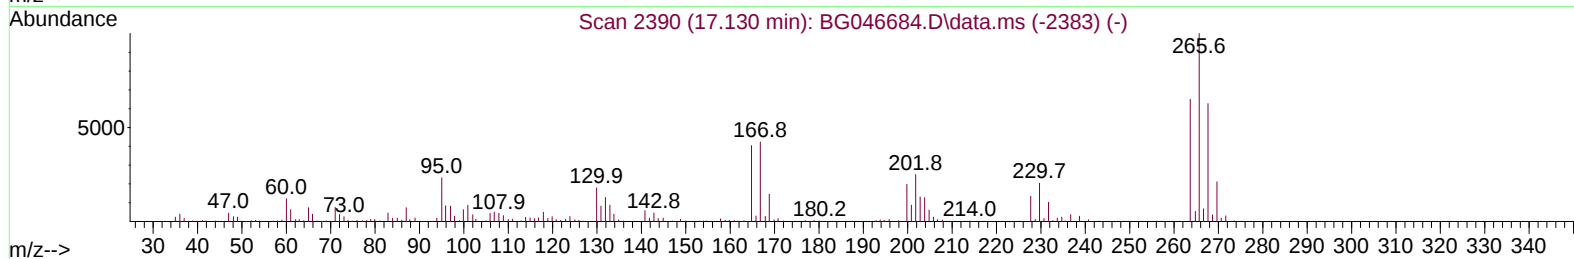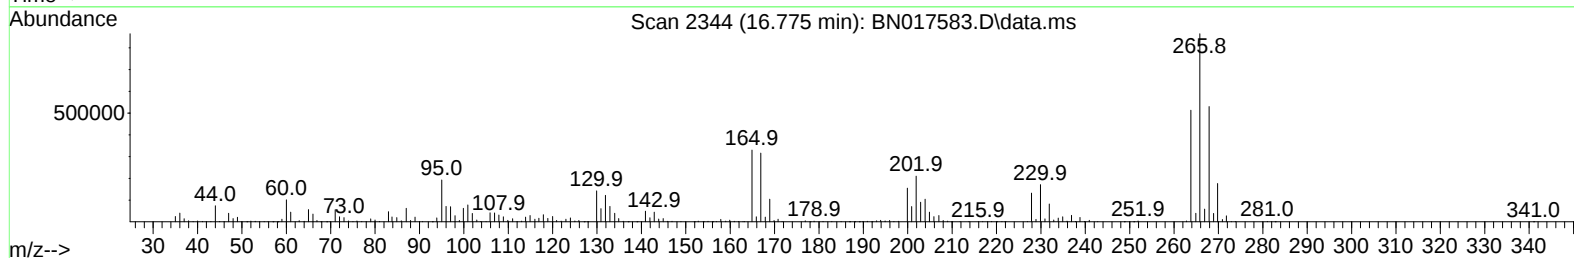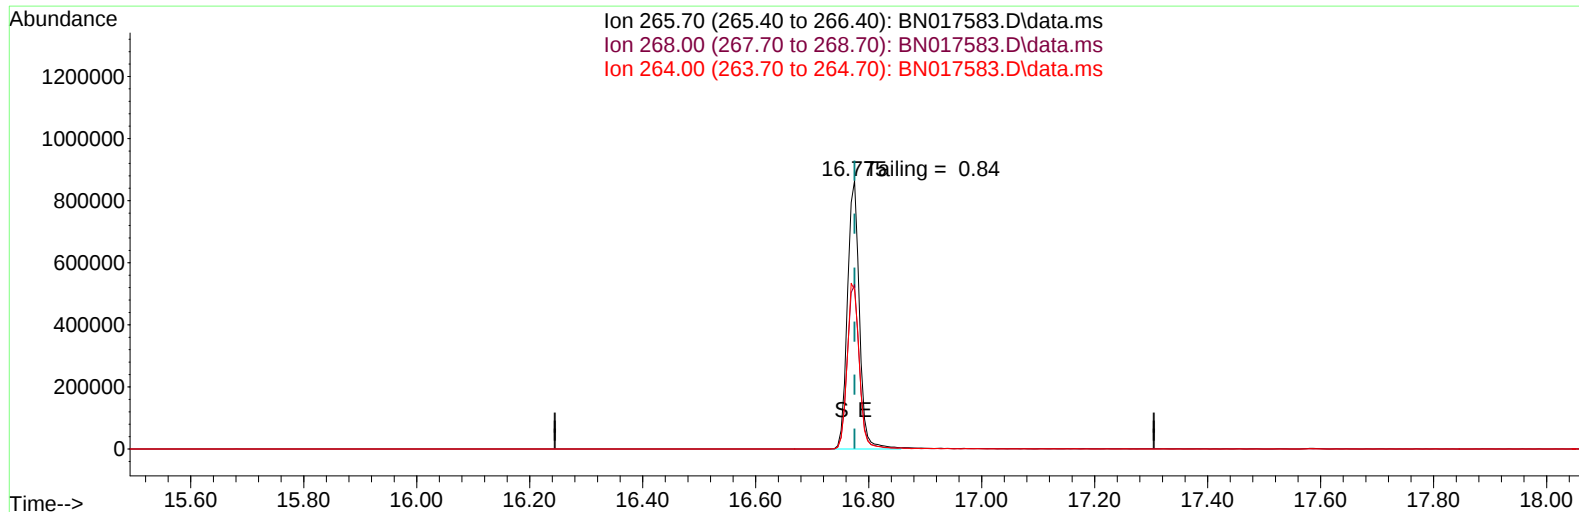

TIC: BN017583.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 28331.64 ng




response 1283344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.26
264.00	61.60	59.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112521\
Data File : BN017583.D
Acq On : 24 Nov 2021 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 25 08:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 25 08:22:06 2021
Response via : Initial Calibration

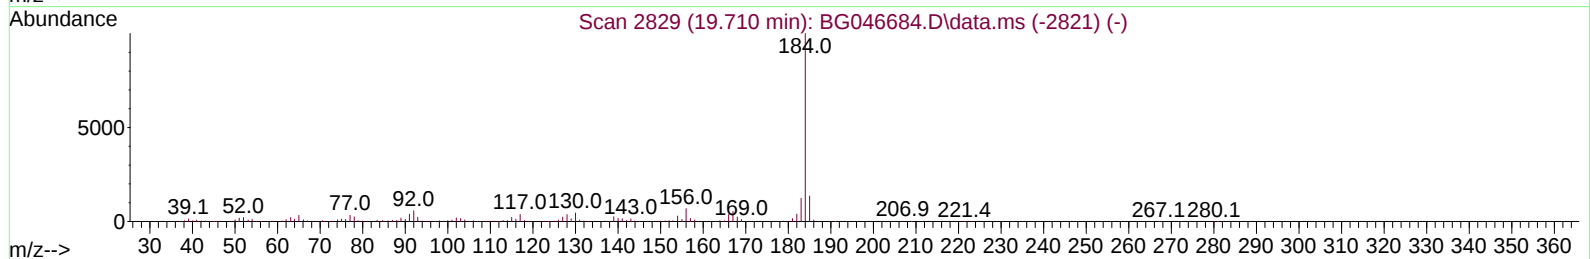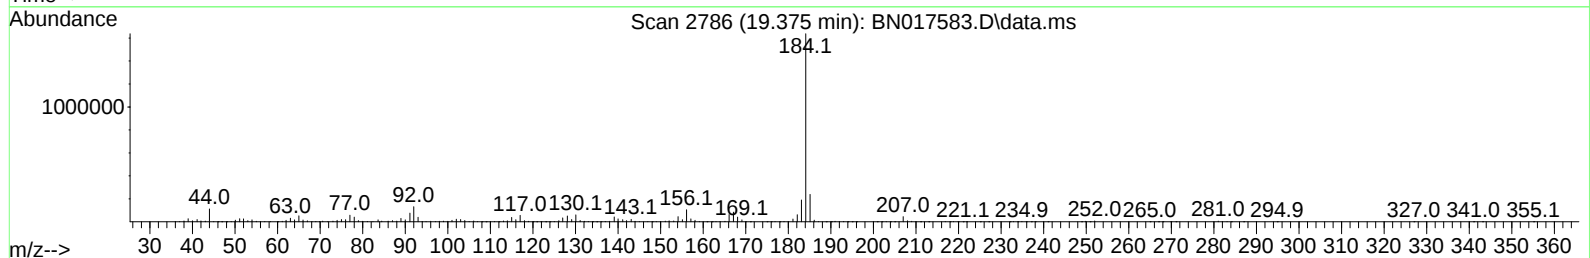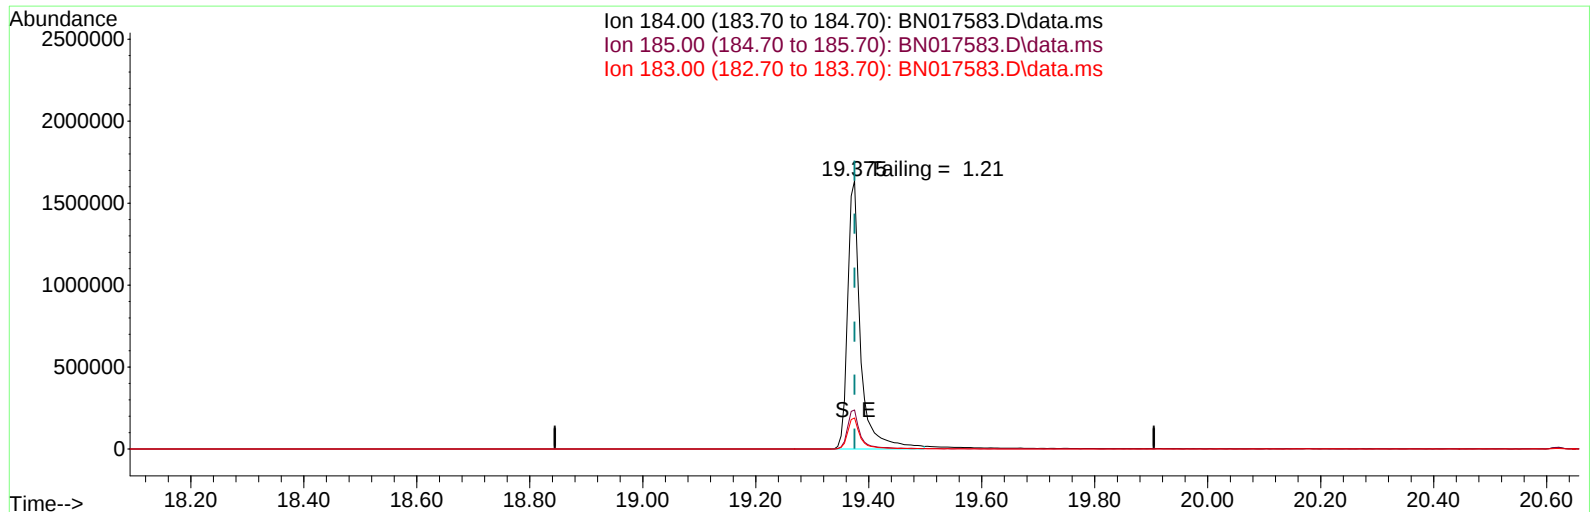

TIC: BN017583.D\data.ms

(77) Benzidine

19.375min (0.000) 57389.52 ng

response 2681885

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.58
183.00	13.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2021	BNA_N	<u>BN017583.D</u>
Compound Name	Response	Retention Time
DDT	1563231	20.622
DDD	288805	20.175
DDE	3416	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
292221	1855452	15.75

Instrument :
BNA_N
ClientSampleId :
DFTPP