
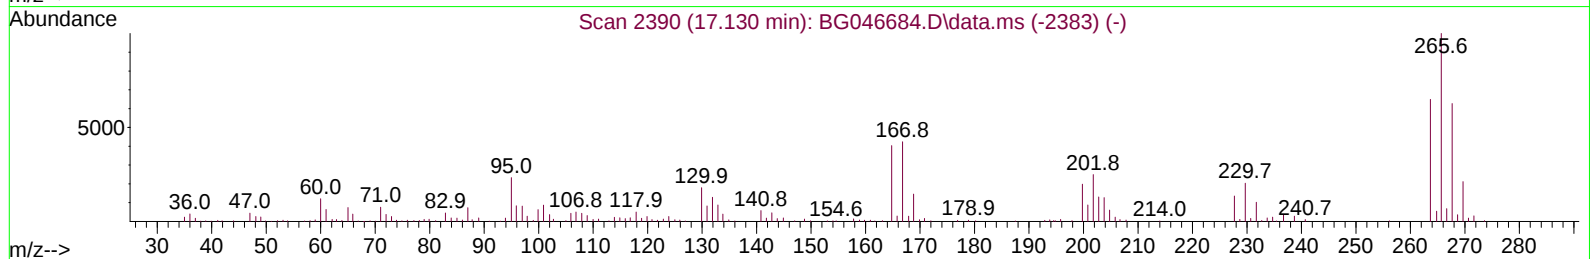
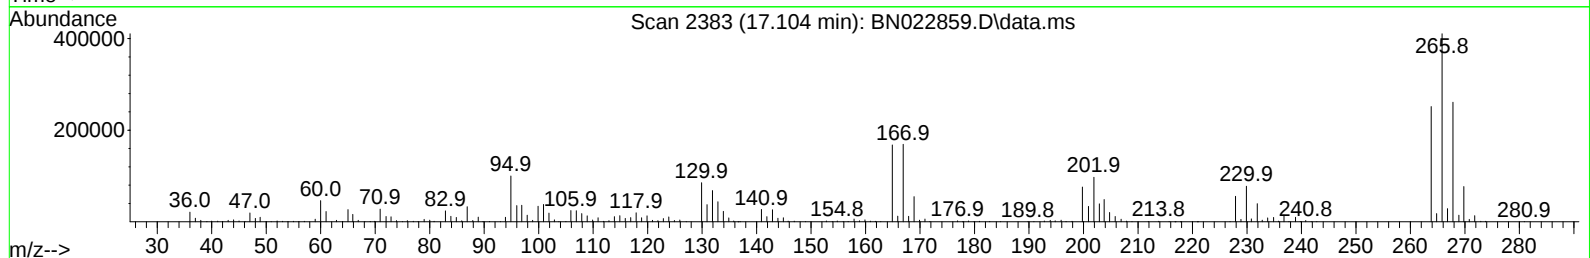


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112522\
Data File : BN022859.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 23:38:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

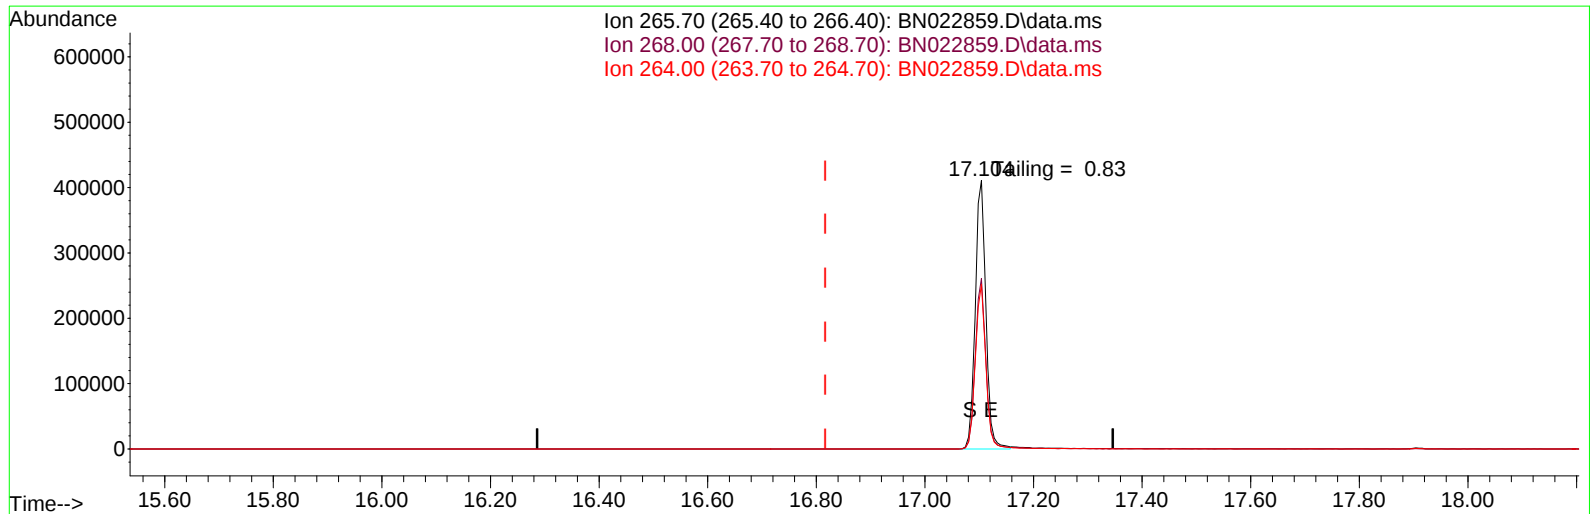

TIC: BN022859.D\data.ms

(70) Pentachlorophenol (C)




17.104min (+ 0.288) 21201.27 ng

response 561540

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.54
264.00	61.60	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112522\
Data File : BN022859.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 23:38:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

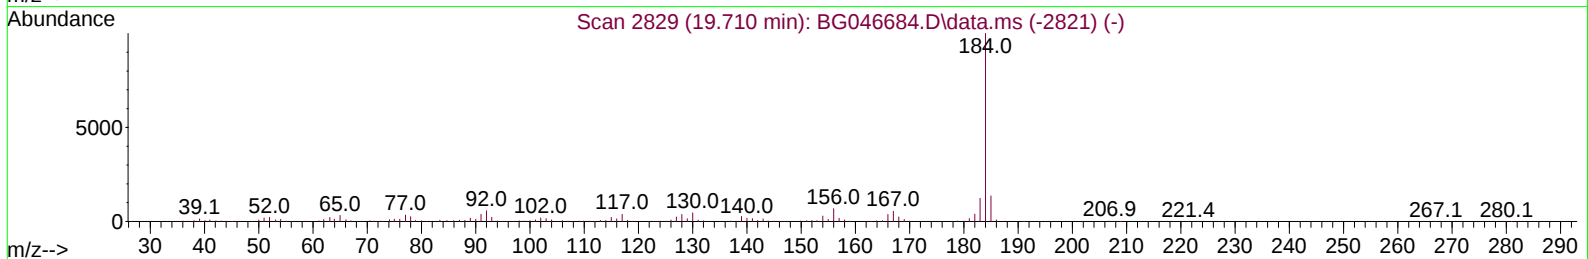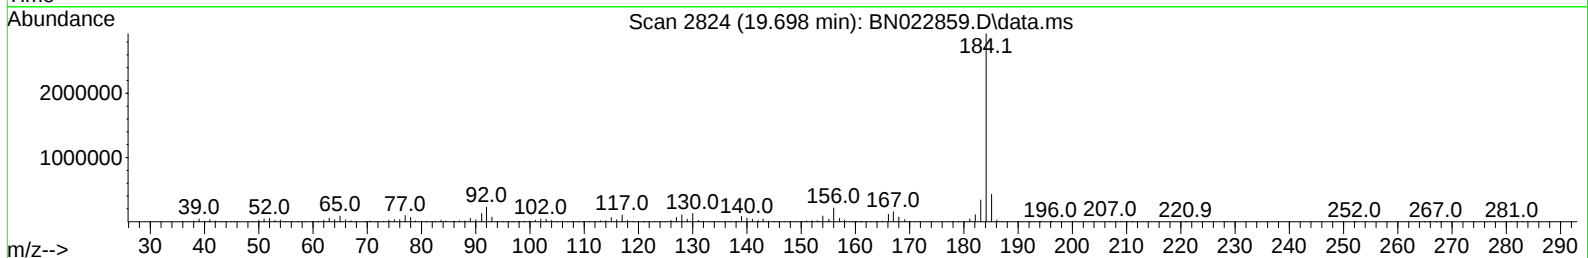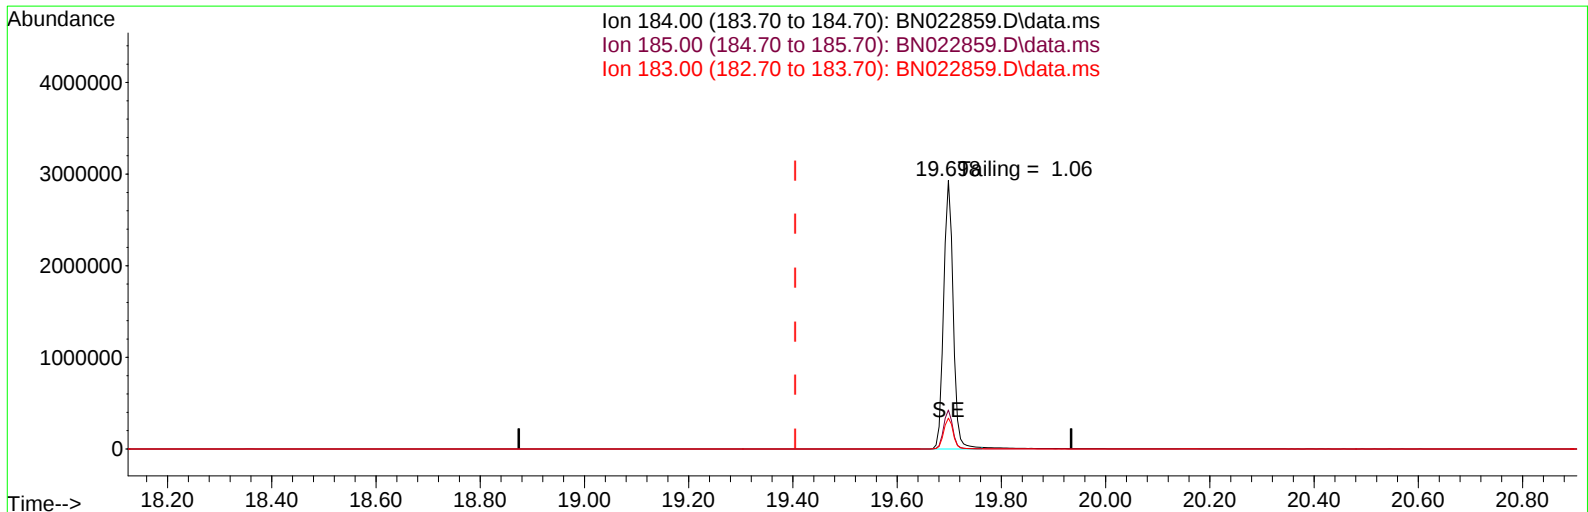

TIC: BN022859.D\data.ms

(77) Benzidine**19.698min (+ 0.294) 0.00 ng****response 3767580**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.51
0.00	0.00	0.00