
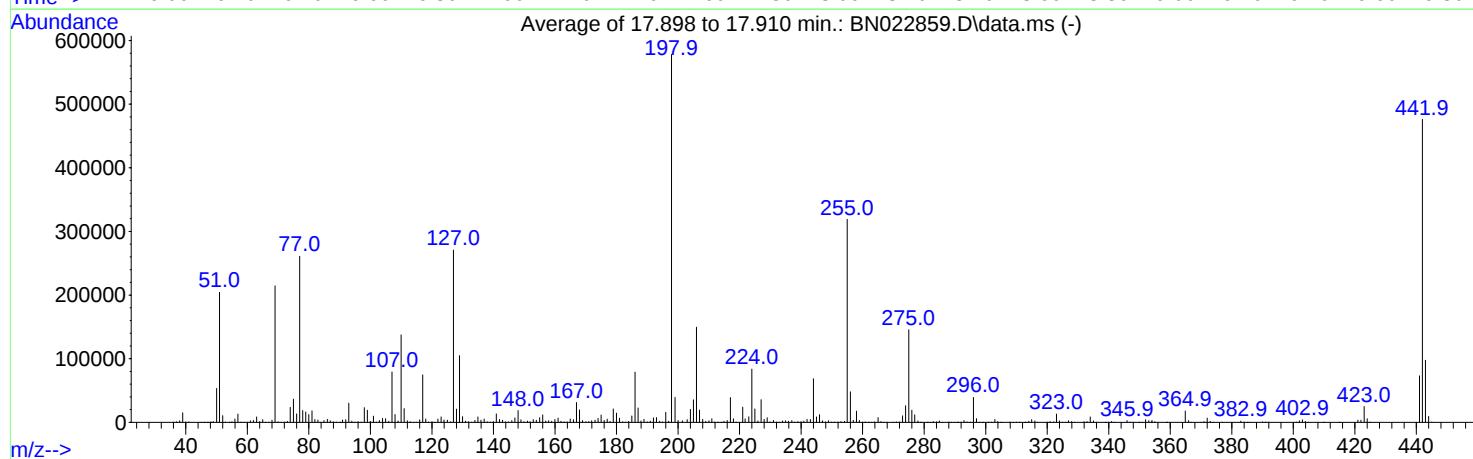


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112522\
 Data File : BN022859.D
 Acq On : 25 Nov 2022 14:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 02 02:30:10 2022

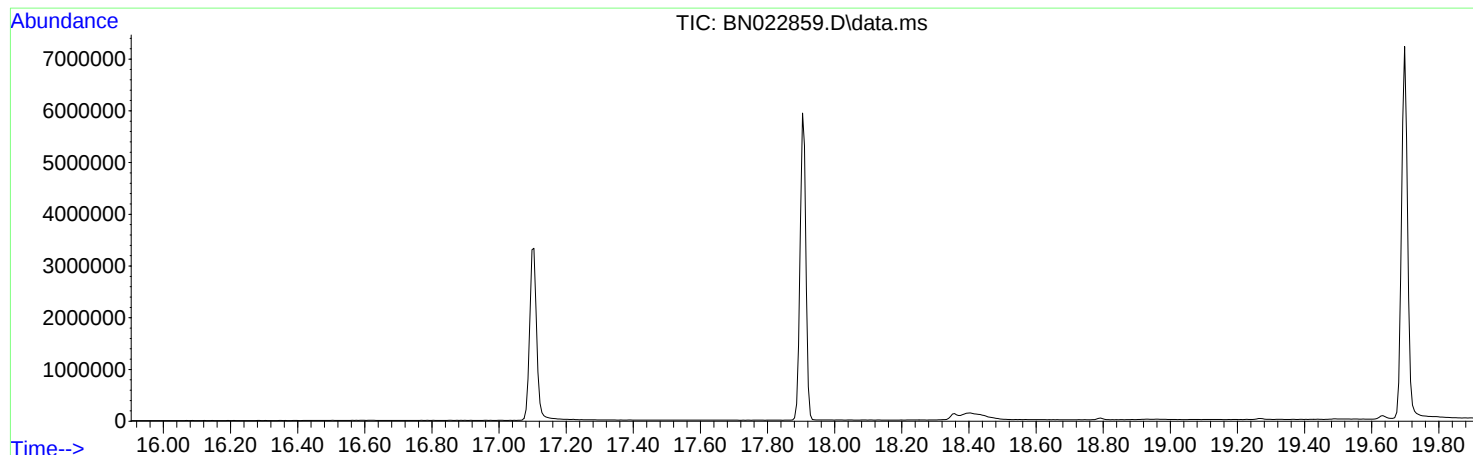




AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	204528	PASS
68	69	0.00	2	1.6	3538	PASS
69	198	0.00	100	37.1	214431	PASS
70	69	0.00	2	0.5	1004	PASS
127	198	10	80	46.9	270912	PASS
197	198	0.00	2	0.3	1853	PASS
198	198	100	100	100.0	578091	PASS
199	198	5	9	6.8	39179	PASS
275	198	10	60	25.2	145600	PASS
365	198	1	100	3.1	17899	PASS
441	198	0.01	100	12.7	73131	PASS
442	442	50	100	100.0	476245	PASS
443	442	15	24	20.5	97488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112522\
 Data File : BN022859.D
 Acq On : 25 Nov 2022 14:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 25 23:38:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 24 05:39:37 2022
 Response via : Initial Calibration

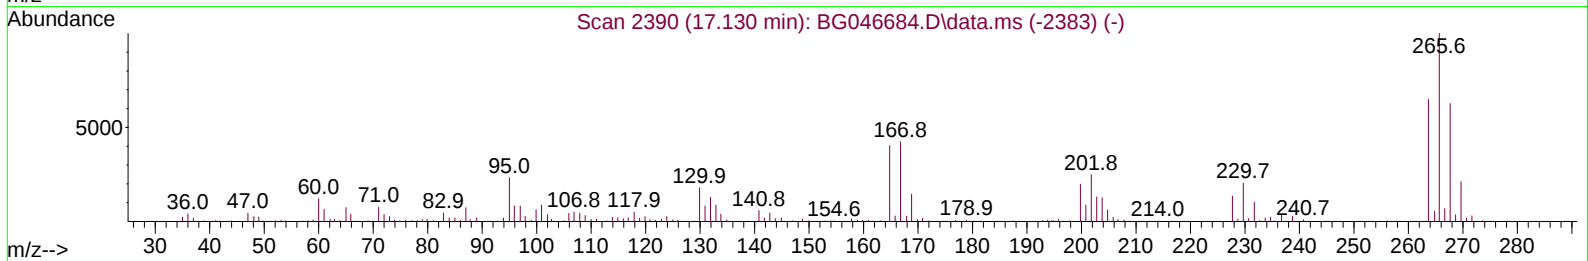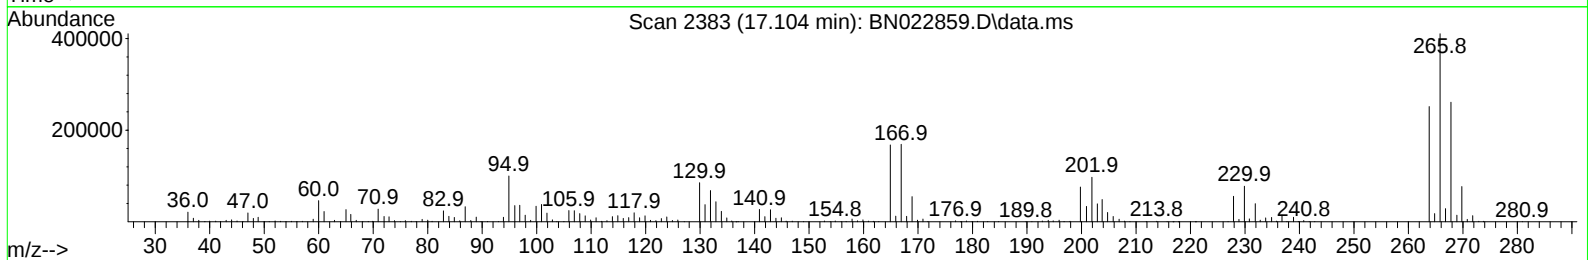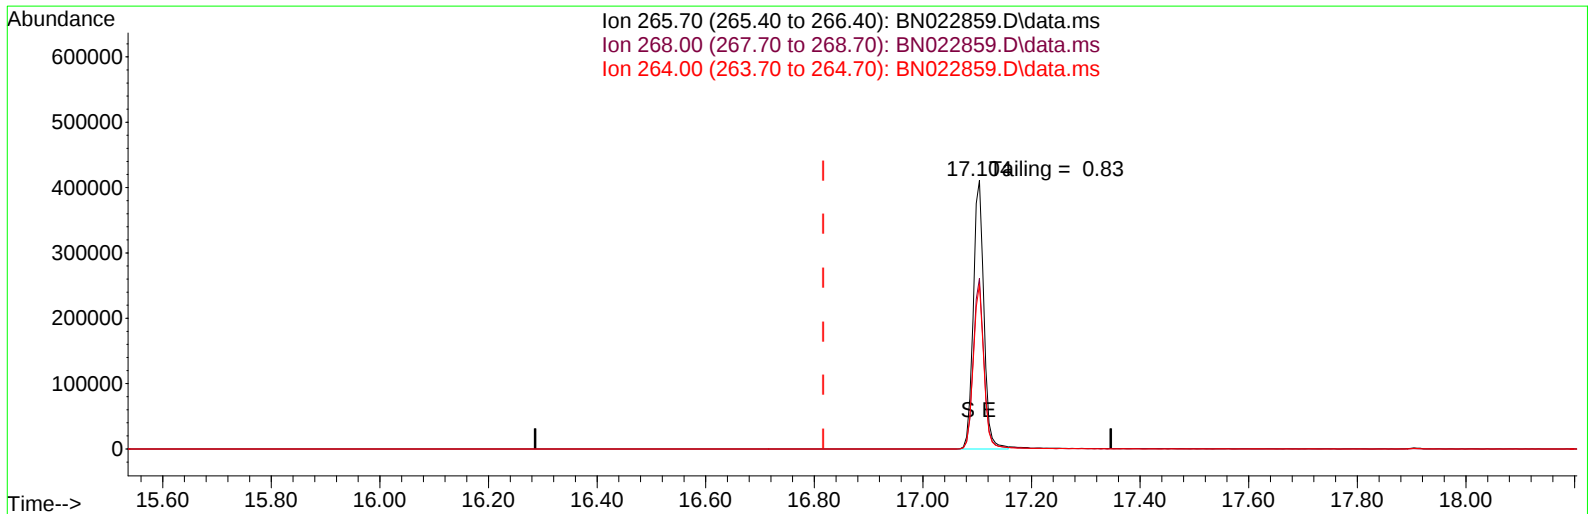

TIC: BN022859.D\data.ms

(70) Pentachlorophenol (C)

17.104min (+ 0.288) 21201.27 ng




response 561540

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.54
264.00	61.60	61.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112522\
Data File : BN022859.D
Acq On : 25 Nov 2022 14:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 25 23:38:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 24 05:39:37 2022
Response via : Initial Calibration

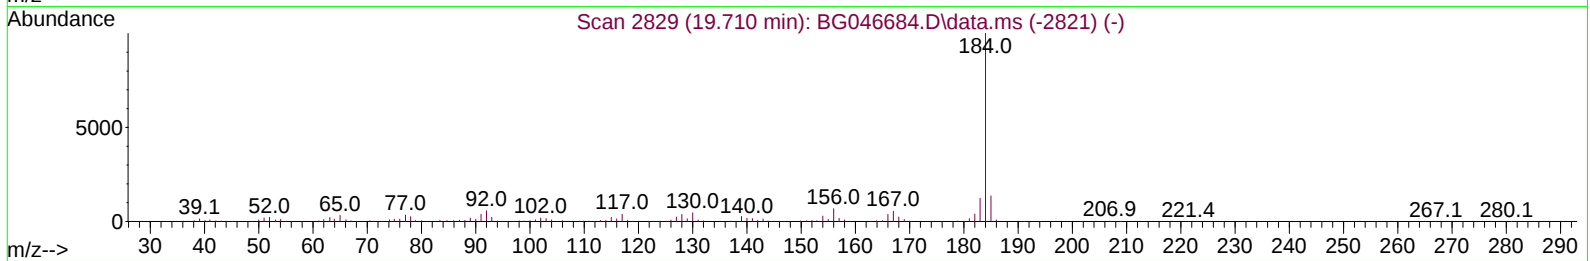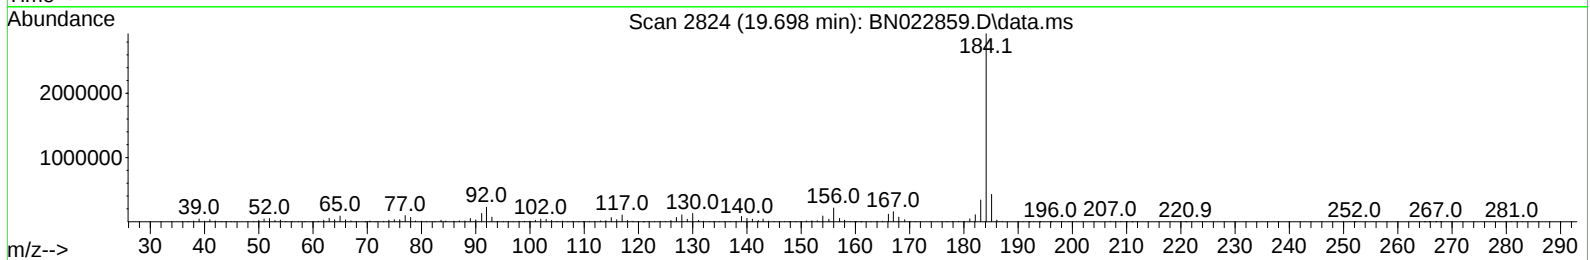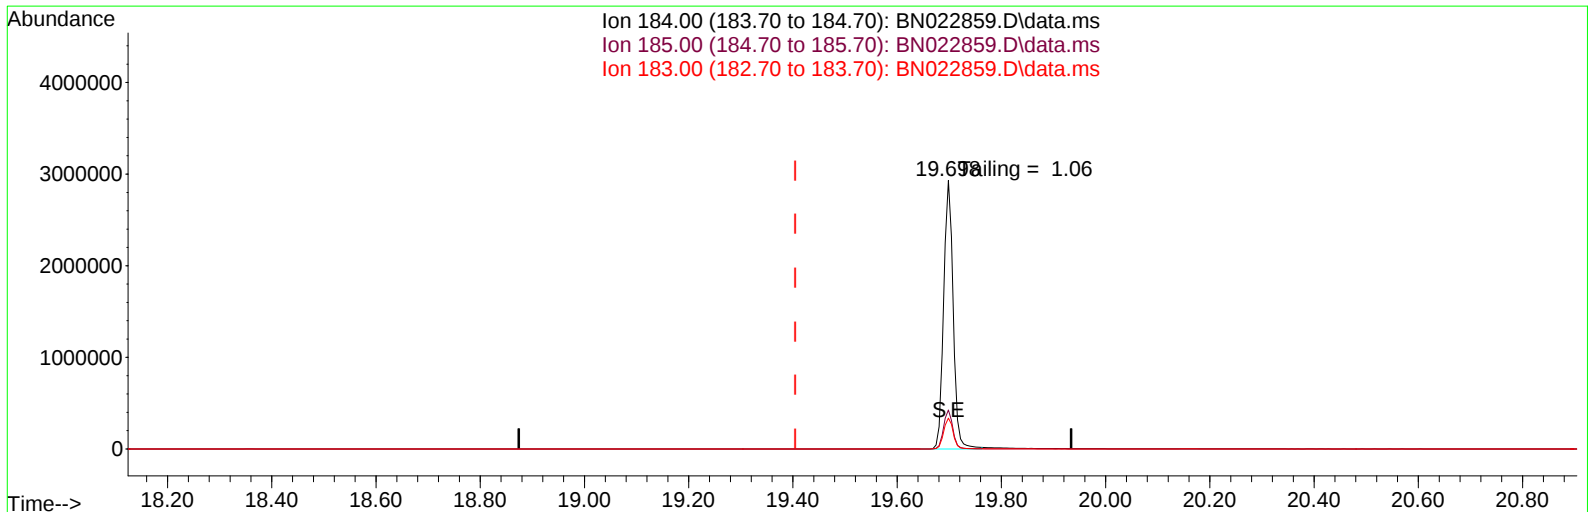

TIC: BN022859.D\data.ms

(77) Benzidine

19.698min (+ 0.294) 0.00 ng

response 3767580

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.51
183.00	13.20	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2022	BNA_N	<u>BN022859.D</u>
Compound Name	Response	Retention Time
DDT	1612870	20.939
DDD	15695	20.551
DDE	0	0
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15695	1628565	0.96

Instrument :
BNA_N
ClientSampleId :
DFTPP