
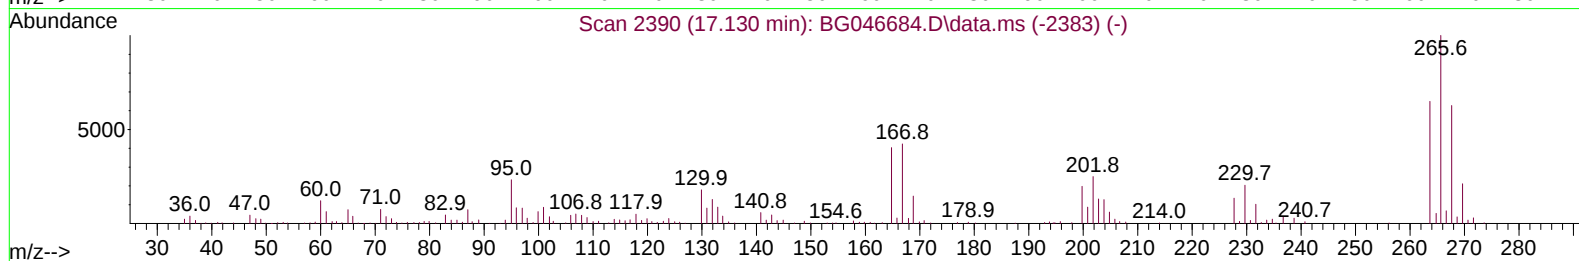
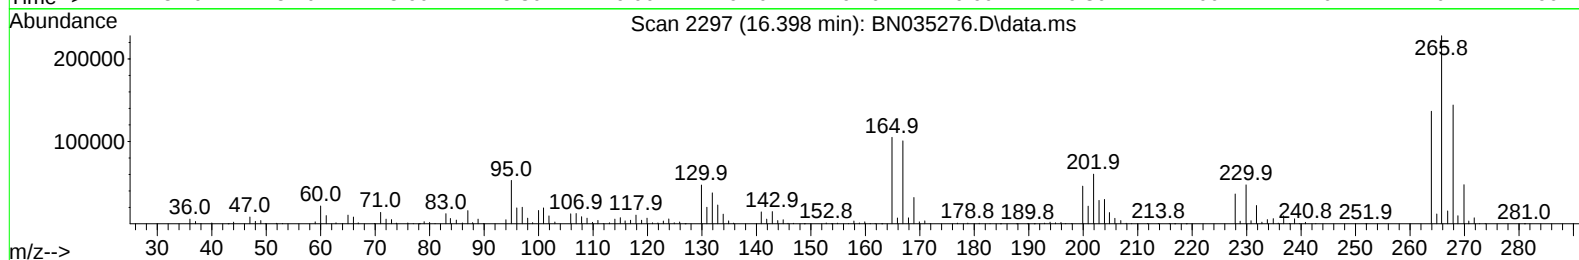


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035276.D
Acq On : 25 Nov 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Nov 26 05:17:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:17:50 2024
Response via : Initial Calibration

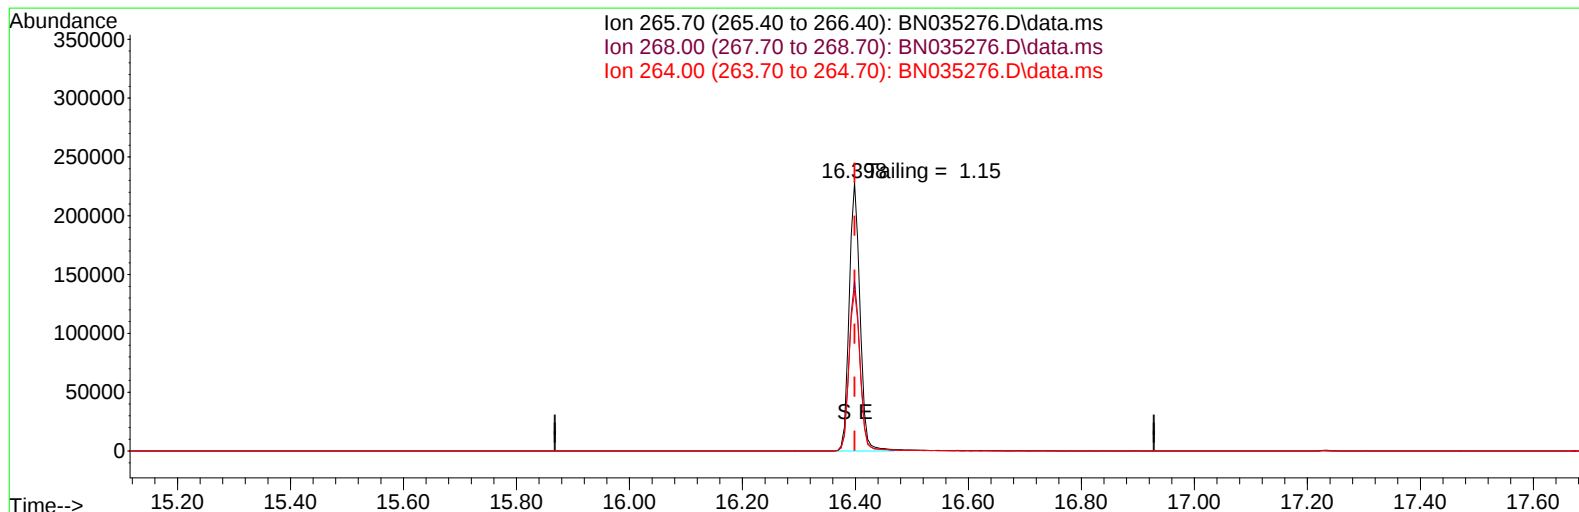

TIC: BN035276.D\data.ms

(70) Pentachlorophenol (C)




16.398min (0.000) 33730.33 ng

response 307325

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.17
264.00	61.60	59.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035276.D
Acq On : 25 Nov 2024 09:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Nov 26 05:17:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:17:50 2024
Response via : Initial Calibration

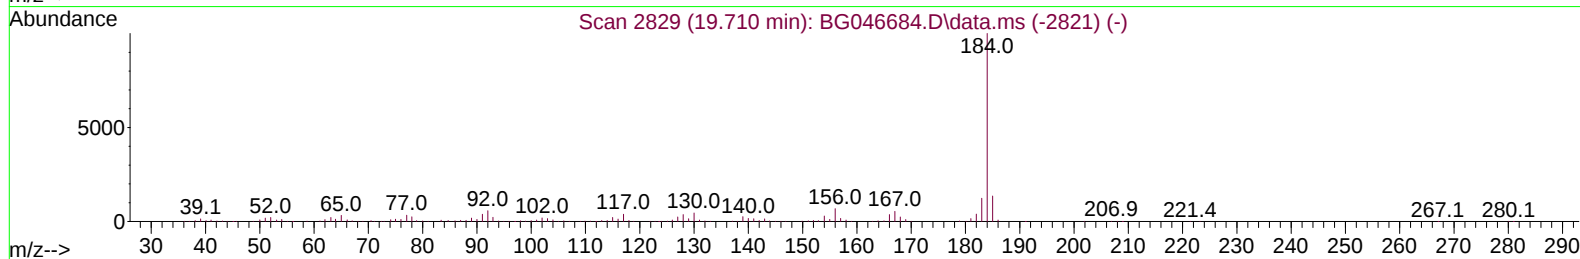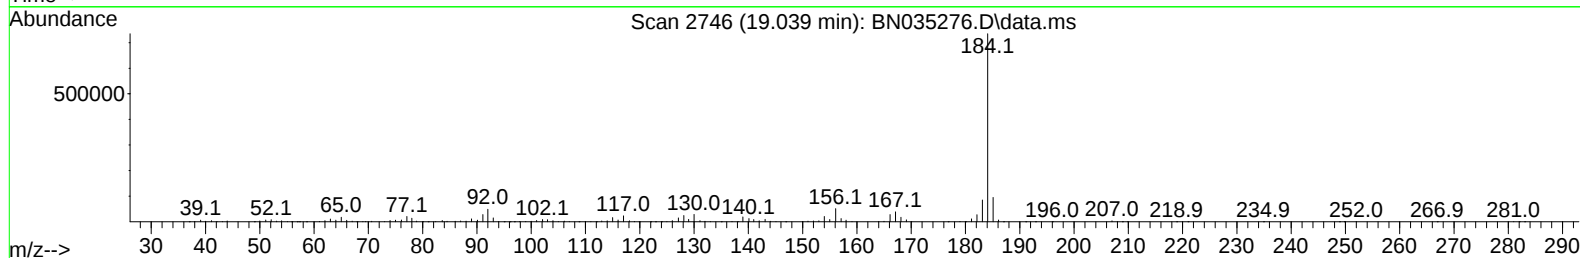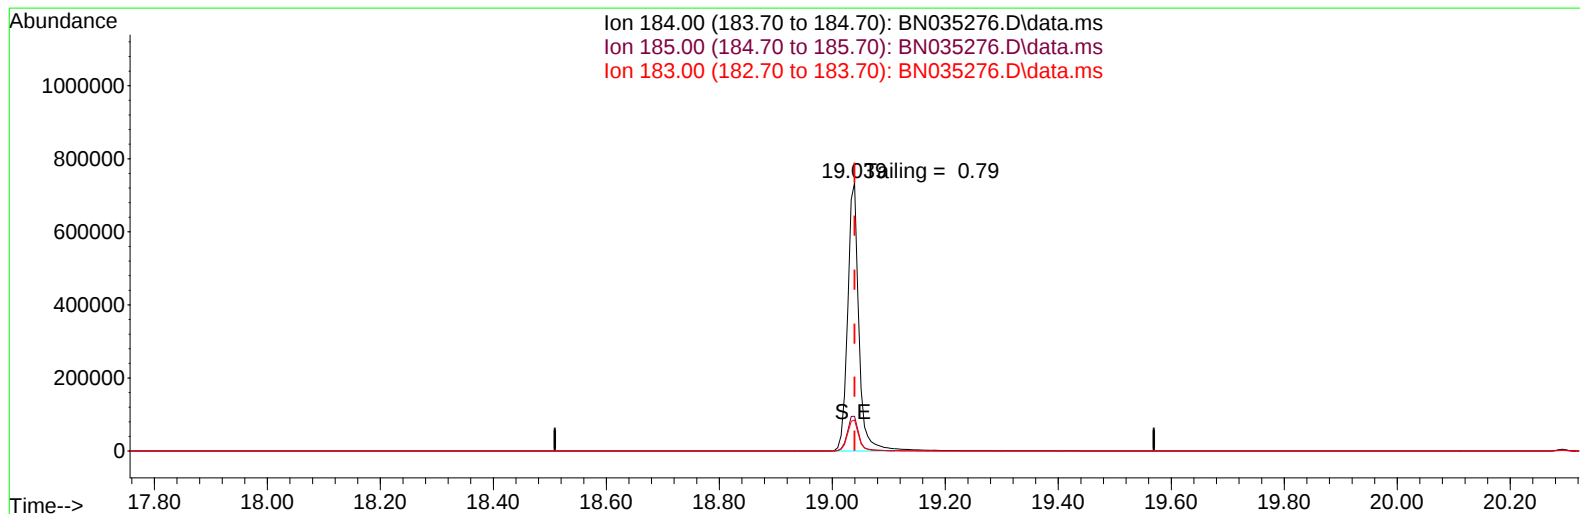

TIC: BN035276.D\data.ms

(77) Benzidine

19.039min (0.000) 0.00 ng

response 1018750

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.97
183.00	13.20	11.60
0.00	0.00	0.00