
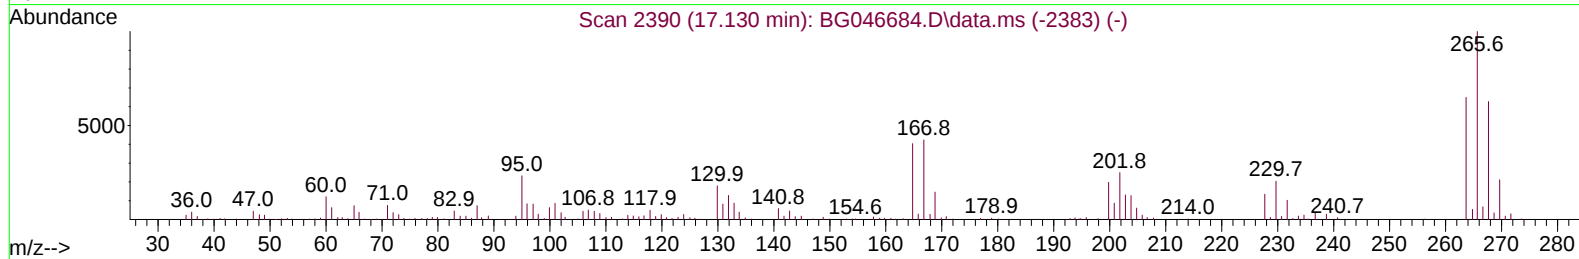
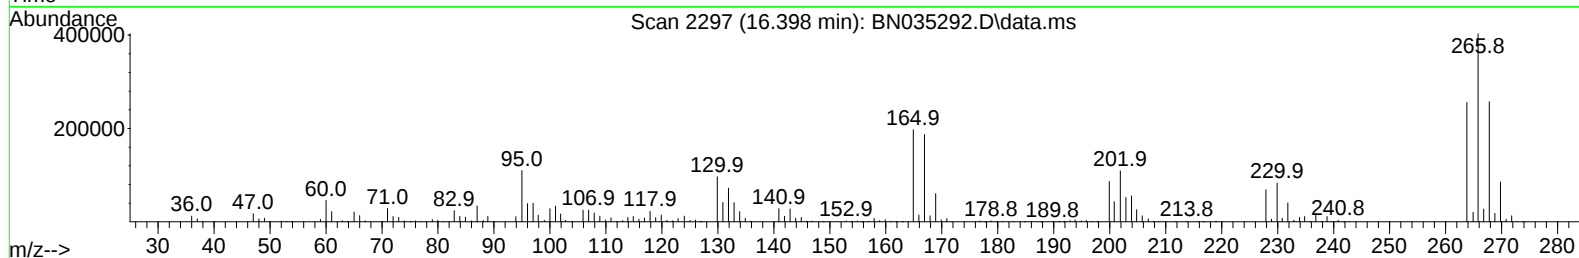


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035292.D
Acq On : 25 Nov 2024 20:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Nov 26 05:22:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:21:56 2024
Response via : Initial Calibration

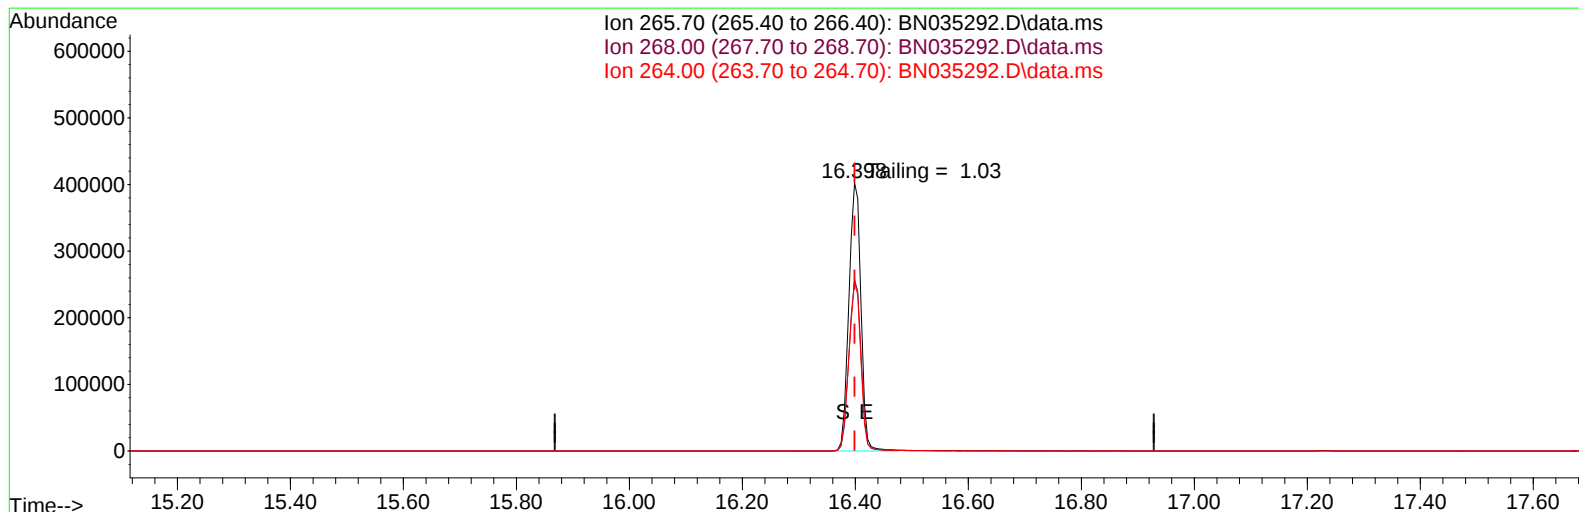

TIC: BN035292.D\data.ms

(70) Pentachlorophenol (C)




16.398min (0.000) 1275879.78 ng

response 600767

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.86
264.00	61.60	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112524\
Data File : BN035292.D
Acq On : 25 Nov 2024 20:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Nov 26 05:22:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 05:21:56 2024
Response via : Initial Calibration

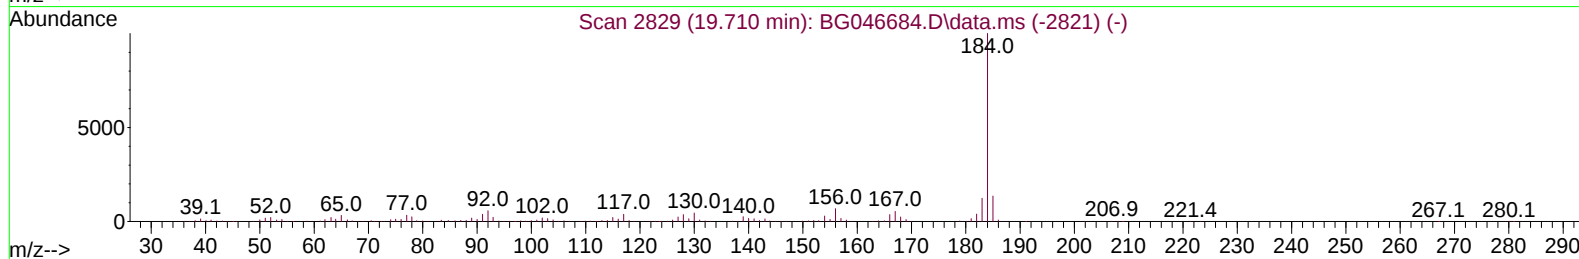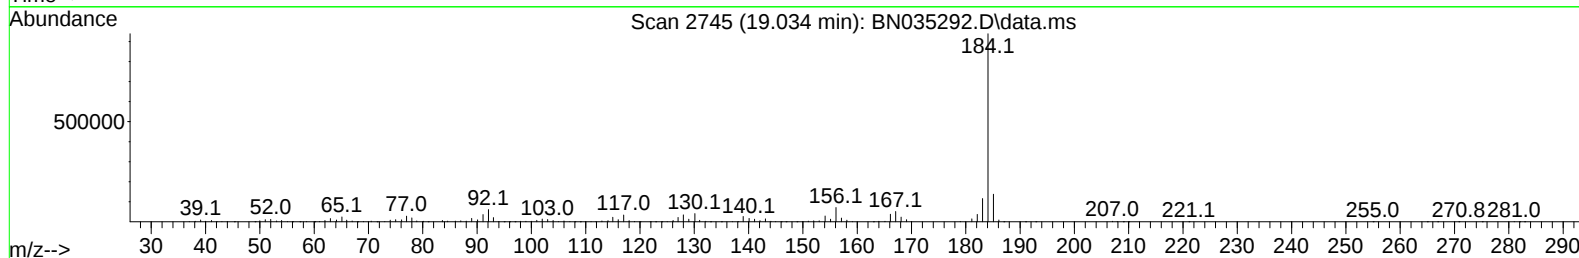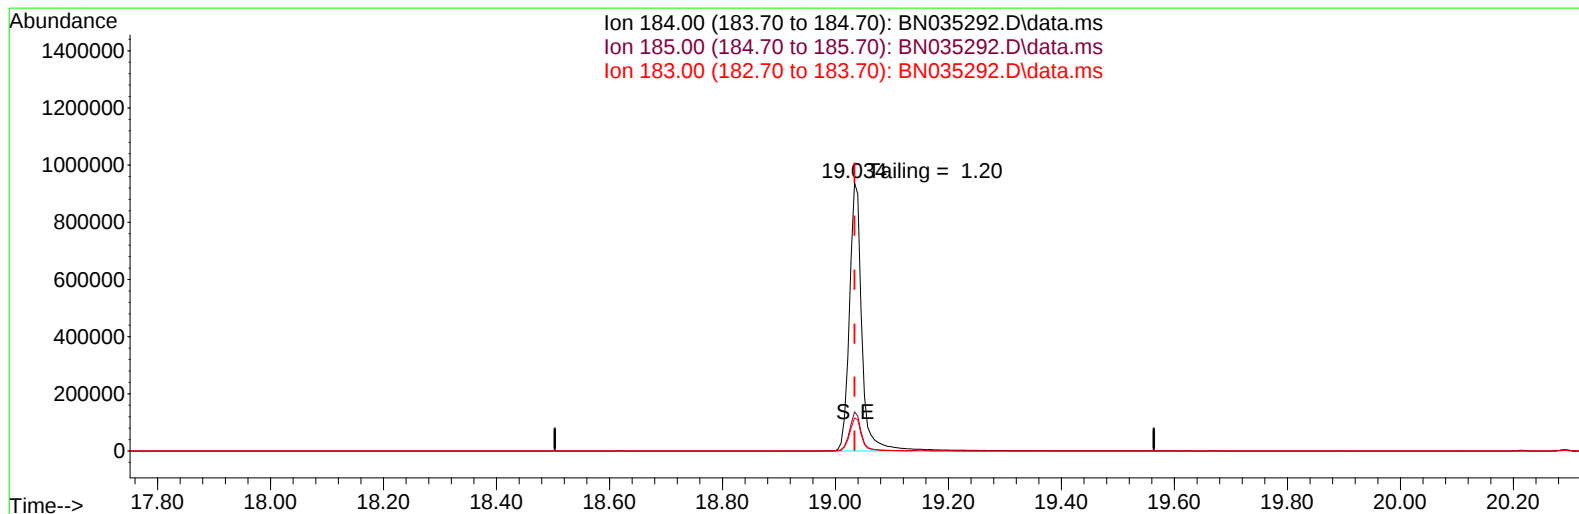

TIC: BN035292.D\data.ms

(77) Benzidine

19.034min (0.000) 201606.82 ng

response 1448003

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.64
183.00	13.20	12.37
0.00	0.00	0.00