

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112720\
 Data File : BN012750.D
 Acq On : 27 Nov 2020 13:07
 Operator : CG/JU
 Sample : L4485-12
 Misc : MDL-WATER-05
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Manual Integrations
 APPROVED

mohammad
 11/30/2020 12:00:52 PM

Quant Time: Nov 27 13:41:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN112520.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 27 10:53:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	105795	20.00	ng/ul	0.00
20) Naphthalene-d8	10.19	136	446574	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.08	164	289021	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.84	188	629584	20.00	ng/ul	0.00
79) Chrysene-d12	21.06	240	664072	20.00	ng/ul	0.00
88) Perylene-d12	23.16	264	740619	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.96	96	12126	4.13	ng/uL	0.00
4) Pyridine-d5	3.36	84	181968	22.92	ng/ul	0.00
7) Phenol-d5	6.61	99	288504	30.46	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.78	67	188735	31.95	ng/ul	0.00
11) 2-Chlorophenol-d4	6.96	132	235705	31.65	ng/ul	0.00
15) 4-Methylphenol-d8	8.13	113	242657	31.46	ng/ul	0.00
21) Nitrobenzene-d5	8.57	128	114476	32.04	ng/ul	0.00
24) 2-Nitrophenol-d4	9.29	143	124969	31.68	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.82	165	229080	30.57	ng/ul	0.00
31) 4-Chloroaniline-d4	10.33	131	304811	29.08	ng/ul	0.00
46) Dimethylphthalate-d6	13.50	166	766477	32.61	ng/ul	0.00
49) Acenaphthylene-d8	13.77	160	907026	33.08	ng/ul	0.00
54) 4-Nitrophenol-d4	14.30	143	115159	27.70	ng/ul	0.00
60) Fluorene-d10	15.09	176	631736	31.84	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.22	200	116644	27.10	ng/ul	0.00
73) Anthracene-d10	16.93	188	970425	30.84	ng/ul	0.00
81) Pyrene-d10	19.25	212	1080528	32.64	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.03	264	1200469	30.00	ng/ul	0.00

Target Compounds

				Ovalue	
2) 1,4-Dioxane	2.99	88	3594m	1.176	ng/uL
5) Pyridine	3.39	79	21326	2.607	ng/ul# 21
6) Benzaldehyde	6.58	77	18777	4.419	ng/ul 92
8) Phenol	6.63	94	24553	2.484	ng/ul# 90
10) Bis(2-Chloroethyl)ether	6.86	93	20718	2.636	ng/ul 97
12) 2-Chlorophenol	6.99	128	19043	2.484	ng/ul 97
13) 2-Methylphenol	7.88	108	15160	2.063	ng/ul 96
14) 2,2'-oxybis(1-Chloropropan	7.96	45	28153m	2.541	ng/ul
16) Acetophenone	8.25	105	32171	2.511	ng/ul 94
17) N-Nitroso-di-n-propylamine	8.23	70	17296	2.605	ng/ul 92
18) 4-Methylphenol	8.20	108	18301	2.286	ng/ul 92
19) Hexachloroethane	8.48	117	9605	2.607	ng/ul# 82
22) Nitrobenzene	8.62	77	26770	2.585	ng/ul 94
23) Isophorone	9.14	82	41476	2.284	ng/ul 99
25) 2-Nitrophenol	9.32	139	10476	2.433	ng/ul# 83
26) 2,4-Dimethylphenol	9.39	107	22308	2.395	ng/ul 96
27) Bis(2-Chloroethoxy)methane	9.63	93	24492	2.342	ng/ul# 98
29) 2,4-Dichlorophenol	9.85	162	17671	2.390	ng/ul 95
30) Naphthalene	10.23	128	64328	2.535	ng/ul 97
32) 4-Chloroaniline	10.36	127	23493	2.300	ng/ul 91
33) Hexachlorobutadiene	10.52	225	12801	2.545	ng/ul 96
34) Caprolactam	11.17	113	3583m	1.485	ng/ul

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN112720\
 Data File : BN012750.D
 Acq On : 27 Nov 2020 13:07
 Operator : CG/JU
 Sample : L4485-12
 Misc : MDL-WATER-05
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleID :
 MDL-WATER-05

Manual Integrations
 APPROVED

mohammad
 11/30/2020 12:00:52 PM

Quant Time: Nov 27 13:41:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN112520.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 27 10:53:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.49	107	18087	2.131	ng/ul#	96
36) 2-Methylnaphthalene	11.86	142	41762	2.333	ng/ul	96
37) 1-Methylnaphthalene	12.09	142	43767	2.536	ng/ul	98
39) 1,2,4,5-Tetrachlorobenzene	12.25	216	22577	2.483	ng/ul	90
40) Hexachlorocyclopentadiene	12.22	237	10137	1.828	ng/ul	94
41) 2,4,6-Trichlorophenol	12.49	196	12368	2.135	ng/ul	87
42) 2,4,5-Trichlorophenol	12.57	196	12574m	1.992	ng/ul	
43) 1,1'-Biphenyl	12.90	154	56687	2.417	ng/ul#	91
44) 2-Chloronaphthalene	12.94	162	45676	2.465	ng/ul	92
45) 2-Nitroaniline	13.16	65	11542	1.902	ng/ul	89
47) Dimethylphthalate	13.55	163	61613	2.561	ng/ul	97
48) 2,6-Dinitrotoluene	13.67	165	10016	2.104	ng/ul	92
50) Acenaphthylene	13.80	152	70588	2.506	ng/ul	95
51) 3-Nitroaniline	14.01	138	7868	2.023	ng/ul#	91
52) Acenaphthene	14.15	153	50287	2.438	ng/ul	90
53) 2,4-Dinitrophenol	14.22	184	3284	1.116	ng/ul	90
55) 4-Nitrophenol	14.32	109	11159	2.569	ng/ul#	76
56) Dibenzofuran	14.49	168	71826	2.519	ng/ul	100
57) 2,4-Dinitrotoluene	14.47	165	14742	2.124	ng/ul#	68
58) 2,3,4,6-Tetrachlorophenol	14.72	232	11675	2.135	ng/ul#	94
59) Diethylphthalate	14.93	149	62495	2.502	ng/ul	96
61) Fluorene	15.14	166	61448	2.550	ng/ul	99
62) 4-Chlorophenyl-phenylether	15.15	204	28345	2.469	ng/ul	98
63) 4-Nitroaniline	15.18	138	10217m	2.597	ng/ul	
66) 4,6-Dinitro-2-methylphenol	15.23	198	10558	2.273	ng/ul#	46
67) N-Nitrosodiphenylamine	15.36	169	45186	2.307	ng/ul	98
68) 4-Bromophenyl-phenylether	16.04	248	17519	2.465	ng/ul	91
69) Hexachlorobenzene	16.14	284	21589	2.588	ng/ul	91
70) Atrazine	16.32	200	15425	2.017	ng/ul	99
71) Pentachlorophenol	16.49	266	8647	1.690	ng/ul#	89
72) Phenanthrene	16.88	178	97949m	2.552	ng/ul	
74) Anthracene	16.97	178	100410	2.579	ng/ul#	95
75) 1,2,3,4-Tetrachlorobenzene	12.86	216	22458	2.491	ng/uL	97
76) Pentachlorobenzene	14.40	250	24284	2.545	ng/uL	94
77) Carbazole	17.25	167	70450	2.061	ng/ul	97
78) Di-n-butylphthalate	17.83	149	88989	2.046	ng/ul	99
80) Fluoranthene	18.91	202	103779	2.392	ng/ul#	96
82) Pyrene	19.27	202	119133	2.615	ng/ul	98
83) Butylbenzylphthalate	20.20	149	36775	1.897	ng/ul	99
84) 3,3'-Dichlorobenzidine	20.99	252	30517	1.962	ng/ul#	96
85) Benzo(a)anthracene	21.04	228	106937	2.411	ng/ul	92
86) Bis(2-ethylhexyl)phthalate	20.99	149	55801	1.778	ng/ul#	97
87) Chrysene	21.09	228	109736	2.542	ng/ul	98
89) Di-n-octyl phthalate	21.84	149	96183	1.668	ng/ul	100
90) Benzo(b)fluoranthene	22.54	252	116934	2.429	ng/ul	98
91) Benzo(k)fluoranthene	22.58	252	118395m	2.450	ng/ul	
93) Benzo(a)pyrene	23.07	252	117126	2.614	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.24	276	142980	2.499	ng/ul	98
95) Dibenzo(a,h)anthracene	25.25	278	119135	2.466	ng/ul	97
96) Benzo(g,h,i)perylene	25.87	276	113105	2.393	ng/ul	94

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN112720\
Data File : BN012750.D
Acq On : 27 Nov 2020 13:07
Operator : CG/JU
Sample : L4485-12
Misc : MDL-WATER-05
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05


Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

Quant Time: Nov 27 13:41:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN112520.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 27 10:53:49 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 1.176 ng/uL m

RT: 2.99 min Scan# 86

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion:	88	Resp:	3594
Ion	Ratio	Lower	Upper
88	100		
43	37.0	29.4	44.0
58	62.6	58.2	87.4

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM



#5

Pyridine

Concen: 2.607 ng/uL




RT: 3.39 min Scan# 153


Delta R.T. 0.01 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion:	79	Resp:	21326
Ion	Ratio	Lower	Upper
79	100		
52	182.9	68.7	103.1#
51	61.5	35.5	53.3#

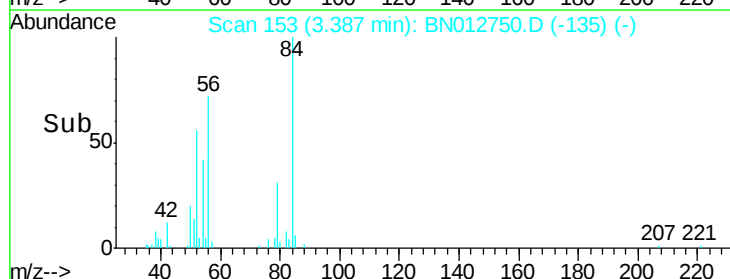



#6

Benzaldehyde

Concen: 4.419 ng/ul

RT: 6.58 min Scan# 696

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion:	77	Resp:	18777
Ion	Ratio	Lower	Upper
77	100		
105	98.7	72.3	108.5
106	82.4	71.8	107.6

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

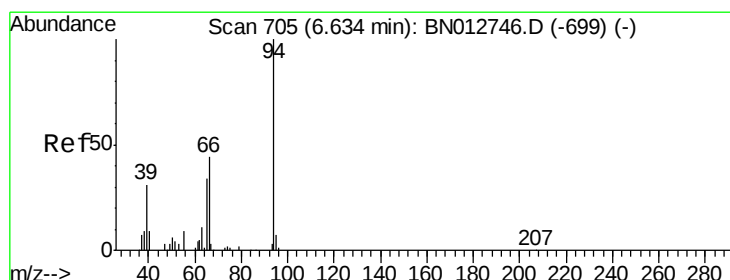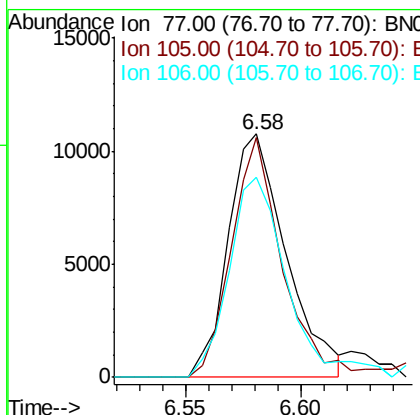

#8

Phenol

Concen: 2.484 ng/ul




RT: 6.63 min Scan# 705




Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion:	94	Resp:	24553
Ion	Ratio	Lower	Upper
94	100		
65	33.1	26.6	39.8
66	57.2	36.9	55.3

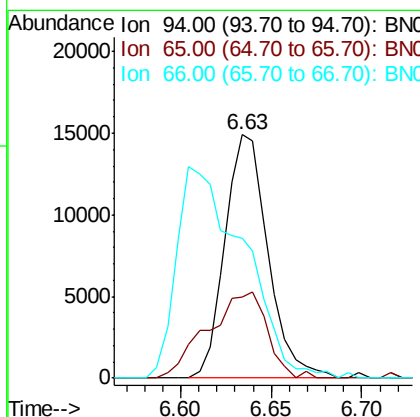

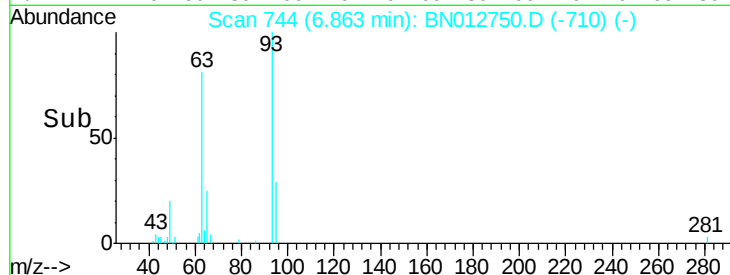





#10
Bis(2-Chloroethyl)ether
Concen: 2.636 ng/ul
RT: 6.86 min Scan# 744
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tot Ion:	93	Resp:	20718
Ion Ratio	Lower	Upper	
93	100		
63	80.7	66.2	99.2
95	28.7	25.9	38.9

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05


Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

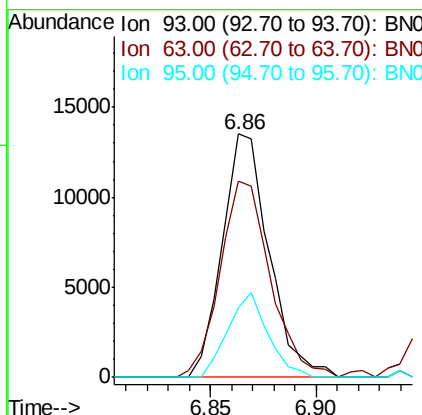

#12
2-Chlorophenol
Concen: 2.484 ng/ul
RT: 6.99 min Scan# 765
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion:	128	Resp:	19043
Ion Ratio	Lower	Upper	
128	100		
64	53.7	41.0	61.6
130	33.8	25.7	38.5

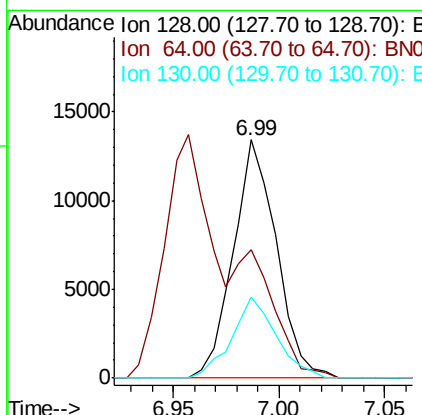

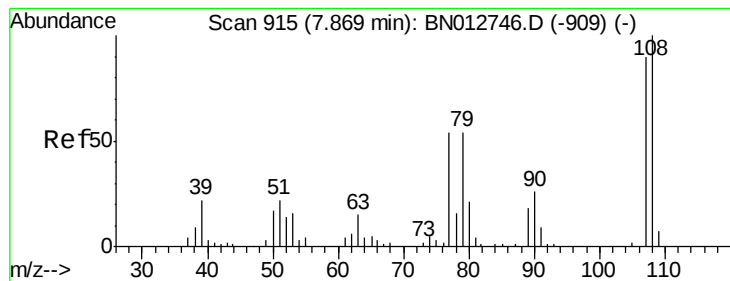

#13

2-Methylphenol

Concen: 2.063 ng/ul

RT: 7.88 min Scan# 916

Delta R.T. 0.01 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N

ClientSampled :

MDL-WATER-05

Tot Ion: 108 Resp: 15160

Ion Ratio Lower Upper

108 100


107 99.9 76.5 114.7

Manual Integrations

APPROVED

mohammad

11/30/2020 12:00:52 PM



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

10000

8000

6000

4000



2000

0

7.85

7.90

Time-->



#14

2,2'-oxybis(1-Chloropropane)

Concen: 2.541 ng/ul m

RT: 7.96 min Scan# 931

Delta R.T. 0.01 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07


Tgt Ion: 45 Resp: 28153

Ion Ratio Lower Upper

45 100

77 19.6 13.1 19.7

79 14.6 9.8 14.6



Abundance Ion 45.00 (44.70 to 45.70): BNC

Ion 77.00 (76.70 to 77.70): BNC

Ion 79.00 (78.70 to 79.70): BNC

15000

10000

5000


0


7.90

7.95

8.00

Time-->

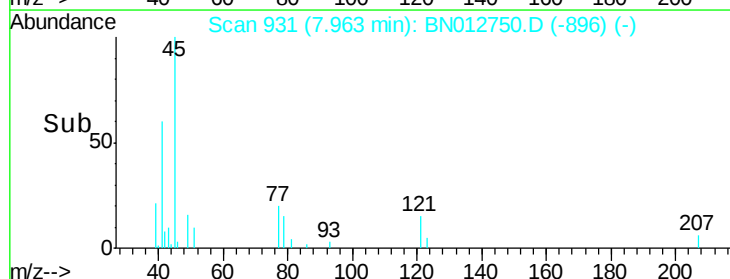







#16
Acetophenone
Concen: 2.511 ng/ul
RT: 8.25 min Scan# 979
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion:	105	Resp:	32171
Ion Ratio	Lower	Upper	
105	100		
77	76.8	66.3	99.5
51	35.1	26.4	39.6




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

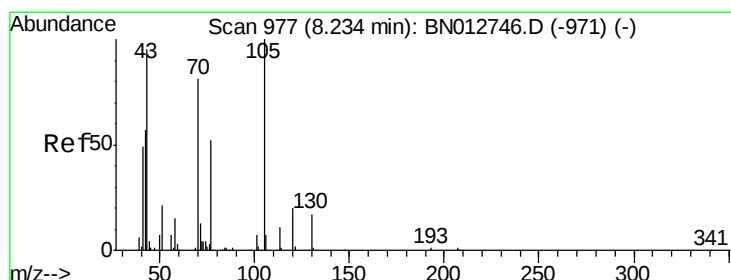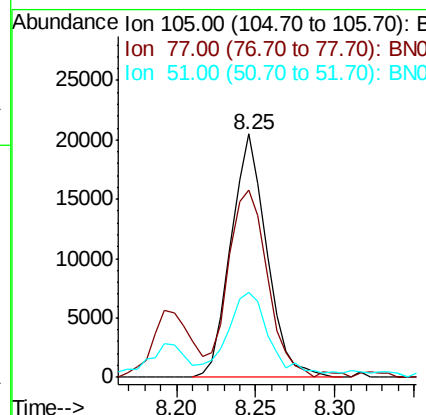

#17
N-Nitroso-di-n-propylamine
Concen: 2.605 ng/ul
RT: 8.23 min Scan# 977
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion:	70	Resp:	17296
Ion Ratio	Lower	Upper	
70	100		
42	60.8	53.7	80.5
101	11.0	7.7	11.5
130	15.2	15.1	22.7

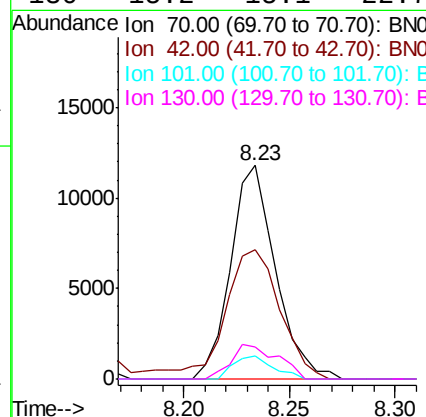







#18
4-Methylphenol
Concen: 2.286 ng/ul
RT: 8.20 min Scan# 971
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
108	100		
107	129.2	95.9	143.9




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

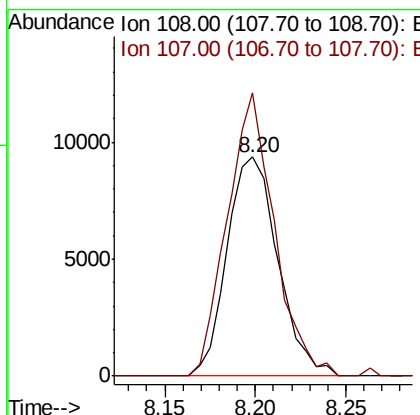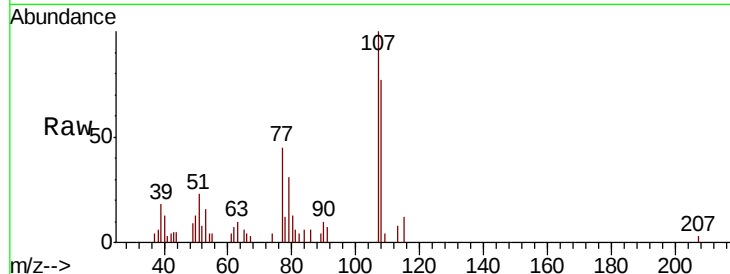

#19
Hexachloroethane
Concen: 2.607 ng/ul
RT: 8.48 min Scan# 1019
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
117	100		
201	109.3	71.0	106.4#
199	67.1	46.7	70.1

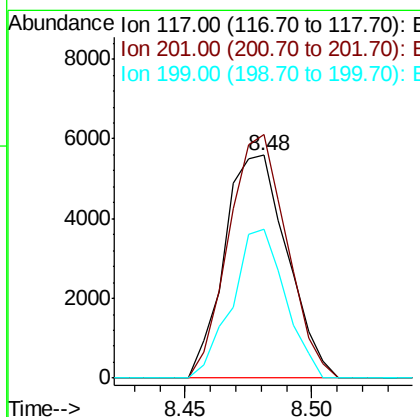







#22
 Nitrobenzene
 Concen: 2.585 ng/ul
 RT: 8.62 min Scan# 1042
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
77	100		
123	34.9	31.3	46.9
65	13.3	11.7	17.5




Manual Integrations
 APPROVED


mohammad
 11/30/2020 12:00:52 PM

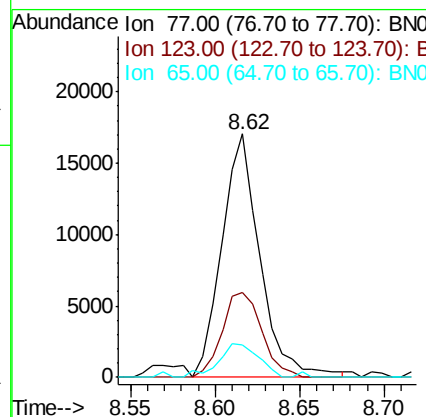

#23
 Isophorone
 Concen: 2.284 ng/ul
 RT: 9.14 min Scan# 1131
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
82	100		
95	8.0	6.5	9.7
138	15.5	12.6	19.0

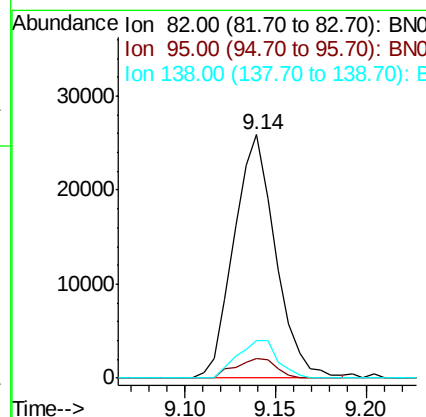







#25
2-Nitrophenol
Concen: 2.433 ng/ul
RT: 9.32 min Scan# 1161
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
139	100		
65	80.5	47.5	71.3#
109	39.6	31.8	47.8




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

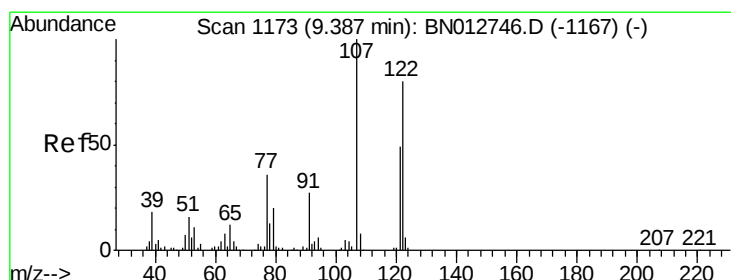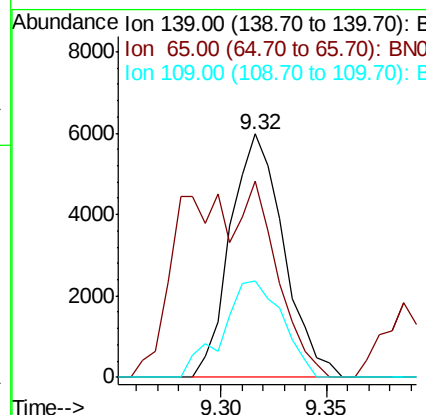

#26
2,4-Dimethylphenol
Concen: 2.395 ng/ul
RT: 9.39 min Scan# 1173
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
107	100		
121	39.1	36.8	55.2
122	71.8	57.9	86.9

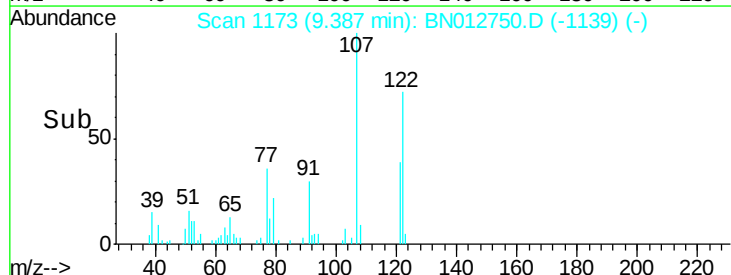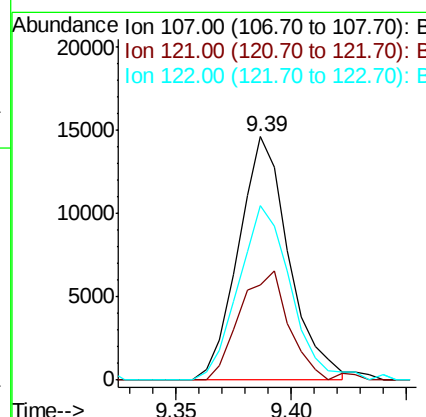

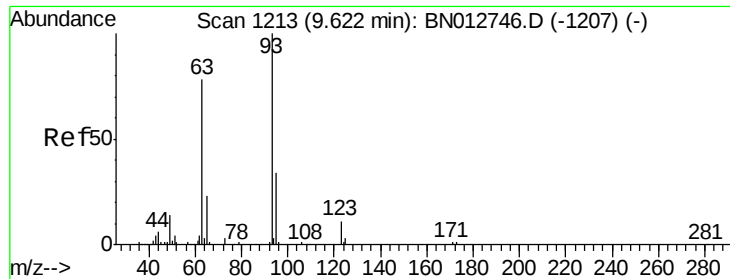

#27

Bis(2-Chloroethoxy)methane

Concen: 2.342 ng/ul

RT: 9.63 min Scan# 1214

Delta R.T. 0.01 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion:	93	Resp:	24492
Ion	Ratio	Lower	Upper
93	100		
95	29.1	23.5	35.3
123	12.7	7.8	11.6

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

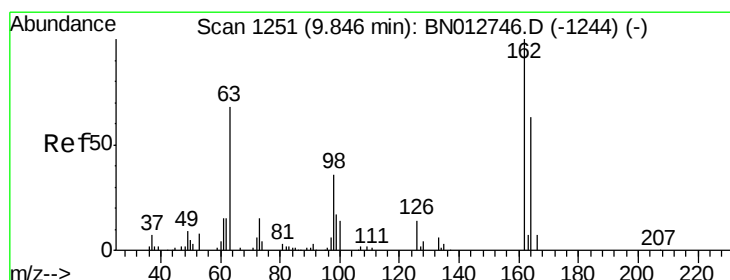

#29

2,4-Dichlorophenol

Concen: 2.390 ng/ul




RT: 9.85 min Scan# 1251


Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion:	162	Resp:	17671
Ion	Ratio	Lower	Upper
162	100		
164	71.6	53.2	79.8
98	40.7	31.0	46.4



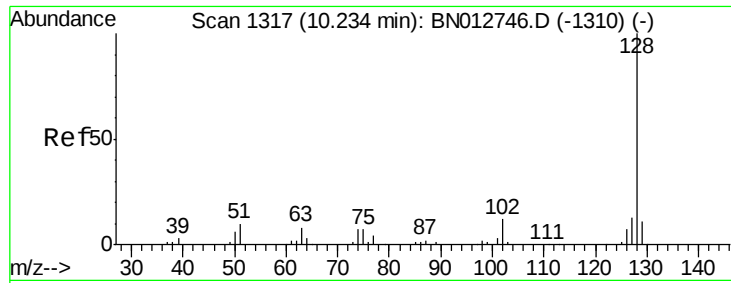





#30
Naphthalene
Concen: 2.535 ng/ul
RT: 10.23 min Scan# 1317
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.0	9.0	13.6
127	15.3	10.5	15.7




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

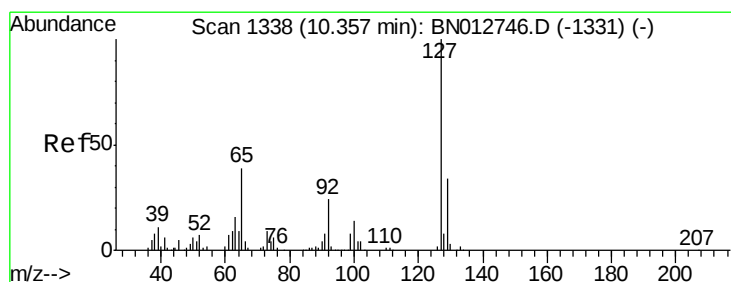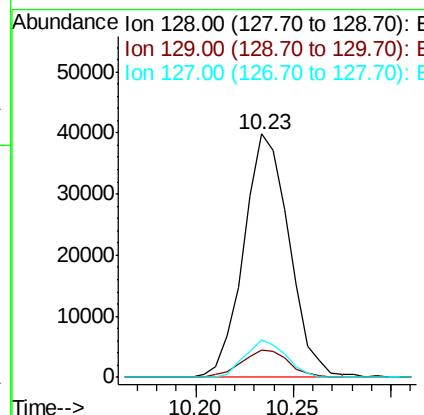

#32
4-Chloroaniline
Concen: 2.300 ng/ul
RT: 10.36 min Scan# 1339
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
127	100		
129	33.5	23.1	34.7

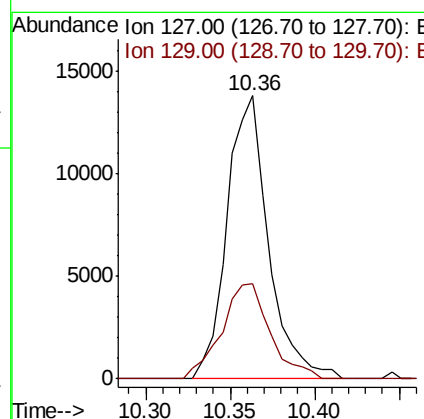

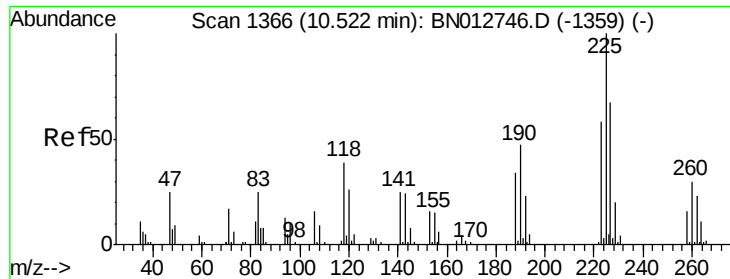





#33
Hexachlorobutadiene
Concen: 2.545 ng/ul
RT: 10.52 min Scan# 1366
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
225	100		
223	61.1	48.3	72.5
227	55.9	48.5	72.7




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

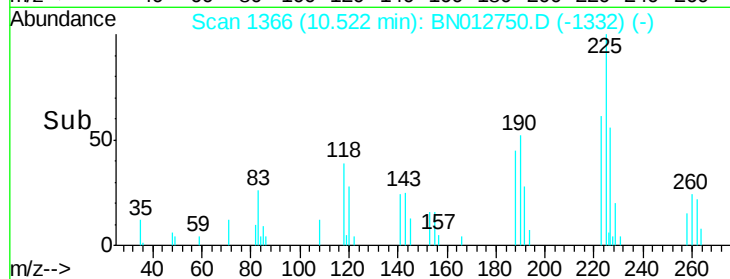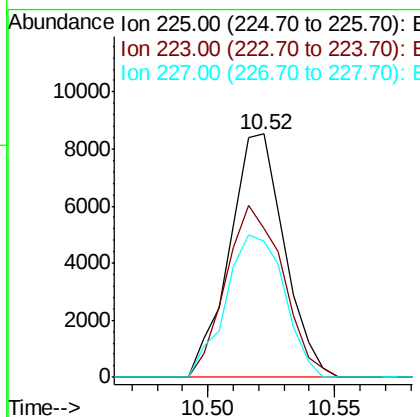

#34
Caprolactam
Concen: 1.485 ng/ul m
RT: 11.17 min Scan# 1476
Delta R.T. 0.04 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
113	100		
55	210.2	135.4	203.2#
56	148.5	90.2	135.2#

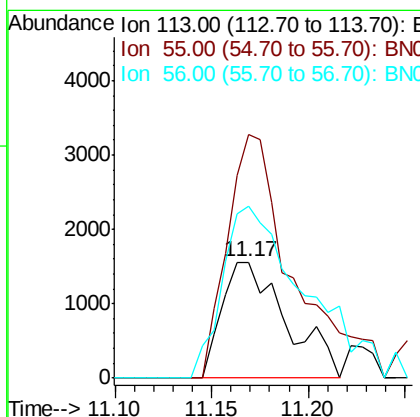







#35
4-Chloro-3-methylphenol
Concen: 2.131 ng/ul
RT: 11.49 min Scan# 1531
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
107	100		
144	18.6	19.4	29.0#
142	72.5	56.9	85.3




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

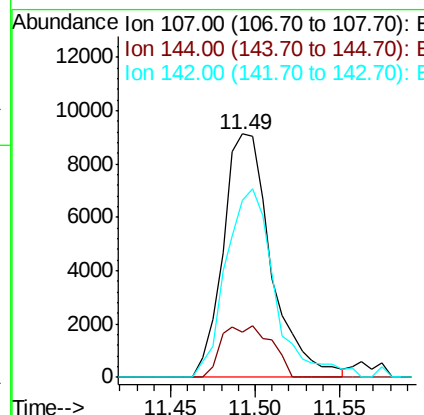

#36
2-Methylnaphthalene
Concen: 2.333 ng/ul
RT: 11.86 min Scan# 1594
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
142	100		
141	91.9	70.4	105.6

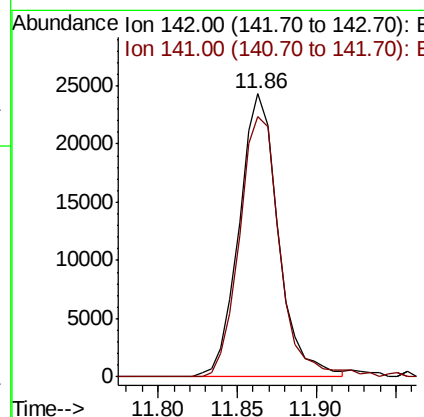







#37
1-Methylnaphthalene
Concen: 2.536 ng/ul
RT: 12.09 min Scan# 1632
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
142	100		
141	90.9	73.9	110.9
116	4.4	3.7	5.5




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

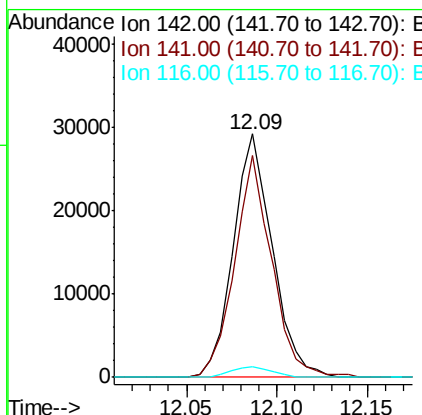

#39
1,2,4,5-Tetrachlorobenzene
Concen: 2.483 ng/ul
RT: 12.25 min Scan# 1659
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
216	100		
214	86.0	60.9	91.3
179	21.1	19.0	28.4
108	24.3	16.2	24.4









#40
Hexachlorocyclopentadiene
Concen: 1.828 ng/ul
RT: 12.22 min Scan# 1654
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
237	100		
235	66.1	48.7	73.1
272	13.3	11.7	17.5




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

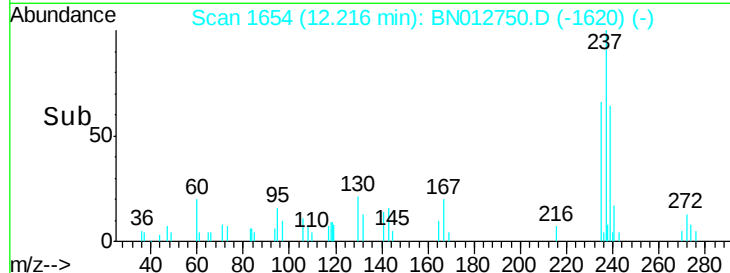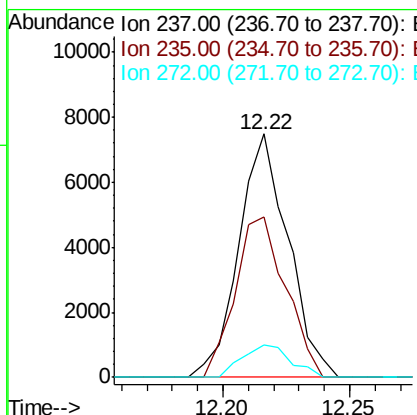

#41
2,4,6-Trichlorophenol
Concen: 2.135 ng/ul
RT: 12.49 min Scan# 1701
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
196	100		
198	97.5	67.0	100.4
200	26.4	25.0	37.4

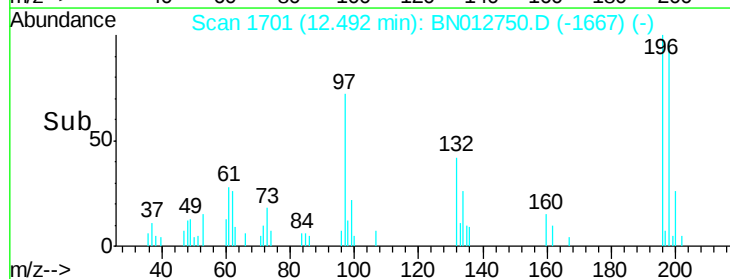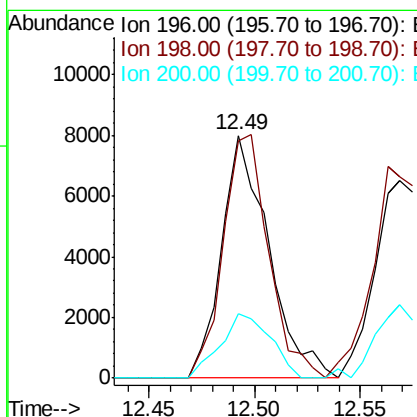







#42
 2,4,5-Trichlorophenol
 Concen: 1.992 ng/ul m
 RT: 12.57 min Scan# 1714
 Delta R.T. 0.01 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
196	100		
198	101.9	74.9	112.3
200	37.0	22.8	34.2




Manual Integrations
 APPROVED


mohammad
 11/30/2020 12:00:52 PM

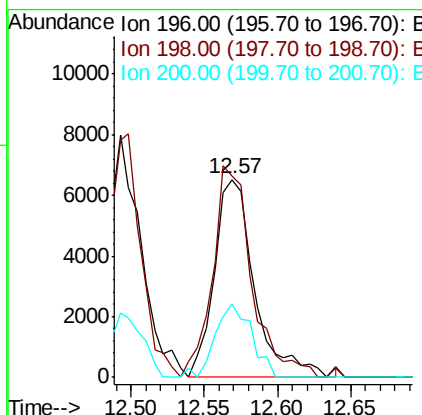

#43
 1,1'-Biphenyl
 Concen: 2.417 ng/ul
 RT: 12.90 min Scan# 1771
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
154	100		
153	36.7	33.8	50.8
76	10.6	11.0	16.6



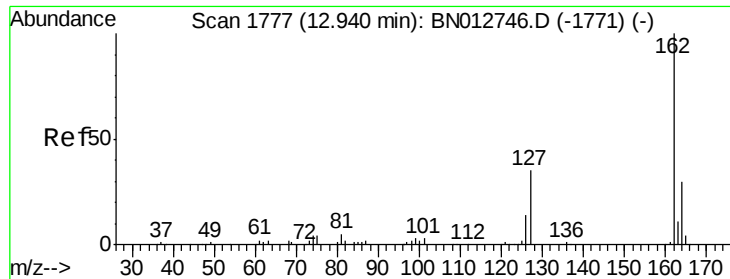





#44
 2-Chloronaphthalene
 Concen: 2.465 ng/ul
 RT: 12.94 min Scan# 1777
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
162	100		
164	27.6	26.8	40.2
127	47.5	35.0	52.4




Manual Integrations
 APPROVED


mohammad
 11/30/2020 12:00:52 PM

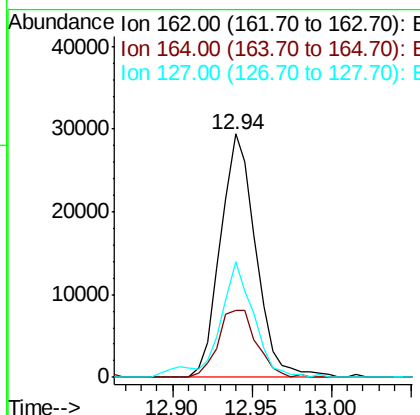

#45
 2-Nitroaniline
 Concen: 1.902 ng/ul
 RT: 13.16 min Scan# 1815
 Delta R.T. 0.01 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
65	100		
92	54.5	48.7	73.1
138	75.5	69.3	103.9

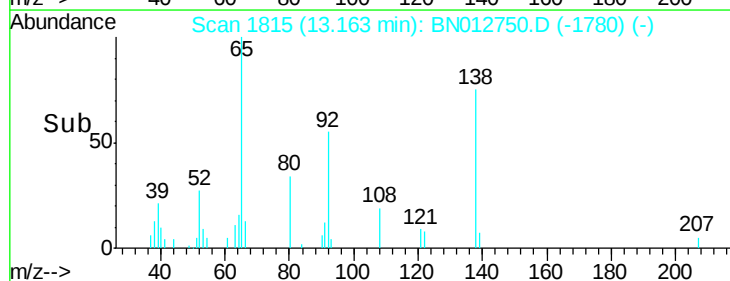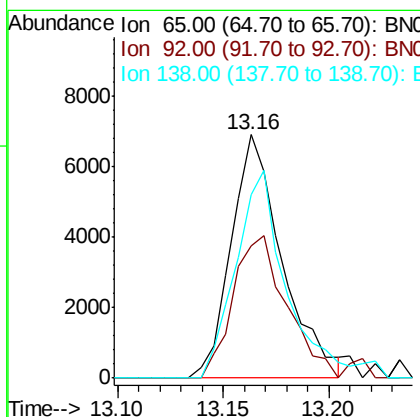

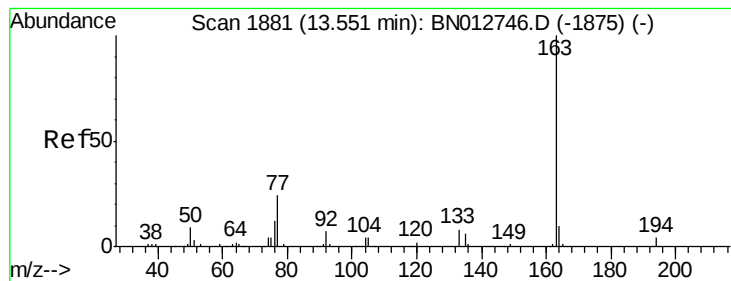

#47

Dimethylphthalate

Concen: 2.561 ng/ul

RT: 13.55 min Scan# 1881

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion:	163	Resp:	61613
Ion Ratio	Lower	Upper	
163	100		
194	4.6	3.1	4.7
164	10.8	7.8	11.6

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

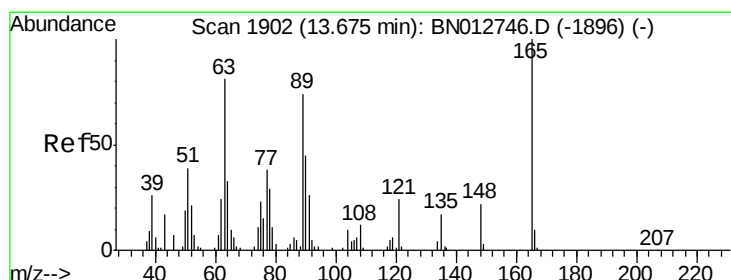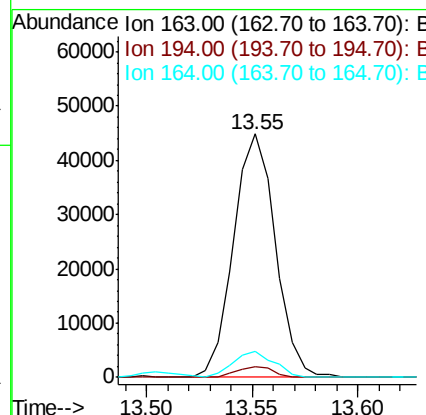

#48

2,6-Dinitrotoluene

Concen: 2.104 ng/ul




RT: 13.67 min Scan# 1902


Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion:	165	Resp:	10016
Ion Ratio	Lower	Upper	
165	100		
89	82.6	60.0	90.0
121	21.5	19.1	28.7

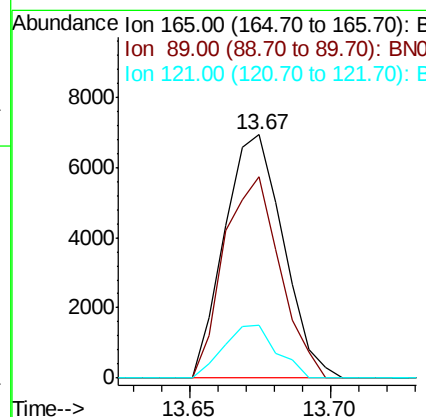







#50
Acenaphthylene
Concen: 2.506 ng/ul
RT: 13.80 min Scan# 1923
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion:152	Resp:	70588
Ion Ratio	Lower	Upper
152 100		
151 20.3	17.8	26.6
153 16.1	10.8	16.2




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

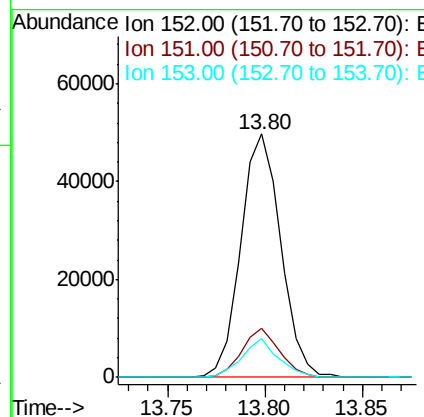

#51
3-Nitroaniline
Concen: 2.023 ng/ul
RT: 14.01 min Scan# 1959
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion:138	Resp:	7868
Ion Ratio	Lower	Upper
138 100		
108 8.8	8.9	13.3#
92 112.6	98.0	147.0

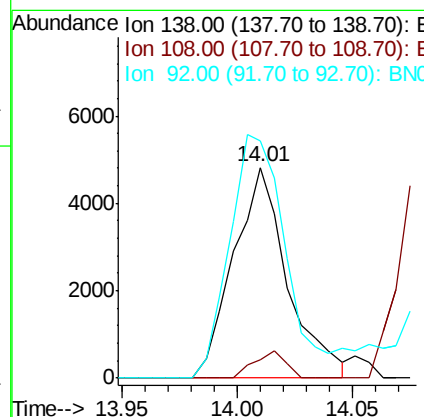



#52

Acenaphthene

Concen: 2.438 ng/ul

RT: 14.15 min Scan# 1982

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N


ClientSampleId :

MDL-WATER-05




Tot Ion:	153	Resp:	50287
Ion Ratio	Lower	Upper	
153	100		
152	46.4	36.2	54.4
154	95.2	65.4	98.0

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

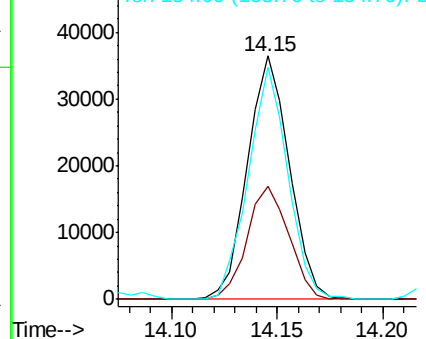

#53

2,4-Dinitrophenol

Concen: 1.116 ng/ul


RT: 14.22 min Scan# 1995

Delta R.T. 0.01 min



Lab File: BN012750.D


Acq: 27 Nov 2020 13:07

Tgt Ion:	184	Resp:	3284
Ion Ratio	Lower	Upper	
184	100		
63	76.6	72.7	109.1
154	61.0	50.6	76.0



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 63.00 (62.70 to 63.70): BNO
Ion 154.00 (153.70 to 154.70): E

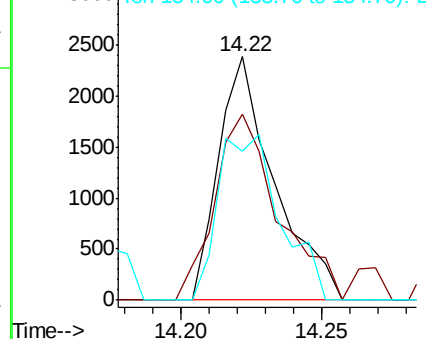







#55
4-Nitrophenol
Concen: 2.569 ng/ul
RT: 14.32 min Scan# 2011
Delta R.T. -0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
109	100		
139	84.1	87.8	131.8#
65	161.3	106.6	160.0#




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

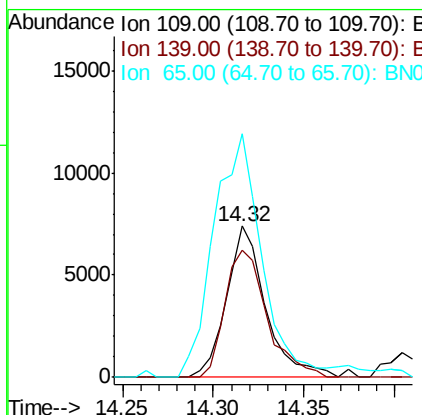

#56
Dibenzofuran
Concen: 2.519 ng/ul
RT: 14.49 min Scan# 2040
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
168	100		
139	40.4	32.5	48.7






#57
2,4-Dinitrotoluene
Concen: 2.124 ng/ul
RT: 14.47 min Scan# 2037
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05




Tot Ion	Ratio	Lower	Upper
165	100		
63	88.0	49.8	74.8#
182	0.0	2.3	3.5#

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM






Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BNO
Ion 182.00 (181.70 to 182.70): E

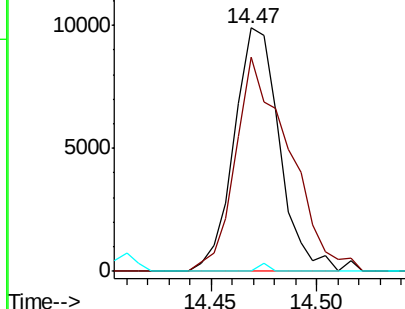


#58
2,3,4,6-Tetrachlorophenol
Concen: 2.135 ng/ul
RT: 14.72 min Scan# 2080
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
232	100		
131	52.3	43.1	64.7
130	0.0	2.7	4.1#
166	28.8	27.8	41.6

Abundance Ion 232.00 (231.70 to 232.70): E
Ion 131.00 (130.70 to 131.70): E
Ion 130.00 (129.70 to 130.70): E
Ion 166.00 (165.70 to 166.70): E

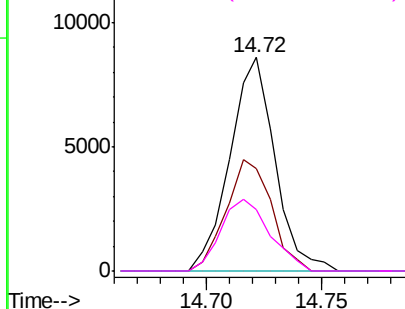







#59
Diethylphthalate
Concen: 2.502 ng/ul
RT: 14.93 min Scan# 2116
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleID :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
149	100		
177	20.2	18.4	27.6
150	12.3	10.3	15.5




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

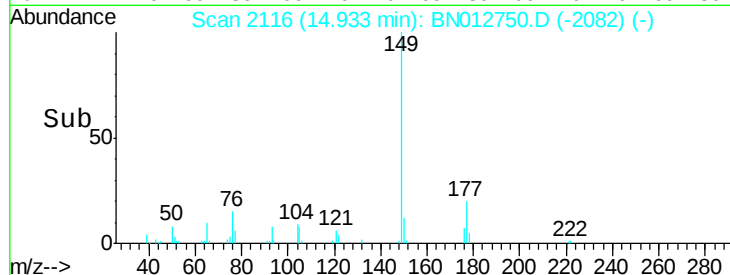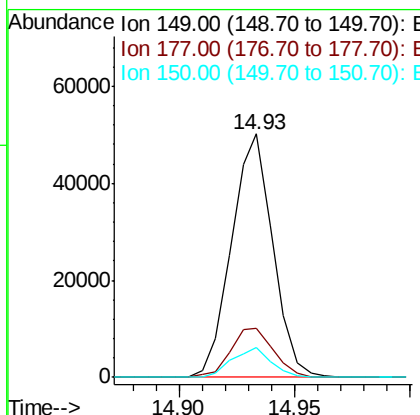

#61
Fluorene
Concen: 2.550 ng/ul
RT: 15.14 min Scan# 2151
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
166	100		
165	89.1	71.8	107.8
167	11.3	10.2	15.2

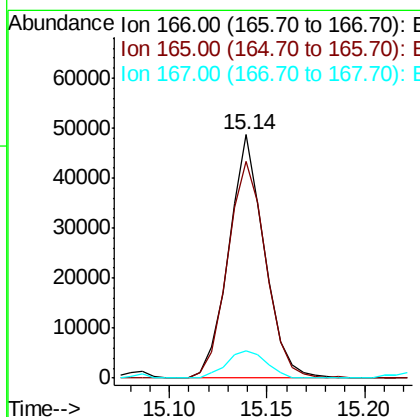

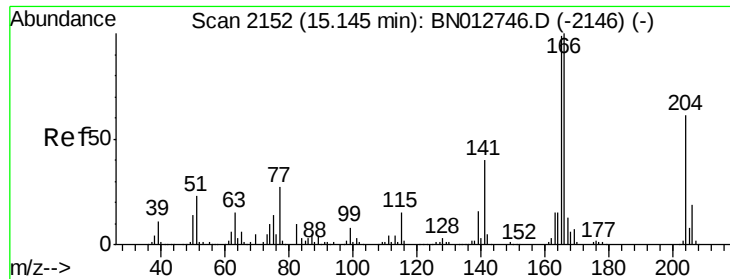





#62
 4-Chlorophenyl-phenylether
 Concen: 2.469 ng/ul
 RT: 15.15 min Scan# 2152
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
204	100		
206	30.1	25.3	37.9
141	65.0	53.0	79.4




Manual Integrations
 APPROVED


mohammad
 11/30/2020 12:00:52 PM

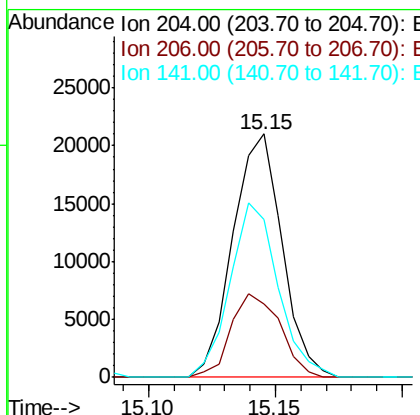

#63
 4-Nitroaniline
 Concen: 2.597 ng/ul m
 RT: 15.18 min Scan# 2158
 Delta R.T. 0.01 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
138	100		
92	71.8	47.0	70.4#
108	97.0	78.2	117.4

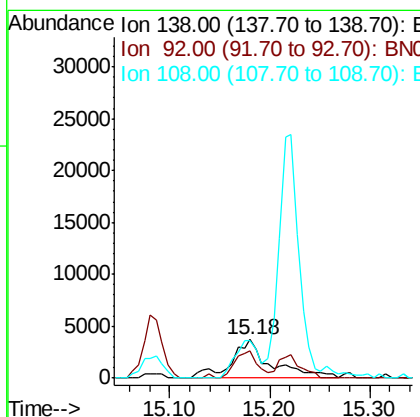




#66
 4,6-Dinitro-2-methylphenol
 Concen: 2.273 ng/ul
 RT: 15.23 min Scan# 2167
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Resp	Lower	Upper
198	100			
182	11.3	4.2	6.2	
77	66.7	26.6	39.8	

Manual Integrations
 APPROVED

mohammad
 11/30/2020 12:00:52 PM






Abundance

Ion 198.00 (197.70 to 198.70): E


Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): BNC

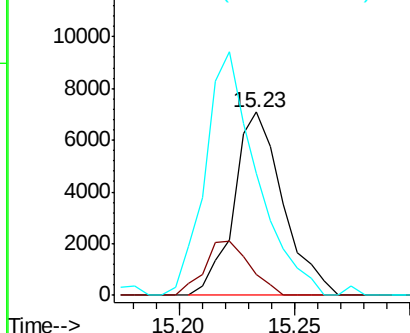

#67
 N-Nitrosodiphenylamine
 Concen: 2.307 ng/ul
 RT: 15.36 min Scan# 2188
 Delta R.T. -0.01 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Resp	Lower	Upper
169	100			
168	66.5	54.2	81.2	
167	37.2	28.0	42.0	






Abundance

Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

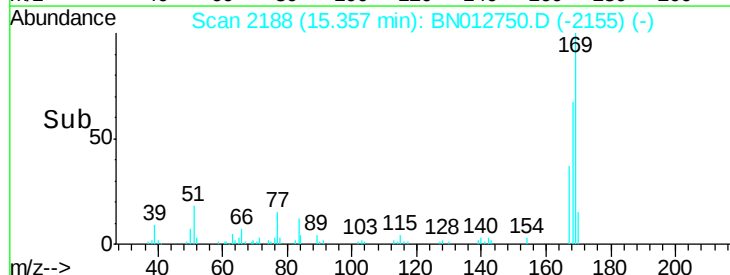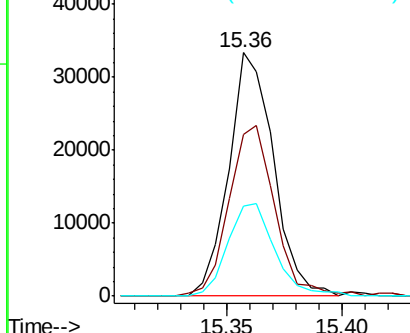




#68
4-Bromophenyl-phenylether
Concen: 2.465 ng/ul
RT: 16.04 min Scan# 2304
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
248	100		
250	101.5	78.6	118.0
141	97.1	66.5	99.7

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM






Abundance

Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

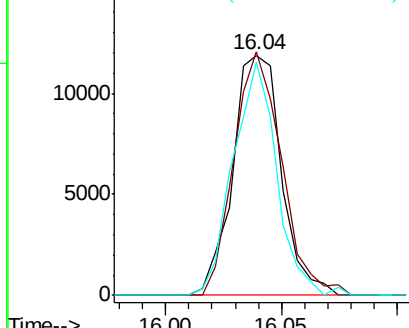

#69
Hexachlorobenzene
Concen: 2.588 ng/ul
RT: 16.14 min Scan# 2321
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07




Tgt Ion	Ratio	Lower	Upper
284	100		
142	36.7	33.7	50.5
249	28.3	26.8	40.2


Abundance

Ion 284.00 (283.70 to 284.70): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

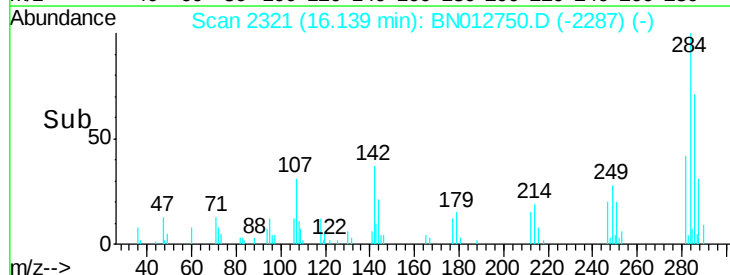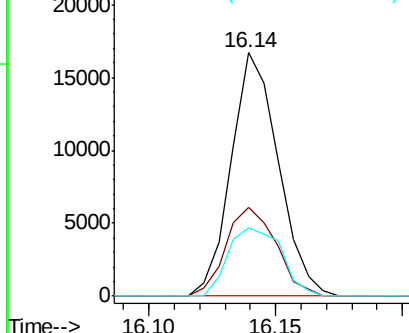

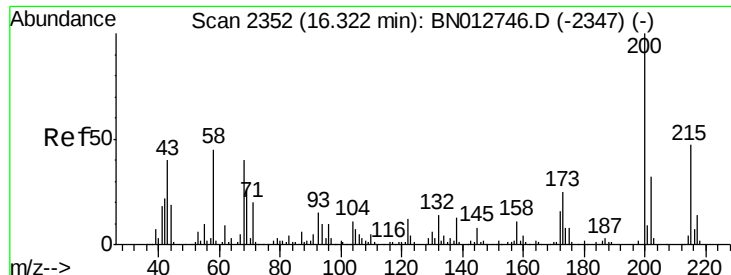





#70
Atrazine
Concen: 2.017 ng/ul
RT: 16.32 min Scan# 2352
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
200	100		
173	27.3	21.8	32.8
215	43.4	35.8	53.8




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

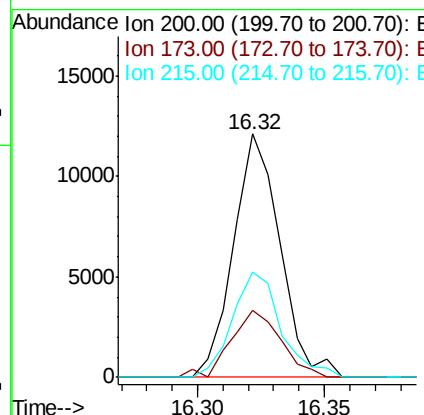

#71
Pentachlorophenol
Concen: 1.690 ng/ul
RT: 16.49 min Scan# 2381
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
266	100		
264	79.1	51.4	77.2#
268	58.4	48.7	73.1

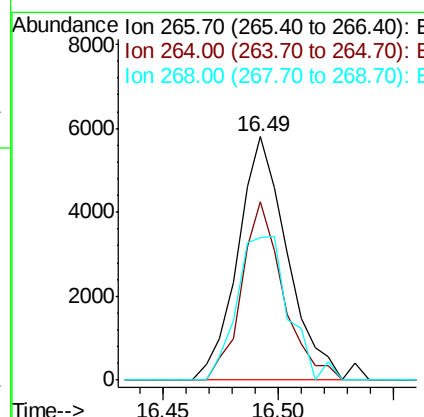



#72

Phenanthrene

Concen: 2.552 ng/ul m

RT: 16.88 min Scan# 2447

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
178	100		
179	11.7	12.0	18.0#
176	16.4	14.4	21.6

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

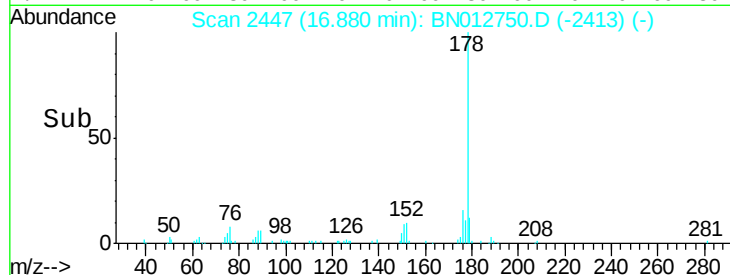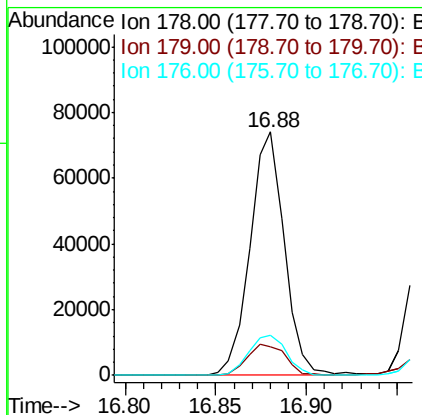

#74

Anthracene

Concen: 2.579 ng/ul




RT: 16.97 min Scan# 2462


Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
178	100		
179	14.9	11.8	17.8
176	15.2	15.4	23.0#

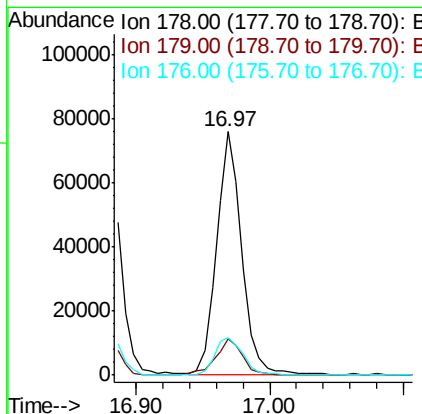



#75

1,2,3,4-Tetrachlorobenzene

Concen: 2.491 ng/uL

RT: 12.86 min Scan# 1764

Delta R.T. 0.01 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N


ClientSampleId :

MDL-WATER-05




Tot Ion:	216	Resp:	22458
Ion Ratio	Lower	Upper	
216	100		
214	77.4	65.6	98.4
218	50.0	39.8	59.8

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM



Abundance Ion 216.00 (215.70 to 216.70): E
Ion 214.00 (213.70 to 214.70): E
Ion 218.00 (217.70 to 218.70): E

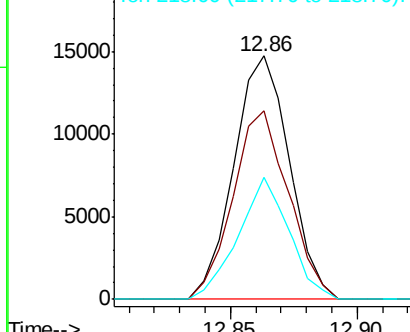

#76

Pentachlorobenzene

Concen: 2.545 ng/uL


RT: 14.40 min Scan# 2026

Delta R.T. -0.00 min



Lab File: BN012750.D


Acq: 27 Nov 2020 13:07

Tgt Ion:	250	Resp:	24284
Ion Ratio	Lower	Upper	
250	100		
248	56.3	46.6	69.8
252	55.8	50.6	76.0



Abundance Ion 250.00 (249.70 to 250.70): E
Ion 248.00 (247.70 to 248.70): E
Ion 252.00 (251.70 to 252.70): E

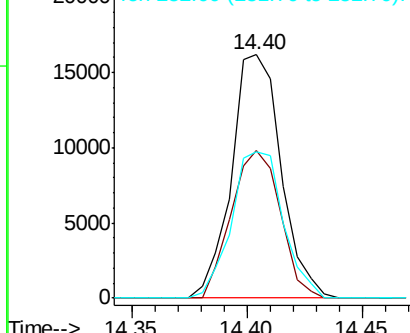







#77
 Carbazole
 Concen: 2.061 ng/ul
 RT: 17.25 min Scan# 2510
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Instrument :
 BNA_N
 ClientSampleId :
 MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
167	100		
166	21.2	17.8	26.6
139	11.9	11.0	16.6




Manual Integrations
 APPROVED


mohammad
 11/30/2020 12:00:52 PM

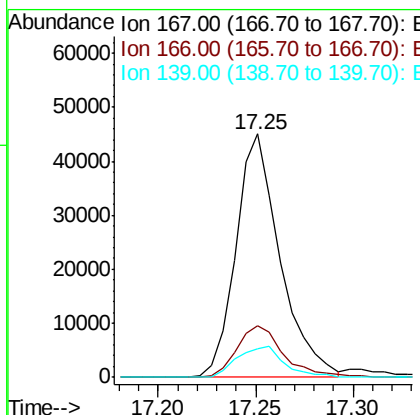

#78
 Di-n-butylphthalate
 Concen: 2.046 ng/ul
 RT: 17.83 min Scan# 2608
 Delta R.T. -0.00 min
 Lab File: BN012750.D
 Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
149	100		
150	9.9	7.4	11.0
104	5.9	4.8	7.2

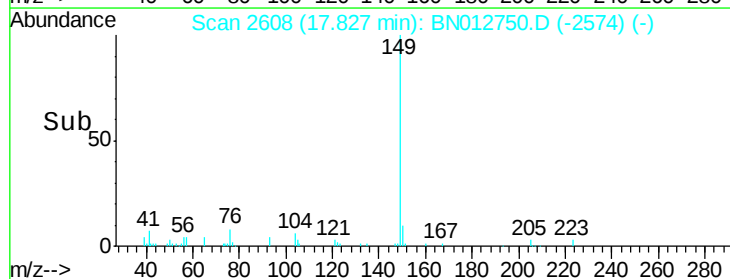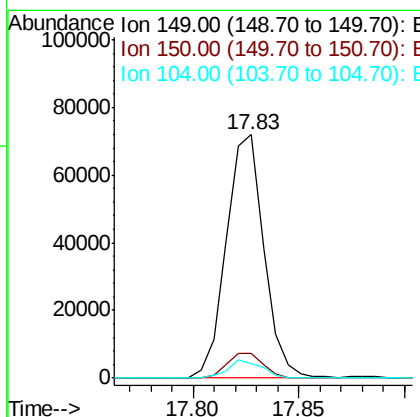







#80
Fluoranthene
Concen: 2.392 ng/ul
RT: 18.91 min Scan# 2792
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	8.2	8.5	12.7#
100	8.3	6.6	10.0




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

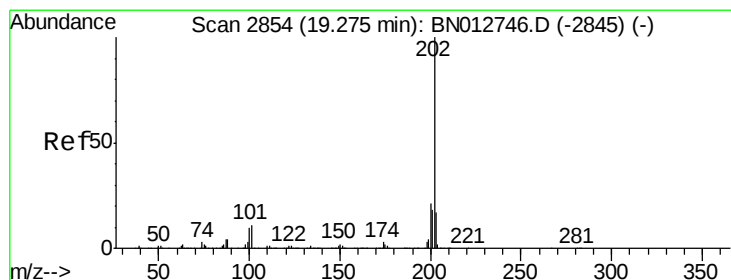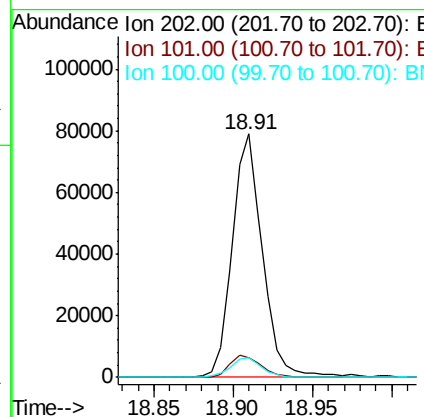

#82
Pyrene
Concen: 2.615 ng/ul
RT: 19.27 min Scan# 2854
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Resp Lower	Upper
202	100		
101	11.6	10.1	15.1
100	10.1	8.6	13.0

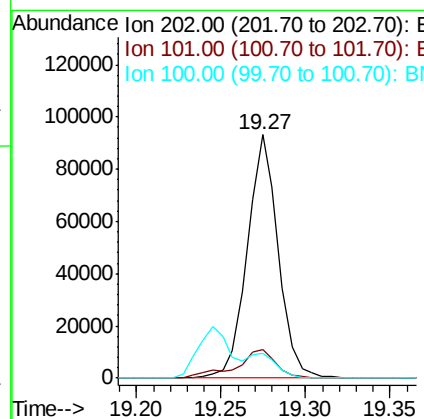







#83
Butylbenzylphthalate
Concen: 1.897 ng/ul
RT: 20.20 min Scan# 3012
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
149	100		
91	76.1	60.5	90.7
206	18.3	16.2	24.4




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM



#84
3,3'-Dichlorobenzidine
Concen: 1.962 ng/ul
RT: 20.99 min Scan# 3145
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
252	100		
254	59.6	49.7	74.5
126	13.8	8.6	13.0





#85

Benzo(a)anthracene

Concen: 2.411 ng/ul

RT: 21.04 min Scan# 3154

Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Instrument :

BNA_N





ClientSampleId :

MDL-WATER-05

Tot Ion:	228	Resp:	106937
Ion Ratio	Lower	Upper	
228	100		
229	18.0	15.6	23.4
226	23.0	22.9	34.3

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

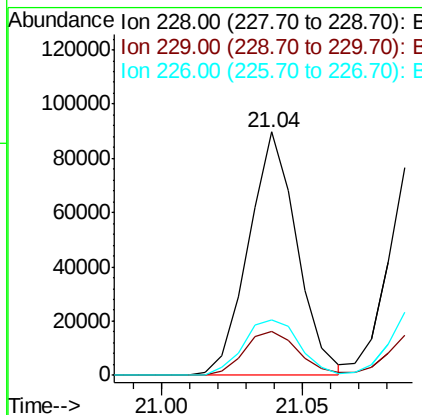

#86

Bis(2-ethylhexyl)phthalate

Concen: 1.778 ng/ul




RT: 20.99 min Scan# 3146


Delta R.T. -0.00 min

Lab File: BN012750.D

Acq: 27 Nov 2020 13:07

Tgt Ion:	149	Resp:	55801
Ion Ratio	Lower	Upper	
149	100		
167	27.4	20.7	31.1
279	5.0	3.1	4.7#









#87
Chrysene
Concen: 2.542 ng/ul
RT: 21.09 min Scan# 3163
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.0	23.8	35.6
229	18.1	15.1	22.7




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

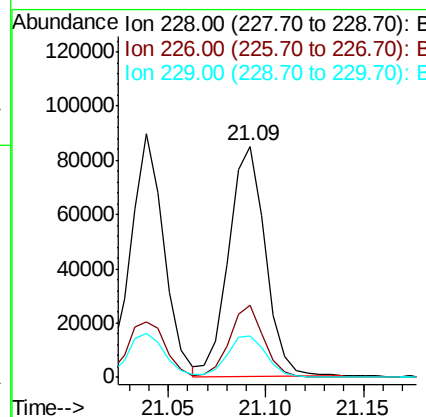

#89
Di-n-octyl phthalate
Concen: 1.668 ng/ul
RT: 21.84 min Scan# 3291
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion:149 Resp: 96183

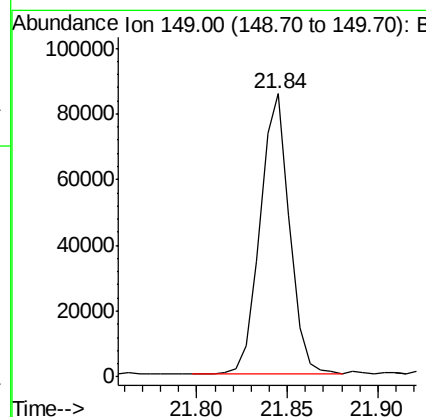







#90
Benzo(b)fluoranthene
Concen: 2.429 ng/ul
RT: 22.54 min Scan# 3410
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.9	17.7	26.5
125	8.8	7.6	11.4




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM



#91
Benzo(k)fluoranthene
Concen: 2.450 ng/ul m
RT: 22.58 min Scan# 3416
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
252	100		
253	19.1	17.4	26.2
125	7.4	7.8	11.8#









#93
Benzo(a)pyrene
Concen: 2.614 ng/uL
RT: 23.07 min Scan# 3500
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.5	16.1	24.1
125	10.1	7.4	11.0




Manual Integrations
APPROVED


mohammad
11/30/2020 12:00:52 PM

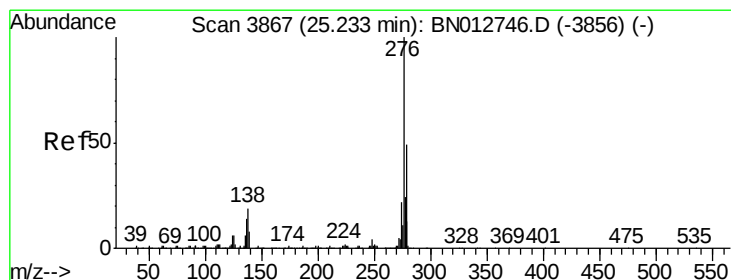

#94
Indeno(1,2,3-cd)pyrene
Concen: 2.499 ng/uL
RT: 25.24 min Scan# 3868
Delta R.T. 0.01 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
276	100		
138	20.0	16.3	24.5
277	24.0	17.7	26.5

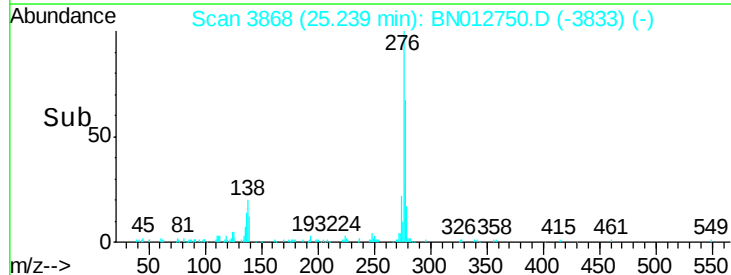

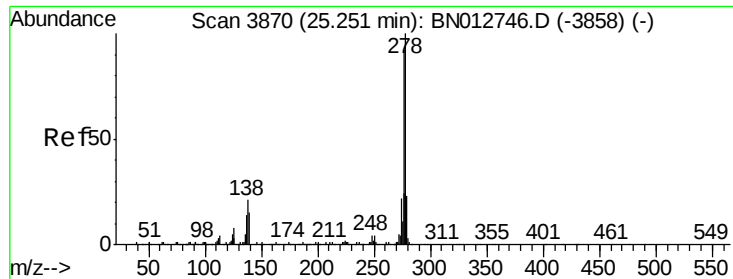





#95
Dibenzo(a,h)anthracene
Concen: 2.466 ng/ul
RT: 25.25 min Scan# 3870
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Instrument :
BNA_N
ClientSampleId :
MDL-WATER-05

Tot Ion	Ratio	Lower	Upper
278	100		
139	11.8	10.6	16.0
279	23.5	17.8	26.8

Manual Integrations
APPROVED

mohammad
11/30/2020 12:00:52 PM

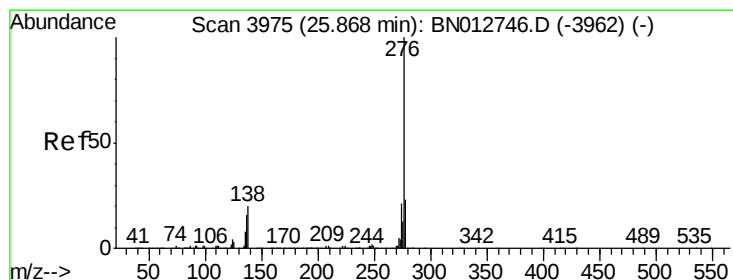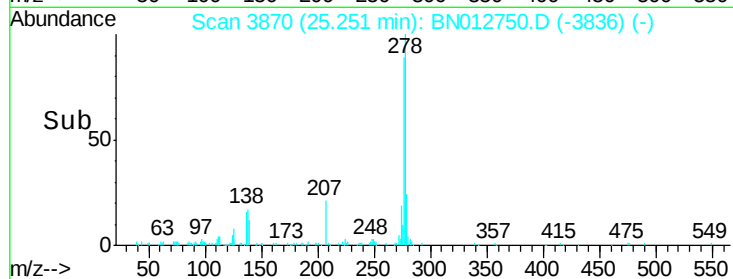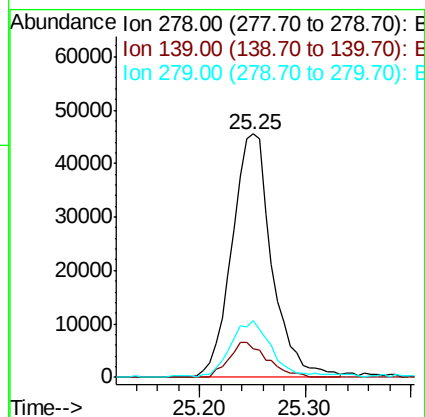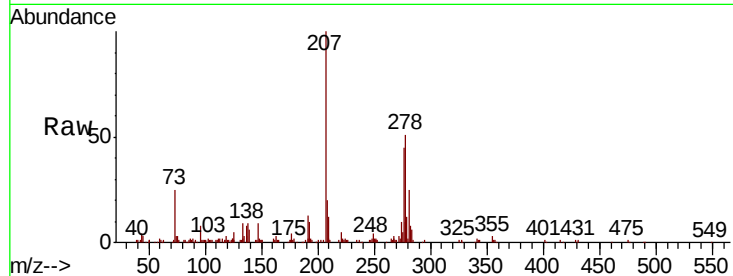

#96
Benzo(g,h,i)perylene
Concen: 2.393 ng/ul
RT: 25.87 min Scan# 3975
Delta R.T. -0.00 min
Lab File: BN012750.D
Acq: 27 Nov 2020 13:07

Tgt Ion	Ratio	Lower	Upper
276	100		
138	16.7	15.0	22.4
277	23.7	16.5	24.7

