

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
 Data File : BN035356.D
 Acq On : 27 Nov 2024 19:09
 Operator : RC/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Nov 27 22:54:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 27 22:48:24 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.308	152	2249	0.400	ng	0.00
7) Naphthalene-d8	10.052	136	5807	0.400	ng	0.00
13) Acenaphthene-d10	13.967	164	4363	0.400	ng	0.00
19) Phenanthrene-d10	16.723	188	10479	0.400	ng	#-0.01
29) Chrysene-d12	20.974	240	11520	0.400	ng	0.00
35) Perylene-d12	23.067	264	12000	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.968	112	26472	4.637	ng	0.00
5) Phenol-d6	6.513	99	34560	4.828	ng	0.00
8) Nitrobenzene-d5	8.440	82	18911	3.741	ng	0.00
11) 2-Methylnaphthalene-d10	11.656	152	47612	4.601	ng	0.00
14) 2,4,6-Tribromophenol	15.475	330	17905	5.689	ng	0.00
15) 2-Fluorobiphenyl	12.574	172	82401	4.650	ng	0.00
27) Fluoranthene-d10	18.785	212	152416	4.748	ng	0.00
31) Terphenyl-d14	19.412	244	110737	4.581	ng	0.00
Target Compounds						
2) 1,4-Dioxane	2.996	88	9786	4.790	ng	99
3) n-Nitrosodimethylamine	3.285	42	8681	4.560	ng	# 96
6) bis(2-Chloroethyl)ether	6.759	93	27872	5.187	ng	99
9) Naphthalene	10.105	128	77668	5.123	ng	97
10) Hexachlorobutadiene	10.404	225	17273	3.887	ng	# 100
12) 2-Methylnaphthalene	11.732	142	57698	5.158	ng	98
16) Acenaphthylene	13.679	152	97129	5.209	ng	99
17) Acenaphthene	14.031	154	62170	5.088	ng	98
18) Fluorene	15.026	166	88648	4.932	ng	99
20) 4,6-Dinitro-2-methylph...	15.122	198	9239	4.235	ng	# 55
21) 4-Bromophenyl-phenylether	15.941	248	31947	4.785	ng	# 94
22) Hexachlorobenzene	16.040	284	36315	5.241	ng	100
23) Atrazine	16.227	200	25034	4.179	ng	96
24) Pentachlorophenol	16.388	266	19691	6.083	ng	86
25) Phenanthrene	16.773	178	147357	5.343	ng	100
26) Anthracene	16.860	178	139399	5.503	ng	99
28) Fluoranthene	18.812	202	199850	5.270	ng	99
30) Pyrene	19.179	202	206018	5.370	ng	100
32) Benzo(a)anthracene	20.956	228	205712	5.128	ng	99
33) Chrysene	21.009	228	204475	5.146	ng	99
34) Bis(2-ethylhexyl)phtha...	20.938	149	78322	3.721	ng	99
36) Indeno(1,2,3-cd)pyrene	25.108	276	252709	5.279	ng	99
37) Benzo(b)fluoranthene	22.456	252	241201	5.974	ng	# 94
38) Benzo(k)fluoranthene	22.497	252	220146	5.449	ng	# 93
39) Benzo(a)pyrene	22.977	252	190665	5.367	ng	# 92
40) Dibenzo(a,h)anthracene	25.126	278	199852	5.269	ng	96
41) Benzo(g,h,i)perylene	25.725	276	209119	5.183	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035356.D
Acq On : 27 Nov 2024 19:09
Operator : RC/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Nov 27 22:54:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 22:48:24 2024
Response via : Initial Calibration

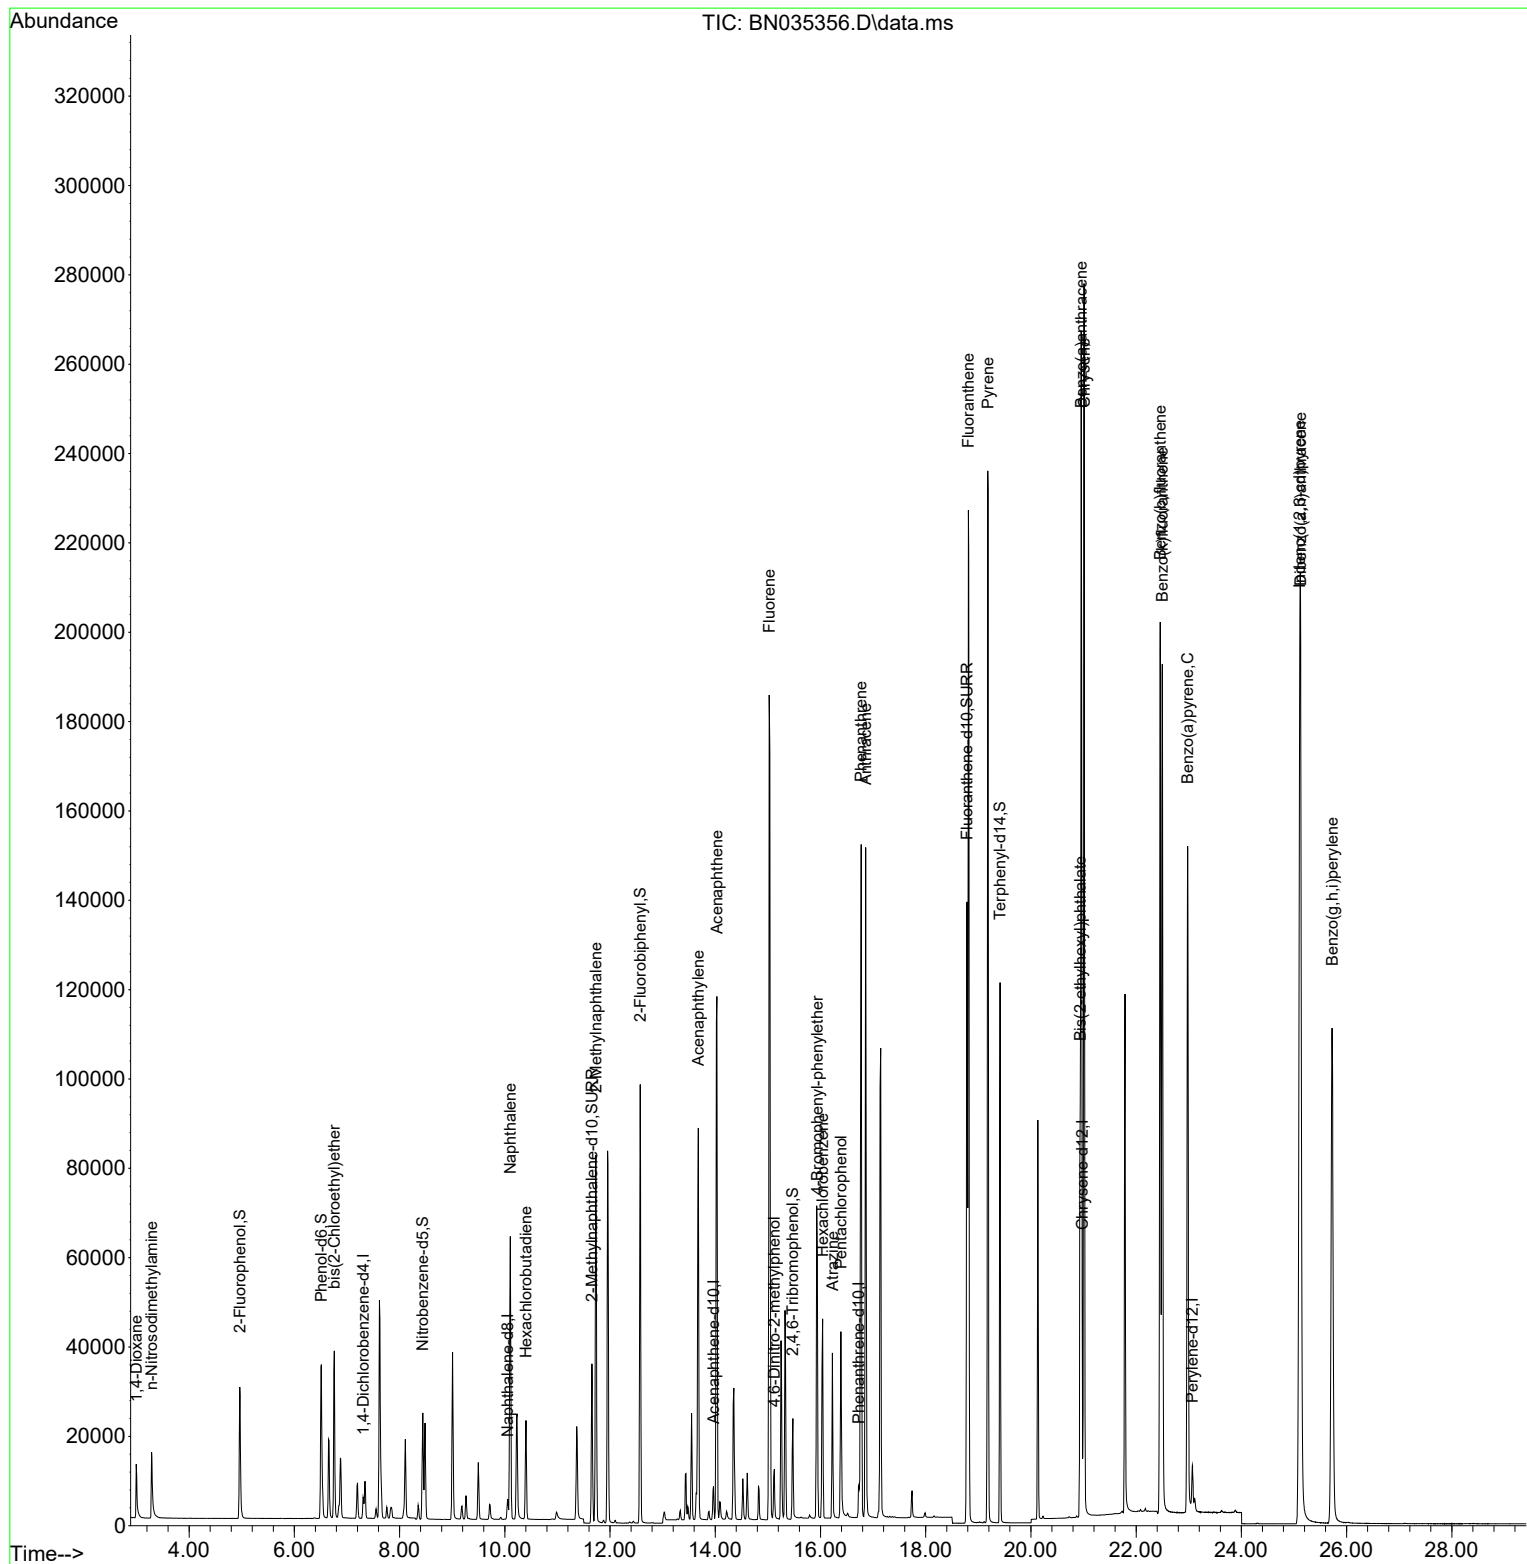





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.308 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0







Tgt Ion:152 Resp: 2249
 Ion Ratio Lower Upper
 152 100
 150 152.9 124.0 186.0
 115 61.0 49.6 74.4

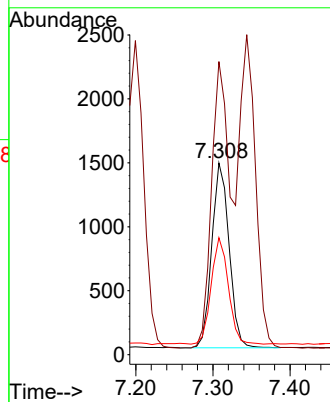

#2
 1,4-Dioxane
 Concen: 4.790 ng
 RT: 2.996 min Scan# 16
 Delta R.T. -0.007 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Tgt Ion: 88 Resp: 9786
 Ion Ratio Lower Upper
 88 100
 43 20.5 17.2 25.8
 58 54.8 44.5 66.7


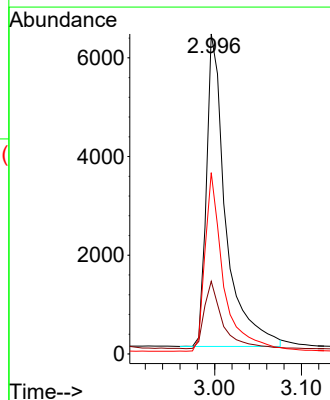






#3
n-Nitrosodimethylamine
Concen: 4.560 ng
RT: 3.285 min Scan# 50
Delta R.T. -0.007 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 42 Resp: 8681
Ion Ratio Lower Upper
42 100
74 161.2 124.9 187.3
44 6.7 2.2 3.4#



#4
2-Fluorophenol
Concen: 4.637 ng
RT: 4.968 min Scan# 289
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion: 112 Resp: 26472
Ion Ratio Lower Upper
112 100
64 50.0 39.8 59.8
63 27.4 21.0 31.6


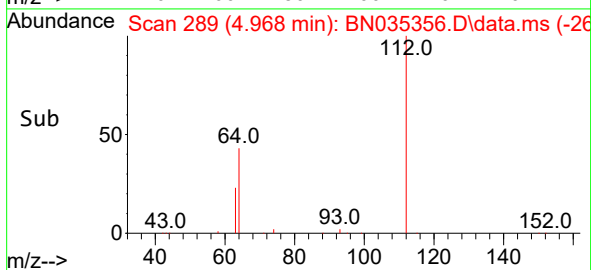






#5
Phenol-d6
Concen: 4.828 ng
RT: 6.513 min Scan# 503
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 34560
Ion Ratio Lower Upper
99 100
42 14.1 11.4 17.2
71 36.4 29.3 43.9

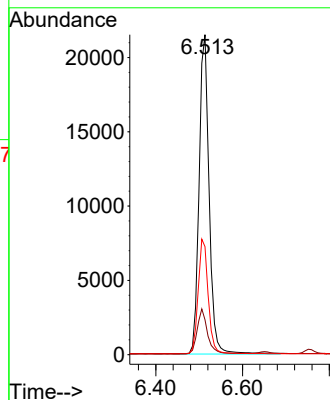

#6
bis(2-Chloroethyl)ether
Concen: 5.187 ng
RT: 6.759 min Scan# 537
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion: 93 Resp: 27872
Ion Ratio Lower Upper
93 100
63 63.7 50.4 75.6
95 32.1 25.7 38.5



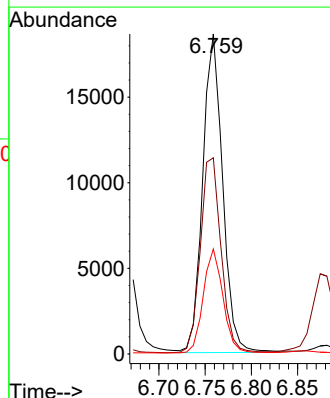





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.052 min Scan# 915
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	5807
Ion	Ratio	Lower	Upper
136	100		
137	12.4	10.2	15.2
54	7.1	6.1	9.1
68	7.1	6.4	9.6

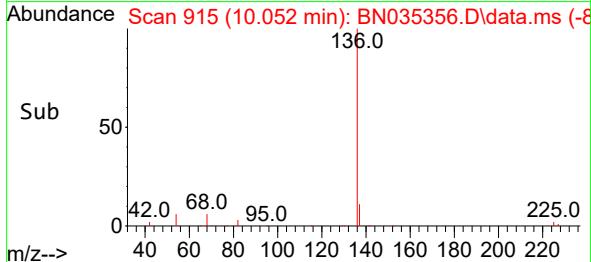

#8
Nitrobenzene-d5
Concen: 3.741 ng
RT: 8.440 min Scan# 764
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:	82	Resp:	18911
Ion	Ratio	Lower	Upper
82	100		
128	40.4	33.4	50.0
54	39.4	36.7	55.1









#9
Naphthalene
Concen: 5.123 ng
RT: 10.105 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 77668
Ion Ratio Lower Upper
128 100
129 10.9 9.8 14.6
127 13.4 11.4 17.2



#10
Hexachlorobutadiene
Concen: 3.887 ng
RT: 10.404 min Scan# 948
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:225 Resp: 17273
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 51.3 76.9





#11

2-Methylnaphthalene-d10

Concen: 4.601 ng

RT: 11.656 min Scan# 1081

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :





SSTDICC5.0

Tgt Ion:152 Resp: 47612

Ion Ratio Lower Upper

152 100

151 20.8 16.6 25.0

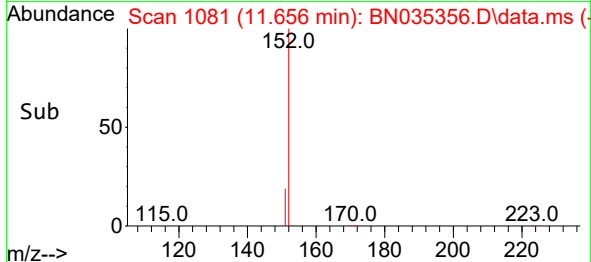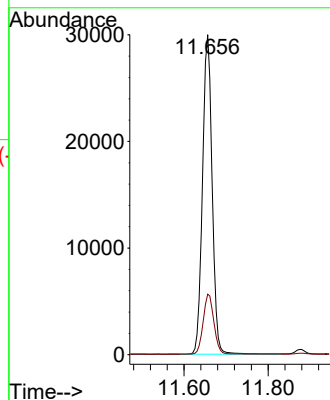

#12

2-Methylnaphthalene

Concen: 5.158 ng

RT: 11.732 min Scan# 1096

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:142 Resp: 57698


Ion Ratio Lower Upper

142 100

141 88.8 72.2 108.4

115 37.6 31.4 47.0

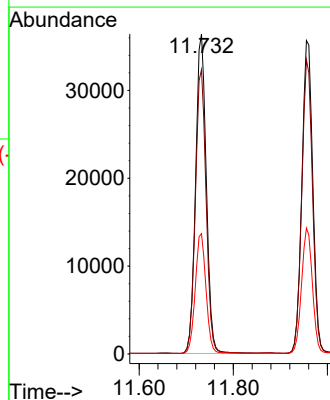



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 13.967 min Scan# 14

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:164 Resp: 4363

Ion Ratio Lower Upper

164 100

162 102.2 82.2 123.2

160 48.4 40.1 60.1

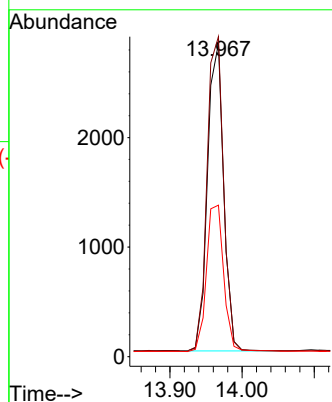

#14

2,4,6-Tribromophenol

Concen: 5.689 ng

RT: 15.475 min Scan# 1578

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:330 Resp: 17905


Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 33.4 26.6 40.0


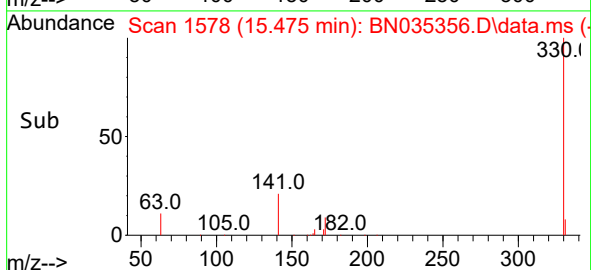






#15
2-Fluorobiphenyl
Concen: 4.650 ng
RT: 12.574 min Scan# 1262
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.9	29.0	43.4
170	23.0	19.8	29.8

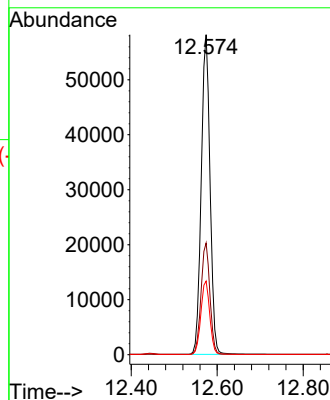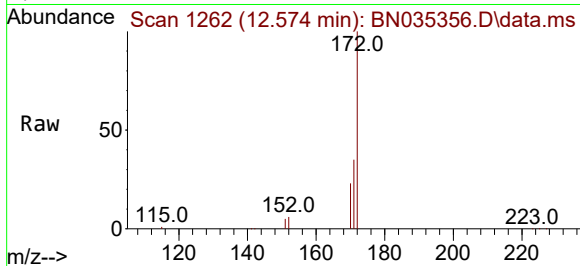

#16
Acenaphthylene
Concen: 5.209 ng
RT: 13.679 min Scan# 1410
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.2	24.2
153	12.9	10.4	15.6

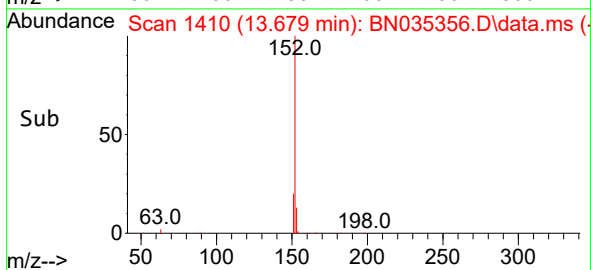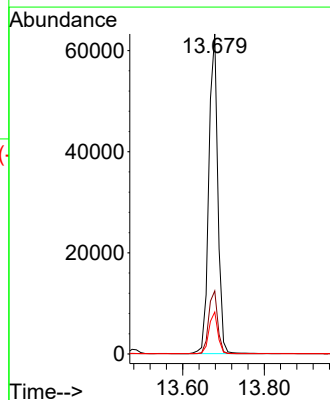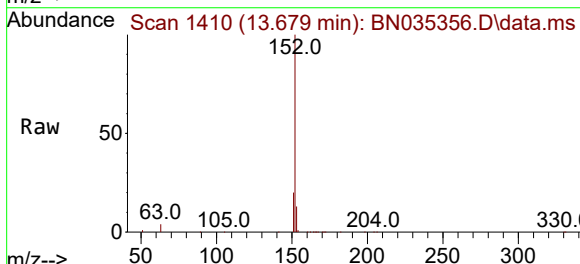



#17

Acenaphthene

Concen: 5.088 ng

RT: 14.031 min Scan# 1443

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:154 Resp: 62170

Ion Ratio Lower Upper

154 100

153 114.7 92.6 139.0

152 58.1 49.0 73.6

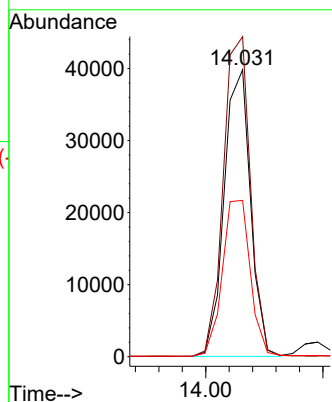

#18

Fluorene

Concen: 4.932 ng

RT: 15.026 min Scan# 1536

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:166 Resp: 88648


Ion Ratio Lower Upper

166 100

165 98.5 79.7 119.5

167 13.4 10.8 16.2

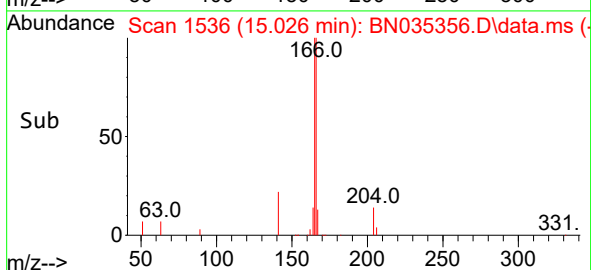



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 16.723 min Scan# 1

Delta R.T. -0.012 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:188 Resp: 10479

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 11.9 4.6 6.8#



#20

4,6-Dinitro-2-methylphenol

Concen: 4.235 ng

RT: 15.122 min Scan# 1545

Delta R.T. -0.011 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:198 Resp: 9239


Ion Ratio Lower Upper

198 100

51 18.7 46.5 69.7#

105 29.0 45.3 67.9#









#21
4-Bromophenyl-phenylether
Concen: 4.785 ng
RT: 15.941 min Scan# 1616
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 31947
Ion Ratio Lower Upper
248 100
250 103.5 80.6 120.8
141 30.8 31.5 47.3#

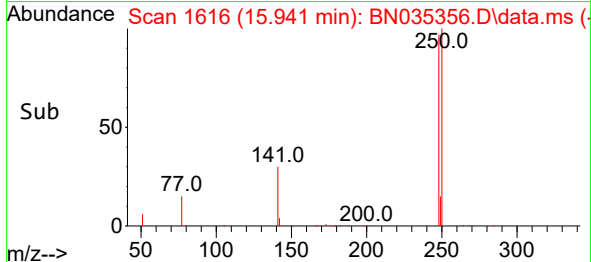

#22
Hexachlorobenzene
Concen: 5.241 ng
RT: 16.040 min Scan# 1624
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:284 Resp: 36315
Ion Ratio Lower Upper
284 100
142 33.4 26.7 40.1
249 30.4 24.6 36.8





#23

Atrazine

Concen: 4.179 ng

RT: 16.227 min Scan# 1639

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:200 Resp: 25034

Ion Ratio Lower Upper

200 100

173 25.7 24.1 36.1

215 45.2 36.9 55.3

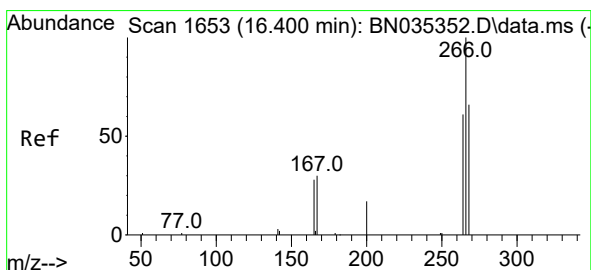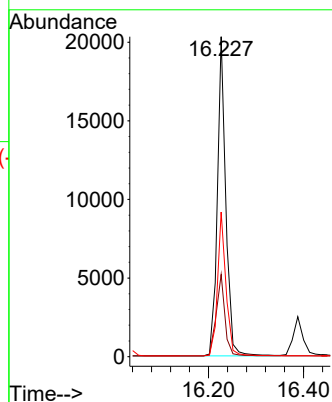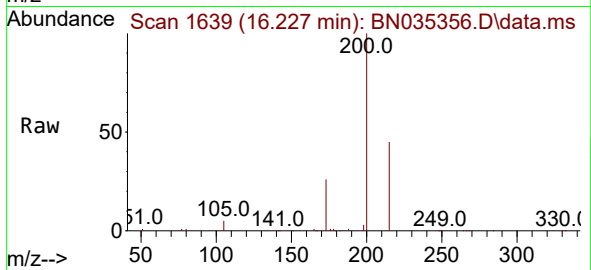

#24

Pentachlorophenol

Concen: 6.083 ng

RT: 16.388 min Scan# 1652

Delta R.T. -0.012 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:266 Resp: 19691


Ion Ratio Lower Upper

266 100

264 62.6 42.3 63.5

268 64.1 43.3 64.9





#25

Phenanthrene

Concen: 5.343 ng

RT: 16.773 min Scan# 1683

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:178 Resp: 147357

Ion Ratio Lower Upper

178 100

176 19.4 15.4 23.2

179 15.2 12.3 18.5

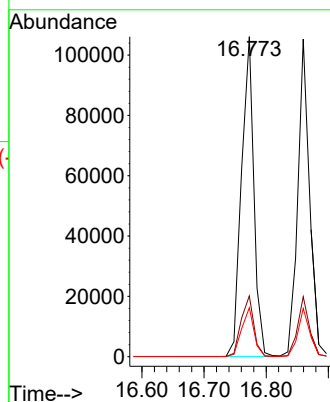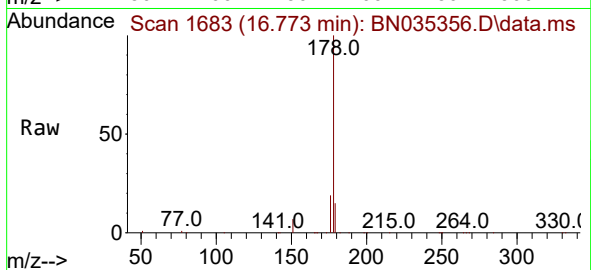

#26

Anthracene

Concen: 5.503 ng

RT: 16.860 min Scan# 1690

Delta R.T. 0.000 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:178 Resp: 139399


Ion Ratio Lower Upper

178 100

176 18.7 15.0 22.6

179 15.1 12.6 18.8


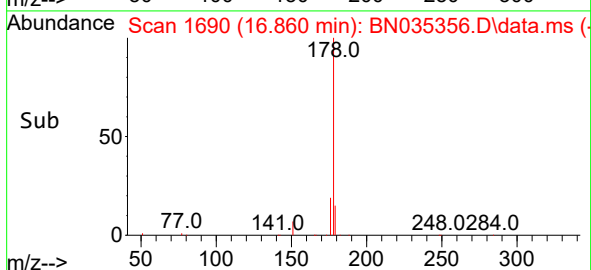
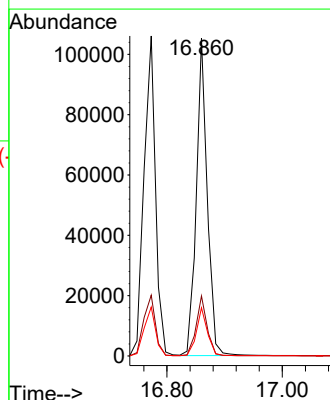





#27
Fluoranthene-d10
Concen: 4.748 ng
RT: 18.785 min Scan# 1882
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 152416
Ion Ratio Lower Upper
212 100
106 11.5 9.2 13.8
104 6.5 5.3 7.9

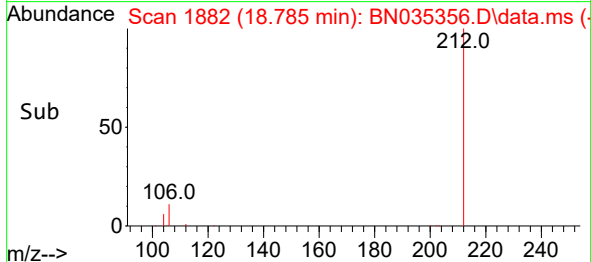

#28
Fluoranthene
Concen: 5.270 ng
RT: 18.812 min Scan# 1888
Delta R.T. -0.005 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:202 Resp: 199850
Ion Ratio Lower Upper
202 100
101 9.1 7.4 11.0
203 17.4 13.7 20.5









#29
Chrysene-d12
Concen: 0.400 ng
RT: 20.974 min Scan# 21
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 11520
Ion Ratio Lower Upper
240 100
120 9.6 7.9 11.9
236 28.1 22.9 34.3



#30
Pyrene
Concen: 5.370 ng
RT: 19.179 min Scan# 1967
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:202 Resp: 206018
Ion Ratio Lower Upper
202 100
200 21.2 17.0 25.4
203 17.7 14.3 21.5







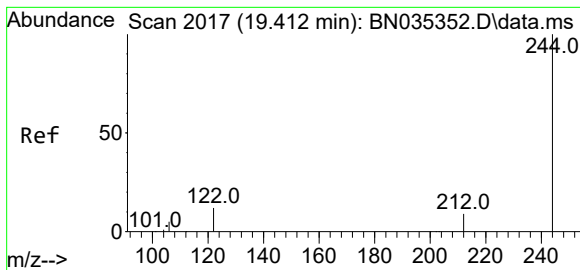

#31
 Terphenyl-d14
 Concen: 4.581 ng
 RT: 19.412 min Scan# 2017
 Delta R.T. 0.000 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	244	Resp:	110737
Ion Ratio	Lower	Upper	
244	100		
212	9.2	8.1	12.1
122	12.1	10.3	15.5

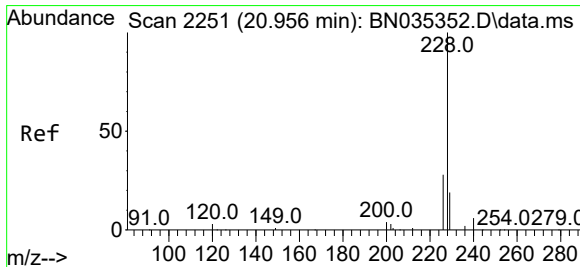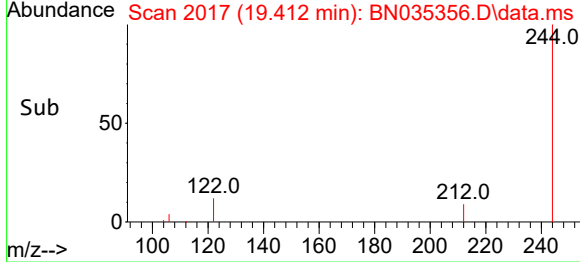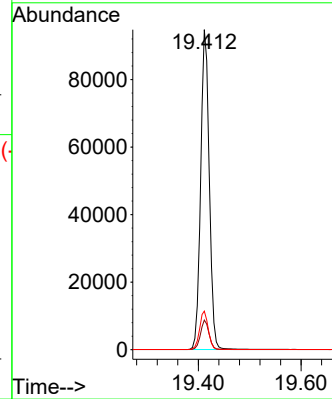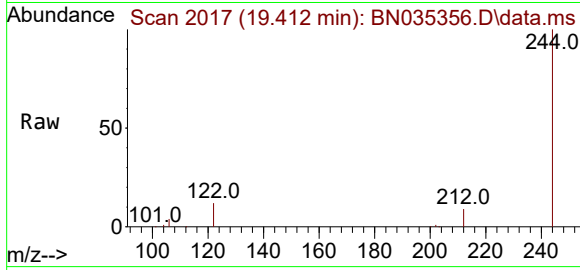

#32
 Benzo(a)anthracene
 Concen: 5.128 ng
 RT: 20.956 min Scan# 2251
 Delta R.T. 0.000 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Tgt Ion:	228	Resp:	205712
Ion Ratio	Lower	Upper	
228	100		
226	27.9	22.5	33.7
229	19.4	15.8	23.8

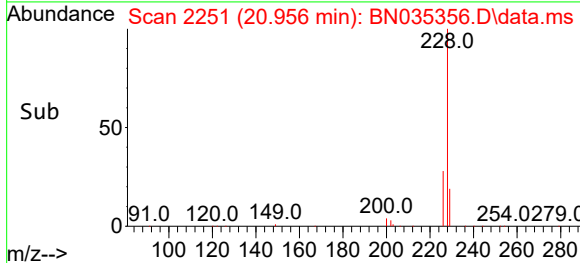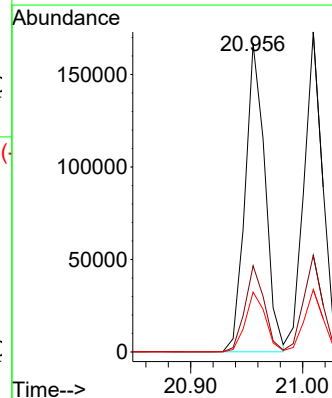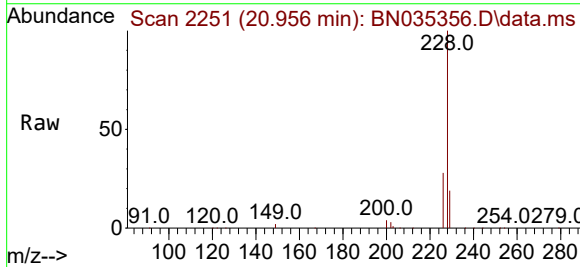




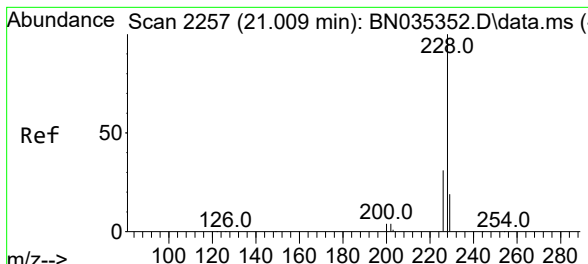


#33
 Chrysene
 Concen: 5.146 ng
 RT: 21.009 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:228 Resp: 204475




Ion	Ratio	Lower	Upper
228	100		
226	30.2	24.6	37.0
229	19.5	15.9	23.9

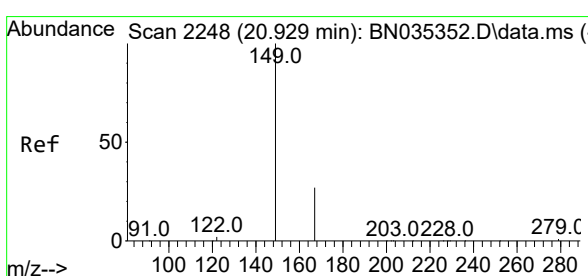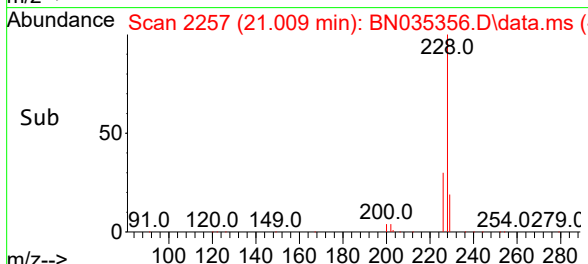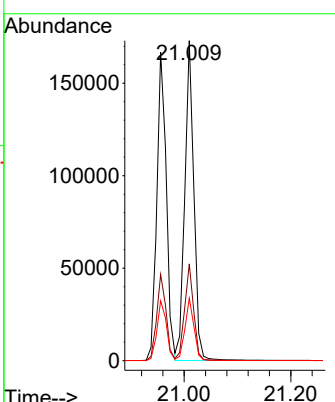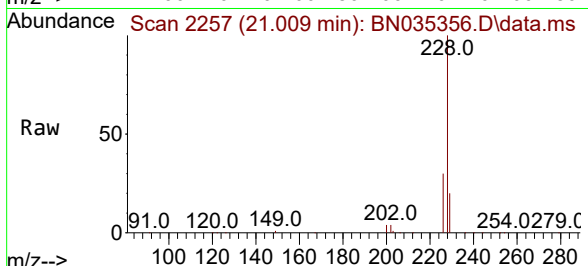


#34
 Bis(2-ethylhexyl)phthalate
 Concen: 3.721 ng
 RT: 20.938 min Scan# 2249
 Delta R.T. 0.009 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Tgt Ion:149 Resp: 78322


Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.2	33.4
279	3.2	2.7	4.1

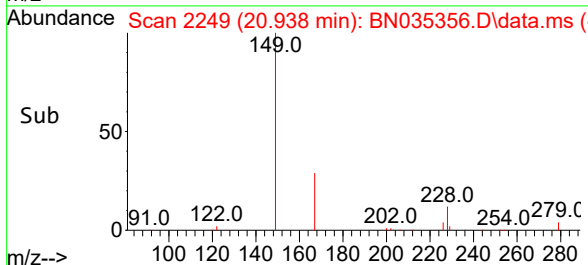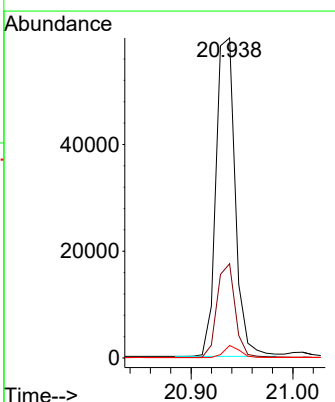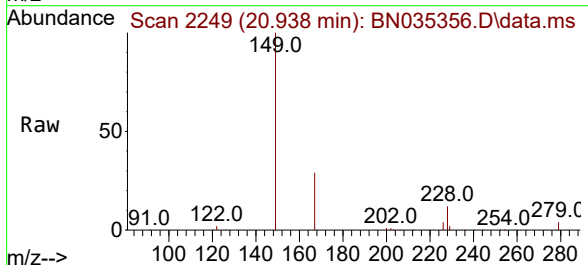






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.067 min Scan# 2
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:264 Resp: 12000
Ion Ratio Lower Upper
264 100
260 26.9 21.4 32.2
265 46.8 40.2 60.4

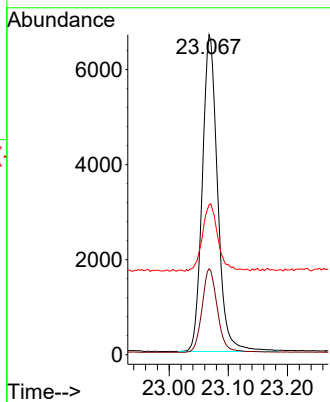

#36
Indeno(1,2,3-cd)pyrene
Concen: 5.279 ng
RT: 25.108 min Scan# 3337
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:276 Resp: 252709
Ion Ratio Lower Upper
276 100
138 23.7 19.4 29.0
277 25.0 19.8 29.6

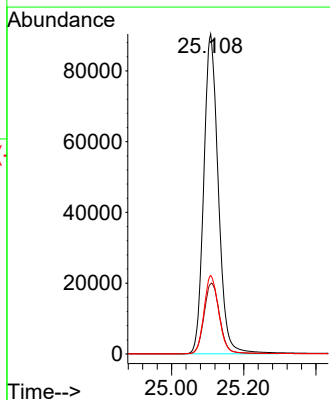



#37

Benzo(b)fluoranthene

Concen: 5.974 ng

RT: 22.456 min Scan# 2430

Delta R.T. 0.003 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09

Instrument :

BNA_N

ClientSampleId :

SSTDICC5.0





Tgt Ion:252 Resp: 241201

Ion Ratio Lower Upper

252 100

253 22.0 19.6 29.4

125 9.0 9.6 14.4#

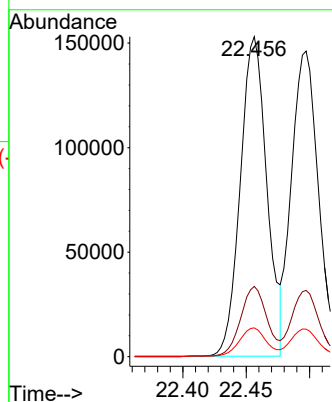

#38

Benzo(k)fluoranthene

Concen: 5.449 ng

RT: 22.497 min Scan# 2444

Delta R.T. 0.003 min

Lab File: BN035356.D

Acq: 27 Nov 2024 19:09




Tgt Ion:252 Resp: 220146


Ion Ratio Lower Upper

252 100

253 21.7 19.5 29.3


125 9.0 10.2 15.4#

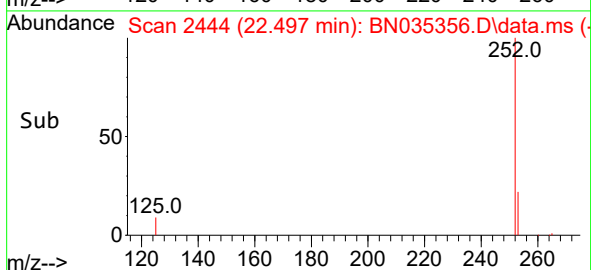






#39
Benzo(a)pyrene
Concen: 5.367 ng
RT: 22.977 min Scan# 20
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 190665
Ion Ratio Lower Upper
252 100
253 21.6 20.2 30.4
125 10.0 10.9 16.3#

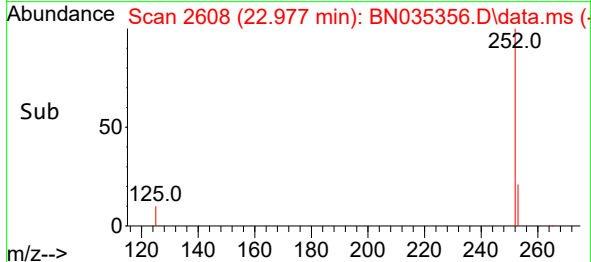

#40
Dibenzo(a,h)anthracene
Concen: 5.269 ng
RT: 25.126 min Scan# 3343
Delta R.T. 0.000 min
Lab File: BN035356.D
Acq: 27 Nov 2024 19:09

Tgt Ion:278 Resp: 199852
Ion Ratio Lower Upper
278 100
139 15.8 14.2 21.4
279 23.3 20.5 30.7



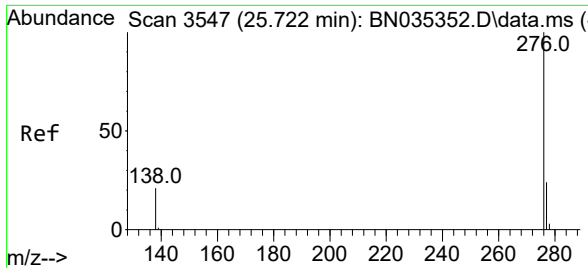

#41
 Benzo(g,h,i)perylene
 Concen: 5.183 ng
 RT: 25.725 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: BN035356.D
 Acq: 27 Nov 2024 19:09

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:	276	Resp:	209119
Ion	Ratio	Lower	Upper
276	100		
277	23.5	19.9	29.9
138	20.4	17.8	26.8

