
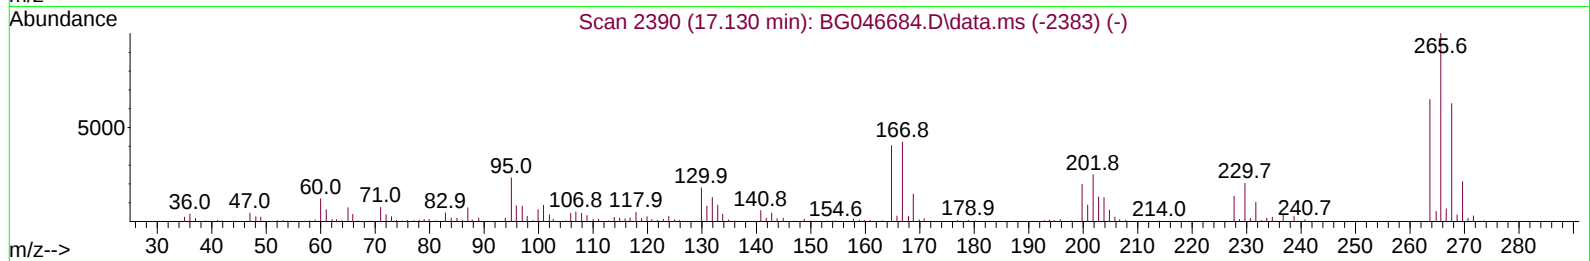
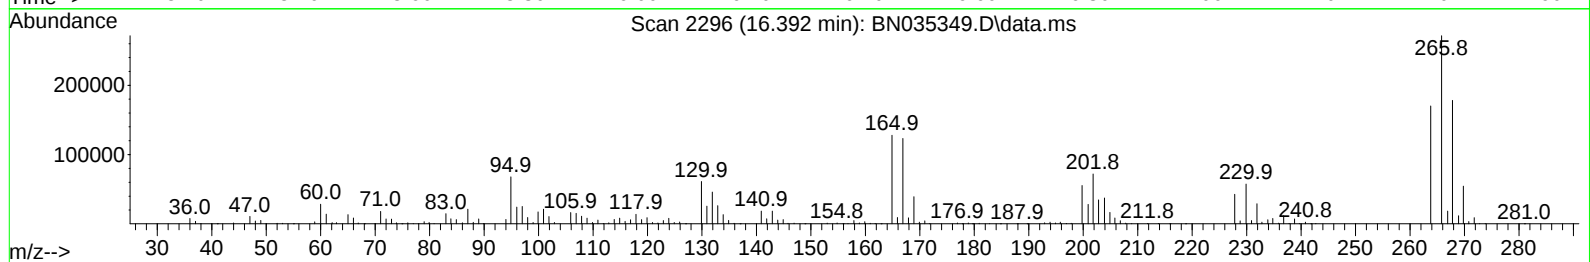


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035349.D
Acq On : 27 Nov 2024 14:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 04:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

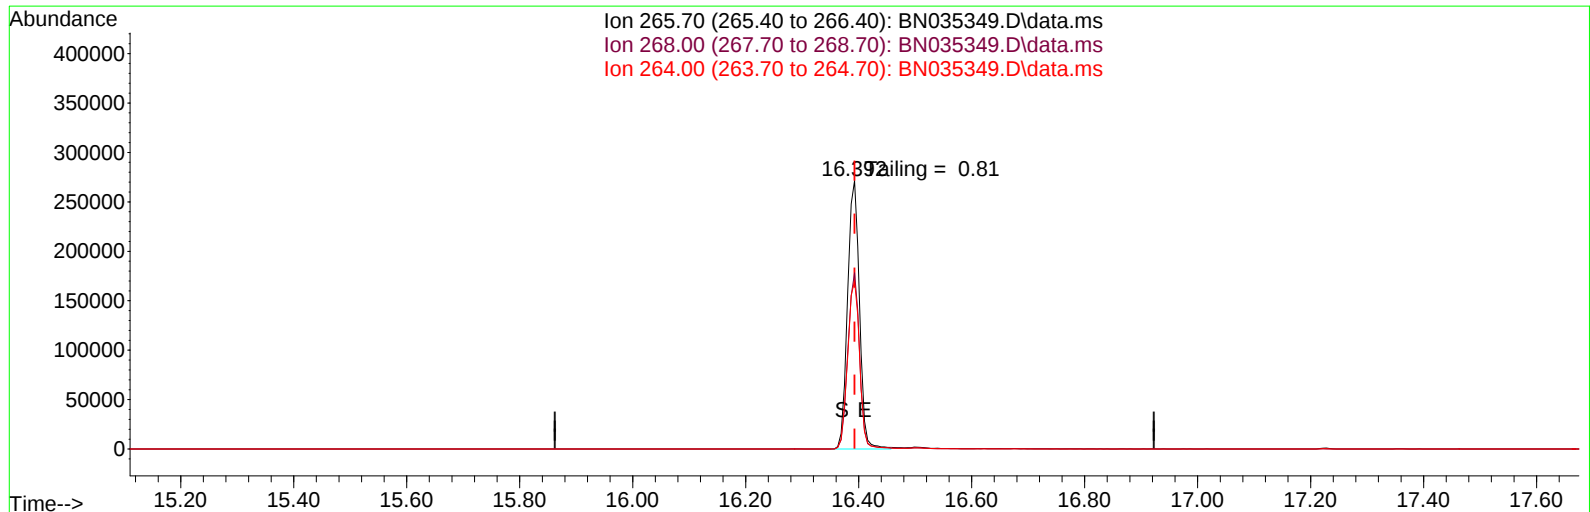

TIC: BN035349.D\data.ms

(70) Pentachlorophenol (C)




16.392min (0.000) 27794.31 ng

response 398074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.68
264.00	61.60	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035349.D
Acq On : 27 Nov 2024 14:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 28 04:07:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

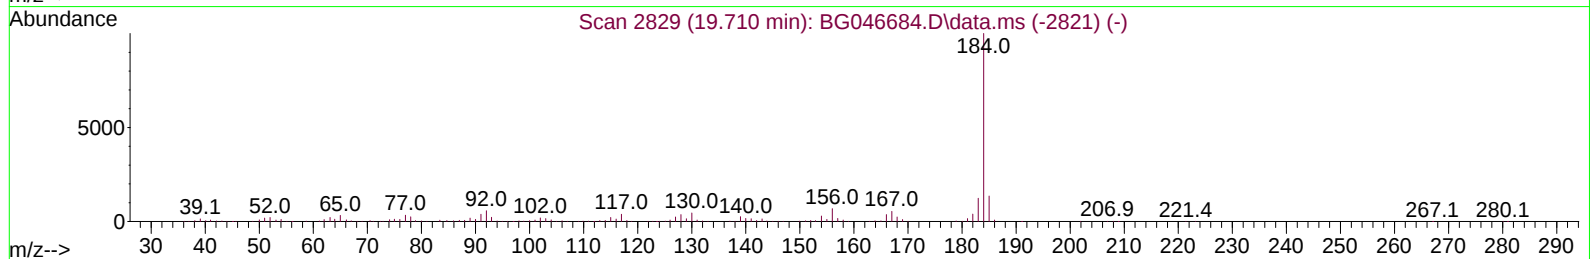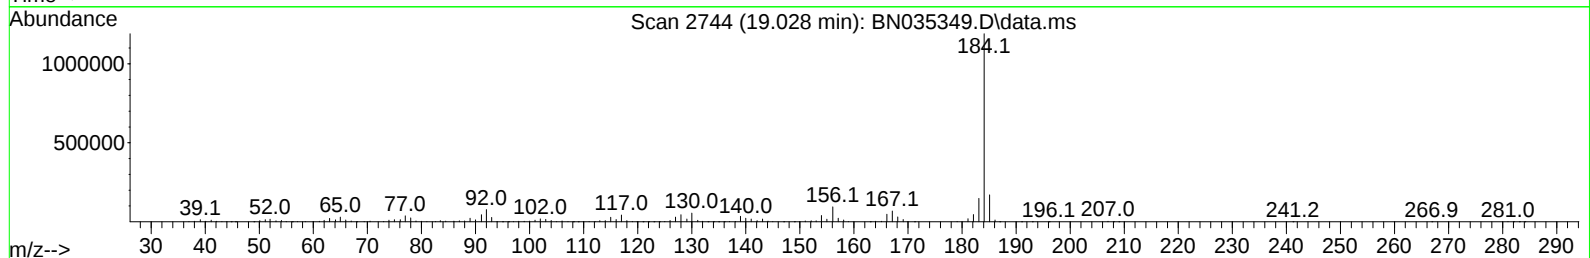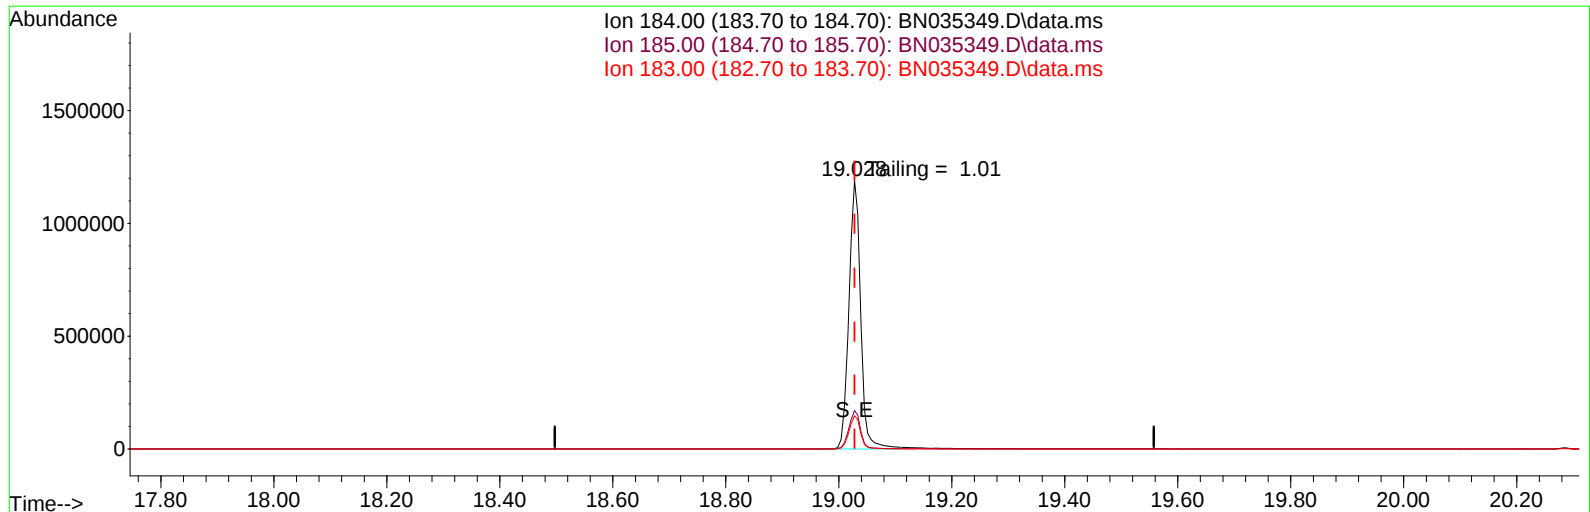

TIC: BN035349.D\data.ms

(77) Benzidine

19.028min (0.000) 0.00 ng

response 1733630

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.34
183.00	13.20	12.42
0.00	0.00	0.00