
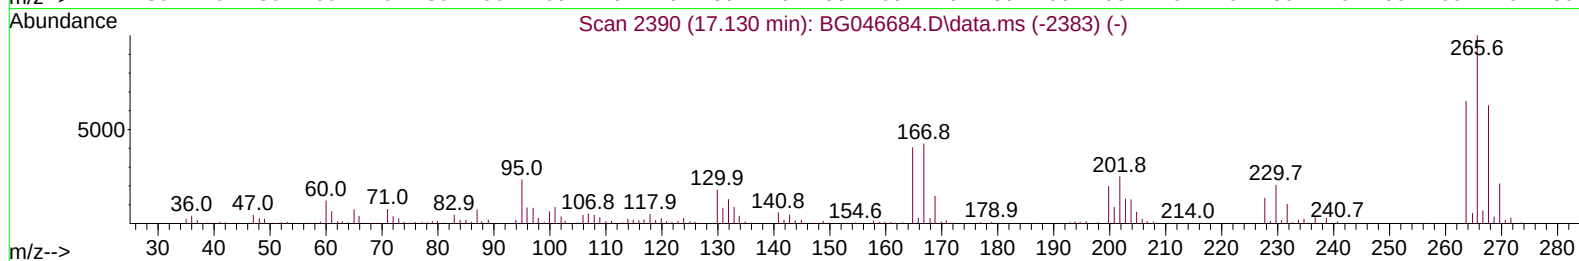
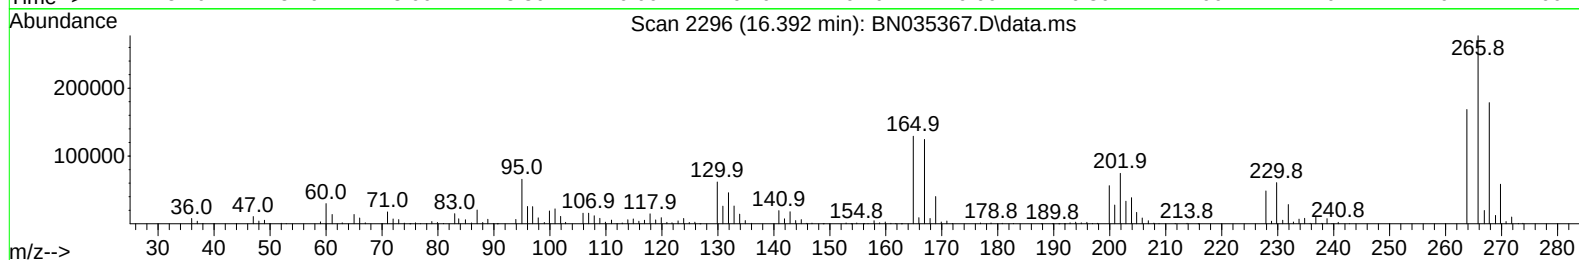


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035367.D
Acq On : 28 Nov 2024 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 28 04:09:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

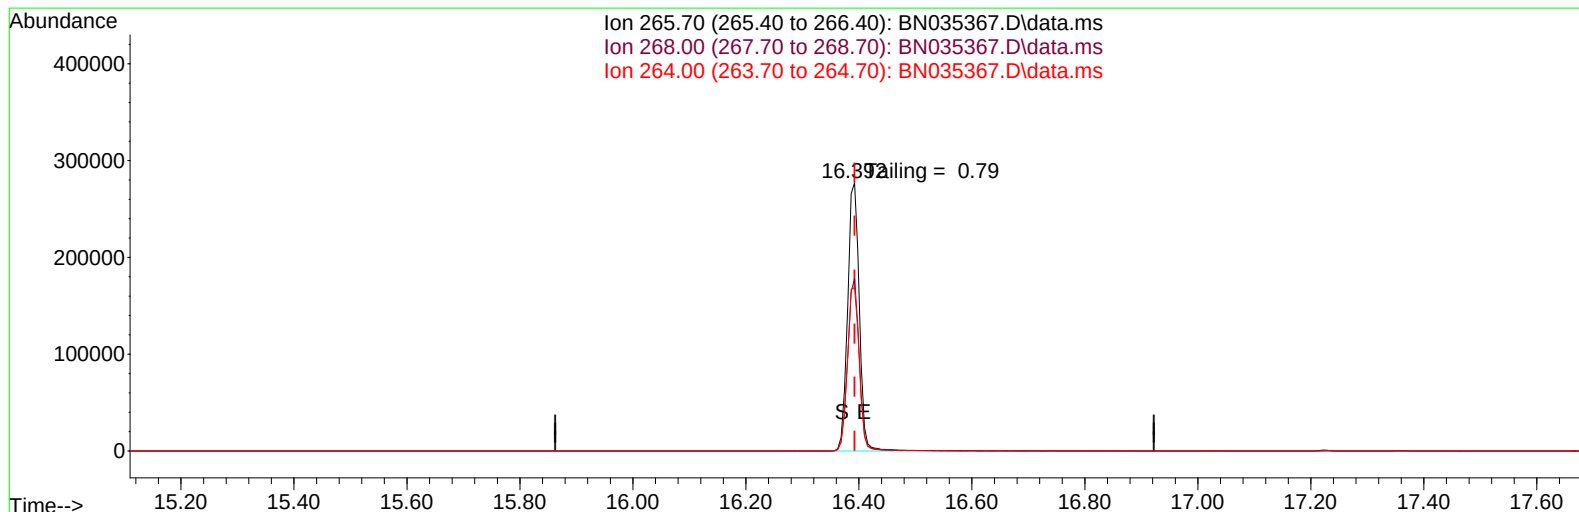

TIC: BN035367.D\data.ms

(70) Pentachlorophenol (C)




16.392min (-0.000) 27424.47 ng

response 398588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.43
264.00	61.60	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
Data File : BN035367.D
Acq On : 28 Nov 2024 03:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Nov 28 04:09:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 28 04:07:30 2024
Response via : Initial Calibration

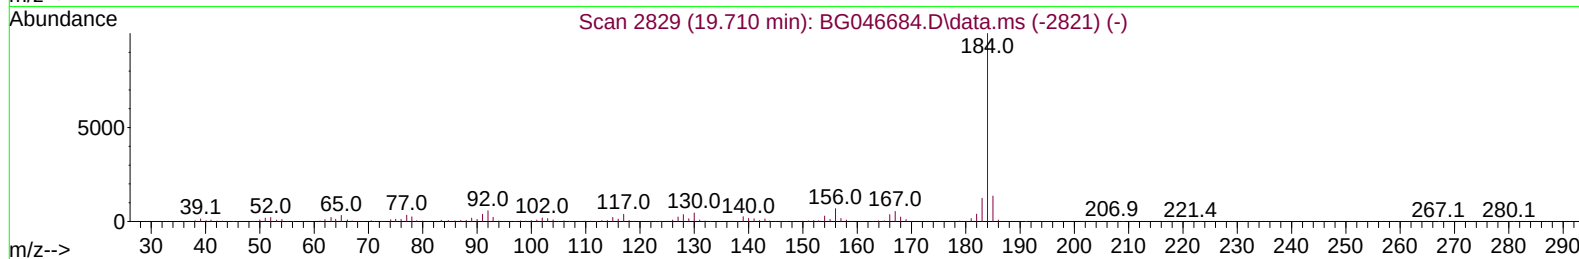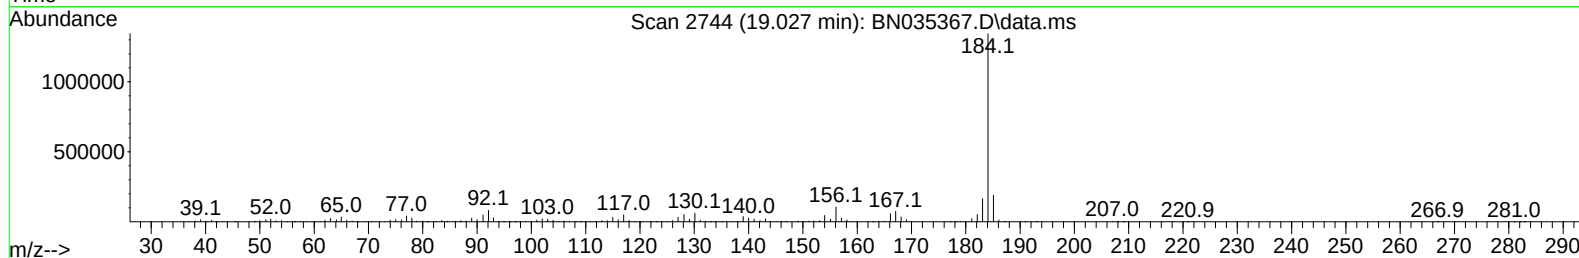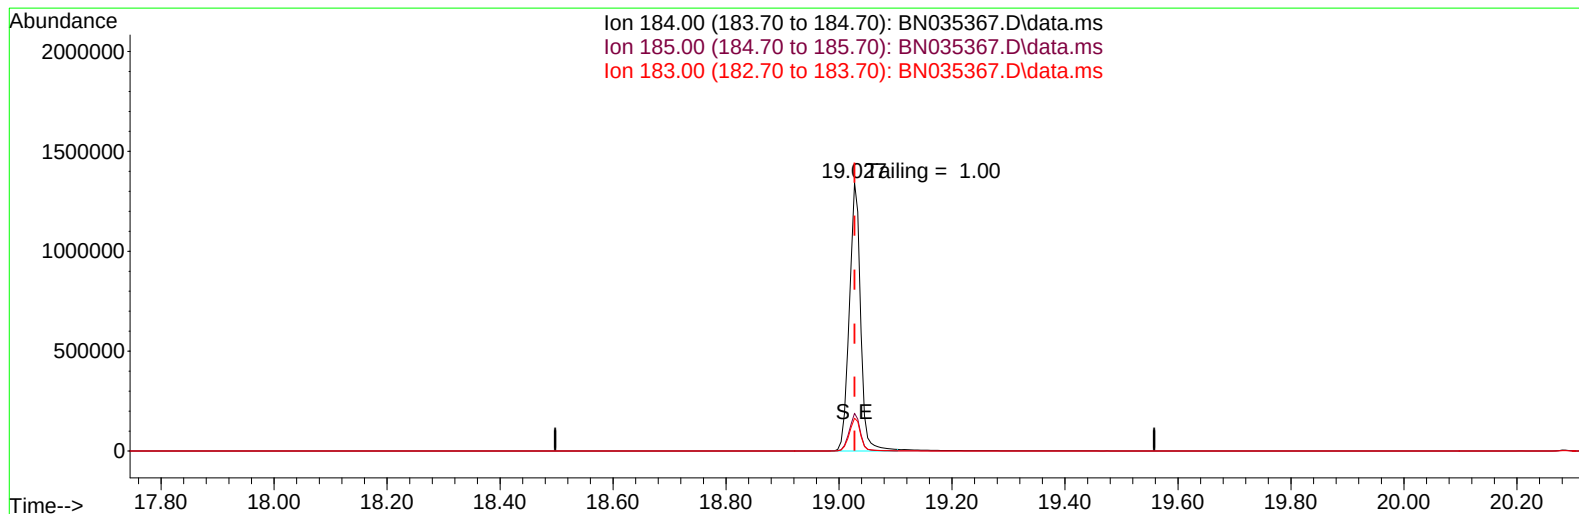

TIC: BN035367.D\data.ms

(77) Benzidine

19.027min (-0.000) 0.00 ng

response 1887713

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	12.25
0.00	0.00	0.00