
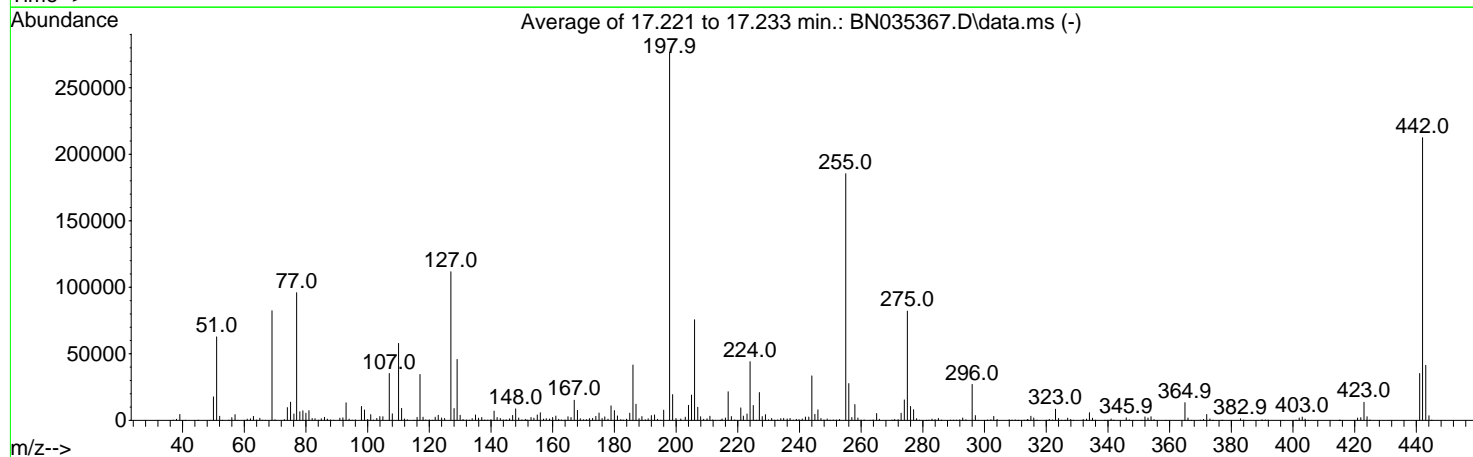


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
 Data File : BN035367.D
 Acq On : 28 Nov 2024 03:35
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112724.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 23:03:24 2024

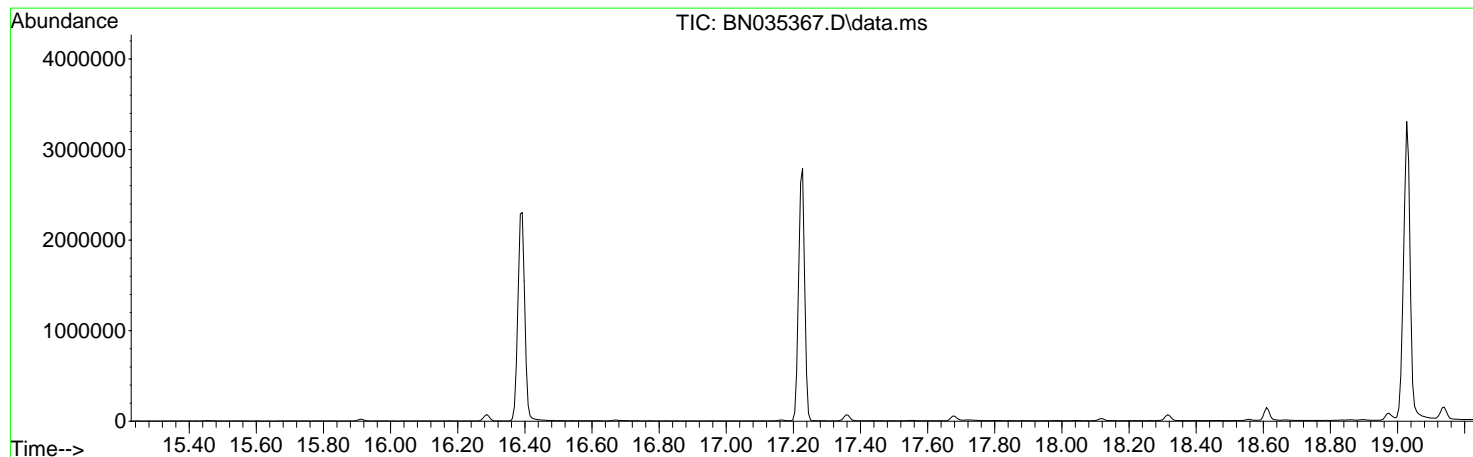

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	62763	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.8	82437	PASS
70	69	0.00	2	0.6	527	PASS
127	198	10	80	40.4	111765	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	276480	PASS
199	198	5	9	7.0	19405	PASS
275	198	10	60	29.7	82176	PASS
365	198	1	100	4.8	13390	PASS
441	198	0.01	100	12.8	35299	PASS
442	442	50	100	100.0	212459	PASS
443	442	15	24	19.5	41341	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/27/2024	BNA_N	<u>BN035367.D</u>
Compound Name	Response	Retention Time
DDT	921975	20.286
DDD	39072	19.833
DDE	1586	19.381
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
40658	962633	4.22

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
 Data File : BN035367.D
 Acq On : 28 Nov 2024 03:35
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 28 04:09:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 28 04:07:30 2024
 Response via : Initial Calibration

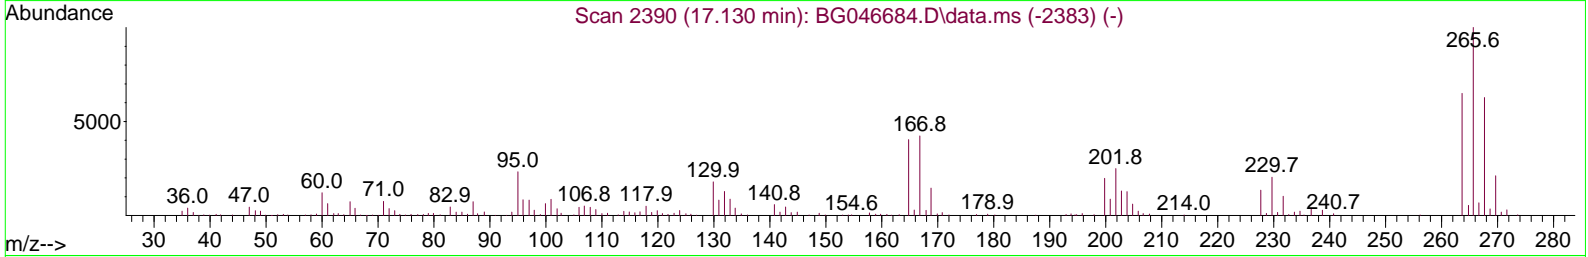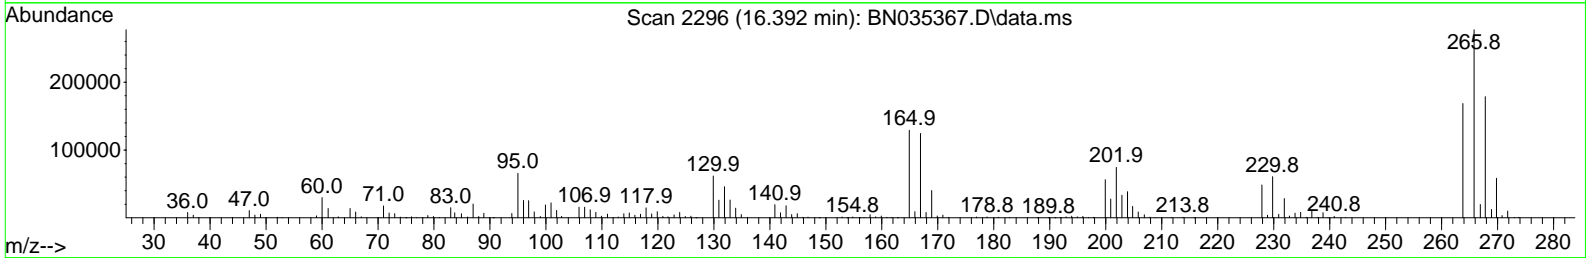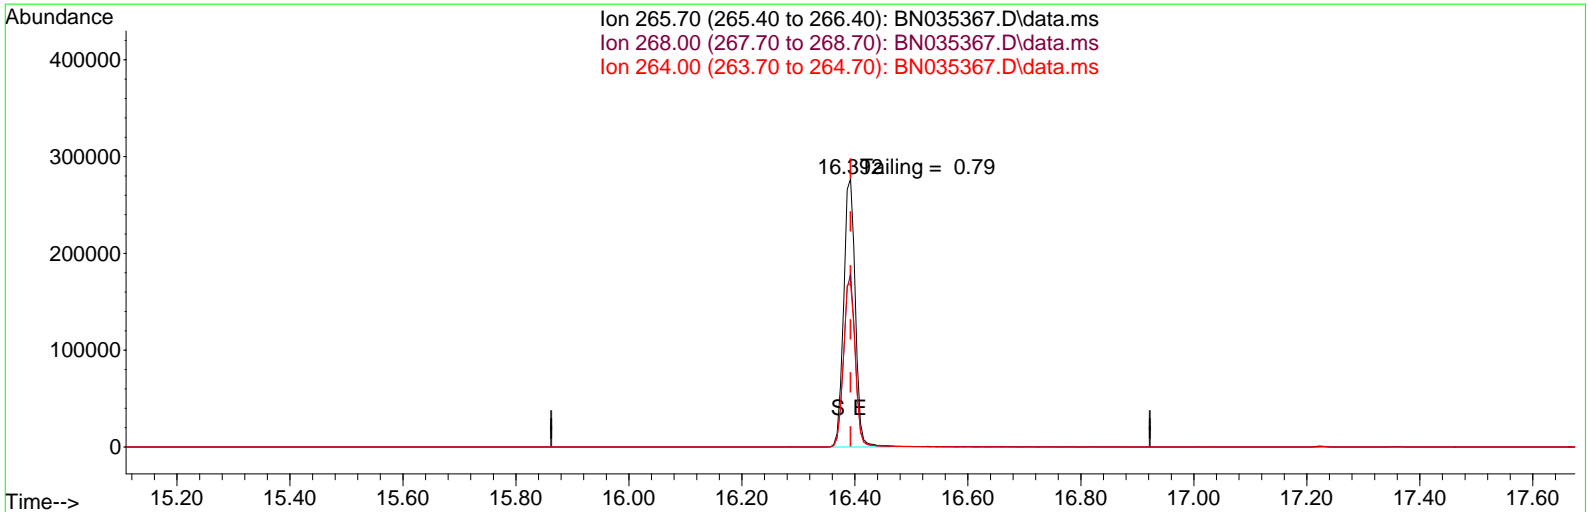

TIC: BN035367.D\data.ms

(70) Pentachlorophenol (C)

16.392min (-0.000) 27424.47 ng




response 398588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.43
264.00	61.60	60.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112724\
 Data File : BN035367.D
 Acq On : 28 Nov 2024 03:35
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 28 04:09:14 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 28 04:07:30 2024
 Response via : Initial Calibration

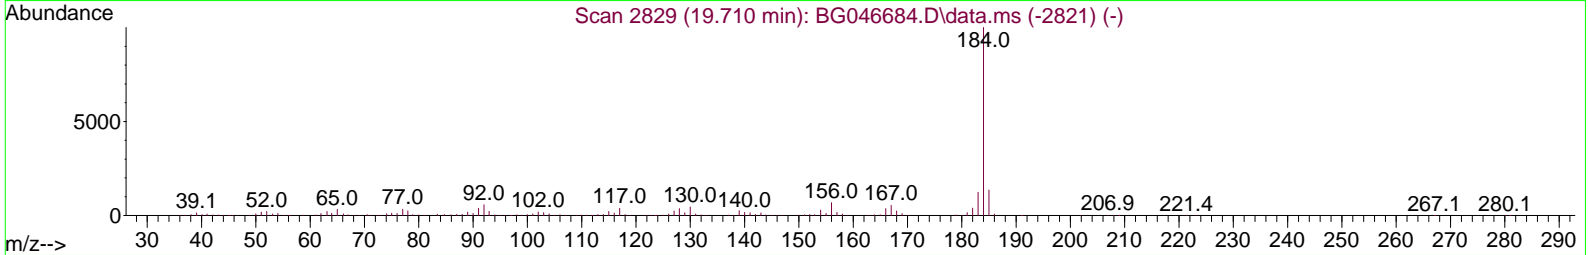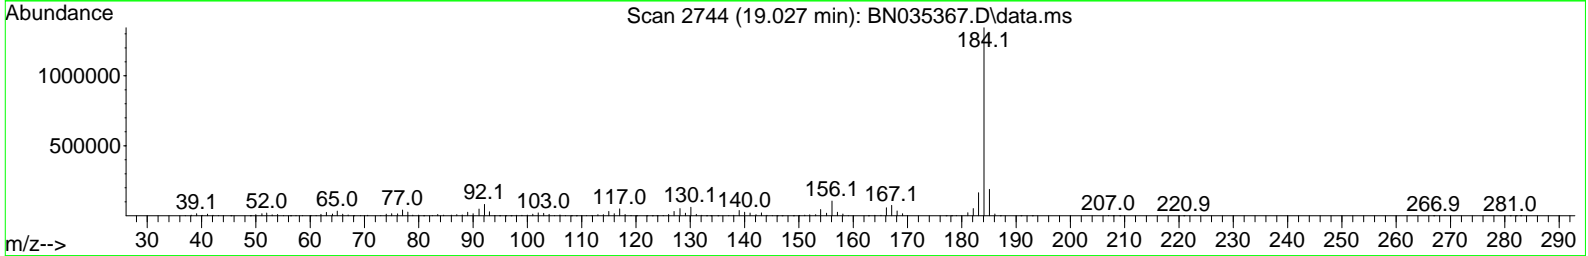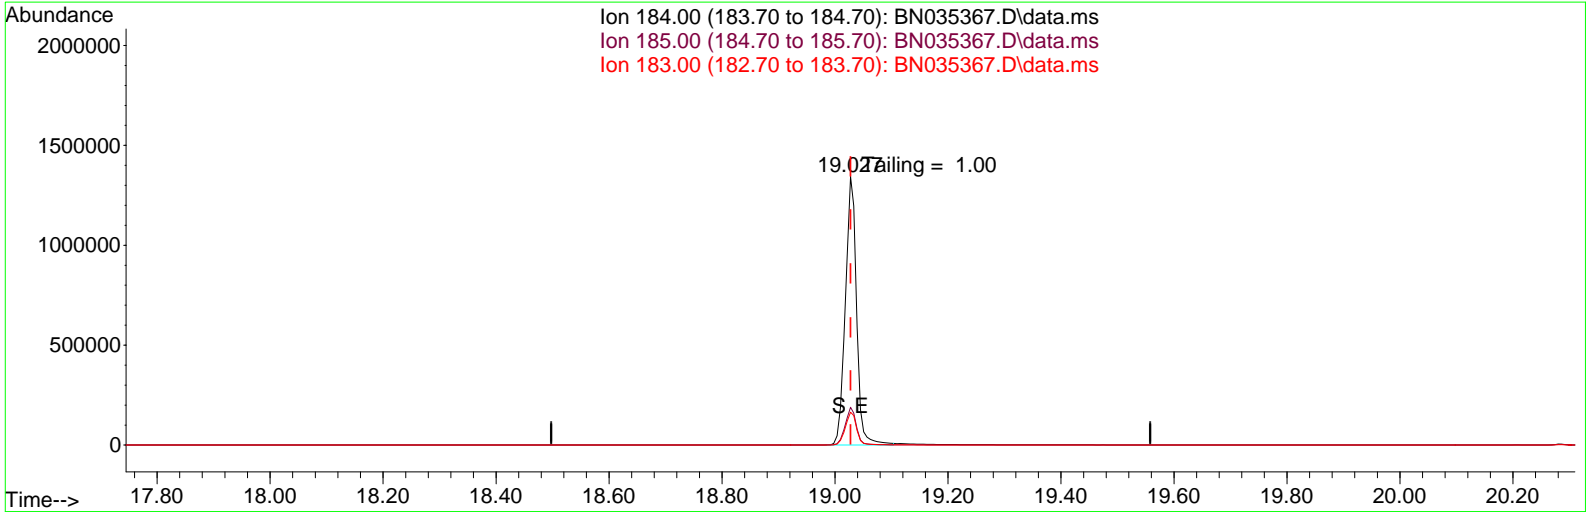

TIC: BN035367.D\data.ms

(77) Benzidine

19.027min (-0.000) 0.00 ng

response 1887713

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	12.25
0.00	0.00	0.00