
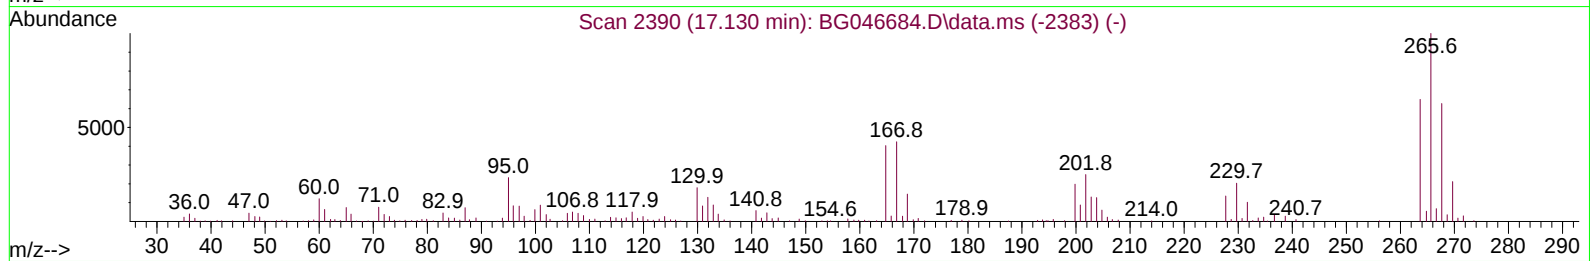
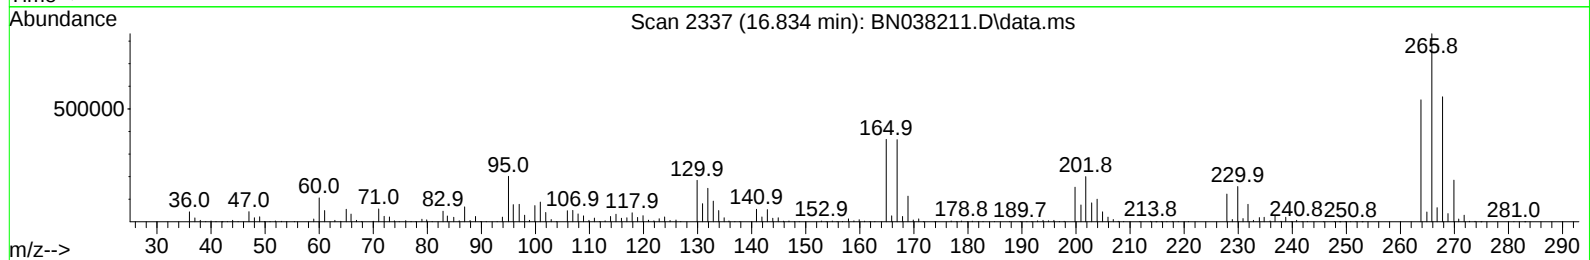


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112725\
Data File : BN038211.D
Acq On : 26 Nov 2025 19:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 01 17:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

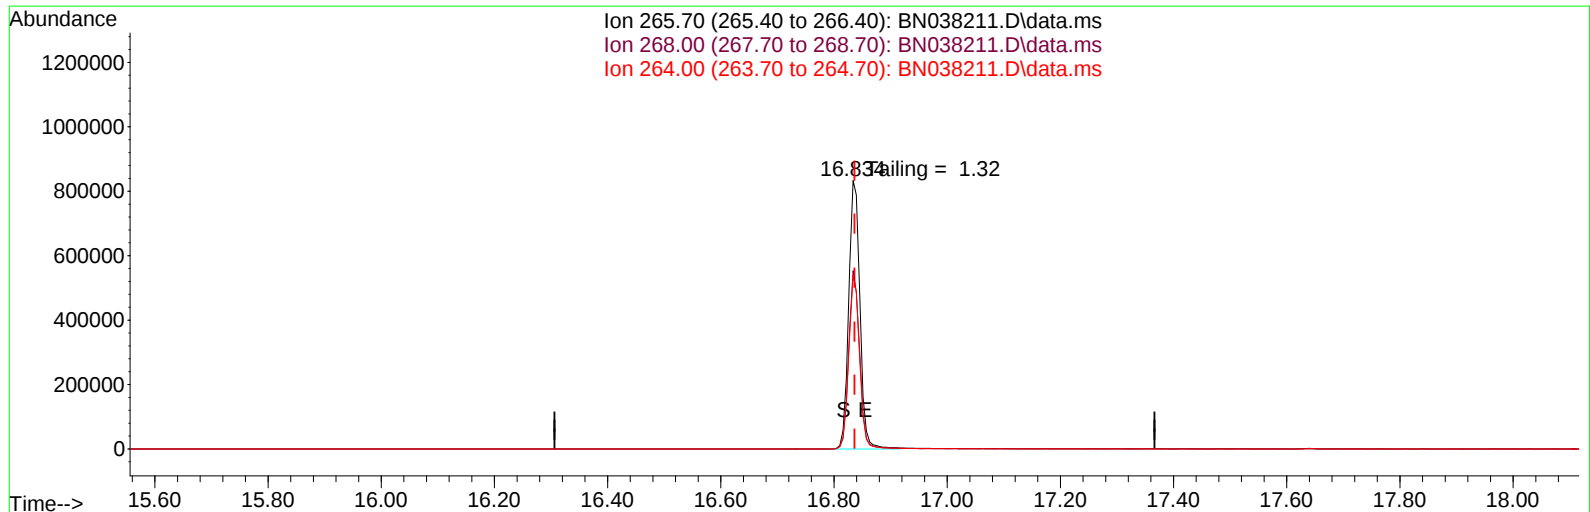

TIC: BN038211.D\data.ms

(70) Pentachlorophenol (C)




16.834min (-0.002) 31780.36 ng

response 1154991

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.41
264.00	61.60	64.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112725\
Data File : BN038211.D
Acq On : 26 Nov 2025 19:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Dec 01 17:45:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 01 10:15:10 2025
Response via : Initial Calibration

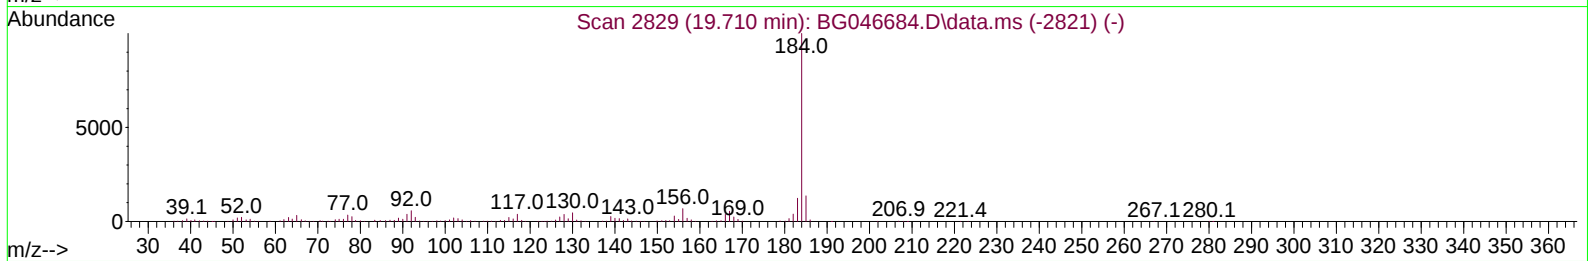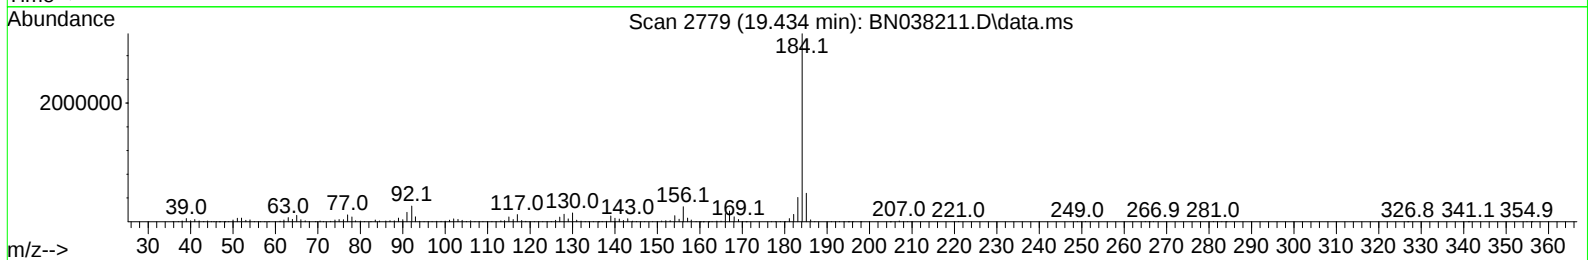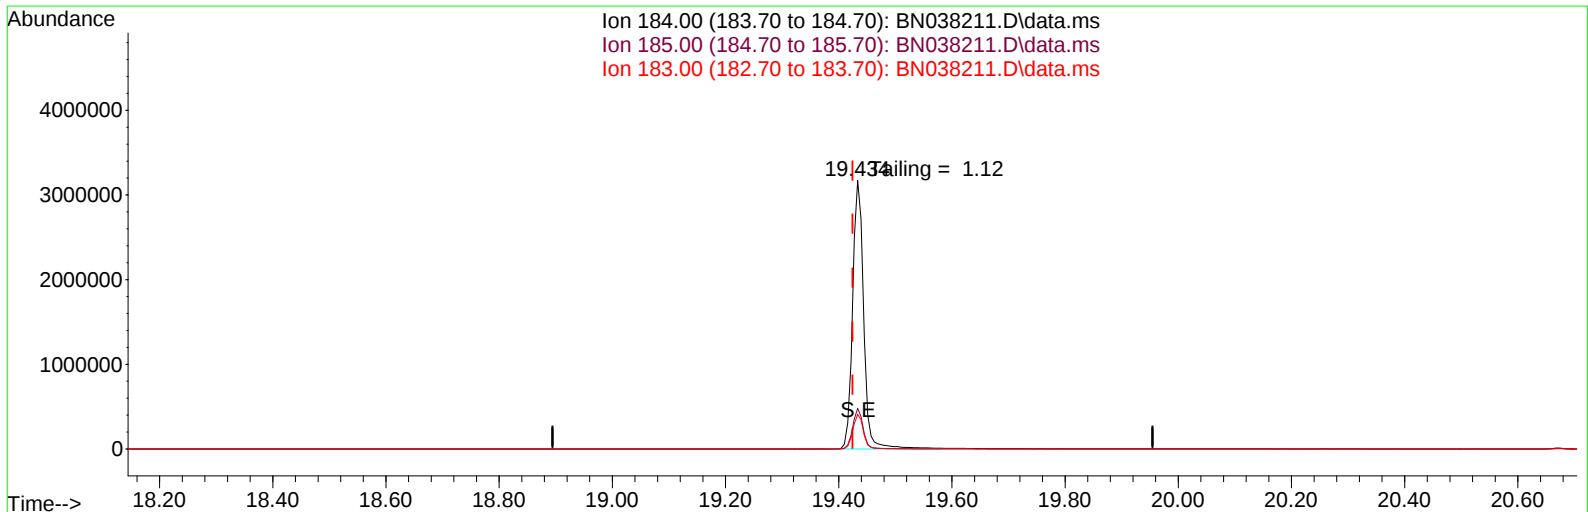

TIC: BN038211.D\data.ms

(77) Benzidine**19.434min (+ 0.009) 0.00 ng****response 4344162**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.12
183.00	13.20	12.88
0.00	0.00	0.00