
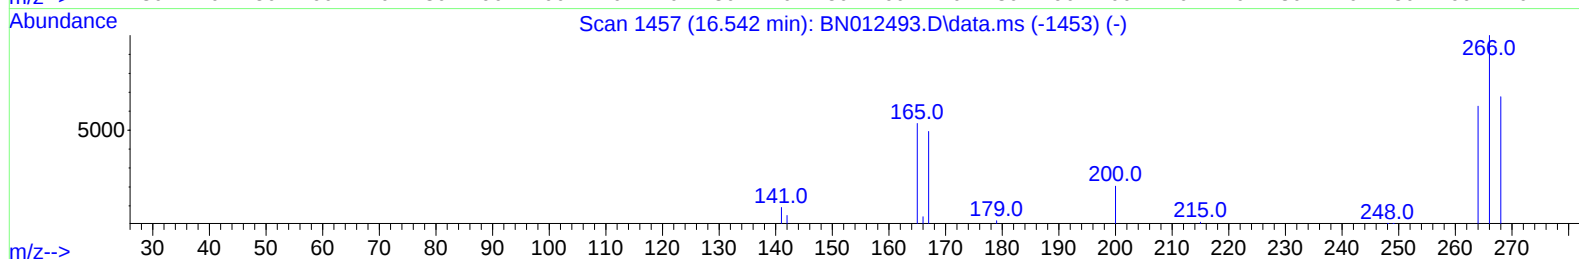
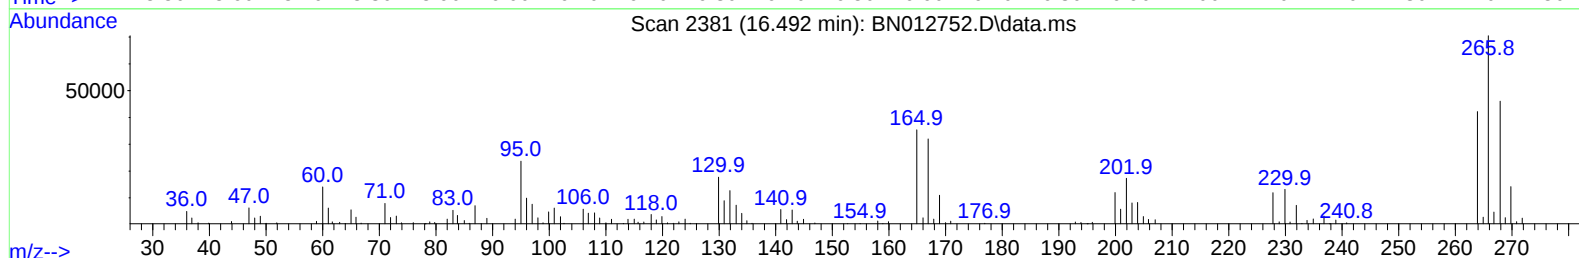


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112820\
Data File : BN012752.D
Acq On : 27 Nov 2020 14:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 23:43:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 27 15:36:21 2020
Response via : Initial Calibration

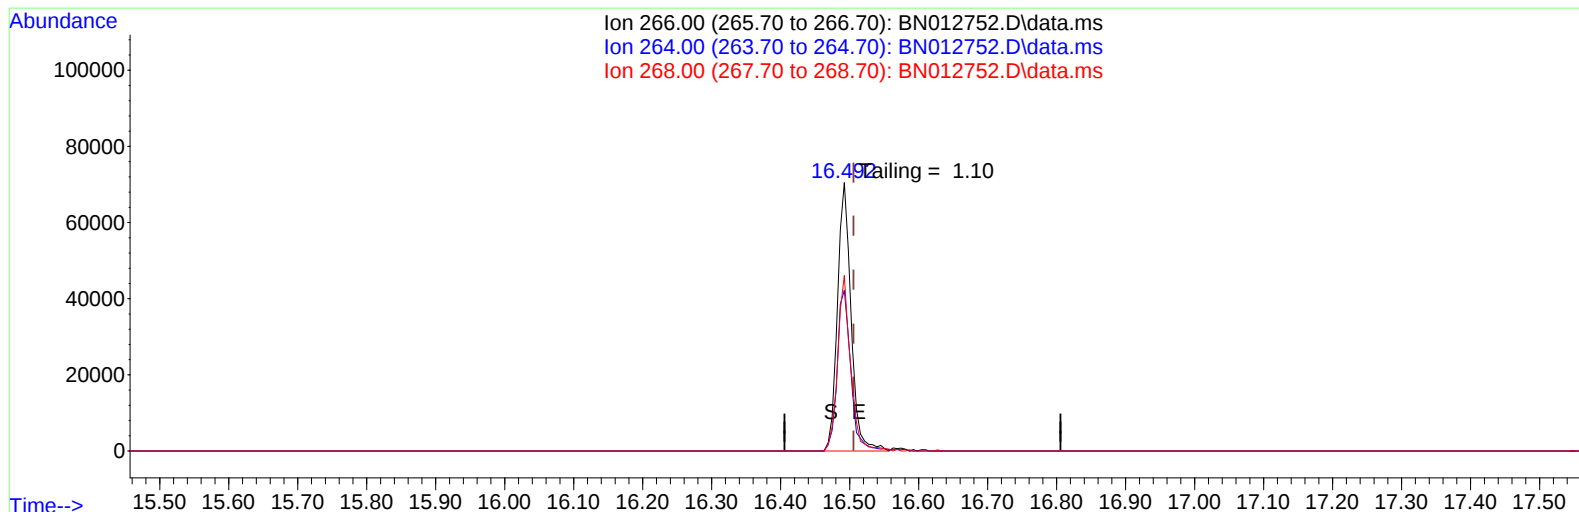

TIC: BN012752.D\data.ms

(24) Pentachlorophenol

16.492min (-0.013) 0.00 ng

response 96678

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	60.07
268.00	64.40	62.70
0.00	0.00	0.00