
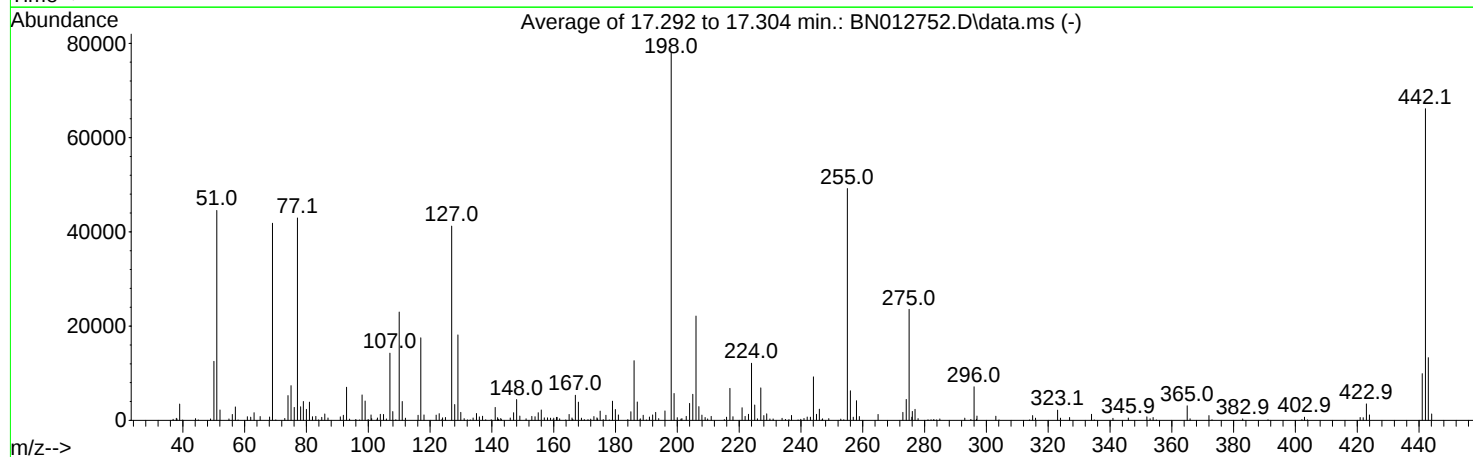


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112820\
 Data File : BN012752.D
 Acq On : 27 Nov 2020 14:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 27 15:36:21 2020

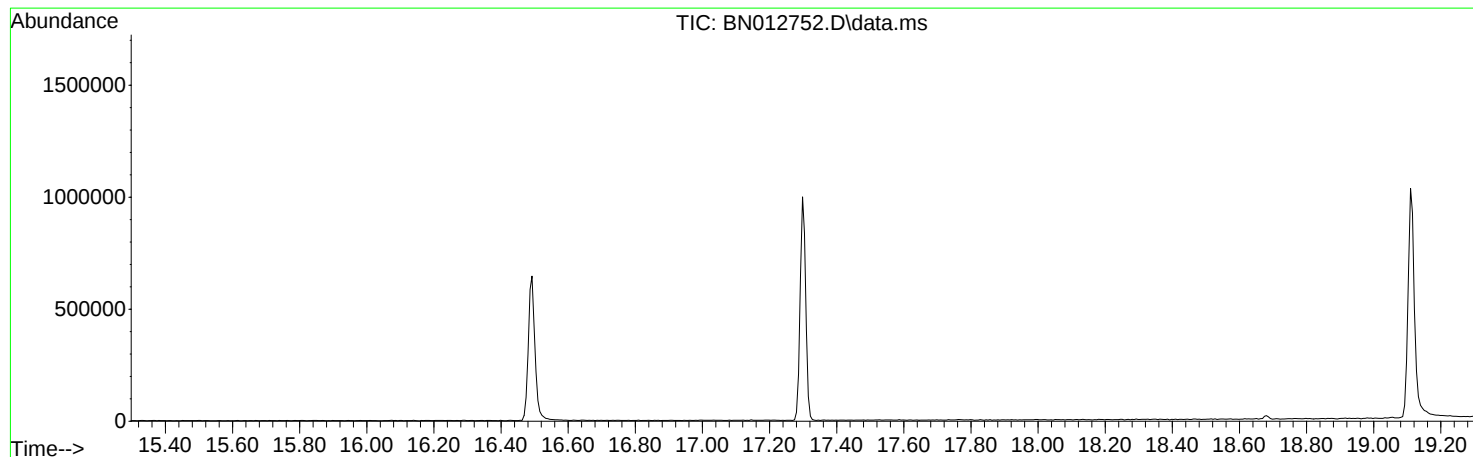

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	44549	PASS
68	69	0.00	2	1.7	723	PASS
69	198	0.00	100	53.6	41827	PASS
70	69	0.00	2	0.2	102	PASS
127	198	10	80	52.8	41203	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78056	PASS
199	198	5	9	7.3	5689	PASS
275	198	10	60	30.2	23555	PASS
365	198	1	100	4.0	3107	PASS
441	198	0.01	100	12.7	9904	PASS
442	442	100	100	100.0	66128	PASS
443	442	15	24	20.1	13318	PASS