
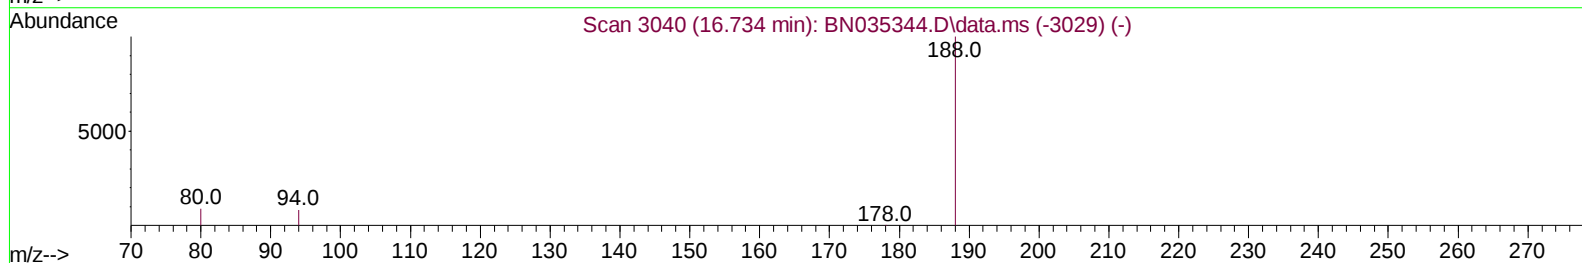
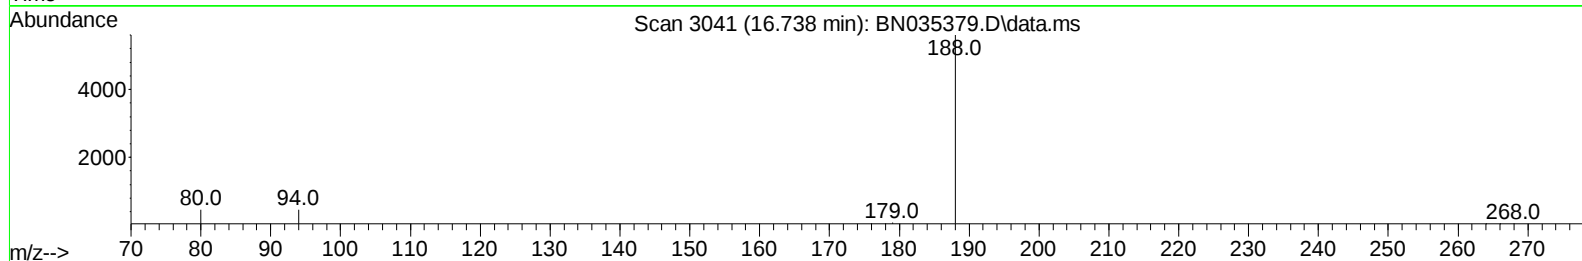


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
Data File : BN035379.D
Acq On : 28 Nov 2024 12:44
Operator : RC/JU
Sample : PB165230BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

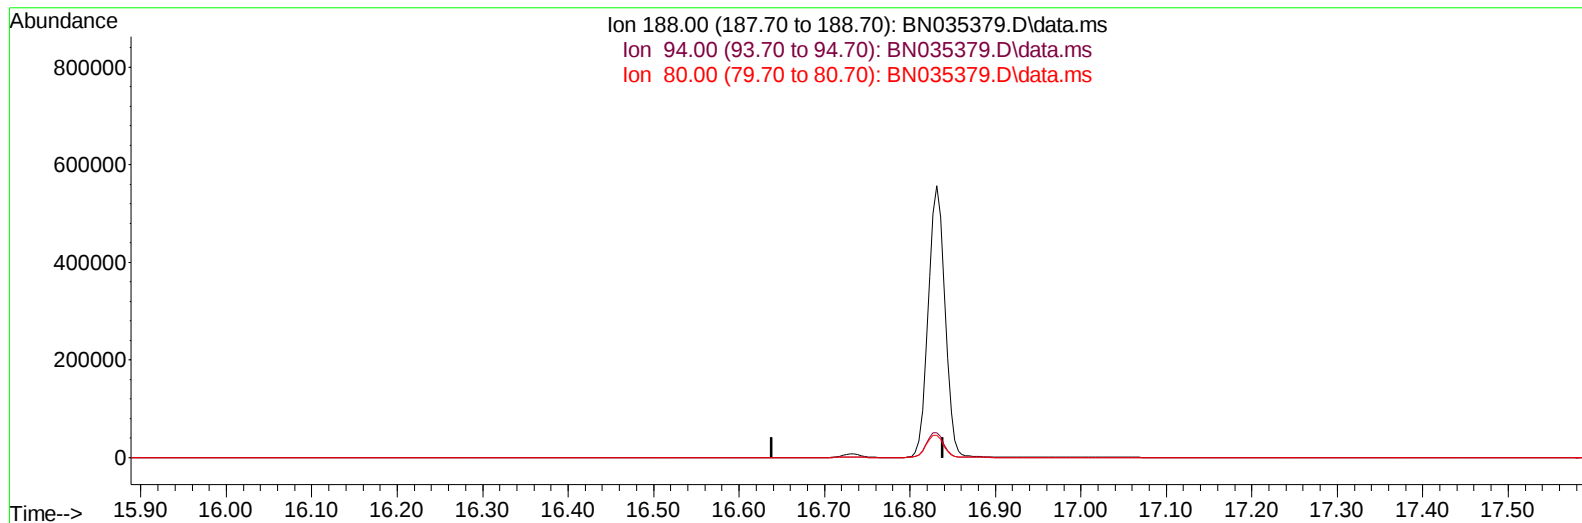

TIC: BN035379.D\data.ms

(13) Phenanthrene-d10 (I)




16.738min (-16.738) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
Data File : BN035379.D
Acq On : 28 Nov 2024 12:44
Operator : RC/JU
Sample : PB165230BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

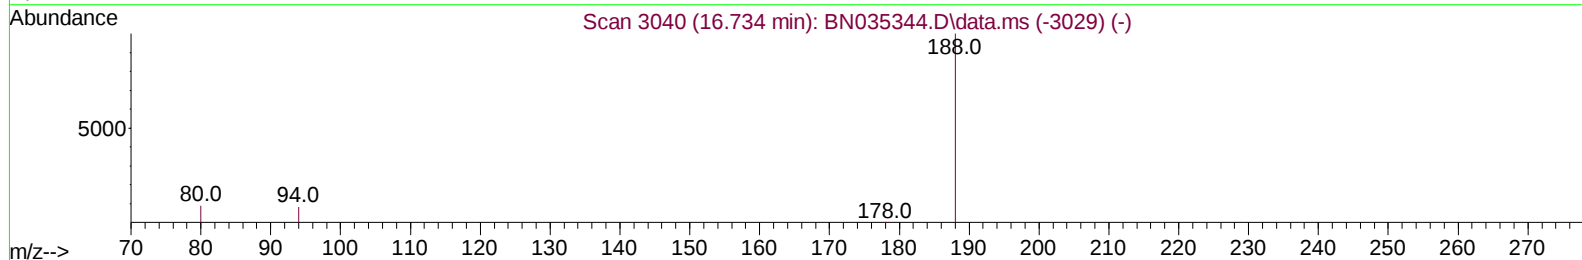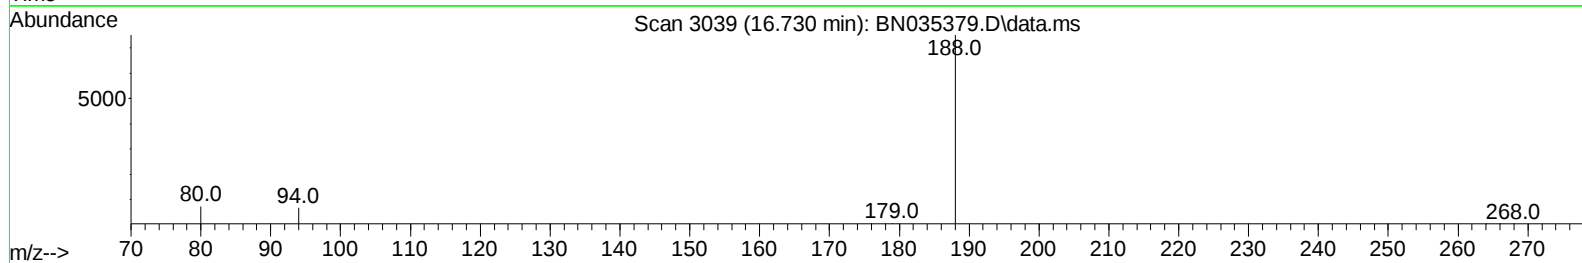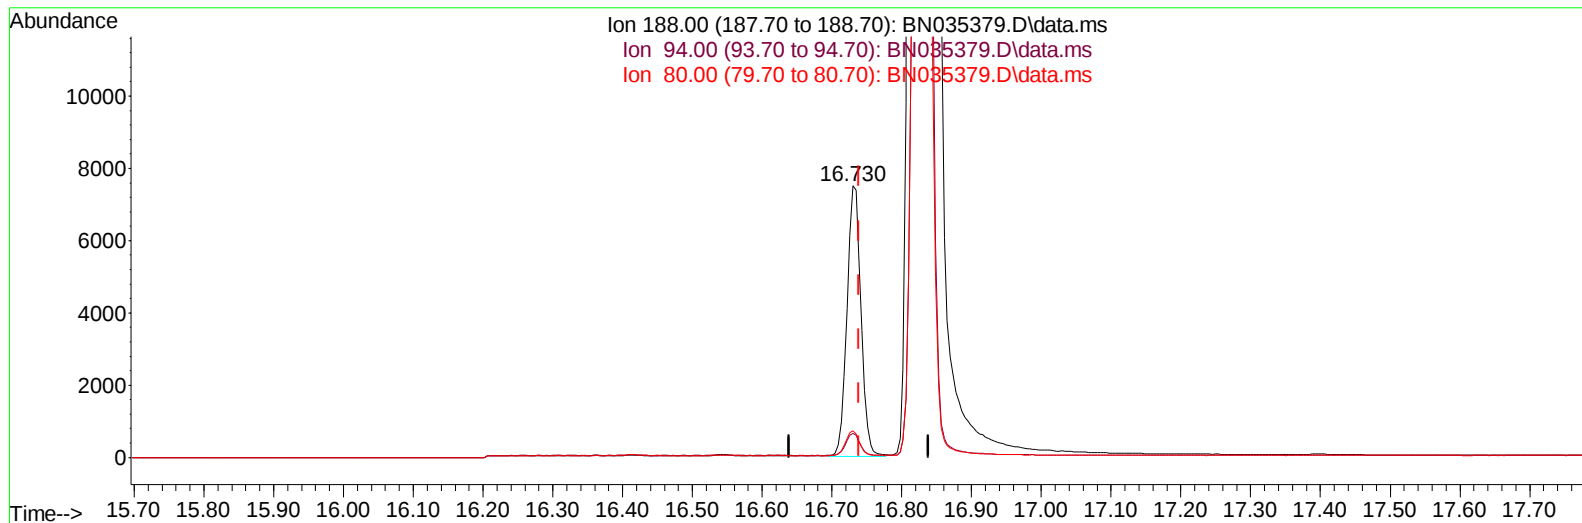

TIC: BN035379.D\data.ms

(13) Phenanthrene-d10 (I)




16.730min (-0.008) 0.40 ng/ul m

response 10404

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	8.94#
80.00	7.60	9.85#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
Data File : BN035379.D
Acq On : 28 Nov 2024 12:44
Operator : RC/JU
Sample : PB165230BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

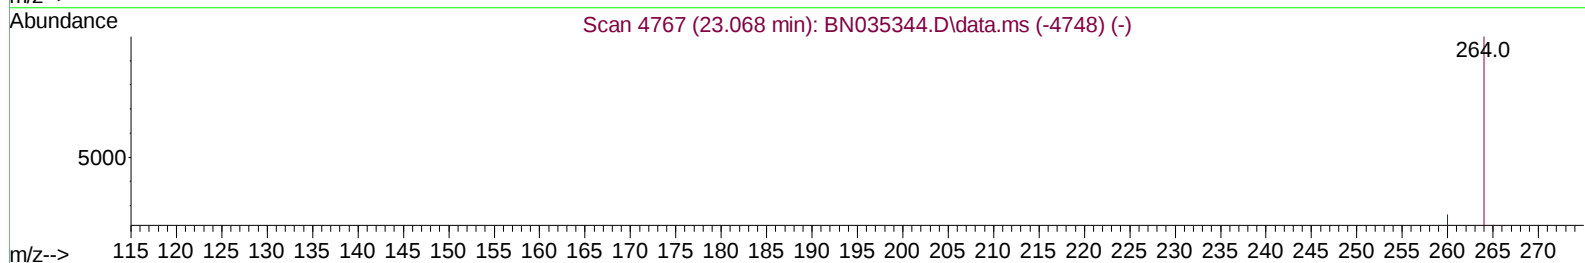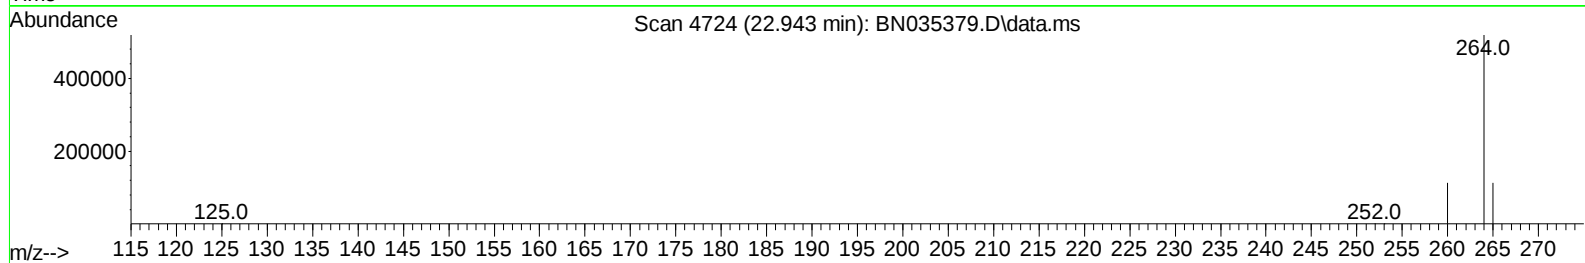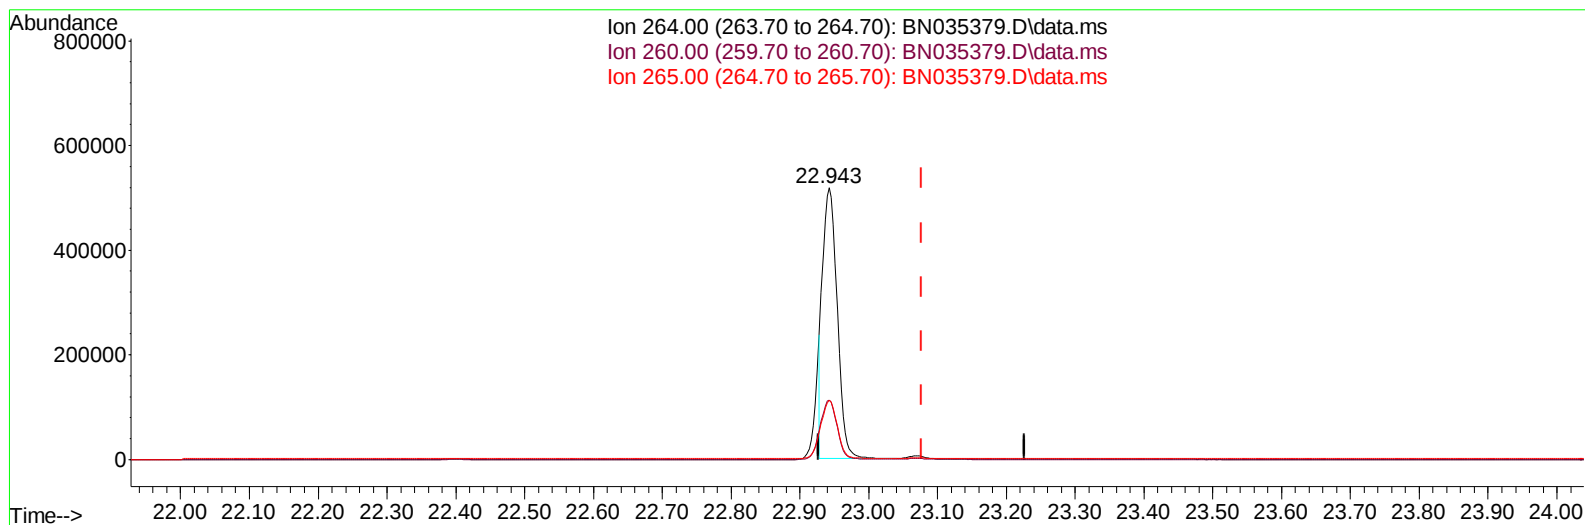

TIC: BN035379.D\data.ms

(23) Perylene-d12 (I)




22.943min (-0.134) 0.40 ng/ul

response 763262

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	21.92
265.00	75.50	21.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
Data File : BN035379.D
Acq On : 28 Nov 2024 12:44
Operator : RC/JU
Sample : PB165230BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

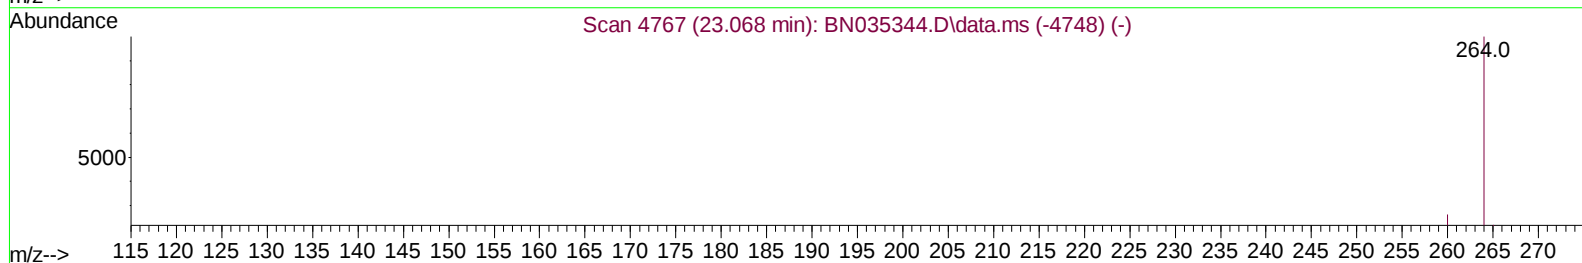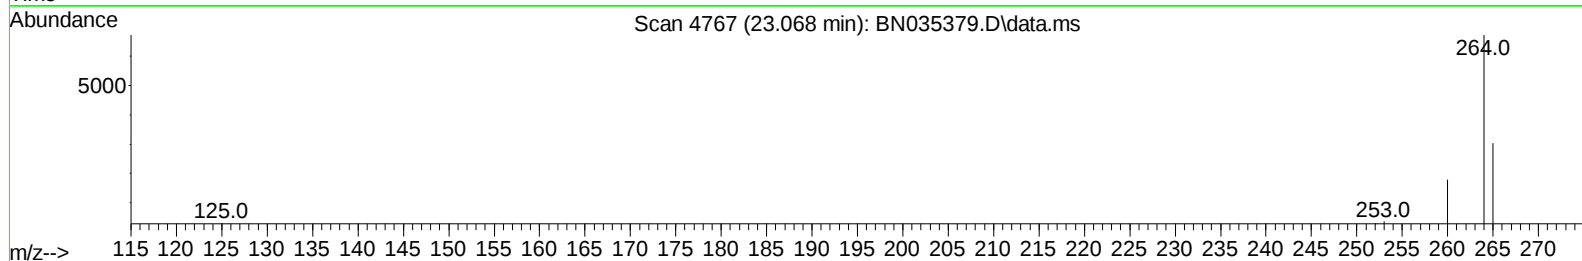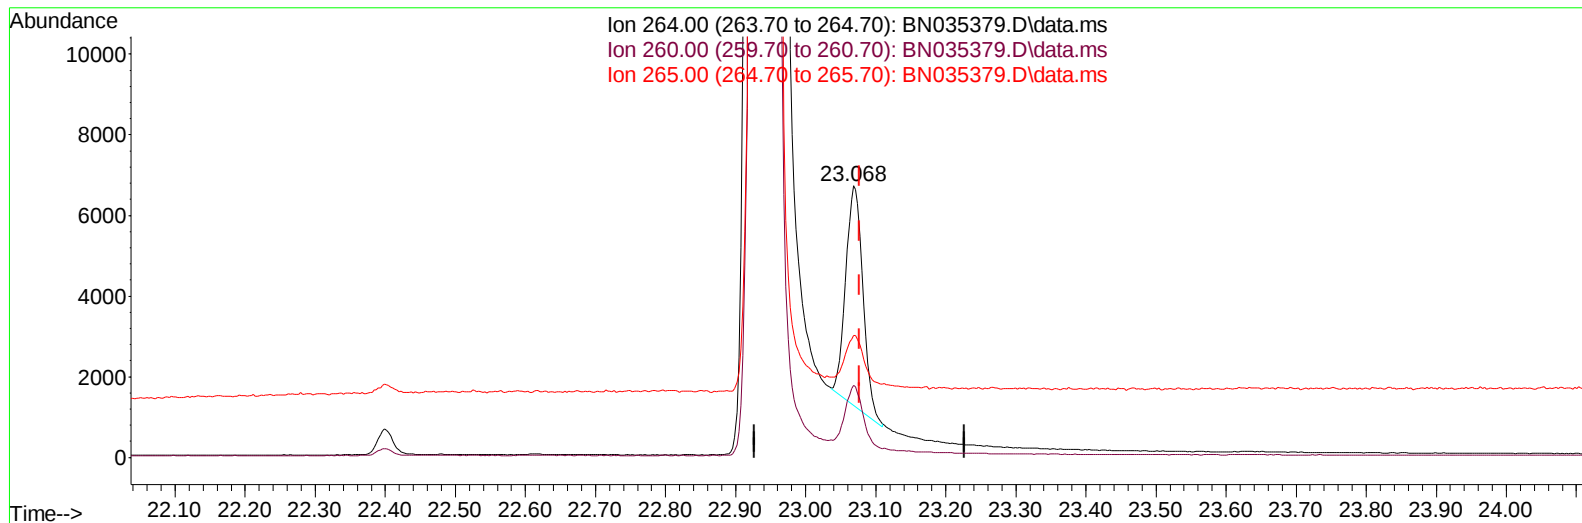

TIC: BN035379.D\data.ms

(23) Perylene-d12 (I)

23.068min (-0.009) 0.40 ng/ul m

response 9285

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.44
265.00	75.50	44.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
 Data File : BN035379.D
 Acq On : 28 Nov 2024 12:44
 Operator : RC/JU
 Sample : PB165230BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 26 06:09:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.310	152	2034	0.400	ng/ul	0.00
4) Naphthalene-d8	10.053	136	6075	0.400	ng/ul	-0.01
9) Acenaphthene-d10	13.967	164	4316	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.730	188	10404m	0.400	ng/ul	0.00
17) Chrysene-d12	20.976	240	9122	0.400	ng/ul	# 0.00
23) Perylene-d12	23.068	264	9285m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.963	96	12669	6.815	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.659	152	3013	0.338	ng/ul	0.00
18) Fluoranthene-d10	18.782	212	9419	0.374	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN112824\
Data File : BN035379.D
Acq On : 28 Nov 2024 12:44
Operator : RC/JU
Sample : PB165230BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Nov 29 01:42:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 26 06:09:15 2024
Response via : Initial Calibration

