
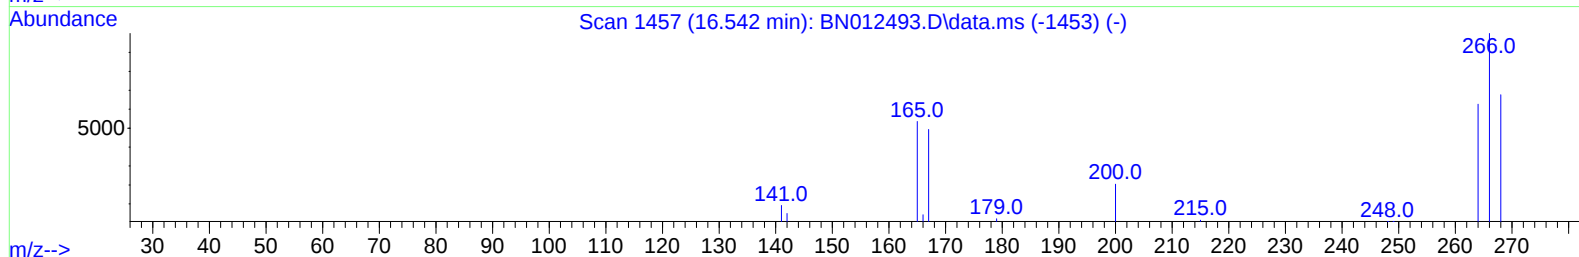
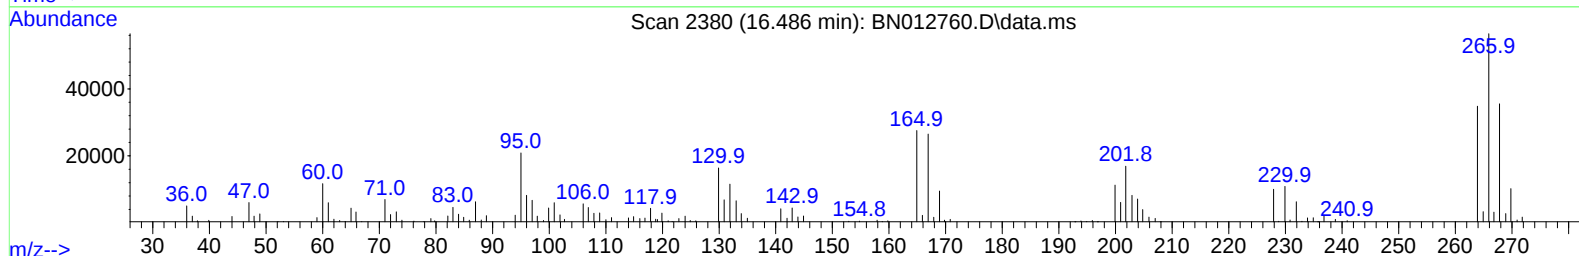


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113020\
Data File : BN012760.D
Acq On : 30 Nov 2020 09:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 01 01:28:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 27 15:36:21 2020
Response via : Initial Calibration

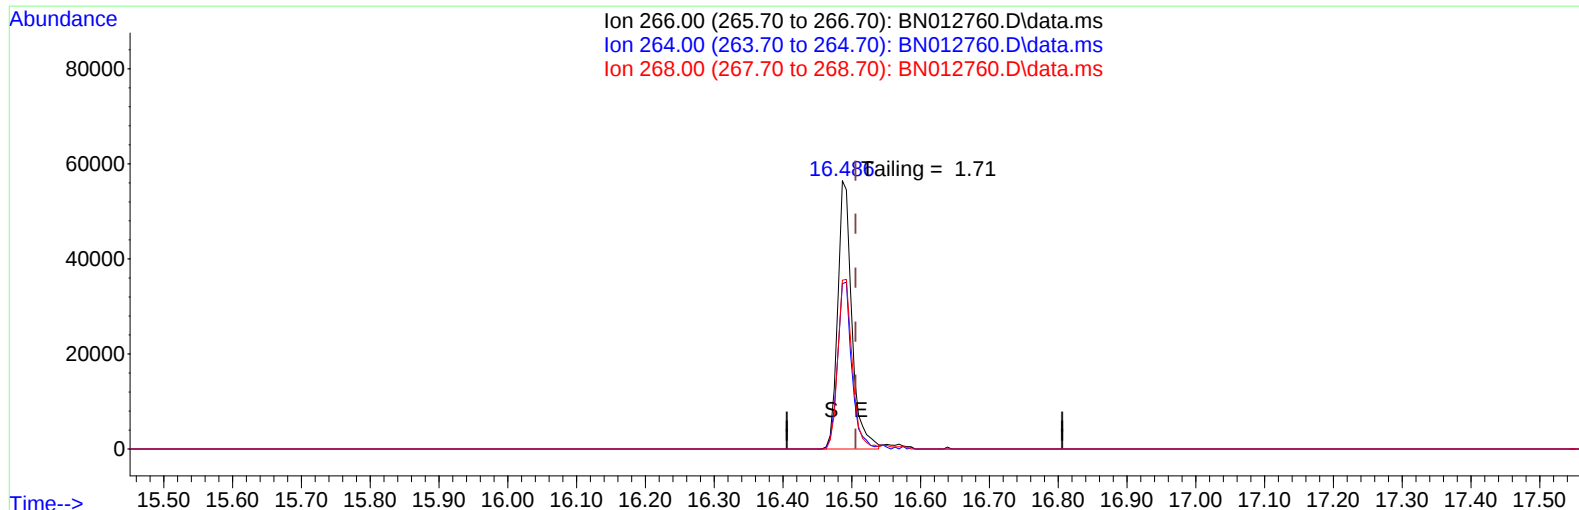

TIC: BN012760.D\data.ms

(24) Pentachlorophenol

16.486min (-0.020) 0.00 ng

response 80832

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.31
268.00	64.40	64.33
0.00	0.00	0.00