

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113020\
 Data File : BN012762.D
 Acq On : 30 Nov 2020 10:54
 Operator : CG/JU
 Sample : PB133253BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB133253BL

Manual Integrations
 APPROVED

mohammad
 12/1/2020 10:43:38 AM

Quant Time: Nov 30 11:28:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 27 15:36:21 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.426	152	784	0.40	ng	0.00
7) Naphthalene-d8	10.201	136	2767	0.40	ng	# 0.01
13) Acenaphthene-d10	14.080	164	1851	0.40	ng	0.00
19) Phenanthrene-d10	16.848	188	4055	0.40	ng	# 0.01
29) Chrysene-d12	21.067	240	4075	0.40	ng	# 0.00
36) Perylene-d12	23.175	264	4470	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.035	112	755	0.28	ng	0.00
5) Phenol-d6	6.621	99	734	0.23	ng	0.00
8) Nitrobenzene-d5	8.604	82	1103m	0.34	ng	0.03
11) 2-Methylnaphthalene-d10	11.808	152	1394	0.31	ng	0.01
14) 2,4,6-Tribromophenol	15.602	330	331	0.25	ng	0.01
15) 2-Fluorobiphenyl	12.709	172	3010	0.42	ng	0.01
27) Fluoranthene-d10	18.888	212	3925	0.31	ng	0.00
31) Terphenyl-d14	19.498	244	6200	0.64	ng	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113020\
Data File : BN012762.D
Acq On : 30 Nov 2020 10:54
Operator : CG/JU
Sample : PB133253BL
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PB133253BL

Manual Integrations
APPROVED


mohammad
12/1/2020 10:43:38 AM

Quant Time: Nov 30 11:28:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 27 15:36:21 2020
Response via : Initial Calibration



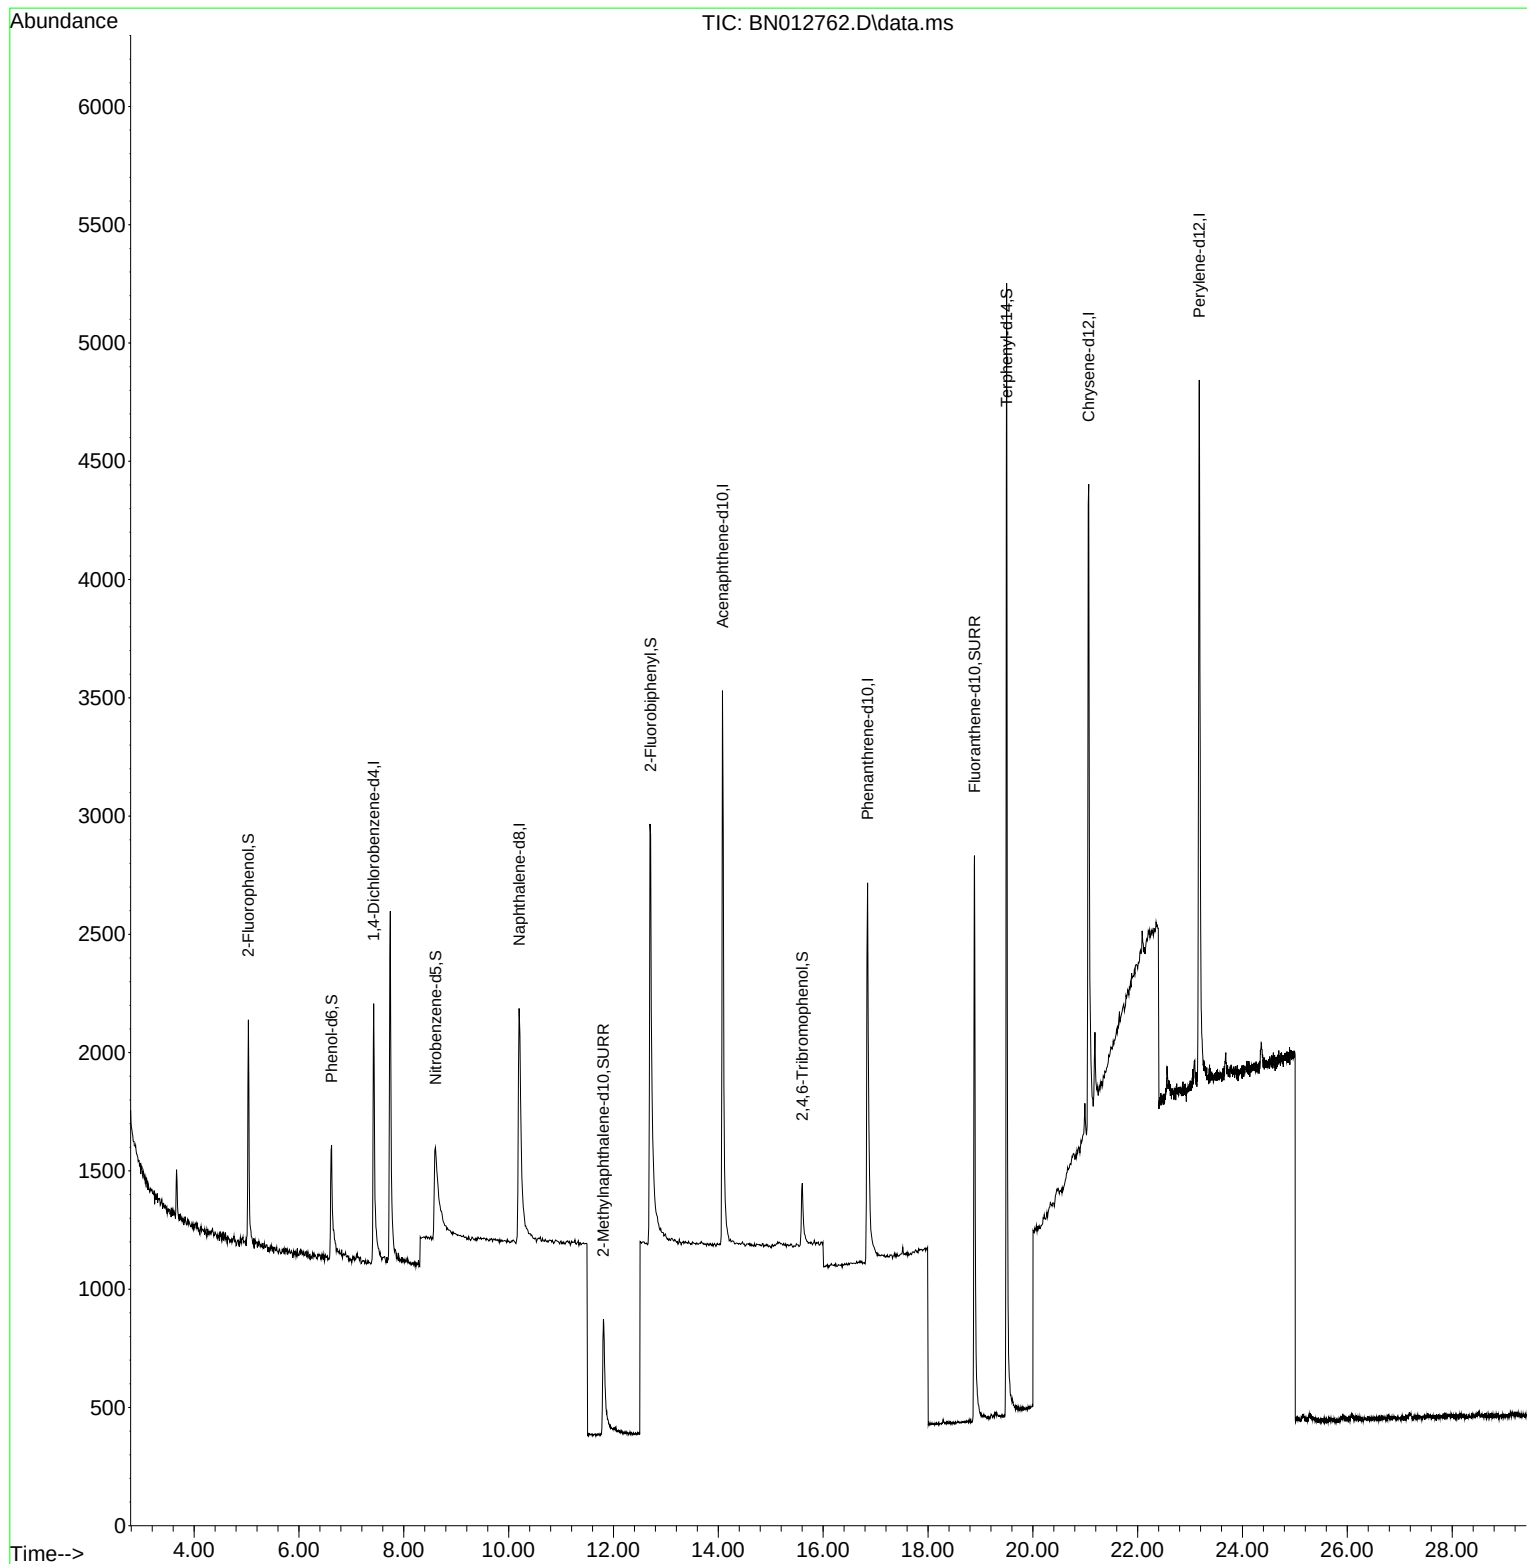


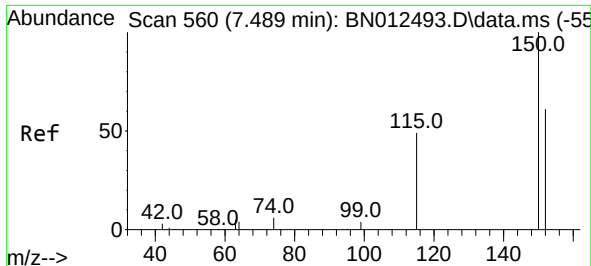


#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.426 min Scan# 577
Delta R.T. 0.001 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54





Tgt Ion:152 Resp: 784
Ion Ratio Lower Upper
152 100
150 147.6 116.6 174.8
115 73.5 52.9 79.3

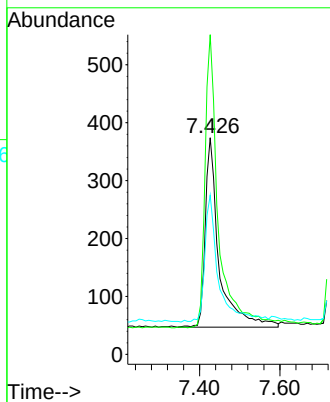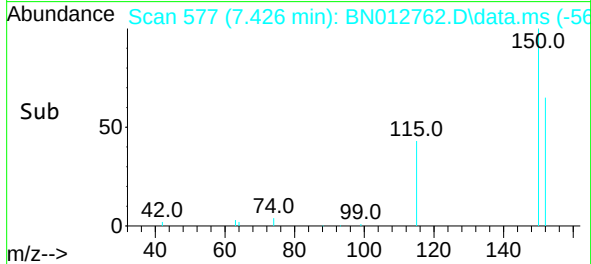

#4
2-Fluorophenol
Concen: 0.28 ng
RT: 5.035 min Scan# 280
Delta R.T. -0.007 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

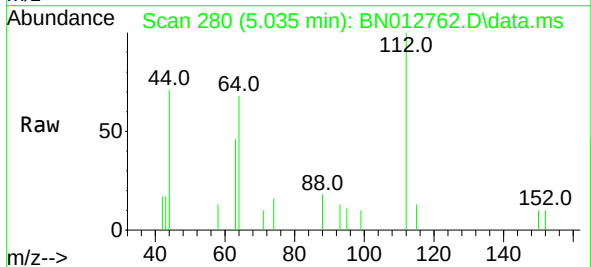


Tgt Ion:112 Resp: 755
Ion Ratio Lower Upper
112 100
64 66.4 49.5 74.3
63 39.6 32.0 48.0

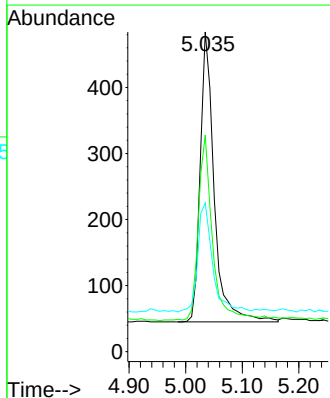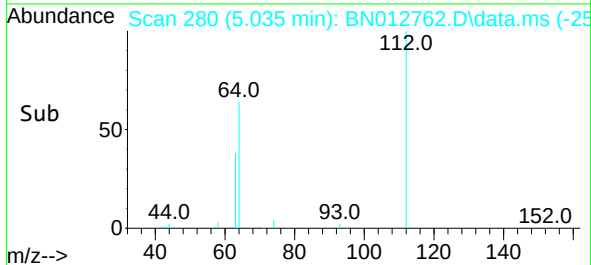

Instrument :
BNA_N
ClientSampleId :
PB133253BL

Manual Integrations
APPROVED

mohammad
12/1/2020 10:43:38 AM

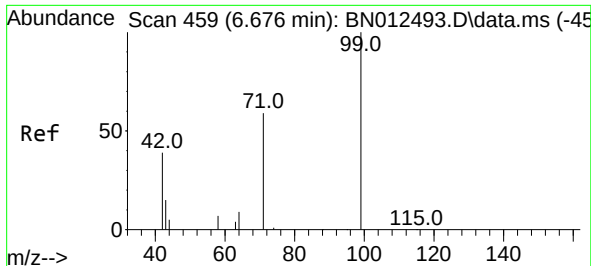





#5
Phenol-d6
Concen: 0.23 ng
RT: 6.621 min Scan# 477
Delta R.T. 0.001 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

Tgt Ion:	99	Resp:	734
Ion	Ratio	Lower	Upper
99	100		
42	28.1	22.4	33.6
71	43.7	37.8	56.6

Instrument :
BNA_N
ClientSampleId :
PB133253BL




Manual Integrations
APPROVED


mohammad
12/1/2020 10:43:38 AM

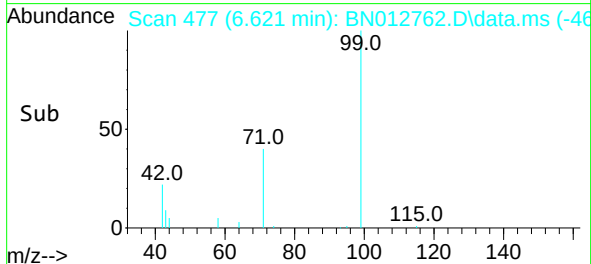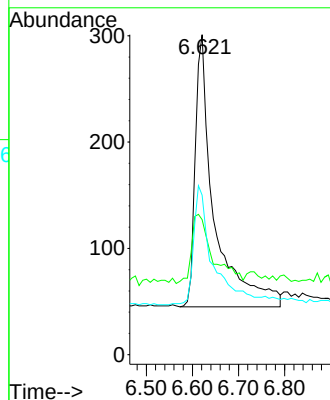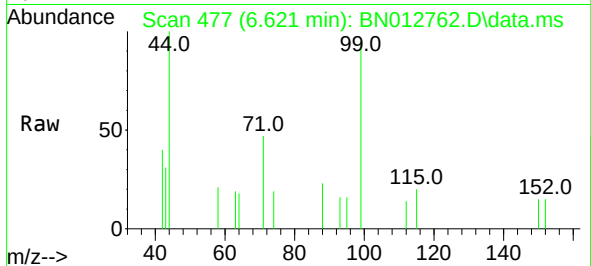

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.201 min Scan# 836
Delta R.T. 0.014 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54


Tgt Ion:	136	Resp:	2767
Ion	Ratio	Lower	Upper
136	100		
137	16.8	10.6	15.8#
54	14.4	8.6	12.8#
68	10.6	5.7	8.5#

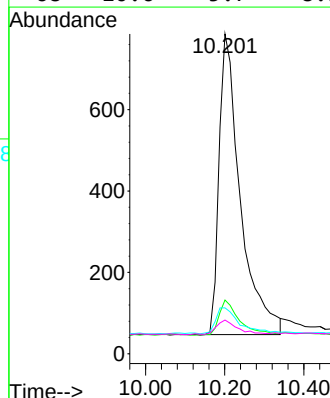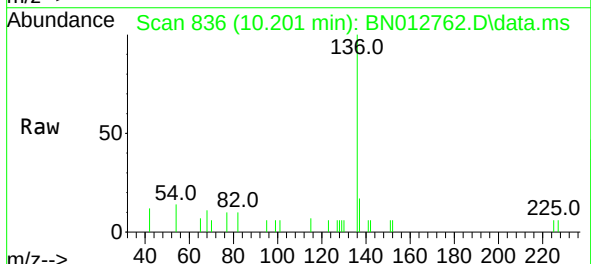

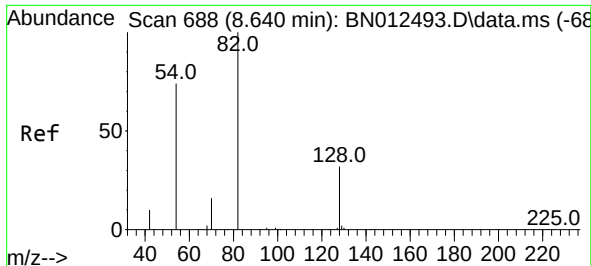

#8
Nitrobenzene-d5
Concen: 0.34 ng m
RT: 8.604 min Scan# 710
Delta R.T. 0.027 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54




Instrument :
BNA_N
ClientSampleId :
PB133253BL

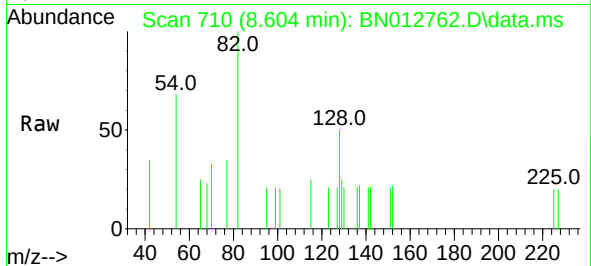


Tgt Ion: 82 Resp: 1103
Ion Ratio Lower Upper
82 100
128 50.0 30.6 46.0#
54 68.3 48.3 72.5

Manual Integrations
APPROVED



mohammad
12/1/2020 10:43:38 AM

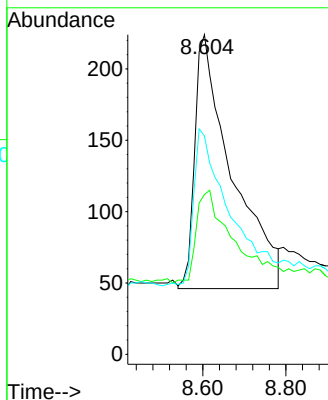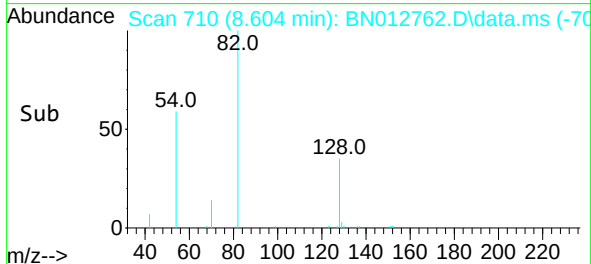


#11
2-Methylnaphthalene-d10
Concen: 0.31 ng
RT: 11.808 min Scan# 1007
Delta R.T. 0.011 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

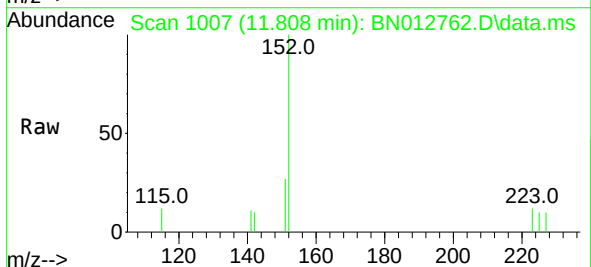


Tgt Ion: 152 Resp: 1394
Ion Ratio Lower Upper
152 100
151 18.7 16.7 25.1

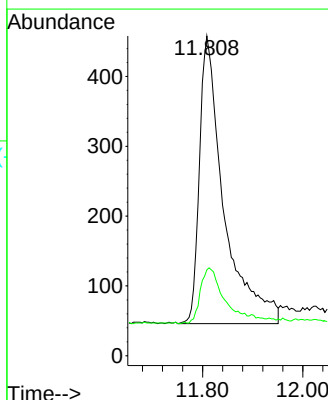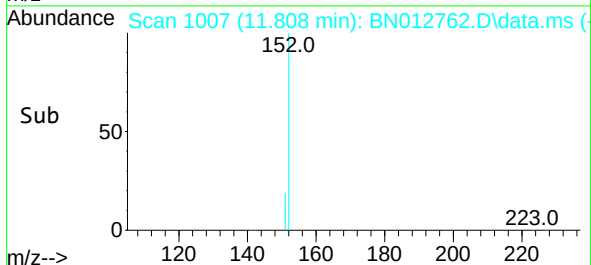

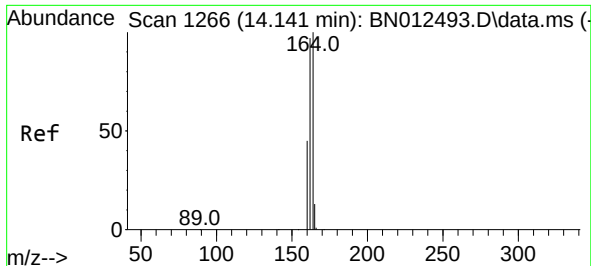

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.080 min Scan# 1288
Delta R.T. 0.002 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54




Instrument :
BNA_N
ClientSampleId :
PB133253BL




Tgt Ion:164 Resp: 1851
Ion Ratio Lower Upper
164 100
162 105.3 80.6 120.8
160 54.3 39.5 59.3

Manual Integrations
APPROVED



mohammad
12/1/2020 10:43:38 AM

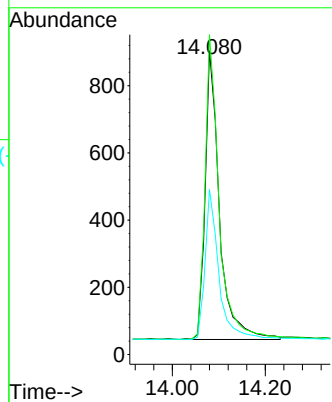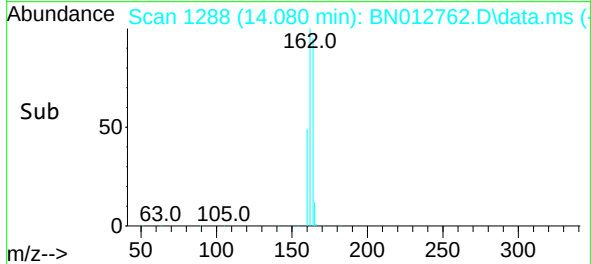


#14
2,4,6-Tribromophenol
Concen: 0.25 ng
RT: 15.602 min Scan# 1408
Delta R.T. 0.015 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

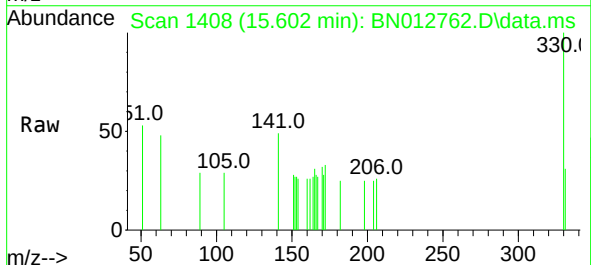


Tgt Ion:330 Resp: 331
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 45.0 34.4 51.6


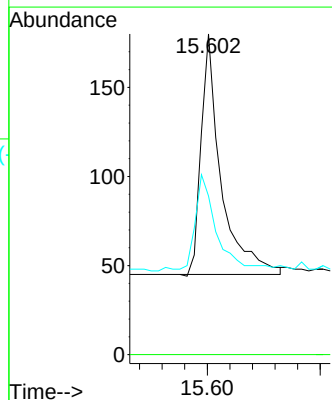
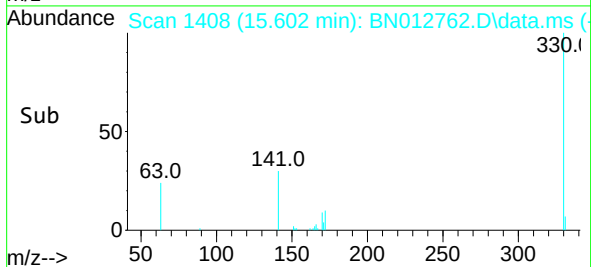


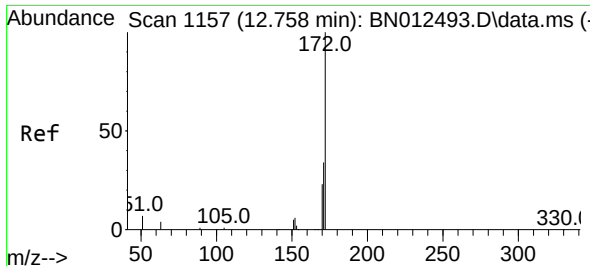


#15
2-Fluorobiphenyl
Concen: 0.42 ng
RT: 12.709 min Scan# 1180
Delta R.T. 0.015 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

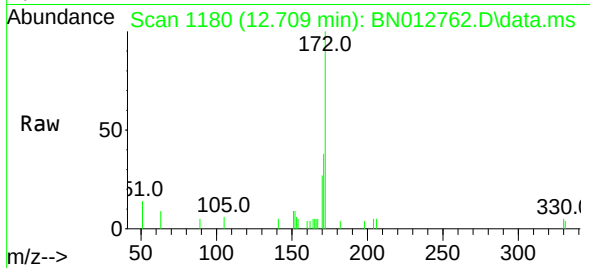



Tgt Ion:172 Resp: 3010
Ion Ratio Lower Upper
172 100
171 37.5 28.2 42.4
170 26.6 20.0 30.0

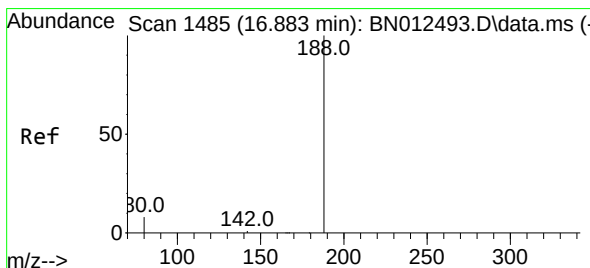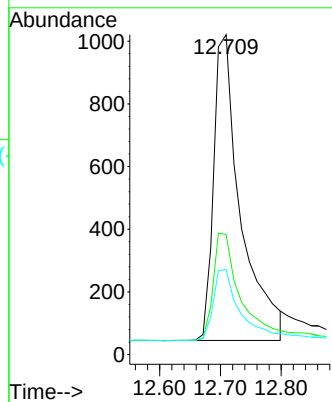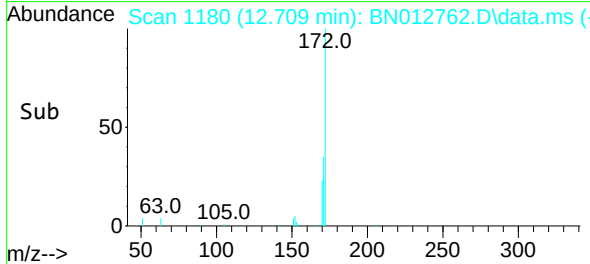

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.848 min Scan# 1509
Delta R.T. 0.014 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

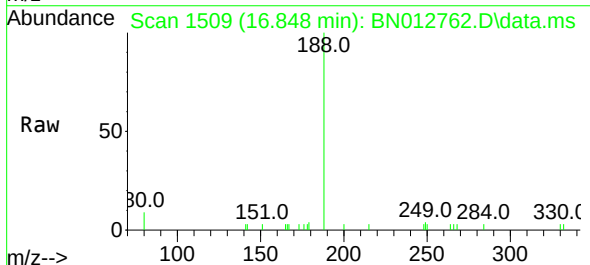


Tgt Ion:188 Resp: 4055
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.4 5.0 7.4#

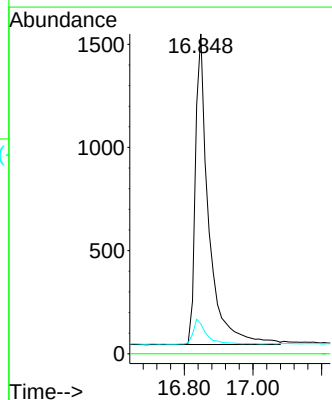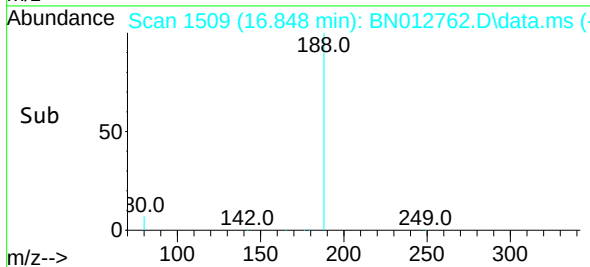

Instrument :
BNA_N
ClientSampleId :
PB133253BL

Manual Integrations
APPROVED

mohammad
12/1/2020 10:43:38 AM

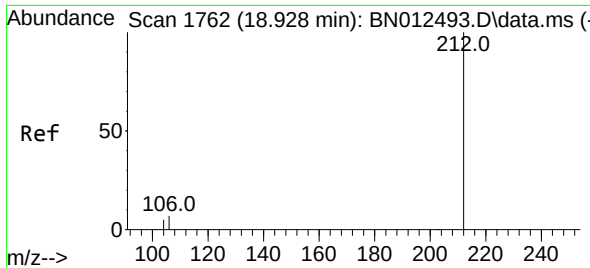





#27
Fluoranthene-d10
Concen: 0.31 ng
RT: 18.888 min Scan# 1782
Delta R.T. 0.004 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

Tgt Ion:212 Resp: 3925
Ion Ratio Lower Upper
212 100
106 8.7 6.8 10.2
104 5.5 4.1 6.1

Instrument :
BNA_N
ClientSampleId :
PB133253BL




Manual Integrations
APPROVED


mohammad
12/1/2020 10:43:38 AM

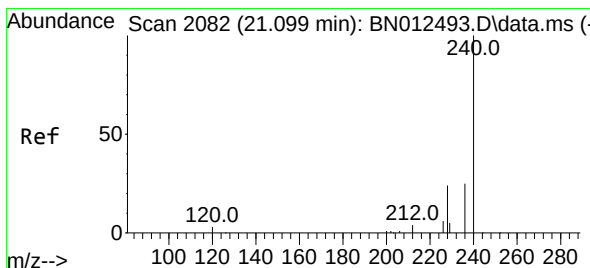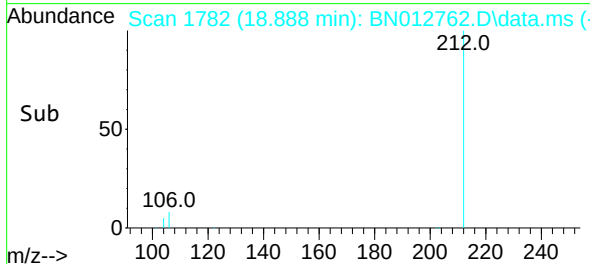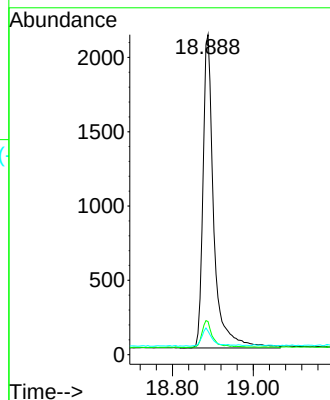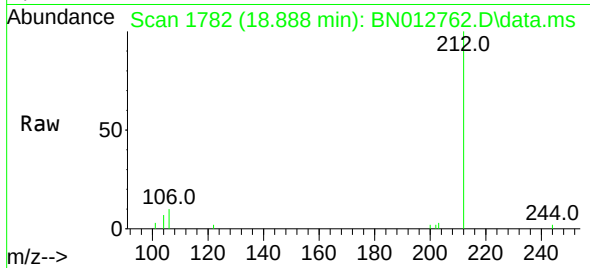


#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.067 min Scan# 2107
Delta R.T. 0.010 min
Lab File: BN012762.D
Acq: 30 Nov 2020 10:54

Tgt Ion:240 Resp: 4075
Ion Ratio Lower Upper
240 100
120 9.1 5.3 7.9#
236 27.5 21.8 32.8

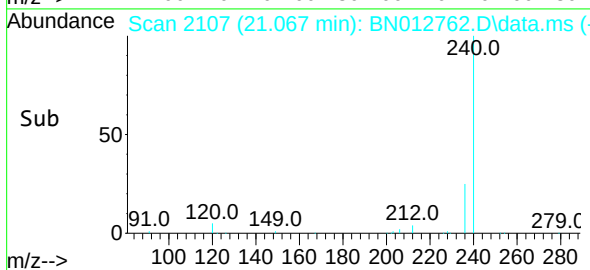
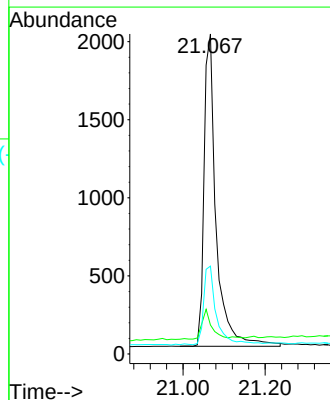
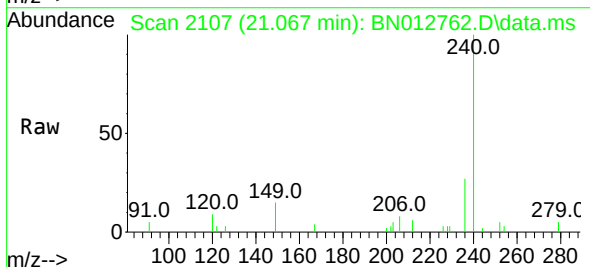





#31
 Terphenyl-d14
 Concen: 0.64 ng
 RT: 19.498 min Scan# 1905
 Delta R.T. -0.001 min
 Lab File: BN012762.D
 Acq: 30 Nov 2020 10:54





Tgt Ion:244 Resp: 6200
 Ion Ratio Lower Upper
 244 100
 212 9.5 7.3 10.9
 122 10.1 7.3 10.9

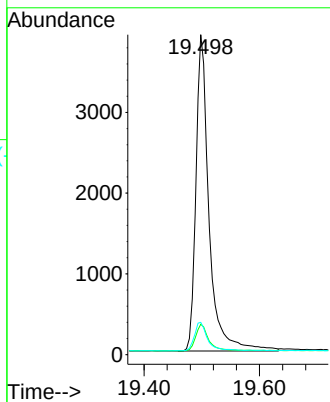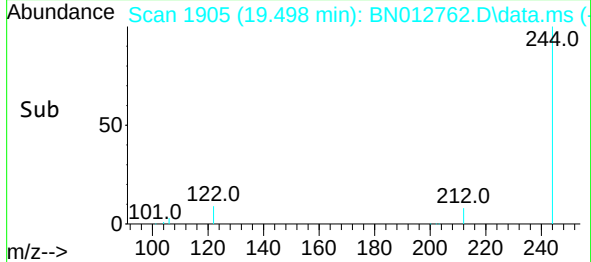

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.175 min Scan# 2458
 Delta R.T. 0.006 min
 Lab File: BN012762.D
 Acq: 30 Nov 2020 10:54

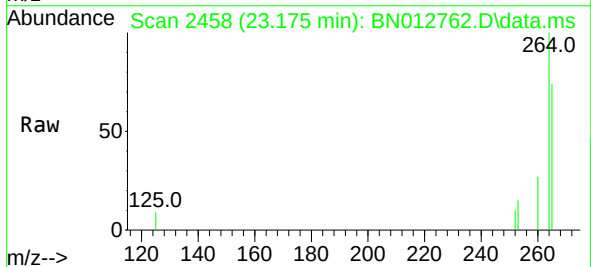

Tgt Ion:264 Resp: 4470
 Ion Ratio Lower Upper
 264 100
 260 27.3 19.8 29.6
 265 73.8 51.4 77.0

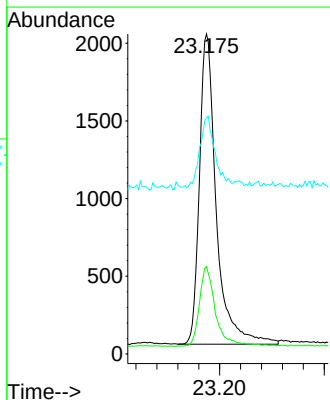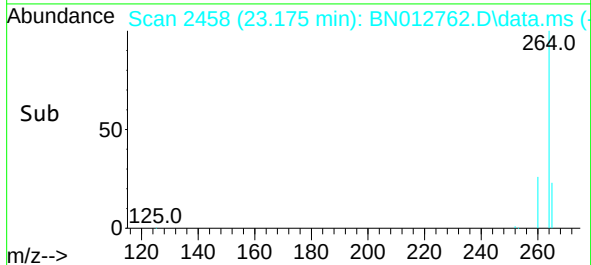

Instrument :
 BNA_N
 ClientSampleId :
 PB133253BL

Manual Integrations
 APPROVED

mohammad
 12/1/2020 10:43:38 AM