
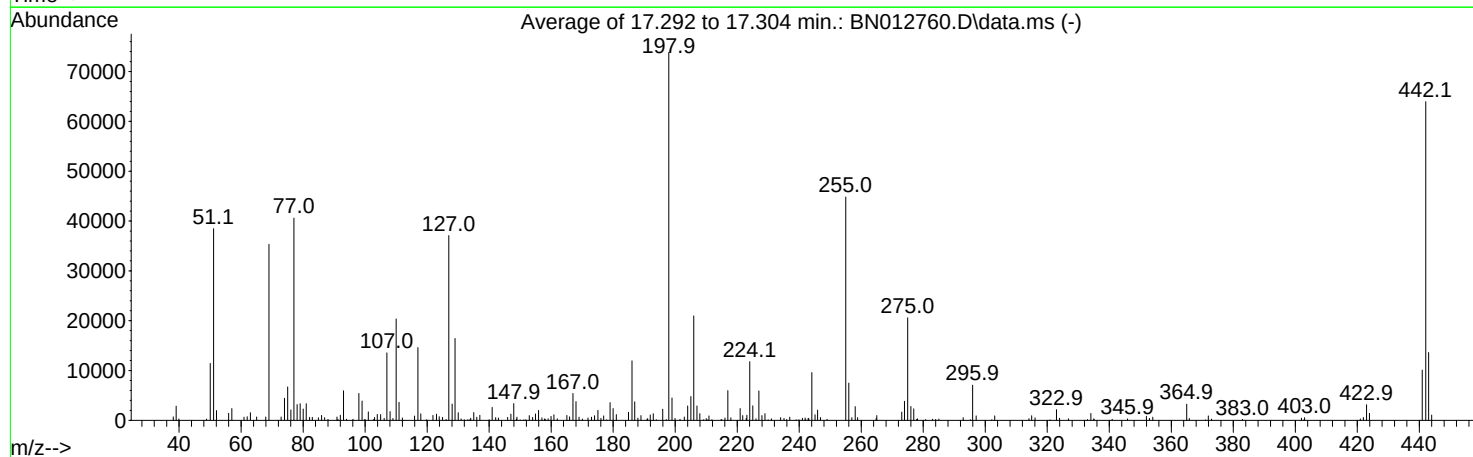


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113020\
 Data File : BN012760.D
 Acq On : 30 Nov 2020 09:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN110420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 27 15:36:21 2020

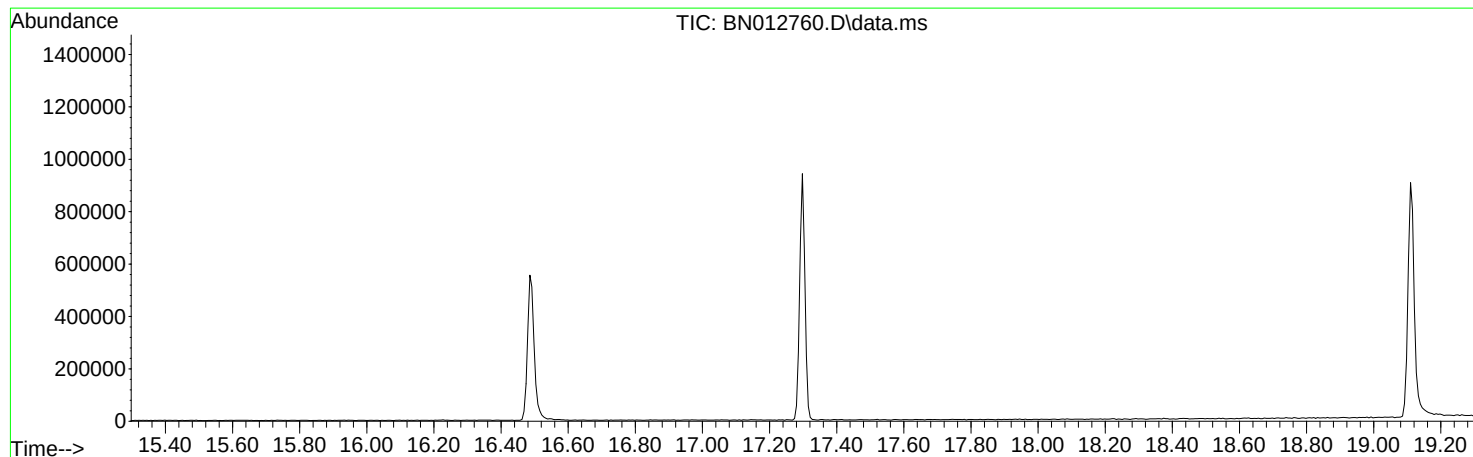

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	38485	PASS
68	69	0.00	2	1.9	687	PASS
69	198	0.00	100	47.8	35317	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	37093	PASS
197	198	0.00	2	0.2	150	PASS
198	198	100	100	100.0	73821	PASS
199	198	5	9	6.1	4514	PASS
275	198	10	60	27.9	20592	PASS
365	198	1	100	4.4	3238	PASS
441	198	0.01	100	13.6	10070	PASS
442	198	50	100	86.6	63960	PASS
443	442	15	24	21.3	13627	PASS