


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113022\
 Data File : BN022978.D
 Acq On : 30 Nov 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 11:51:26 2022

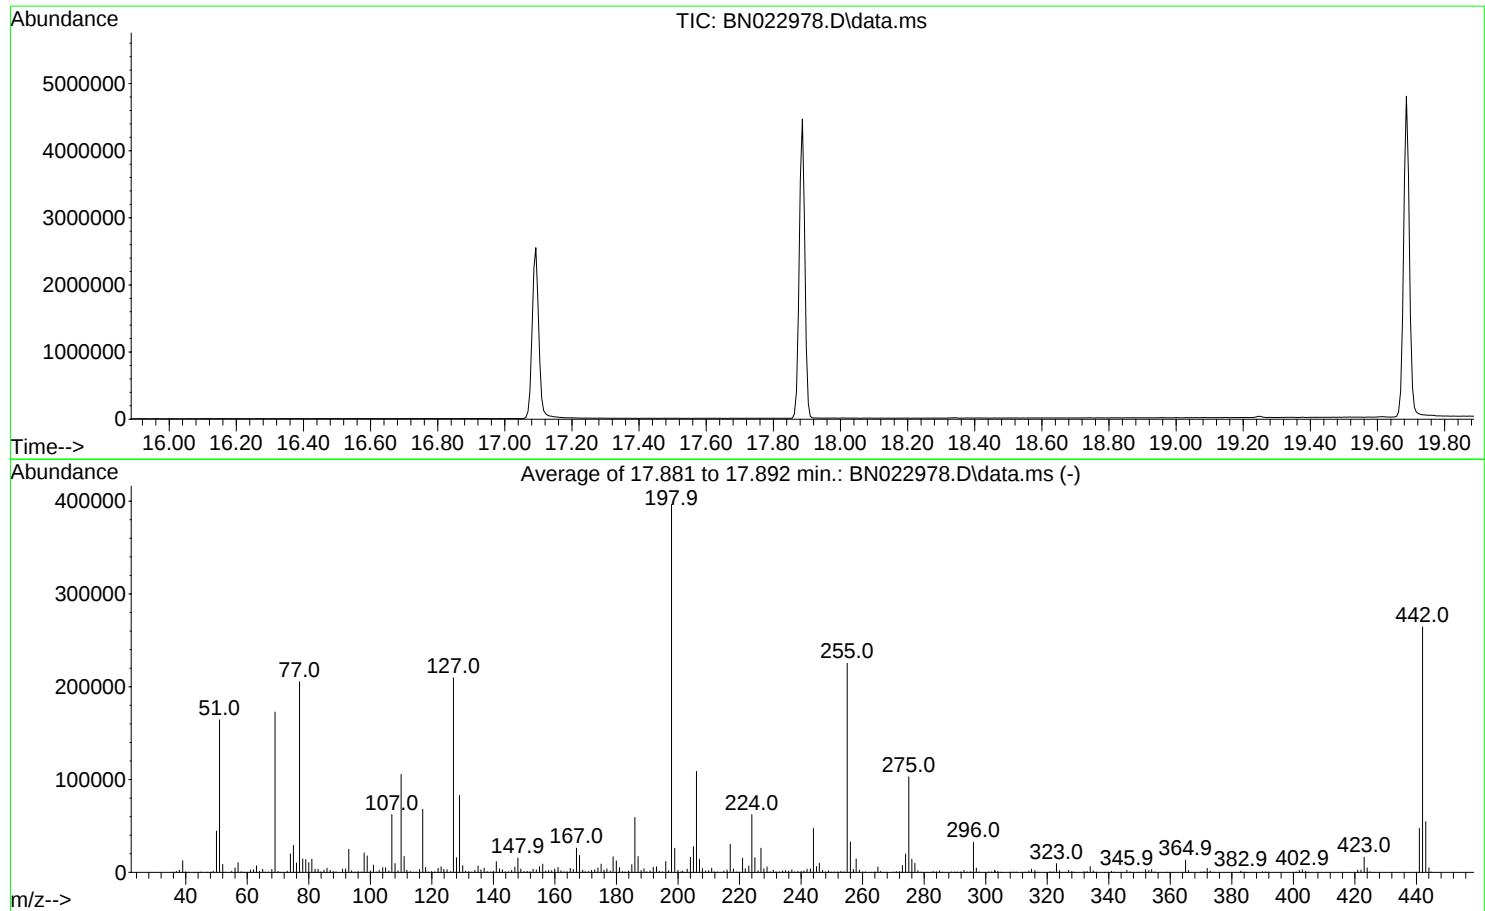




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	164144	PASS
68	69	0.00	2	1.7	2959	PASS
69	198	0.00	100	43.6	172725	PASS
70	69	0.00	2	0.6	1015	PASS
127	198	10	80	52.9	209621	PASS
197	198	0.00	2	0.5	1852	PASS
198	198	100	100	100.0	396395	PASS
199	198	5	9	6.5	25923	PASS
275	198	10	60	26.0	102888	PASS
365	198	1	100	3.3	13157	PASS
441	198	0.01	100	11.9	47245	PASS
442	442	50	100	100.0	264597	PASS
443	442	15	24	20.6	54579	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113022\
 Data File : BN022978.D
 Acq On : 30 Nov 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 01 04:40:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 01 04:40:35 2022
 Response via : Initial Calibration

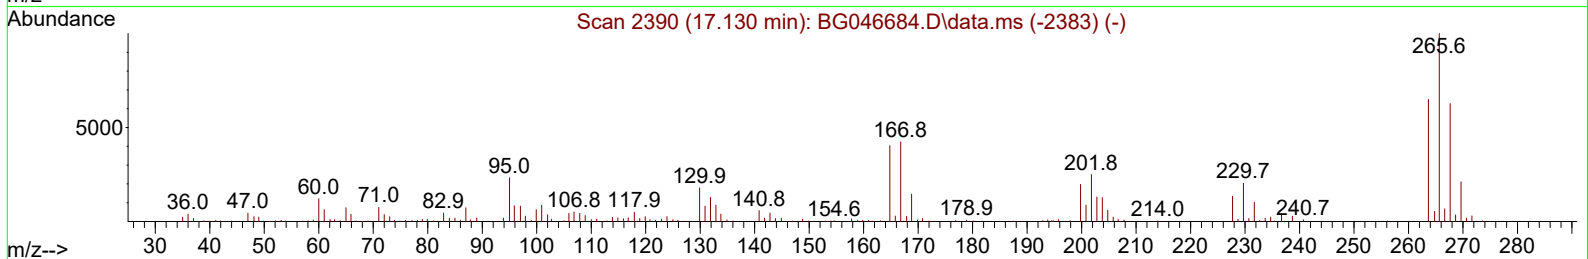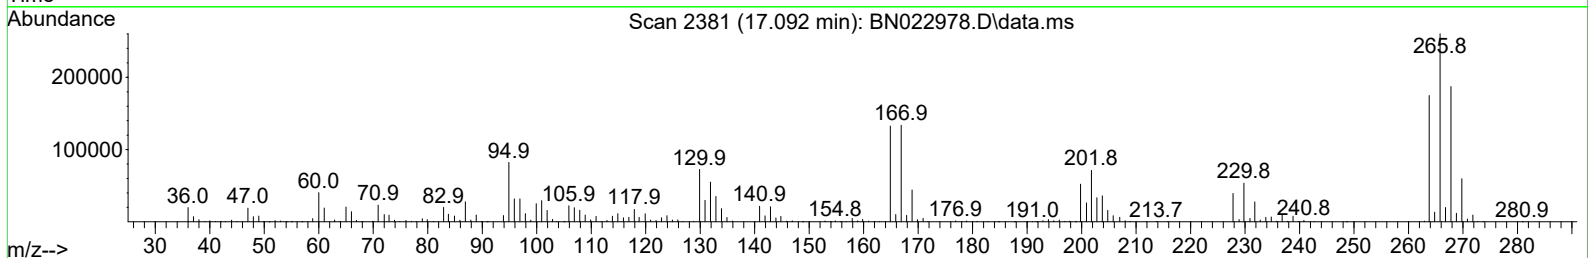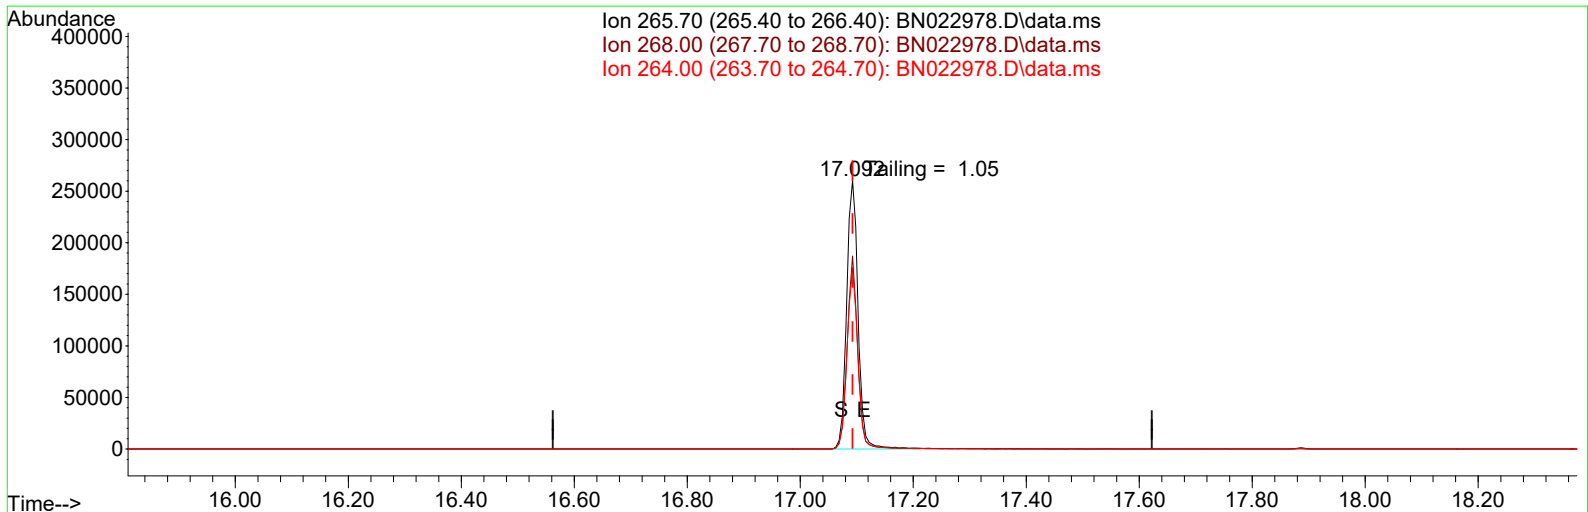

TIC: BN022978.D\data.ms

(70) Pentachlorophenol (C)

17.092min (0.000) 16740.61 ng




response 366802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.91
264.00	61.60	67.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN113022\
Data File : BN022978.D
Acq On : 30 Nov 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 01 04:40:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 01 04:40:35 2022
Response via : Initial Calibration

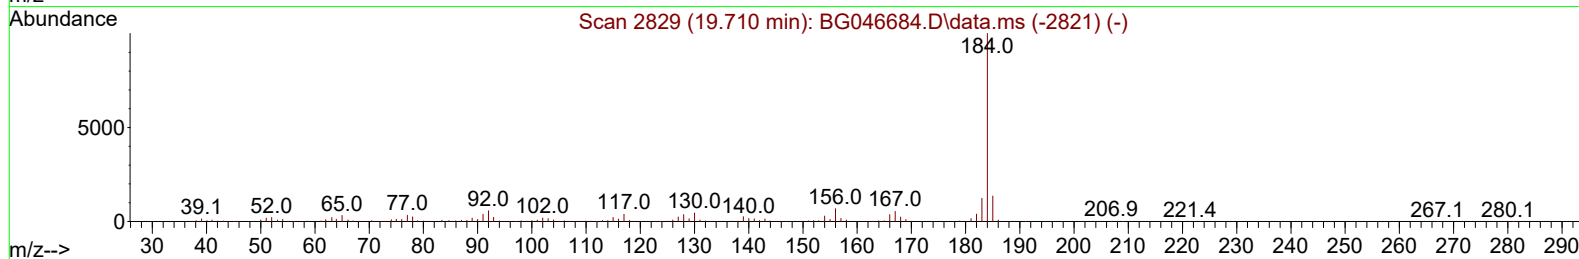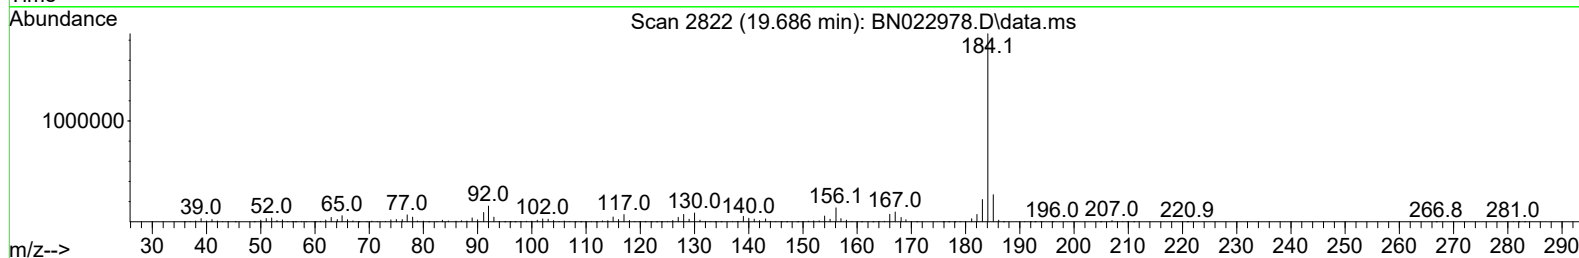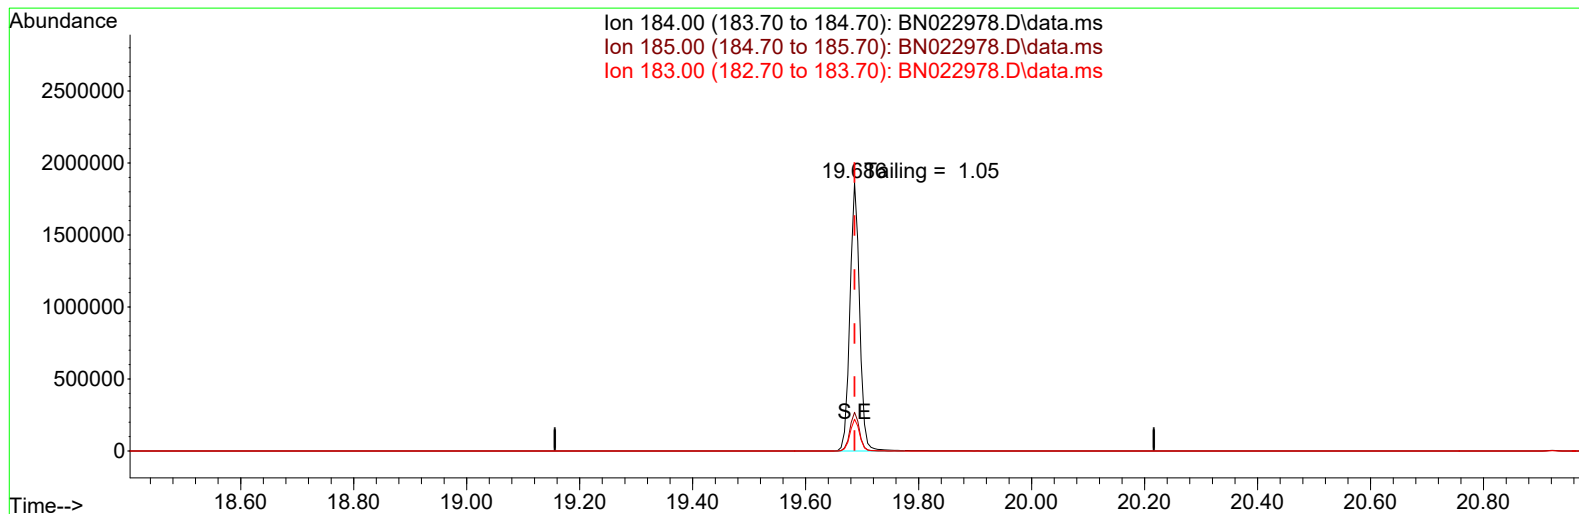

TIC: BN022978.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 2236553

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/30/2022	BNA_N	<u>BN022978.D</u>
Compound Name	Response	Retention Time
DDT	1070898	20.922
DDD	13718	20.533
DDE	435	19.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14153	1085051	1.30

Instrument :
BNA_N
ClientSampleId :
DFTPP