
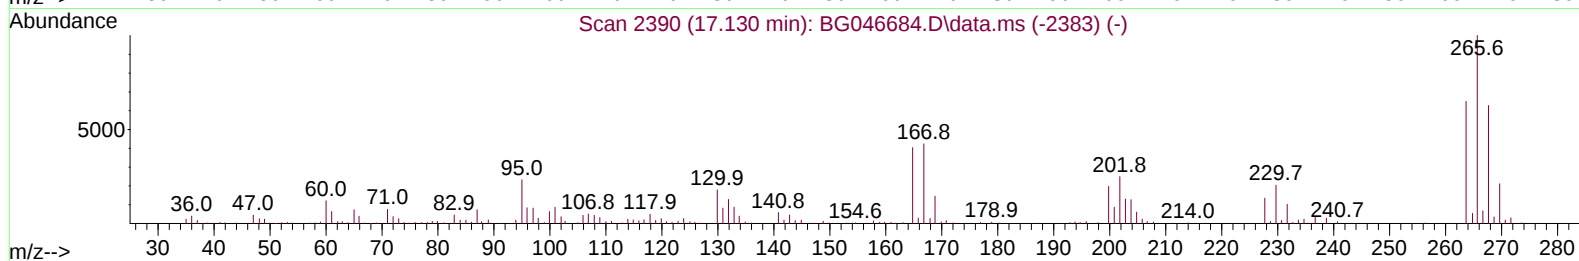
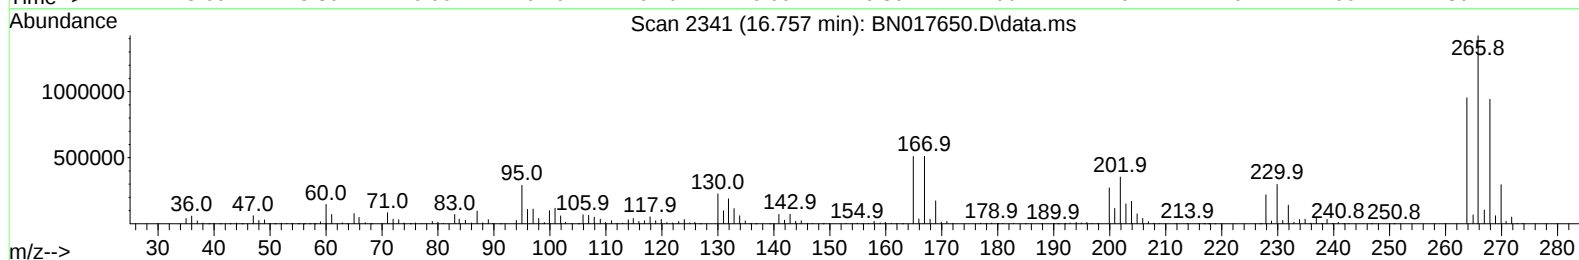


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120121\
 Data File : BN017650.D
 Acq On : 01 Dec 2021 14:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 02:31:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 02 02:31:15 2021
 Response via : Initial Calibration

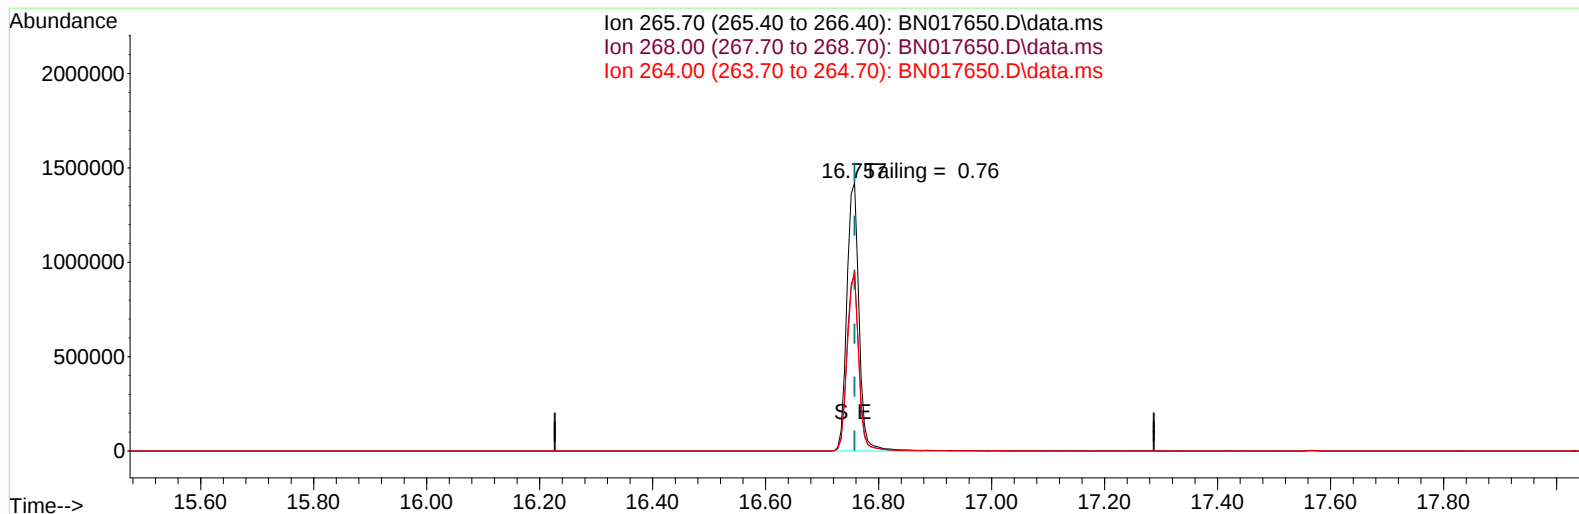

TIC: BN017650.D\data.ms

(70) Pentachlorophenol (C)




16.757min (0.000) 31334.70 ng

response 2127832

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.20
264.00	61.60	66.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120121\
 Data File : BN017650.D
 Acq On : 01 Dec 2021 14:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 02:31:25 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 02 02:31:15 2021
 Response via : Initial Calibration

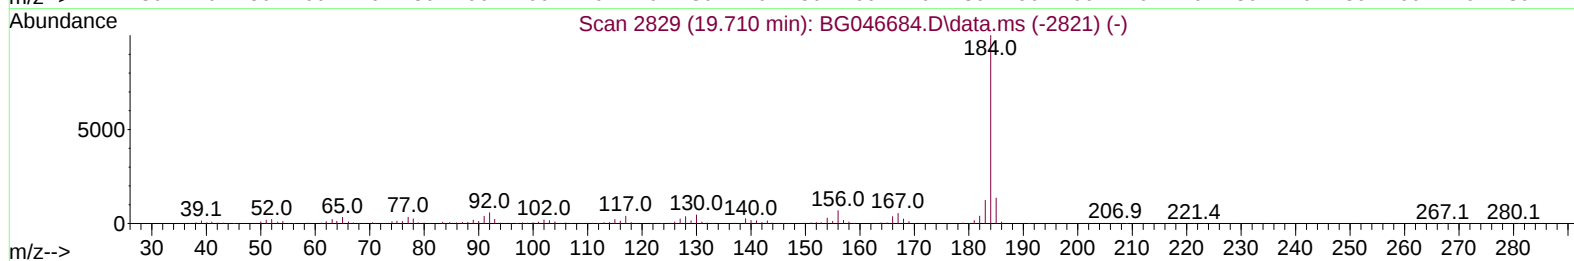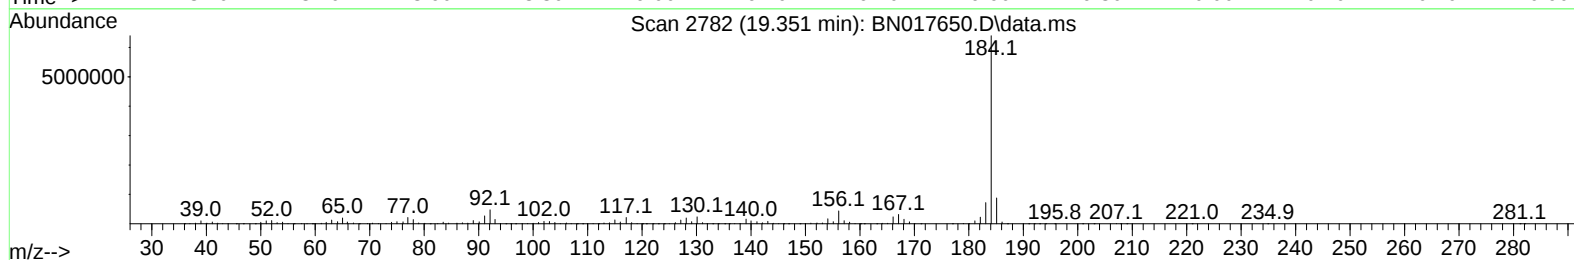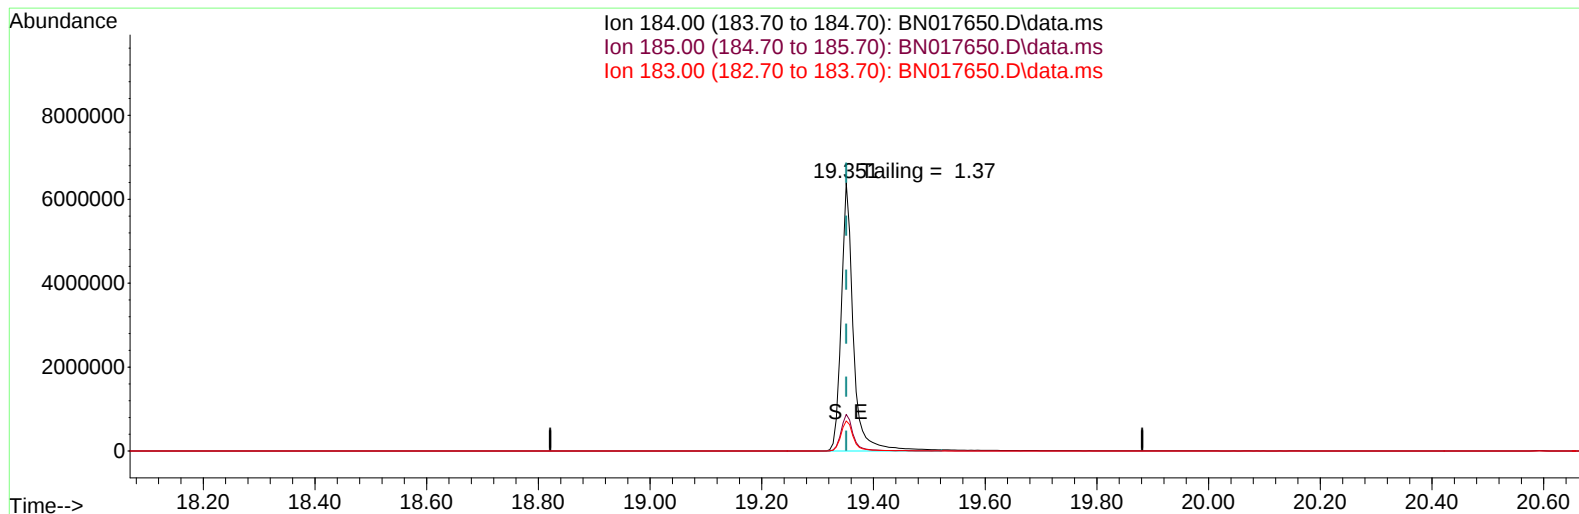

TIC: BN017650.D\data.ms

(77) Benzidine**19.351min (0.000) 2729508.43 ng****response 9760021**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.67
183.00	13.20	11.22
0.00	0.00	0.00