
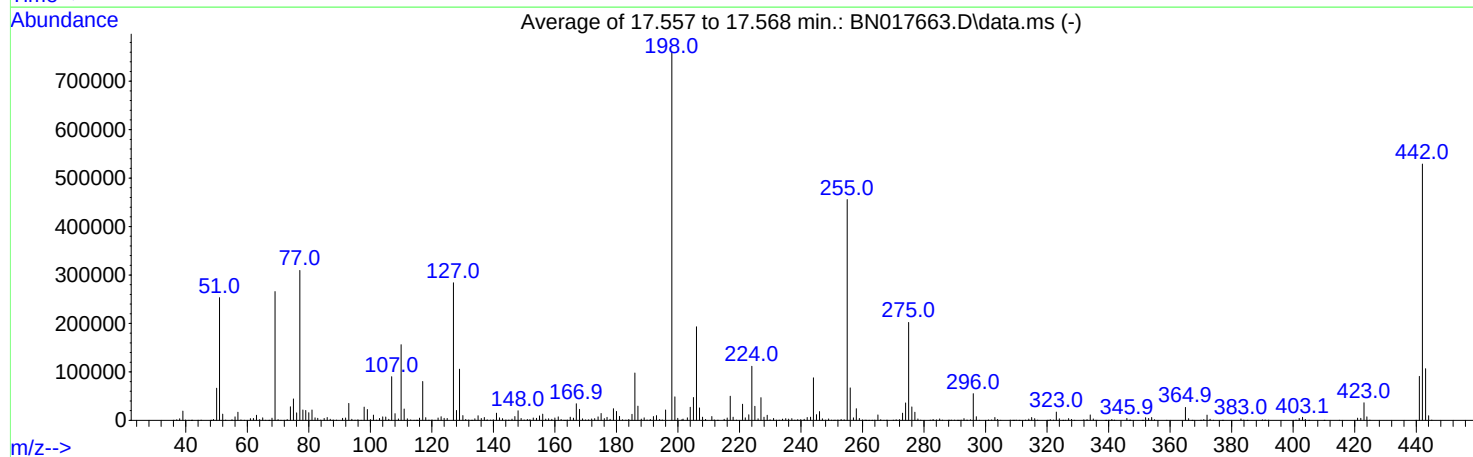


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120121\
 Data File : BN017663.D
 Acq On : 01 Dec 2021 23:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN113021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 02 01:51:49 2021

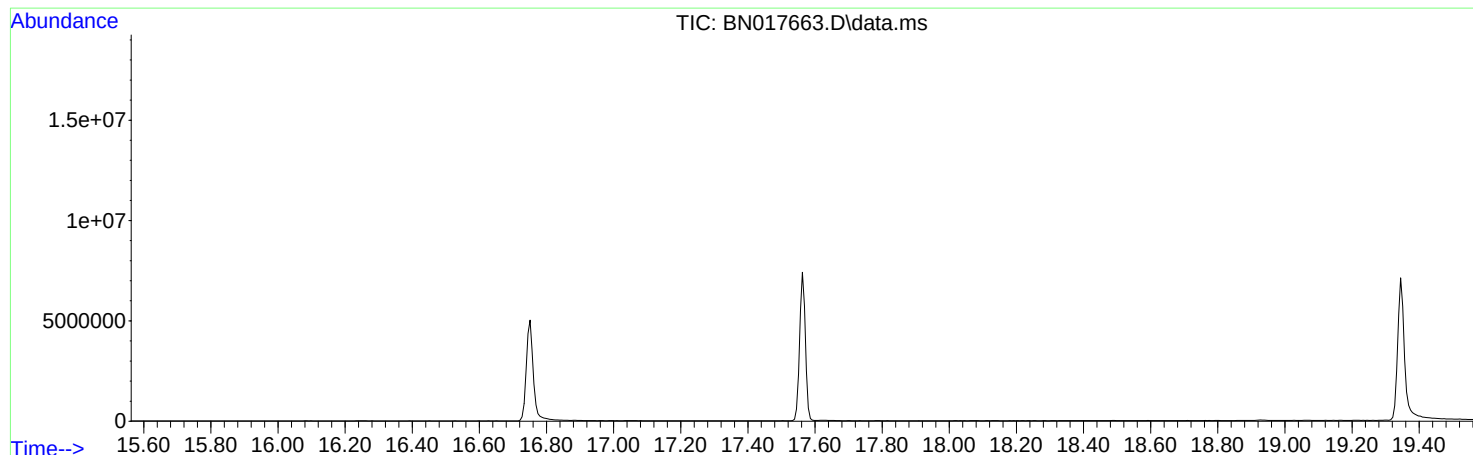




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	253197	PASS
68	69	0.00	2	1.7	4587	PASS
69	198	0.00	100	35.0	266002	PASS
70	69	0.00	2	0.6	1549	PASS
127	198	10	80	37.4	283968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	759211	PASS
199	198	5	9	6.4	48640	PASS
275	198	10	60	26.6	202155	PASS
365	198	1	100	3.5	26797	PASS
441	198	0.01	100	11.9	90659	PASS
442	442	50	100	100.0	528896	PASS
443	442	15	24	20.2	106845	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120121\
Data File : BN017663.D
Acq On : 01 Dec 2021 23:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 02 02:23:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 02 02:23:45 2021
Response via : Initial Calibration

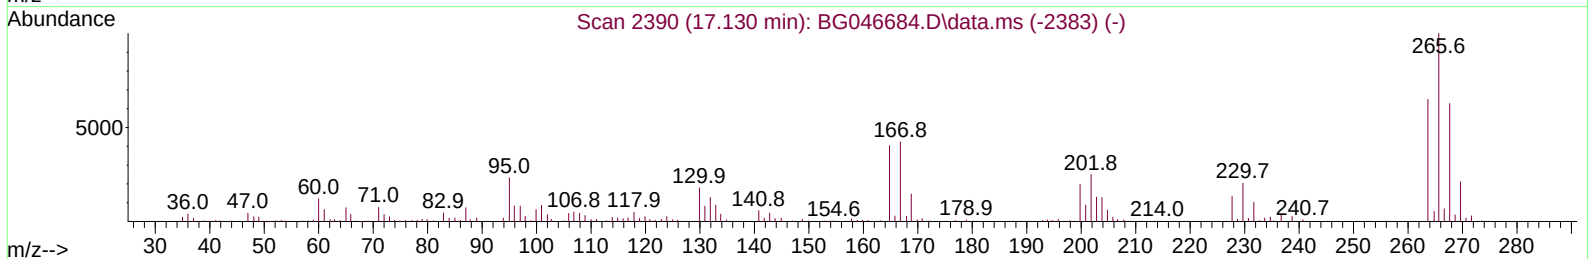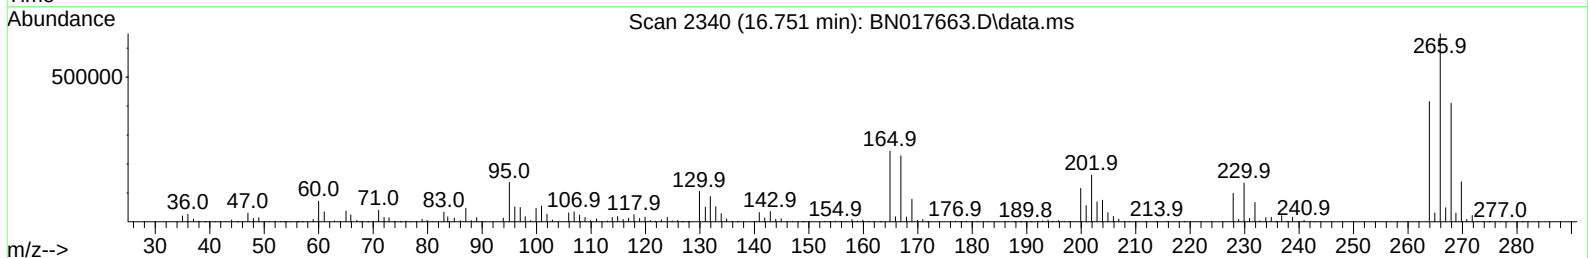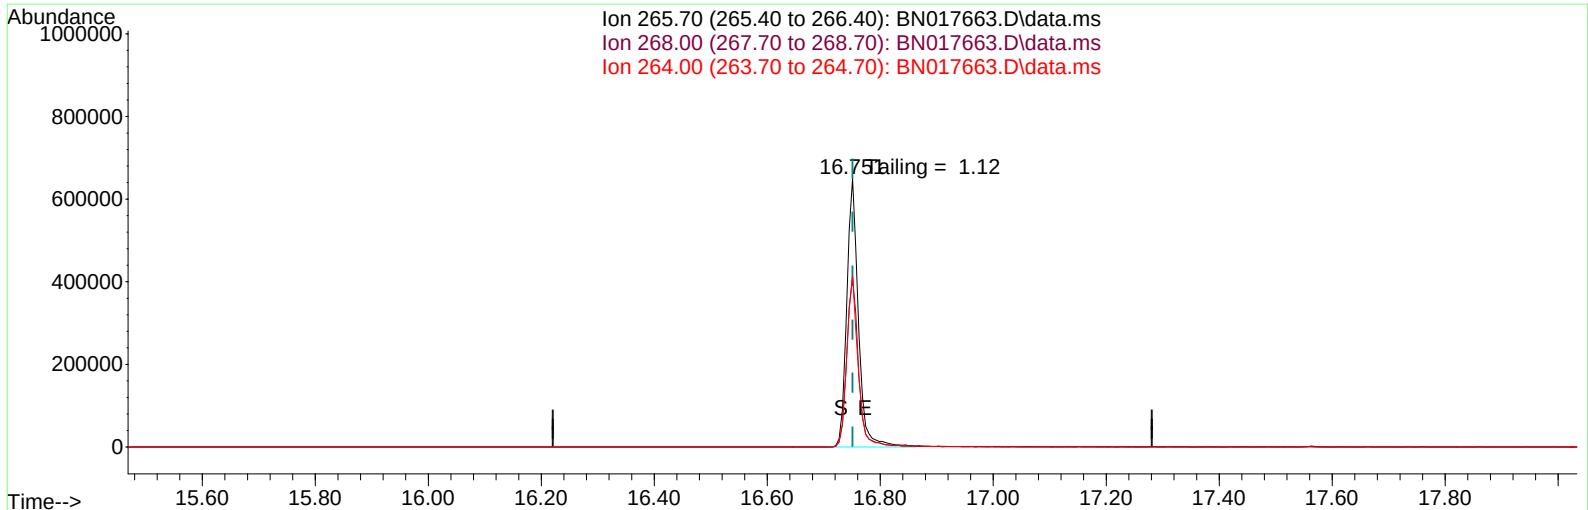

TIC: BN017663.D\data.ms

(70) Pentachlorophenol (C)

16.751min (0.000) 32662.79 ng




response 937140

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.09
264.00	61.60	63.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120121\
Data File : BN017663.D
Acq On : 01 Dec 2021 23:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 02 02:23:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 02 02:23:45 2021
Response via : Initial Calibration

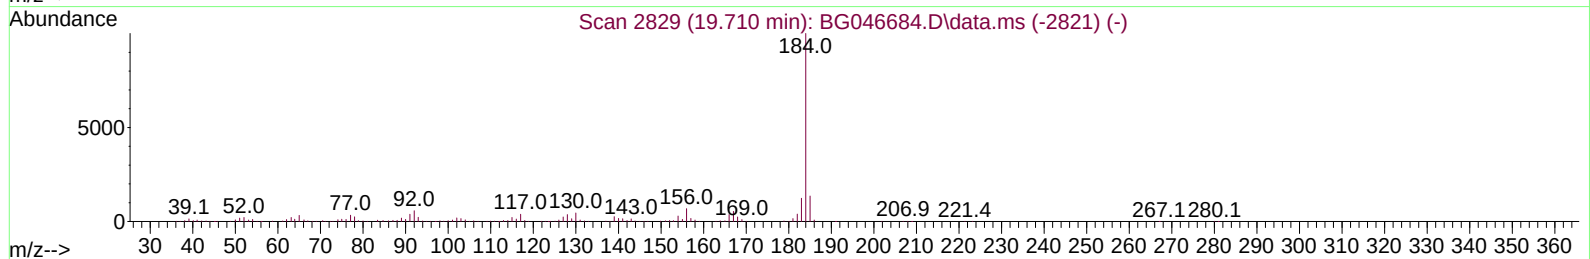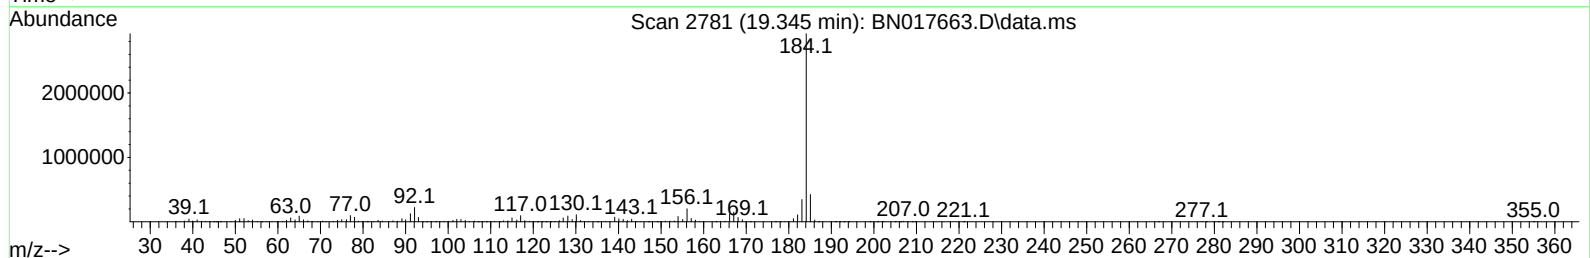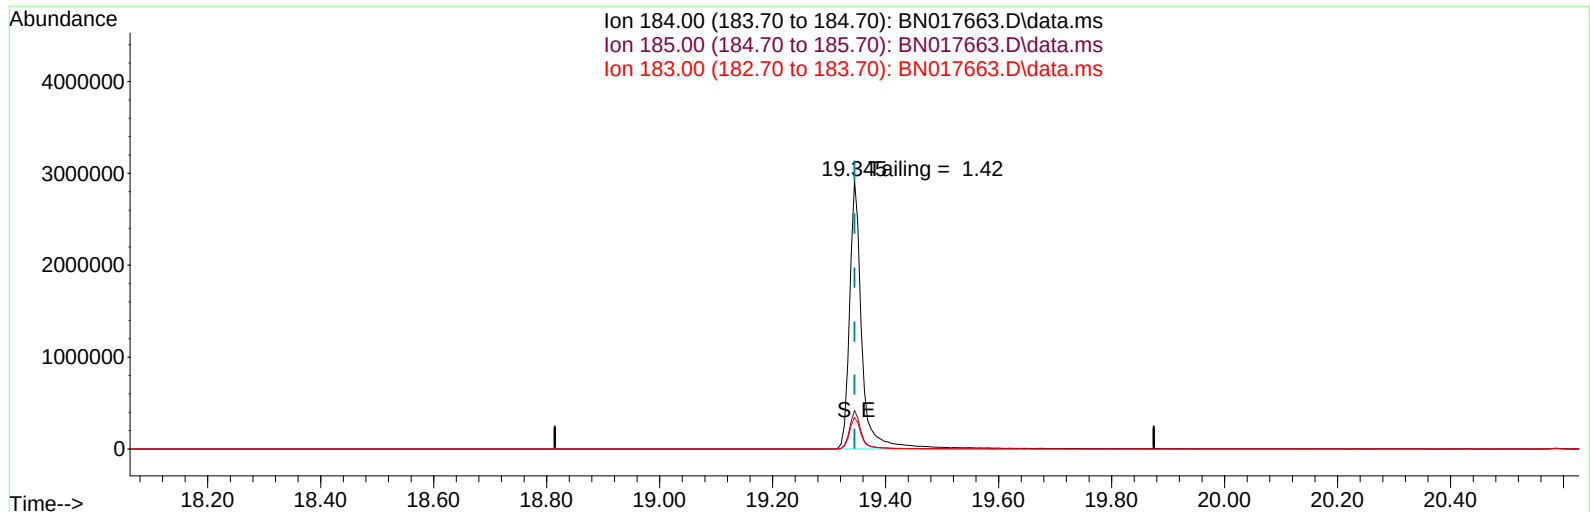

TIC: BN017663.D\data.ms

(77) Benzidine

19.345min (0.000) 0.00 ng

response 4431388

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.44
183.00	13.20	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2021	BNA_N	<u>BN017663.D</u>
Compound Name	Response	Retention Time
DDT	1750548	20.586
DDD	207727	20.145
DDE	732	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
208459	1959007	10.64

Instrument :
BNA_N
ClientSampleId :
DFTPP