

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
 Data File : BN023037.D
 Acq On : 02 Dec 2022 04:19
 Operator : CG/JU
 Sample : N5757-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 TT101D2-20221121

Quant Time: Dec 02 05:12:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 02:30:10 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.057	152	4756	0.400	ng	0.00
7) Naphthalene-d8	10.872	136	12462	0.400	ng	0.00
13) Acenaphthene-d10	14.688	164	5634	0.400	ng	0.00
19) Phenanthrene-d10	17.439	188	10622	0.400	ng	0.00
29) Chrysene-d12	21.616	240	6602	0.400	ng	# 0.00
35) Perylene-d12	24.097	264	4891	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.594	112	1408	0.114	ng	0.00
5) Phenol-d6	7.204	99	1068	0.068	ng	0.00
8) Nitrobenzene-d5	9.217	82	3328	0.344	ng	0.00
11) 2-Methylnaphthalene-d10	12.454	152	6726	0.249	ng	0.00
14) 2,4,6-Tribromophenol	16.186	330	581	0.214	ng	0.00
15) 2-Fluorobiphenyl	13.319	172	9596	0.372	ng	0.00
27) Fluoranthene-d10	19.464	212	8496	0.294	ng	0.00
31) Terphenyl-d14	20.058	244	6399	0.413	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.442	88	17000	2.816	ng	98
6) bis(2-Chloroethyl)ether	7.472	93	434	0.029	ng	98
32) Benzo(a)anthracene	21.598	228	702	0.026	ng	# 85
33) Chrysene	21.652	228	913	0.033	ng	# 89
34) Bis(2-ethylhexyl)phtha...	21.527	149	778	0.073	ng	# 92
36) Indeno(1,2,3-cd)pyrene	26.693	276	675	0.033	ng	# 91
37) Benzo(b)fluoranthene	23.337	252	852	0.039	ng	# 8
38) Benzo(k)fluoranthene	23.390	252	727	0.031	ng	# 1
39) Benzo(a)pyrene	23.986	252	362	0.022	ng	# 1
40) Dibenzo(a,h)anthracene	26.717	278	596	0.037	ng	# 25
41) Benzo(g,h,i)perylene	27.491	276	666	0.038	ng	# 52

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023037.D
Acq On : 02 Dec 2022 04:19
Operator : CG/JU
Sample : N5757-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Quant Time: Dec 02 05:12:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 02:30:10 2022
Response via : Initial Calibration

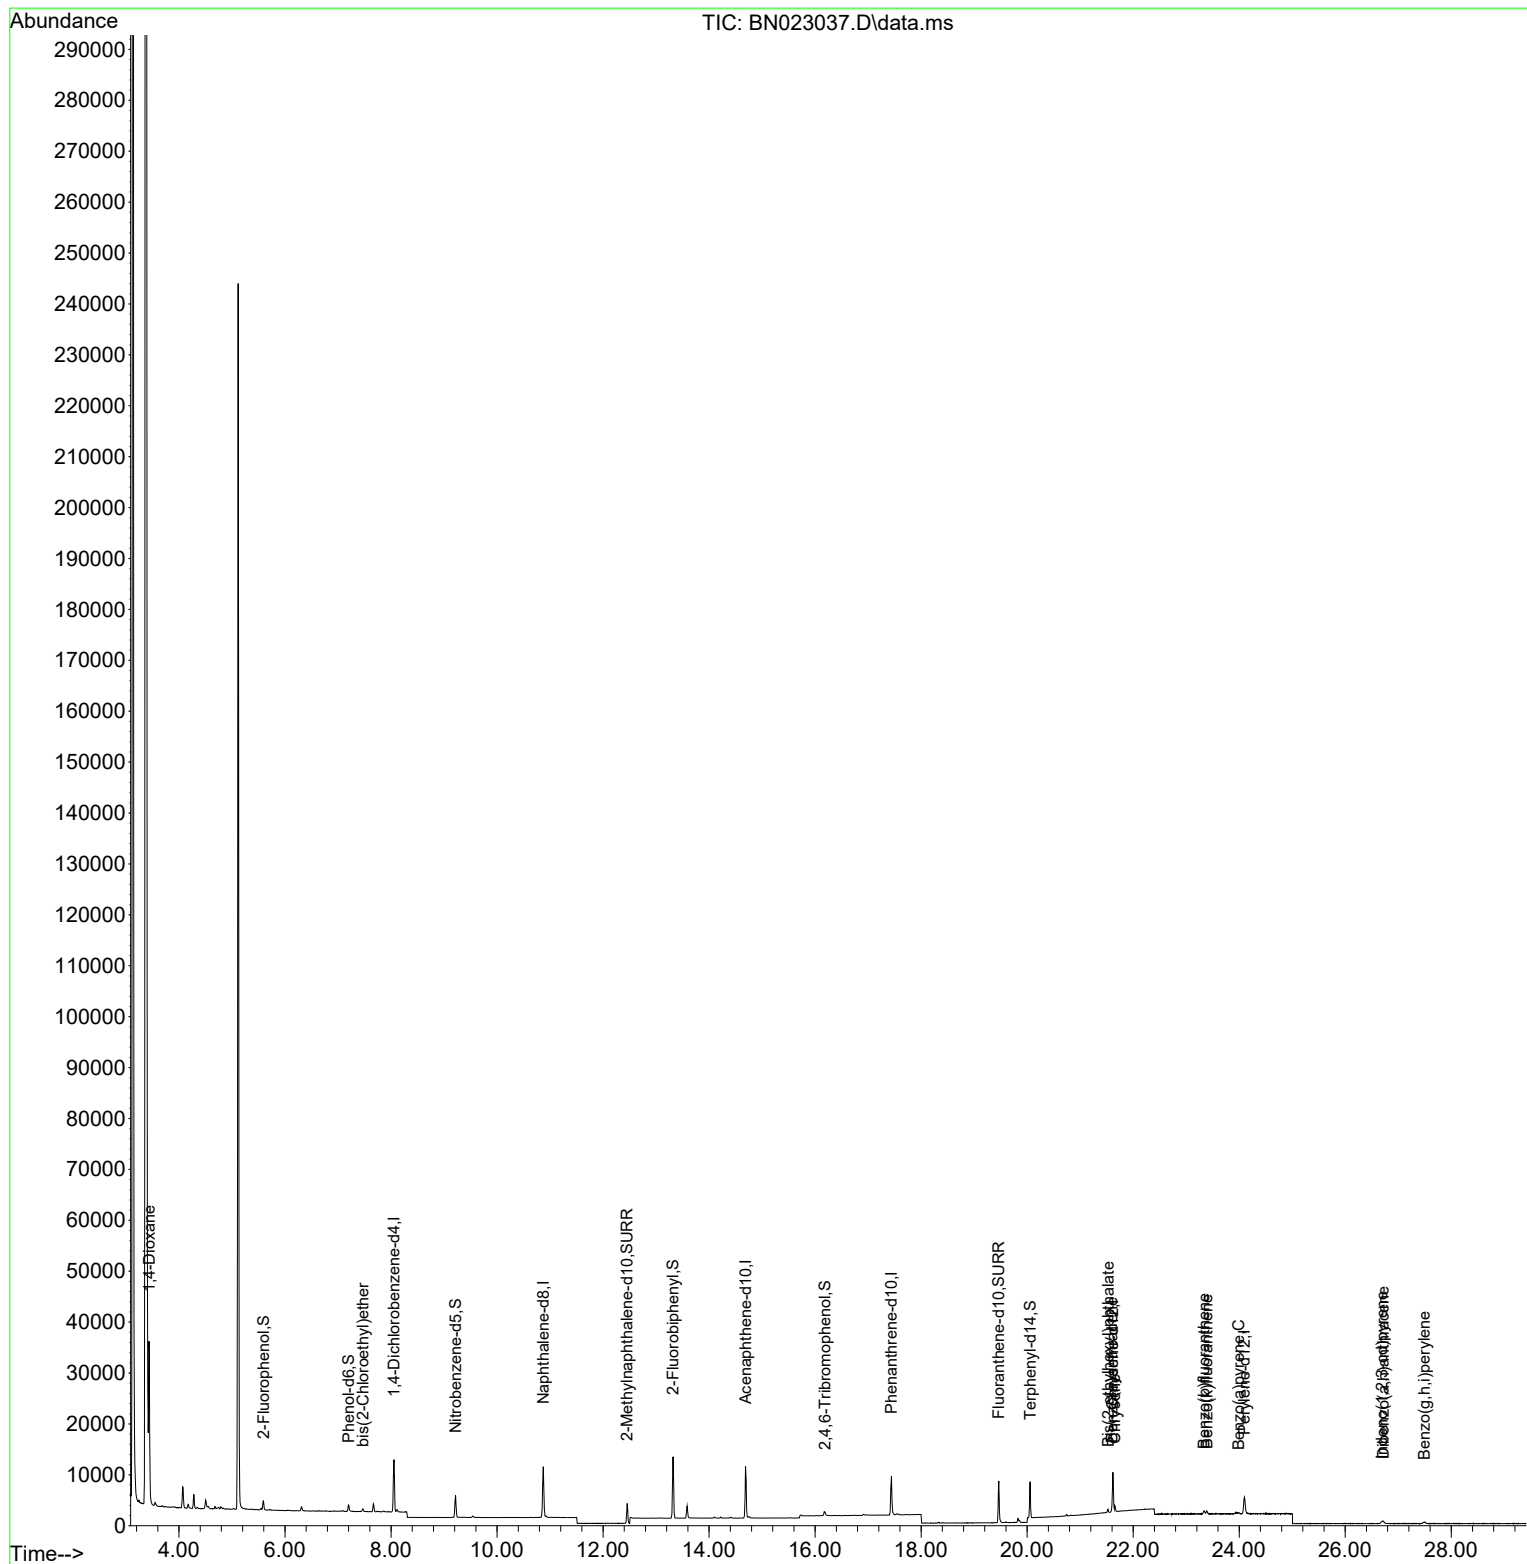






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.057 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN023037.D
 Acq: 02 Dec 2022 04:19


Instrument :
 BNA_N
 ClientSampleId :
 TT101D2-20221121





Tgt Ion:152 Resp: 4756
 Ion Ratio Lower Upper
 152 100
 150 152.9 121.2 181.8
 115 61.1 46.2 69.4

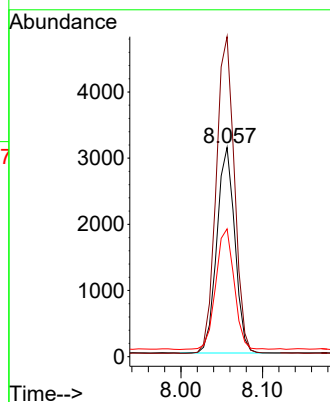

#2
 1,4-Dioxane
 Concen: 2.816 ng
 RT: 3.442 min Scan# 50
 Delta R.T. -0.000 min
 Lab File: BN023037.D
 Acq: 02 Dec 2022 04:19



Tgt Ion: 88 Resp: 17000
 Ion Ratio Lower Upper
 88 100
 43 33.4 25.4 38.2
 58 69.5 56.5 84.7



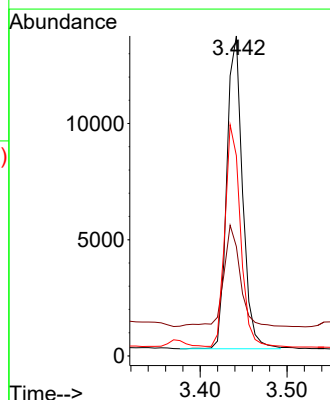
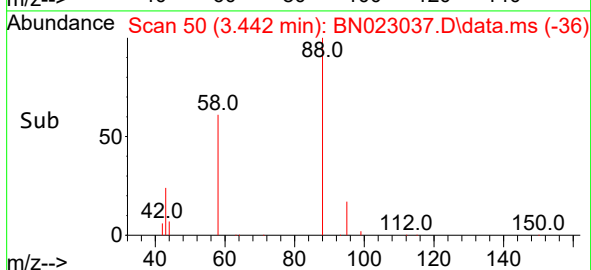




#4
2-Fluorophenol
Concen: 0.114 ng
RT: 5.594 min Scan# 34
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion:112 Resp: 1408
Ion Ratio Lower Upper
112 100
64 55.5 43.4 65.2
63 30.1 23.4 35.2

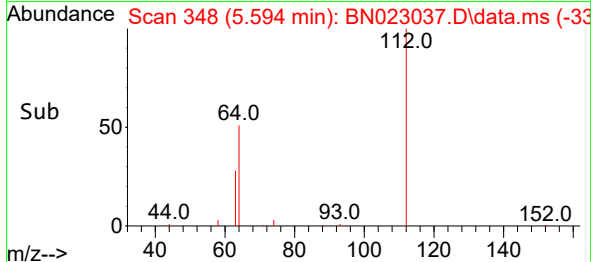

#5
Phenol-d6
Concen: 0.068 ng
RT: 7.204 min Scan# 571
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion: 99 Resp: 1068
Ion Ratio Lower Upper
99 100
42 25.2 16.0 24.0#
71 41.4 26.8 40.2#


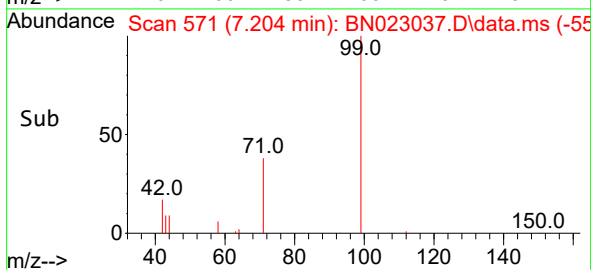

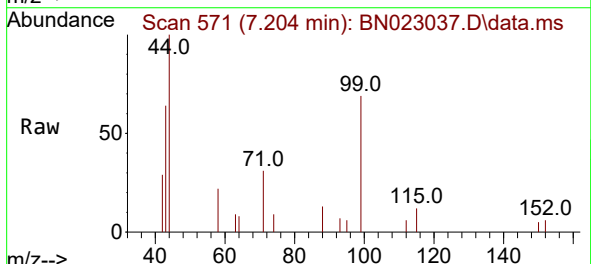




#6
bis(2-Chloroethyl)ether
Concen: 0.029 ng
RT: 7.472 min Scan# 608
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion: 93 Resp: 434
Ion Ratio Lower Upper
93 100
63 71.9 58.3 87.5
95 29.7 25.8 38.6

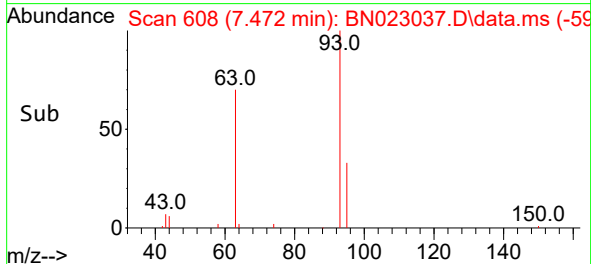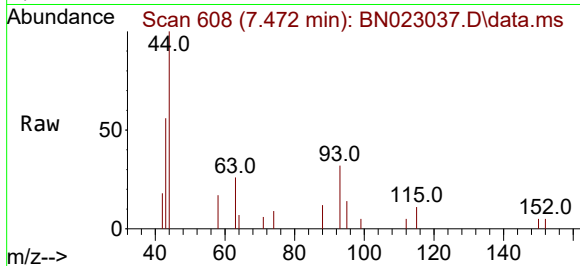

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.872 min Scan# 964
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion: 136 Resp: 12462
Ion Ratio Lower Upper
136 100
137 11.6 9.0 13.4
54 8.5 6.6 9.8
68 6.7 5.5 8.3


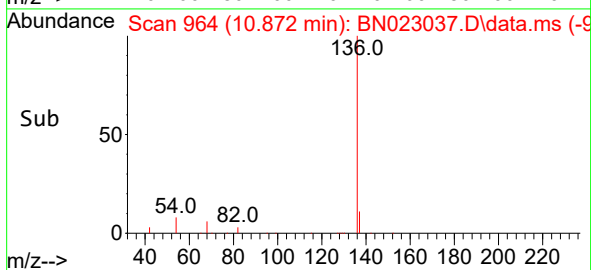

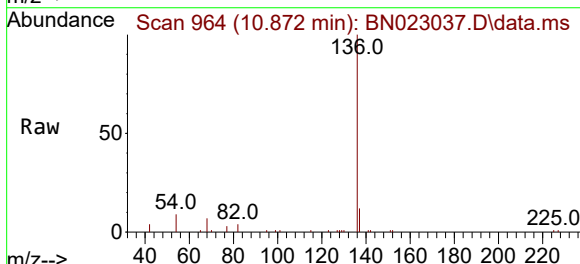




#8
Nitrobenzene-d5
Concen: 0.344 ng
RT: 9.217 min Scan# 809
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion: 82 Resp: 3328
Ion Ratio Lower Upper
82 100
128 42.0 36.6 54.8
54 50.5 38.5 57.7

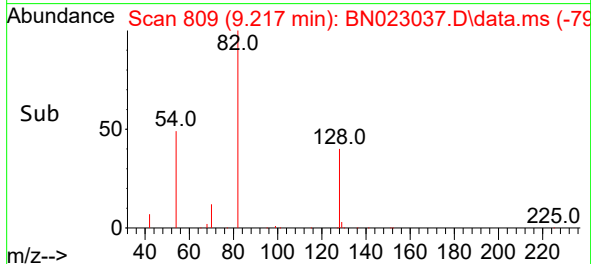

#11
2-Methylnaphthalene-d10
Concen: 0.249 ng
RT: 12.454 min Scan# 1273
Delta R.T. -0.004 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion: 152 Resp: 6726
Ion Ratio Lower Upper
152 100
151 17.6 18.6 27.8#


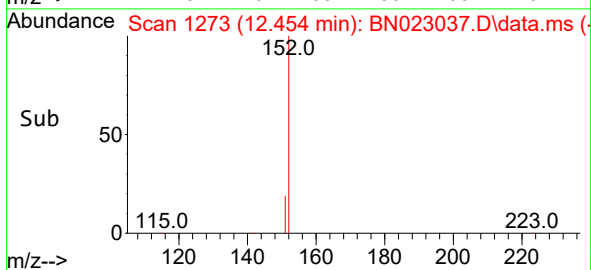

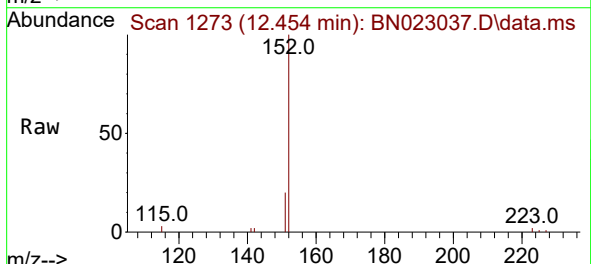




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.688 min Scan# 1491
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion:164 Resp: 5634
Ion Ratio Lower Upper
164 100
162 104.3 84.2 126.4
160 55.9 42.5 63.7

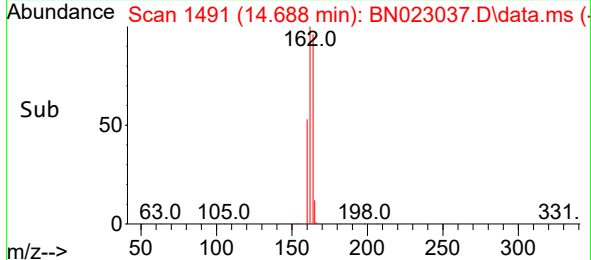

#14
2,4,6-Tribromophenol
Concen: 0.214 ng
RT: 16.186 min Scan# 1625
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion:330 Resp: 581
Ion Ratio Lower Upper
330 100
332 98.1 76.5 114.7
141 47.0 32.6 48.8


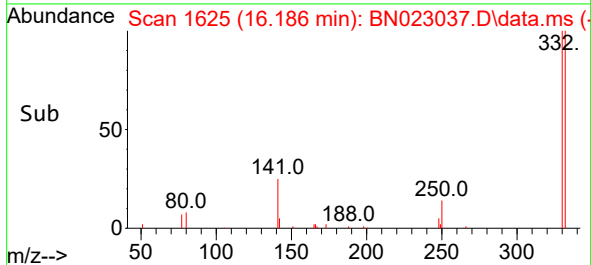

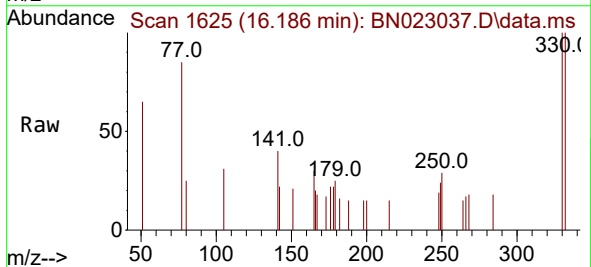


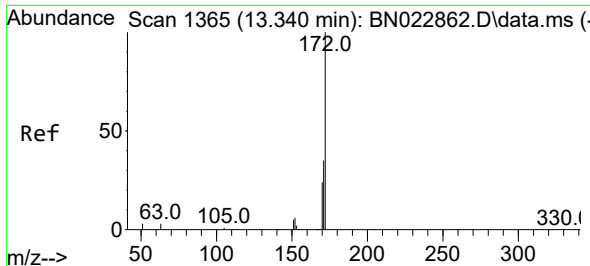

#15
2-Fluorobiphenyl
Concen: 0.372 ng
RT: 13.319 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion:172	Resp:	9596
Ion Ratio	Lower	Upper
172	100	
171	35.3	28.2 42.4
170	23.7	19.3 28.9

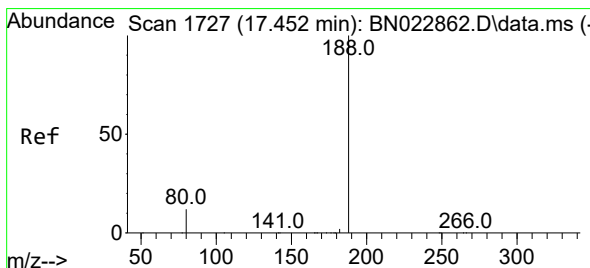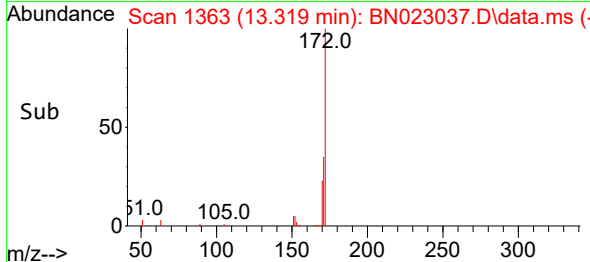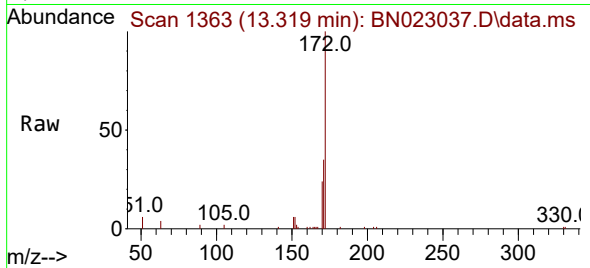

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.439 min Scan# 1726
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion:188	Resp:	10622
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0 0.0
80	10.6	10.3 15.5


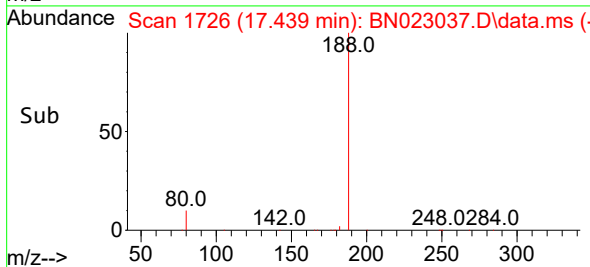

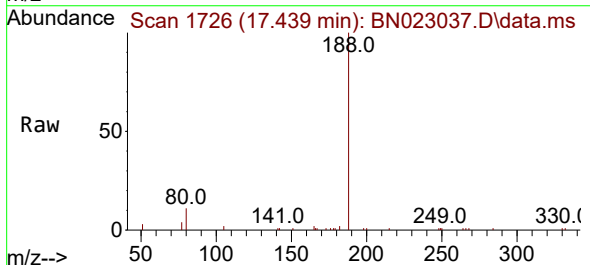




#27
Fluoranthene-d10
Concen: 0.294 ng
RT: 19.464 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion:212 Resp: 8496
Ion Ratio Lower Upper
212 100
106 17.7 12.3 18.5
104 10.2 7.0 10.4

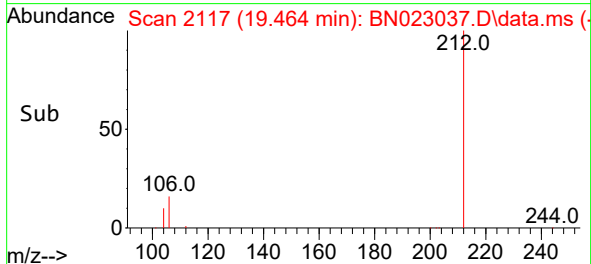

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.616 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion:240 Resp: 6602
Ion Ratio Lower Upper
240 100
120 22.2 9.2 13.8#
236 30.4 22.6 34.0

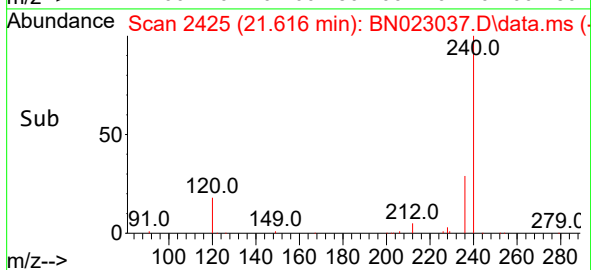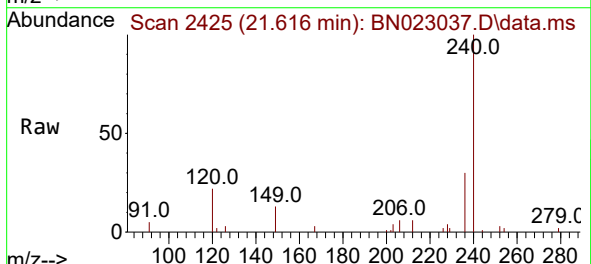

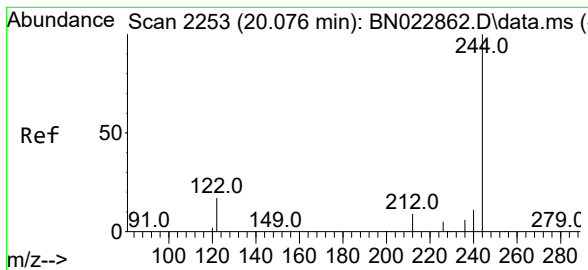

#31

Terphenyl-d14

Concen: 0.413 ng

RT: 20.058 min Scan# 21

Delta R.T. -0.000 min

Lab File: BN023037.D

Acq: 02 Dec 2022 04:19

Instrument :

BNA_N

ClientSampleId :

TT101D2-20221121





Tgt Ion:244 Resp: 6399

Ion Ratio Lower Upper

244 100

212 8.7 7.9 11.9

122 12.0 13.9 20.9#

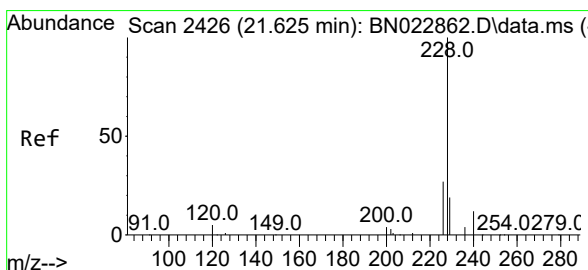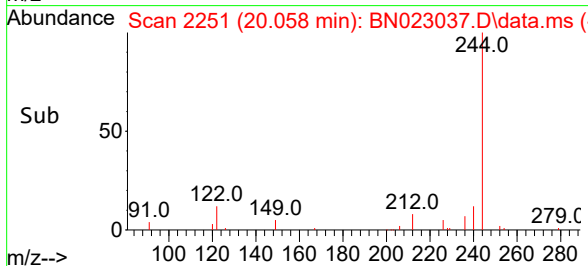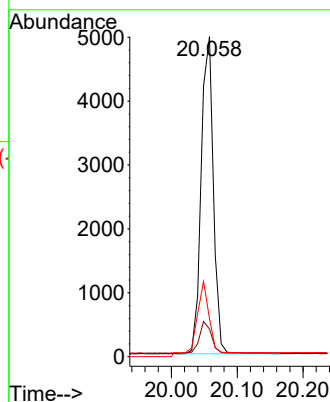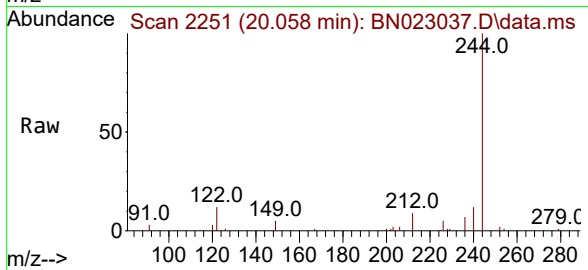

#32

Benzo(a)anthracene

Concen: 0.026 ng

RT: 21.598 min Scan# 2423

Delta R.T. -0.009 min

Lab File: BN023037.D

Acq: 02 Dec 2022 04:19




Tgt Ion:228 Resp: 702


Ion Ratio Lower Upper

228 100

226 34.7 22.1 33.1#

229 27.5 15.8 23.6#

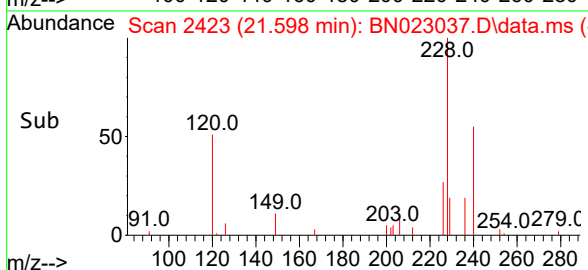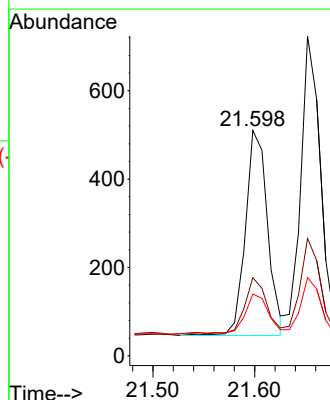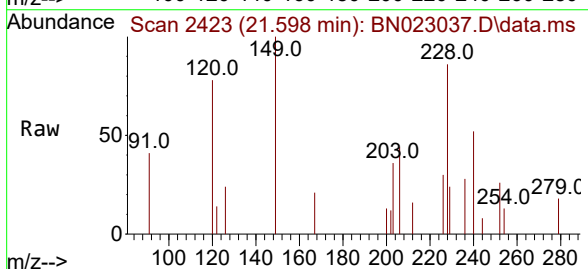

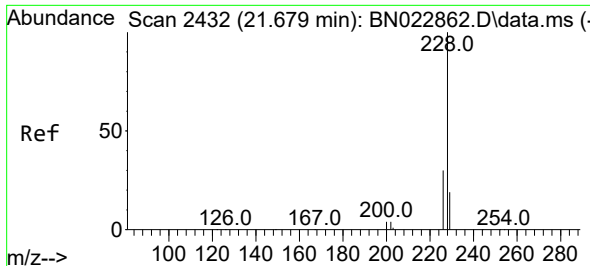

#33

Chrysene

Concen: 0.033 ng

RT: 21.652 min Scan# 2415

Delta R.T. -0.009 min

Lab File: BN023037.D


Acq: 02 Dec 2022 04:19

Instrument :

BNA_N

ClientSampleId :

TT101D2-20221121

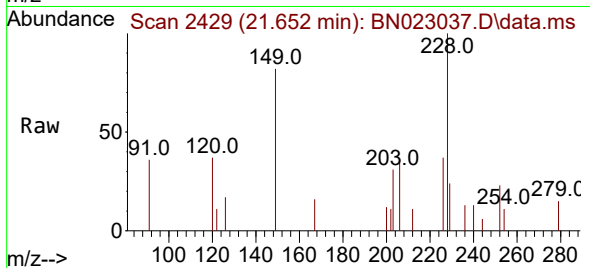




Tgt Ion:228 Resp: 913

Ion Ratio Lower Upper

228 100

226 36.7 24.5 36.7#

229 24.4 15.8 23.6#

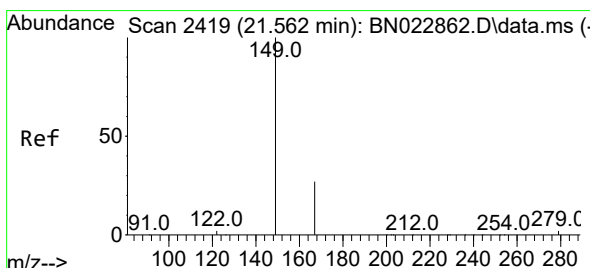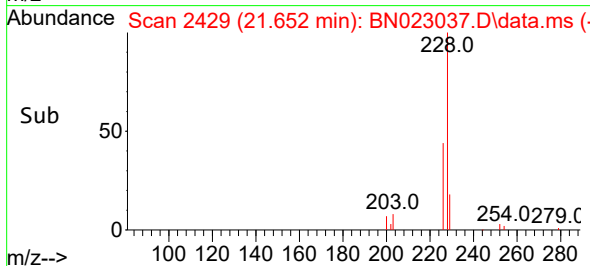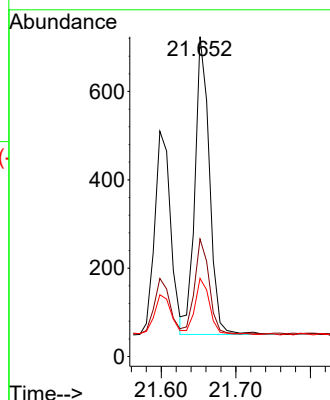

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.073 ng

RT: 21.527 min Scan# 2415

Delta R.T. -0.000 min

Lab File: BN023037.D

Acq: 02 Dec 2022 04:19




Tgt Ion:149 Resp: 778


Ion Ratio Lower Upper

149 100

167 22.0 21.3 31.9

279 2.3 2.3 3.5#


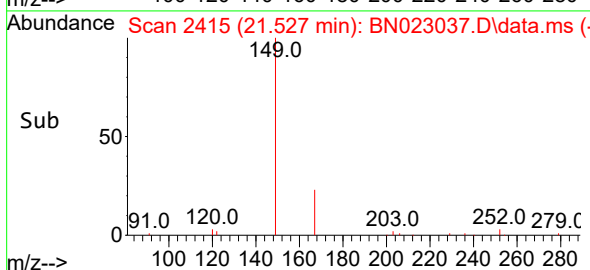
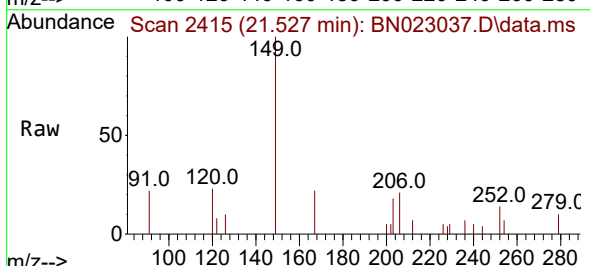
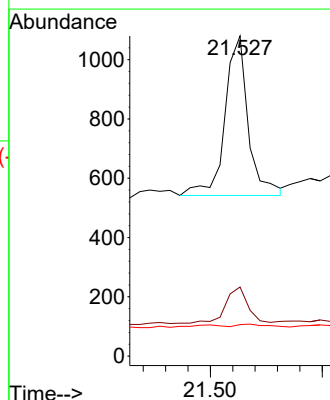




#35
Perylene-d12
Concen: 0.400 ng
RT: 24.097 min Scan# 3092
Delta R.T. -0.006 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19




Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121


Tgt Ion:264 Resp: 4891
Ion Ratio Lower Upper
264 100
260 27.7 21.7 32.5
265 81.6 31.0 46.4#

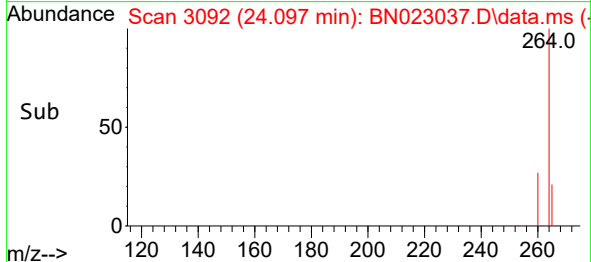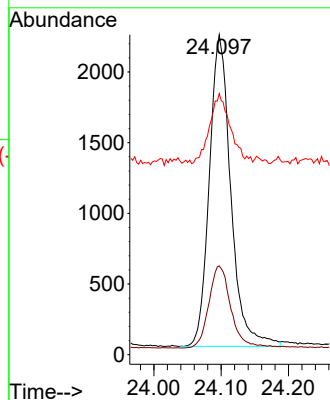

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.033 ng
RT: 26.693 min Scan# 3980
Delta R.T. -0.003 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19


Tgt Ion:276 Resp: 675
Ion Ratio Lower Upper
276 100
138 37.0 24.4 36.6#
277 22.2 19.9 29.9

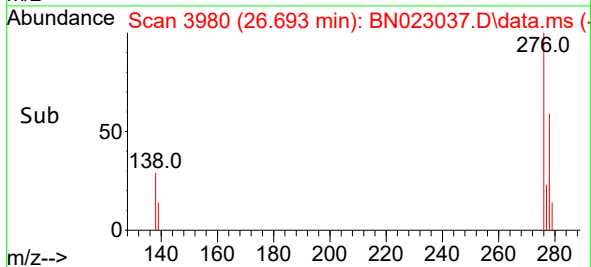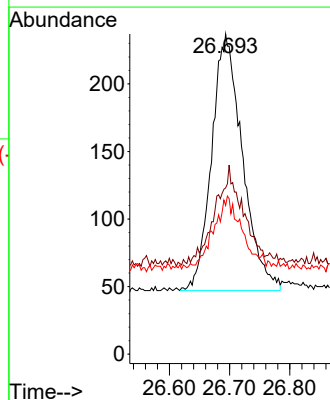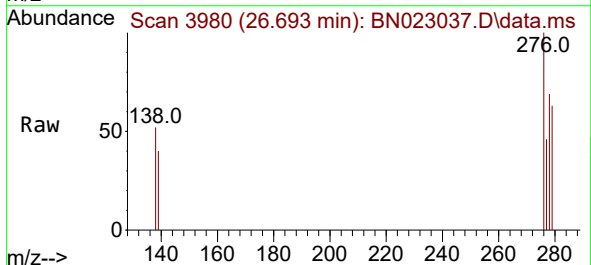






#37
Benzo(b)fluoranthene
Concen: 0.039 ng
RT: 23.337 min Scan# 2832
Delta R.T. -0.003 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Instrument :
BNA_N
ClientSampleId :
TT101D2-20221121







Tgt Ion:252 Resp: 852
Ion Ratio Lower Upper
252 100
253 53.4 18.5 27.7#
125 70.4 10.8 16.2#

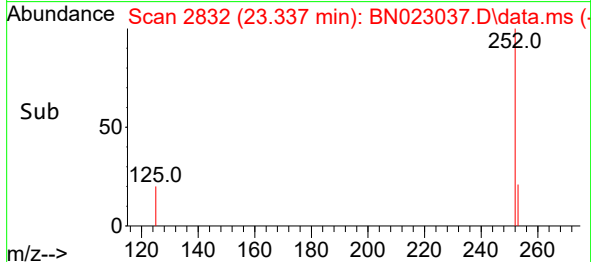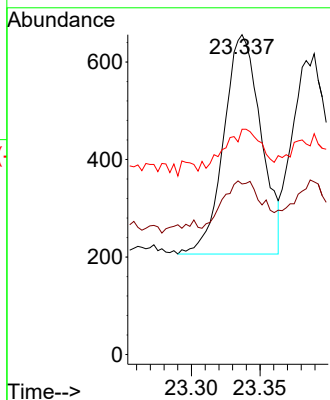

#38
Benzo(k)fluoranthene
Concen: 0.031 ng
RT: 23.390 min Scan# 2850
Delta R.T. -0.000 min
Lab File: BN023037.D
Acq: 02 Dec 2022 04:19

Tgt Ion:252 Resp: 727
Ion Ratio Lower Upper
252 100
253 57.4 18.6 27.8#
125 73.4 11.0 16.4#

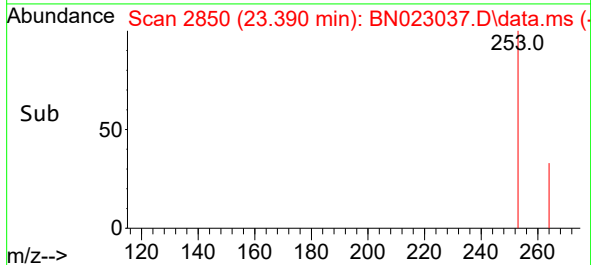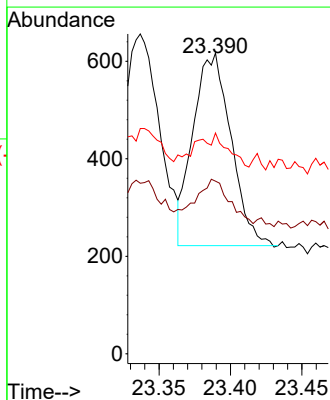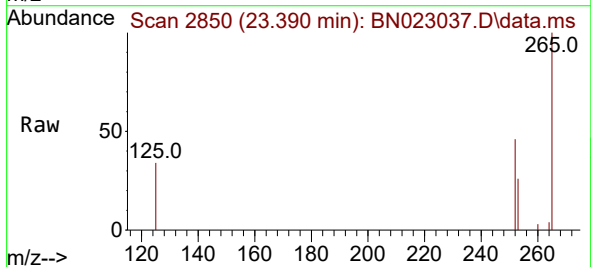



#39

Benzo(a)pyrene

Concen: 0.022 ng

RT: 23.986 min Scan# 3067

Delta R.T. -0.006 min

Lab File: BN023037.D

Acq: 02 Dec 2022 04:19

Instrument :

BNA_N

ClientSampleId :

TT101D2-20221121





Tgt Ion:252 Resp: 362

Ion Ratio Lower Upper

252 100

253 80.3 19.2 28.8#

125 107.7 12.7 19.1#

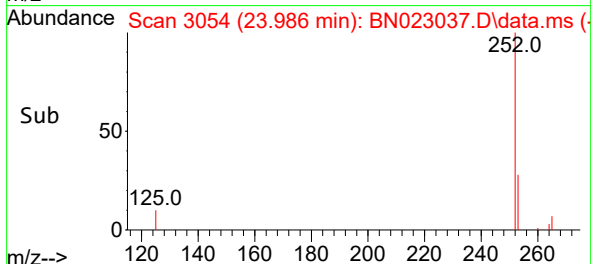

#40

Dibenzo(a,h)anthracene

Concen: 0.037 ng

RT: 26.717 min Scan# 3988

Delta R.T. -0.000 min

Lab File: BN023037.D

Acq: 02 Dec 2022 04:19




Tgt Ion:278 Resp: 596


Ion Ratio Lower Upper

278 100

139 46.6 17.4 26.0#

279 72.2 20.0 30.0#

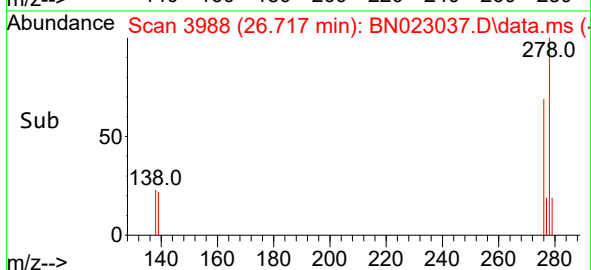

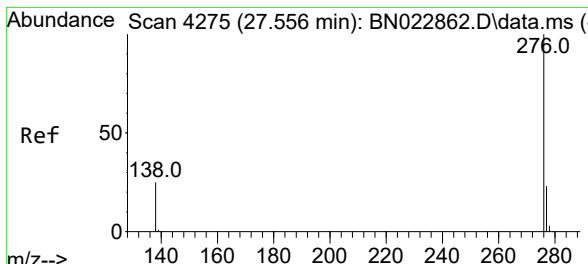

#41

Benzo(g,h,i)perylene

Concen: 0.038 ng

RT: 27.491 min Scan# 41

Delta R.T. -0.003 min

Lab File: BN023037.D


Acq: 02 Dec 2022 04:19

Instrument :

BNA_N

ClientSampleId :

TT101D2-20221121

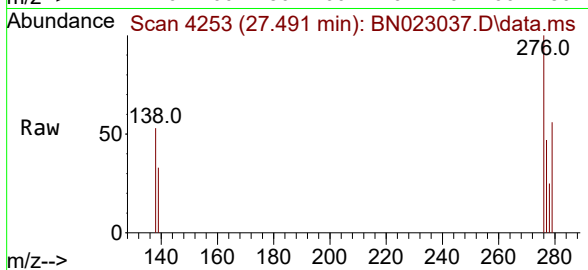

Tgt Ion:276 Resp: 666

Ion Ratio Lower Upper

276 100

277 46.6 19.7 29.5#

138 53.4 21.4 32.2#

