
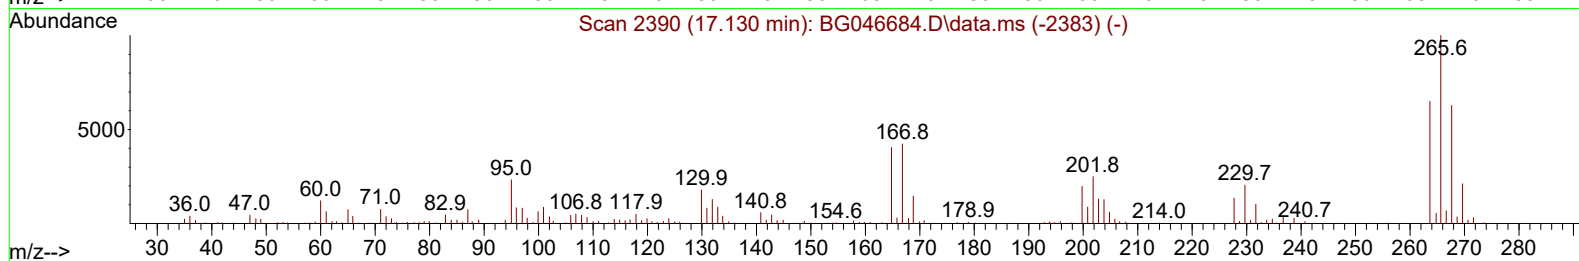
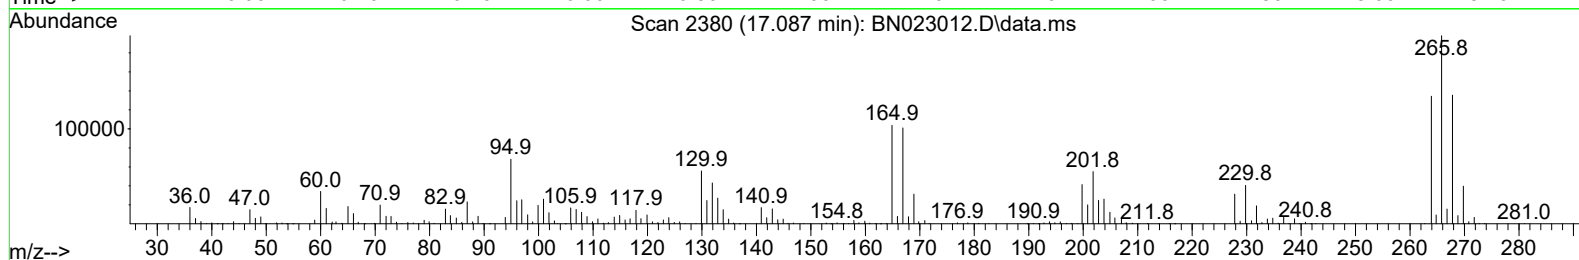


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023012.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 06:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 06:06:28 2022
Response via : Initial Calibration

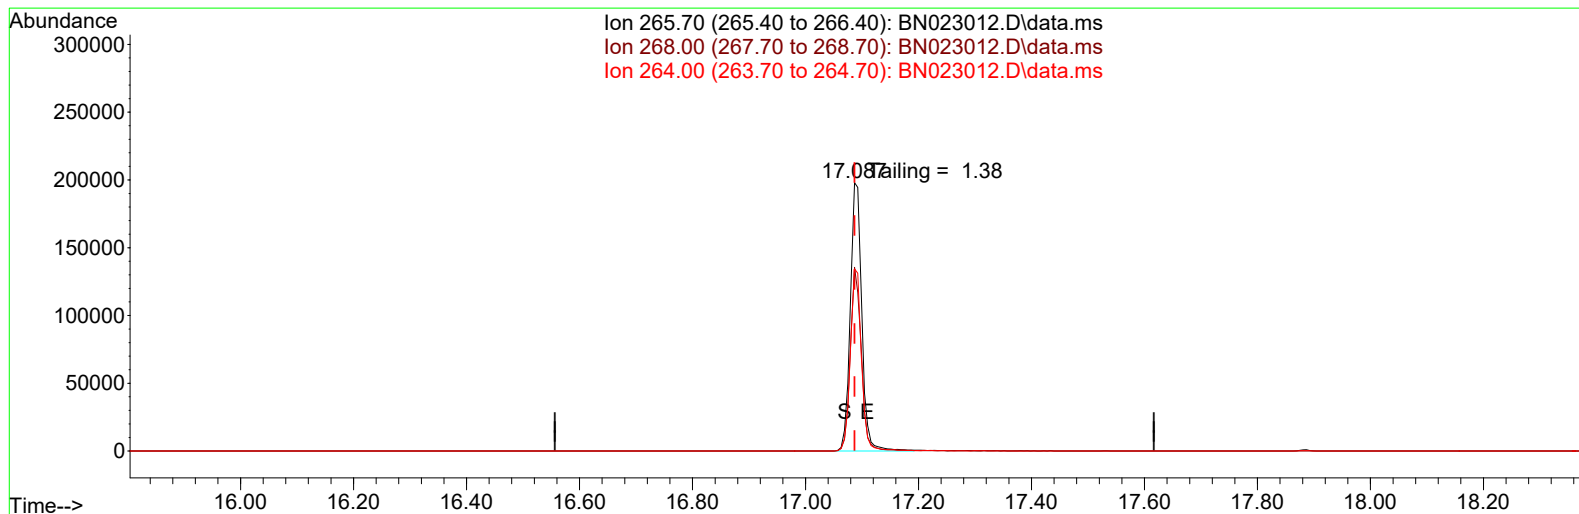

TIC: BN023012.D\data.ms

(70) Pentachlorophenol (C)




17.087min (0.000) 15379.27 ng

response 282300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.46
264.00	61.60	67.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
 Data File : BN023012.D
 Acq On : 01 Dec 2022 09:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 06:06:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 06:06:28 2022
 Response via : Initial Calibration

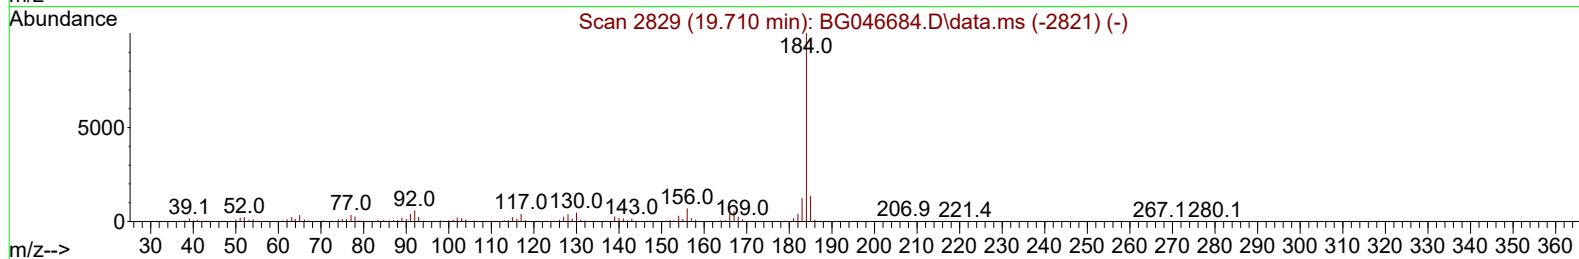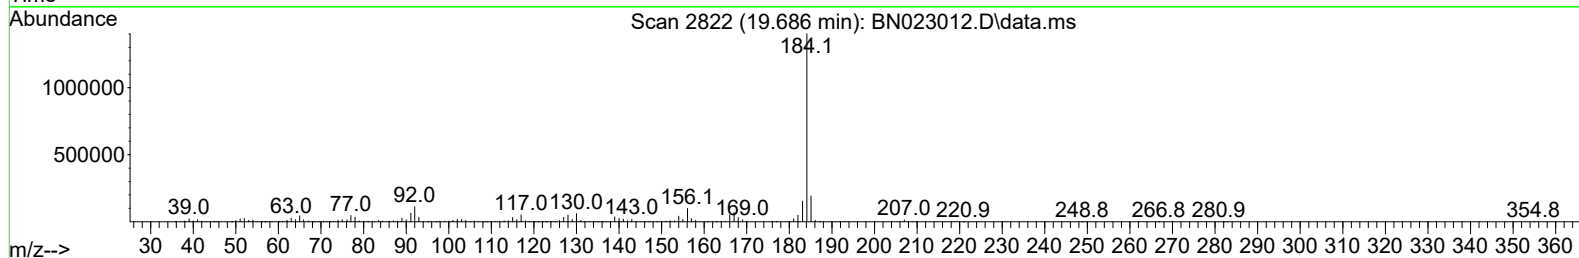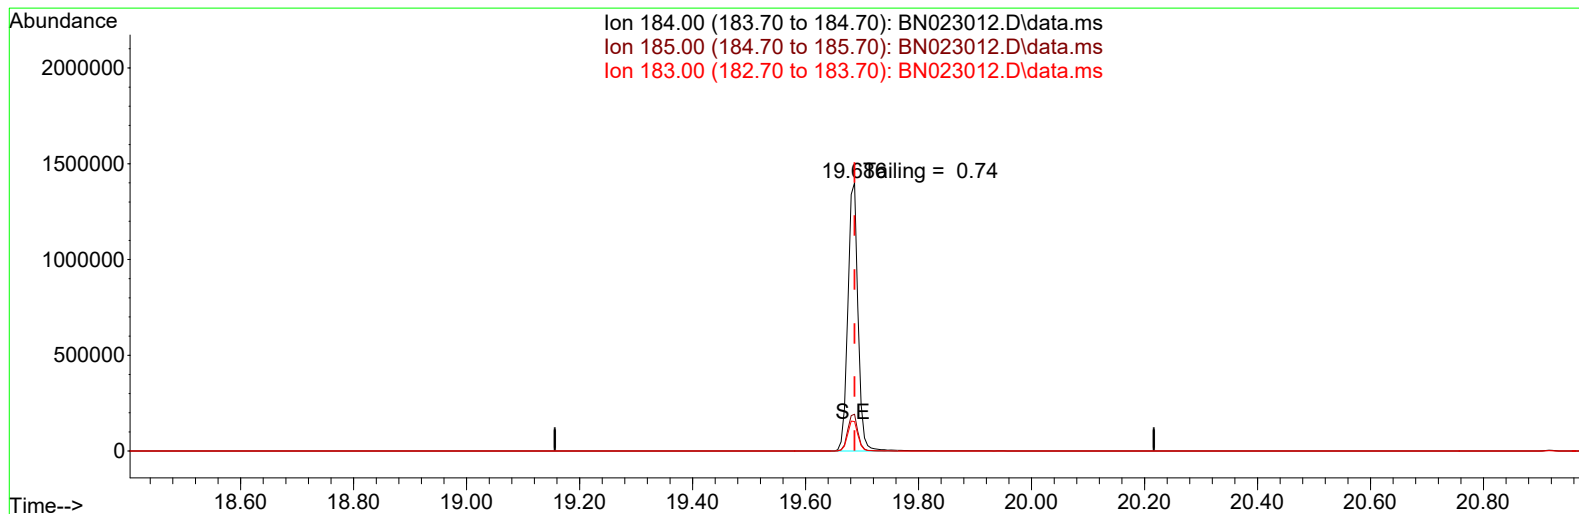

TIC: BN023012.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 1749590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	10.99
0.00	0.00	0.00