
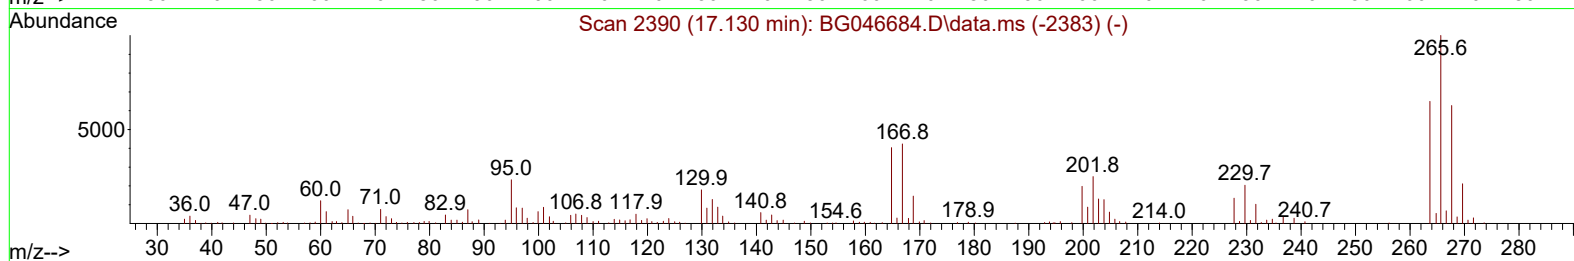
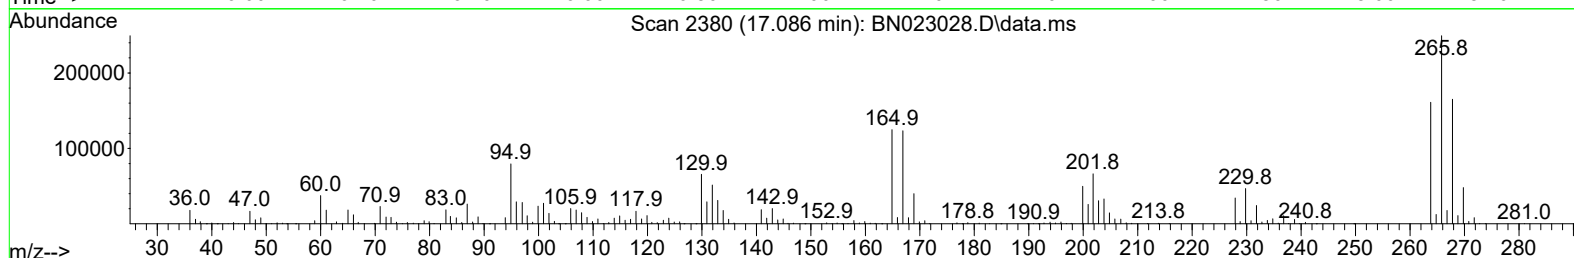


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023028.D
Acq On : 01 Dec 2022 22:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 06:08:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 06:06:28 2022
Response via : Initial Calibration

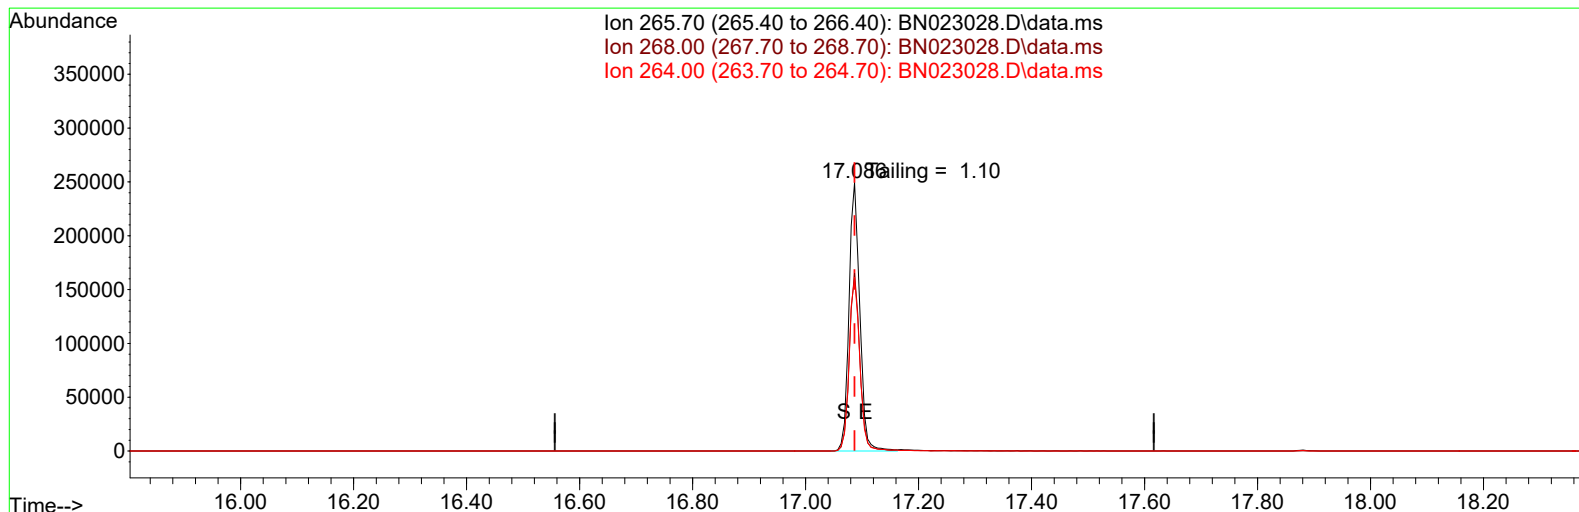

TIC: BN023028.D\data.ms

(70) Pentachlorophenol (C)




17.086min (-0.000) 16055.75 ng

response 331510

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.27
264.00	61.60	64.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
 Data File : BN023028.D
 Acq On : 01 Dec 2022 22:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 06:08:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 02 06:06:28 2022
 Response via : Initial Calibration

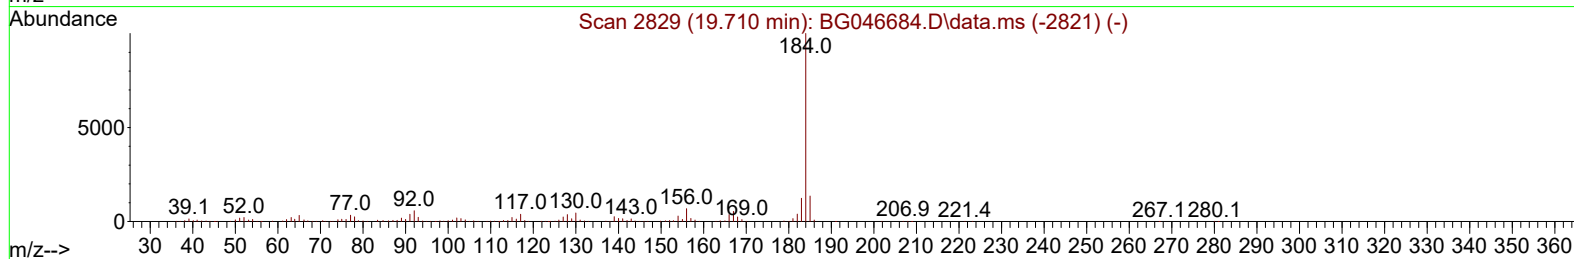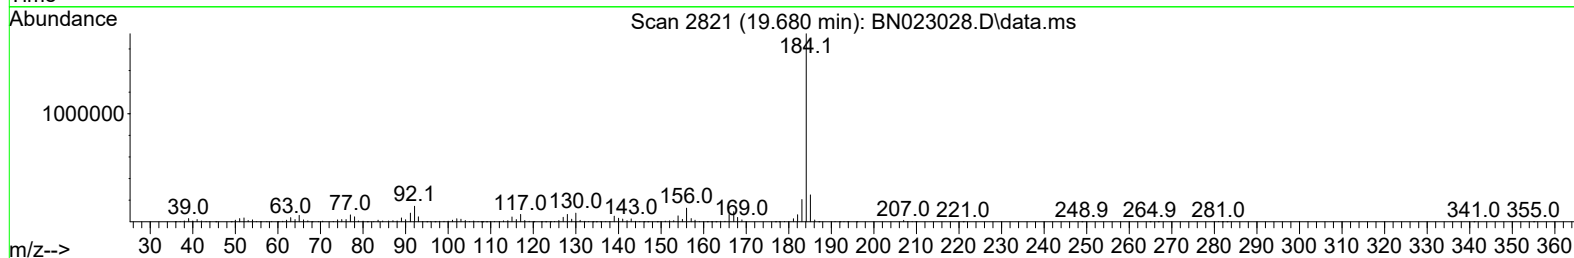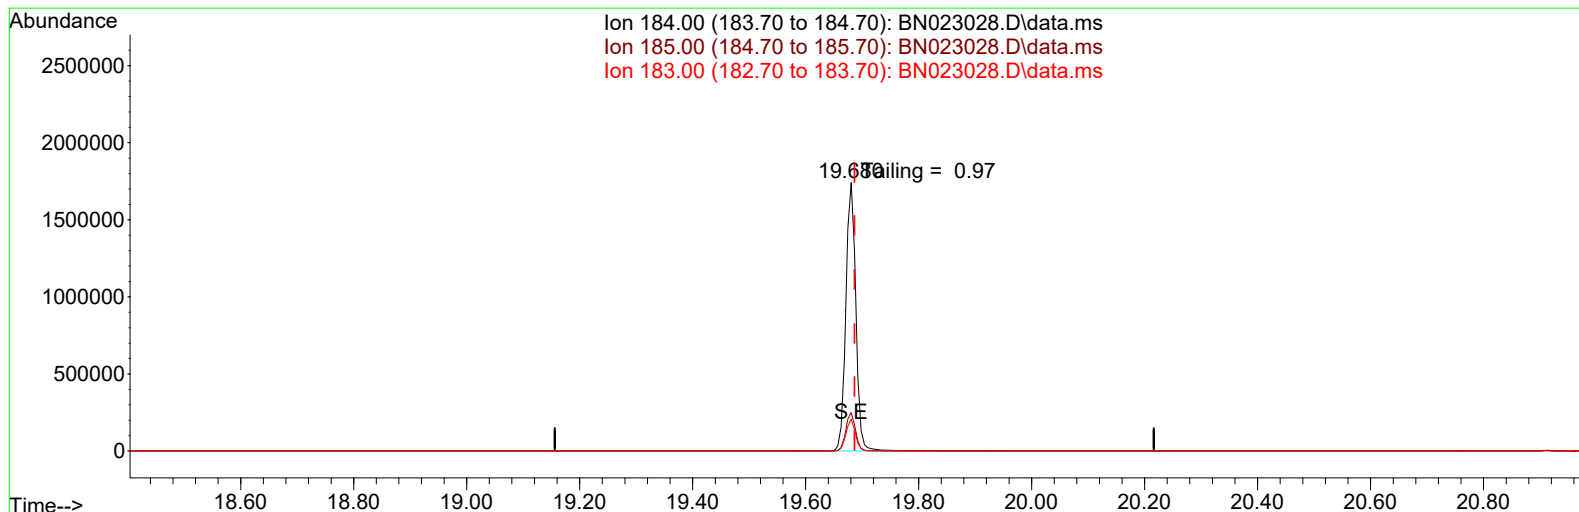

TIC: BN023028.D\data.ms

(77) Benzidine

19.680min (-0.006) 0.00 ng

response 2133664

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	11.80
0.00	0.00	0.00