


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023012.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN112522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 02 02:30:10 2022

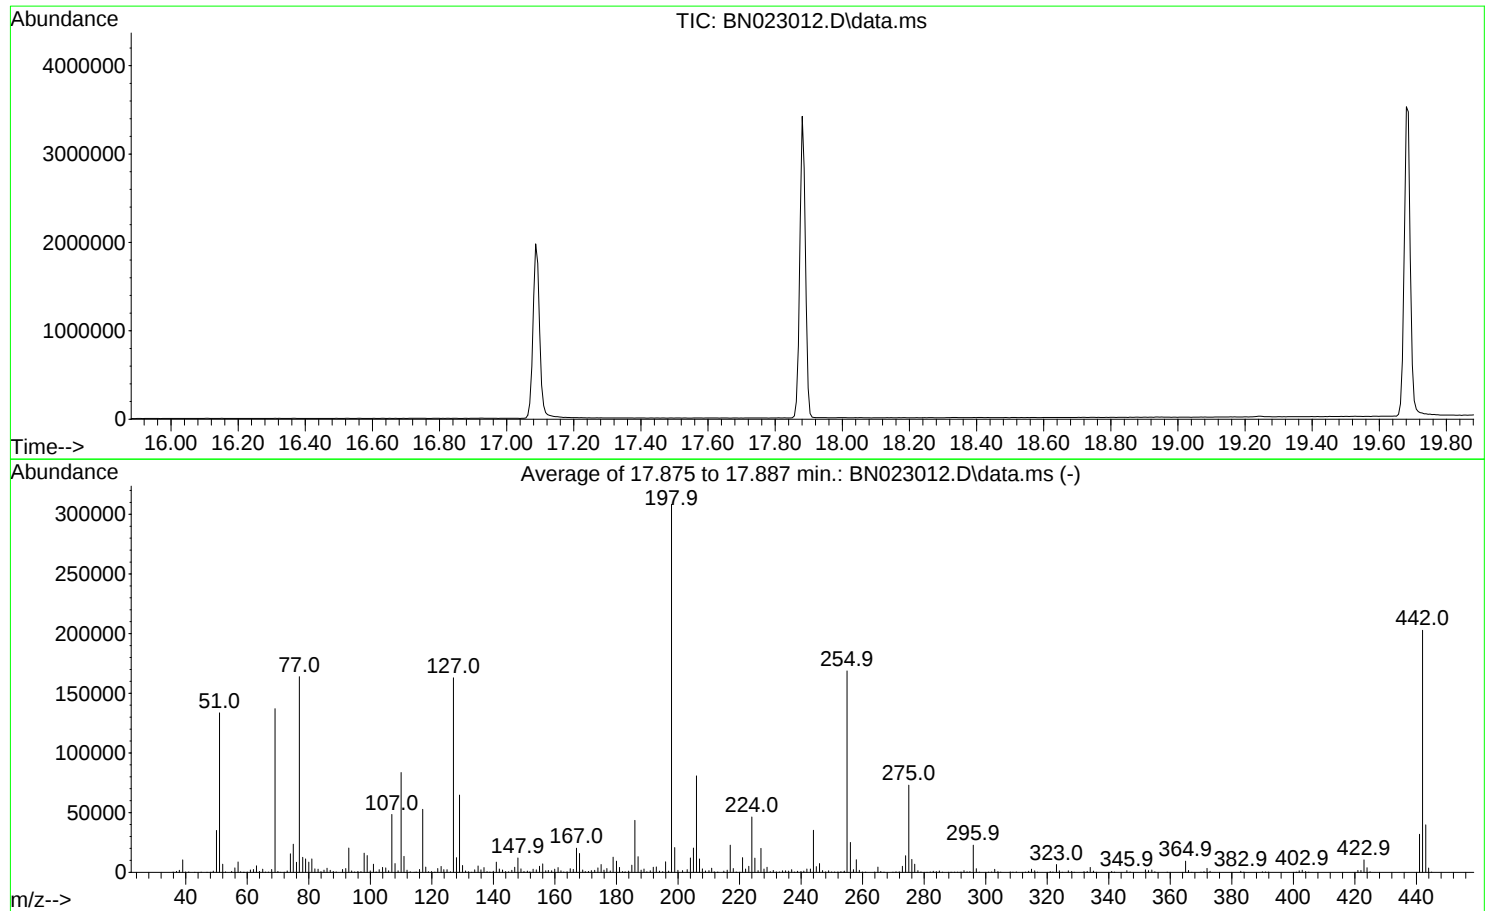




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	133653	PASS
68	69	0.00	2	1.7	2385	PASS
69	198	0.00	100	44.5	137173	PASS
70	69	0.00	2	0.5	731	PASS
127	198	10	80	52.9	163051	PASS
197	198	0.00	2	0.3	997	PASS
198	198	100	100	100.0	308288	PASS
199	198	5	9	6.7	20691	PASS
275	198	10	60	23.7	73035	PASS
365	198	1	100	3.0	9274	PASS
441	198	0.01	100	10.3	31851	PASS
442	442	50	100	100.0	202789	PASS
443	442	15	24	19.6	39827	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023012.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 02 06:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 06:06:28 2022
Response via : Initial Calibration

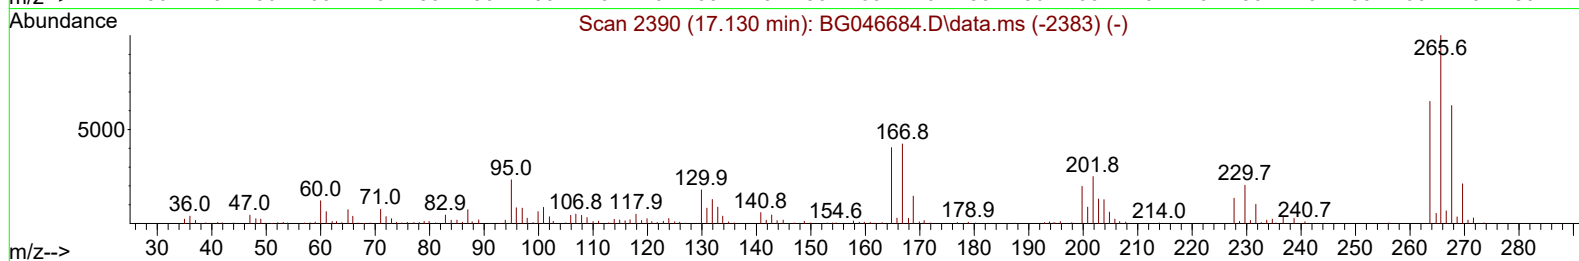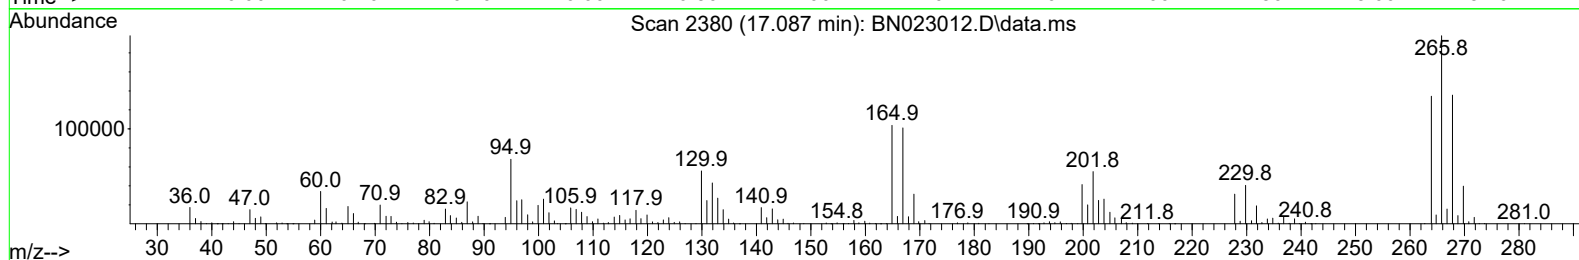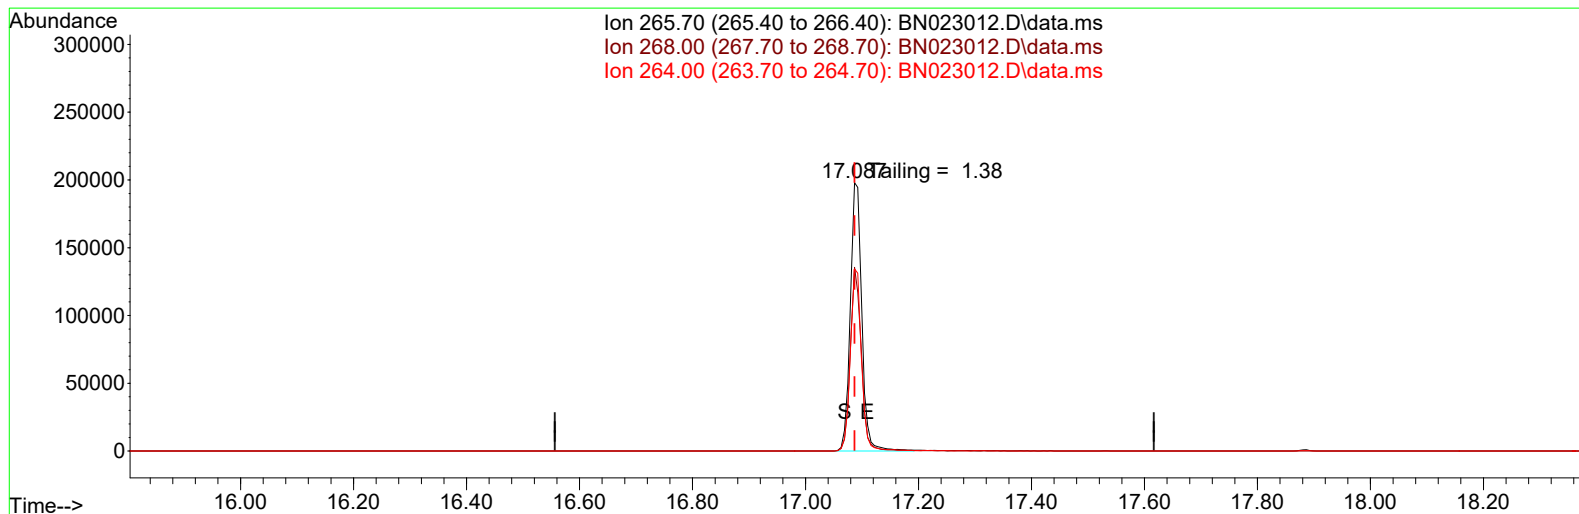

TIC: BN023012.D\data.ms

(70) Pentachlorophenol (C)

17.087min (0.000) 15379.27 ng




response 282300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.46
264.00	61.60	67.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120122\
Data File : BN023012.D
Acq On : 01 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 02 06:06:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 02 06:06:28 2022
Response via : Initial Calibration

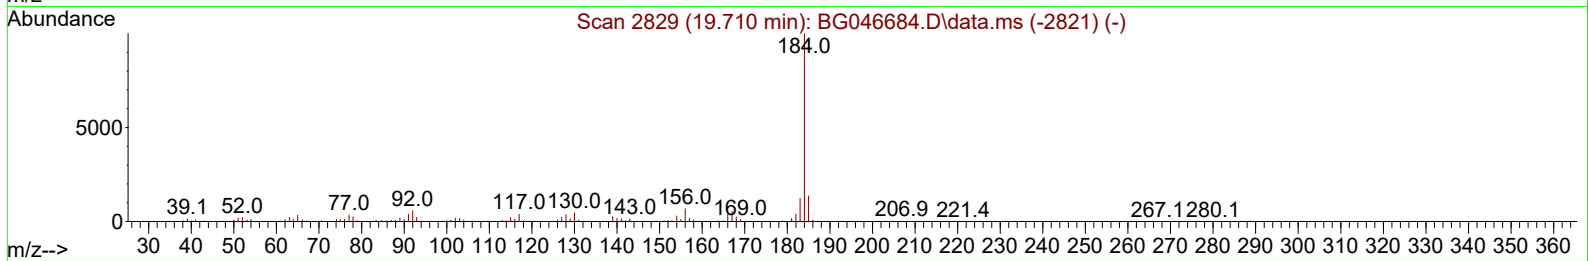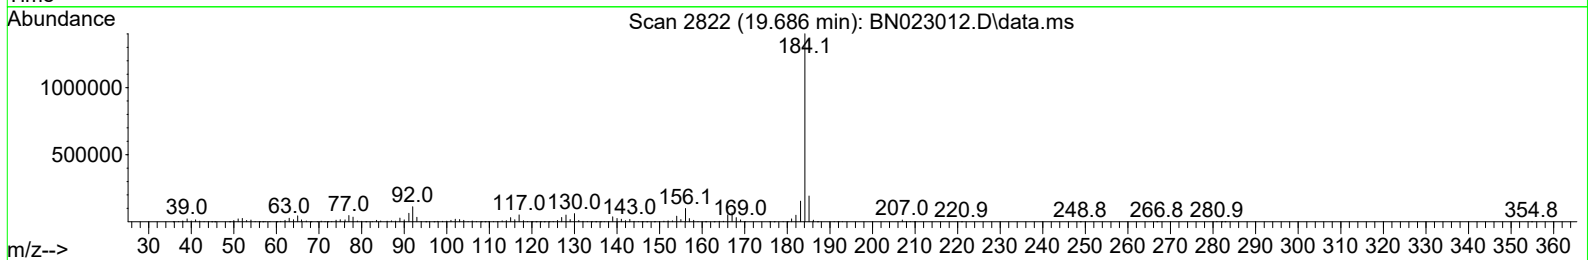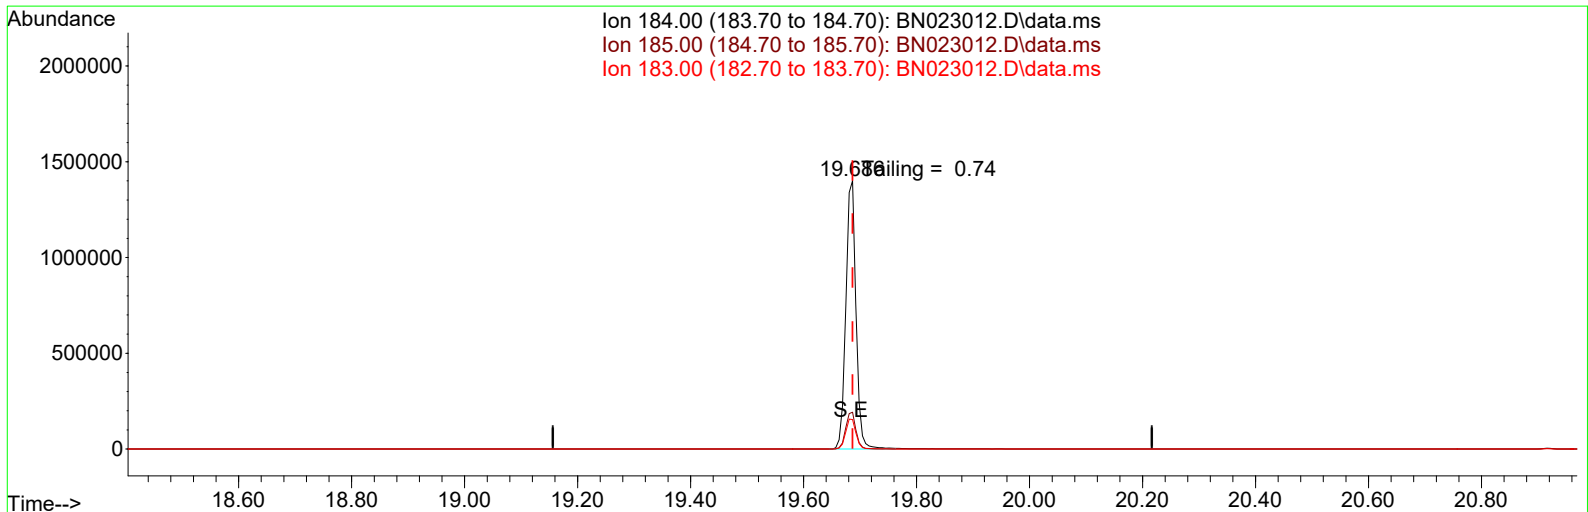

TIC: BN023012.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 1749590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	10.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/1/2022	BNA_N	<u>BN023012.D</u>
Compound Name	Response	Retention Time
DDT	821183	20.916
DDD	10283	20.475
DDE	466	19.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10749	831932	1.29

Instrument :
BNA_N
ClientSampleId :
DFTPP