

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012786.D
 Acq On : 01 Dec 2020 17:39
 Operator : CG/JU
 Sample : PB133292BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK92

Quant Time: Dec 02 00:56:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	955	0.40	ng/ul	0.00
2) Naphthalene-d8	10.19	136	4028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2433	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.84
16) Chrysene-d12	21.06	240	3954	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4514	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.80	152	1859	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	4368	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.08	166	878	0.080	ng/ul#	18
17) Pyrene	19.25	202	941	0.053	ng/ul#	1
23) Benzo(a)pyrene	23.04	252	1962	0.100	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012786.D
Acq On : 01 Dec 2020 17:39
Operator : CG/JU
Sample : PB133292BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK92

Quant Time: Dec 02 00:56:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration




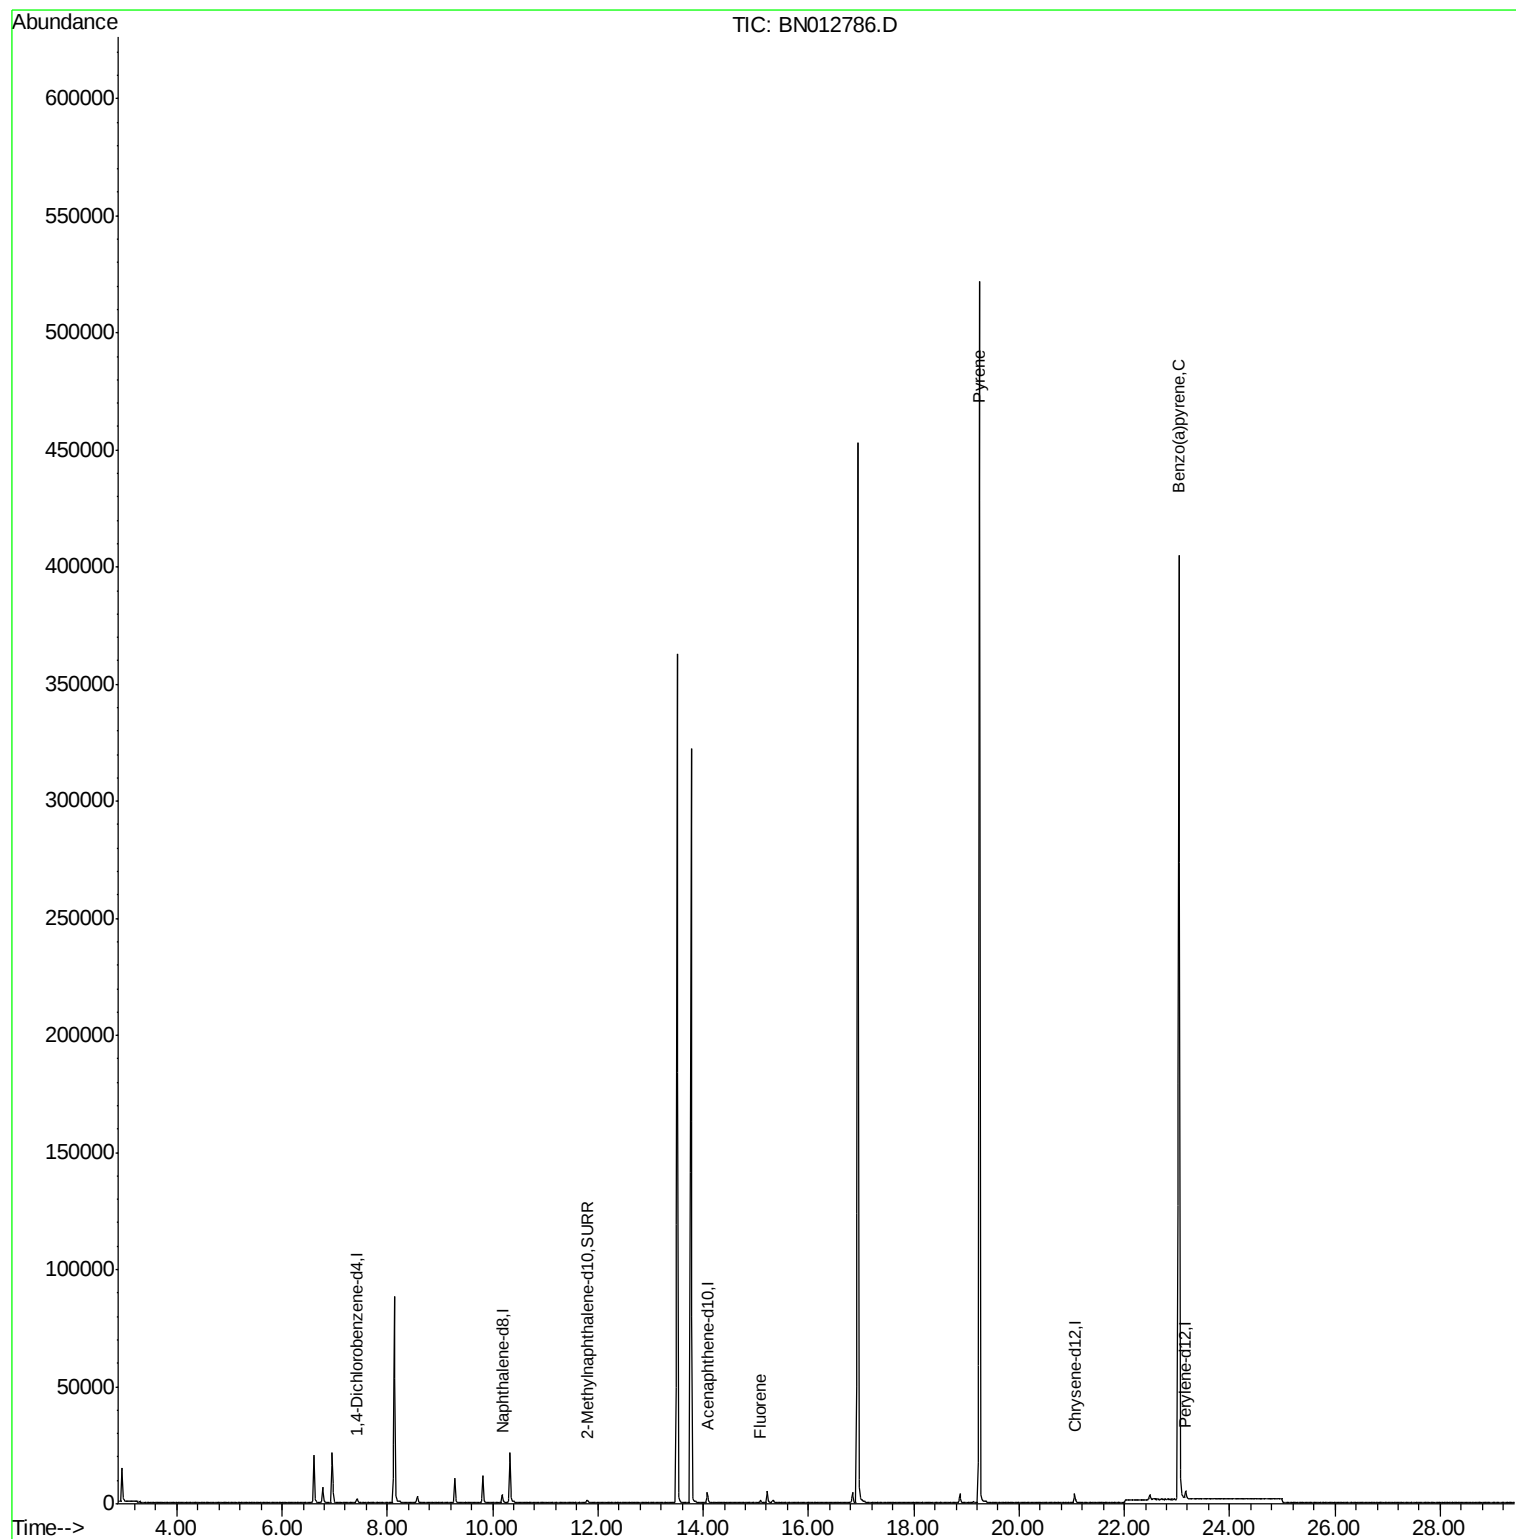


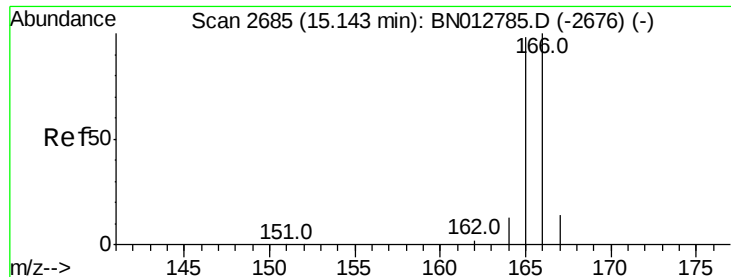

#9
Fluorene
 Concen: 0.080 ng/ul
 RT: 15.08 min Scan# 2672
 Delta R.T. -0.06 min
 Lab File: BN012786.D
 Acq: 01 Dec 2020 17:39




Instrument :
 BNA_N
 ClientSampleId :
 SBLK92


Tot Ion:166 Resp: 878
 Ion Ratio Lower Upper
 166 100
 165 11.0 78.5 117.7#
 167 35.1 12.7 19.1#

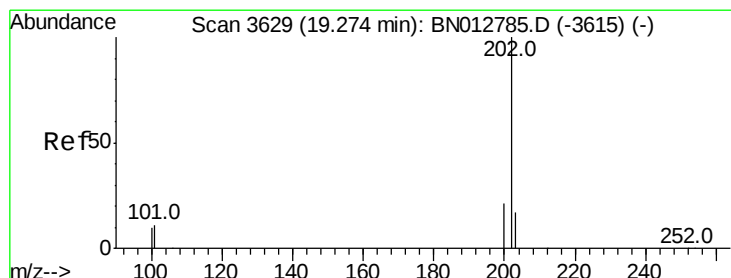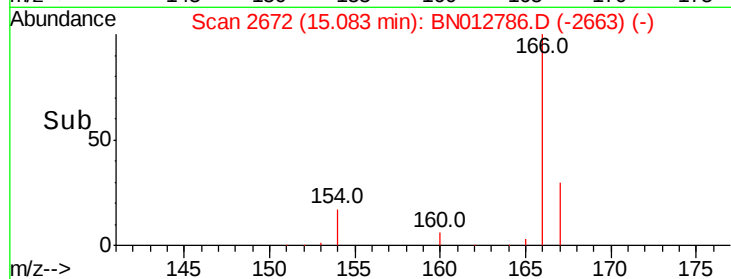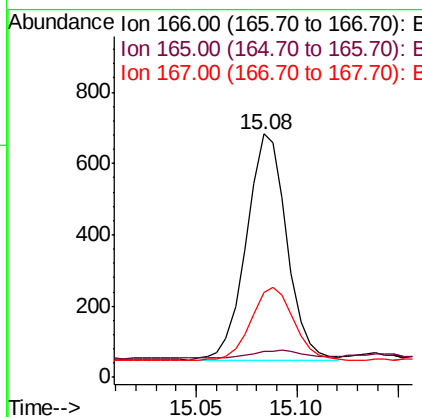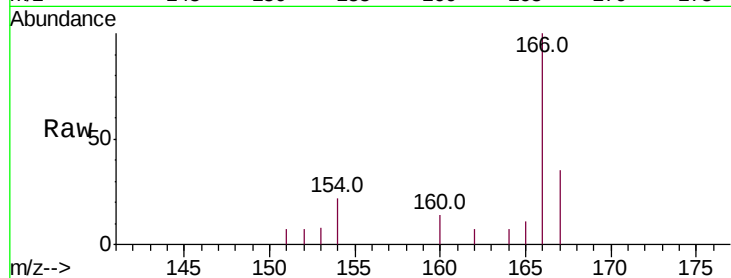

#17
Pyrene
 Concen: 0.053 ng/ul
 RT: 19.25 min Scan# 3623
 Delta R.T. -0.03 min
 Lab File: BN012786.D
 Acq: 01 Dec 2020 17:39

Tgt Ion:202 Resp: 941
 Ion Ratio Lower Upper
 202 100
 101 195.4 8.9 13.3#
 100 1389.6 7.4 11.2#

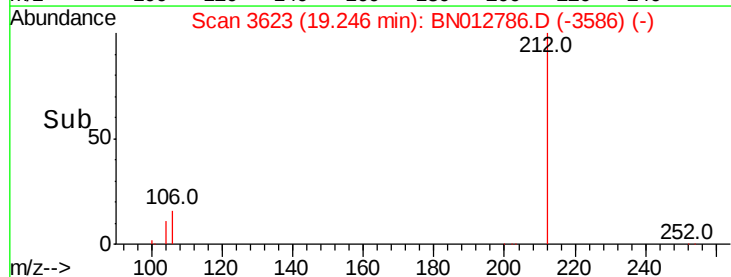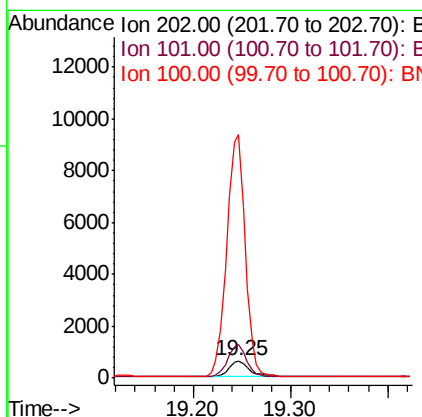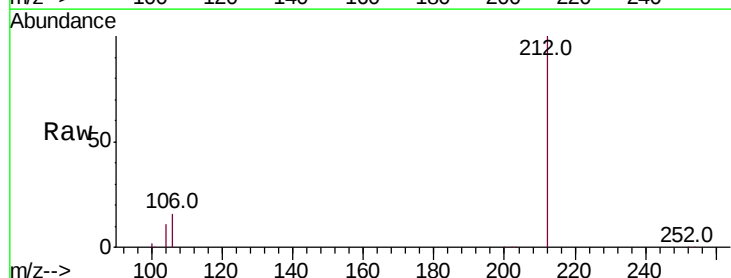

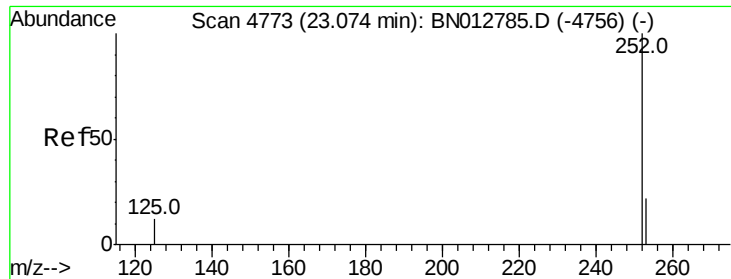

#23

Benzo(a)pyrene

Concen: 0.100 ng/ul

RT: 23.04 min Scan# 4760

Delta R.T. -0.04 min

Lab File: BN012786.D

Acq: 01 Dec 2020 17:39

Instrument :

BNA_N

ClientSampleId :

SBLK92


Tot Ion: 252 Resp: 1962

Ion Ratio Lower Upper

252 100

253 46.4 27.6 41.4#

125 38.8 17.0 25.4#

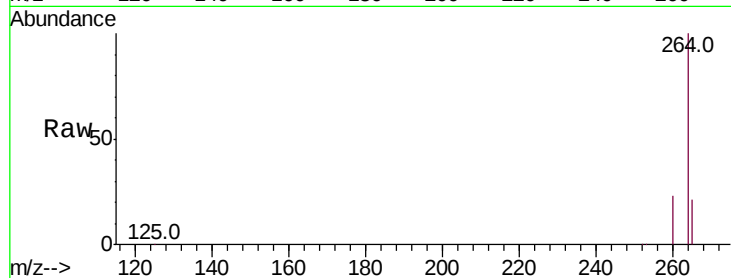

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

