

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012797.D
 Acq On : 02 Dec 2020 00:16
 Operator : CG/JU
 Sample : L4793-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BB2

Quant Time: Dec 02 00:57:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	910	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	3688	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2194	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.84
16) Chrysene-d12	21.05	240	3952	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4353	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.79	152	1133	0.21	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	2463	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.24	202	530	0.030	ng/ul#	1
23) Benzo(a)pyrene	23.03	252	1187	0.063	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012797.D
Acq On : 02 Dec 2020 00:16
Operator : CG/JU
Sample : L4793-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BB2

Quant Time: Dec 02 00:57:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

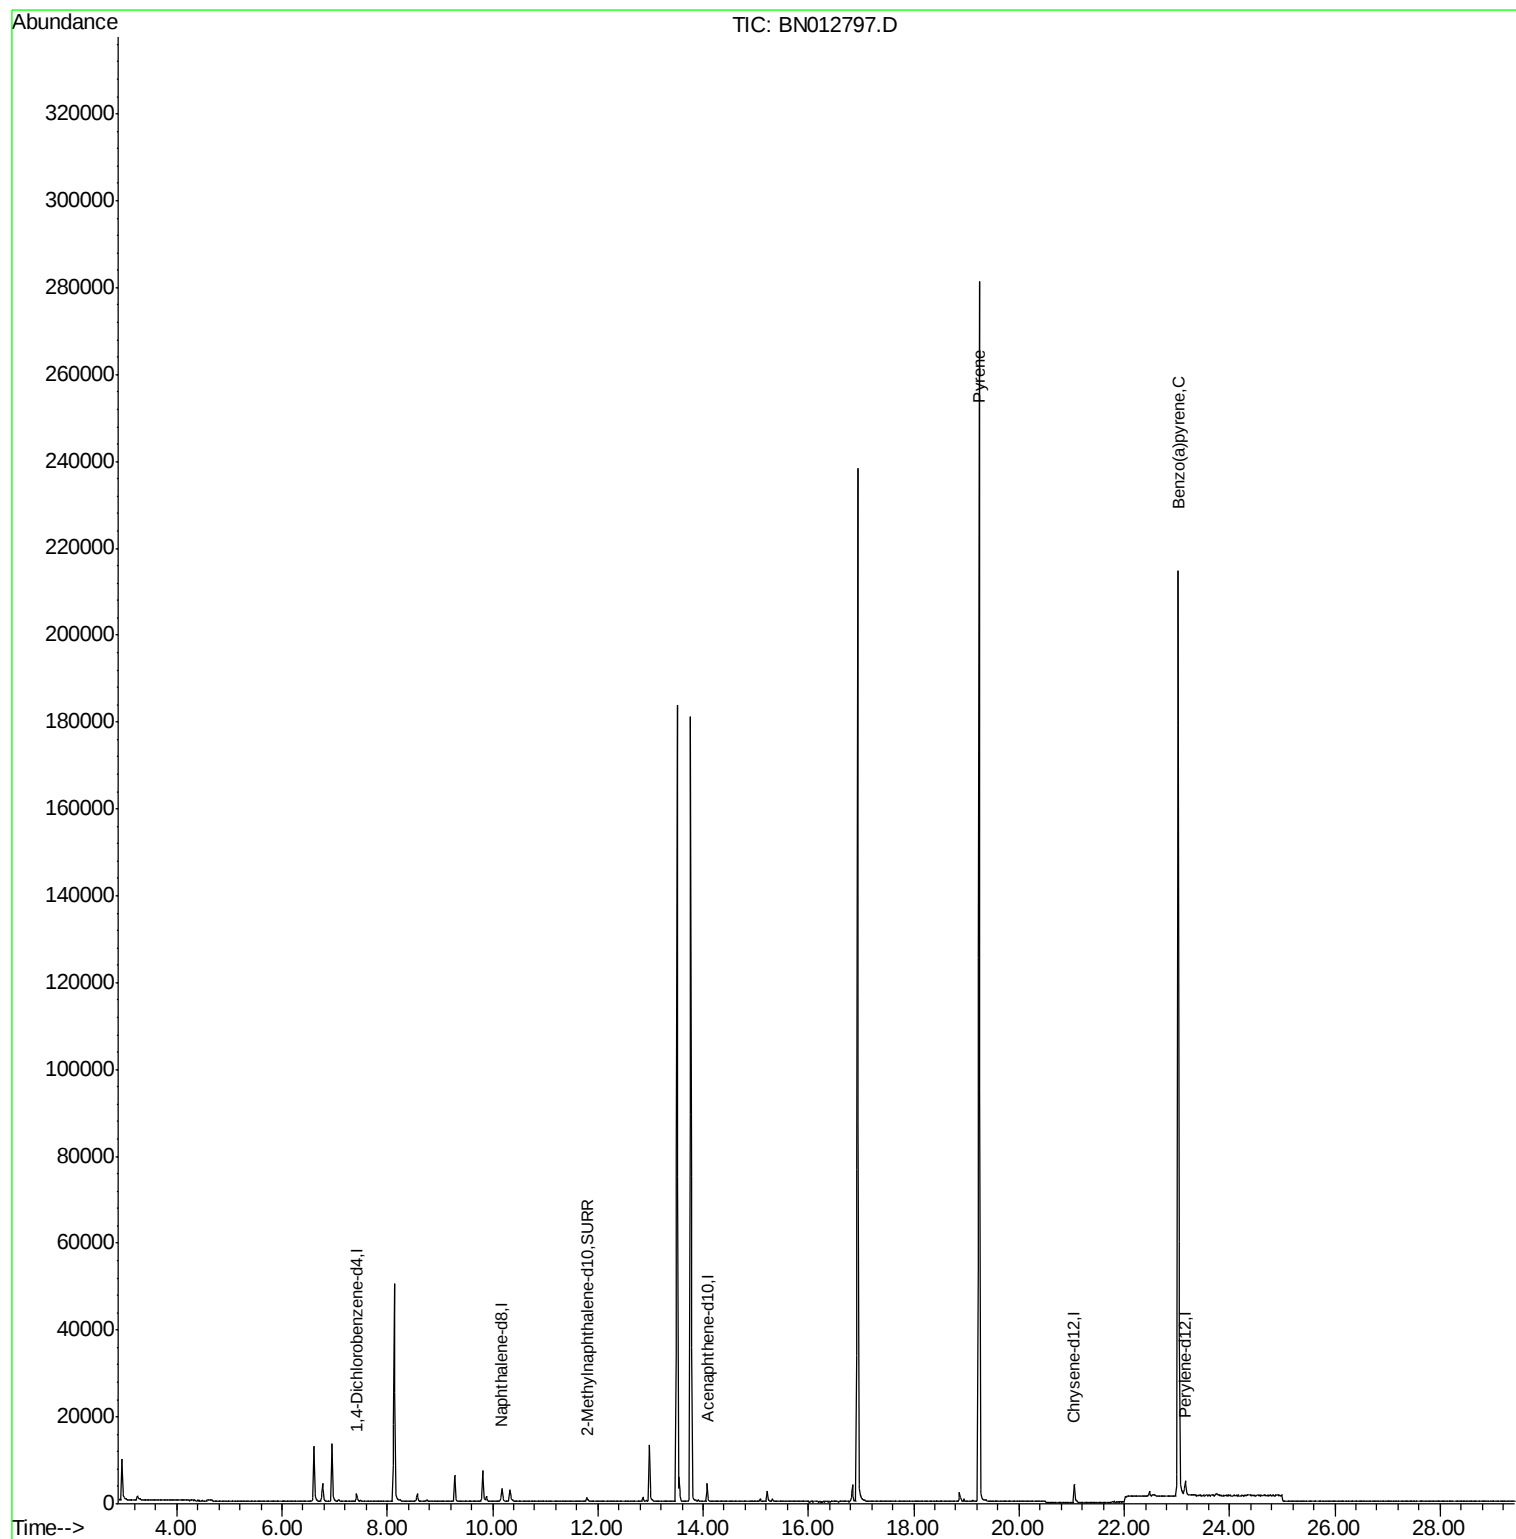

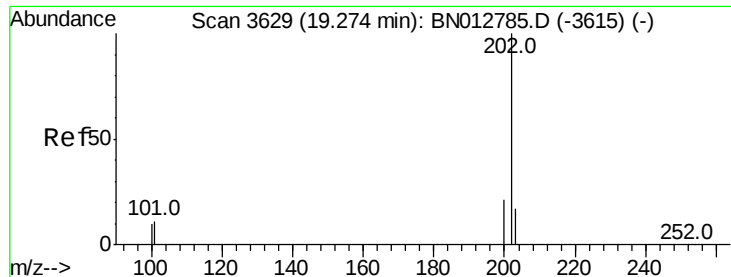

#17

Pvrene

Concen: 0.030 ng/ul

RT: 19.24 min Scan# 3622

Delta R.T. -0.03 min

Lab File: BN012797.D

Acq: 02 Dec 2020 00:16

Instrument :

BNA_N

ClientSampleId :

C0BB2



Tot Ion:202 Resp: 530

Ion Ratio Lower Upper

202 100

101 204.0 8.9 13.3#



100 1442.6 7.4 11.2#

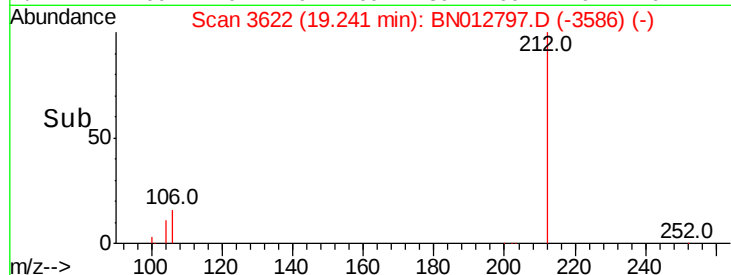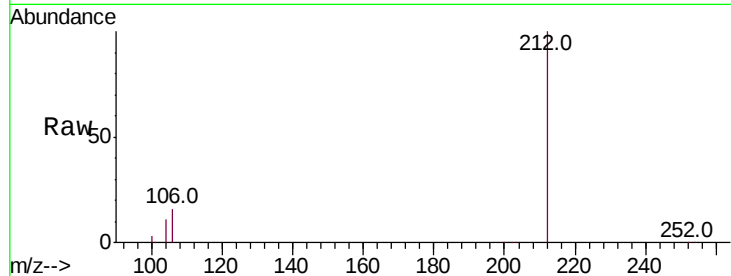

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

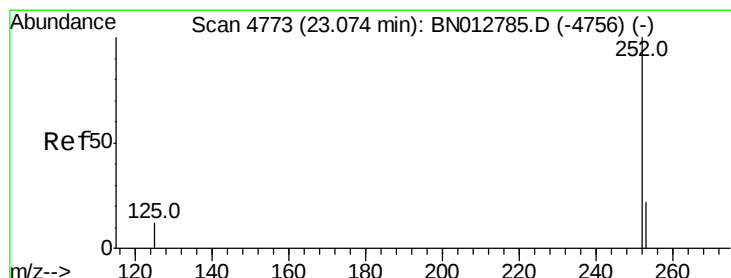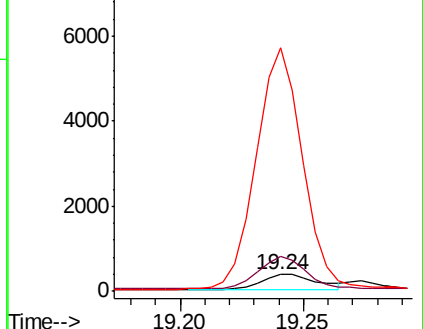

#23

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 23.03 min Scan# 4757

Delta R.T. -0.05 min

Lab File: BN012797.D

Acq: 02 Dec 2020 00:16



Tgt Ion:252 Resp: 1187

Ion Ratio Lower Upper

252 100

253 57.1 27.6 41.4#

125 48.0 17.0 25.4#

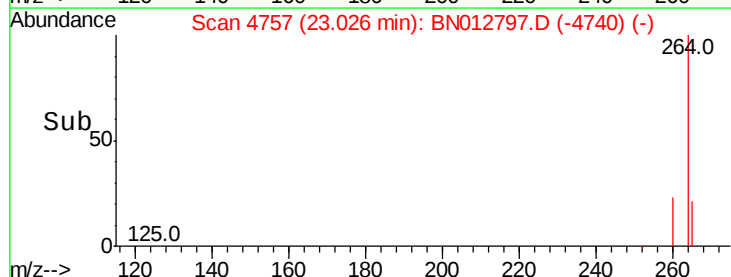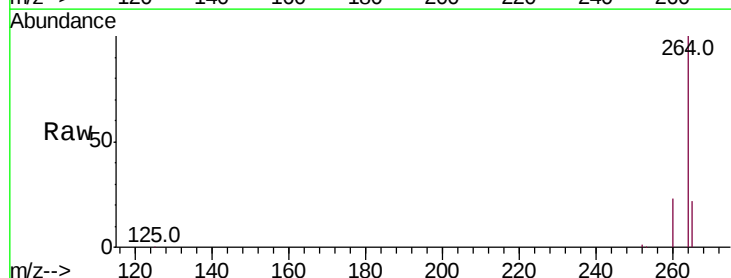

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

