

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012798.D
 Acq On : 02 Dec 2020 00:52
 Operator : CG/JU
 Sample : L4793-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BA8

Quant Time: Dec 02 02:00:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	915	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	3691	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2256	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.84
16) Chrysene-d12	21.05	240	3984	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4532	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.79	152	1471	0.28	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	3288	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.25	202	785	0.044	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012798.D
Acq On : 02 Dec 2020 00:52
Operator : CG/JU
Sample : L4793-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BA8

Quant Time: Dec 02 02:00:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

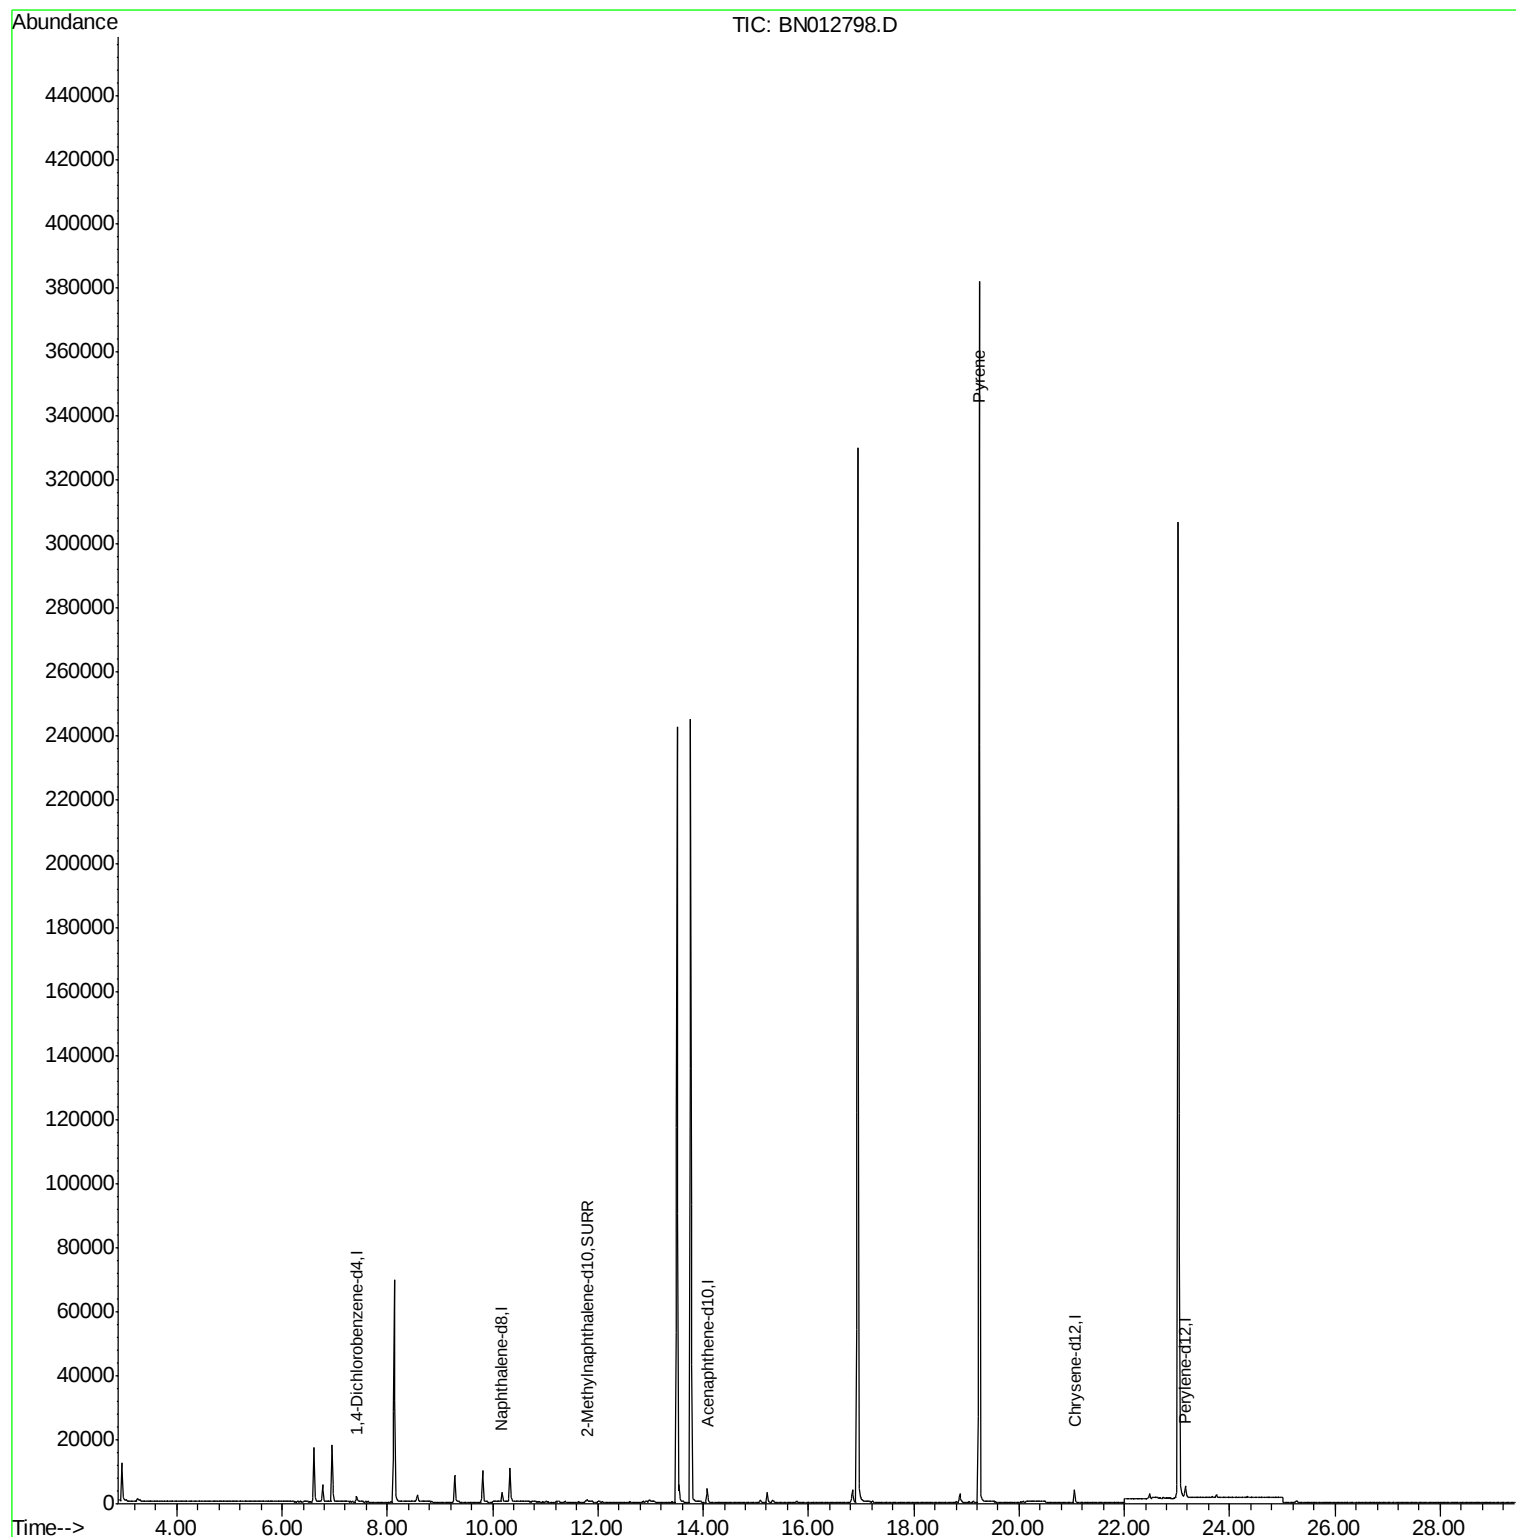

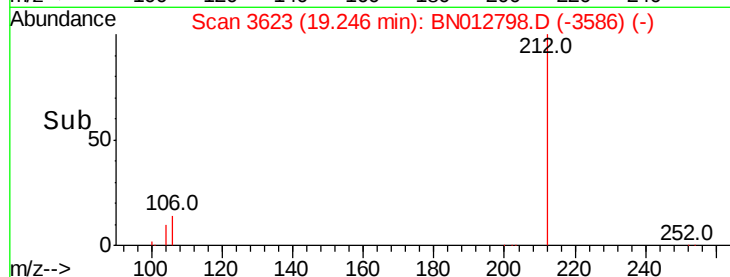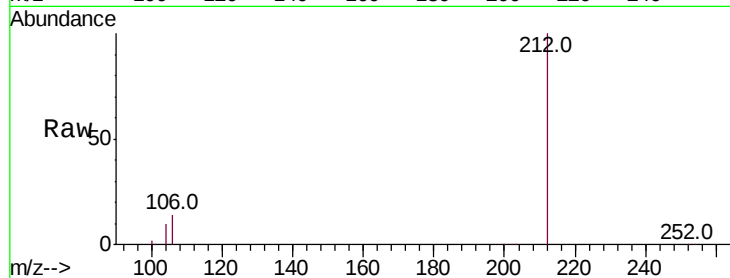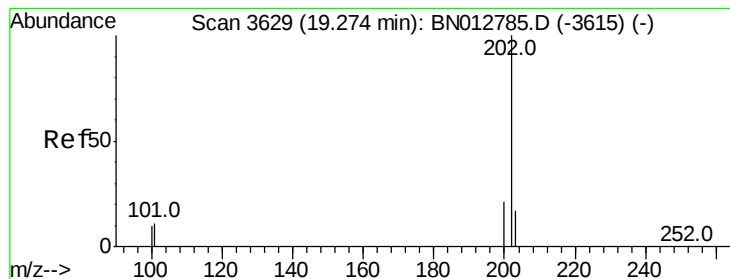

#17

Pvrene

Concen: 0.044 ng/ul

RT: 19.25 min Scan# 3623

Delta R.T. -0.03 min

Lab File: BN012798.D

Acq: 02 Dec 2020 00:52

Instrument :

BNA_N

ClientSampleId :

C0BA8

Tot Ion:202 Resp: 785

Ion Ratio Lower Upper

202 100

101 181.7 8.9 13.3#

100 1229.0 7.4 11.2#

