

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012804.D
 Acq On : 02 Dec 2020 05:05
 Operator : CG/JU
 Sample : L4793-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B54

Quant Time: Dec 02 07:01:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 05:08:42 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	945	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	3903	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2269	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.83	188	4828	0.40	ng/ul	0.00
16) Chrysene-d12	21.05	240	4003	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4369	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.79	152	672	0.12	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	1627	0.13	ng/ul	0.00
Target Compounds				Ovalue		
12) Phenanthrene	16.87	178	1517	0.090	ng/ul	95
15) Fluoranthene	18.90	202	5003	0.258	ng/ul	98
17) Pyrene	19.27	202	5062	0.283	ng/ul	97
18) Benzo(a)anthracene	21.04	228	2175	0.152	ng/ul	96
19) Chrysene	21.09	228	3005	0.168	ng/ul	95
21) Benzo(b)fluoranthene	22.54	252	6270	0.312	ng/ul#	84
22) Benzo(k)fluoranthene	22.54	252	6270	0.271	ng/ul#	83
23) Benzo(a)pyrene	23.07	252	2729	0.144	ng/ul#	86
24) Indeno(1,2,3-cd)pyrene	25.23	276	2230	0.090	ng/ul#	92
25) Dibenzo(a,h)anthracene	25.23	278	498	0.025	ng/ul#	22
26) Benzo(g,h,i)perylene	25.86	276	2131	0.096	ng/ul#	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012804.D
Acq On : 02 Dec 2020 05:05
Operator : CG/JU
Sample : L4793-21
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B54

Quant Time: Dec 02 07:01:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 05:08:42 2020
Response via : Initial Calibration

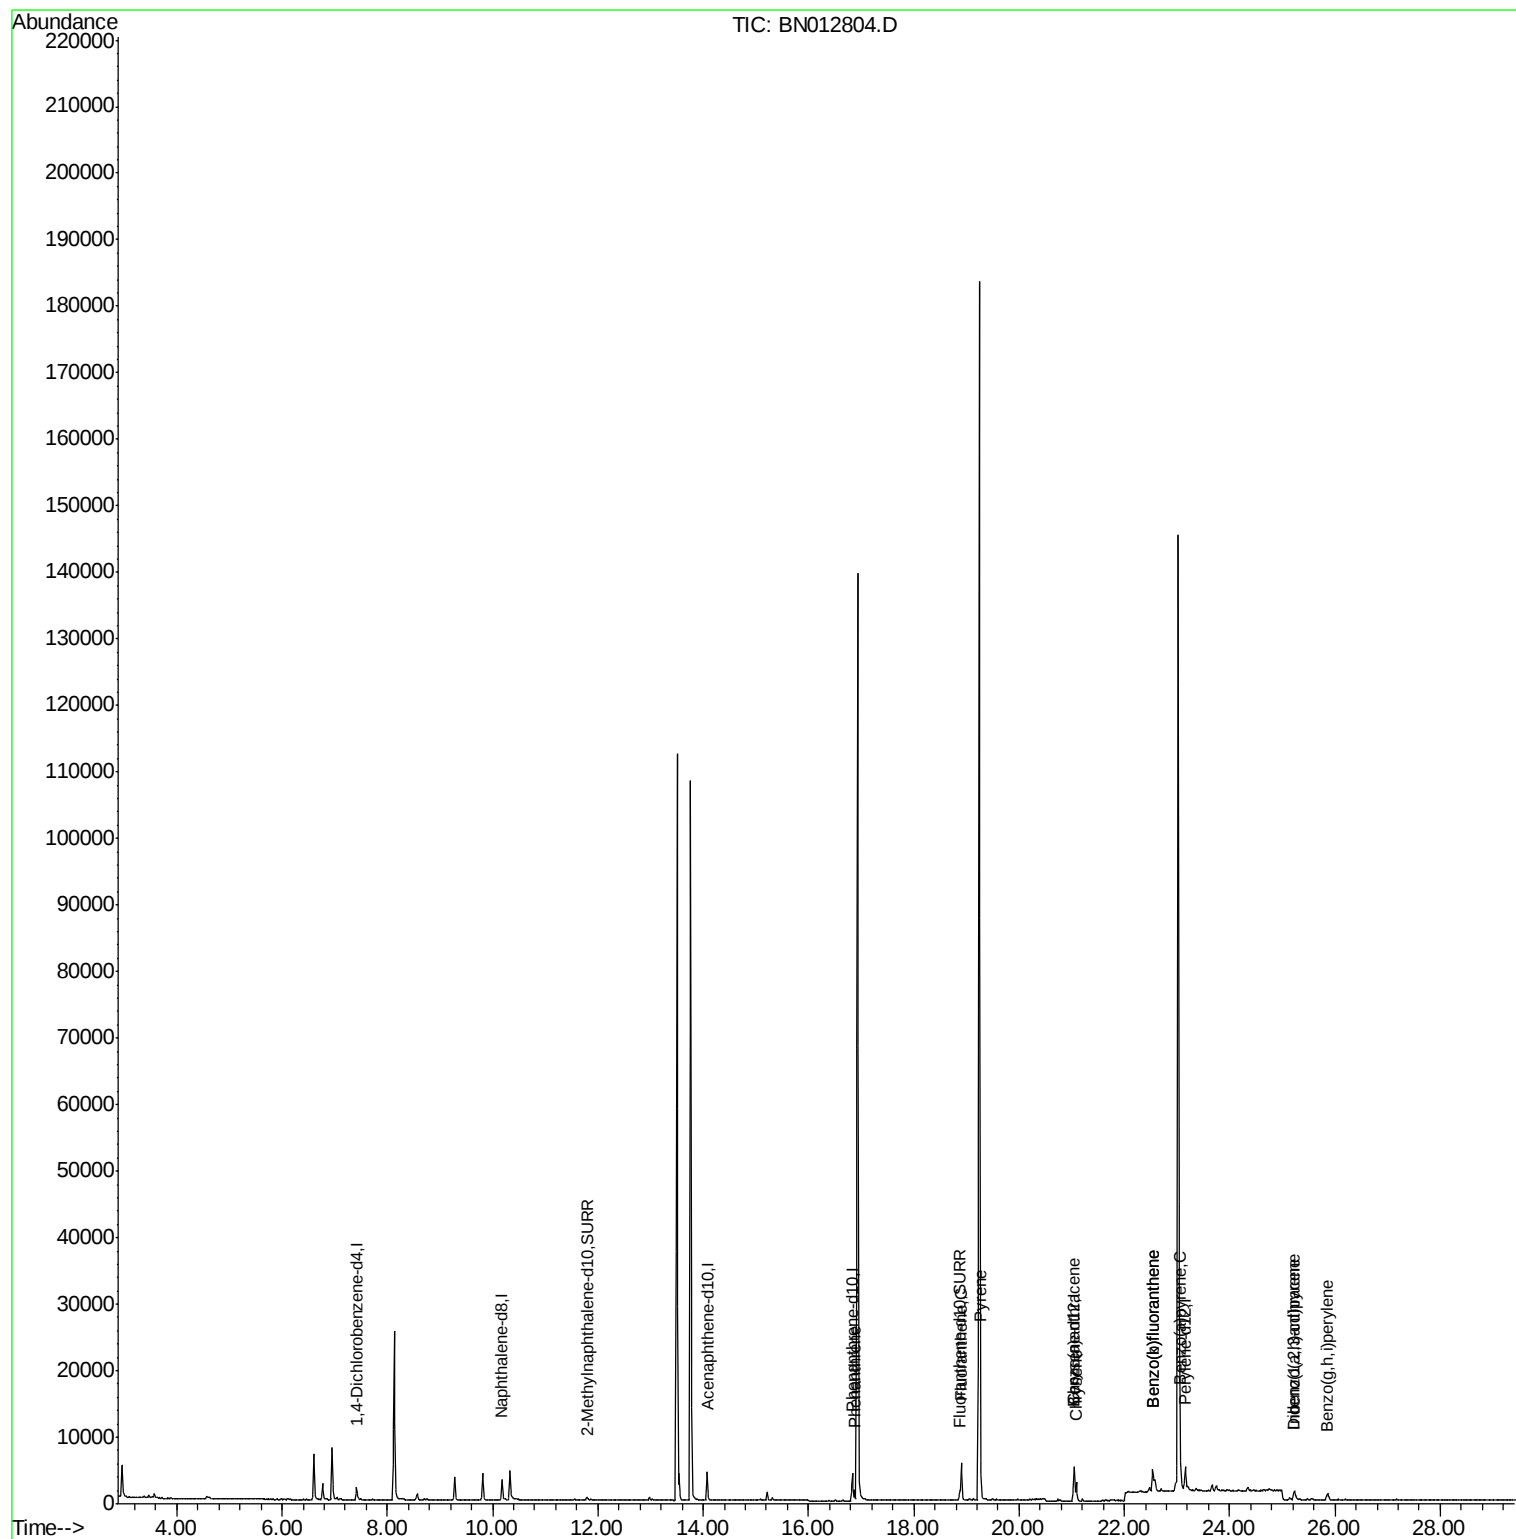

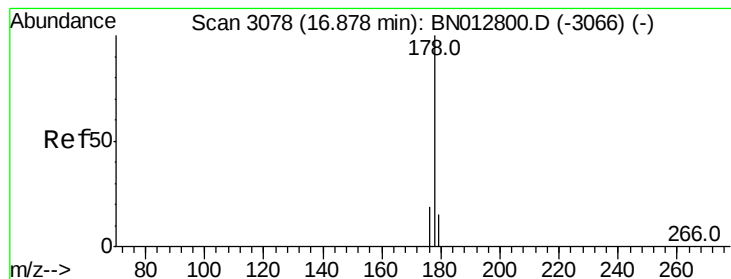

#12

Phenanthrene

Concen: 0.090 ng/ul

RT: 16.87 min Scan# 3077

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05

Instrument :

BNA_N

ClientSampleId :

C0B54


Tot Ion:178 Resp: 1517

Ion Ratio Lower Upper

178 100

179 19.6 13.8 20.6




176 22.8 16.7 25.1

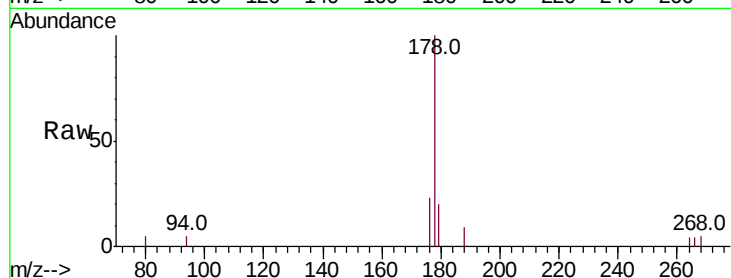

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

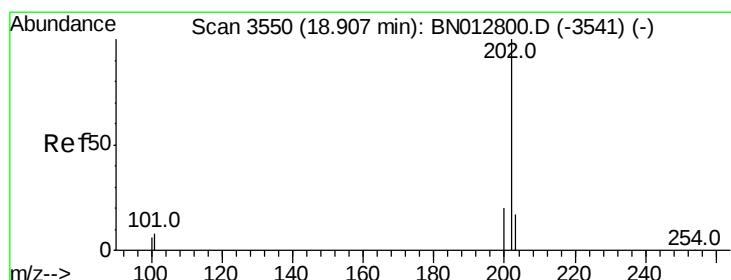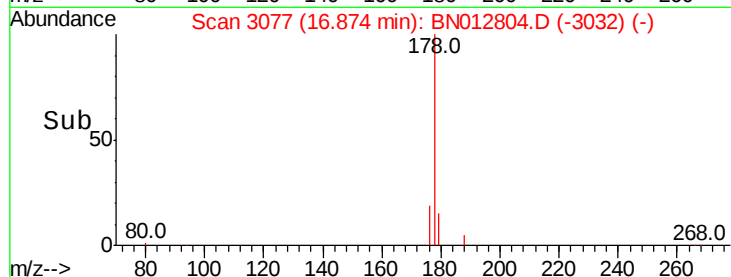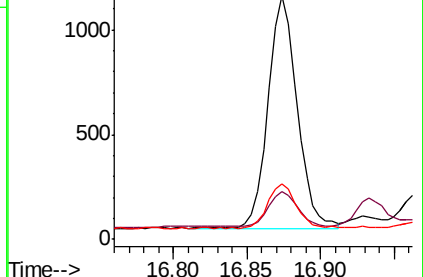

#15

Fluoranthene

Concen: 0.258 ng/ul

RT: 18.90 min Scan# 3549

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05


Tgt Ion:202 Resp: 5003

Ion Ratio Lower Upper

202 100

101 11.4 0.0 30.5



100 9.2 0.0 28.4

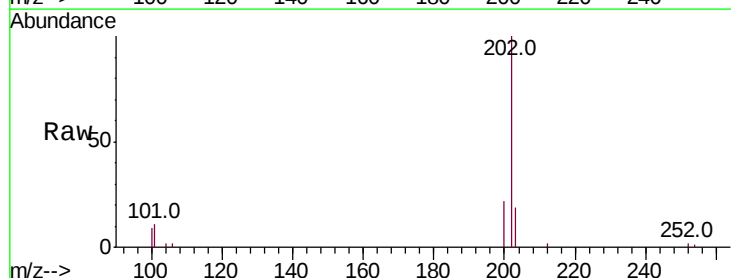


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

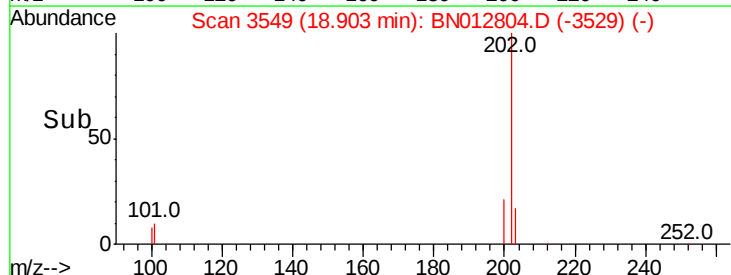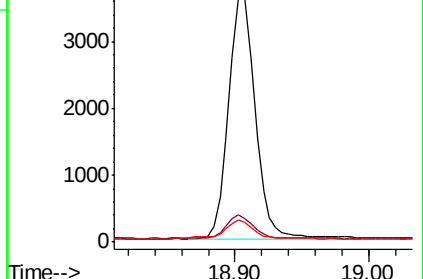

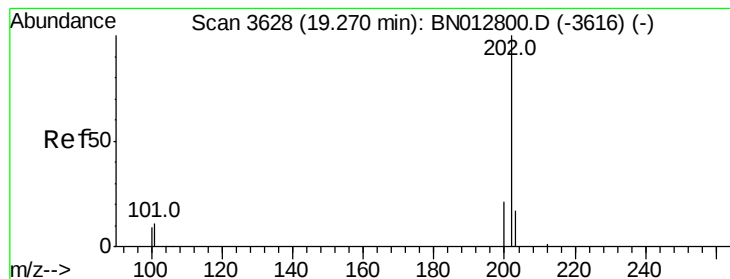

#17

Pvrene

Concen: 0.283 ng/ul

RT: 19.27 min Scan# 3628

Delta R.T. -0.00 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05

Instrument :

BNA_N

ClientSampleId :

C0B54


Tot Ion:202 Resp: 5062

Ion Ratio Lower Upper

202 100

101 12.3 8.9 13.3




100 10.6 7.4 11.2

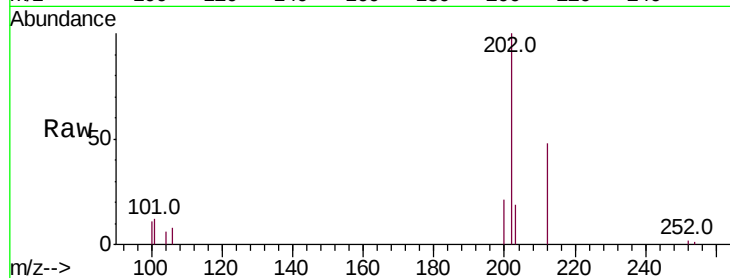

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

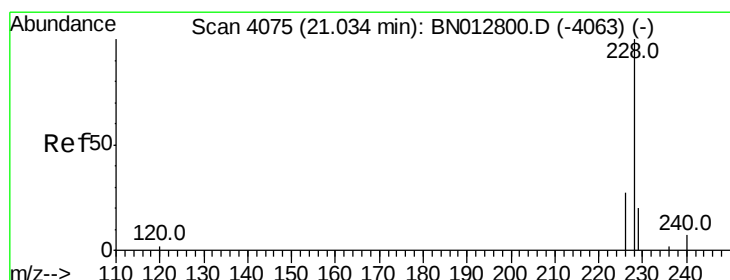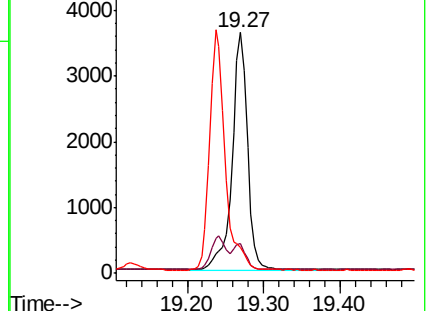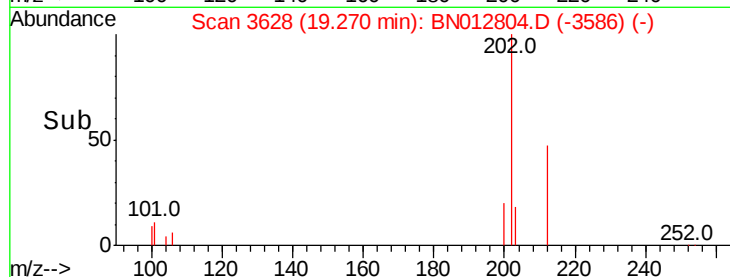

#18

Benzo(a)anthracene

Concen: 0.152 ng/ul

RT: 21.04 min Scan# 4076

Delta R.T. -0.00 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05


Tgt Ion:228 Resp: 2175

Ion Ratio Lower Upper

228 100

229 23.0 16.9 25.3



226 31.3 23.1 34.7

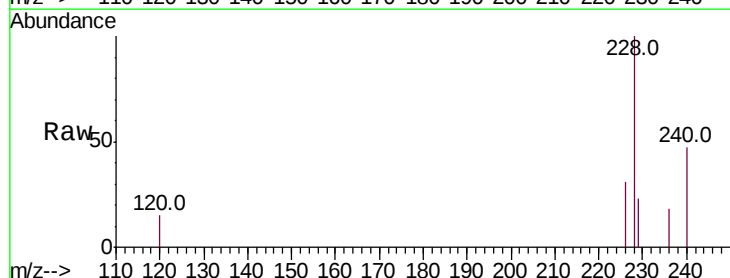


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

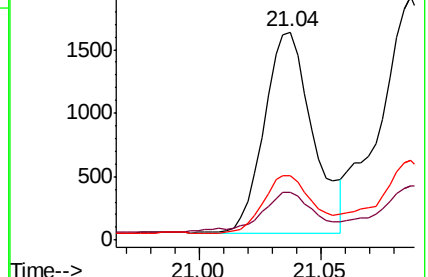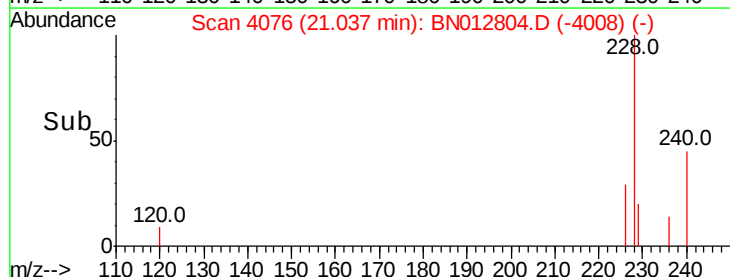

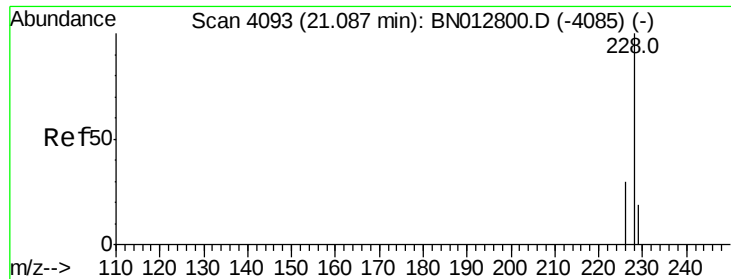

#19

Chrysene

Concen: 0.168 ng/ul

RT: 21.09 min Scan# 4093

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05

Instrument :

BNA_N

ClientSampleId :

C0B54


Tot Ion:228 Resp: 3005

Ion Ratio Lower Upper

228 100

226 33.0 24.4 36.6




229 22.3 16.1 24.1

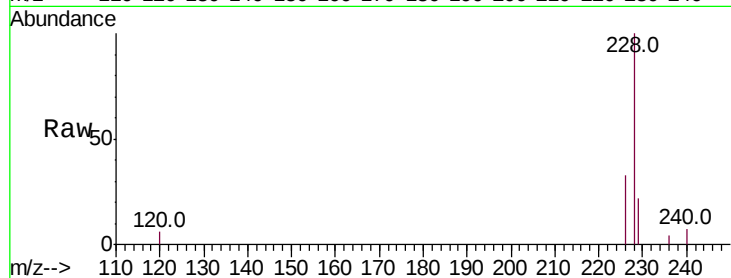

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

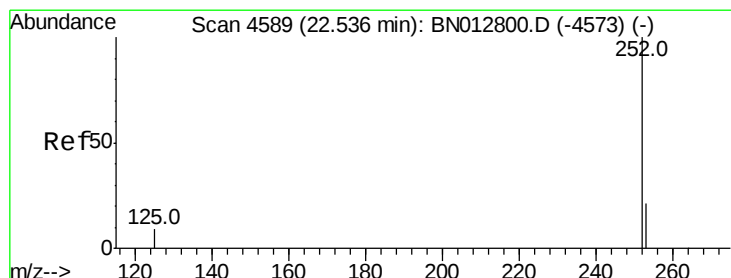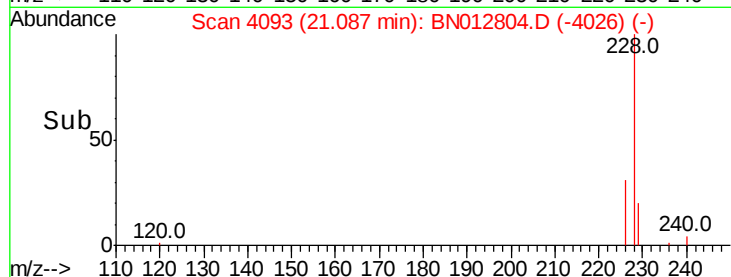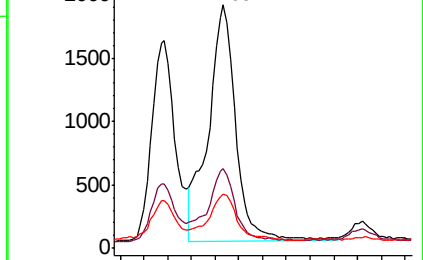

#21

Benzo(b)fluoranthene

Concen: 0.312 ng/ul

RT: 22.54 min Scan# 4589

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05


Tgt Ion:252 Resp: 6270

Ion Ratio Lower Upper

252 100

253 33.1 0.0 58.4



125 28.7 0.0 28.6#

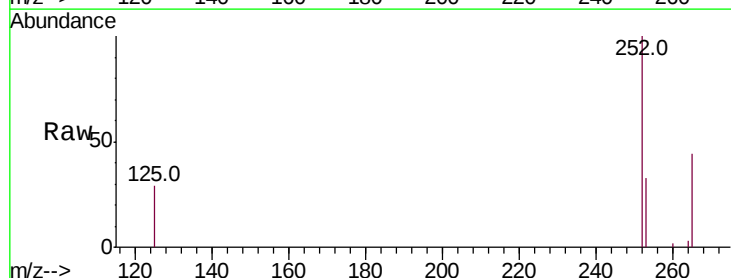


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

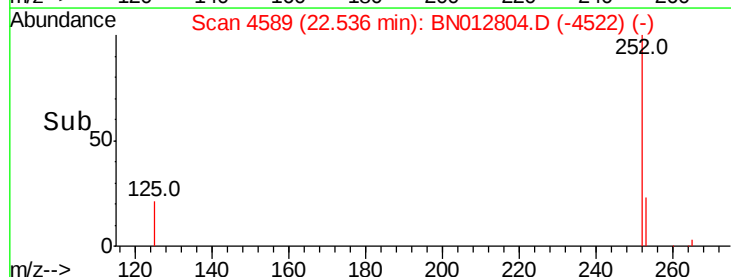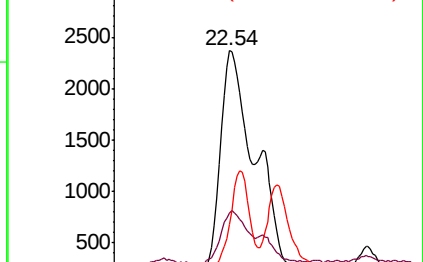

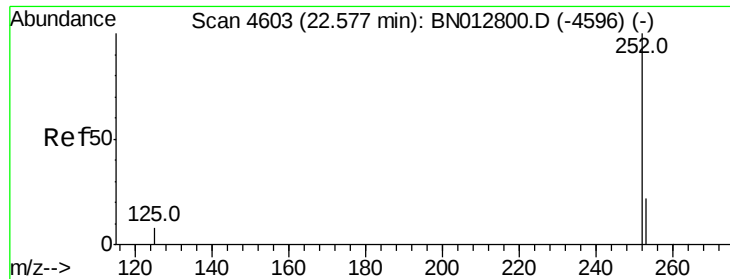

#22

Benzo(k)fluoranthene

Concen: 0.271 ng/ul

RT: 22.54 min Scan# 4589

Delta R.T. -0.05 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05

Instrument :

BNA_N

ClientSampleId :

C0B54


Tot Ion:252 Resp: 6270

Ion Ratio Lower Upper

252 100

253 33.1 23.4 35.2




125 28.7 10.2 15.2#

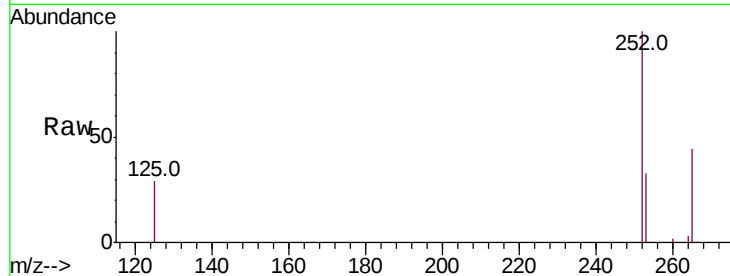

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

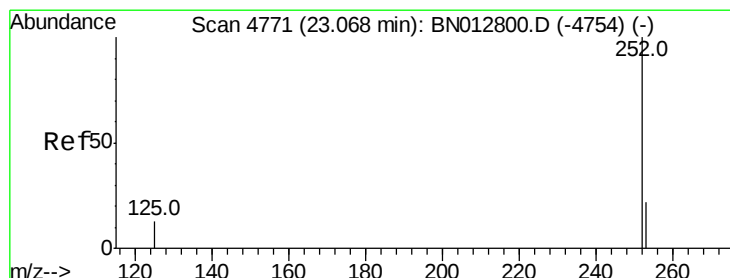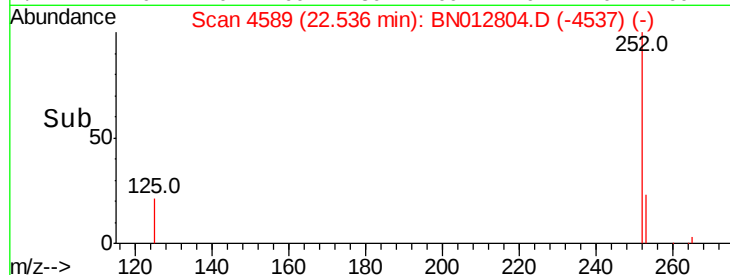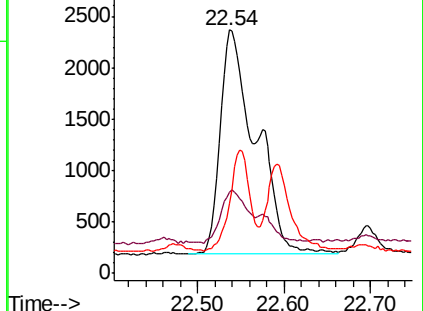

#23

Benzo(a)pyrene

Concen: 0.144 ng/ul

RT: 23.07 min Scan# 4770

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05


Tgt Ion:252 Resp: 2729

Ion Ratio Lower Upper

252 100

253 36.8 27.6 41.4



125 35.7 17.0 25.4#

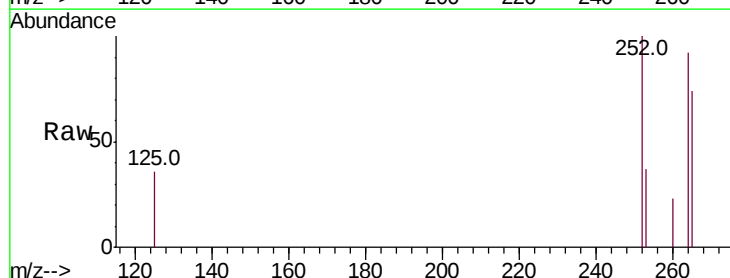


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

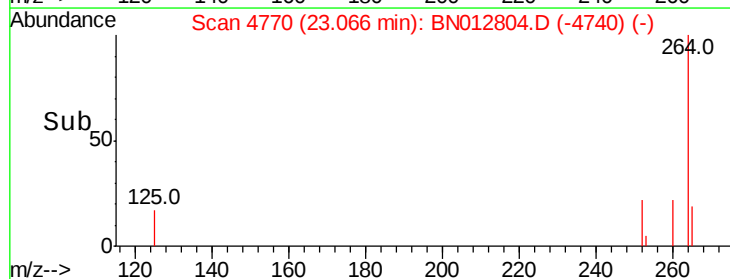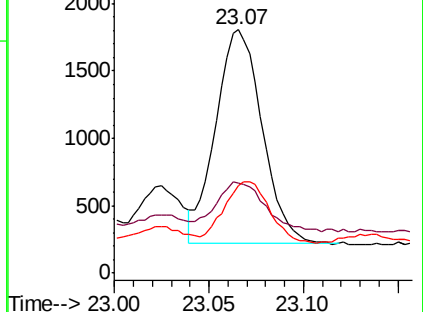




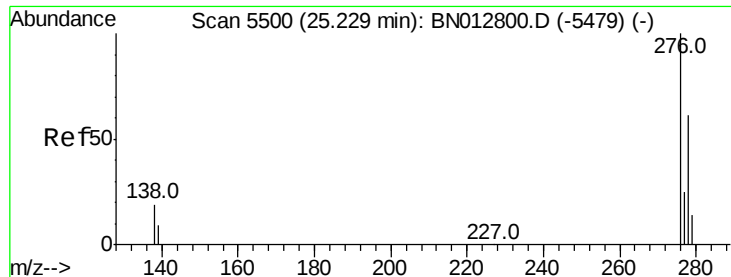


#24

Indeno(1,2,3-cd)pyrene
Concen: 0.090 ng/u1
RT: 25.23 min Scan# 5500
Delta R.T. -0.01 min
Lab File: BN012804.D
Acq: 02 Dec 2020 05:05

Instrument :
BNA_N
ClientSampleId :
C0B54




Tot Ion:276 Resp: 2230
Ion Ratio Lower Upper
276 100
138 24.3 16.5 24.7
227 0.2 0.1 0.1#

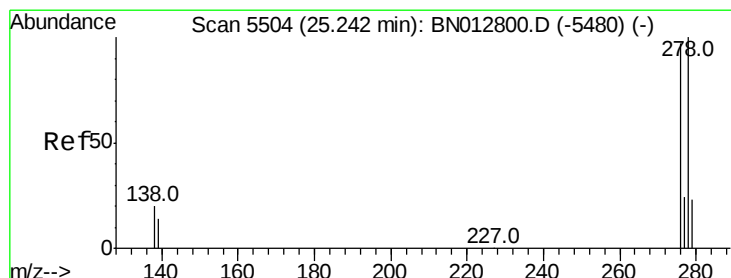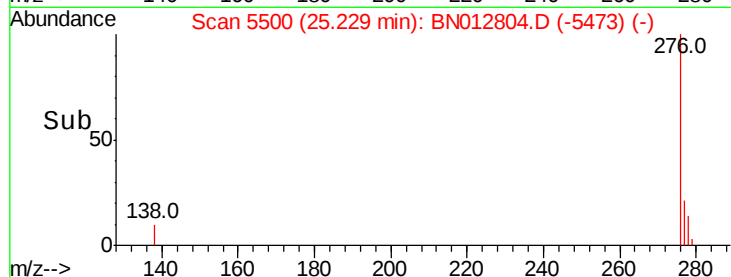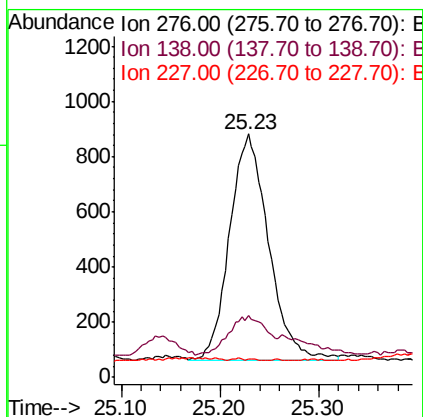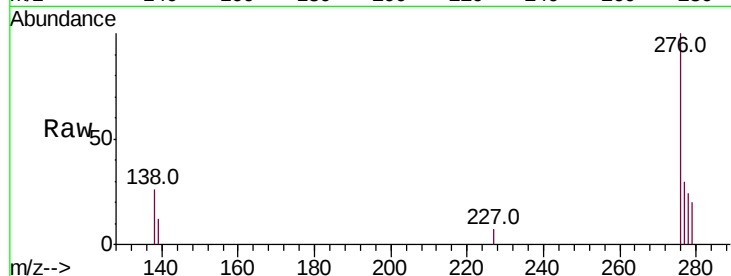


#25

Dibenzo(a,h)anthracene
Concen: 0.025 ng/u1
RT: 25.23 min Scan# 5501
Delta R.T. -0.02 min
Lab File: BN012804.D
Acq: 02 Dec 2020 05:05

Tgt Ion:278 Resp: 498
Ion Ratio Lower Upper
278 100
139 47.3 13.8 20.8#
279 78.3 25.6 38.4#

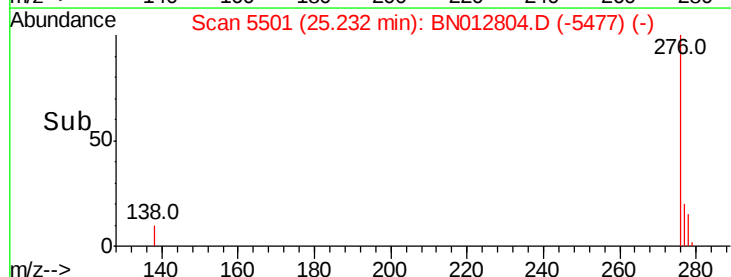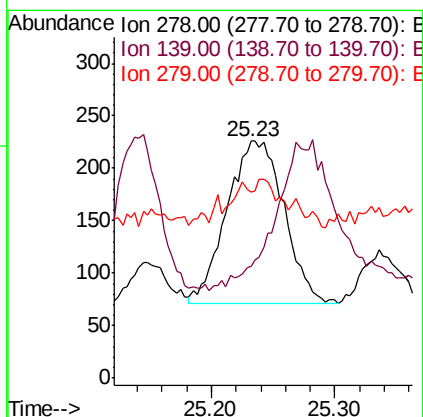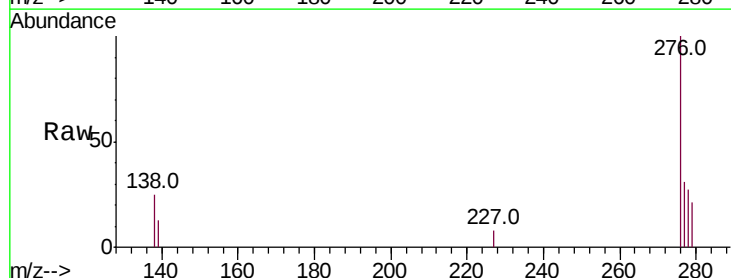

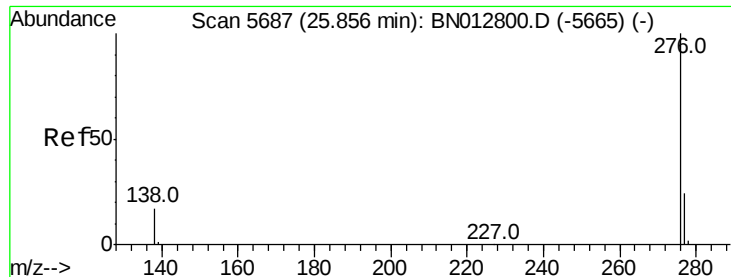

#26

Benzo(a,h,i)perylene

Concen: 0.096 ng/ul

RT: 25.86 min Scan# 5688

Delta R.T. -0.01 min

Lab File: BN012804.D

Acq: 02 Dec 2020 05:05

Instrument :

BNA_N

ClientSampleId :

C0B54


Tot Ion:276 Resp: 2131

Ion Ratio Lower Upper

276 100

138 26.9 16.3 24.5#

277 30.4 21.8 32.8

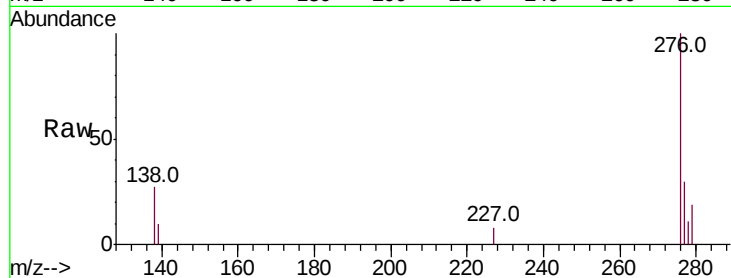

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

