

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012805.D
 Acq On : 02 Dec 2020 05:41
 Operator : CG/JU
 Sample : L4865-09
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC6

Quant Time: Dec 02 07:01:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 05:08:42 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	913	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	3765	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2253	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.84
16) Chrysene-d12	21.05	240	3887	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4234	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.79	152	1172	0.22	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	2581	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.24	202	586	0.034	ng/ul#	1
23) Benzo(a)pyrene	23.03	252	1256	0.069	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012805.D
Acq On : 02 Dec 2020 05:41
Operator : CG/JU
Sample : L4865-09
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC6

Quant Time: Dec 02 07:01:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 05:08:42 2020
Response via : Initial Calibration




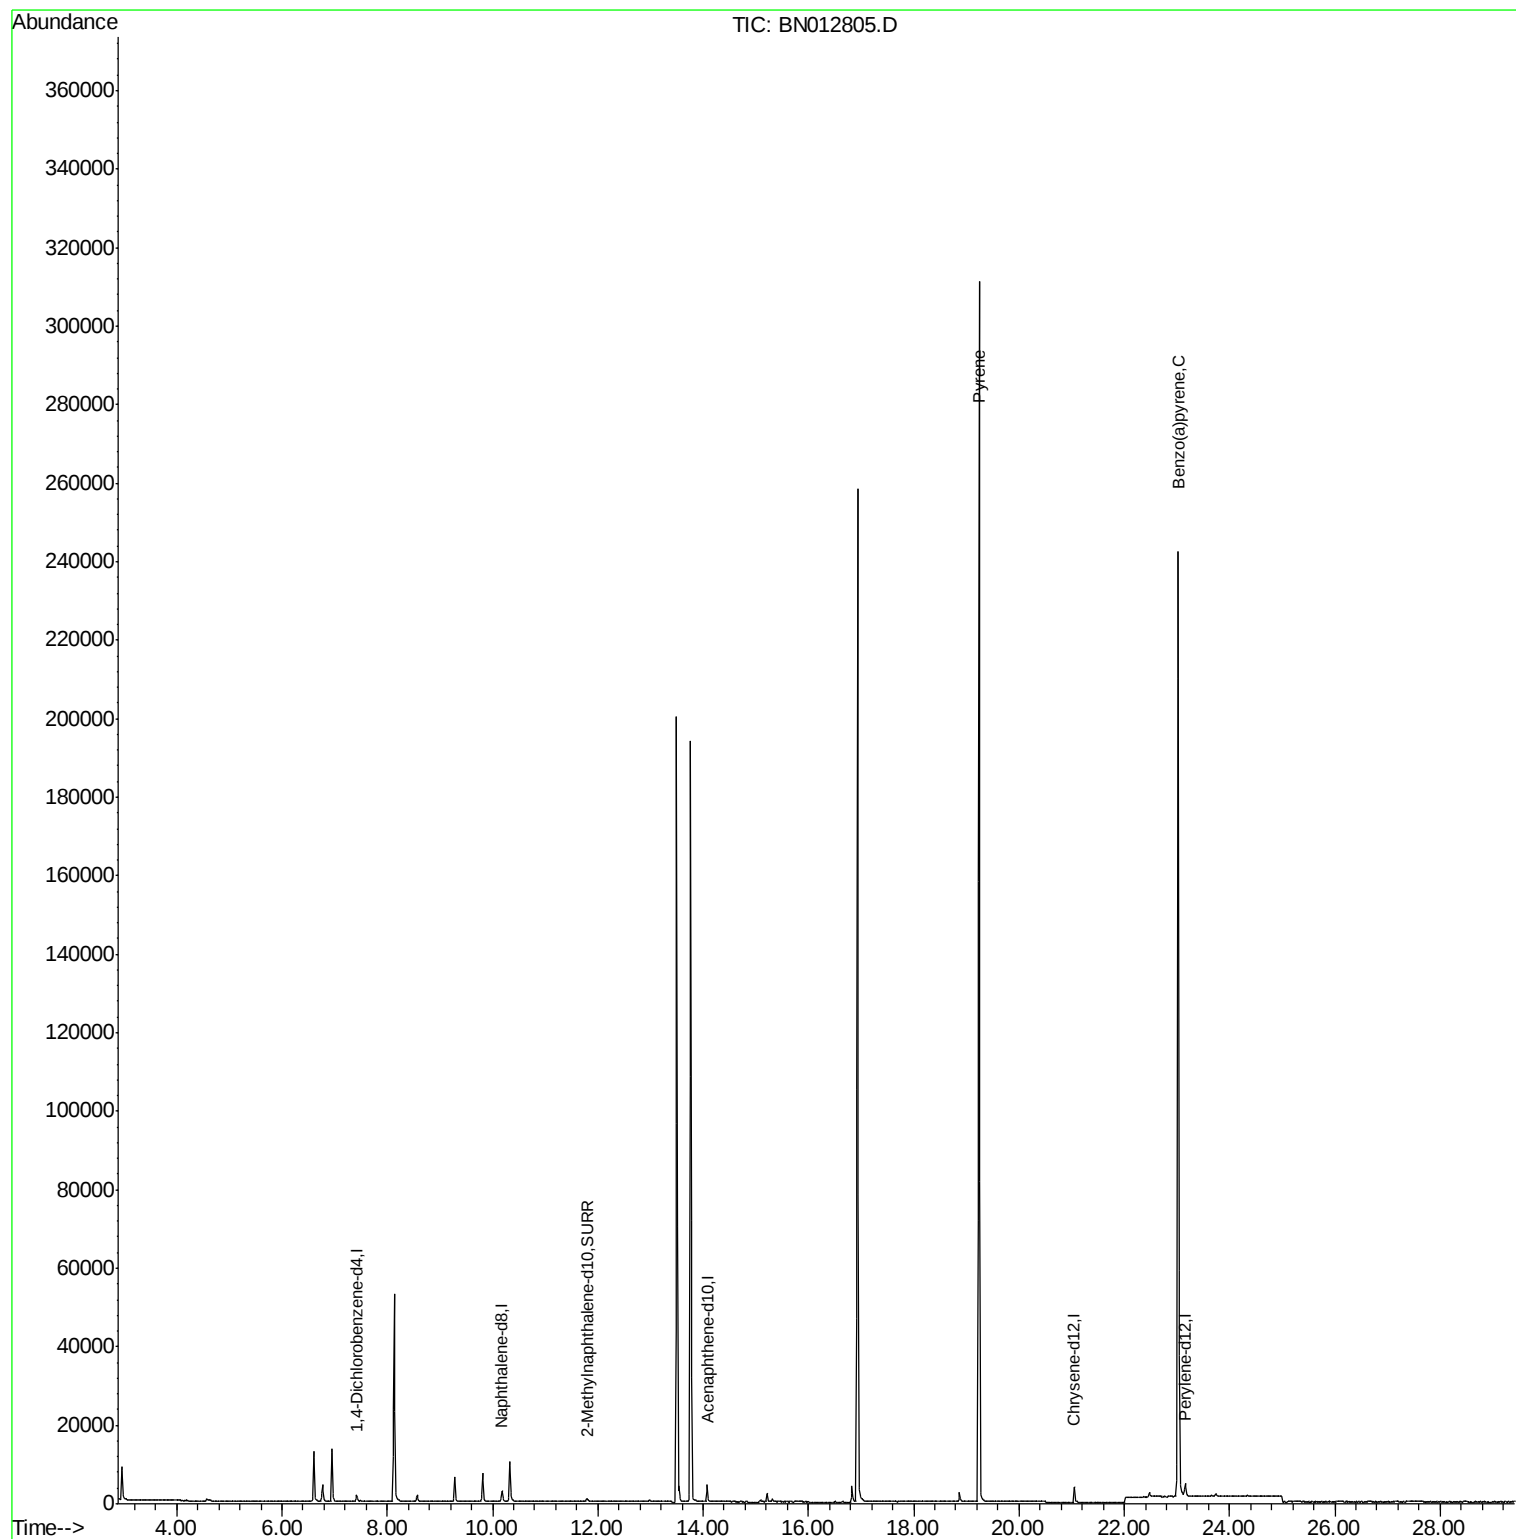


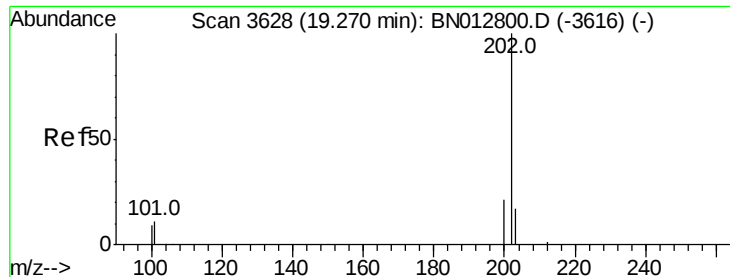

#17
Pvrene
Concen: 0.034 ng/ul
RT: 19.24 min Scan# 3622
Delta R.T. -0.03 min
Lab File: BN012805.D
Acq: 02 Dec 2020 05:41

Instrument :
BNA_N
ClientSampleId :
C0BC6

Tot Ion:202 Resp: 586
Ion Ratio Lower Upper
202 100
101 204.3 8.9 13.3#
100 1429.6 7.4 11.2#

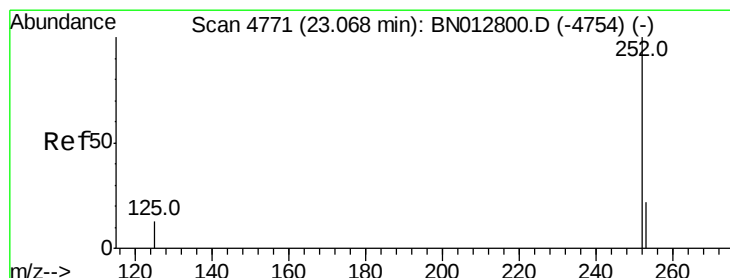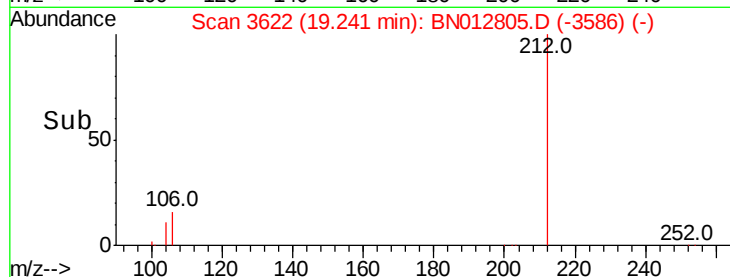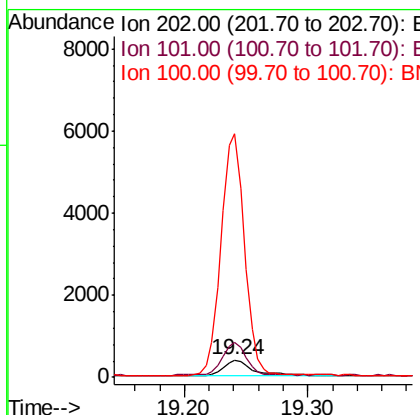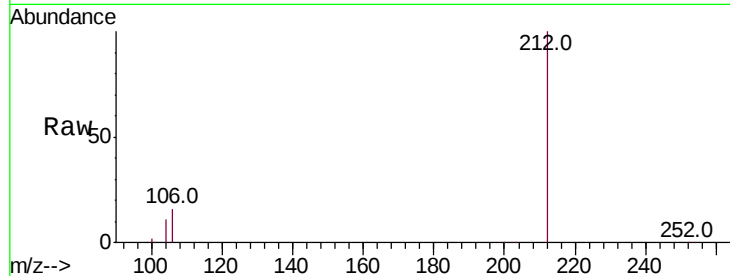

#23
Benzo(a)pyrene
Concen: 0.069 ng/ul
RT: 23.03 min Scan# 4757
Delta R.T. -0.05 min
Lab File: BN012805.D
Acq: 02 Dec 2020 05:41

Tgt Ion:252 Resp: 1256
Ion Ratio Lower Upper
252 100
253 55.8 27.6 41.4#
125 44.3 17.0 25.4#

