


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120220\
Data File : BN012775.D
Acq On : 01 Dec 2020 10:55
Operator : CG/JU
Sample : PB133172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:13 PM

Quant Time: Dec 01 11:28:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 10:54:12 2020
Response via : Initial Calibration

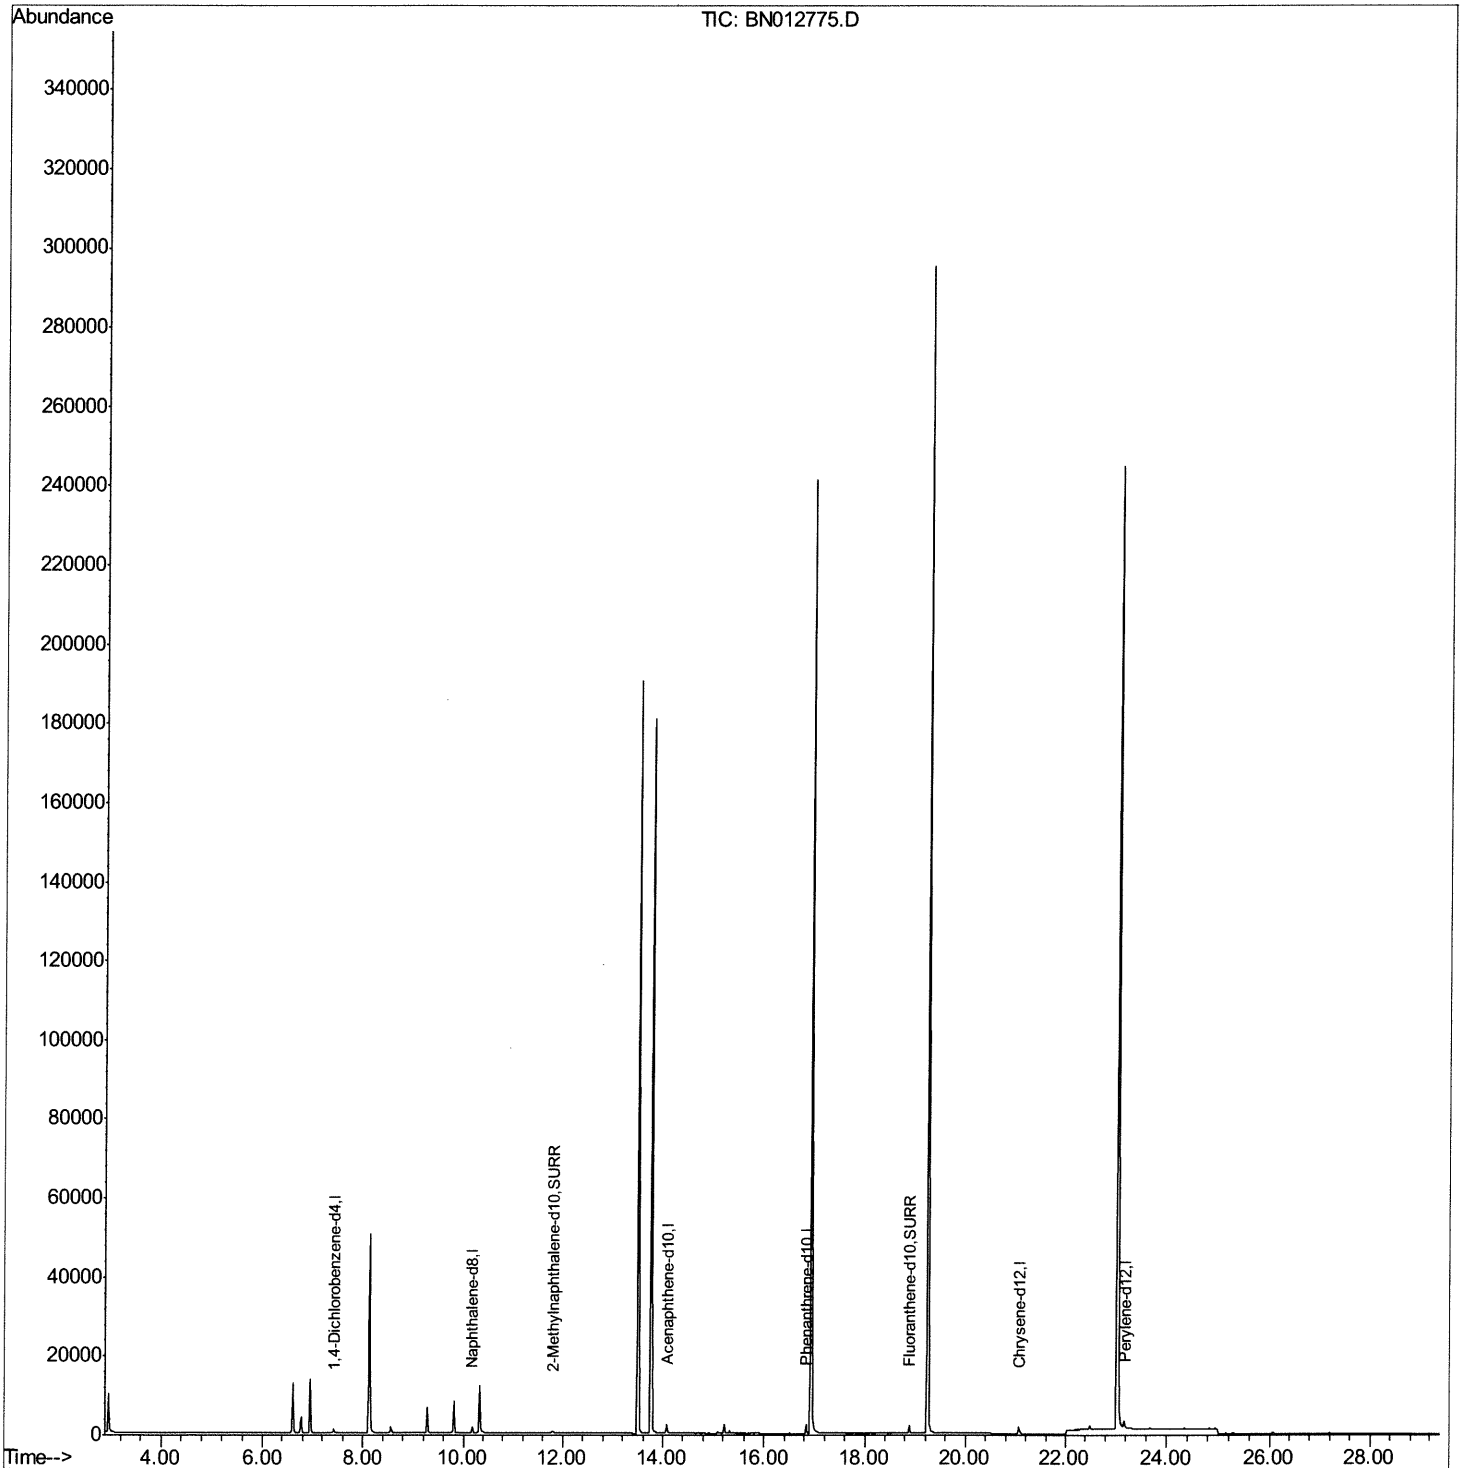

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120220\
Data File : BN012775.D
Acq On : 01 Dec 2020 10:55
Operator : CG/JU
Sample : PB133172BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK72

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:13 PM

Quant Time: Dec 01 11:27:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 10:54:12 2020
Response via : Initial Calibration

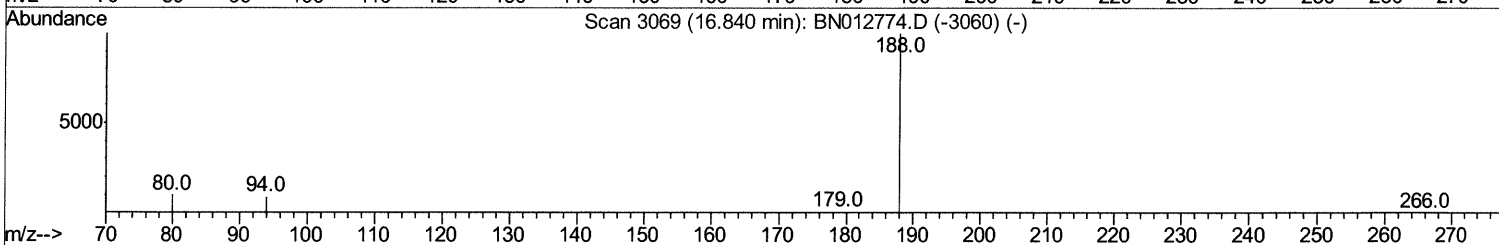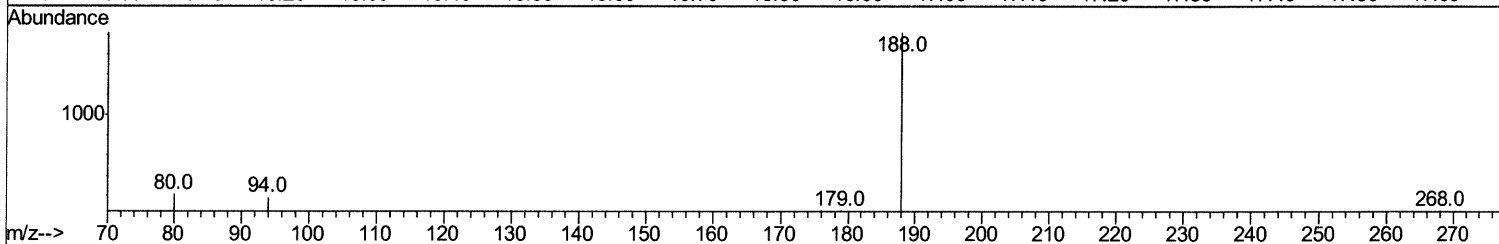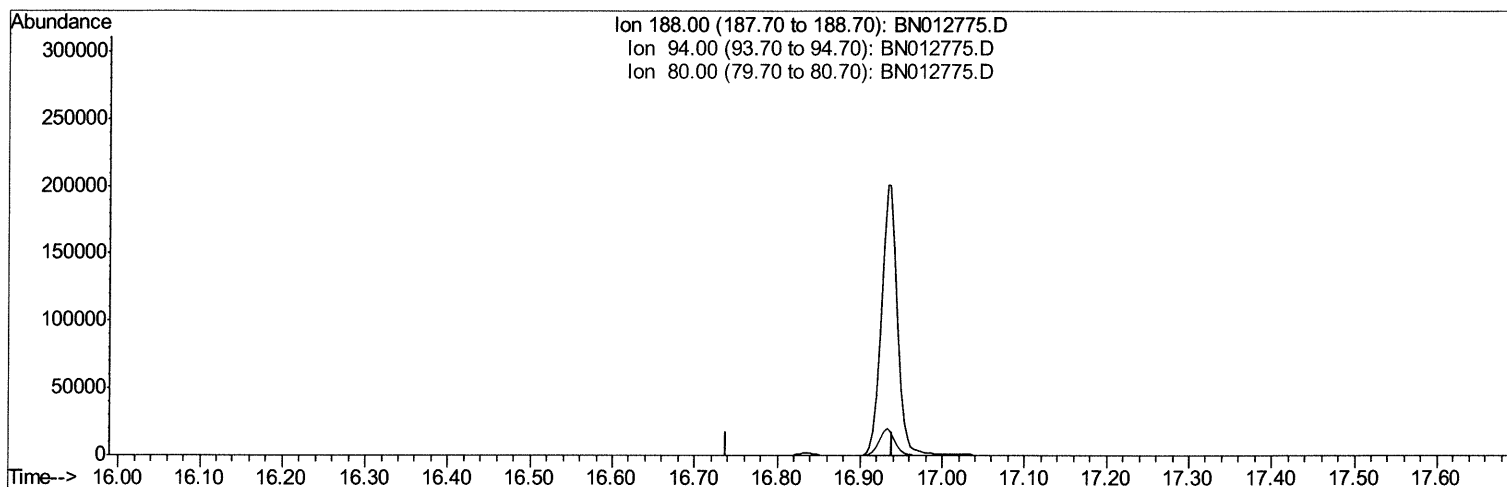

TIC: BN012775.D

(10) Phenanthrene-d10 (I)

16.840min (-16.840) 0.00ng/ui

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120220\
 Data File : BN012775.D
 Acq On : 01 Dec 2020 10:55
 Operator : CG/JU
 Sample : PB133172BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK72

Manual Integrations
 APPROVED

mohammad
 12/2/2020 2:27:13 PM

Quant Time: Dec 01 11:27:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 10:54:12 2020
 Response via : Initial Calibration

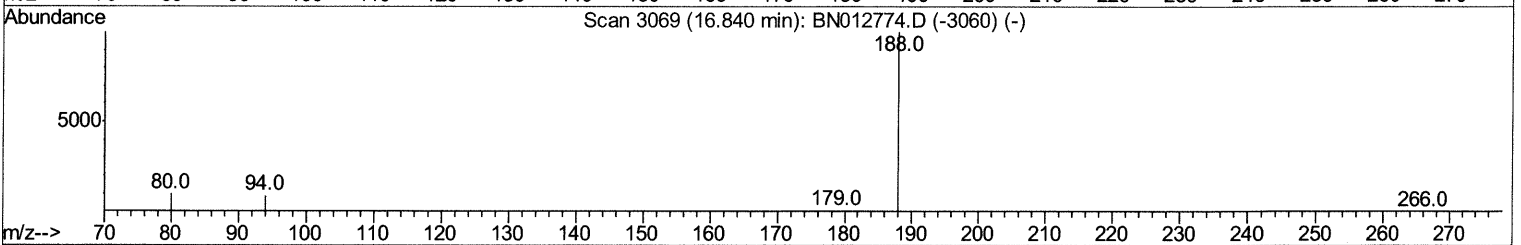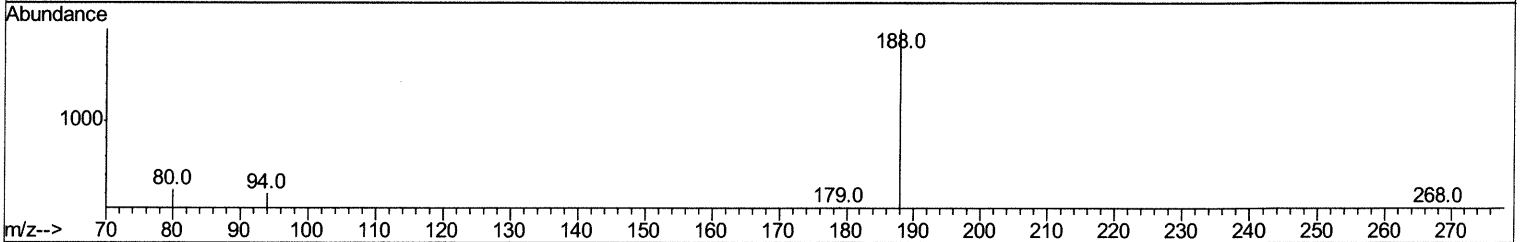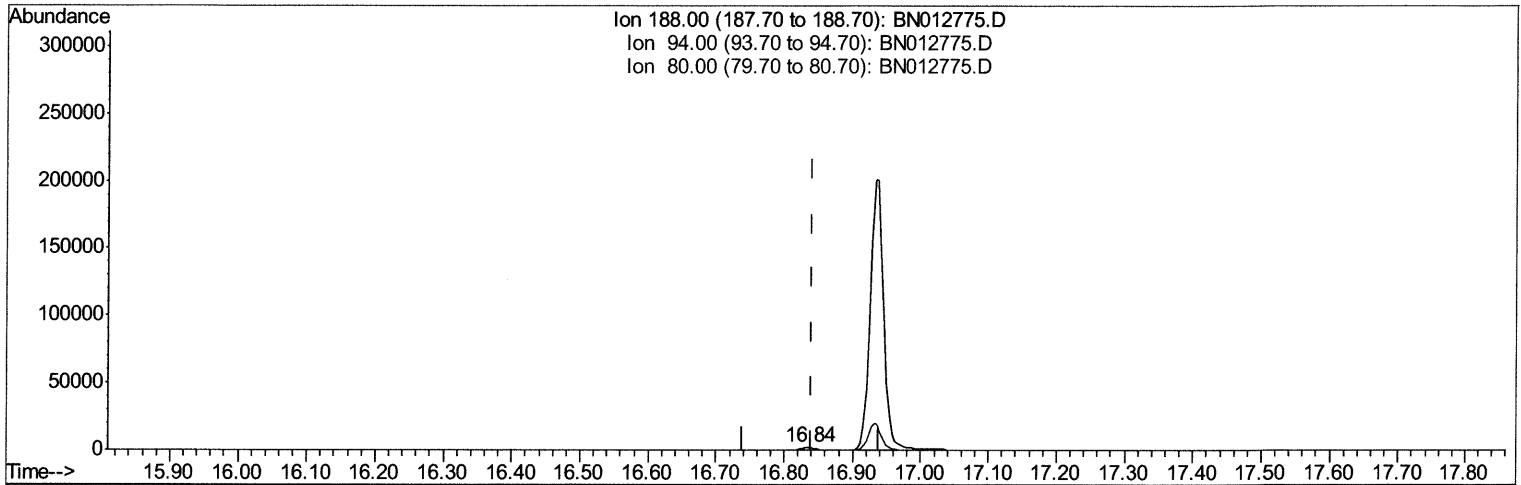

TIC: BN012775.D

(10) Phenanthrene-d10 (I)

16.835min (-0.004) 0.40ng/ul m 12/04/20 JU

response 2748

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	10.02
80.00	12.60	12.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN120220\
 Data File : BN012775.D
 Acq On : 01 Dec 2020 10:55
 Operator : CG/JU
 Sample : PB133172BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK72

Manual Integrations
 APPROVED

mohammad
 12/2/2020 2:27:13 PM

Quant Time: Dec 01 11:28:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 10:54:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	528	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	2061	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	1297	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.84	188	2748m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.06	240	2166	0.40	ng/ul	0.00
20) Perylene-d12	23.17	264	2676	0.40	ng/ul	0.00

12/04/2020

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.80	152	1017	0.34	ng/ul	0.01
14) Fluoranthene-d10	18.88	212	2287	0.32	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed