


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012786.D
Acq On : 01 Dec 2020 17:39
Operator : CG/JU
Sample : PB133292BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:35 PM

Quant Time: Dec 02 01:04:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

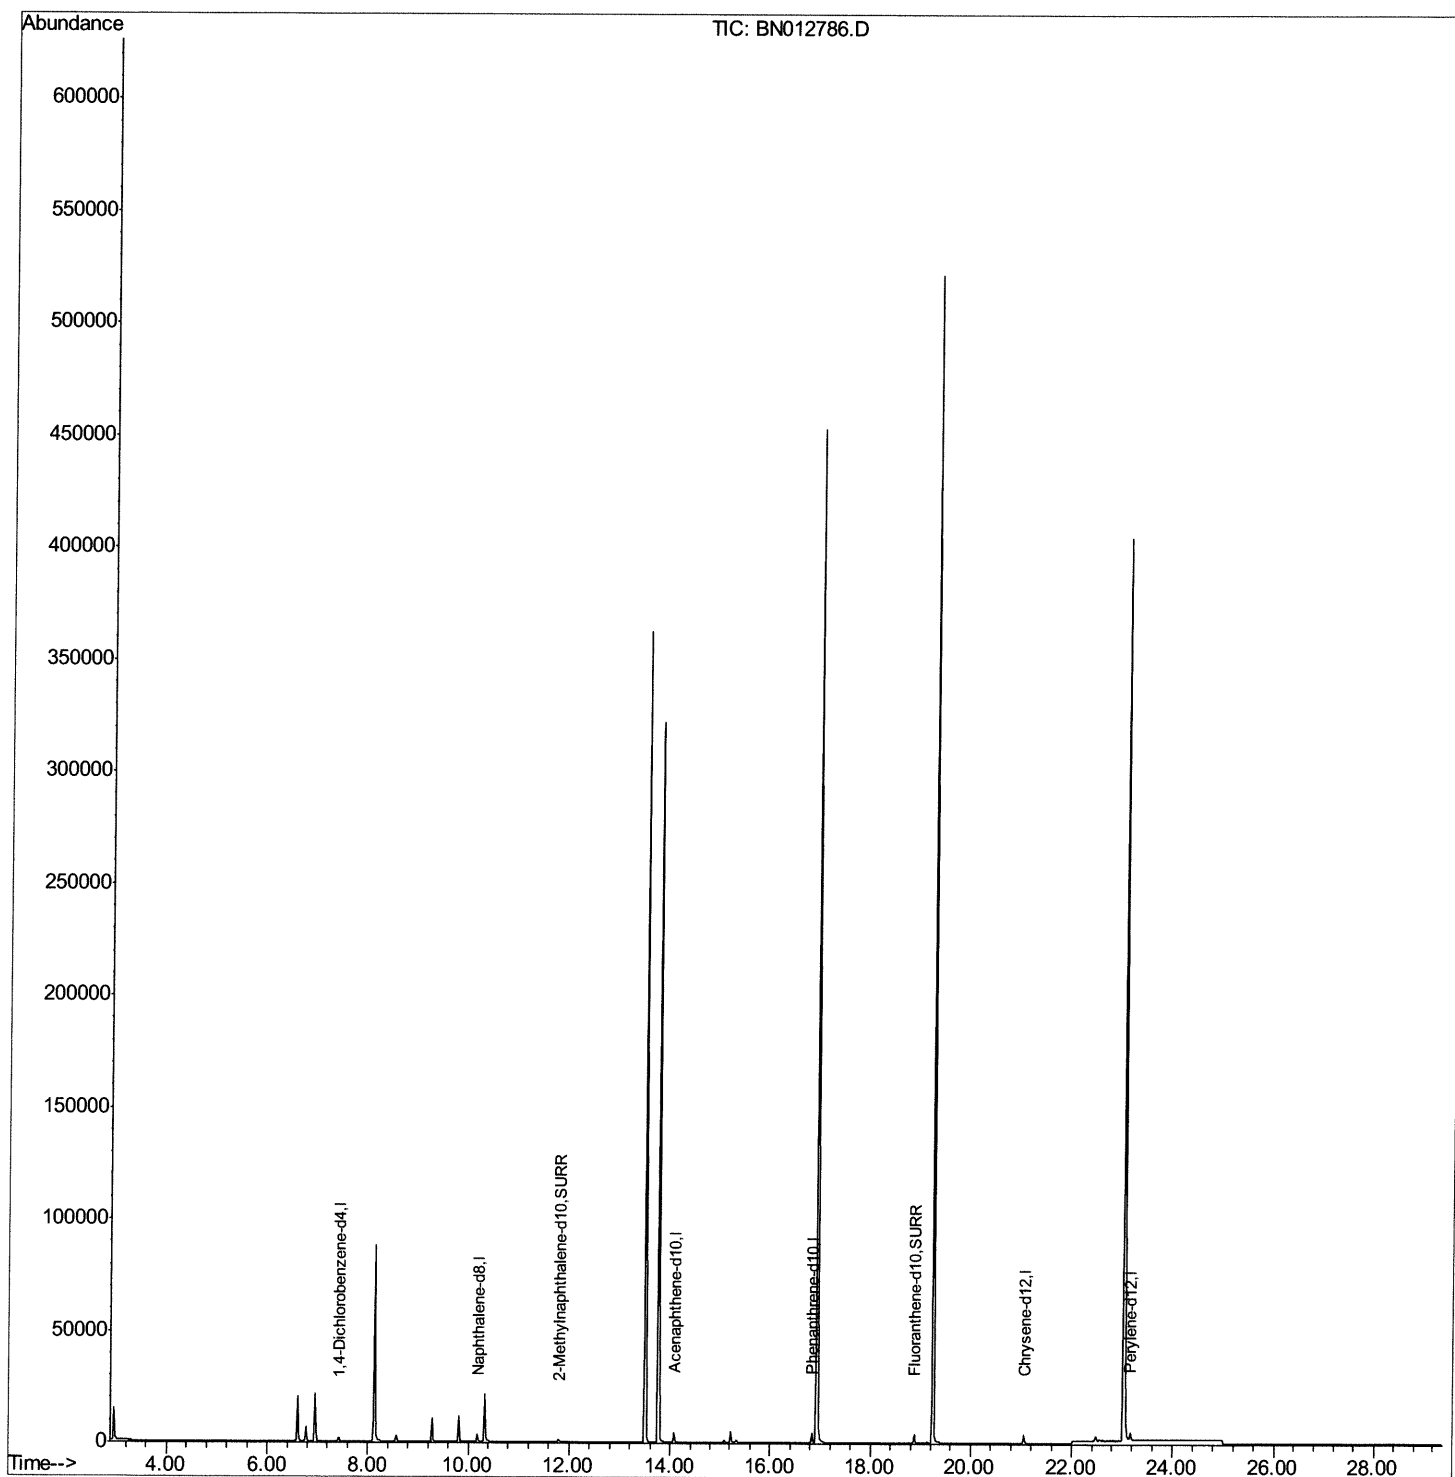

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012786.D
Acq On : 01 Dec 2020 17:39
Operator : CG/JU
Sample : PB133292BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:35 PM

Quant Time: Dec 02 00:56:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

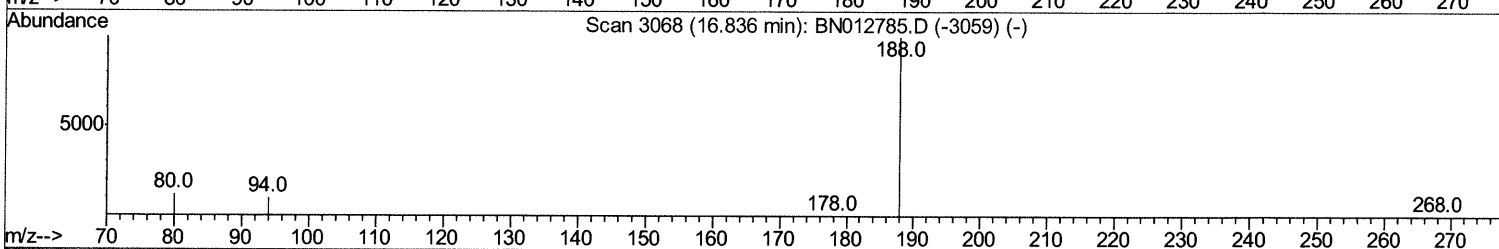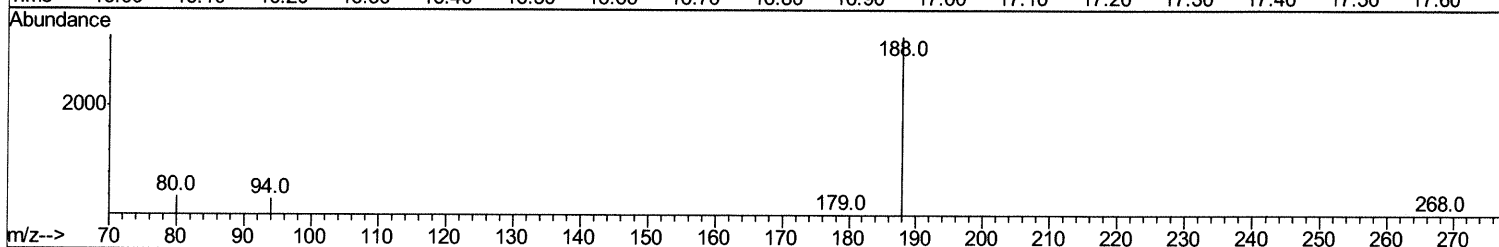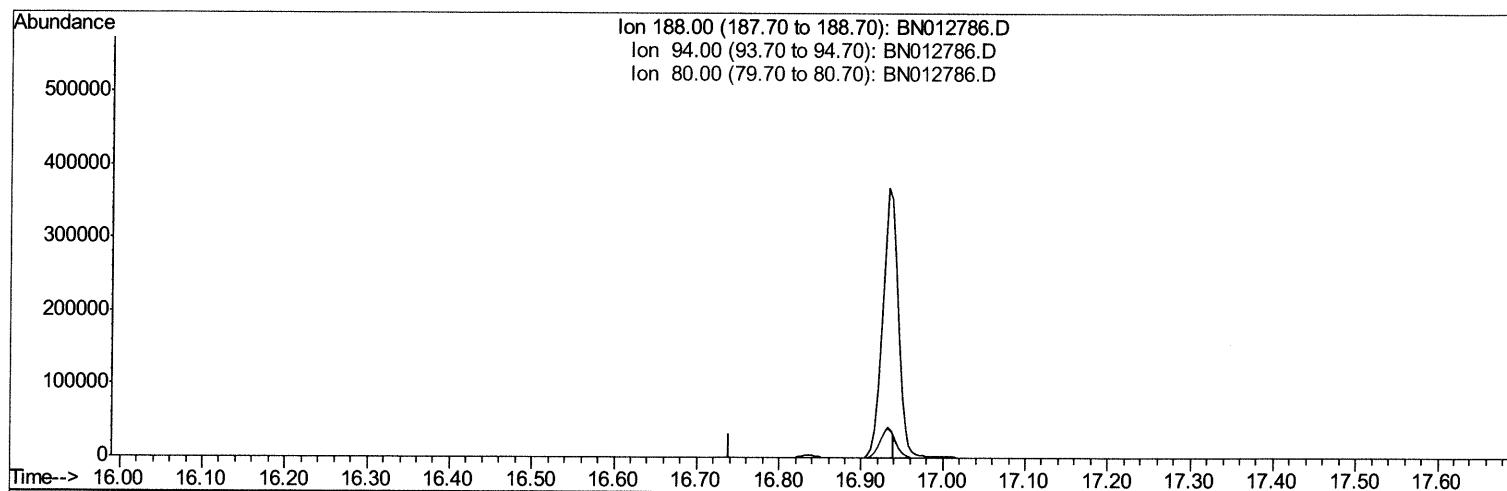

TIC: BN012786.D

(10) Phenanthrene-d10 (I)

16.840min (-16.840) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012786.D
Acq On : 01 Dec 2020 17:39
Operator : CG/JU
Sample : PB133292BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:35 PM

Quant Time: Dec 02 00:56:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

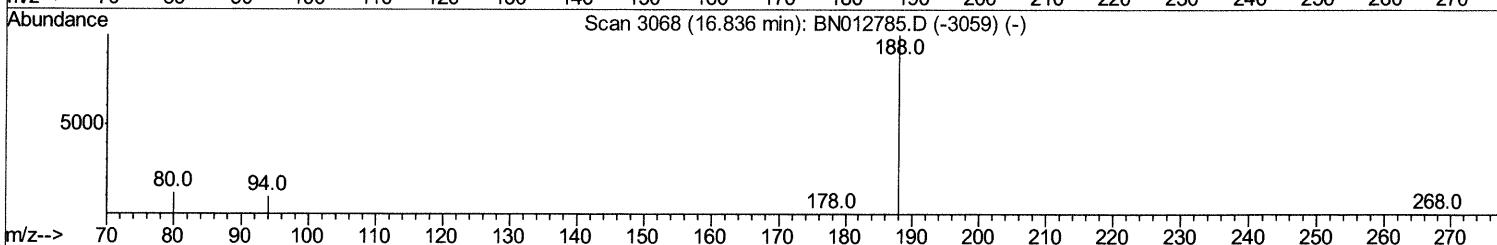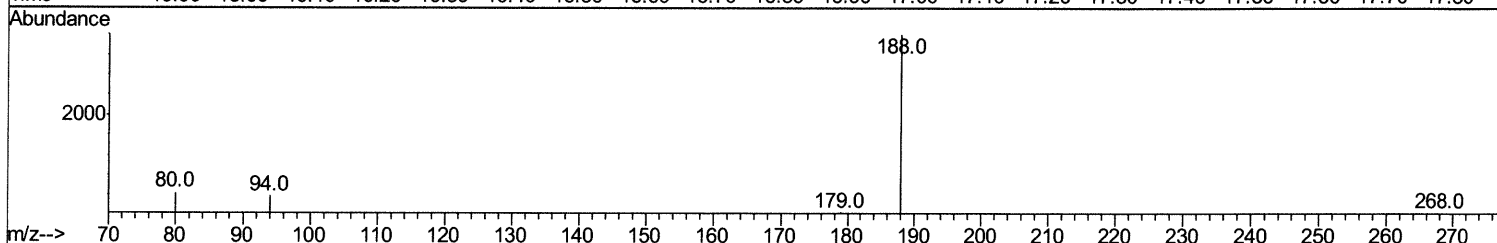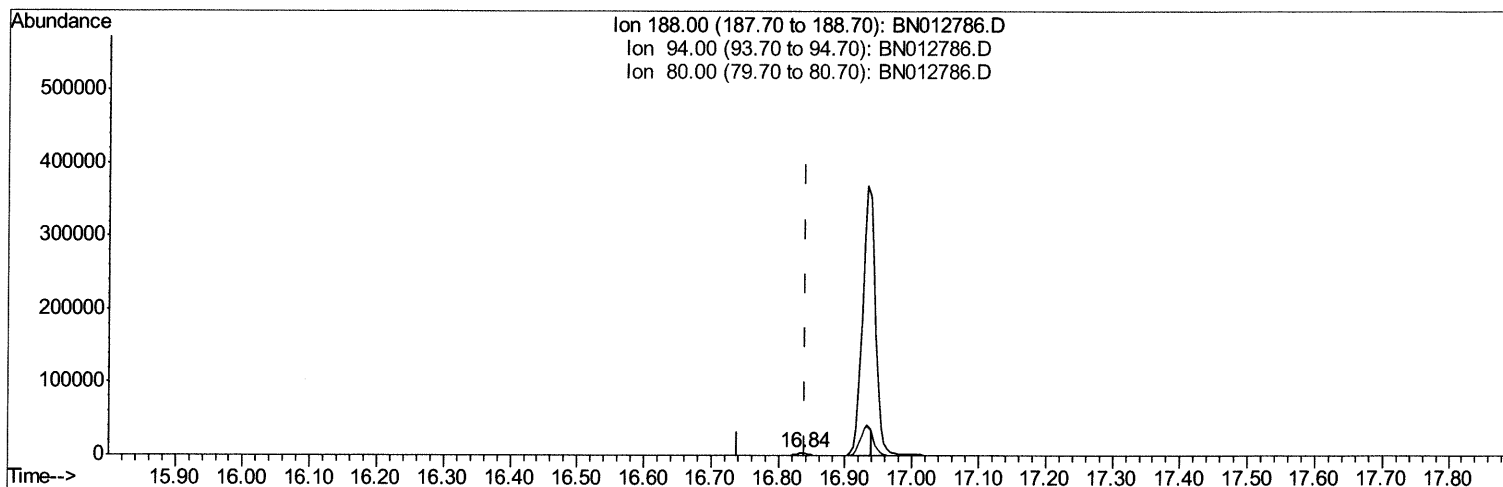

TIC: BN012786.D

(10) Phenanthrene-d10 (I)

16.836min (-0.004) 0.40ng/ul m 12/04/2024

response 4954

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	10.60
80.00	12.60	12.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012786.D
Acq On : 01 Dec 2020 17:39
Operator : CG/JU
Sample : PB133292BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK92

Manual Integrations
APPROVED

mohammad
12/2/2020 2:27:35 PM

Quant Time: Dec 02 01:04:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	955	0.40	ng/ul	0.00
2) Naphthalene-d8	10.19	136	4028	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	2433	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.84	188	4954m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.06	240	3954	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4514	0.40	ng/ul	0.00

12/04/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.80	152	1859	0.32	ng/ul	0.00
14) Fluoranthene-d10	18.88	212	4368	0.34	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed