


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012801.D
Acq On : 02 Dec 2020 03:17
Operator : CG/JU
Sample : L4793-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BG6

Manual Integrations
APPROVED

mohammad
12/2/2020 2:28:22 PM

Quant Time: Dec 02 05:14:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 00:53:21 2020
Response via : Initial Calibration

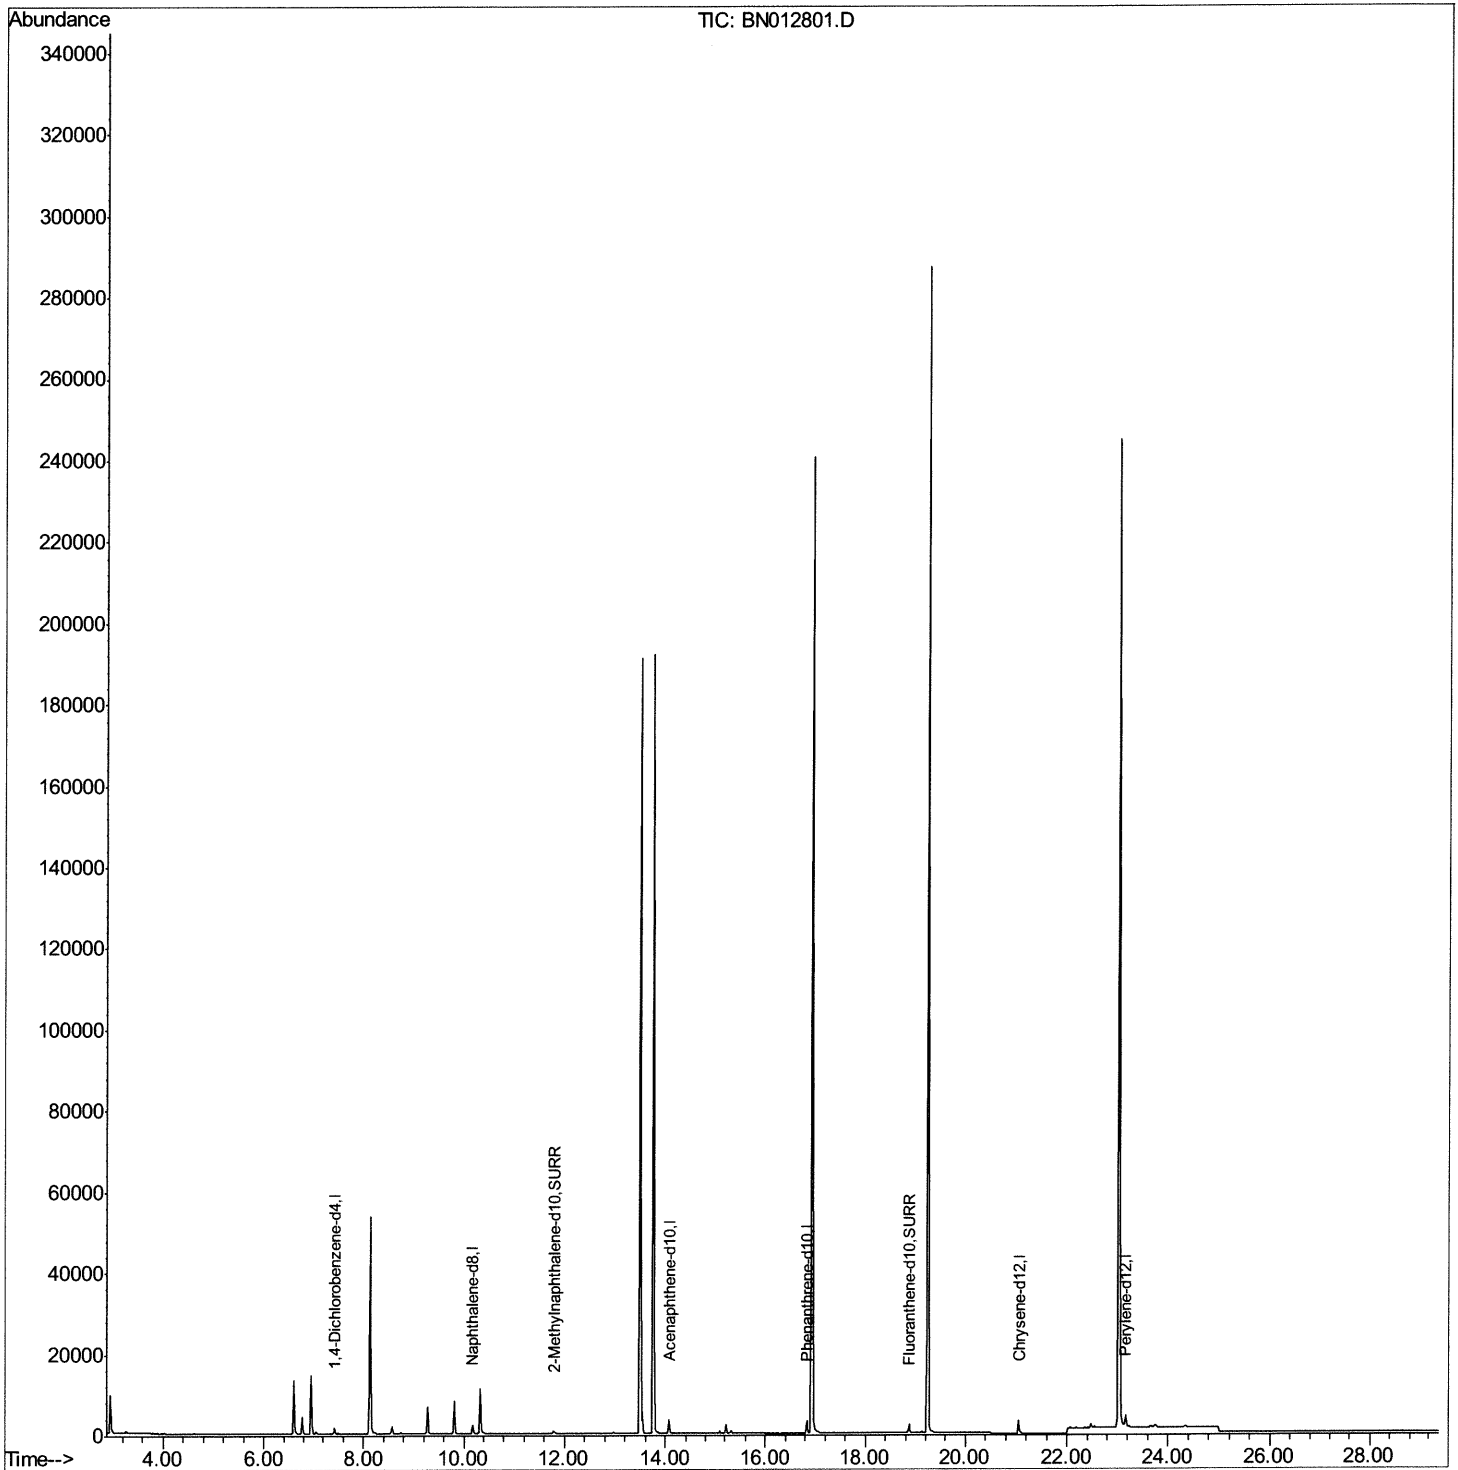

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012801.D
 Acq On : 02 Dec 2020 03:17
 Operator : CG/JU
 Sample : L4793-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BG6

Manual Integrations
 APPROVED

mohammad
 12/2/2020 2:28:22 PM

Quant Time: Dec 02 05:09:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration

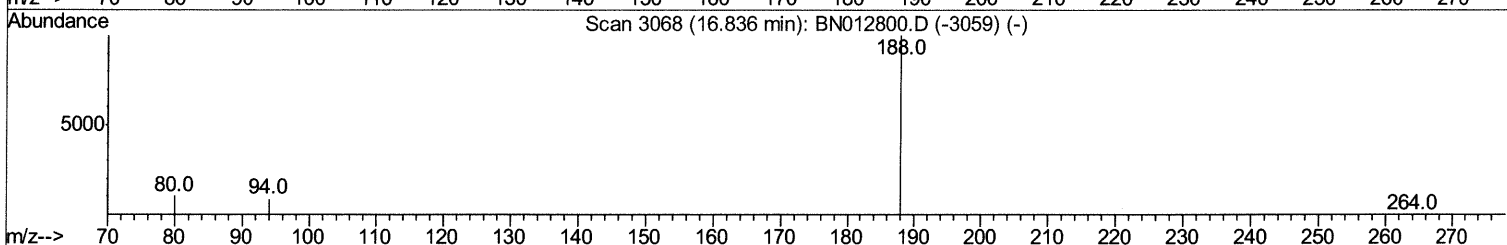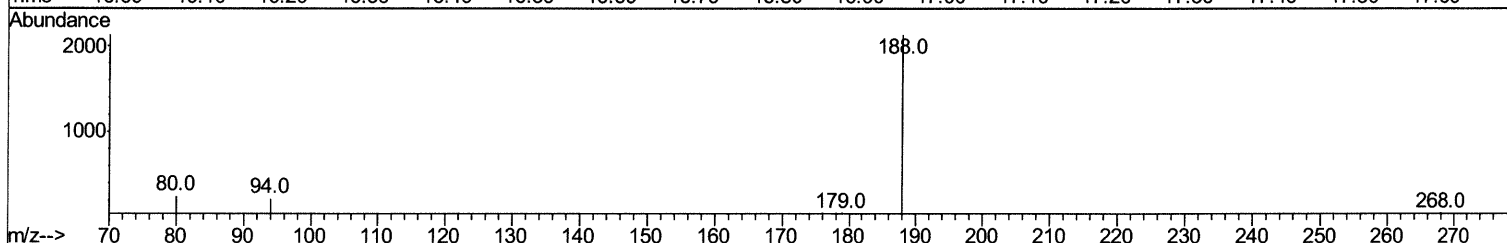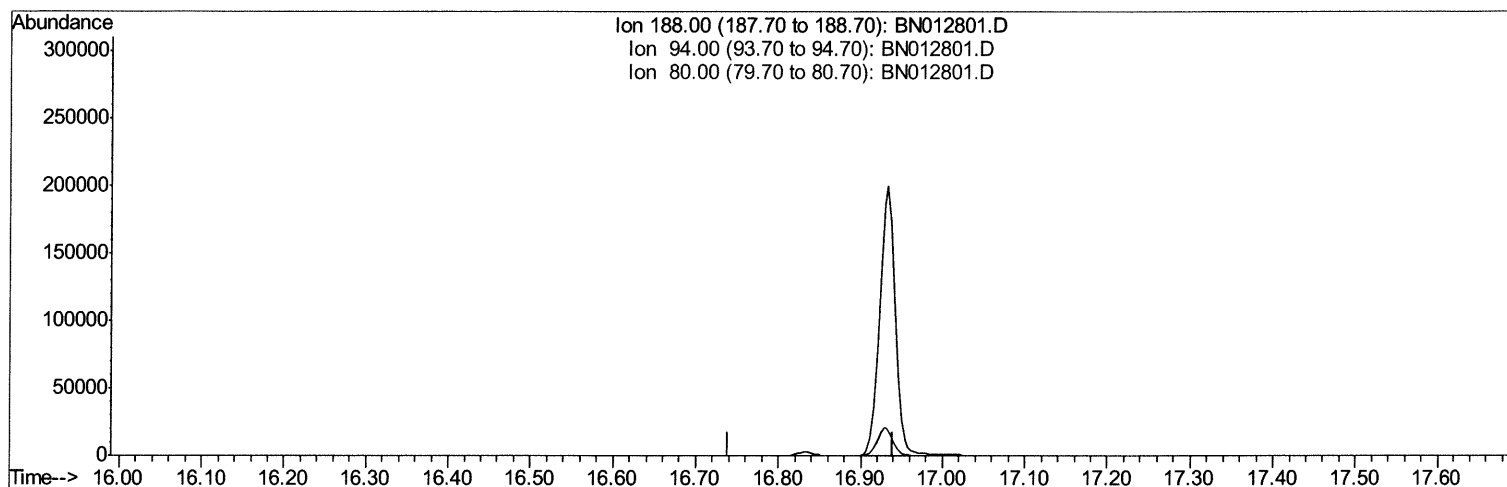

TIC: BN012801.D

(10) Phenanthrene-d10 (I)

16.840min (-16.840) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012801.D
 Acq On : 02 Dec 2020 03:17
 Operator : CG/JU
 Sample : L4793-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BG6

Manual Integrations
 APPROVED

mohammad
 12/2/2020 2:28:22 PM

Quant Time: Dec 02 05:09:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration

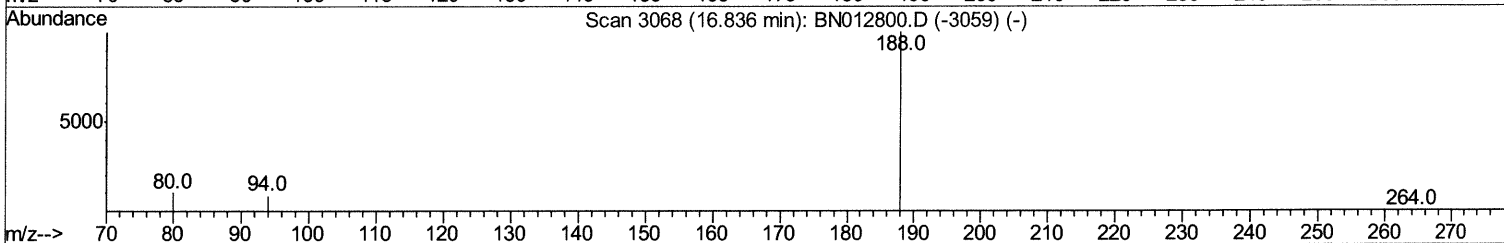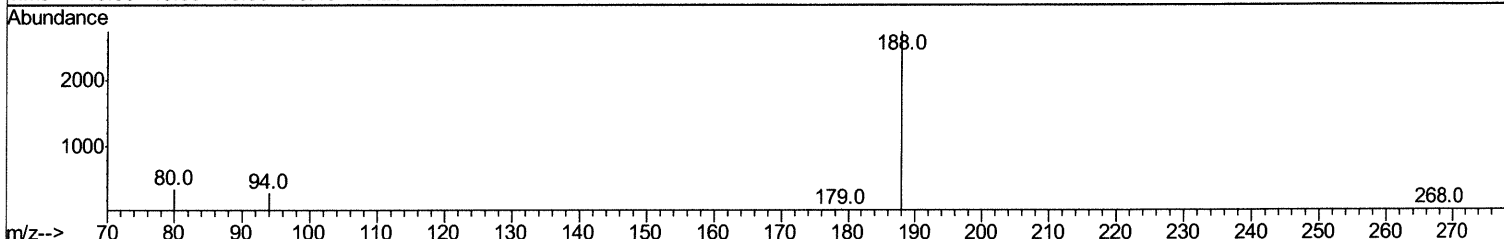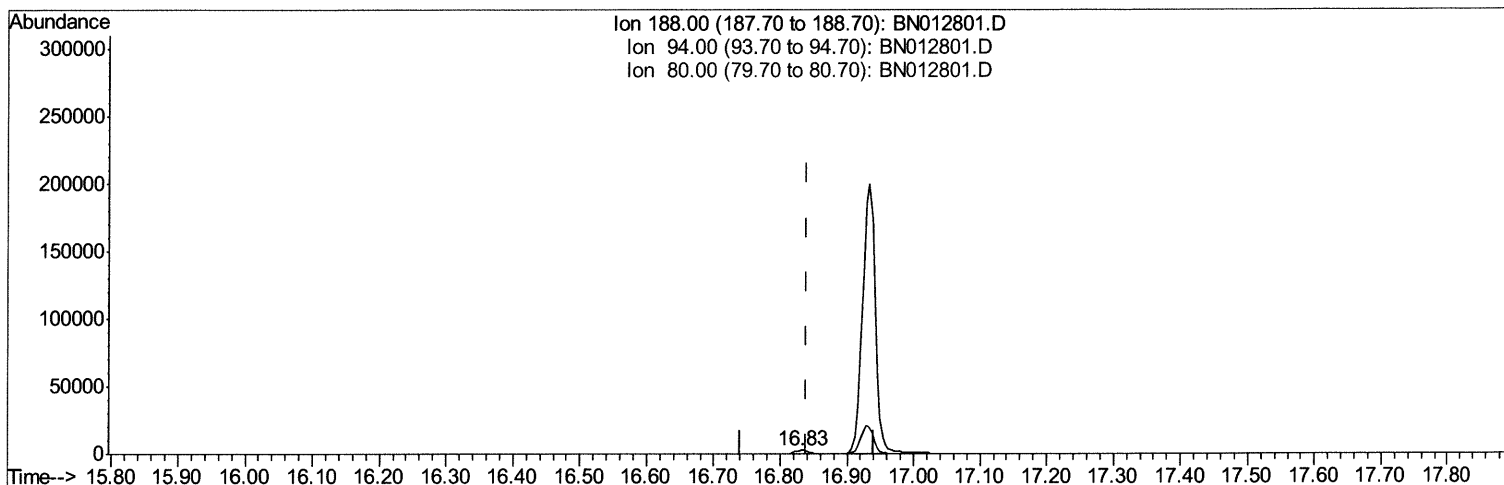

TIC: BN012801.D

(10) Phenanthrene-d10 (I)

16.831min (-0.008) 0.40ng/ul m | 2/04/20 JU

response 3815

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	10.86
80.00	12.60	12.80
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012801.D
 Acq On : 02 Dec 2020 03:17
 Operator : CG/JU
 Sample : L4793-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BG6

Manual Integrations
 APPROVED

mohammad
 12/2/2020 2:28:22 PM

Quant Time: Dec 02 05:14:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 00:53:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	764	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	2982	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.08	164	1816	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.83	188	3815m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.05	240	3252	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	3789	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.79	152	1117	0.26	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	2479	0.25	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed