


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
Data File : BN012813.D
Acq On : 02 Dec 2020 10:28
Operator : CG/JU
Sample : L4865-17
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BC2

Manual Integrations
APPROVED

mohammad
12/3/2020 3:43:29 PM

Quant Time: Dec 02 11:11:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 01 10:54:12 2020
Response via : Initial Calibration

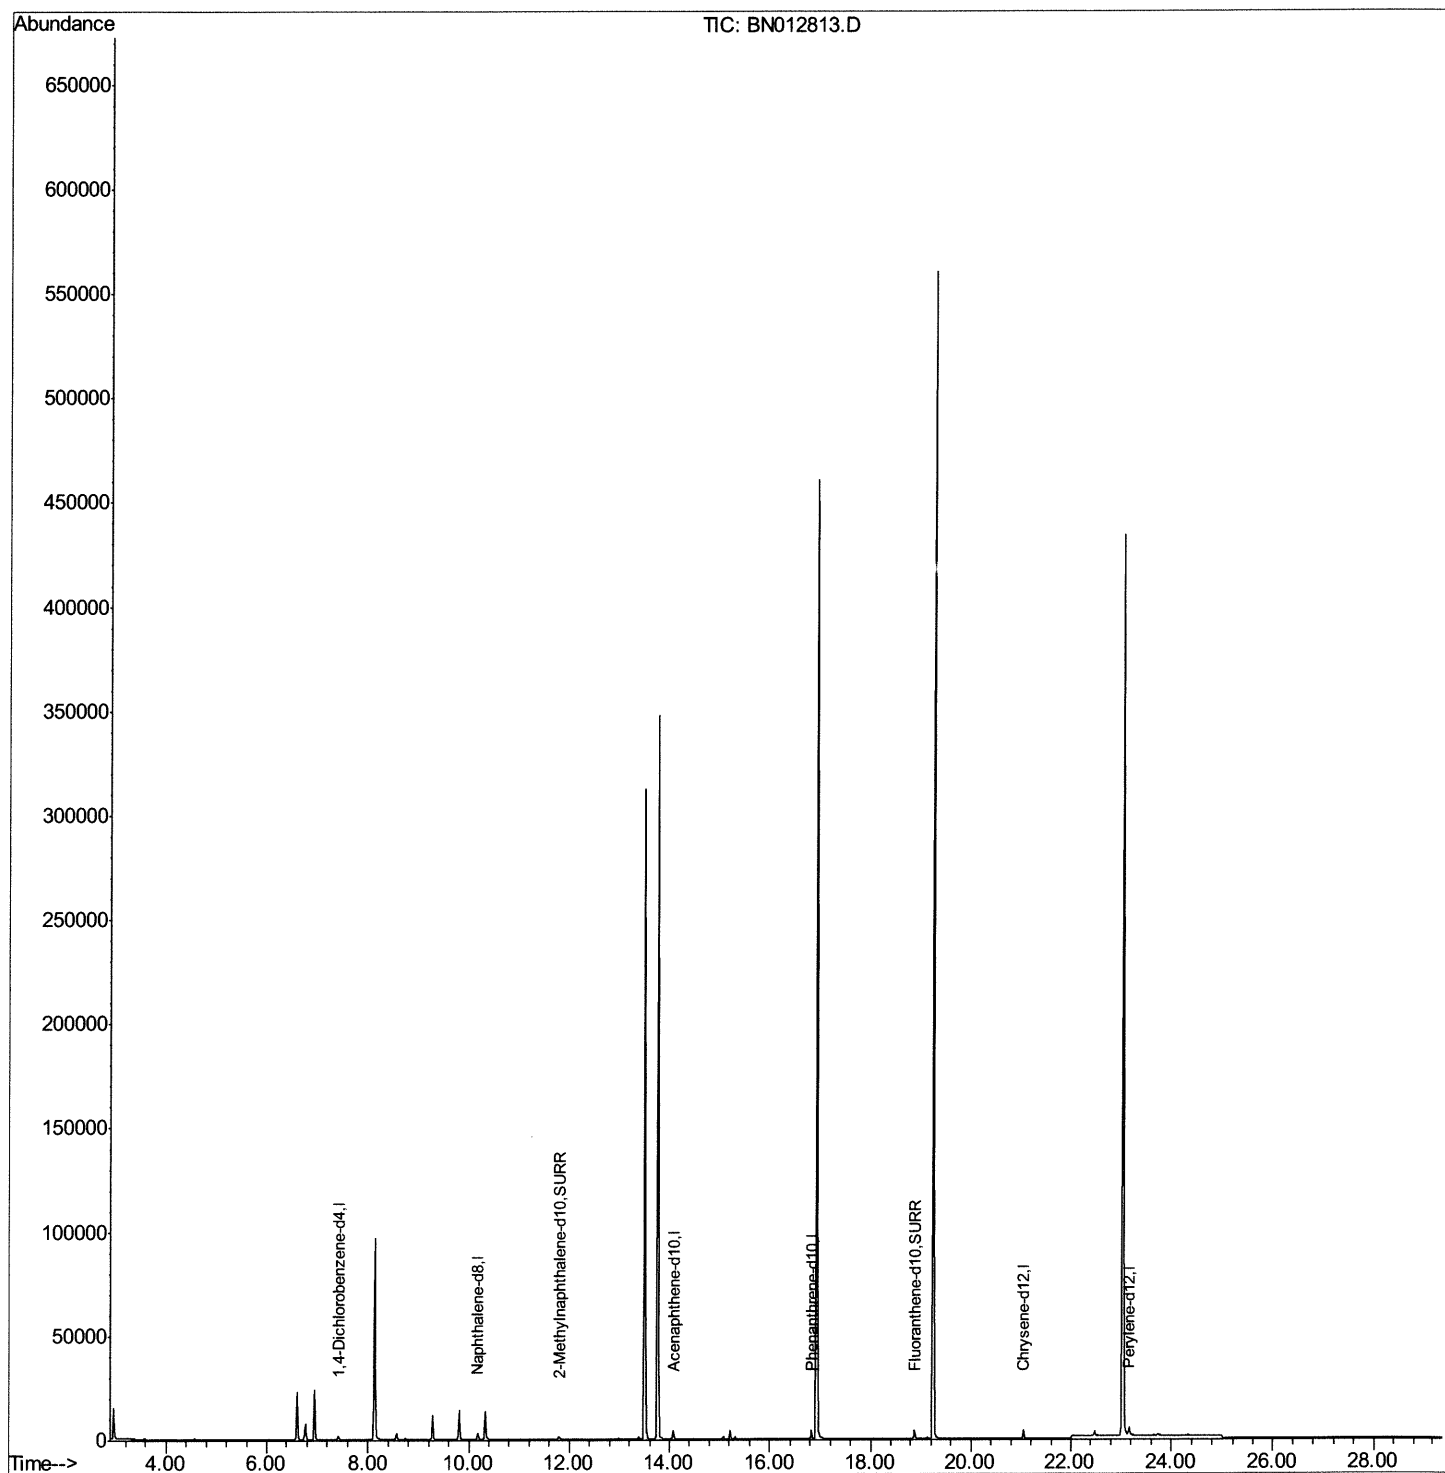

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012813.D
 Acq On : 02 Dec 2020 10:28
 Operator : CG/JU
 Sample : L4865-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC2

Manual Integrations
 APPROVED

mohammad
 12/3/2020 3:43:29 PM

Quant Time: Dec 02 11:02:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 10:54:12 2020
 Response via : Initial Calibration

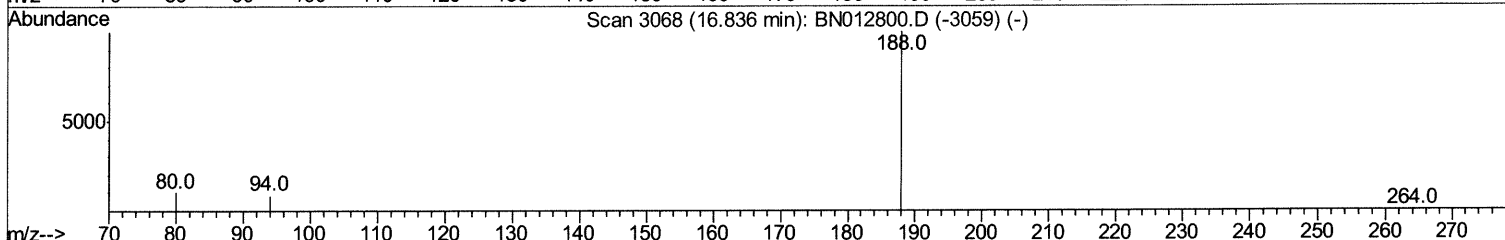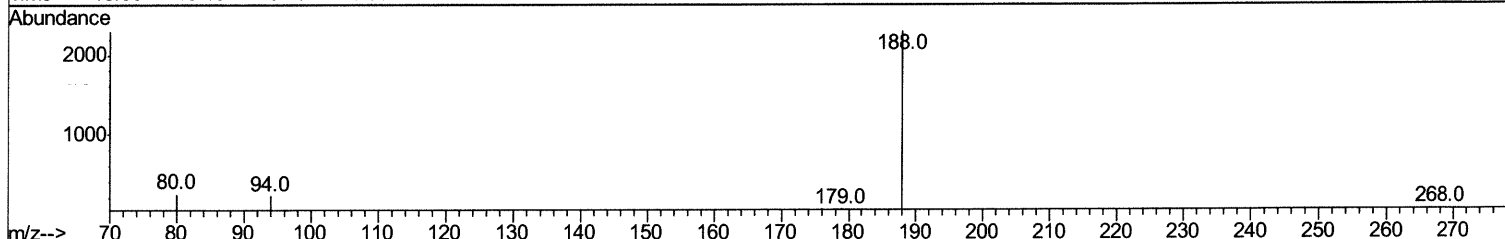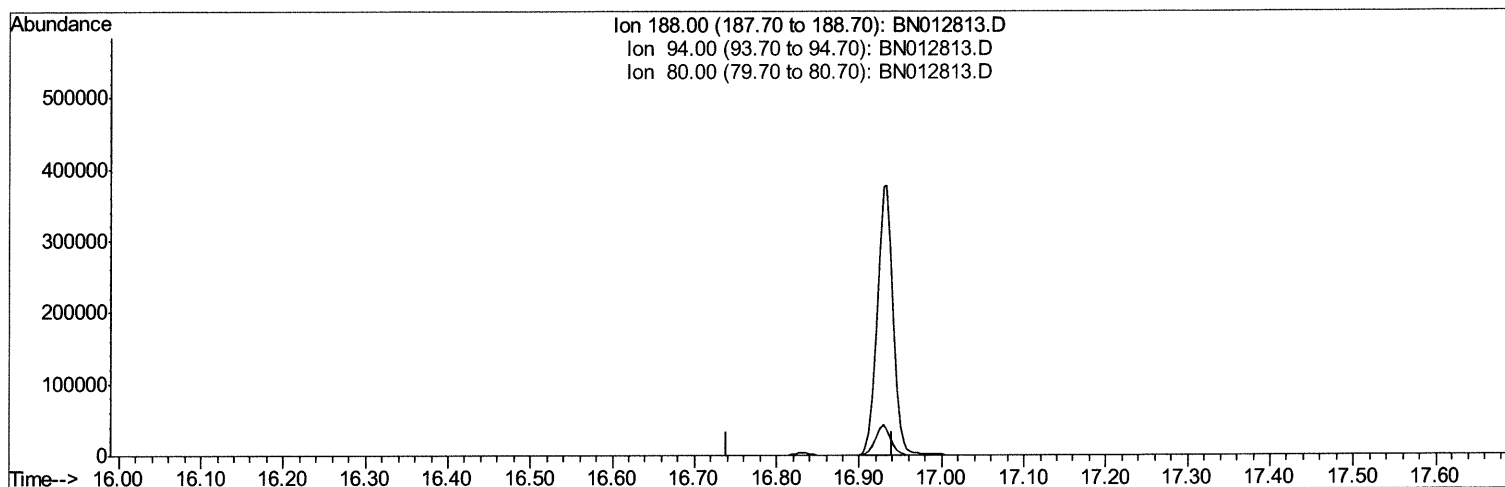

TIC: BN012813.D

(10) Phenanthrene-d10 (I)
 16.840min (-16.840) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	12.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012813.D
 Acq On : 02 Dec 2020 10:28
 Operator : CG/JU
 Sample : L4865-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC2

Manual Integrations
 APPROVED

mohammad
 12/3/2020 3:43:29 PM

Quant Time: Dec 02 11:02:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 10:54:12 2020
 Response via : Initial Calibration

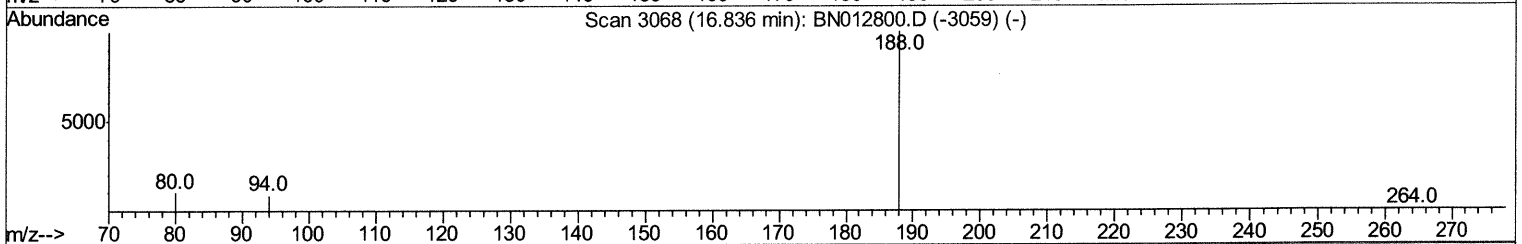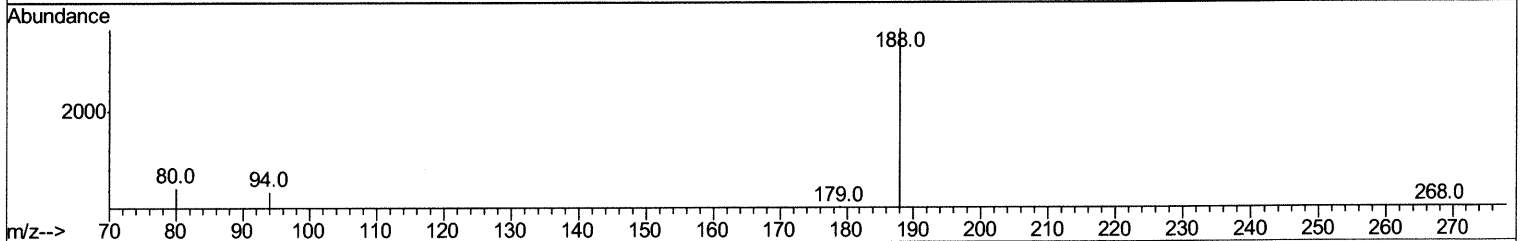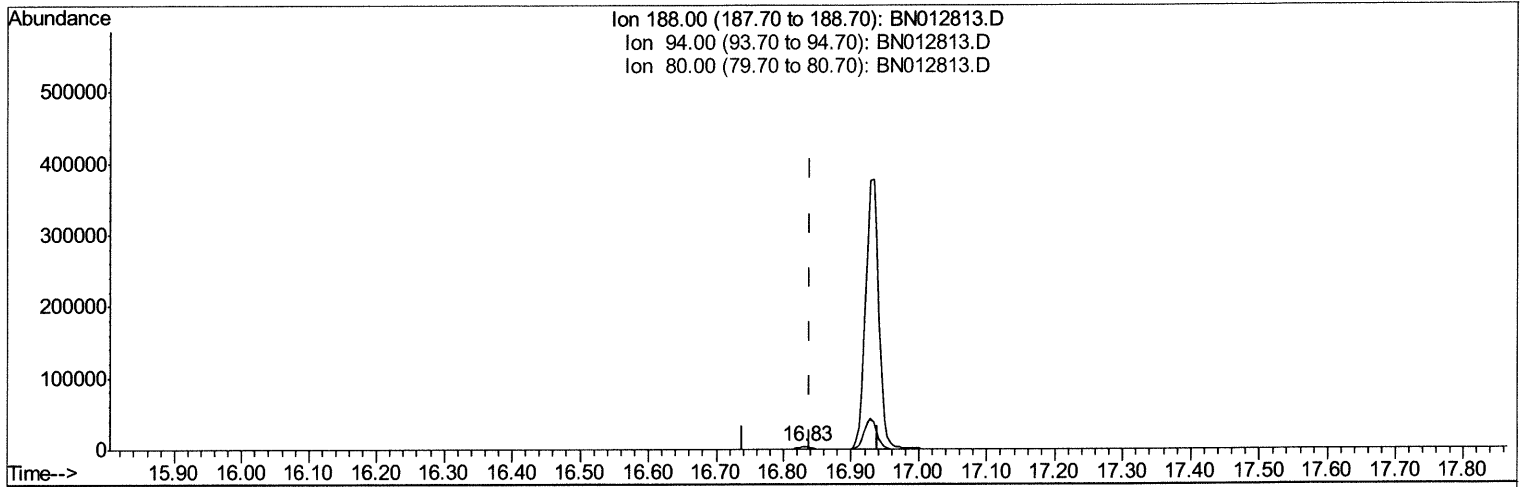

TIC: BN012813.D

(10) Phenanthrene-d10 (I)

16.831min (-0.008) 0.40ng/ul m (12/04/20 JU

response 4931

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	10.14
80.00	12.60	12.09
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN120220\
 Data File : BN012813.D
 Acq On : 02 Dec 2020 10:28
 Operator : CG/JU
 Sample : L4865-17
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BC2

Manual Integrations
 APPROVED

mohammad
 12/3/2020 3:43:29 PM

Quant Time: Dec 02 11:11:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN112020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 01 10:54:12 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	877	0.40	ng/ul	0.00
2) Naphthalene-d8	10.18	136	3605	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.07	164	2230	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.83	188	4931m>	0.40	ng/ul >	0.00
16) Chrysene-d12	21.05	240	4034	0.40	ng/ul	0.00
20) Perylene-d12	23.16	264	4547	0.40	ng/ul	0.00

12/04/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.79	152	1991	0.38	ng/ul	0.00
14) Fluoranthene-d10	18.87	212	4463	0.35	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed